

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 00:55
 Operator : SM\AJ
 Sample : PB124307BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 01:17:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.168	1233.6E6	642.2E6	901.288	913.086
Target Compounds							
1) T	Dalapon	2.002	1.714	90148127	86477961	53.875	95.030 #
2) T	3,5-DICHL...	0.000	4.503	0	104.0E6	N.D.	120.914
3) T	4-Nitroph...	0.000	4.847	0	18064222	N.D.	45.744
10) T	Pentachlo...	0.000	6.456	0	17144076	N.D.	1.783
11) T	2,4,5-TP ...	0.000	6.767	0	87673688	N.D.	23.050
12) T	2,4,5-T	0.000	7.218	0	21558762	N.D.	6.153
14) T	DINOSEB	0.000	8.001	0	50045411	N.D.	17.826
15) T	Picloram	8.949	8.910	111.7E6	67595952	10.123	11.009
16) T	DCPA	0.000	8.910	0	67595952	N.D.	13.480



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 00:55
Operator : SM\AJ
Sample : PB124307BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 01:17:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

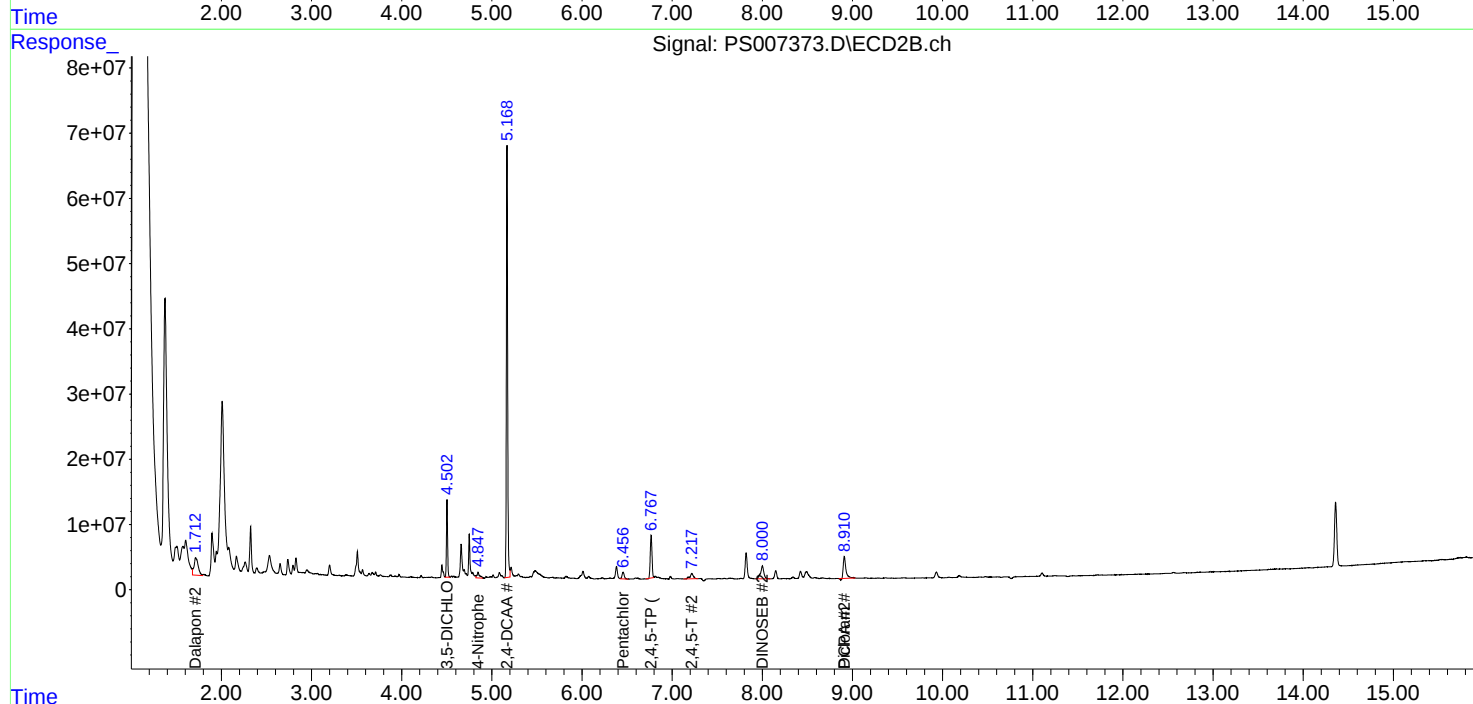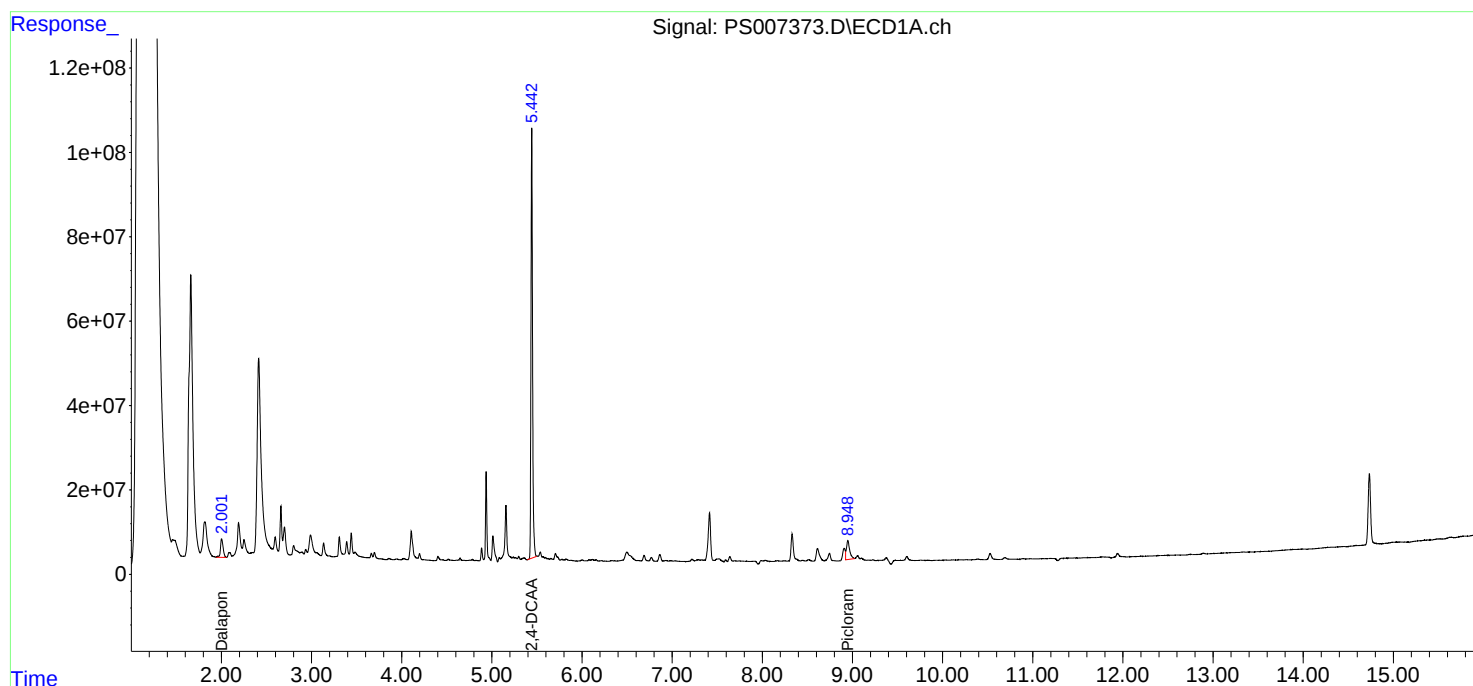


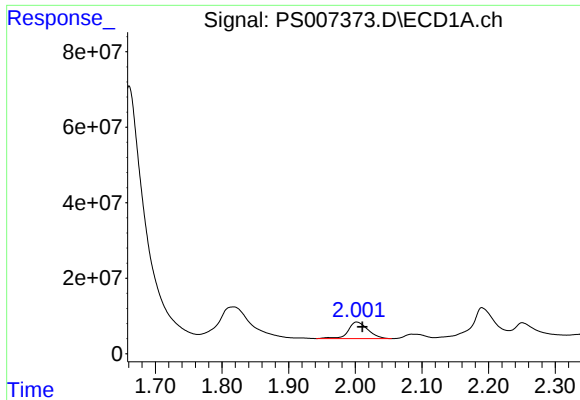

#1 Dalapon


R.T.: 2.002 min
Delta R.T.: -0.009 min
Response: 90148127
Conc: 53.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

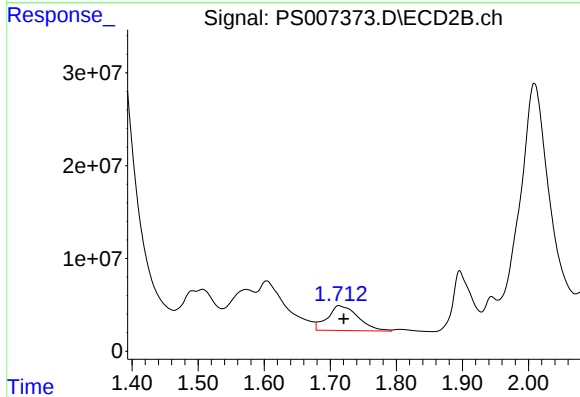


#1 Dalapon

R.T.: 1.714 min
Delta R.T.: -0.007 min
Response: 86477961
Conc: 95.03 ng/ml

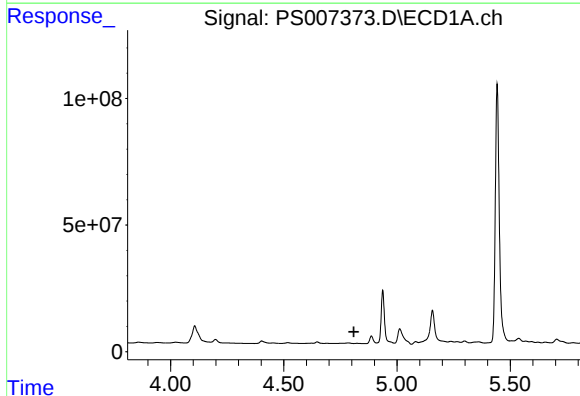


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

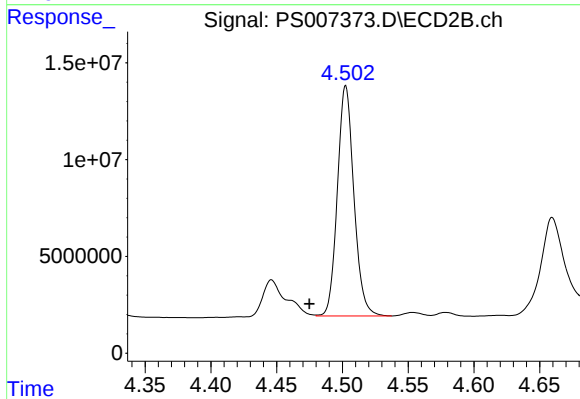

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.503 min
Delta R.T.: 0.028 min
Response: 104037899
Conc: 120.91 ng/ml

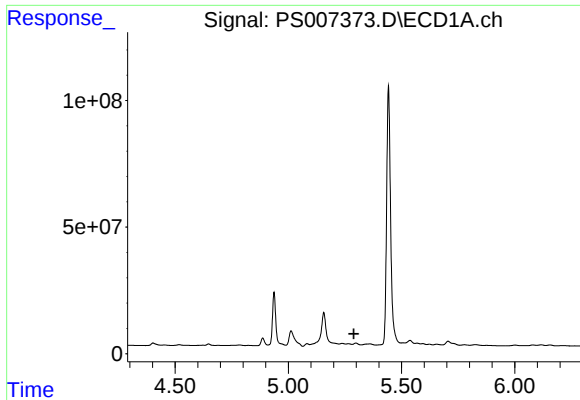

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

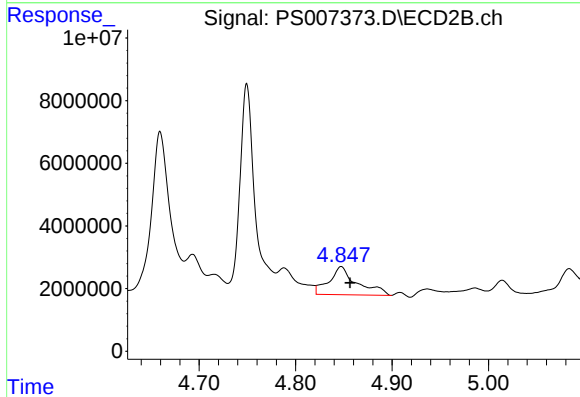


#3 4-Nitrophenol

R.T.: 4.847 min
Delta R.T.: -0.009 min
Response: 18064222
Conc: 45.74 ng/ml

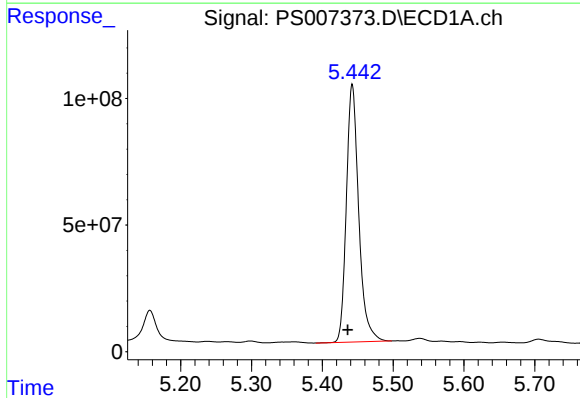


#4 2,4-DCAA

R.T.: 5.442 min
Delta R.T.: 0.007 min
Response: 1233564971
Conc: 901.29 ng/ml

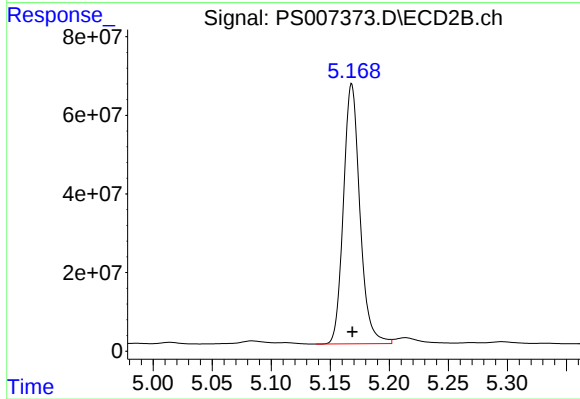

#4 2,4-DCAA


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 642179180
Conc: 913.09 ng/ml

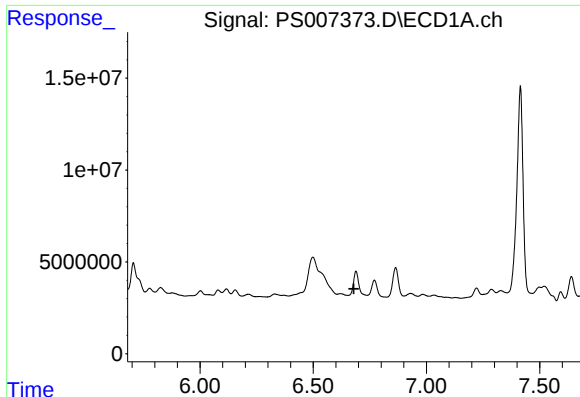

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

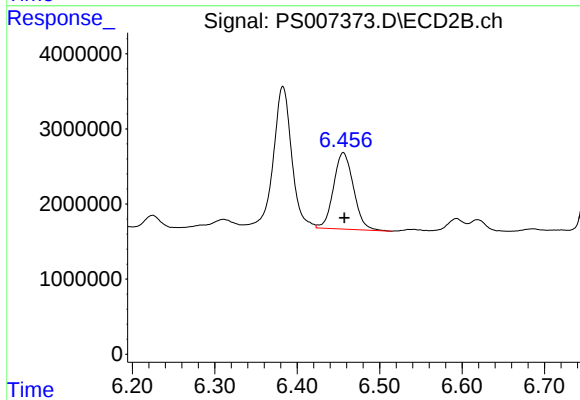


#10 Pentachlorophenol

R.T.: 6.456 min
Delta R.T.: -0.001 min
Response: 17144076
Conc: 1.78 ng/ml

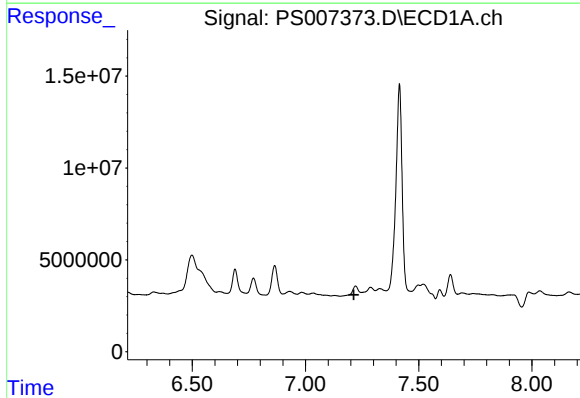


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

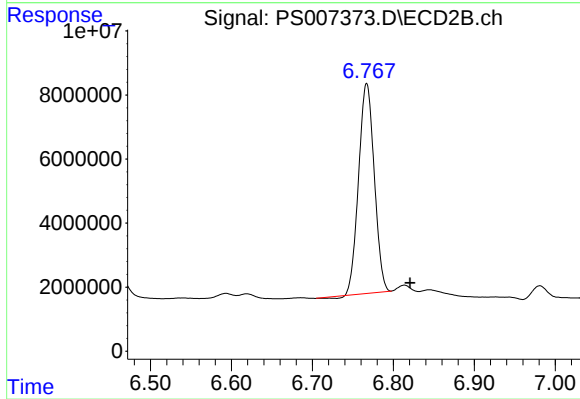

#11 2,4,5-TP (SILVEX)


R.T.: 6.767 min
Delta R.T.: -0.053 min
Response: 87673688
Conc: 23.05 ng/ml

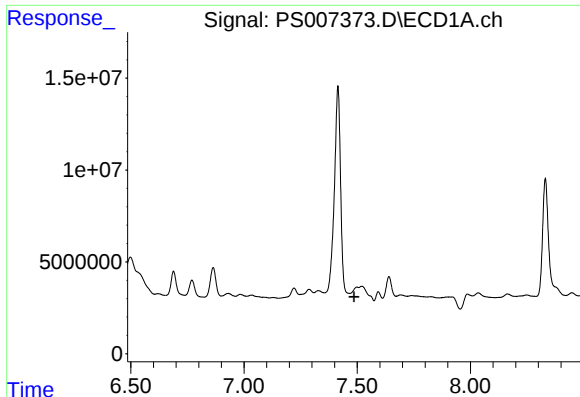

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

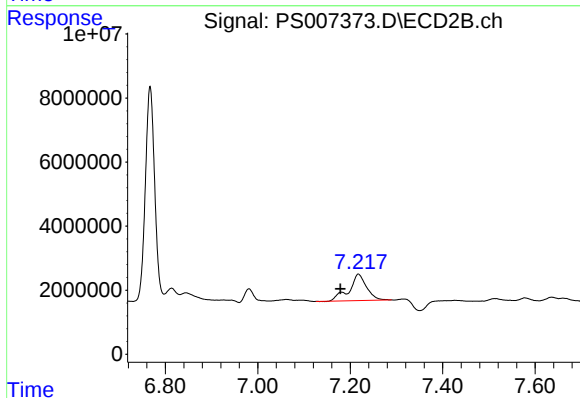


#12 2,4,5-T

R.T.: 7.218 min
Delta R.T.: 0.039 min
Response: 21558762
Conc: 6.15 ng/ml

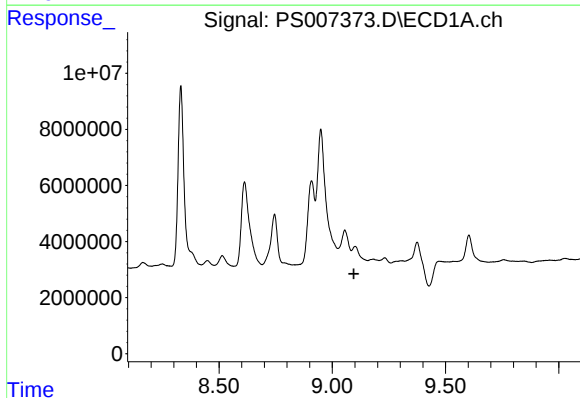


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

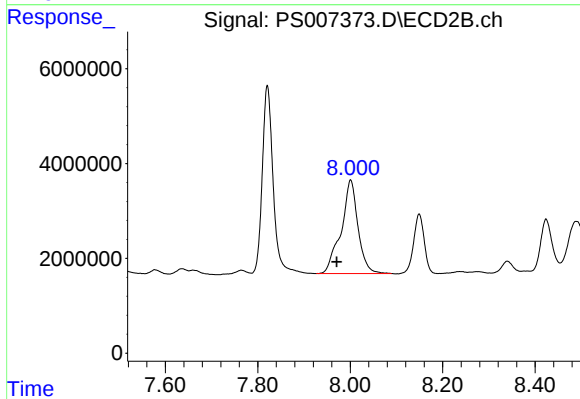

#14 DINOSEB


R.T.: 8.001 min
Delta R.T.: 0.030 min
Response: 50045411
Conc: 17.83 ng/ml

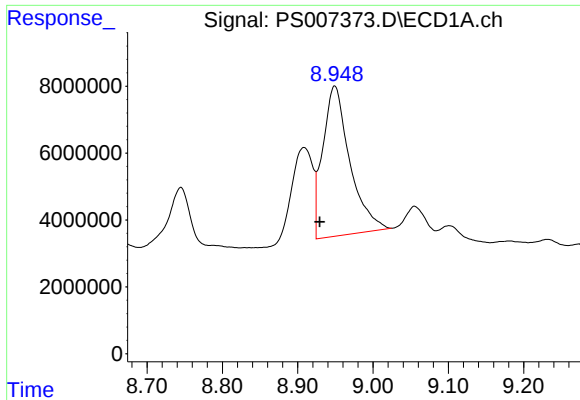

#15 Picloram


R.T.: 8.949 min
Delta R.T.: 0.020 min
Response: 111726142
Conc: 10.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

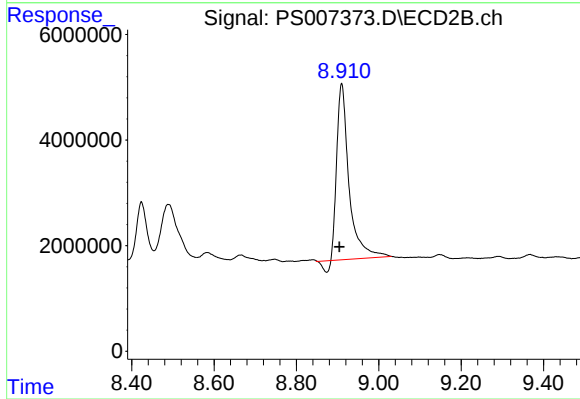


#15 Picloram

R.T.: 8.910 min
Delta R.T.: 0.005 min
Response: 67595952
Conc: 11.01 ng/ml

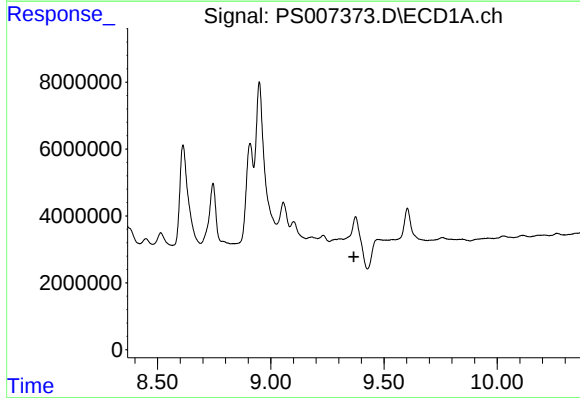

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

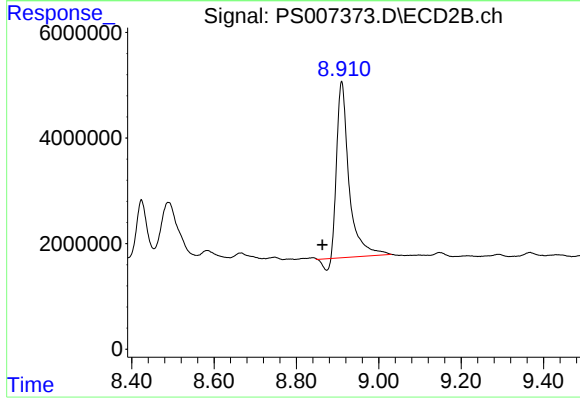

#16 DCPA

R.T.: 8.910 min
Delta R.T.: 0.047 min
Response: 67595952
Conc: 13.48 ng/ml