

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 01:39
 Operator : SM\AJ
 Sample : PB124307TB
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:31:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.452	5.178	1254.7E6	642.2E6	916.765	913.113
Target Compounds							
1) T	Dalapon	2.012	1.723	91977724	108.2E6	54.969	118.950 #
2) T	3,5-DICHL...	0.000	4.456	0	22790845	N.D.	26.488
3) T	4-Nitroph...	0.000	4.857	0	17856773	N.D.	45.219
5) T	DICAMBA	5.547	0.000	34559559	0	7.034	N.D. #
7) T	MCPA	0.000	5.491	0	46838735	N.D.	16.112
10) T	Pentachlo...	0.000	6.466	0	16766430	N.D.	1.744
11) T	2,4,5-TP ...	0.000	6.777	0	83197346	N.D.	21.873
12) T	2,4,5-T	7.424	0.000	195.0E6	0	25.510	N.D. #
14) T	DINOSEB	0.000	8.011	0	49877868	N.D.	17.767
15) T	Picloram	8.916	8.924	81371043	7990451	7.372	1.301 #
16) T	DCPA	0.000	8.924	0	7990451	N.D.	1.593



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 01:39
Operator : SM\AJ
Sample : PB124307TB
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:31:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

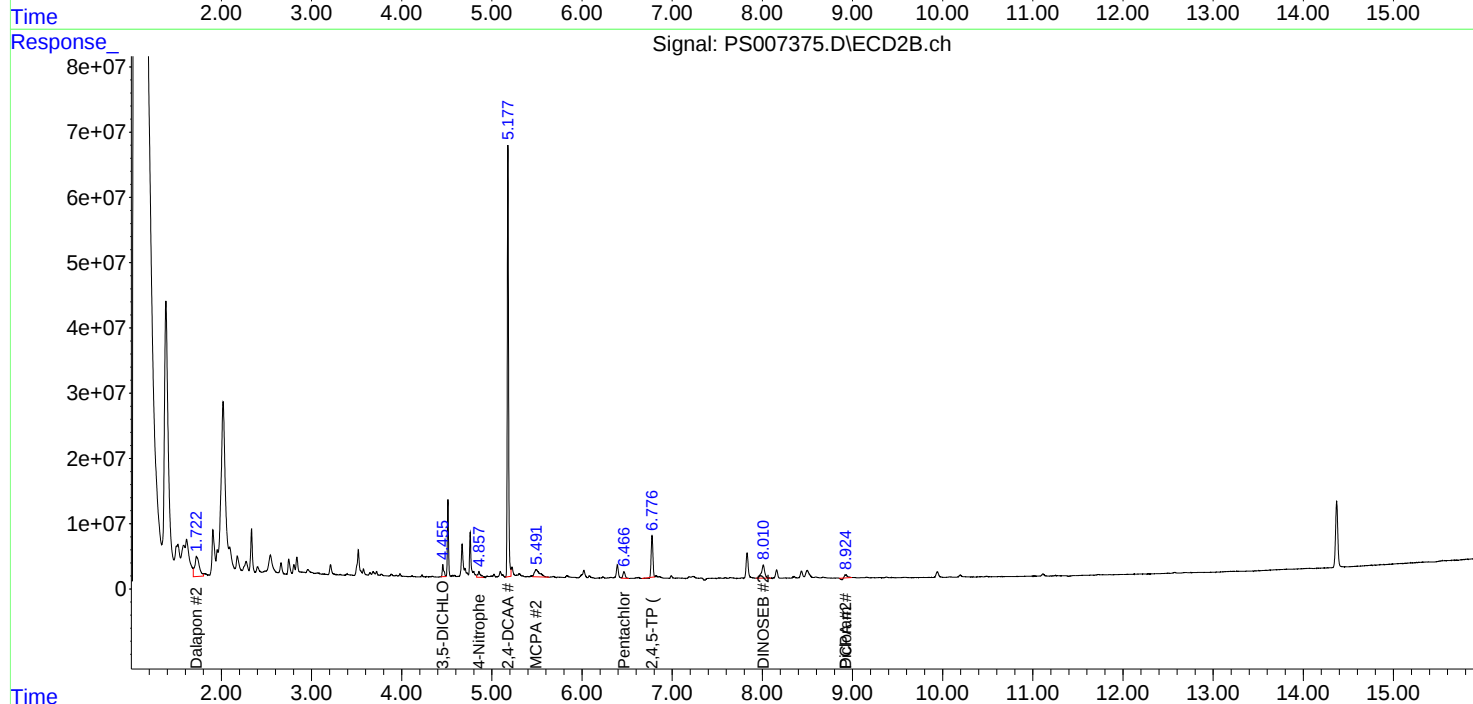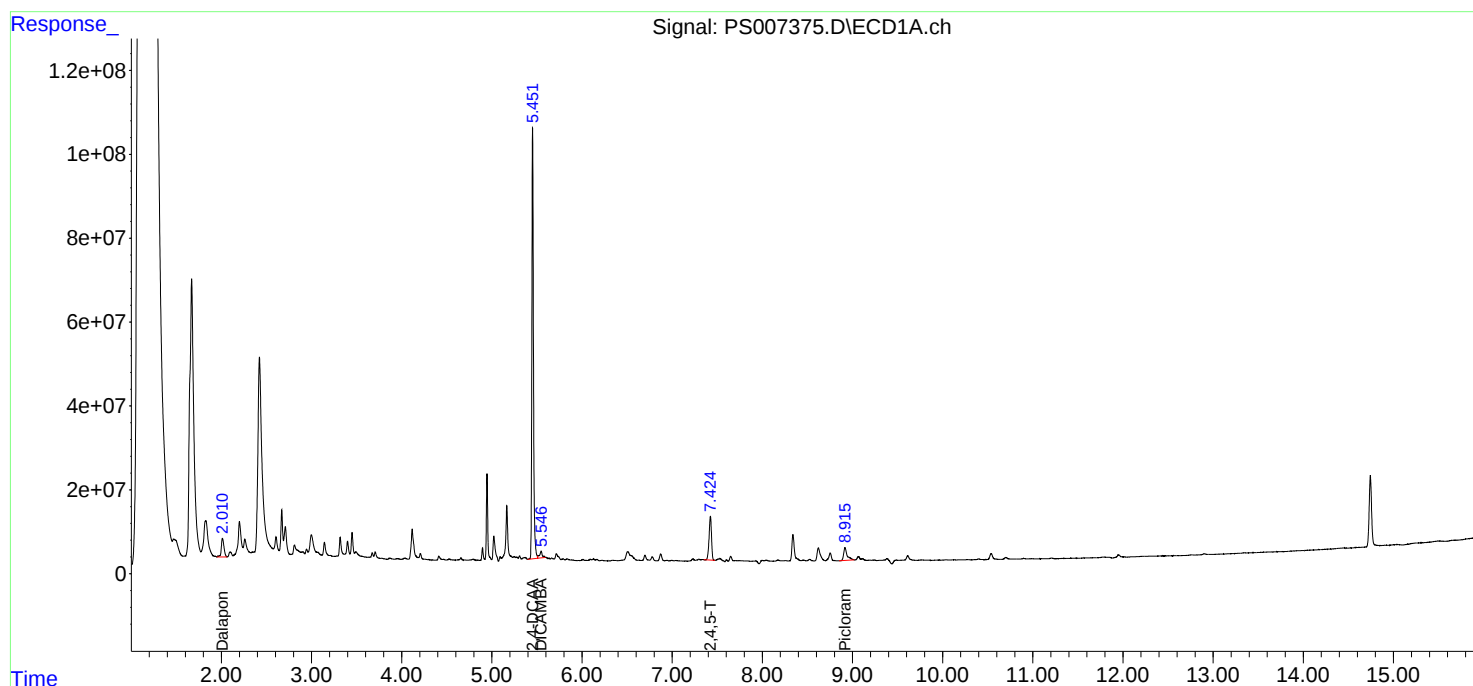


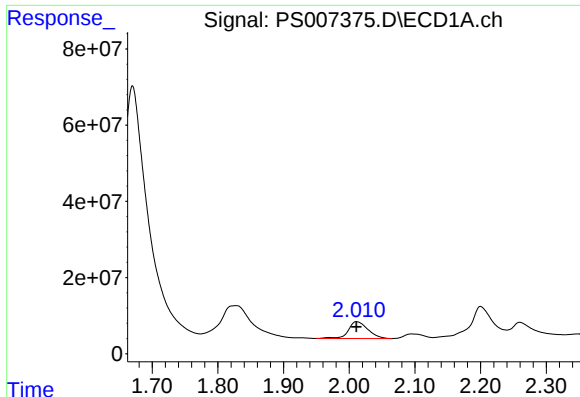

#1 Dalapon


R.T.: 2.012 min
Delta R.T.: 0.000 min
Response: 91977724
Conc: 54.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

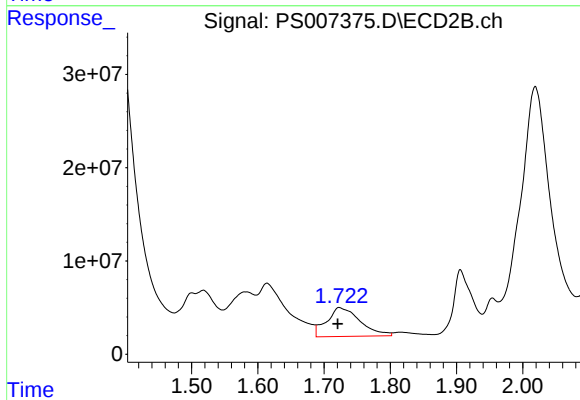


#1 Dalapon

R.T.: 1.723 min
Delta R.T.: 0.003 min
Response: 108244585
Conc: 118.95 ng/ml

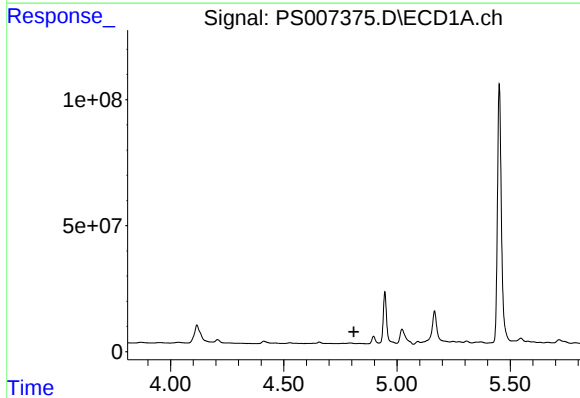


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

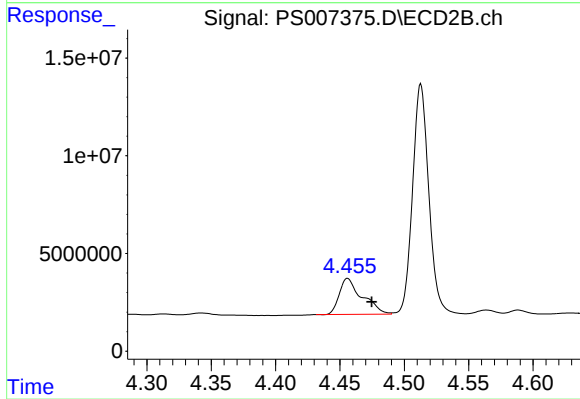

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.456 min
Delta R.T.: -0.019 min
Response: 22790845
Conc: 26.49 ng/ml

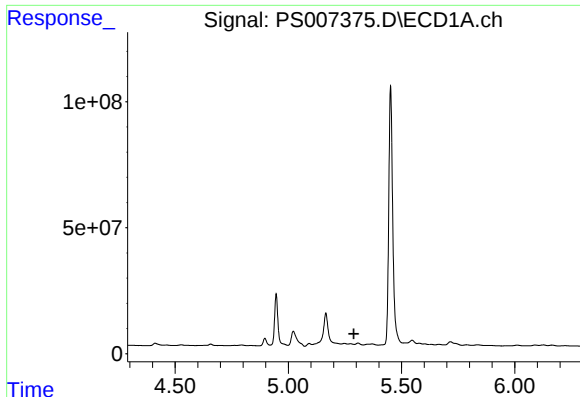

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

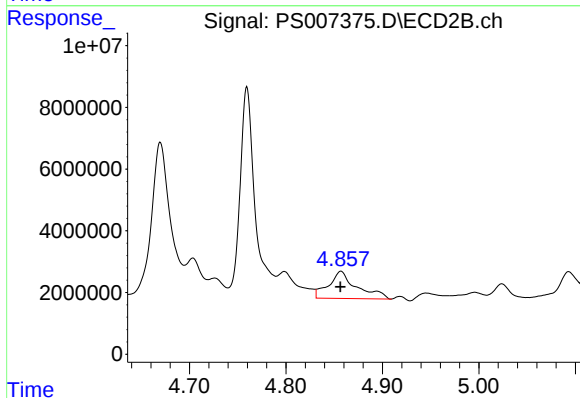


#3 4-Nitrophenol

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 17856773
Conc: 45.22 ng/ml

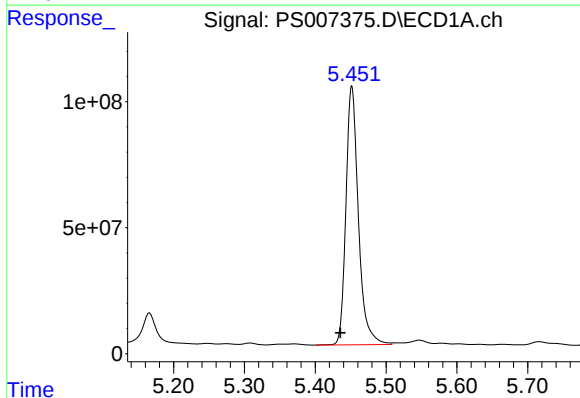


#4 2,4-DCAA

R.T.: 5.452 min
Delta R.T.: 0.016 min
Response: 1254748141
Conc: 916.77 ng/ml

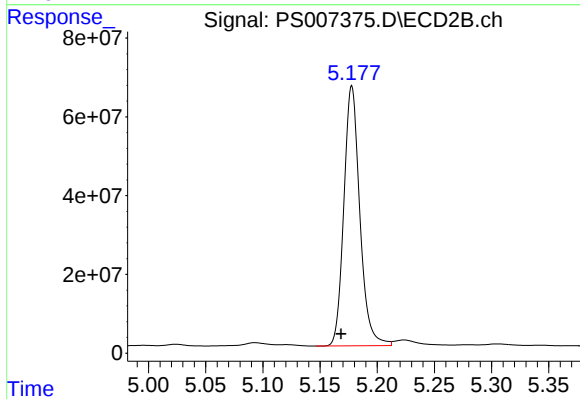

#4 2,4-DCAA


R.T.: 5.178 min
Delta R.T.: 0.009 min
Response: 642198582
Conc: 913.11 ng/ml

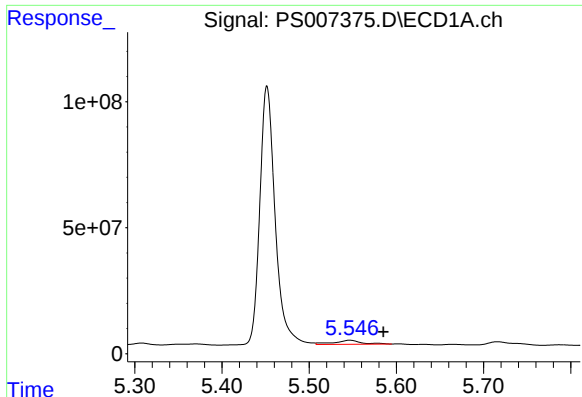

#5 DICAMBA


R.T.: 5.547 min
Delta R.T.: -0.039 min
Response: 34559559
Conc: 7.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

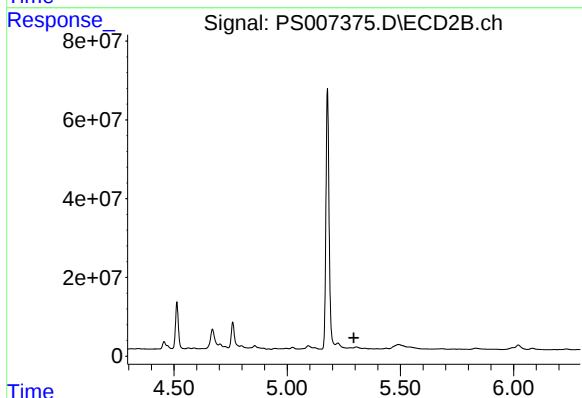


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

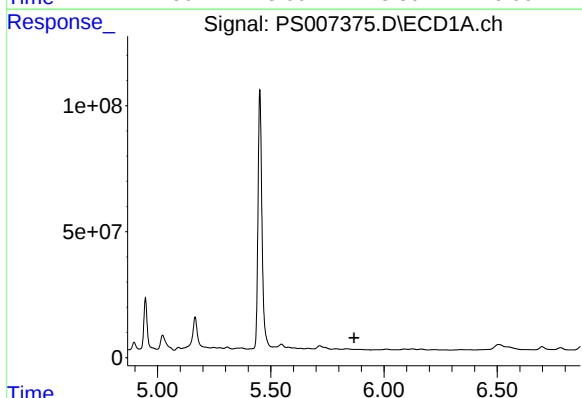


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

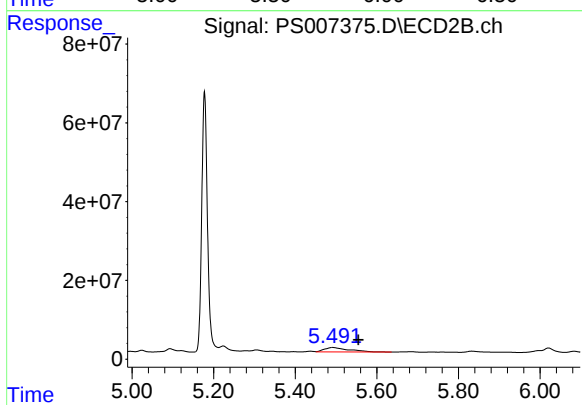

#7 MCPA


R.T.: 5.491 min
Delta R.T.: -0.063 min
Response: 46838735
Conc: 16.11 ug/ml

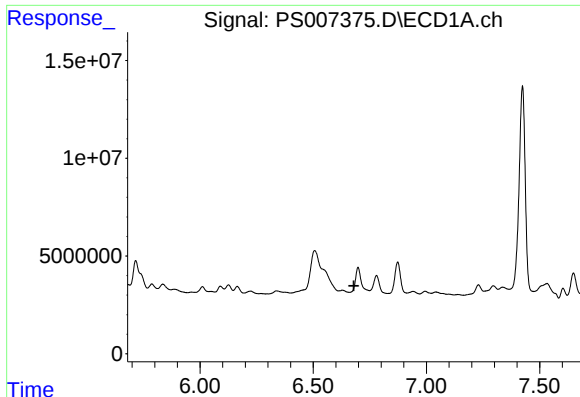

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

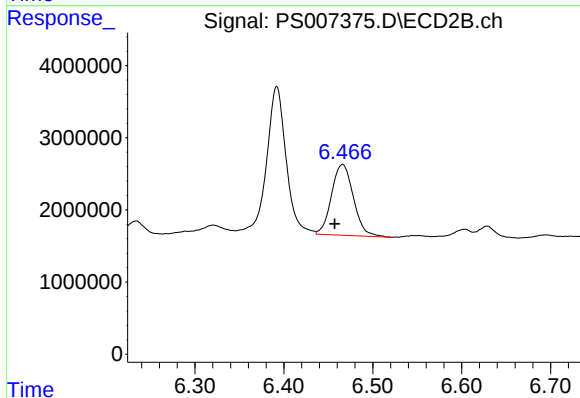


#10 Pentachlorophenol

R.T.: 6.466 min
Delta R.T.: 0.009 min
Response: 16766430
Conc: 1.74 ng/ml

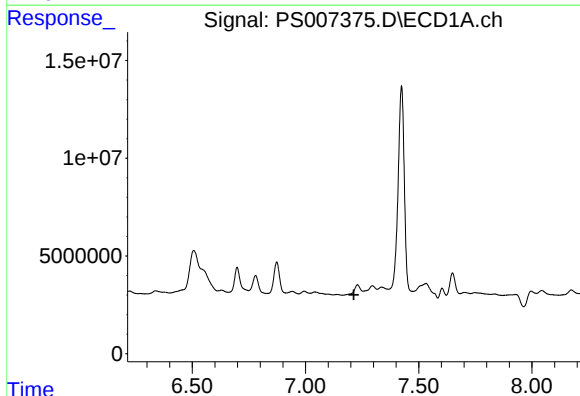


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

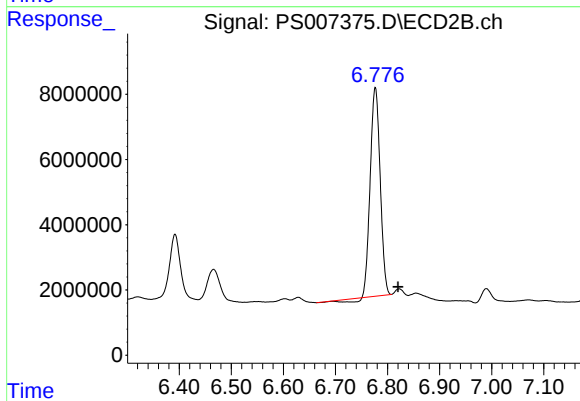

#11 2,4,5-TP (SILVEX)


R.T.: 6.777 min
Delta R.T.: -0.044 min
Response: 83197346
Conc: 21.87 ng/ml

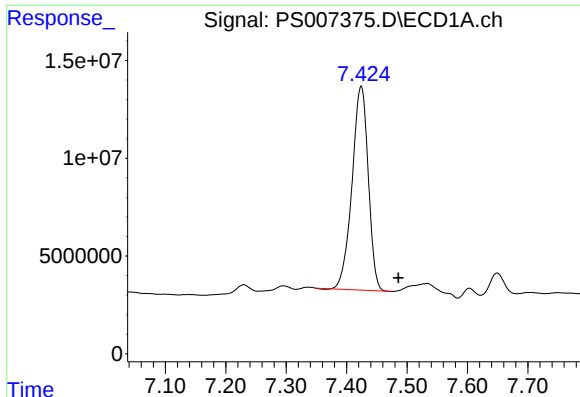

#12 2,4,5-T


R.T.: 7.424 min
Delta R.T.: -0.062 min
Response: 195020707
Conc: 25.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

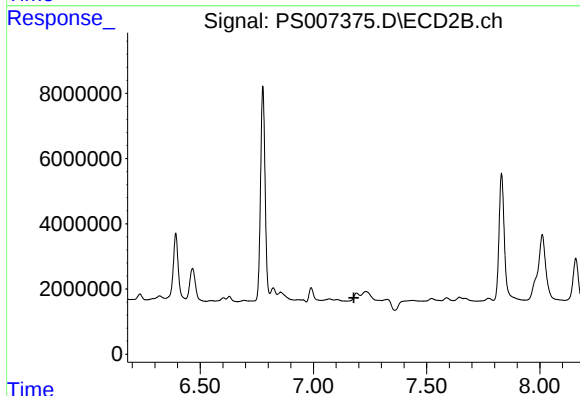


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.

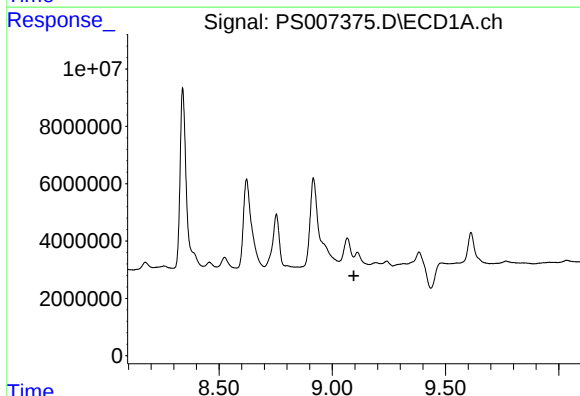


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

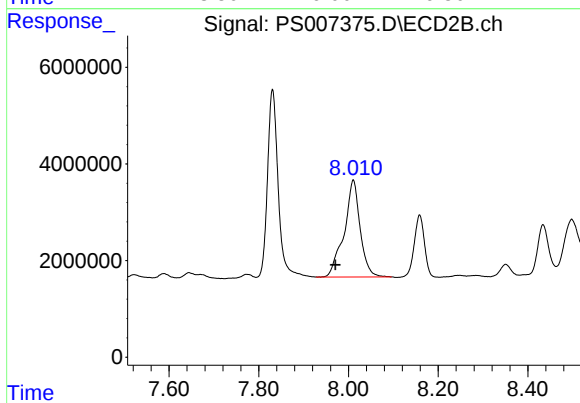

#14 DINOSEB


R.T.: 8.011 min
Delta R.T.: 0.040 min
Response: 49877868
Conc: 17.77 ng/ml

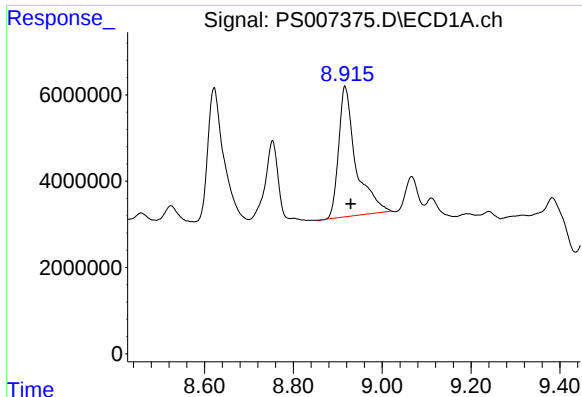

#15 Picloram


R.T.: 8.916 min
Delta R.T.: -0.013 min
Response: 81371043
Conc: 7.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

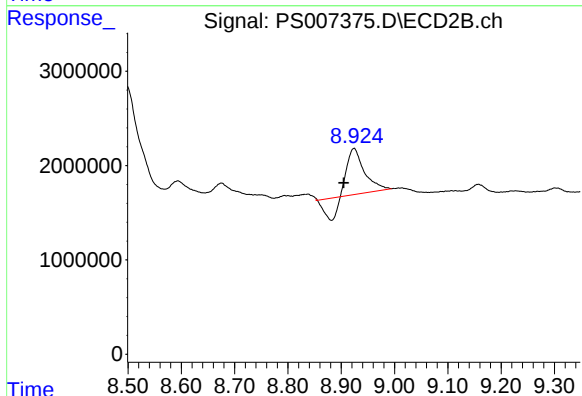


#15 Picloram

R.T.: 8.924 min
Delta R.T.: 0.019 min
Response: 7990451
Conc: 1.30 ng/ml

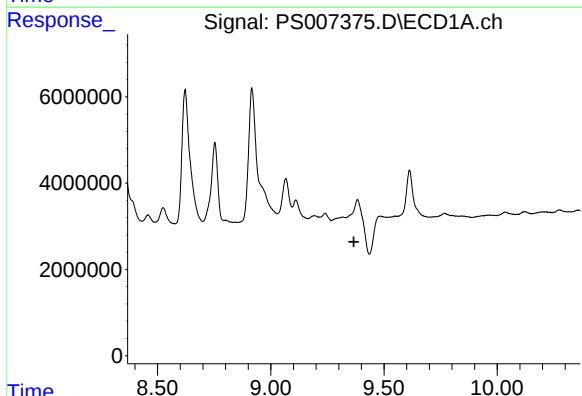

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

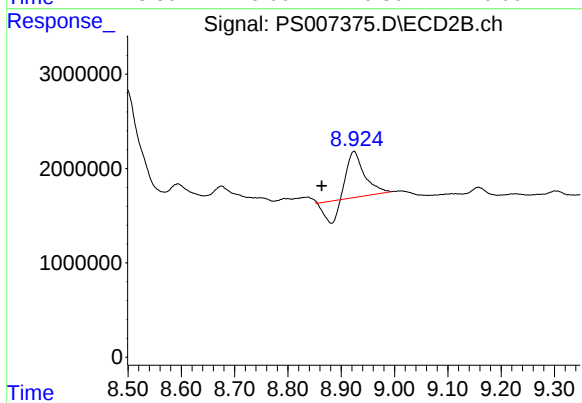

#16 DCPA

R.T.: 8.924 min
Delta R.T.: 0.061 min
Response: 7990451
Conc: 1.59 ng/ml