

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
 Data File : PS007380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 03:29
 Operator : SM\AJ
 Sample : K5542-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:32:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.162	941.2E6	507.2E6	687.668	721.134
Target Compounds							
1) T	Dalapon	1.995	1.706	64430234	31614816	38.505	34.741
2) T	3,5-DICHL...	0.000	4.497	0	50306694	N.D.	58.467
5) T	DICAMBA	5.530	5.294	61067241	15798101	12.429	6.071 #
7) T	MCPA	5.906	5.532	25184945	27718356	4.883	9.535 #
9) T	2,4-D	6.488	0.000	82977152	0	67.333	N.D. #
10) T	Pentachlo...	6.681	6.448	27872852	22684402	1.561	2.359 #
11) T	2,4,5-TP ...	0.000	6.808	0	6305644	N.D.	1.658
14) T	DINOSEB	0.000	7.957	0	16486243	N.D.	5.873
15) T	Picloram	0.000	8.911	0	20502437	N.D.	3.339
16) T	DCPA	0.000	8.911	0	20502437	N.D.	4.089



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102519\
Data File : PS007380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 03:29
Operator : SM\AJ
Sample : K5542-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:32:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

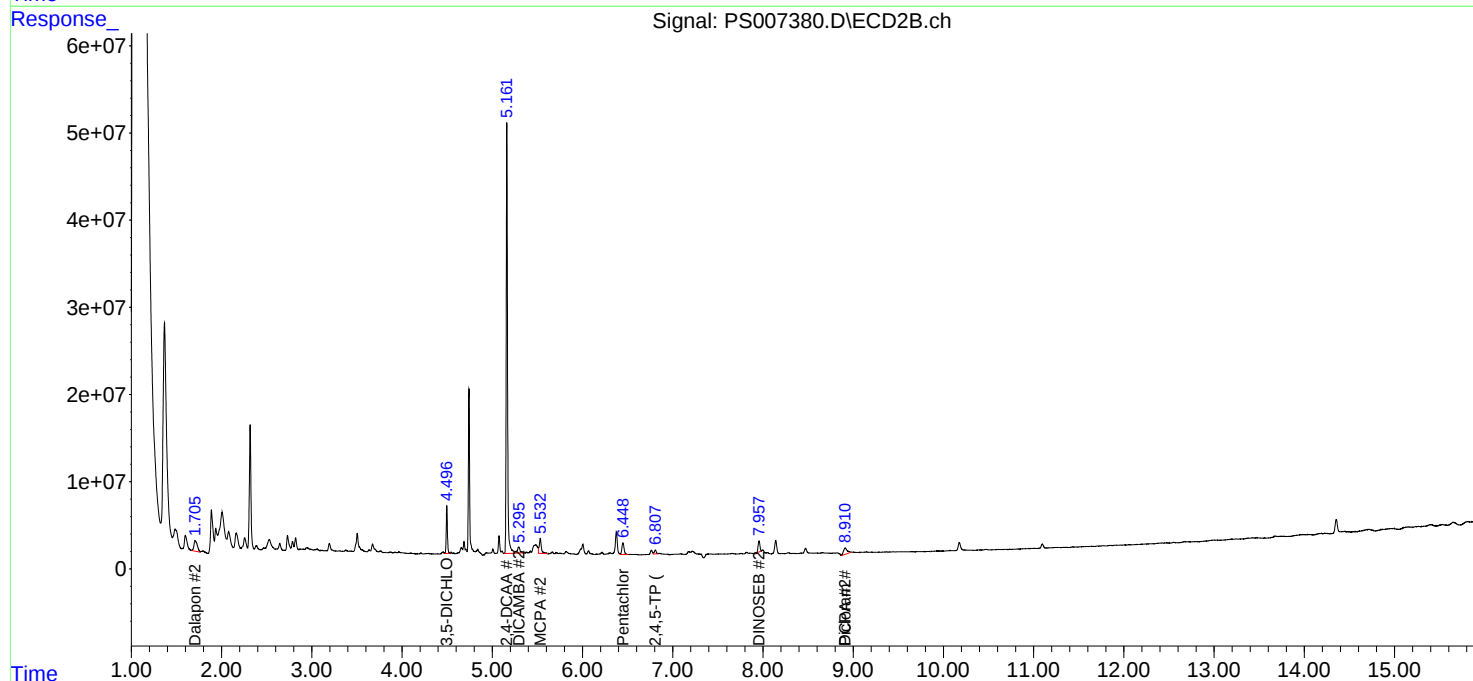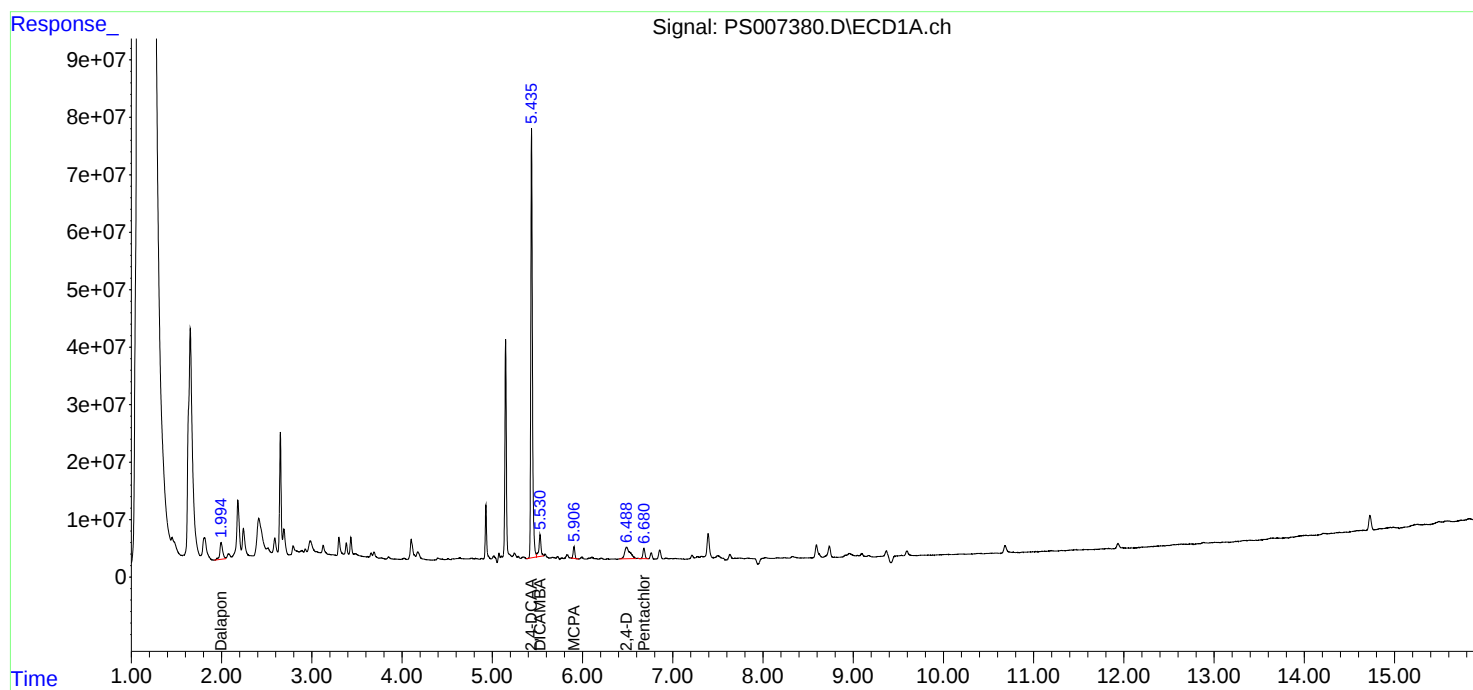


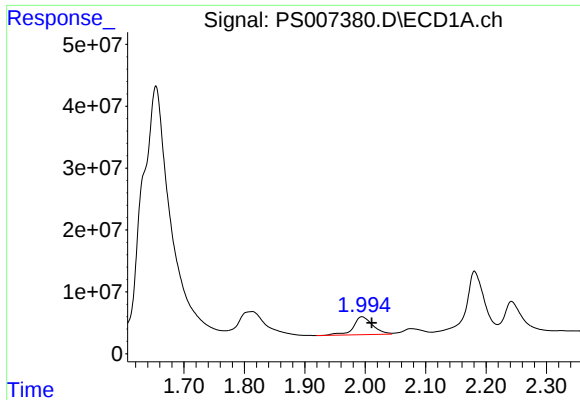

#1 Dalapon


R.T.: 1.995 min
Delta R.T.: -0.016 min
Response: 64430234
Conc: 38.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

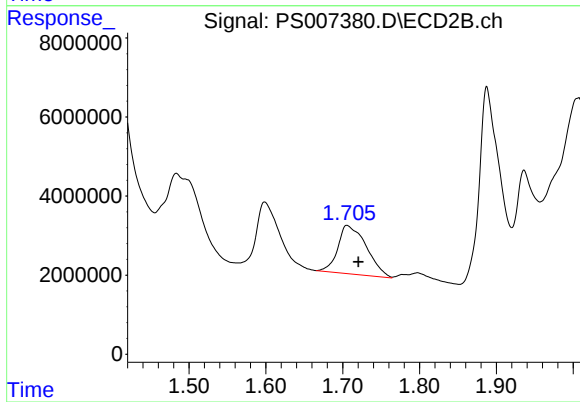


#1 Dalapon

R.T.: 1.706 min
Delta R.T.: -0.014 min
Response: 31614816
Conc: 34.74 ng/ml

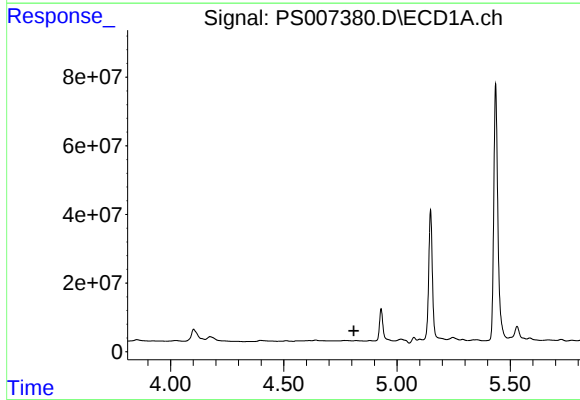


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

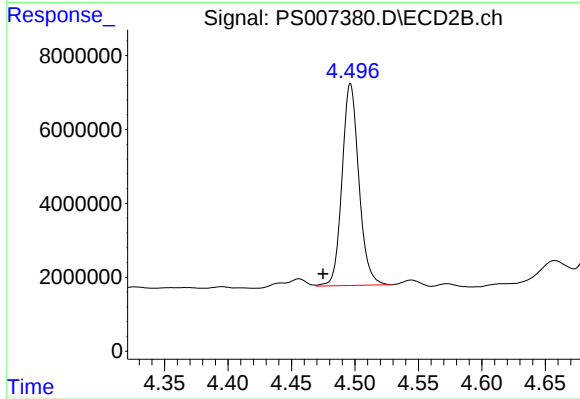

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.497 min
Delta R.T.: 0.022 min
Response: 50306694
Conc: 58.47 ng/ml

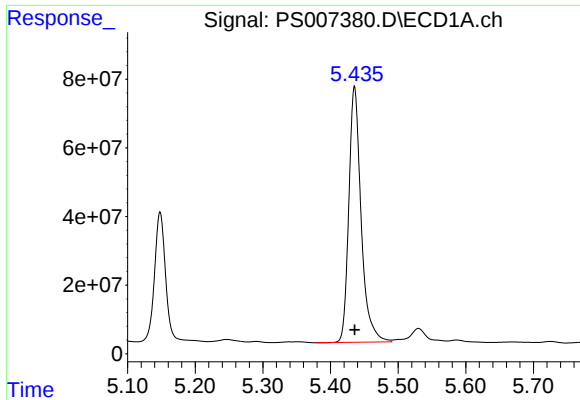

#4 2,4-DCAA


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 941190076
Conc: 687.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

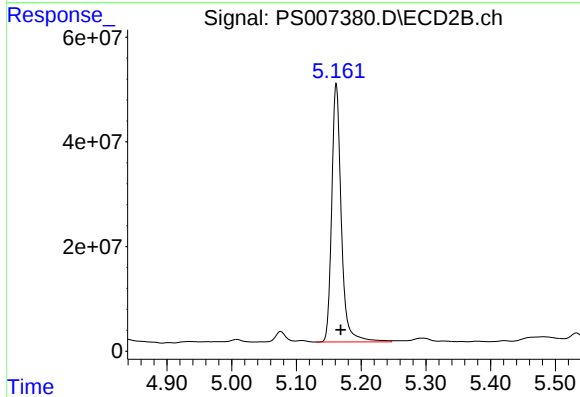


#4 2,4-DCAA

R.T.: 5.162 min
Delta R.T.: -0.007 min
Response: 507178587
Conc: 721.13 ng/ml

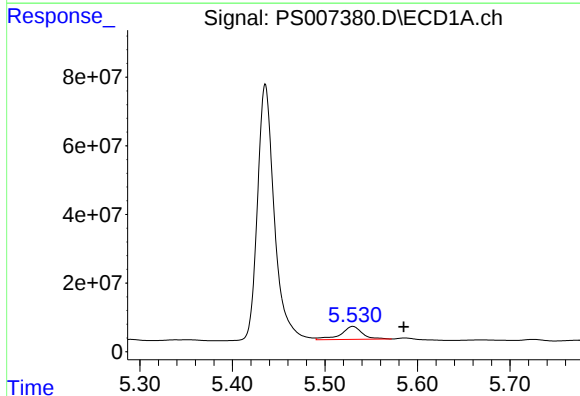


#5 DICAMBA

R.T.: 5.530 min
Delta R.T.: -0.055 min
Response: 61067241
Conc: 12.43 ng/ml

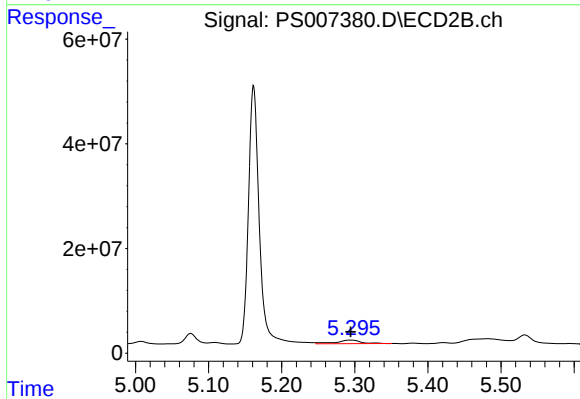

#5 DICAMBA


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 15798101
Conc: 6.07 ng/ml

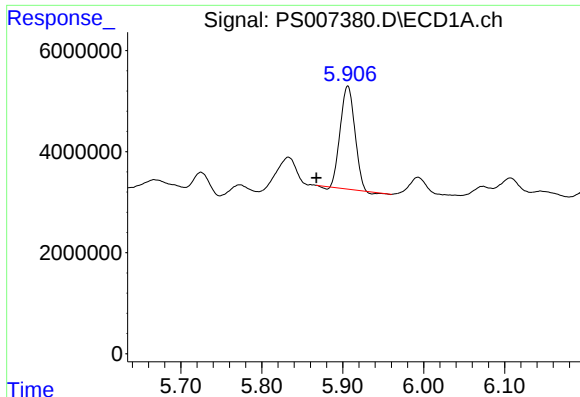

#7 MCPA


R.T.: 5.906 min
Delta R.T.: 0.039 min
Response: 25184945
Conc: 4.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

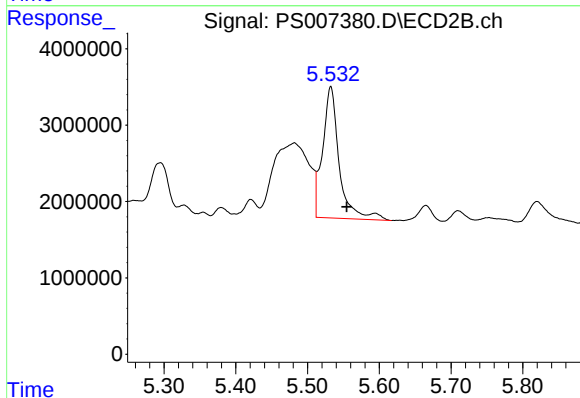


#7 MCPA

R.T.: 5.532 min
Delta R.T.: -0.022 min
Response: 27718356
Conc: 9.53 ug/ml

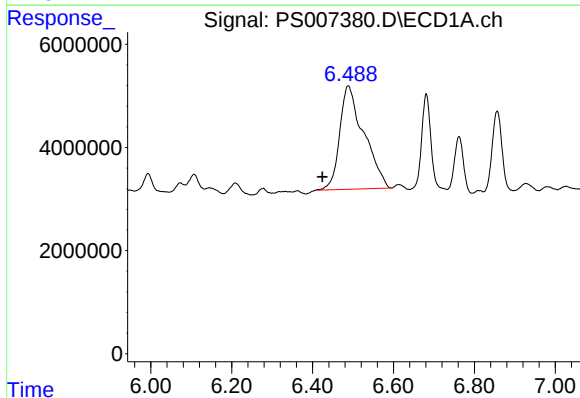


#9 2,4-D

R.T.: 6.488 min
Delta R.T.: 0.064 min
Response: 82977152
Conc: 67.33 ng/ml

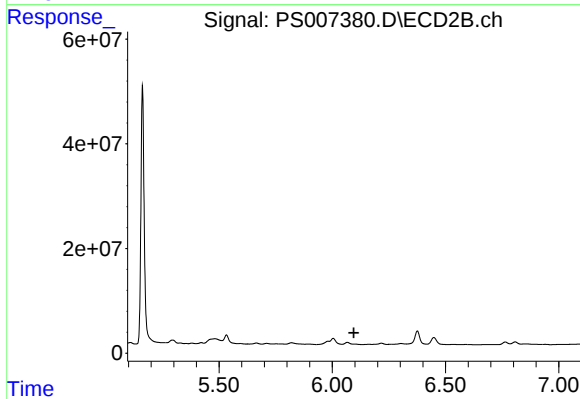

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

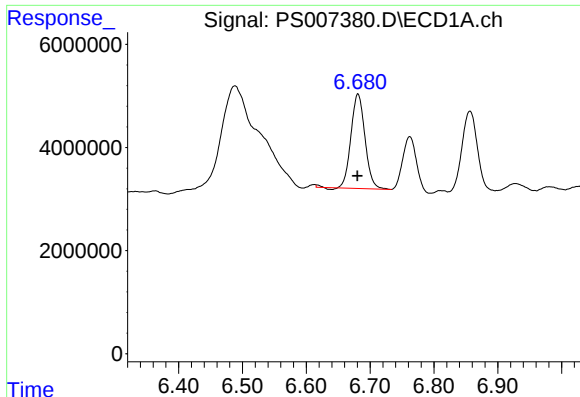

#10 Pentachlorophenol


R.T.: 6.681 min
Delta R.T.: 0.001 min
Response: 27872852
Conc: 1.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

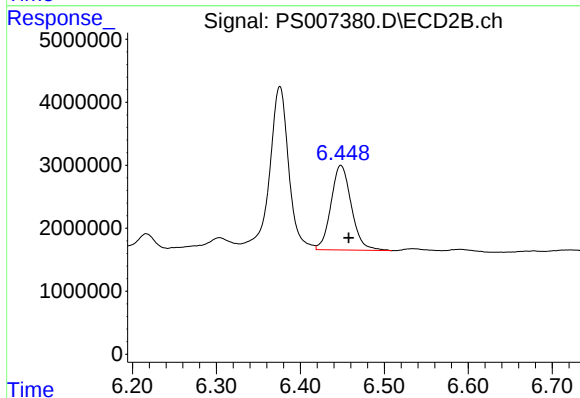


#10 Pentachlorophenol

R.T.: 6.448 min
Delta R.T.: -0.009 min
Response: 22684402
Conc: 2.36 ng/ml

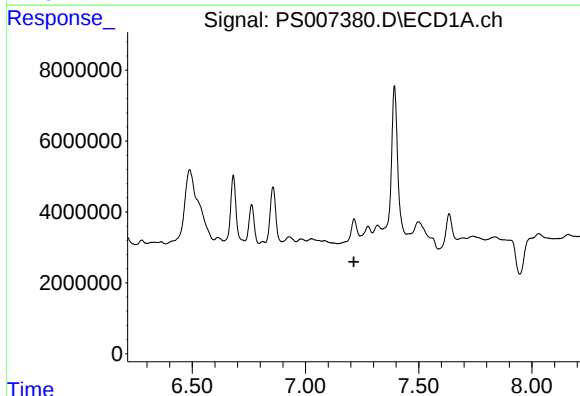


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

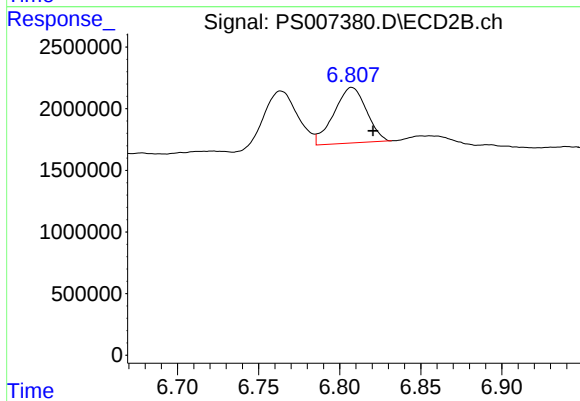

#11 2,4,5-TP (SILVEX)


R.T.: 6.808 min
Delta R.T.: -0.013 min
Response: 6305644
Conc: 1.66 ng/ml

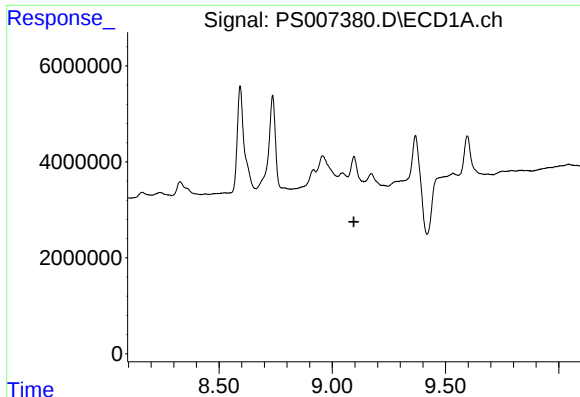

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

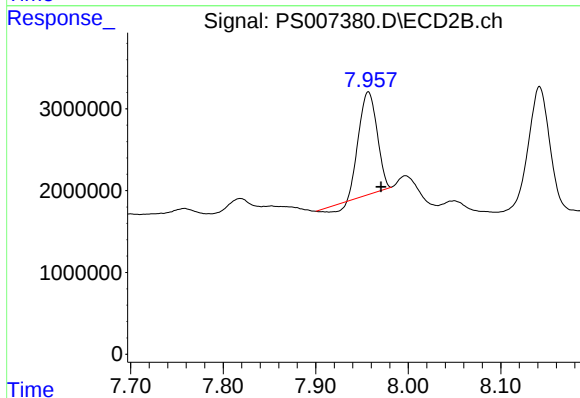


#14 DINOSEB

R.T.: 7.957 min
Delta R.T.: -0.014 min
Response: 16486243
Conc: 5.87 ng/ml

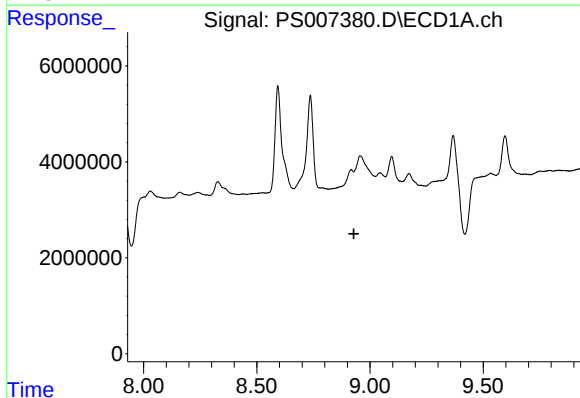


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

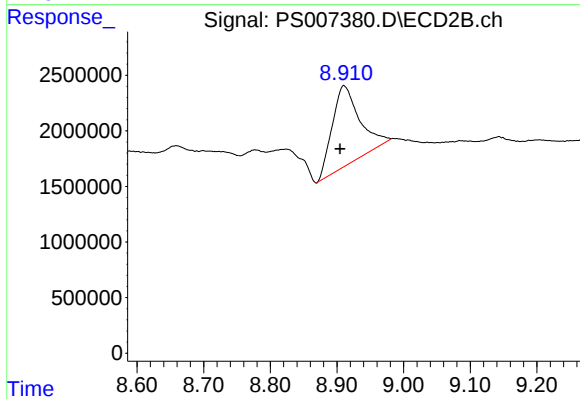

#15 Picloram


R.T.: 8.911 min
Delta R.T.: 0.006 min
Response: 20502437
Conc: 3.34 ng/ml

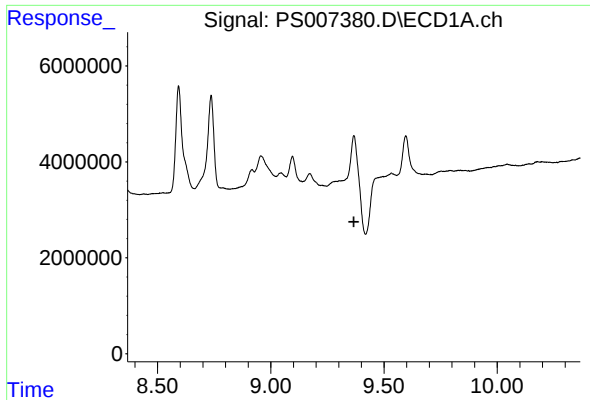

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

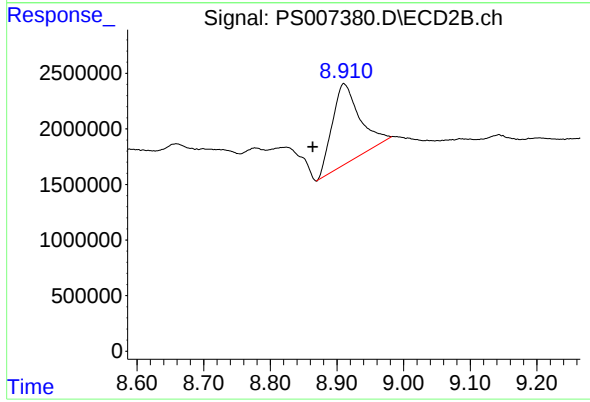

#16 DCPA

R.T.: 8.911 min
Delta R.T.: 0.047 min
Response: 20502437
Conc: 4.09 ng/ml