

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102521\
 Data File : PS017165.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2021 08:53
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 13:15:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.157	0.000	17915777	0	11.721	N.D.	#
Target Compounds								
5) T	DICAMBA	7.343	0.000	3135523	0	<MDL	N.D.	#
6) T	MCPD	7.578f	0.000	3384154	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.982f	0.000	2475250	0	1.651	N.D.	#
9) T	2,4-D	8.207f	0.000	2916735	0	1.647	N.D.	#
10) T	Pentachlo...	8.569	0.000	5354512	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.122	0.000	3460177	0	<MDL	N.D.	#
12) T	2,4,5-T	9.408	9.017f	7662010	7442729	<MDL	2.348	#
13) T	2,4-DB	9.884f	0.000	4854388	0	3.227	N.D.	#
14) T	DINOSEB	11.105	0.000	7806973	0	1.378	N.D.	#
15) T	Picloram	10.938	10.777	49851801	15575678	4.667	4.067	
16) T	DCPA	11.373	10.777f	8421517	15575678	<MDL	3.650	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102521\
Data File : PS017165.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2021 08:53
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 13:15:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

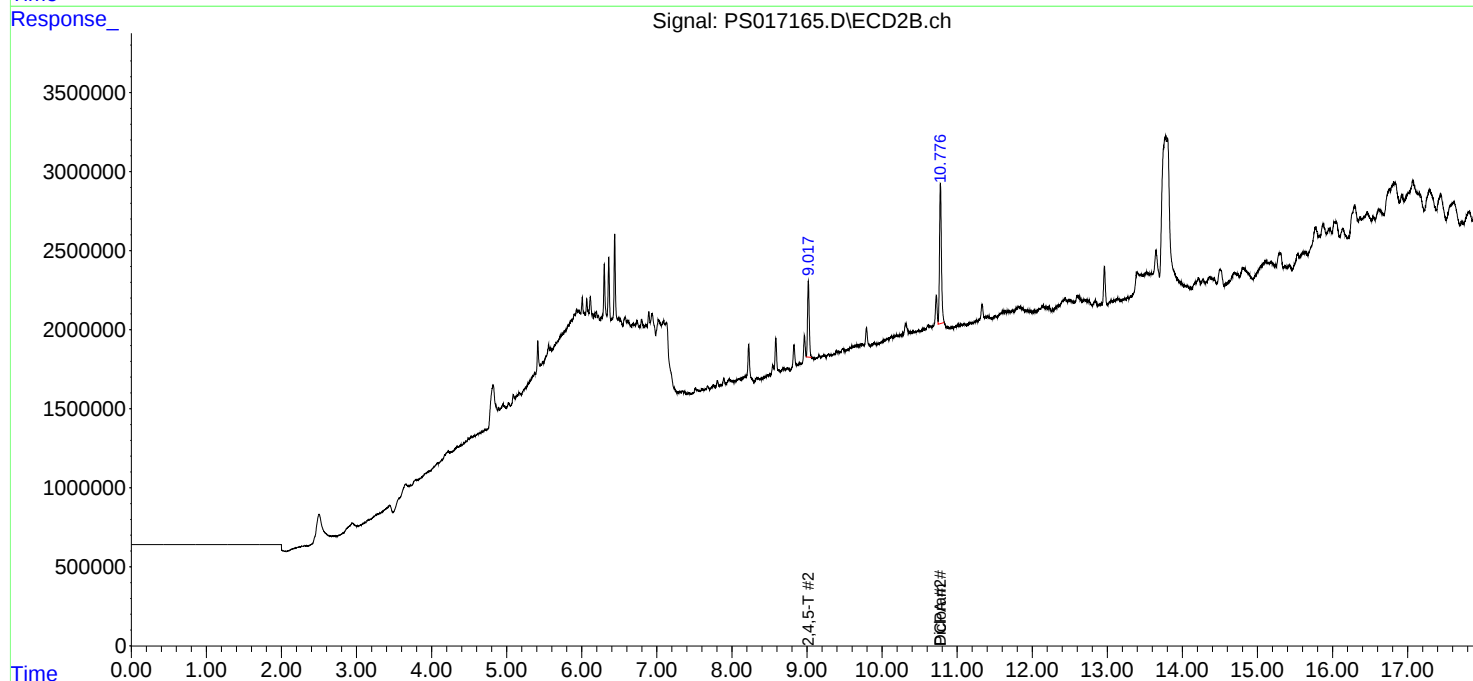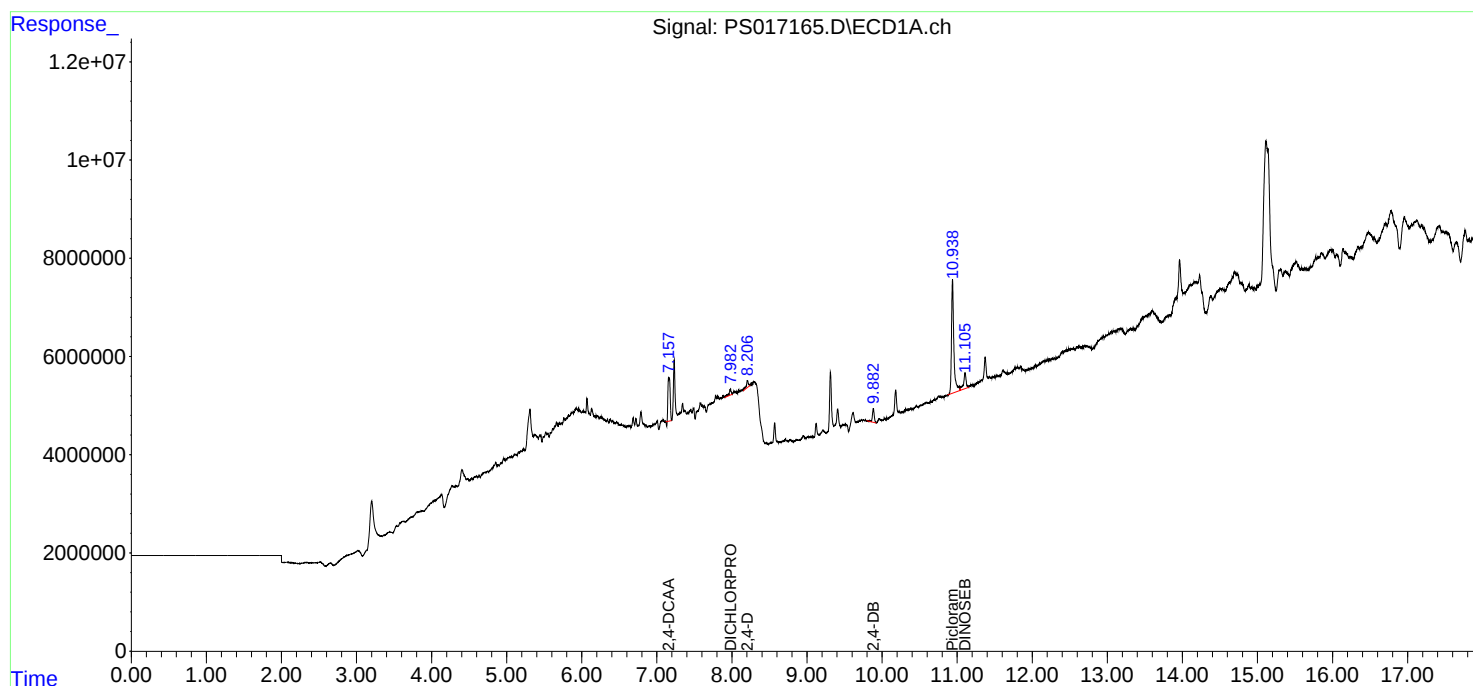


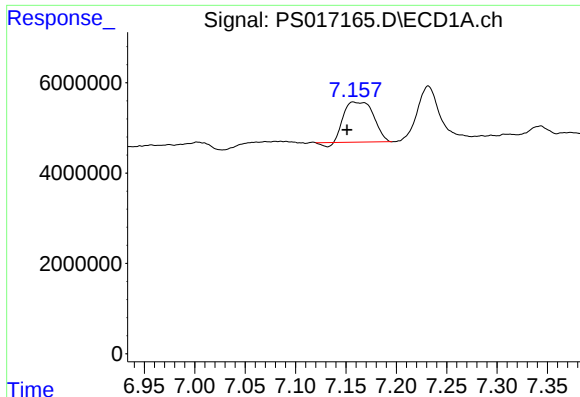

#4 2,4-DCAA


R.T.: 7.157 min
Delta R.T.: 0.006 min
Response: 17915777
Conc: 11.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

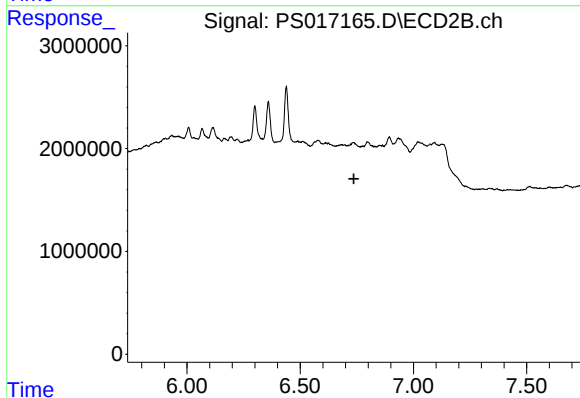


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

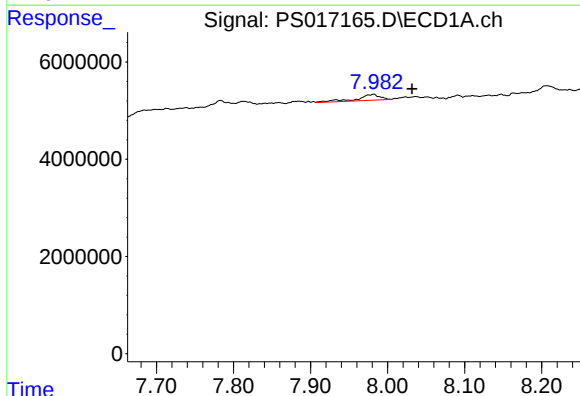


#8 DICHLORPROP

R.T.: 7.982 min
Delta R.T.: -0.050 min
Response: 2475250
Conc: 1.65 ng/ml

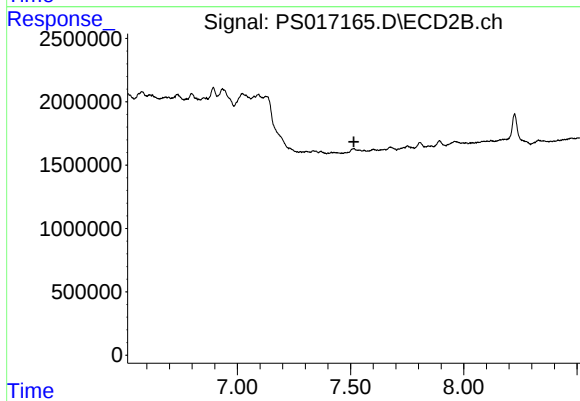

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

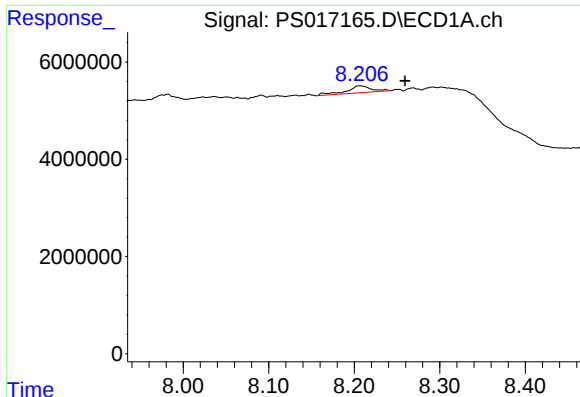

#9 2,4-D


R.T.: 8.207 min
Delta R.T.: -0.053 min
Response: 2916735
Conc: 1.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

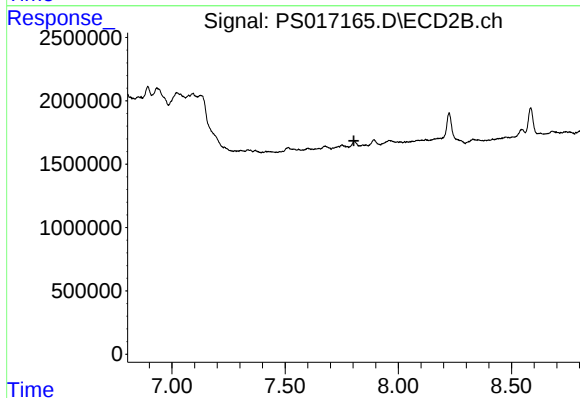


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.804 min
Response: 0
Conc: N.D.

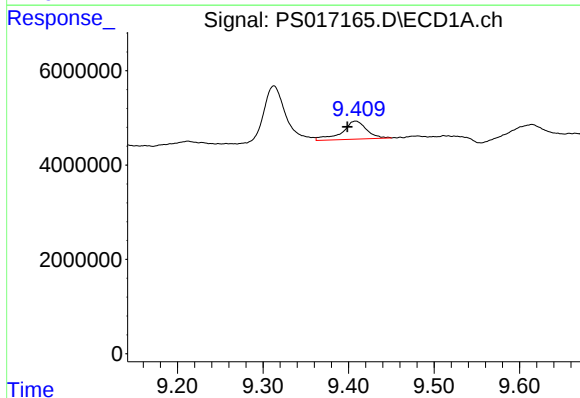


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: 0.010 min
Response: 7662010
Conc: N.D.

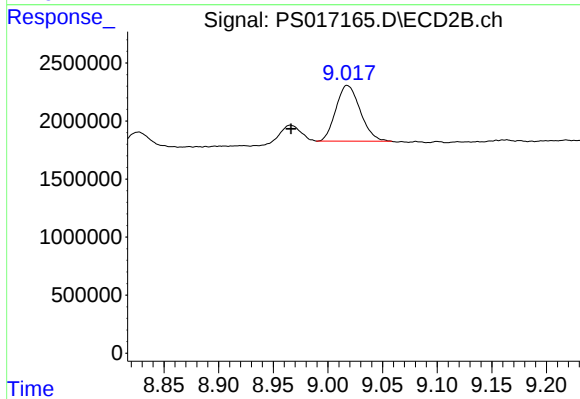

#12 2,4,5-T


R.T.: 9.017 min
Delta R.T.: 0.051 min
Response: 7442729
Conc: 2.35 ng/ml

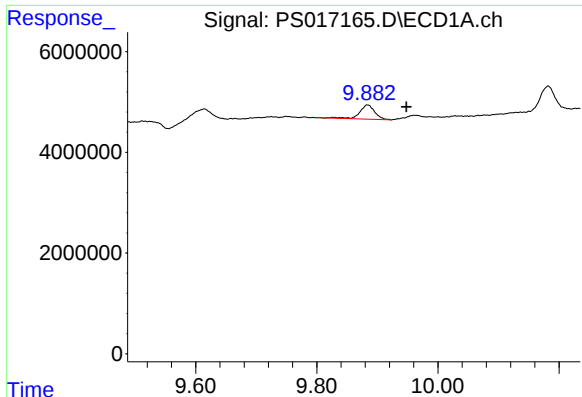

#13 2,4-DB


R.T.: 9.884 min
Delta R.T.: -0.064 min
Response: 4854388
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

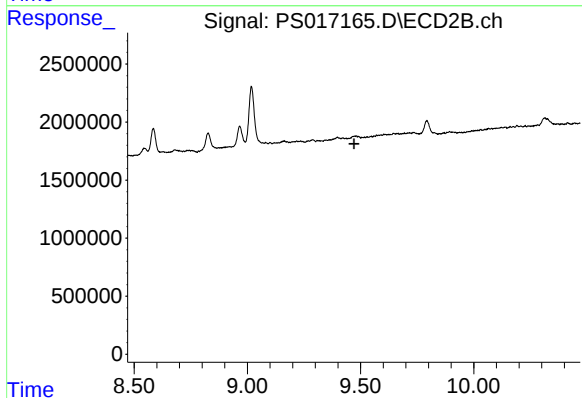


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

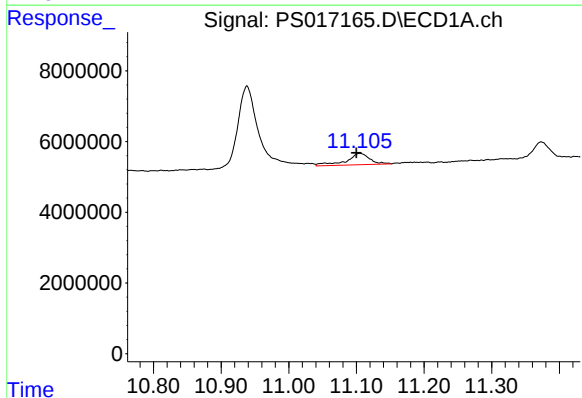


#14 DINOSEB

R.T.: 11.105 min
Delta R.T.: 0.005 min
Response: 7806973
Conc: 1.38 ng/ml

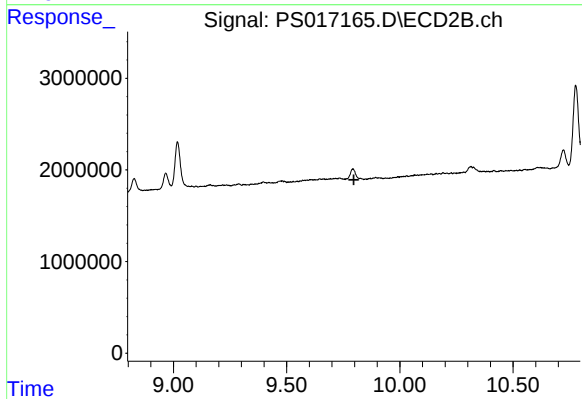

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.797 min
Response: 0
Conc: N.D.

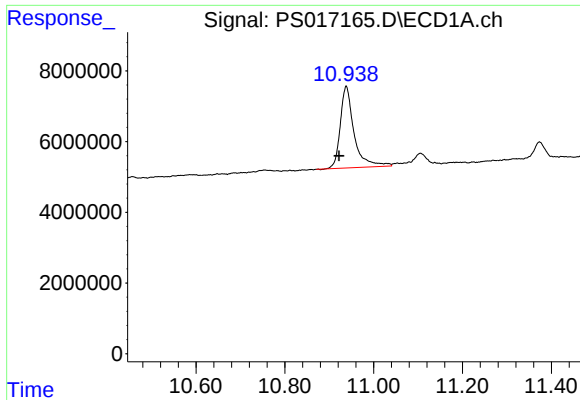

#15 Picloram


R.T.: 10.938 min
Delta R.T.: 0.016 min
Response: 49851801
Conc: 4.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

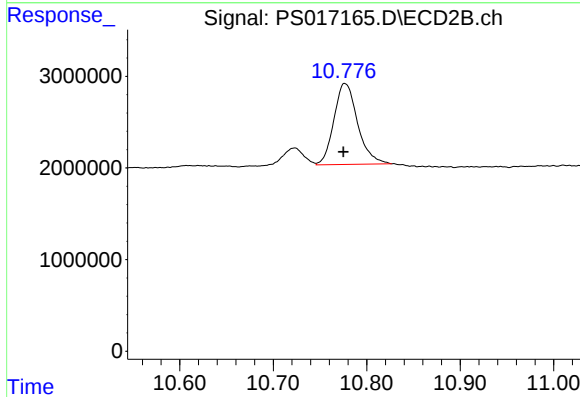


#15 Picloram

R.T.: 10.777 min
Delta R.T.: 0.002 min
Response: 15575678
Conc: 4.07 ng/ml

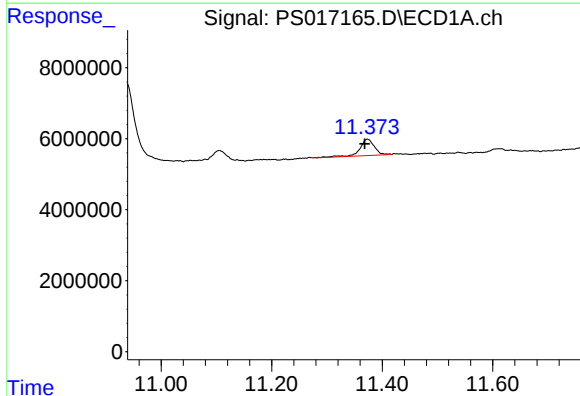

#16 DCPA

R.T.: 11.373 min
Delta R.T.: 0.005 min
Response: 8421517
Conc: N.D.

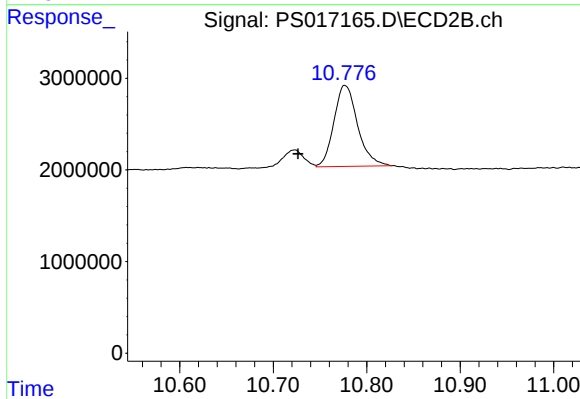

#16 DCPA

R.T.: 10.777 min
Delta R.T.: 0.050 min
Response: 15575678
Conc: 3.65 ng/ml