

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102522\
 Data File : PS020857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 09:11
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 21:42:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.414	0.000	219765	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.501	0.000	550968	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.774	0.000	9139781	0	3.042	N.D. #
3) T	4-Nitroph...	6.251	6.446	6231081	848747	<MDL	1.029 #
5) T	DICAMBA	6.555	0.000	381964	0	<MDL	N.D. #
6) T	MCPD	6.752	0.000	6226503	0	1.060	N.D. #
7) T	MCPA	6.857	0.000	338248	0	<MDL	N.D. #
8) T	DICHLORPROP	7.188	0.000	338906	0	<MDL	N.D. #
9) T	2,4-D	7.367	7.886f	1390651	1460237	<MDL	<MDL #
10) T	Pentachlo...	7.602	8.377	1044802	3170125	<MDL	<MDL #
11) T	2,4,5-TP ...	8.129	8.739	985445	2091446	<MDL	<MDL #
12) T	2,4,5-T	8.387	9.115	598130	1363959	<MDL	<MDL #
13) T	2,4-DB	8.878	0.000	260897	0	<MDL	N.D. #
14) T	DINOSEB	9.958	0.000	599951	0	<MDL	N.D. #
15) T	Picloram	9.784	10.924	17839717	9313923	1.071	<MDL #
16) T	DCPA	10.229	10.924	979499	9313923	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102522\
Data File : PS020857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 09:11
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 21:42:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

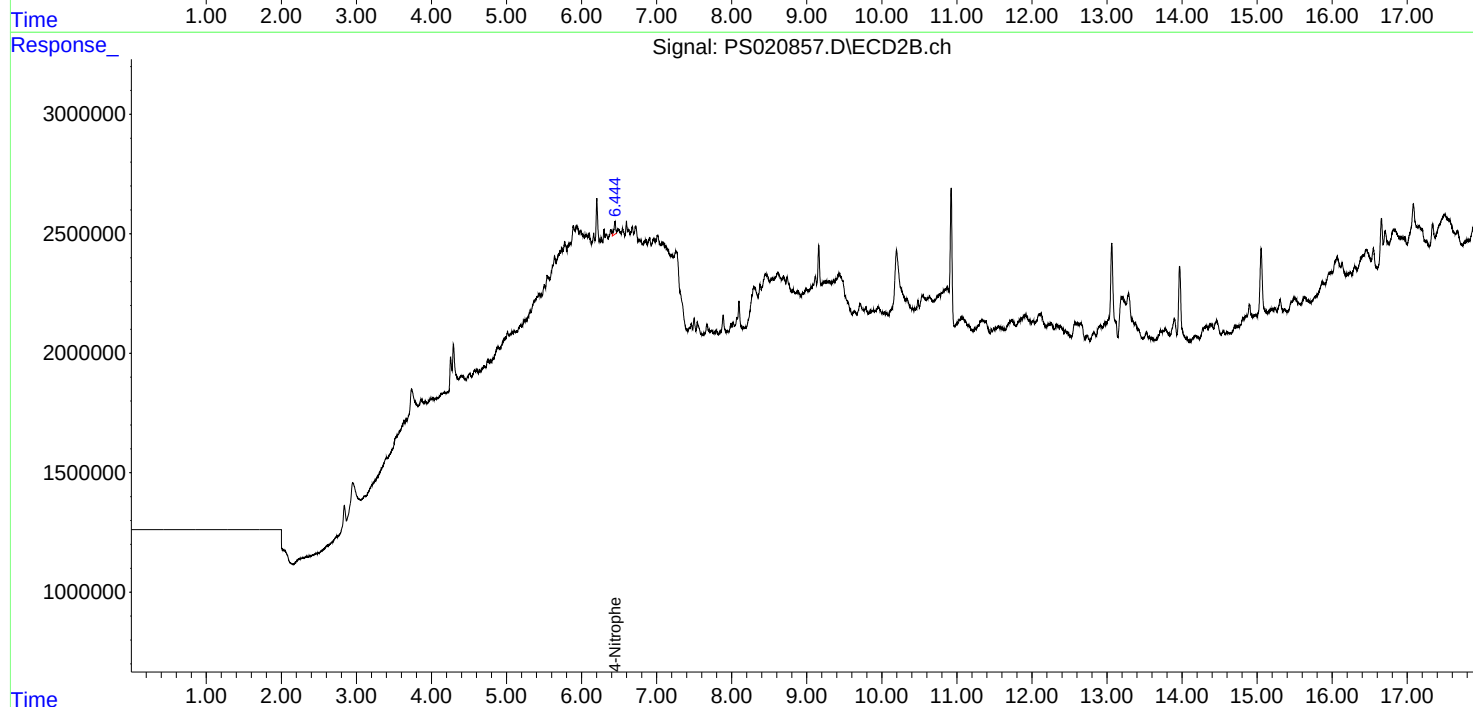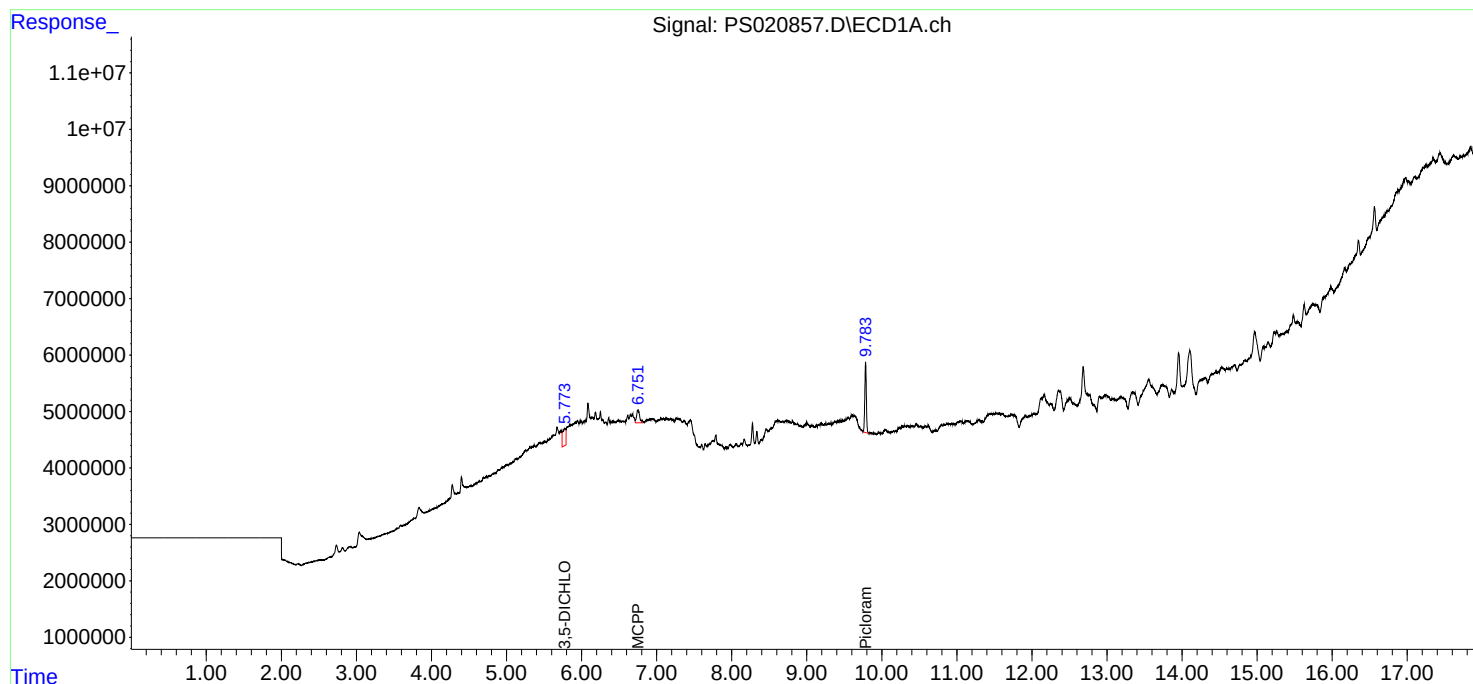


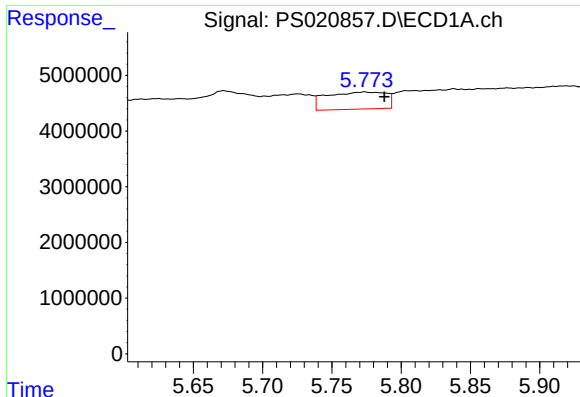

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.774 min
Delta R.T.: -0.014 min
Response: 9139781
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

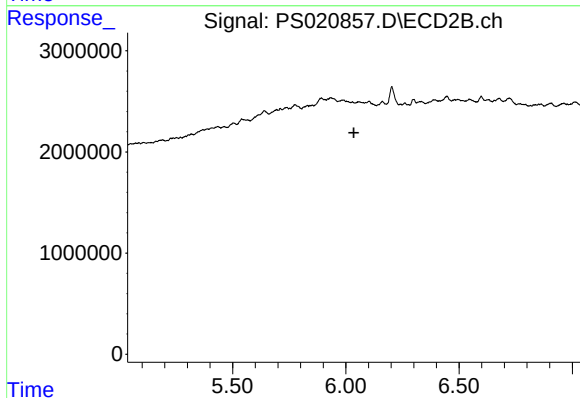


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

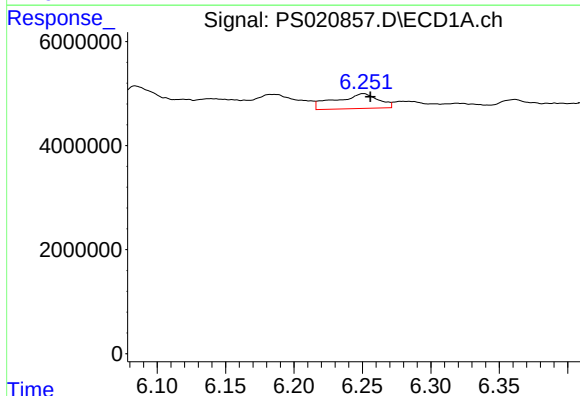


#3 4-Nitrophenol

R.T.: 6.251 min
Delta R.T.: -0.005 min
Response: 6231081
Conc: N.D.

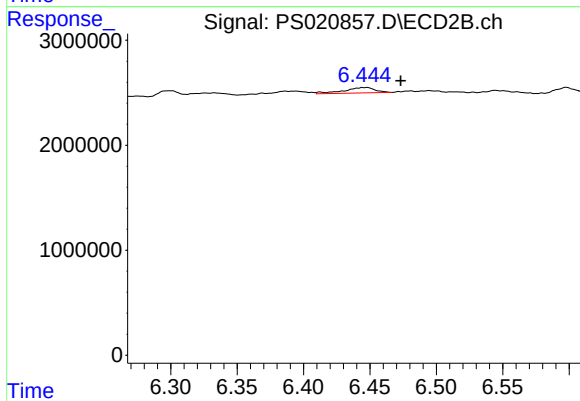

#3 4-Nitrophenol


R.T.: 6.446 min
Delta R.T.: -0.028 min
Response: 848747
Conc: 1.03 ng/ml

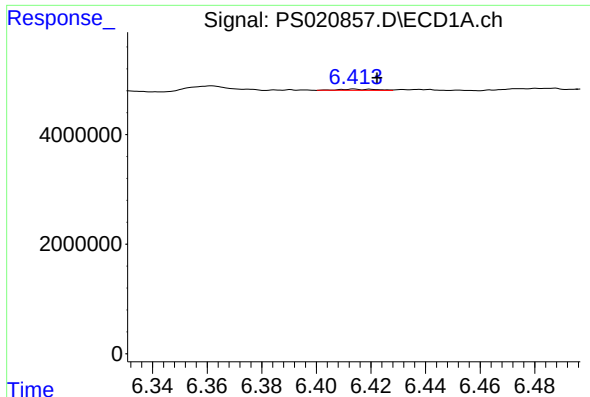

#4 2,4-DCAA


R.T.: 6.414 min
Delta R.T.: -0.008 min
Response: 219765
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

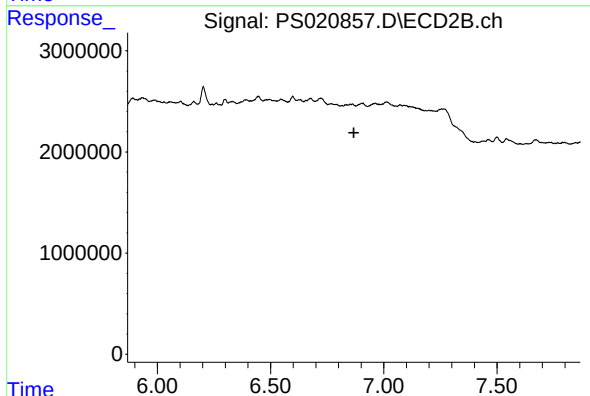


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.868 min
Response: 0
Conc: N.D.

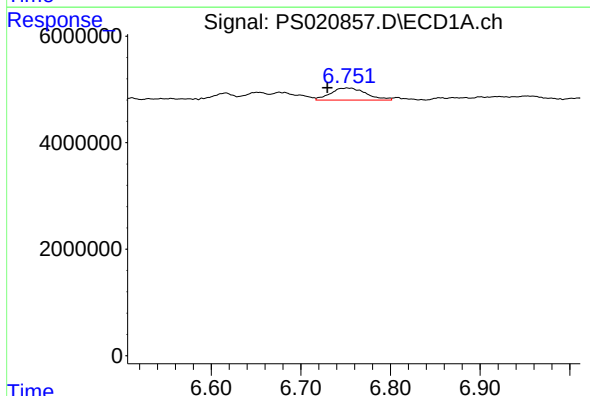


#6 MCP

R.T.: 6.752 min
Delta R.T.: 0.022 min
Response: 6226503
Conc: 1.06 ug/ml

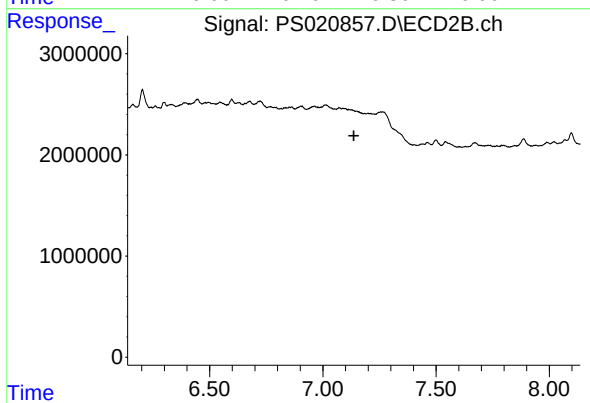

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.137 min
Response: 0
Conc: N.D.

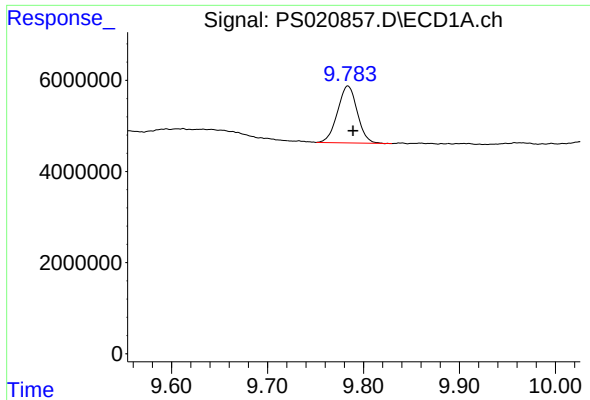

#15 Picloram

R.T.: 9.784 min
Delta R.T.: -0.005 min
Response: 17839717
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

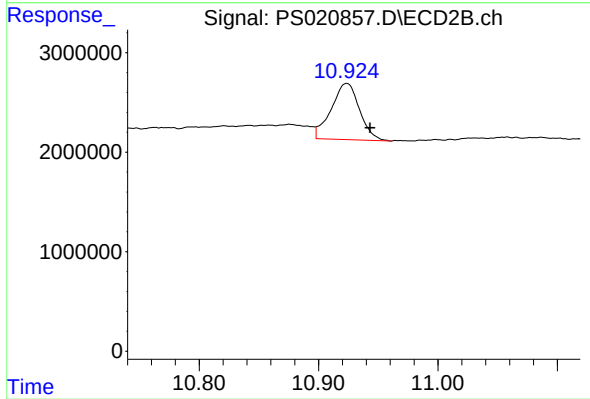

#15 Picloram

R.T.: 10.924 min
Delta R.T.: -0.020 min
Response: 9313923
Conc: N.D.