

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102522\
 Data File : PS020858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 09:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 21:43:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.415	6.856	1023.8E6	664.6E6	542.694	496.364
Target Compounds							
1) T	Dalapon	2.542	0.000	444320	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.797	6.105f	1275304	71184	<MDL	<MDL #
5) T	DICAMBA	6.608	0.000	910536	0	<MDL	N.D. #
6) T	MCP	6.744	0.000	2742934	0	<MDL	N.D. #
7) T	MCPA	6.920f	0.000	162081	0	<MDL	N.D. #
8) T	DICHLORPROP	7.209	0.000	1411695	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.127	0.000	987301	0	<MDL	N.D. #
12) T	2,4,5-T	8.385	9.160	879055	2109889	<MDL	<MDL #
13) T	2,4-DB	8.837f	0.000	1679571	0	<MDL	N.D. #
14) T	DINOSEB	9.958	0.000	505155	0	<MDL	N.D. #
15) T	Picloram	9.778	10.924	17792115	12999874	1.068	1.103
16) T	DCPA	10.216	10.924	1455904	12999874	<MDL	1.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102522\
Data File : PS020858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 09:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 21:43:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

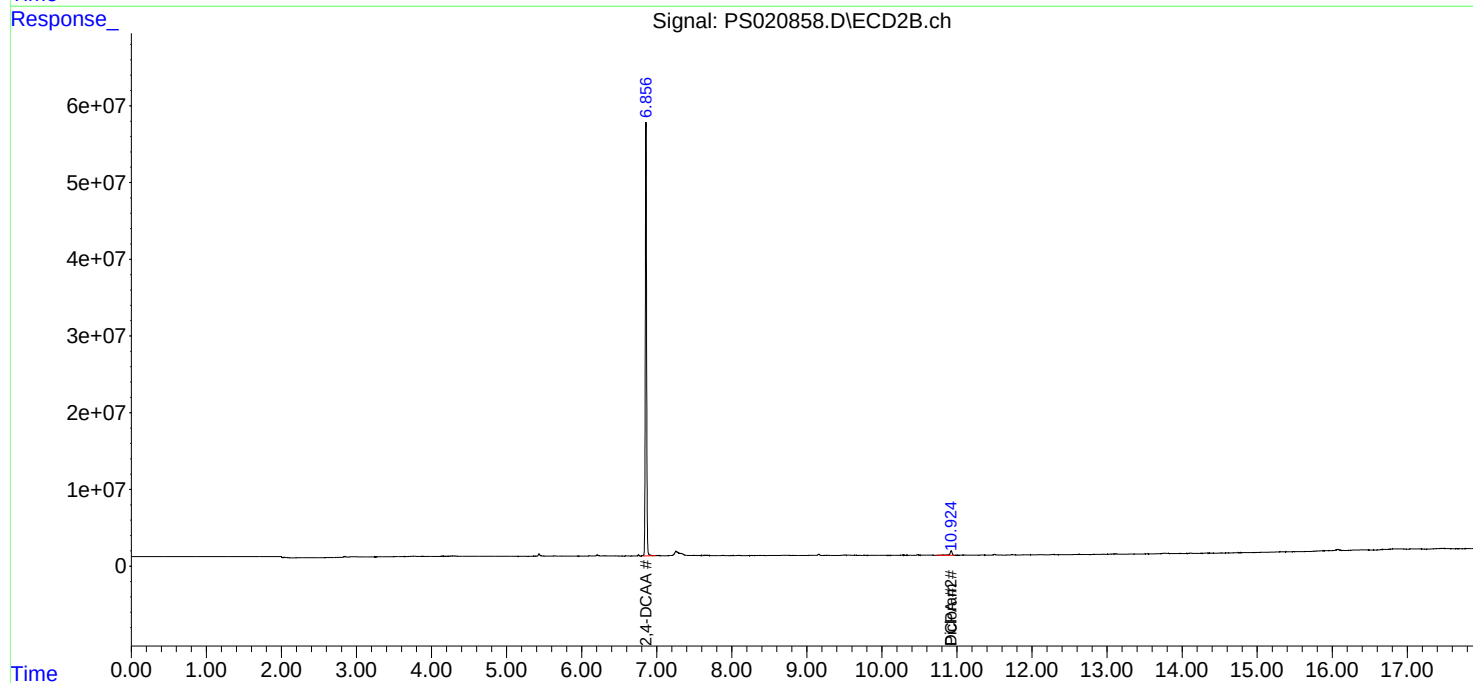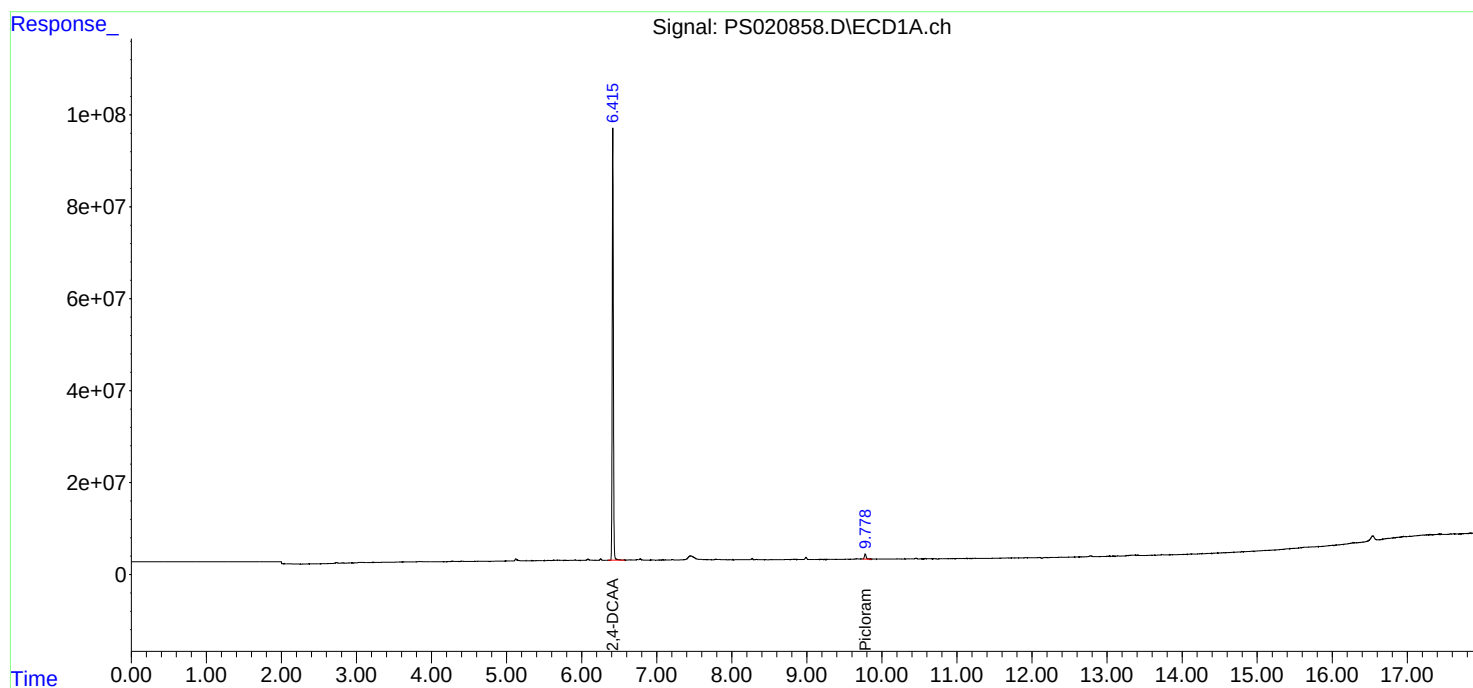


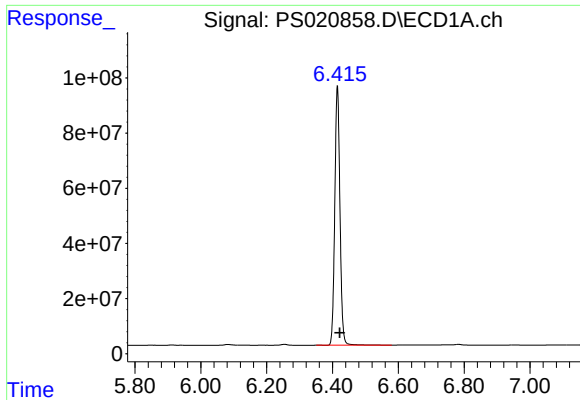

#4 2,4-DCAA


R.T.: 6.415 min
Delta R.T.: -0.007 min
Response: 1023764586
Conc: 542.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

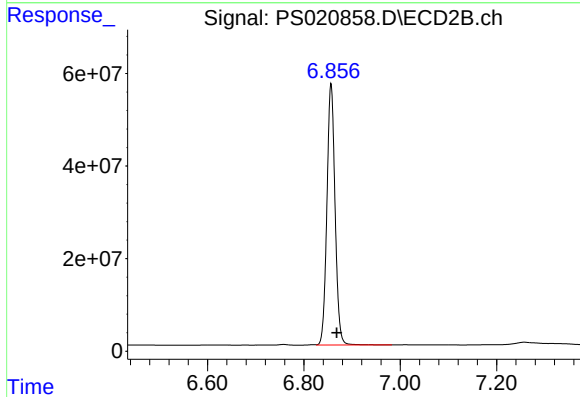


#4 2,4-DCAA

R.T.: 6.856 min
Delta R.T.: -0.012 min
Response: 664622042
Conc: 496.36 ng/ml

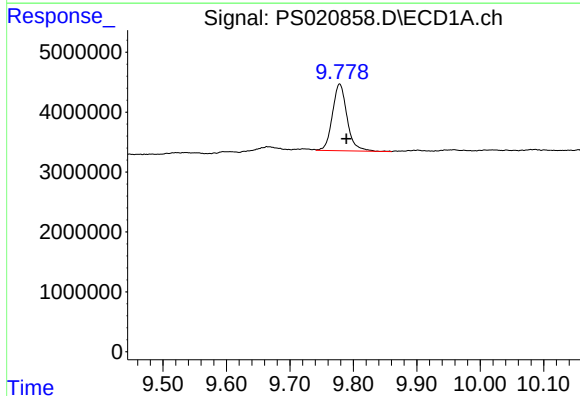


#15 Picloram

R.T.: 9.778 min
Delta R.T.: -0.011 min
Response: 17792115
Conc: 1.07 ng/ml

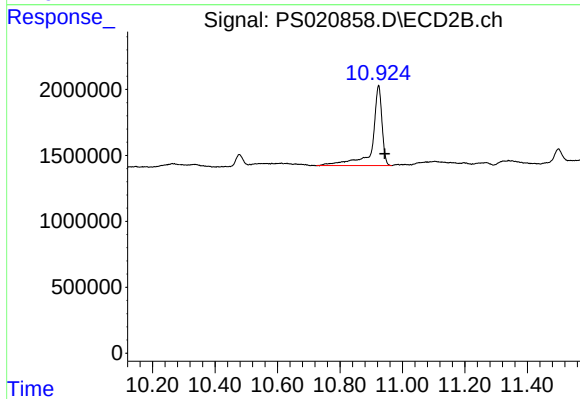

#15 Picloram


R.T.: 10.924 min
Delta R.T.: -0.019 min
Response: 12999874
Conc: 1.10 ng/ml

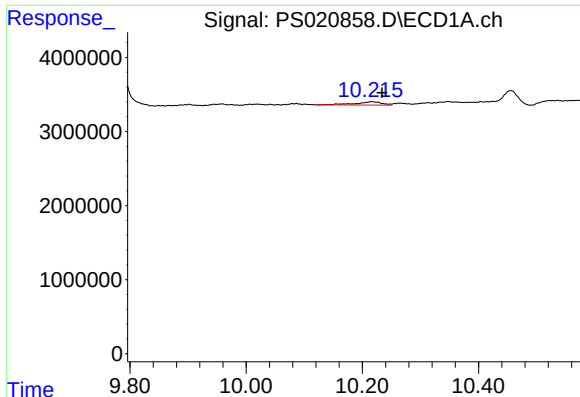

#16 DCPA

R.T.: 10.216 min
Delta R.T.: -0.018 min
Response: 1455904
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

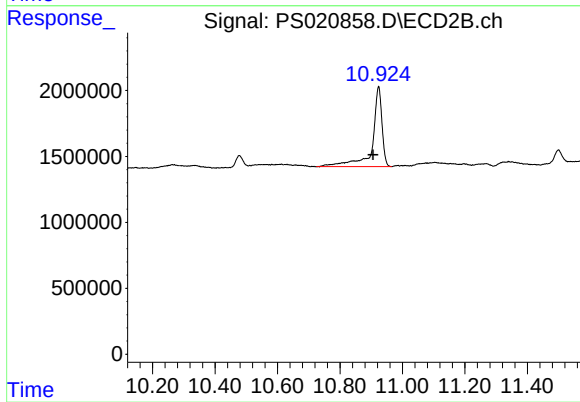

#16 DCPA

R.T.: 10.924 min
Delta R.T.: 0.017 min
Response: 12999874
Conc: 1.27 ng/ml