

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
 Data File : PS024704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 09:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 12:45:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.327	6.838f	14999732	396899	7.291	<MDL #
Target Compounds							
1) T	Dalapon	0.000	2.562	0	2369538	N.D.	2.117
2) T	3,5-DICHL...	5.699	6.030f	790.9E6	104448	252.145	<MDL #
3) T	4-Nitroph...	0.000	6.396	0	30032	N.D.	<MDL
5) T	DICAMBA	0.000	6.978	0	690.7E6	N.D.	233.241
6) T	MCP	6.680	6.978f	5677429	690.7E6	<MDL	350.499 #
8) T	DICHLORPROP	7.081	7.562	4688977	3820410	1.995	5.080 #
9) T	2,4-D	7.248	7.866	4268.1E6	797930	1544.745	<MDL #
11) T	2,4,5-TP ...	8.045	8.615	8934366	554333	<MDL	<MDL #
12) T	2,4,5-T	0.000	9.029	0	1943270	N.D.	<MDL
13) T	2,4-DB	0.000	9.477	0	329136	N.D.	<MDL
15) T	Picloram	9.658	10.771	190.6E6	30751584	10.929	4.948 #
16) T	DCPA	0.000	10.771	0	30751584	N.D.	5.894



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
Data File : PS024704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 09:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 12:45:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

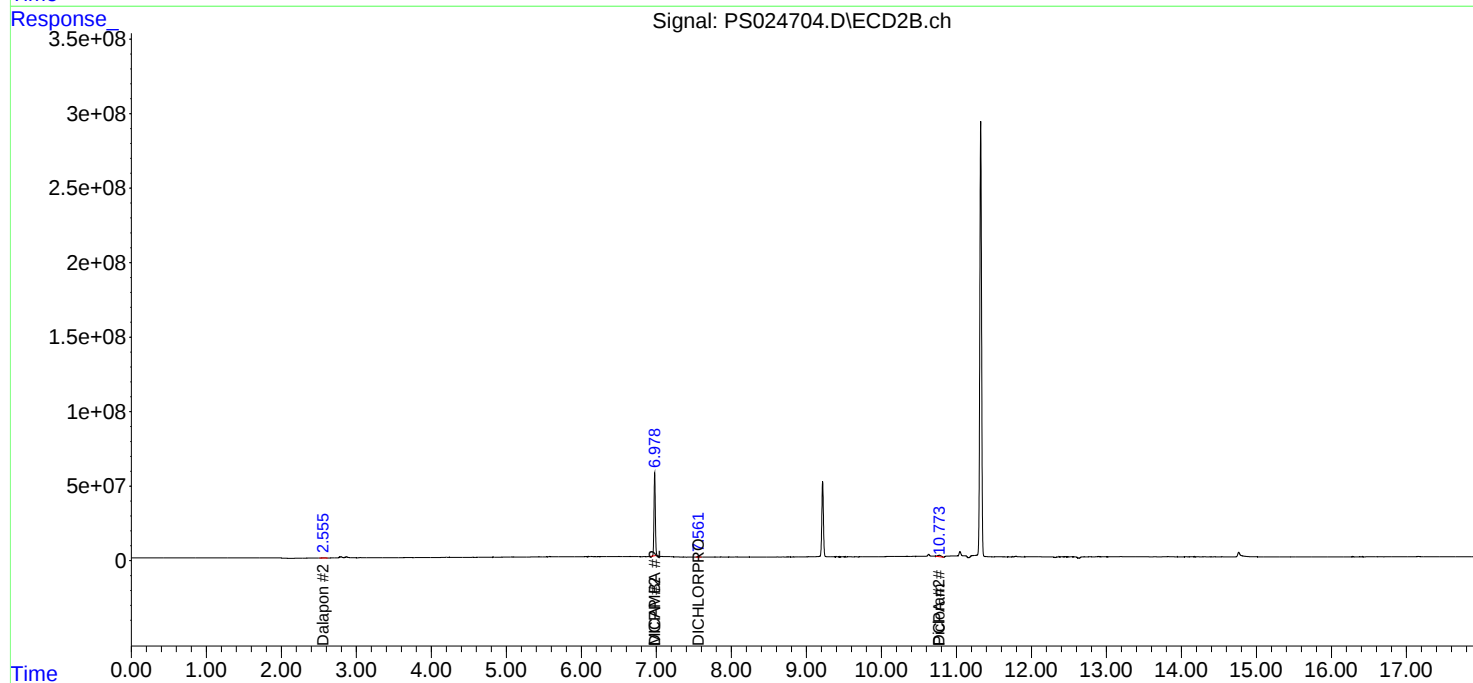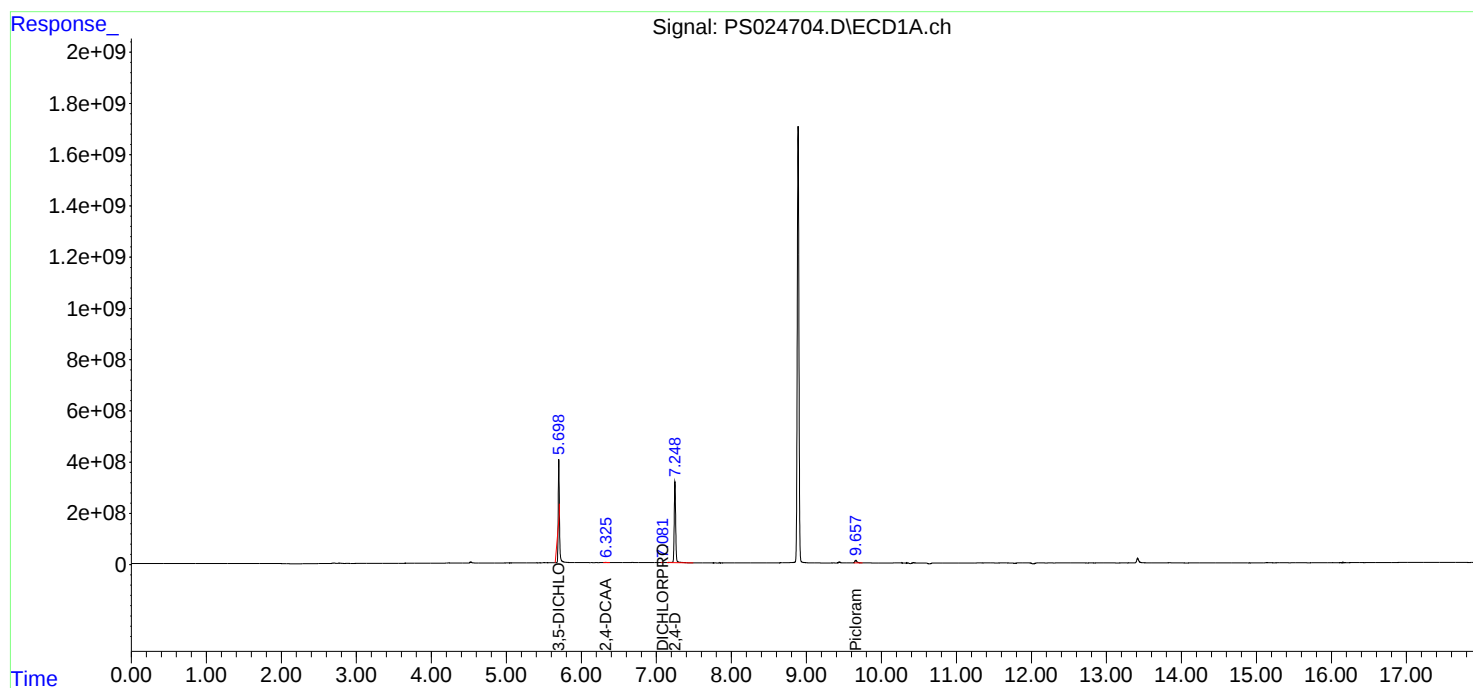


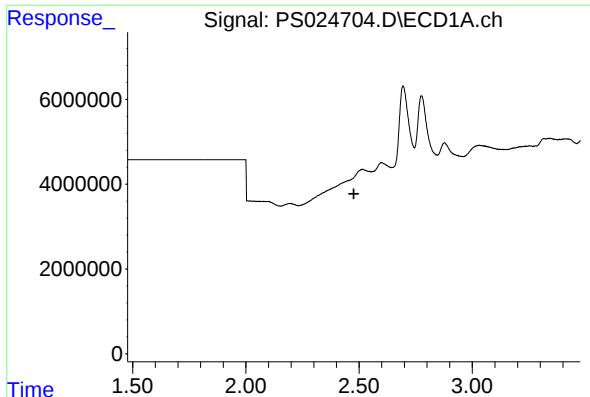

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

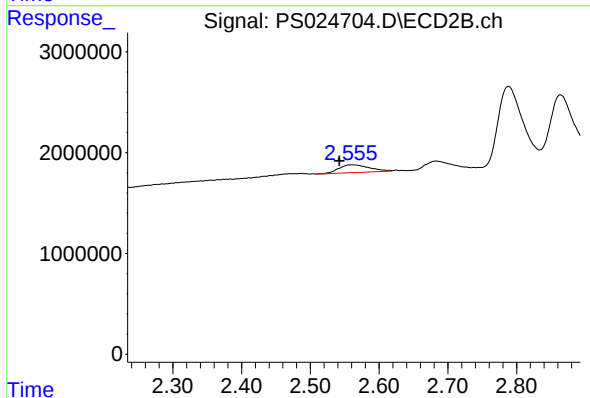


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.020 min
Response: 2369538
Conc: 2.12 ng/ml

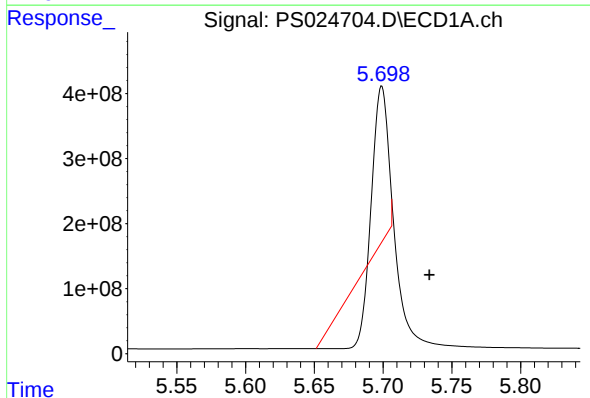


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.699 min
Delta R.T.: -0.035 min
Response: 790923311
Conc: 252.14 ng/ml

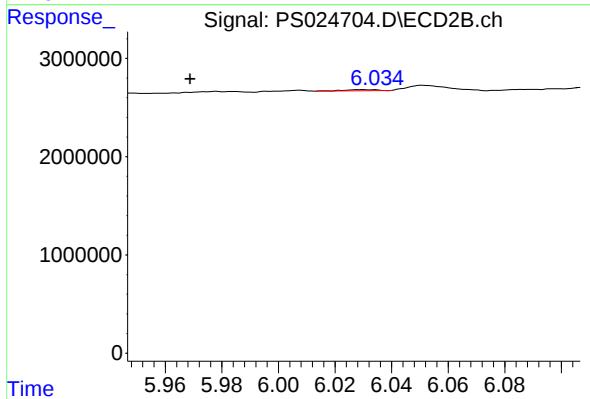

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.030 min
Delta R.T.: 0.061 min
Response: 104448
Conc: N.D.

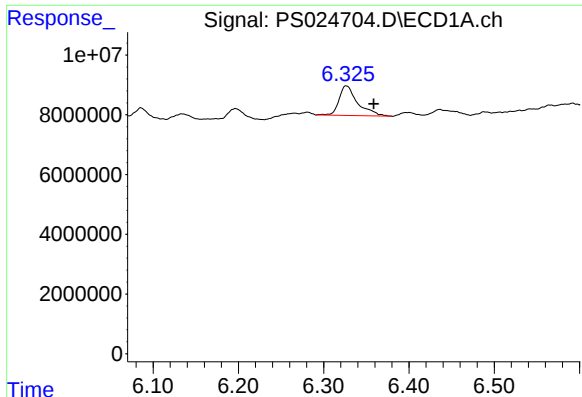

#4 2,4-DCAA


R.T.: 6.327 min
Delta R.T.: -0.032 min
Response: 14999732
Conc: 7.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

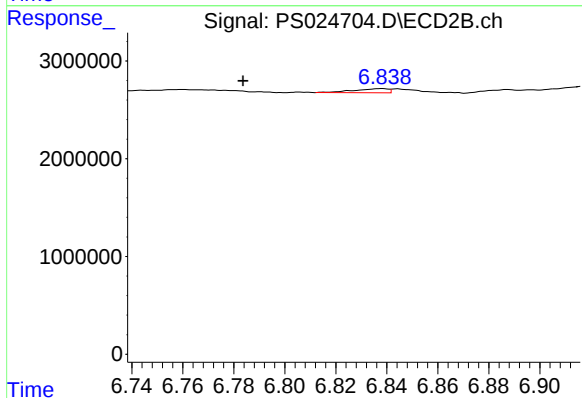


#4 2,4-DCAA

R.T.: 6.838 min
Delta R.T.: 0.055 min
Response: 396899
Conc: N.D.

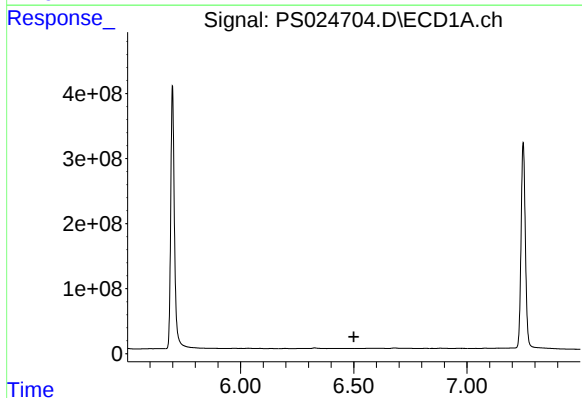


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.501 min
Response: 0
Conc: N.D.

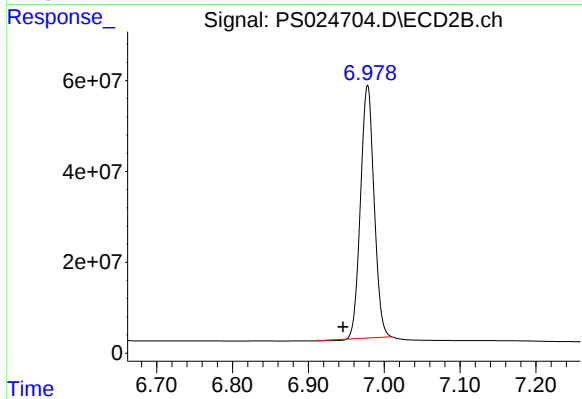

#5 DICAMBA


R.T.: 6.978 min
Delta R.T.: 0.033 min
Response: 690696126
Conc: 233.24 ng/ml

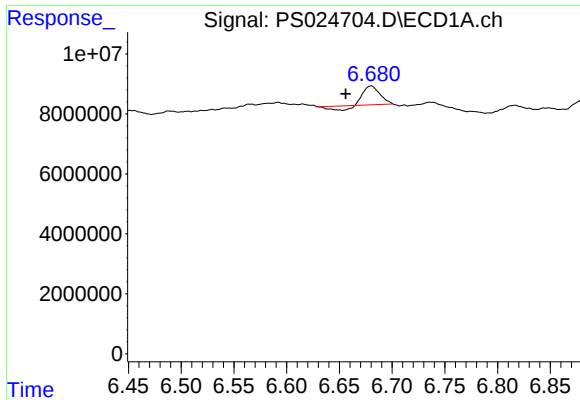

#6 MCP


R.T.: 6.680 min
Delta R.T.: 0.024 min
Response: 5677429
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

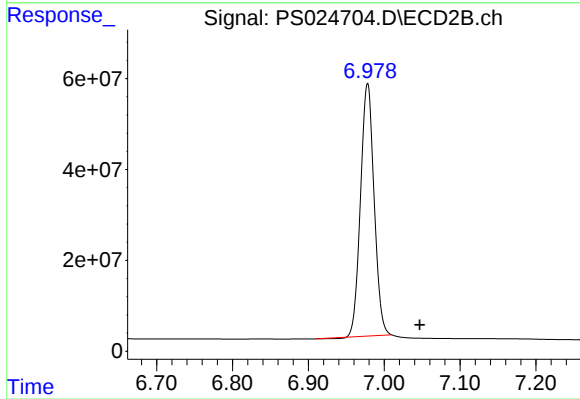


#6 MCP

R.T.: 6.978 min
Delta R.T.: -0.069 min
Response: 690696126
Conc: 350.50 ug/ml

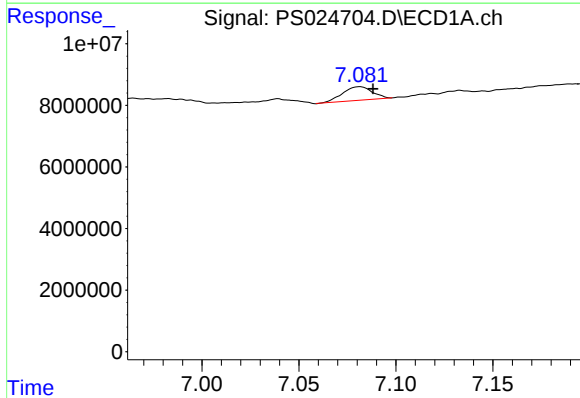


#8 DICHLORPROP

R.T.: 7.081 min
Delta R.T.: -0.007 min
Response: 4688977
Conc: 1.99 ng/ml

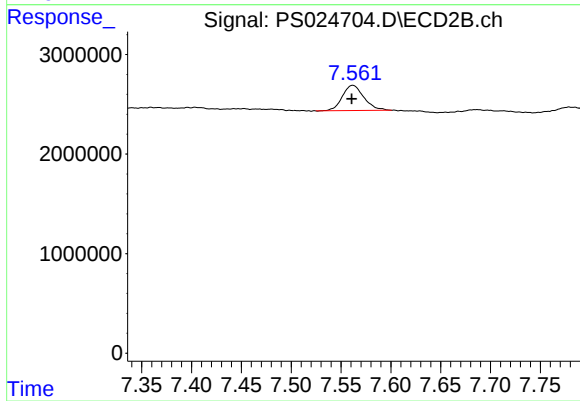

#8 DICHLORPROP


R.T.: 7.562 min
Delta R.T.: 0.001 min
Response: 3820410
Conc: 5.08 ng/ml

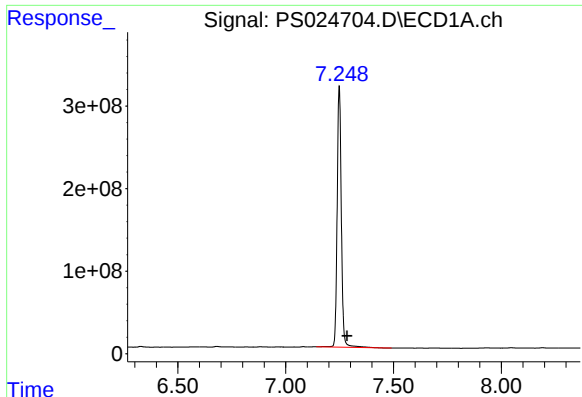

#9 2,4-D


R.T.: 7.248 min
Delta R.T.: -0.036 min
Response: 4268121129
Conc: 1544.75 ng/m

Instrument :
ECD_S
ClientSampleId :

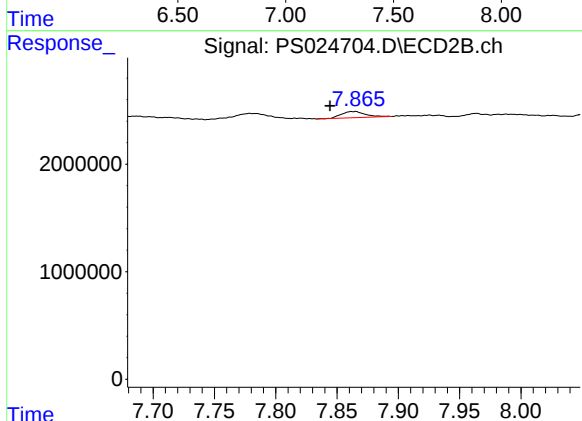


#9 2,4-D

R.T.: 7.866 min
Delta R.T.: 0.021 min
Response: 797930
Conc: N.D.

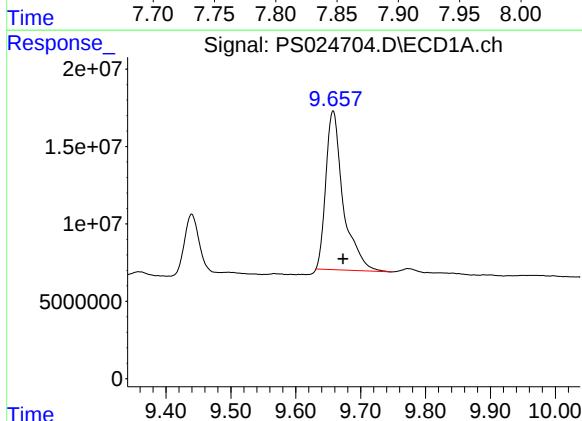


#15 Picloram

R.T.: 9.658 min
Delta R.T.: -0.016 min
Response: 190566318
Conc: 10.93 ng/ml

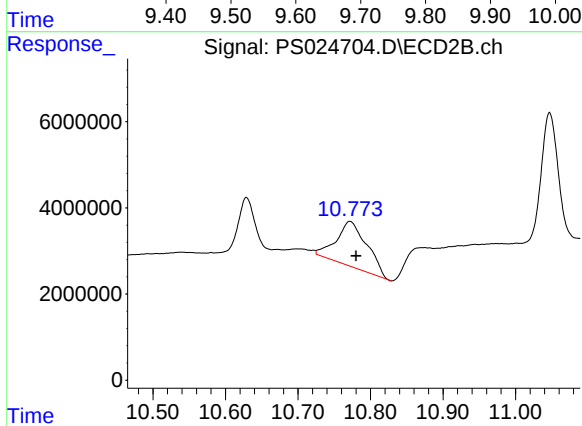

#15 Picloram


R.T.: 10.771 min
Delta R.T.: -0.009 min
Response: 30751584
Conc: 4.95 ng/ml

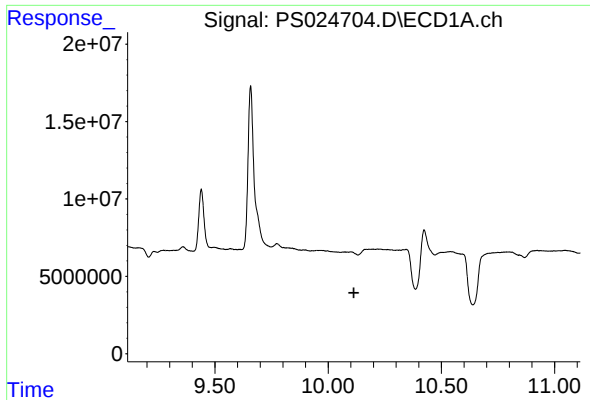

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

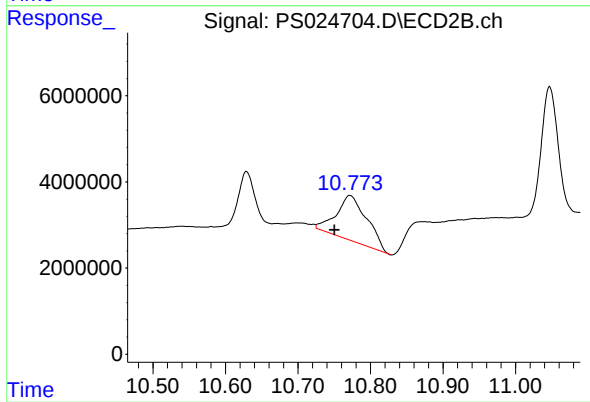

#16 DCPA

R.T.: 10.771 min
Delta R.T.: 0.021 min
Response: 30751584
Conc: 5.89 ng/ml