

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
 Data File : PS024705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 10:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 12:45:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.777	962.8E6	314.5E6	467.997	454.981
Target Compounds							
1) T	Dalapon	0.000	2.570	0	3046727	N.D.	2.722
2) T	3,5-DICHL...	5.697	0.000	537557	0	<MDL	N.D. #
3) T	4-Nitroph...	6.198	0.000	7429371	0	5.488	N.D. #
5) T	DICAMBA	0.000	6.978	0	1380701	N.D.	<MDL
6) T	MCPD	0.000	6.978f	0	1380701	N.D.	<MDL
7) T	MCPA	0.000	7.247	0	5558809	N.D.	1.735
8) T	DICHLORPROP	0.000	7.568	0	1750507	N.D.	2.328
9) T	2,4-D	7.249	7.783f	8751038	1063655	3.167	1.156 #
11) T	2,4,5-TP ...	0.000	8.618	0	535413	N.D.	<MDL
12) T	2,4,5-T	0.000	9.032	0	2021774	N.D.	<MDL
13) T	2,4-DB	0.000	9.481	0	680007	N.D.	1.334
15) T	Picloram	9.687	10.775	36705373	10197874	2.105	1.641
16) T	DCPA	0.000	10.775	0	10197874	N.D.	1.955



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
Data File : PS024705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 10:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 12:45:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

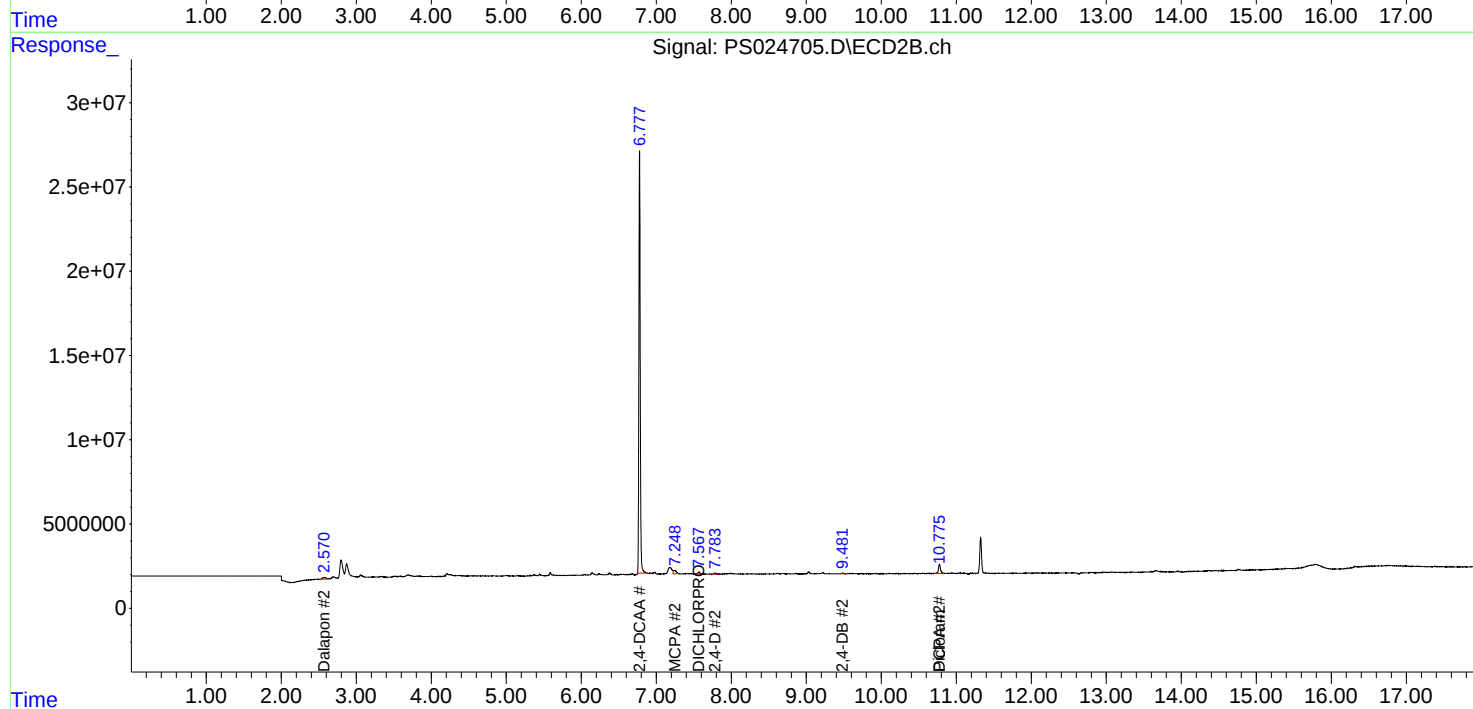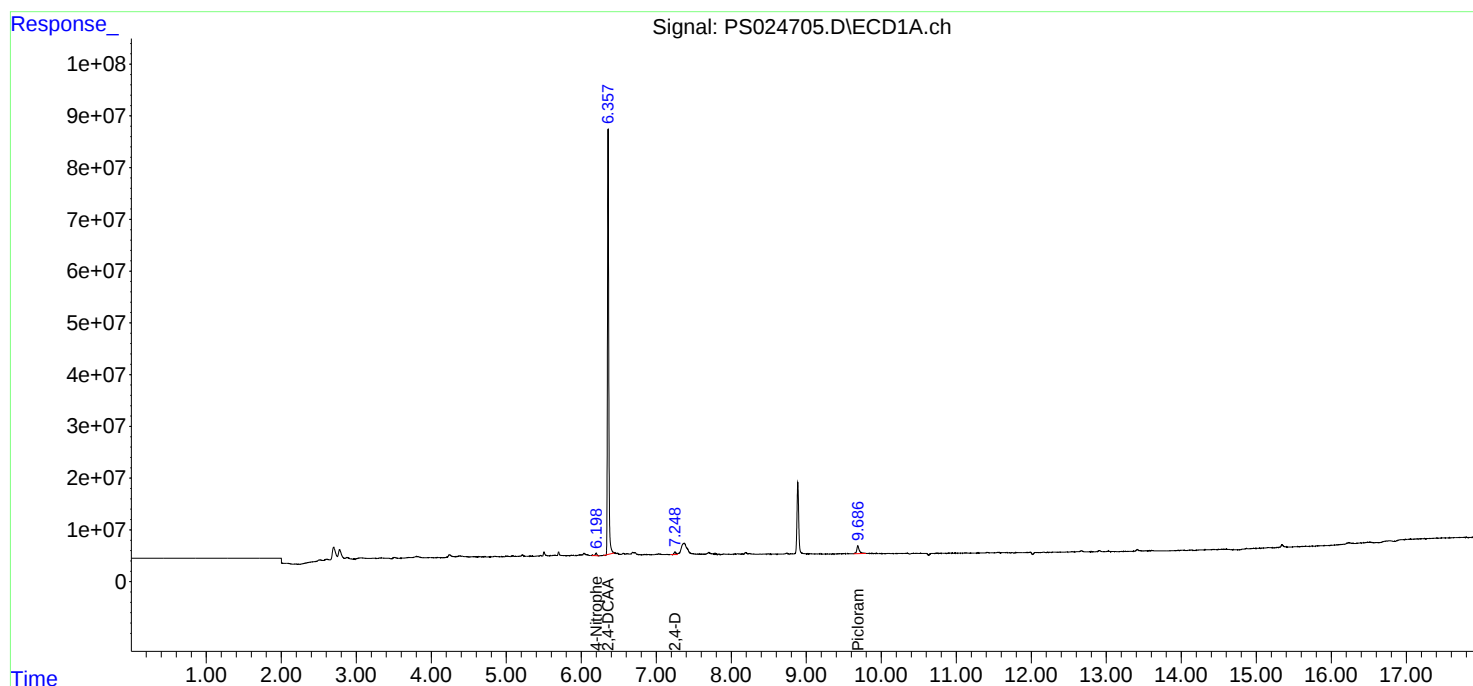


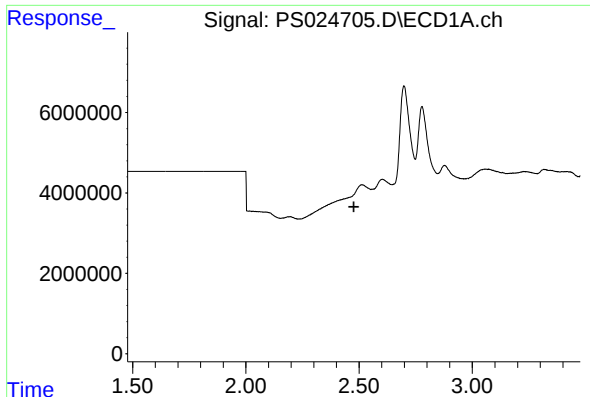

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

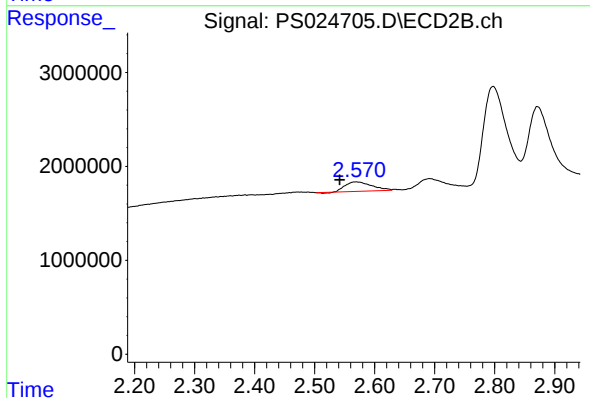


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: 0.028 min
Response: 3046727
Conc: 2.72 ng/ml

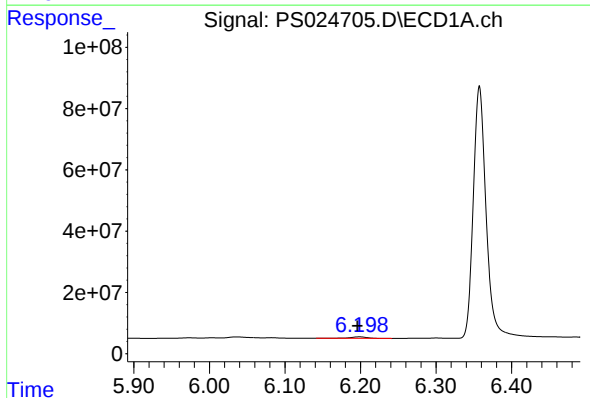


#3 4-Nitrophenol

R.T.: 6.198 min
Delta R.T.: 0.002 min
Response: 7429371
Conc: 5.49 ng/ml

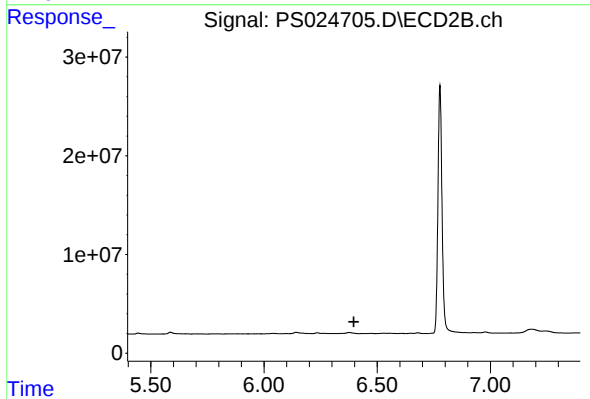

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

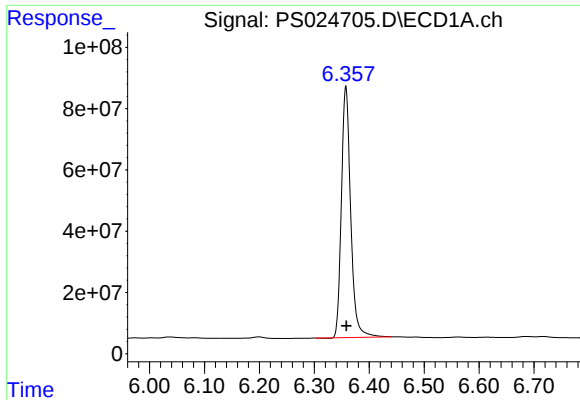

#4 2,4-DCAA


R.T.: 6.358 min
Delta R.T.: -0.001 min
Response: 962824498
Conc: 468.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

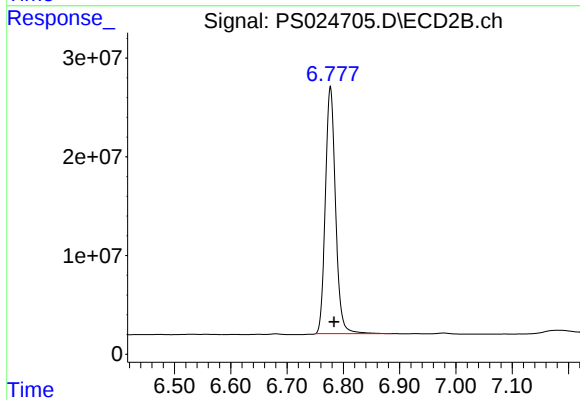


#4 2,4-DCAA

R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 314524087
Conc: 454.98 ng/ml

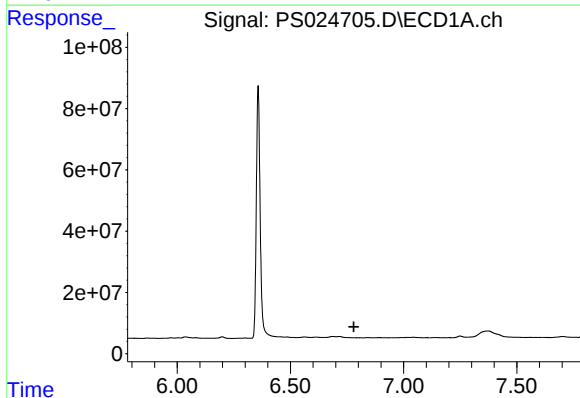


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

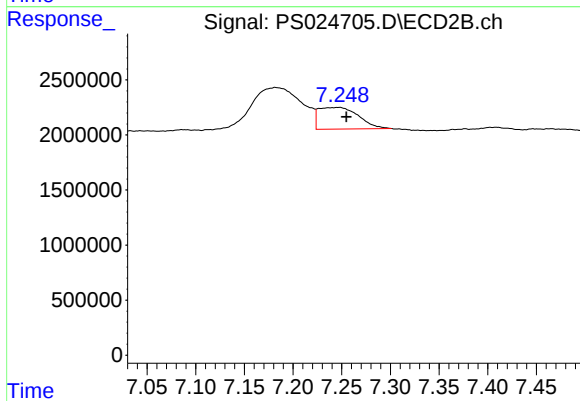

#7 MCPA


R.T.: 7.247 min
Delta R.T.: -0.008 min
Response: 5558809
Conc: 1.73 ug/ml

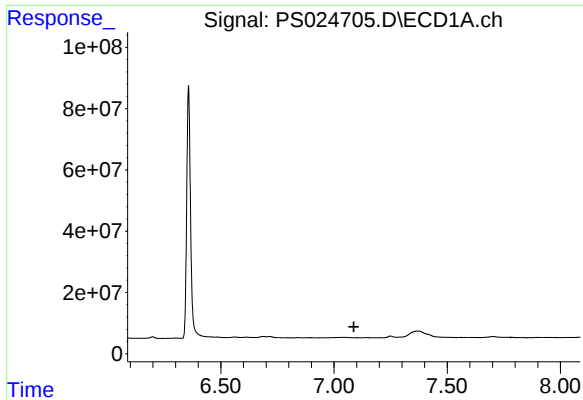

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

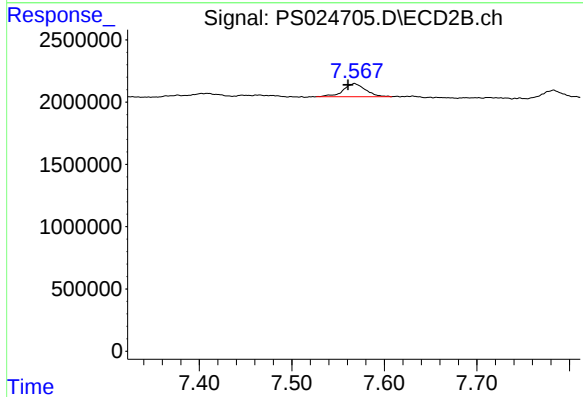


#8 DICHLORPROP

R.T.: 7.568 min
Delta R.T.: 0.007 min
Response: 1750507
Conc: 2.33 ng/ml

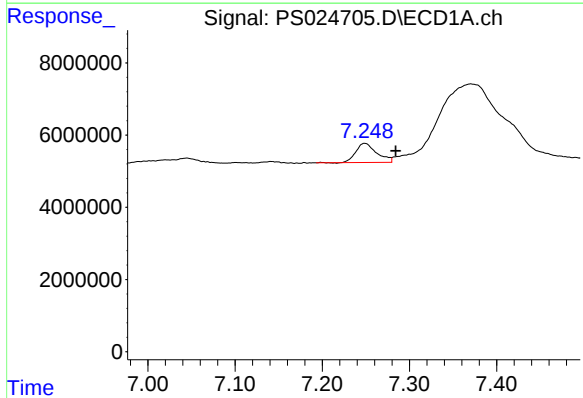


#9 2,4-D

R.T.: 7.249 min
Delta R.T.: -0.036 min
Response: 8751038
Conc: 3.17 ng/ml

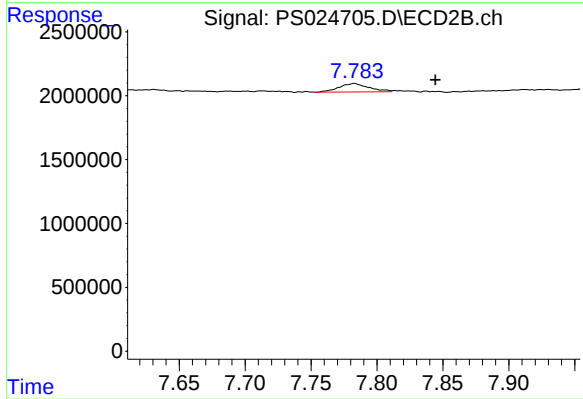

#9 2,4-D


R.T.: 7.783 min
Delta R.T.: -0.061 min
Response: 1063655
Conc: 1.16 ng/ml

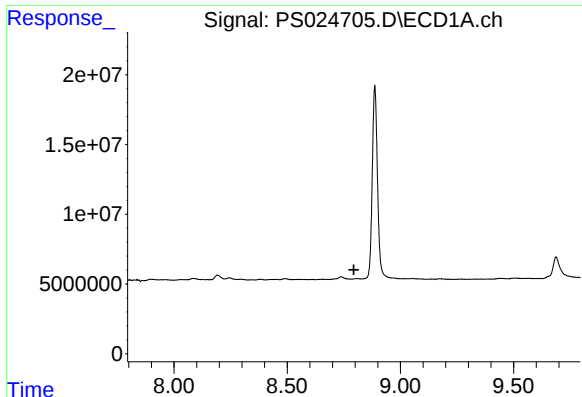

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

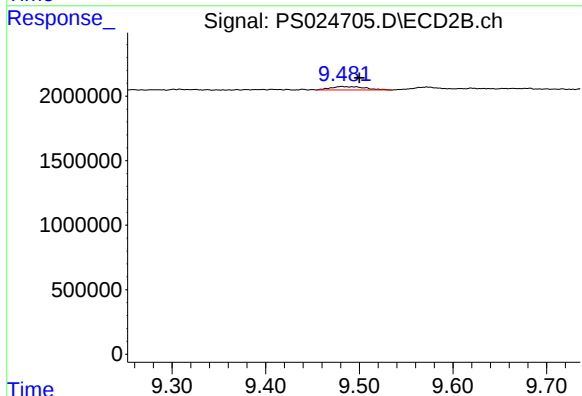


#13 2,4-DB

R.T.: 9.481 min
Delta R.T.: -0.019 min
Response: 680007
Conc: 1.33 ng/ml

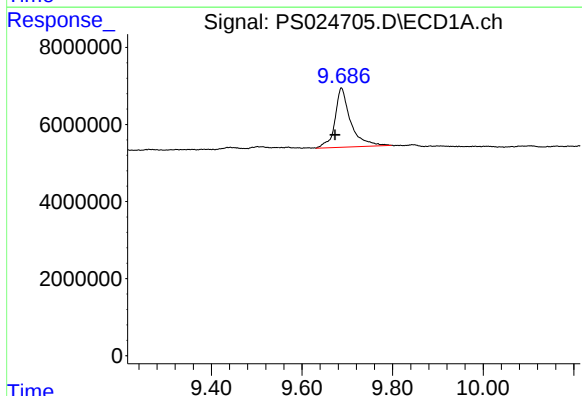


#15 Picloram

R.T.: 9.687 min
Delta R.T.: 0.014 min
Response: 36705373
Conc: 2.11 ng/ml

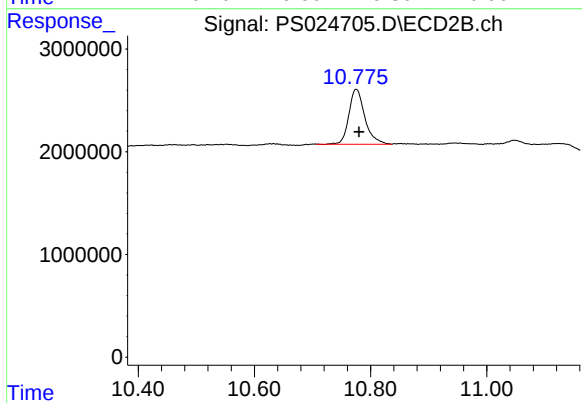

#15 Picloram


R.T.: 10.775 min
Delta R.T.: -0.005 min
Response: 10197874
Conc: 1.64 ng/ml

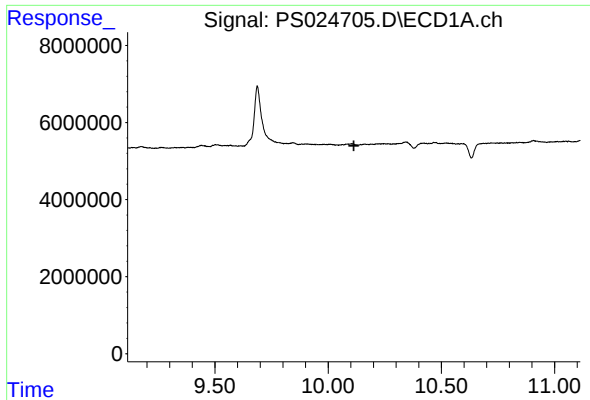

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

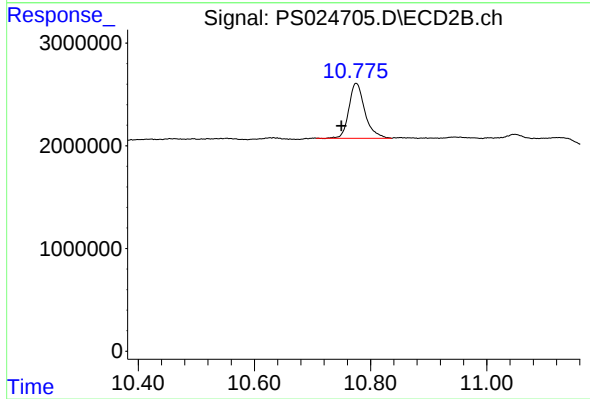

#16 DCPA

R.T.: 10.775 min
Delta R.T.: 0.025 min
Response: 10197874
Conc: 1.95 ng/ml