

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
 Data File : PS024709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 13:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 13:29:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.778	976.5E6	320.3E6	474.655	463.329
Target Compounds							
1) T	Dalapon	0.000	2.573	0	3808303	N.D.	3.403
2) T	3,5-DICHL...	5.751	0.000	13315624	0	4.245	N.D. #
5) T	DICAMBA	0.000	7.001f	0	4533192	N.D.	1.531
6) T	MCP	0.000	7.001f	0	4533192	N.D.	2.300
7) T	MCPA	0.000	7.254	0	6417908	N.D.	2.003
8) T	DICHLORPROP	0.000	7.567	0	2306849	N.D.	3.067
9) T	2,4-D	7.261	7.781f	57878124	594023	20.948	<MDL #
11) T	2,4,5-TP ...	0.000	8.617	0	489415	N.D.	<MDL
12) T	2,4,5-T	0.000	9.033	0	889637	N.D.	<MDL
13) T	2,4-DB	0.000	9.488	0	846255	N.D.	1.661
15) T	Picloram	9.689	10.777	15446160	4474803	<MDL	<MDL #
16) T	DCPA	0.000	10.777	0	4474803	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
Data File : PS024709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 13:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 13:29:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

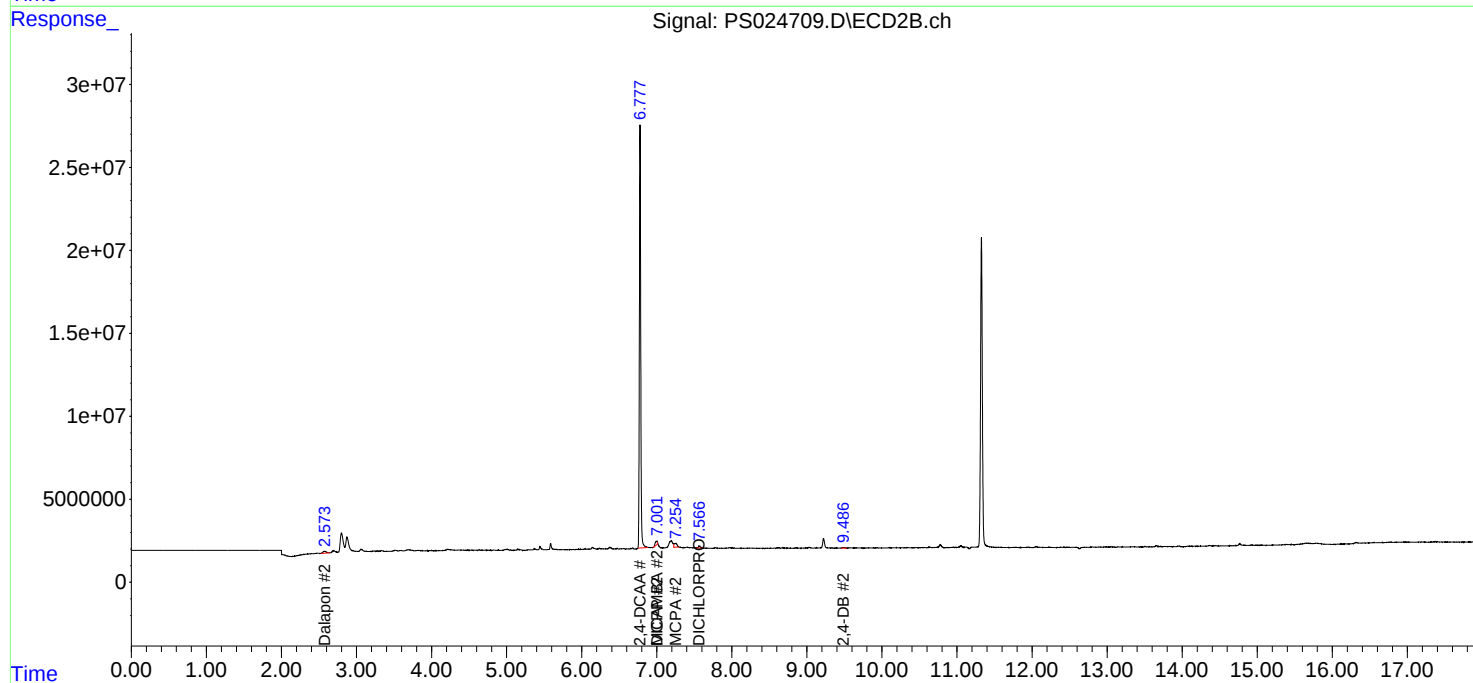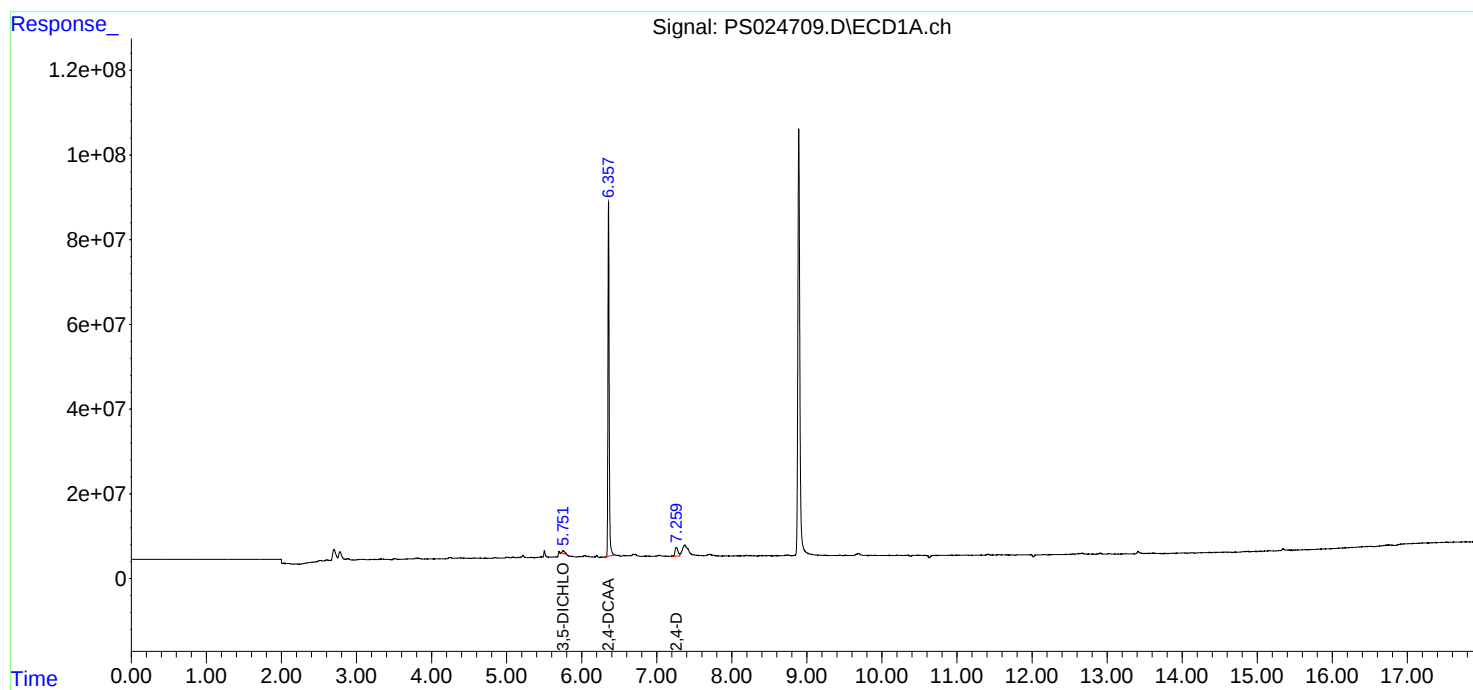


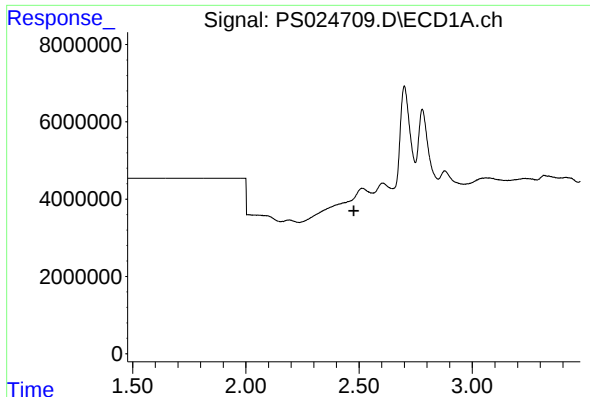

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

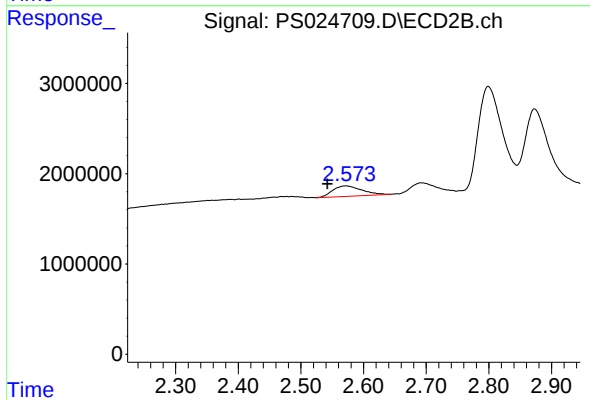


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.031 min
Response: 3808303
Conc: 3.40 ng/ml

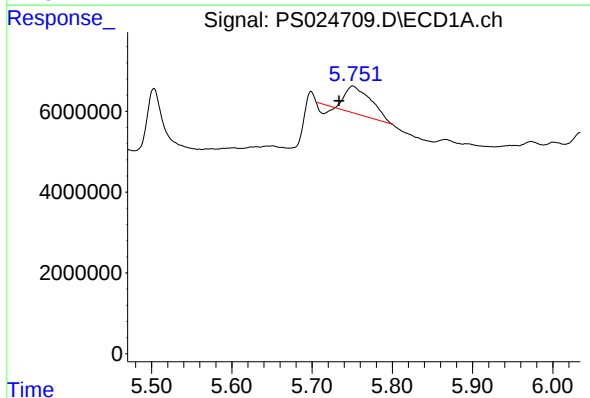


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.751 min
Delta R.T.: 0.017 min
Response: 13315624
Conc: 4.24 ng/ml

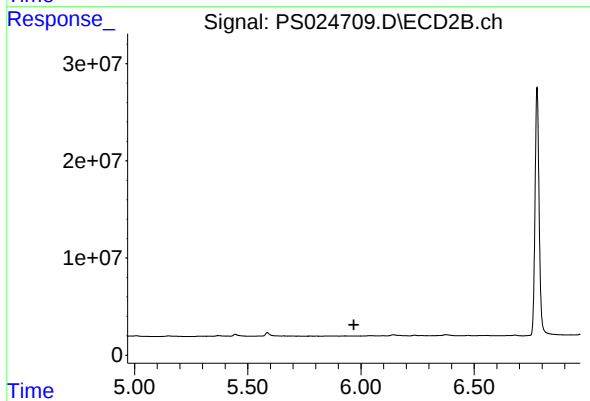

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.969 min
Response: 0
Conc: N.D.

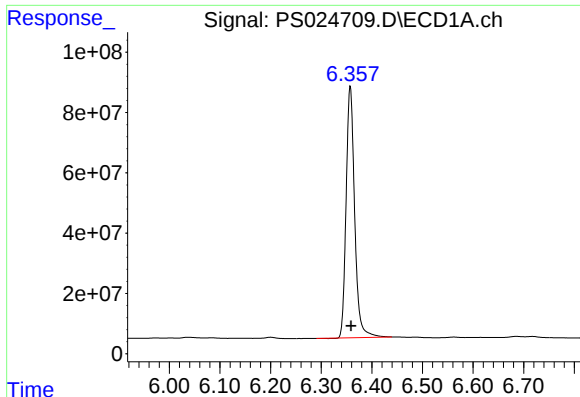

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: -0.001 min
Response: 976520866
Conc: 474.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

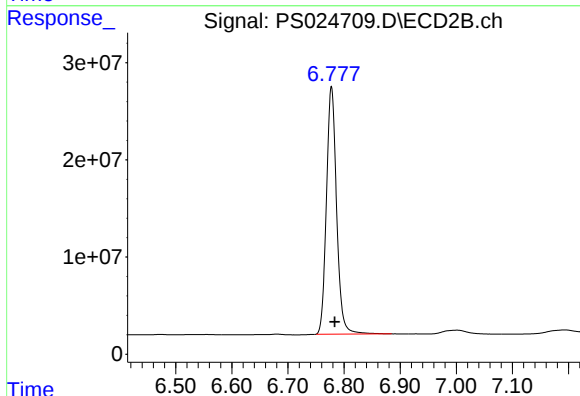


#4 2,4-DCAA

R.T.: 6.778 min
Delta R.T.: -0.006 min
Response: 320294620
Conc: 463.33 ng/ml

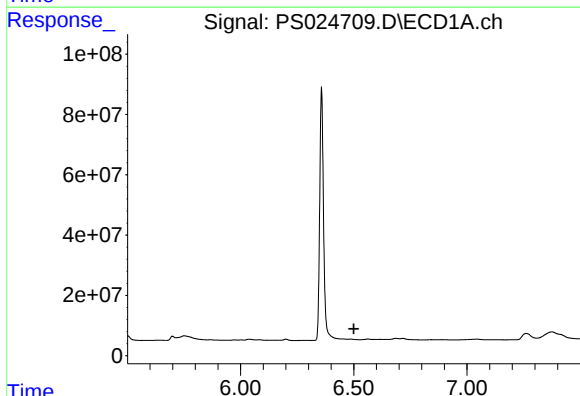


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.501 min
Response: 0
Conc: N.D.

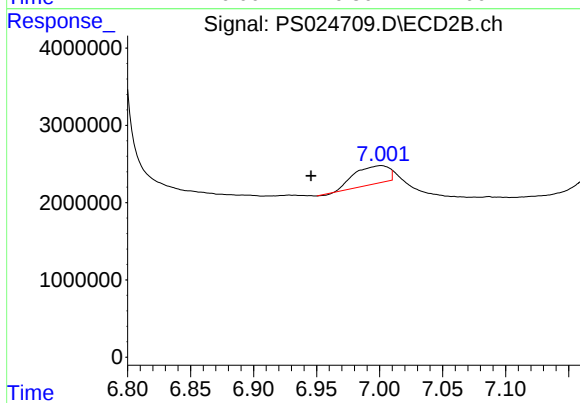

#5 DICAMBA


R.T.: 7.001 min
Delta R.T.: 0.055 min
Response: 4533192
Conc: 1.53 ng/ml

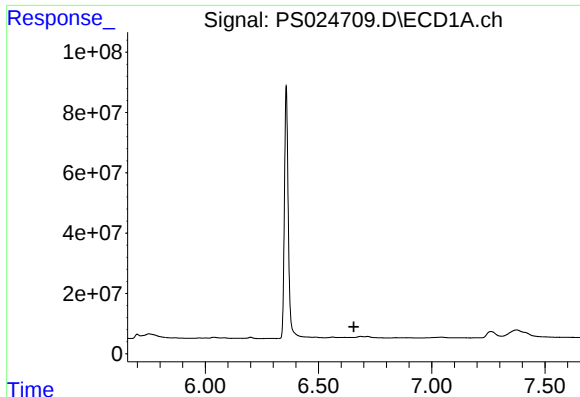

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

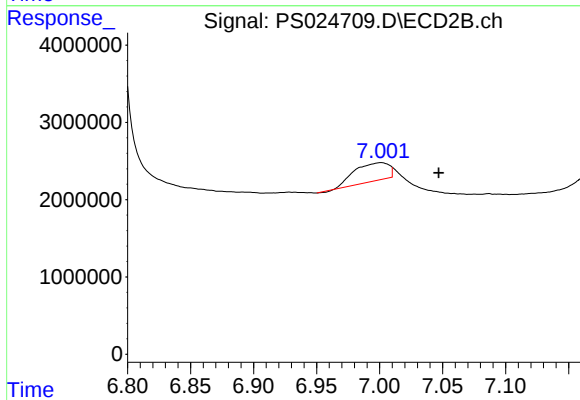


#6 MCPP

R.T.: 7.001 min
Delta R.T.: -0.046 min
Response: 4533192
Conc: 2.30 ug/ml

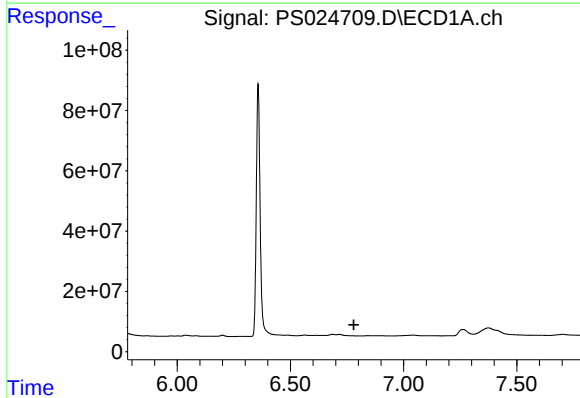


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

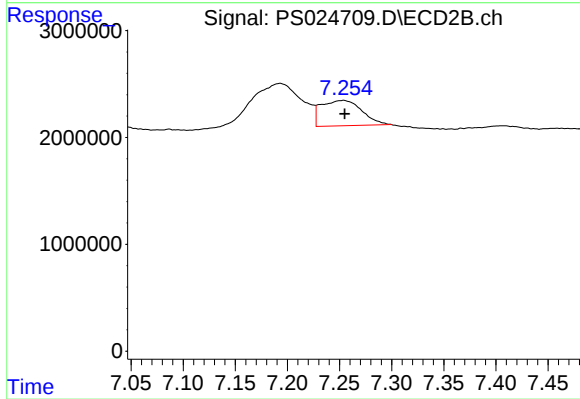

#7 MCPA


R.T.: 7.254 min
Delta R.T.: -0.001 min
Response: 6417908
Conc: 2.00 ug/ml

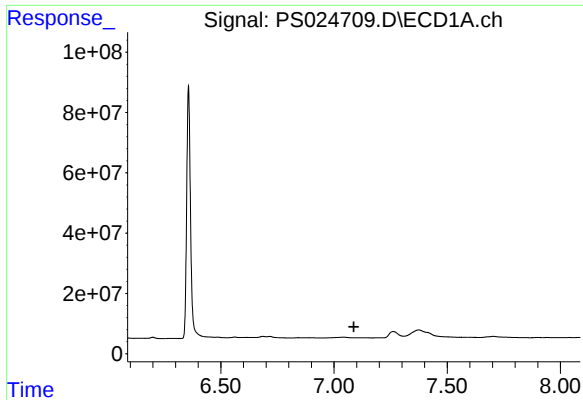

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

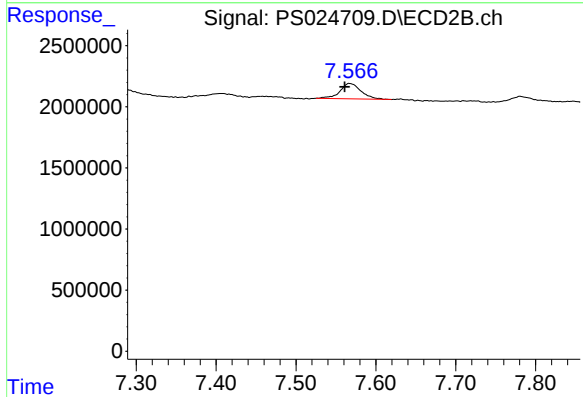


#8 DICHLORPROP

R.T.: 7.567 min
Delta R.T.: 0.006 min
Response: 2306849
Conc: 3.07 ng/ml

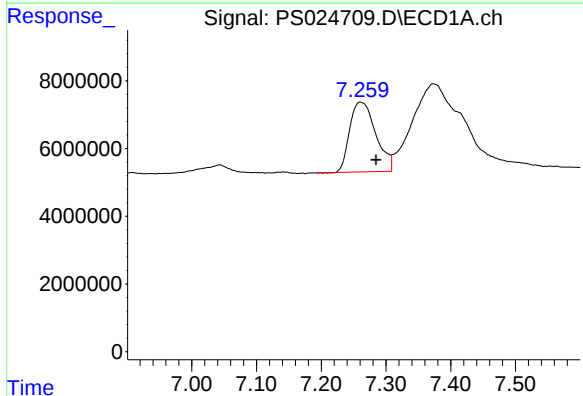


#9 2,4-D

R.T.: 7.261 min
Delta R.T.: -0.023 min
Response: 57878124
Conc: 20.95 ng/ml

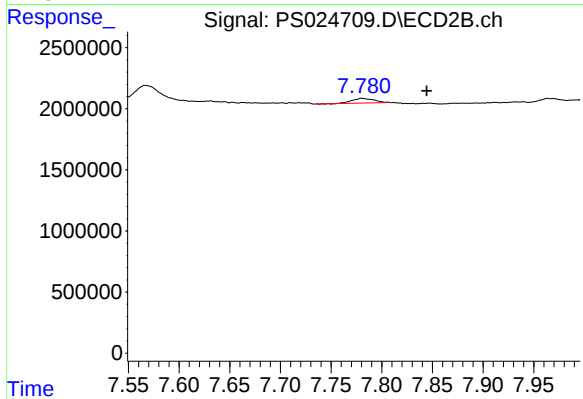

#9 2,4-D


R.T.: 7.781 min
Delta R.T.: -0.064 min
Response: 594023
Conc: N.D.

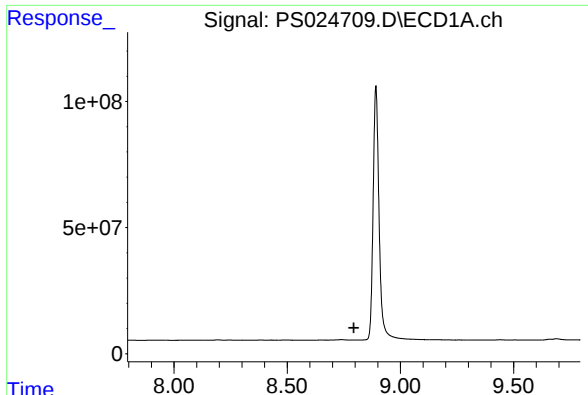

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

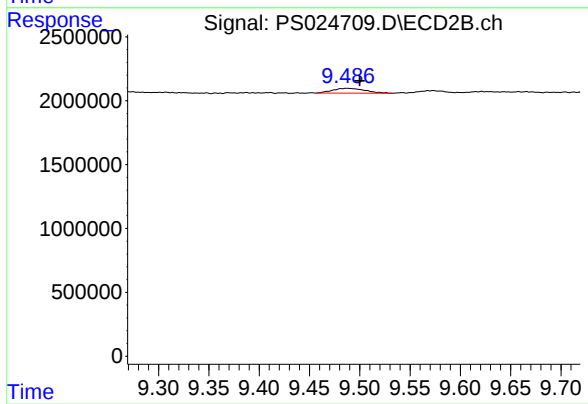

#13 2,4-DB

R.T.: 9.488 min
Delta R.T.: -0.012 min
Response: 846255
Conc: 1.66 ng/ml