

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
 Data File : PS024720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 22:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 00:38:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.777	976.3E6	320.6E6	474.523	463.737
Target Compounds							
1) T	Dalapon	0.000	2.563	0	2815424	N.D.	2.516
5) T	DICAMBA	0.000	6.979	0	3926082	N.D.	1.326
6) T	MCP	6.682	7.086	4305245	435752	<MDL	<MDL #
7) T	MCPA	0.000	7.234	0	7158051	N.D.	2.234
8) T	DICHLORPROP	0.000	7.566	0	4438967	N.D.	5.903
9) T	2,4-D	7.248	7.777f	35022103	1010470	12.675	1.098 #
11) T	2,4,5-TP ...	0.000	8.614	0	588405	N.D.	<MDL
12) T	2,4,5-T	0.000	9.031	0	711196	N.D.	<MDL
13) T	2,4-DB	0.000	9.488	0	1071648	N.D.	2.103
15) T	Picloram	0.000	10.775	0	3270412	N.D.	<MDL
16) T	DCPA	0.000	10.775	0	3270412	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102523\
Data File : PS024720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 22:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 00:38:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

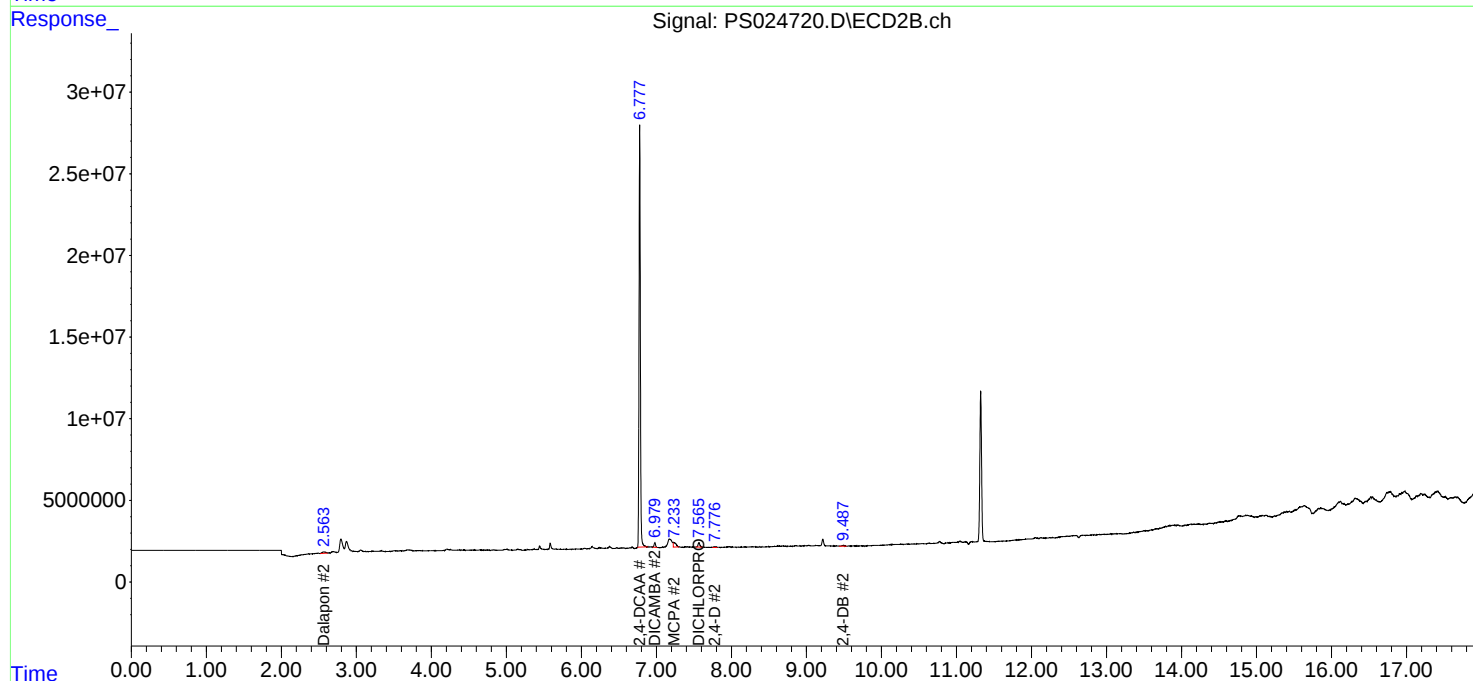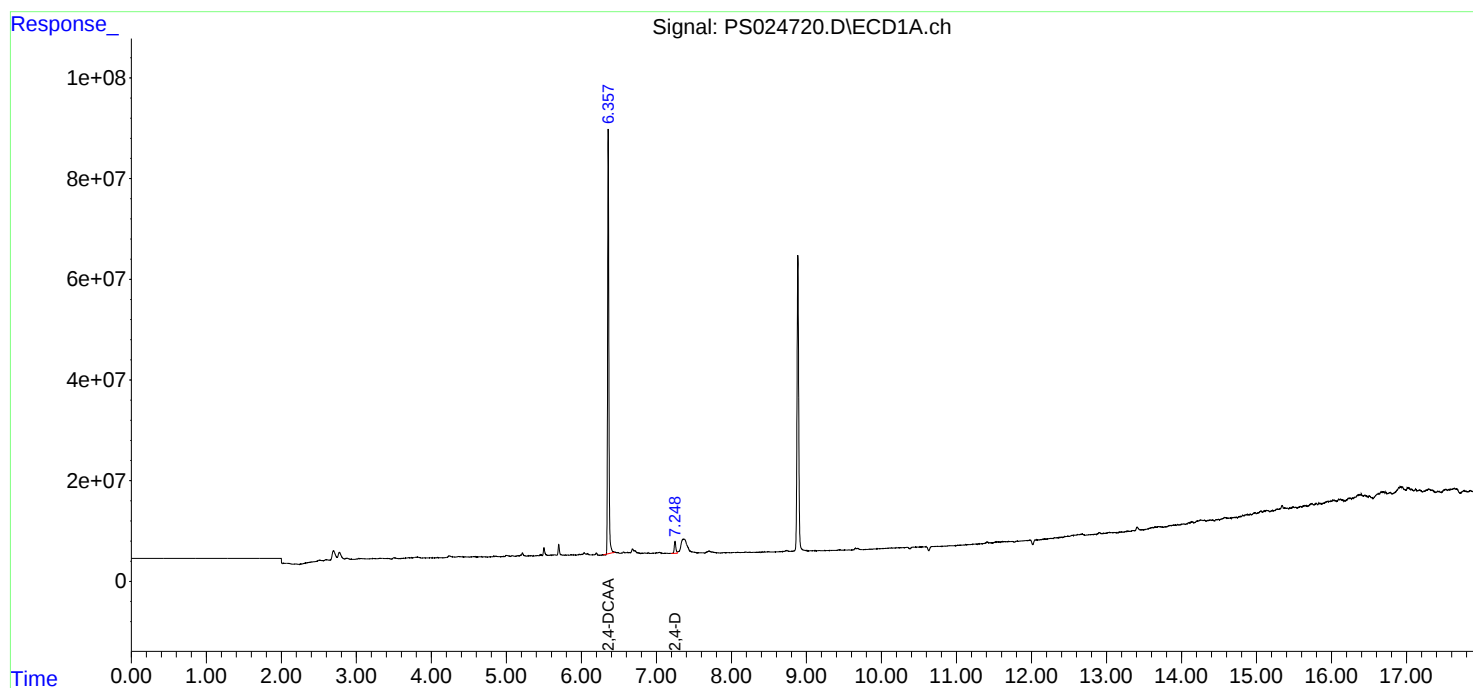


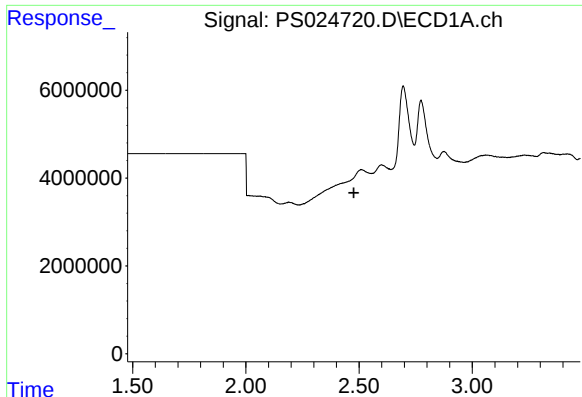

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

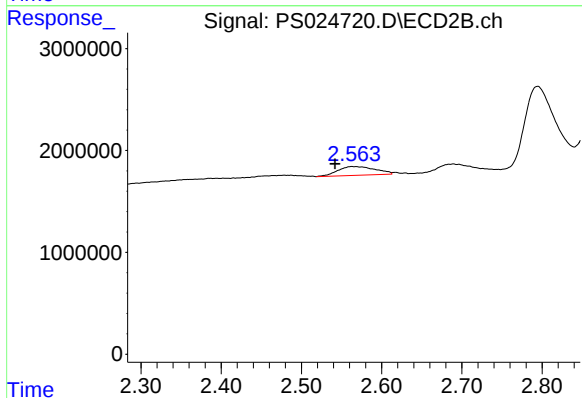


#1 Dalapon

R.T.: 2.563 min
Delta R.T.: 0.021 min
Response: 2815424
Conc: 2.52 ng/ml

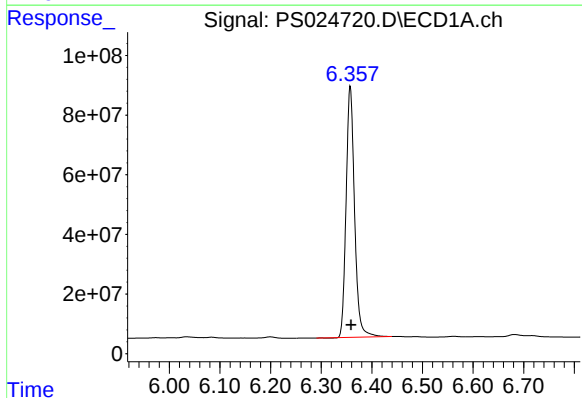


#4 2,4-DCAA

R.T.: 6.357 min
Delta R.T.: -0.001 min
Response: 976250588
Conc: 474.52 ng/ml

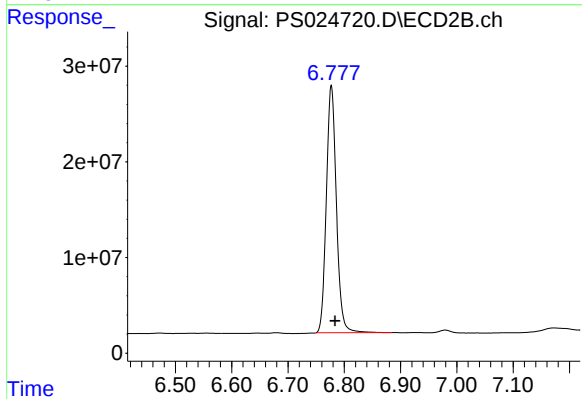

#4 2,4-DCAA


R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 320577149
Conc: 463.74 ng/ml

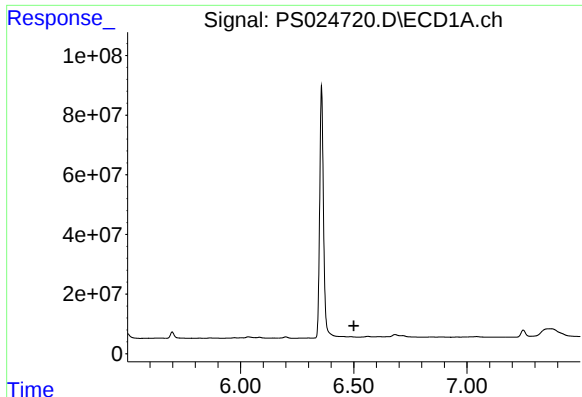

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

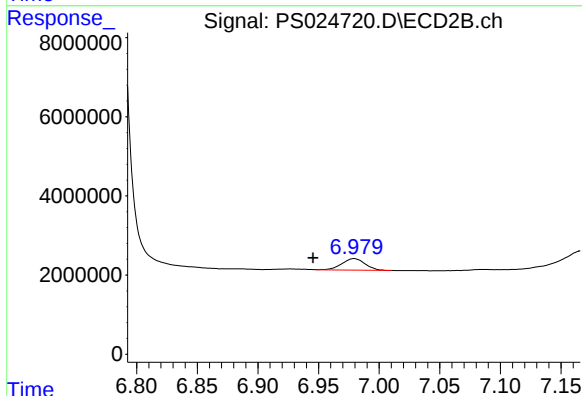


#5 DICAMBA

R.T.: 6.979 min
Delta R.T.: 0.034 min
Response: 3926082
Conc: 1.33 ng/ml

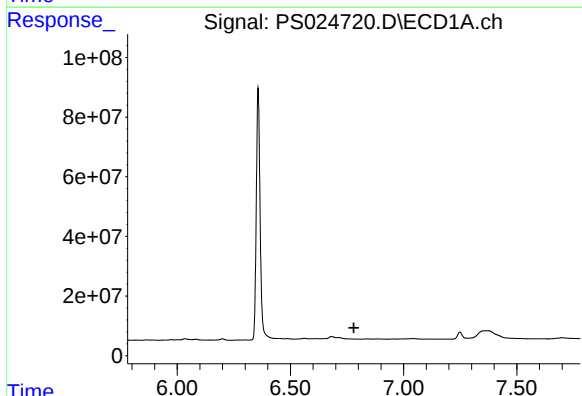


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

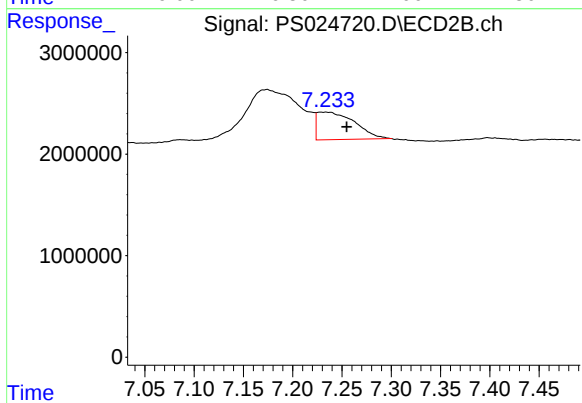

#7 MCPA


R.T.: 7.234 min
Delta R.T.: -0.021 min
Response: 7158051
Conc: 2.23 ug/ml

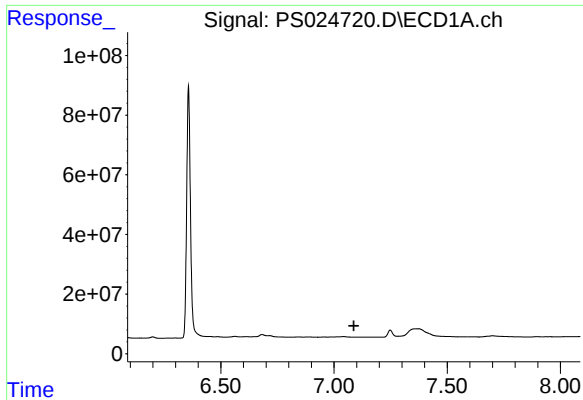

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

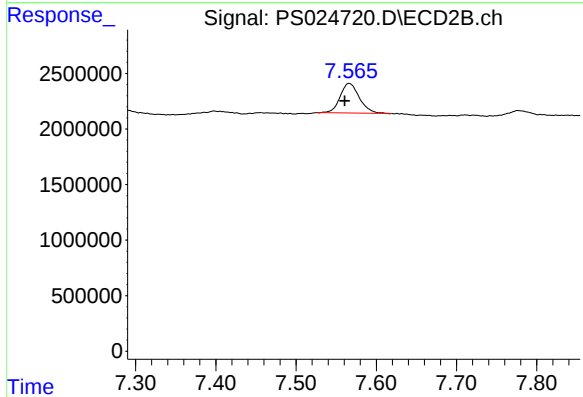


#8 DICHLORPROP

R.T.: 7.566 min
Delta R.T.: 0.005 min
Response: 4438967
Conc: 5.90 ng/ml

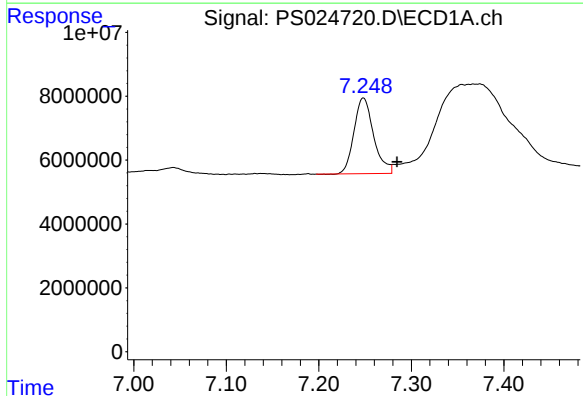


#9 2,4-D

R.T.: 7.248 min
Delta R.T.: -0.036 min
Response: 35022103
Conc: 12.68 ng/ml

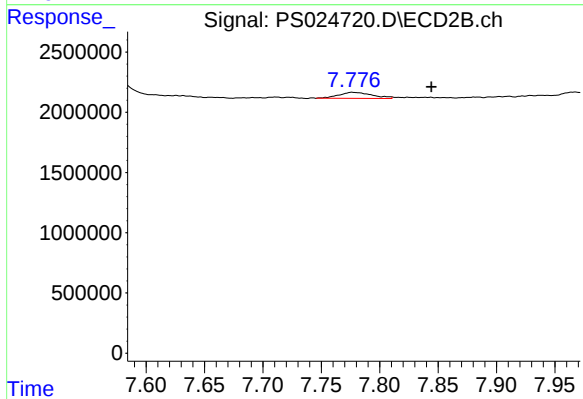

#9 2,4-D


R.T.: 7.777 min
Delta R.T.: -0.068 min
Response: 1010470
Conc: 1.10 ng/ml

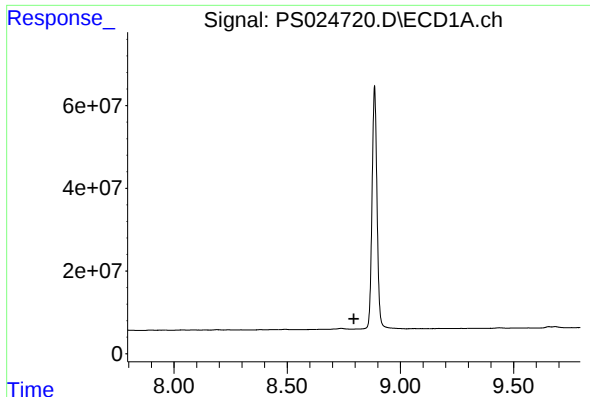

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

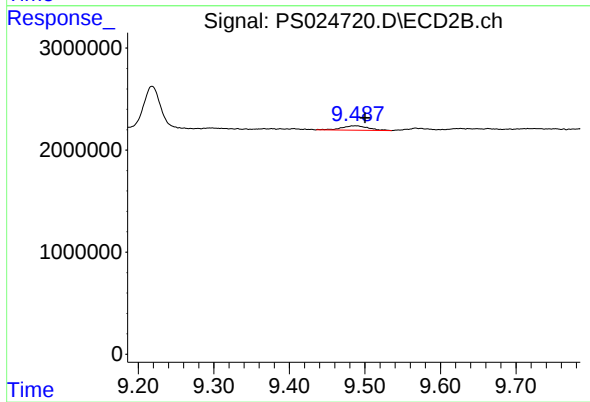

#13 2,4-DB

R.T.: 9.488 min
Delta R.T.: -0.012 min
Response: 1071648
Conc: 2.10 ng/ml