

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102618\
 Data File : PS002143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 23:36
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 01:48:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.467	10.940	158.3E6	154.3E6	502.892	429.573
Target Compounds							
7) T	MCPA	0.000	11.828	0	1271381	N.D.	0.939 #
12) T	2,4,5-T	0.000	14.555	0	4547255	N.D.	3.037 #
15) T	Picloram	16.990	0.000	7224399	0	3.029	N.D. #
16) T	DCPA	0.000	16.861	0	11660649	N.D.	4.925 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102618\
Data File : PS002143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 23:36
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 01:48:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

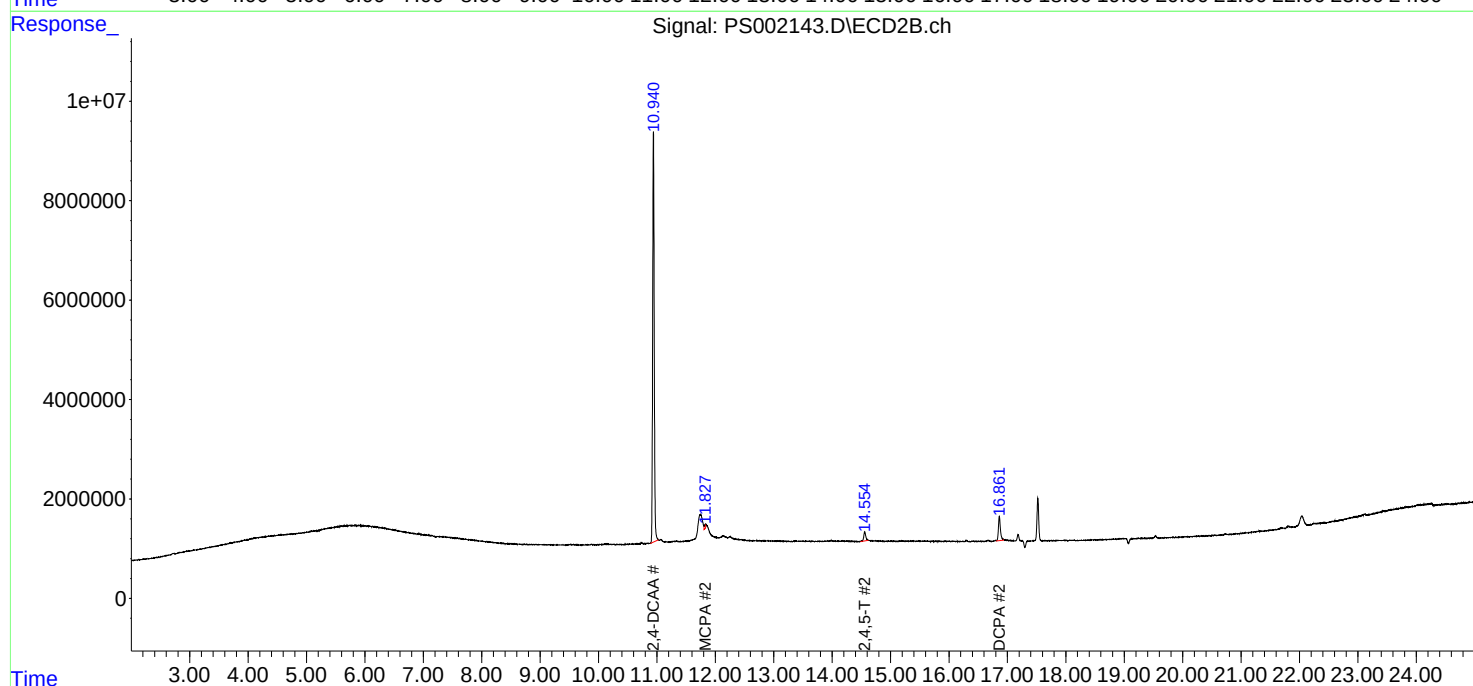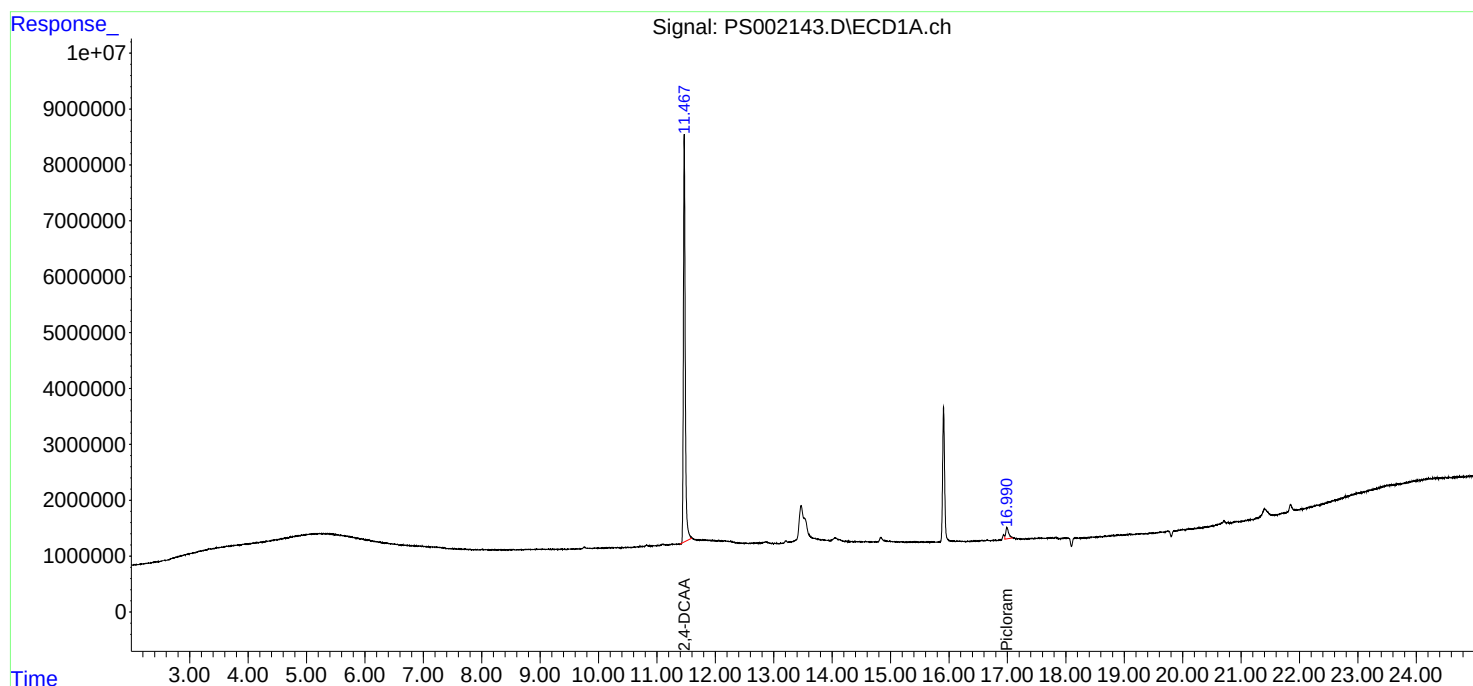


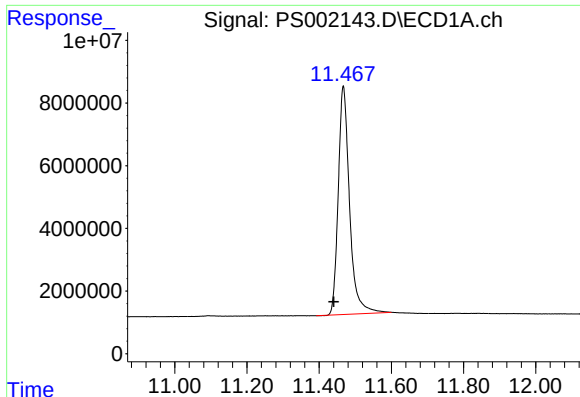

#4 2,4-DCAA


R.T.: 11.467 min
Delta R.T.: 0.026 min
Response: 158252888
Conc: 502.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

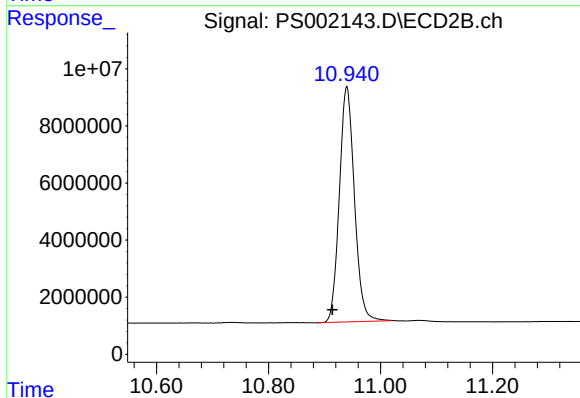


#4 2,4-DCAA

R.T.: 10.940 min
Delta R.T.: 0.026 min
Response: 154258595
Conc: 429.57 ng/ml

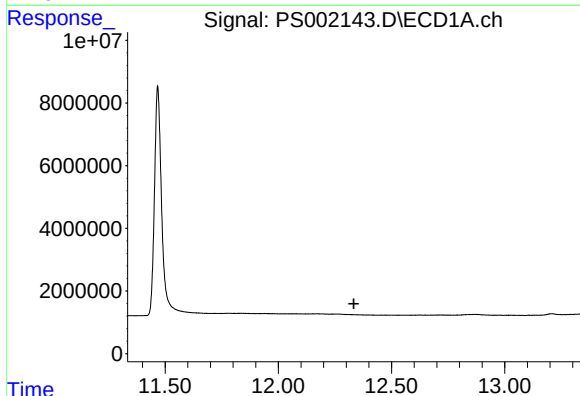


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

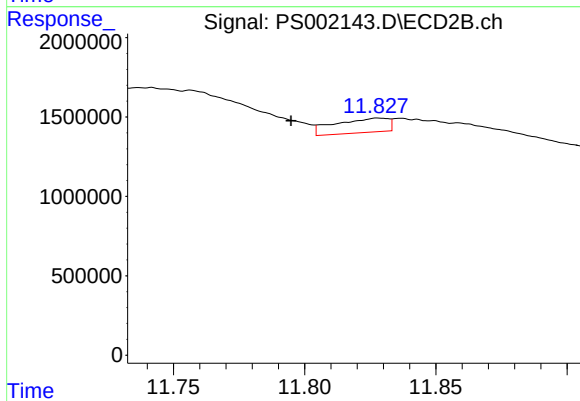

#7 MCPA


R.T.: 11.828 min
Delta R.T.: 0.033 min
Response: 1271381
Conc: 0.94 ug/ml

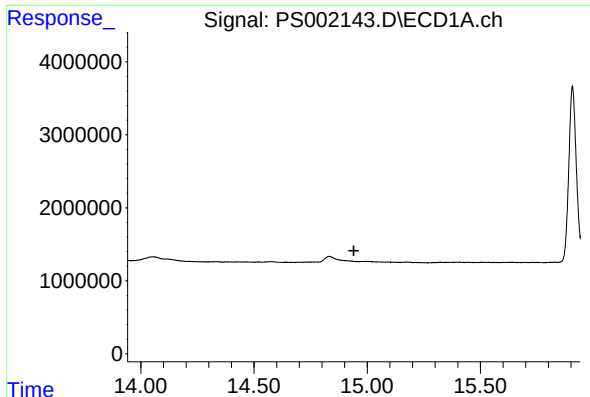

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

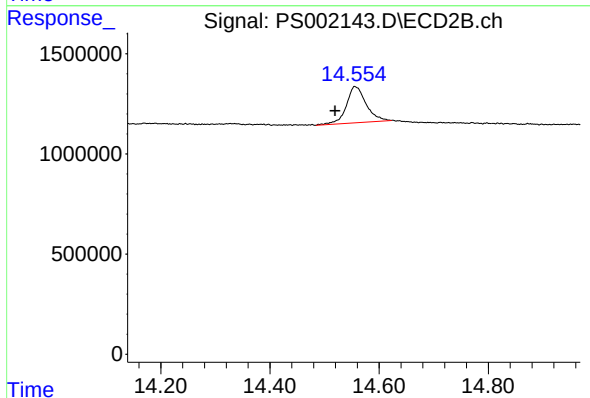


#12 2,4,5-T

R.T.: 14.555 min
Delta R.T.: 0.036 min
Response: 4547255
Conc: 3.04 ng/ml

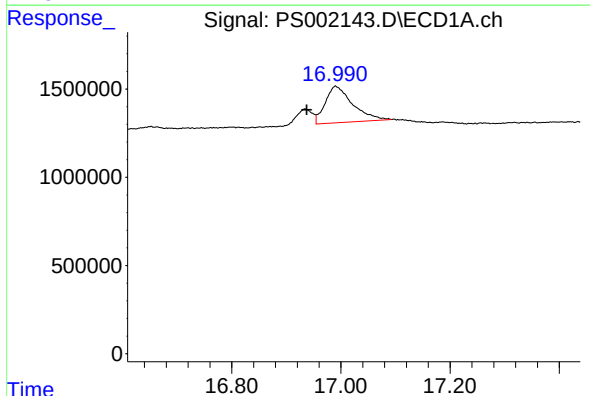


#15 Picloram

R.T.: 16.990 min
Delta R.T.: 0.053 min
Response: 7224399
Conc: 3.03 ng/ml

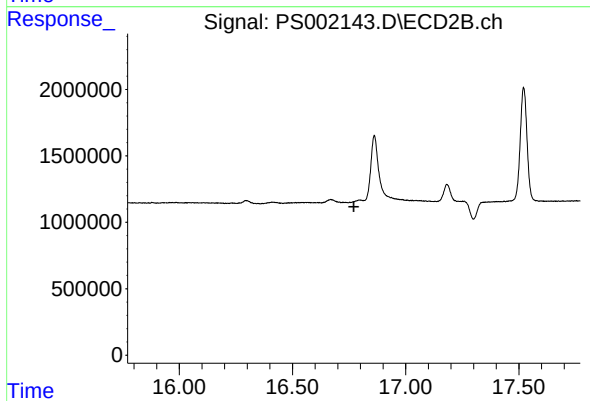

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.771 min
Response: 0
Conc: N.D.

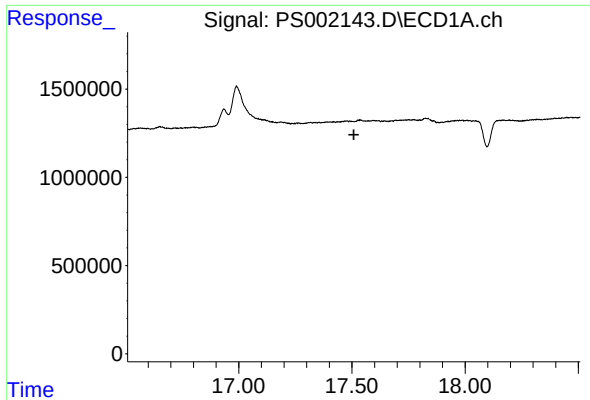

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

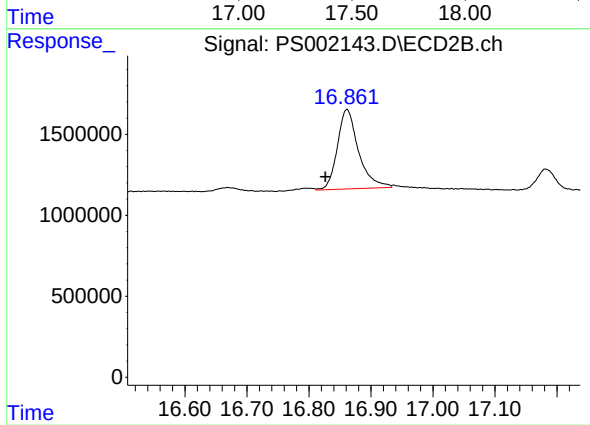

#16 DCPA

R.T.: 16.861 min
Delta R.T.: 0.035 min
Response: 11660649
Conc: 4.92 ng/ml