

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102620\
 Data File : PS012978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 19:35
 Operator : DD\AJ
 Sample : L4496-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 01:25:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.214	6.917	258.1E6	136.9E6	288.349	341.059
Target Compounds							
1) T	Dalapon	2.992	2.589	68285536	132.5E6	67.172	251.890 #
2) T	3,5-DICHL...	0.000	6.046	0	3321731	N.D.	5.272
3) T	4-Nitroph...	6.983	0.000	4292342	0	10.263	N.D. #
5) T	DICAMBA	7.389	7.049	12190251	4659534	3.424	2.738
7) T	MCPA	7.724	0.000	132.9E6	0	34.697	N.D. #
9) T	2,4-D	8.391	0.000	77791171	0	75.393	N.D. #
10) T	Pentachlo...	8.685	0.000	14977072	0	1.167	N.D. #
11) T	2,4,5-TP ...	0.000	8.810	0	61692404	N.D.	26.024
12) T	2,4,5-T	9.399	0.000	82750239	0	15.803	N.D. #
15) T	Picloram	11.002	0.000	21555070	0	3.405	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102620\
Data File : PS012978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 19:35
Operator : DD\AJ
Sample : L4496-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 01:25:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

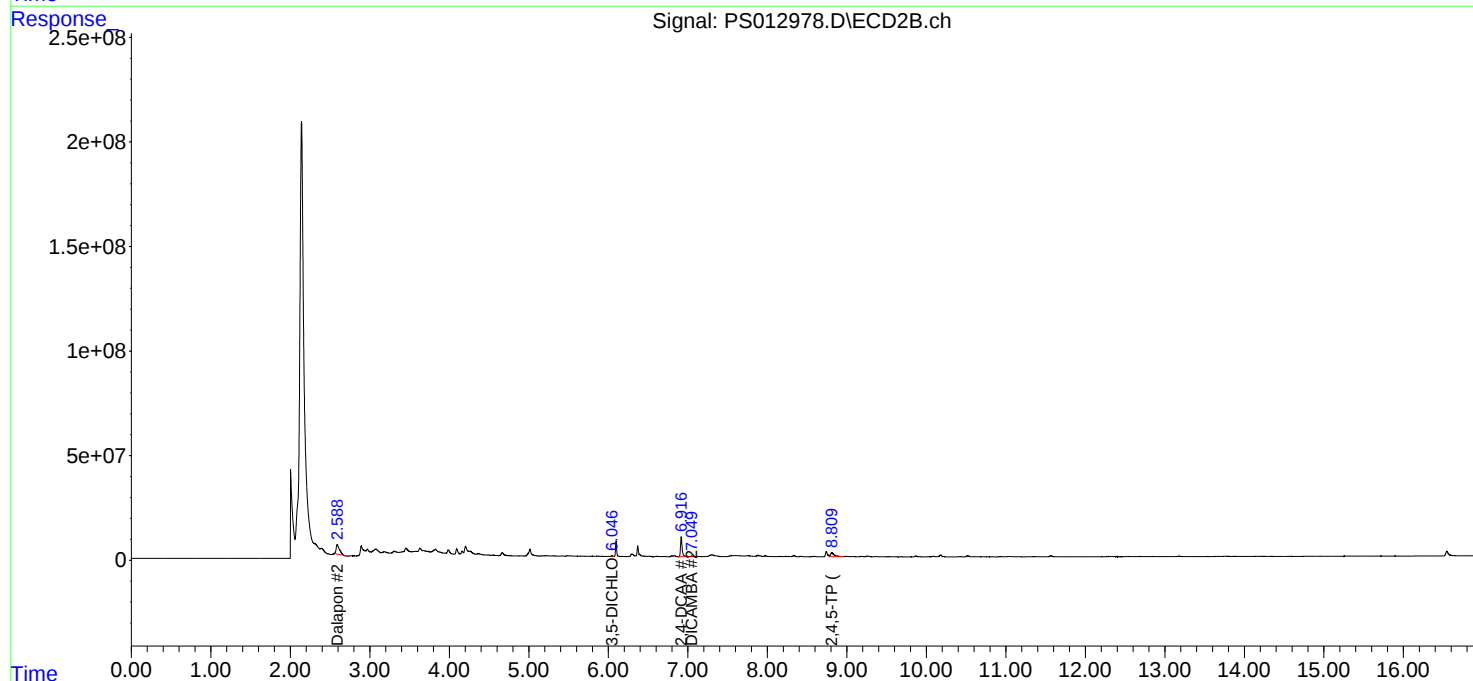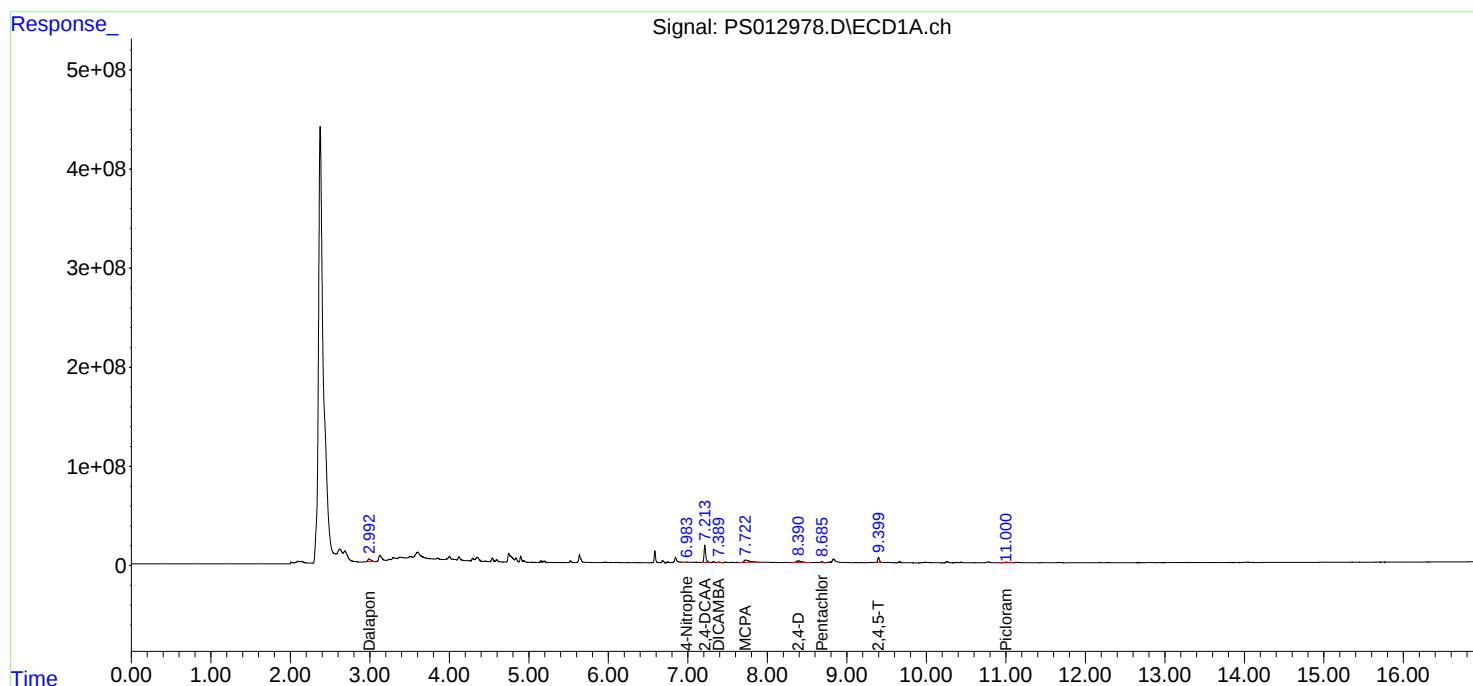


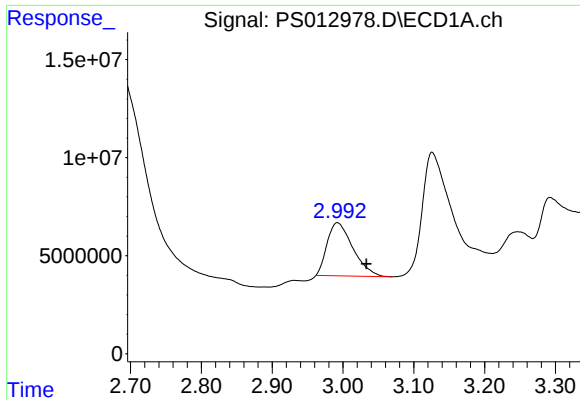

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.041 min
Response: 68285536
Conc: 67.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

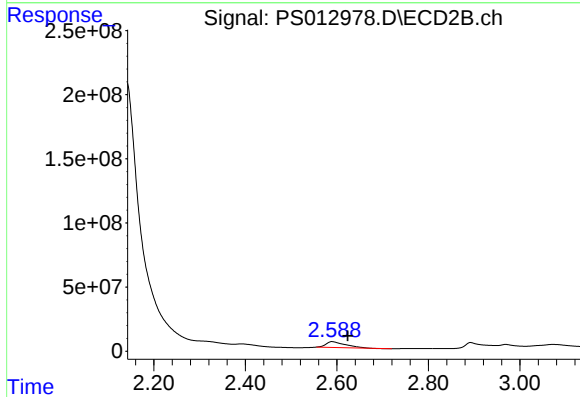


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.035 min
Response: 132462749
Conc: 251.89 ng/ml

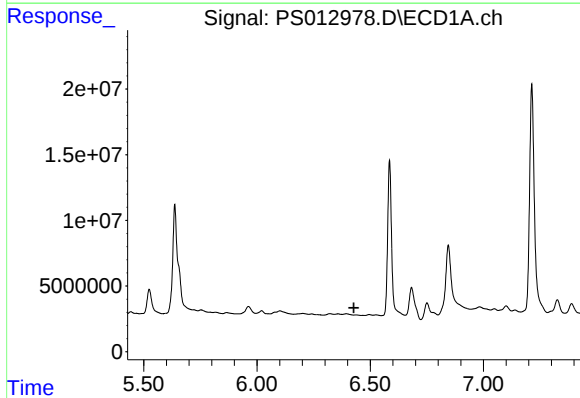


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

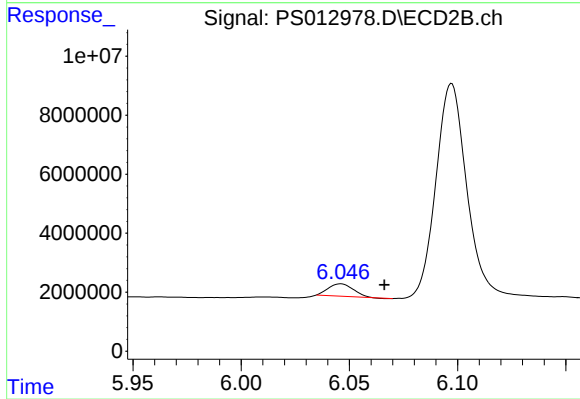

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.046 min
Delta R.T.: -0.020 min
Response: 3321731
Conc: 5.27 ng/ml

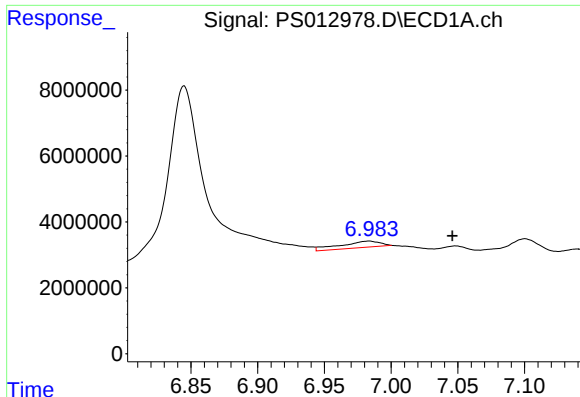

#3 4-Nitrophenol


R.T.: 6.983 min
Delta R.T.: -0.063 min
Response: 4292342
Conc: 10.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

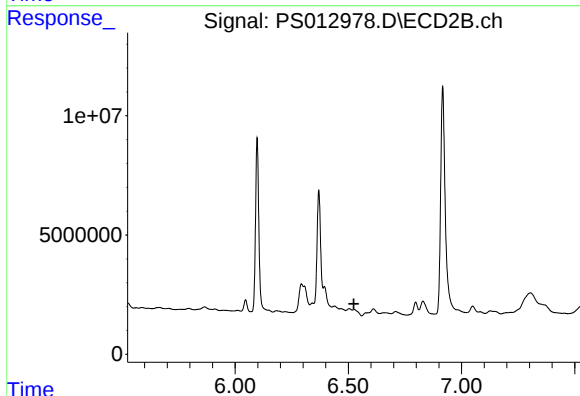


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

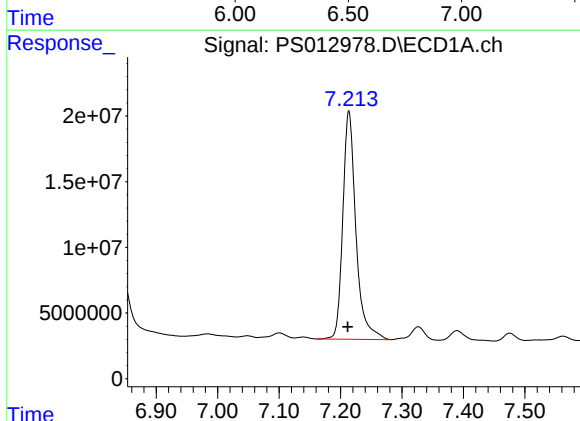


#4 2,4-DCAA

R.T.: 7.214 min
Delta R.T.: 0.002 min
Response: 258092395
Conc: 288.35 ng/ml

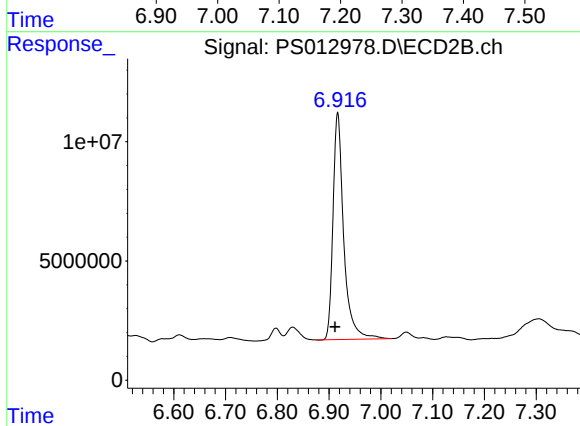

#4 2,4-DCAA


R.T.: 6.917 min
Delta R.T.: 0.005 min
Response: 136850347
Conc: 341.06 ng/ml

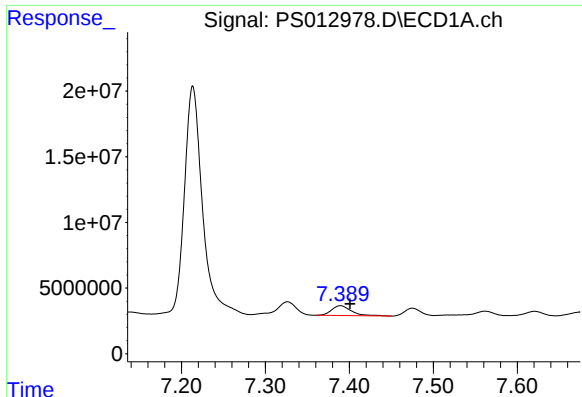

#5 DICAMBA


R.T.: 7.389 min
Delta R.T.: -0.011 min
Response: 12190251
Conc: 3.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

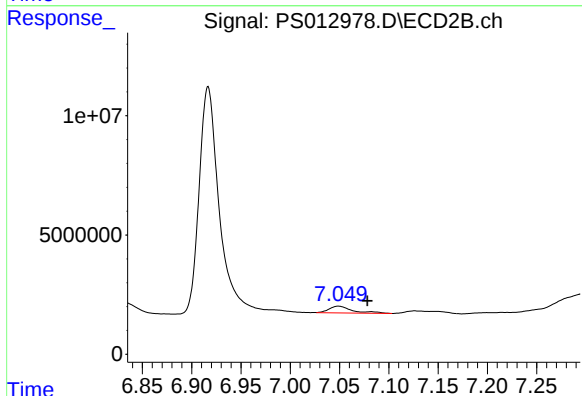


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.029 min
Response: 4659534
Conc: 2.74 ng/ml

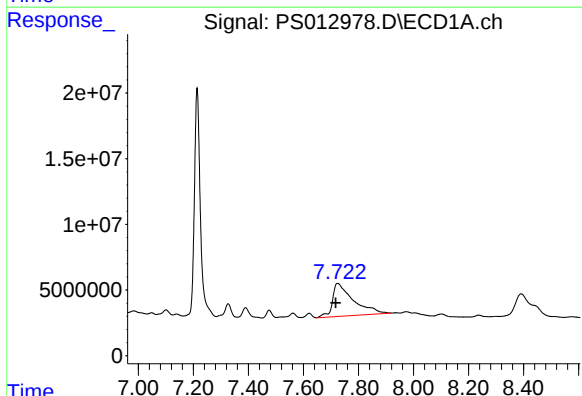


#7 MCPA

R.T.: 7.724 min
Delta R.T.: 0.007 min
Response: 132856088
Conc: 34.70 ug/ml

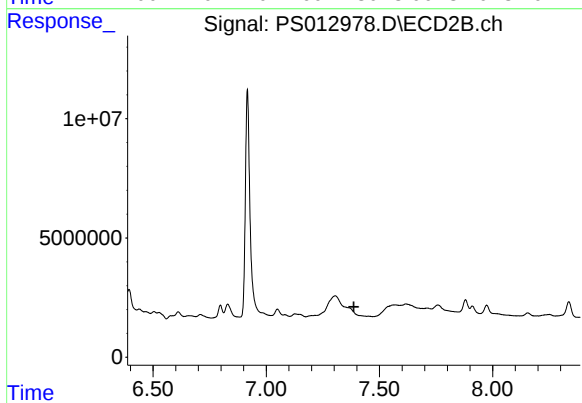

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

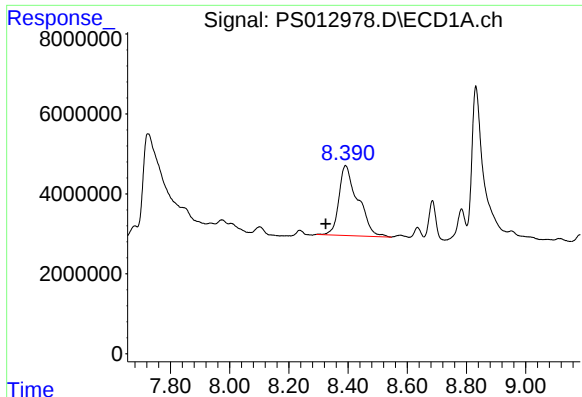

#9 2,4-D


R.T.: 8.391 min
Delta R.T.: 0.067 min
Response: 77791171
Conc: 75.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

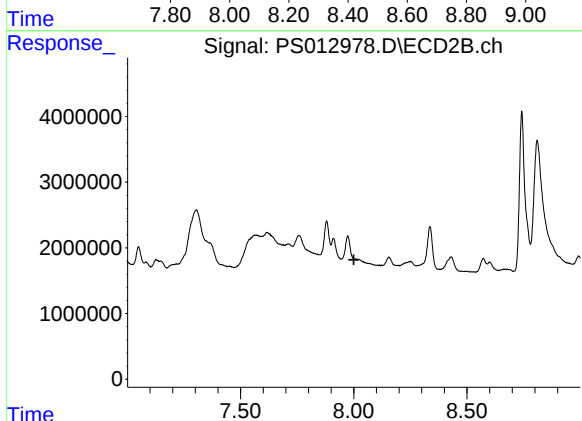


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

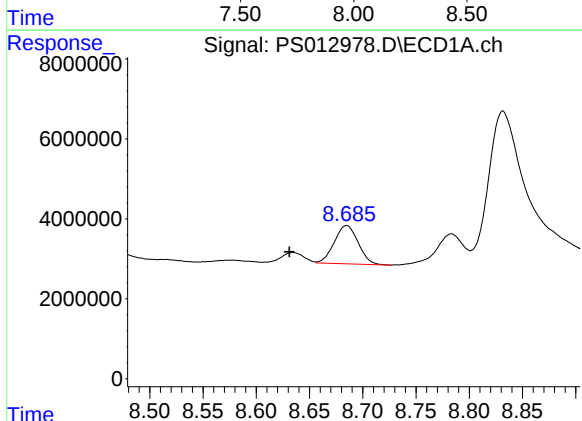


#10 Pentachlorophenol

R.T.: 8.685 min
Delta R.T.: 0.054 min
Response: 14977072
Conc: 1.17 ng/ml

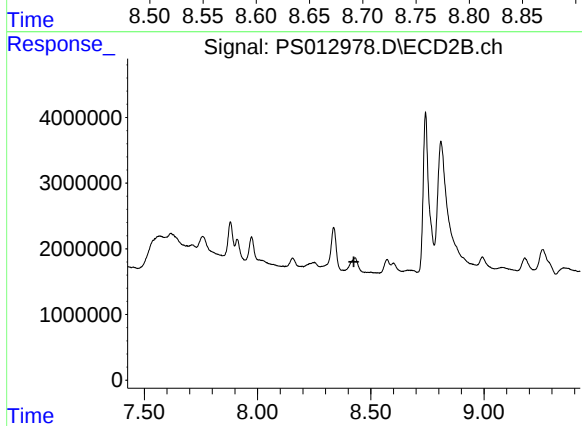

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 8.425 min
Response: 0
Conc: N.D.

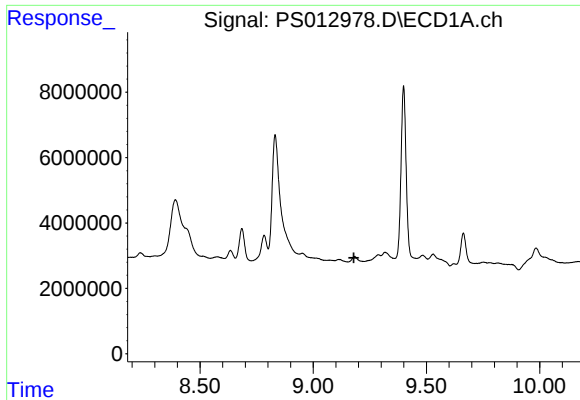

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

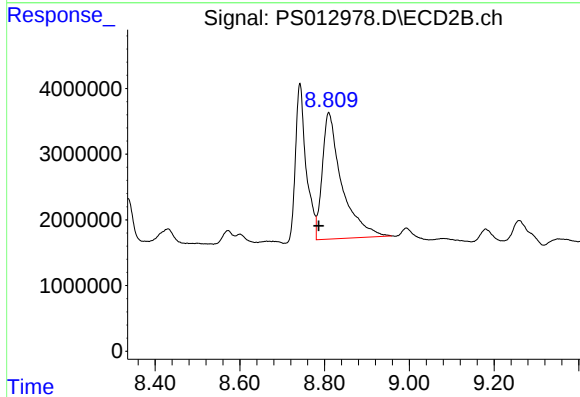


#11 2,4,5-TP (SILVEX)

R.T.: 8.810 min
Delta R.T.: 0.024 min
Response: 61692404
Conc: 26.02 ng/ml

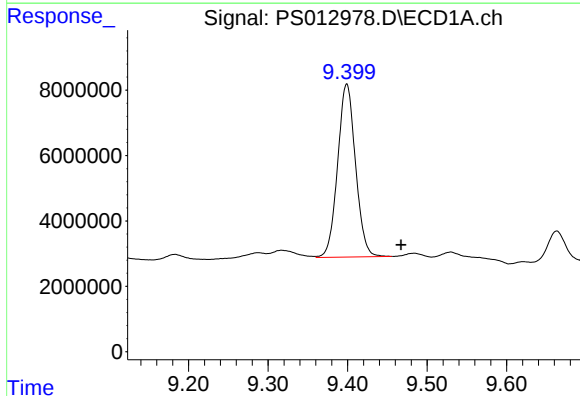


#12 2,4,5-T

R.T.: 9.399 min
Delta R.T.: -0.068 min
Response: 82750239
Conc: 15.80 ng/ml

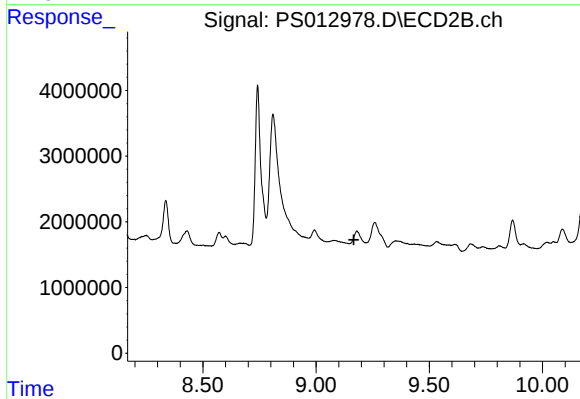

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.167 min
Response: 0
Conc: N.D.

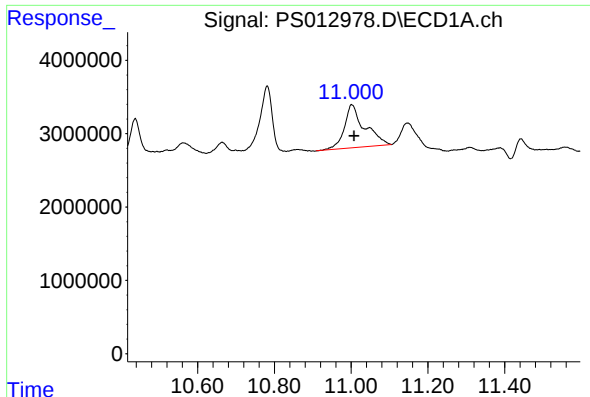

#15 Picloram

R.T.: 11.002 min
Delta R.T.: -0.006 min
Response: 21555070
Conc: 3.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

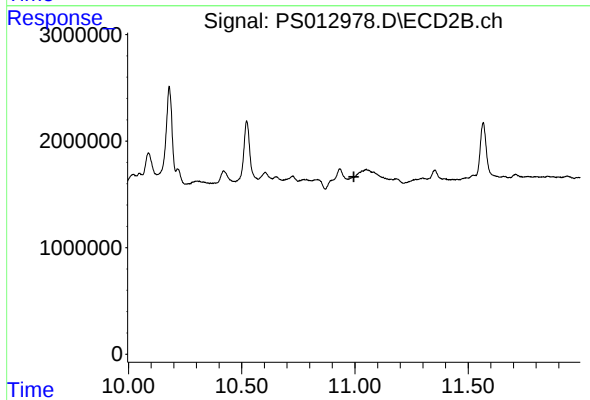

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.