

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102620\
 Data File : PS012990.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2020 00:11
 Operator : DD\AJ
 Sample : L4503-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 01:29:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.916	459.2E6	244.0E6	513.068	608.121
Target Compounds							
1) T	Dalapon	2.992	2.589	65088346	118.7E6	64.027	225.790 #
2) T	3,5-DICHL...	0.000	6.099	0	46364357	N.D.	73.583
3) T	4-Nitroph...	6.987	0.000	6983534	0	16.698	N.D. #
5) T	DICAMBA	0.000	7.050	0	7560791	N.D.	4.443
7) T	MCPA	7.756	7.373	30042548	30321029	7.846	13.840 #
8) T	DICHLORPROP	0.000	7.768	0	4484440	N.D.	9.762
9) T	2,4-D	8.389	0.000	72271400	0	70.044	N.D. #
10) T	Pentachlo...	8.685	0.000	14269794	0	1.112	N.D. #
11) T	2,4,5-TP ...	0.000	8.769	0	6535032	N.D.	2.757
12) T	2,4,5-T	9.401	0.000	32699449	0	6.245	N.D. #
14) T	DINOSEB	0.000	10.007	0	12720322	N.D.	7.564
15) T	Picloram	0.000	10.936	0	4297238	N.D.	1.194
16) T	DCPA	0.000	10.936	0	4297238	N.D.	1.410



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102620\
Data File : PS012990.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2020 00:11
Operator : DD\AJ
Sample : L4503-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 01:29:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

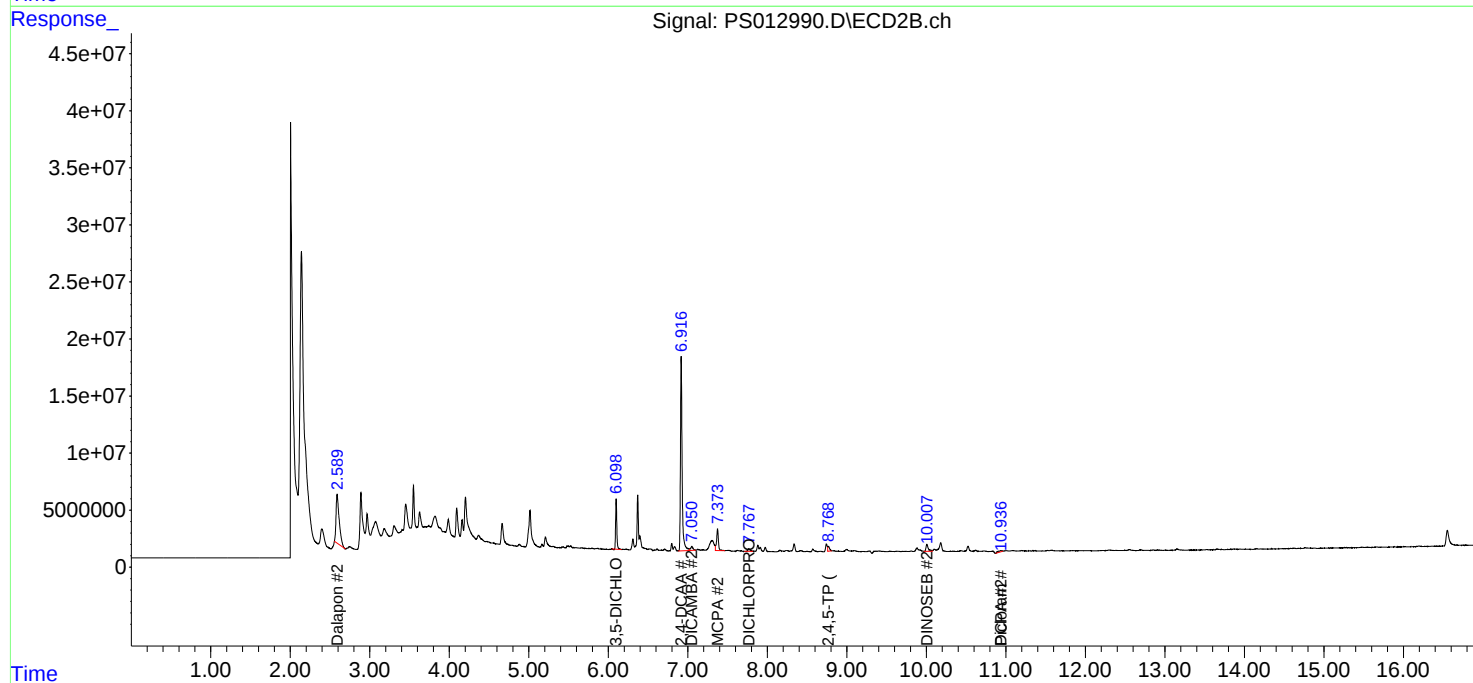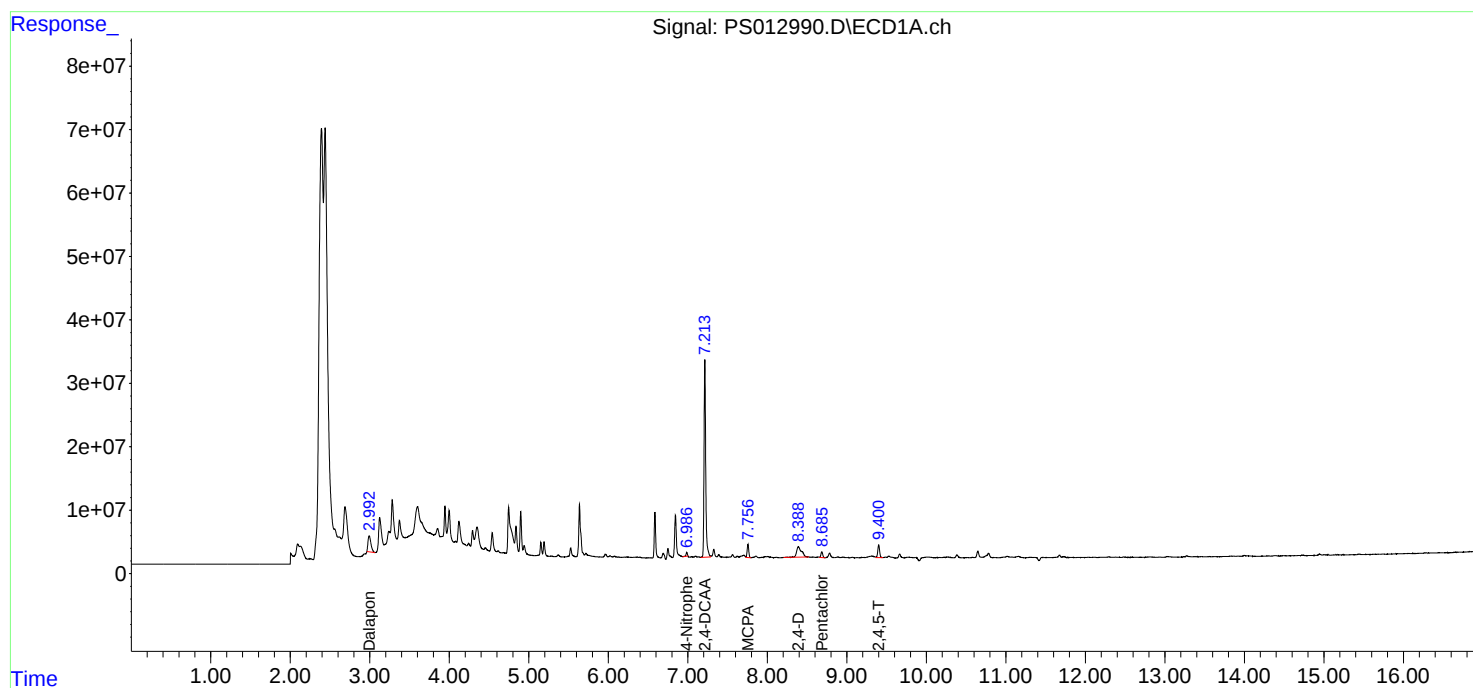


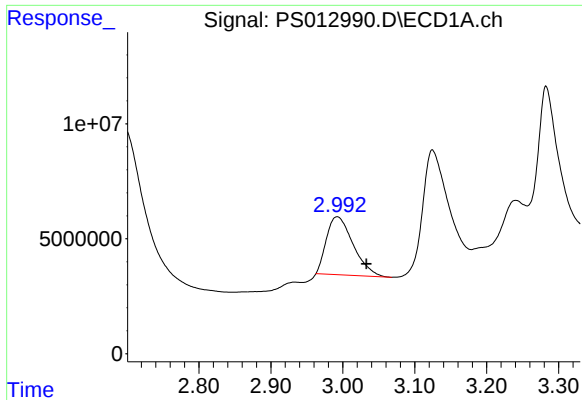

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.041 min
Response: 65088346
Conc: 64.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

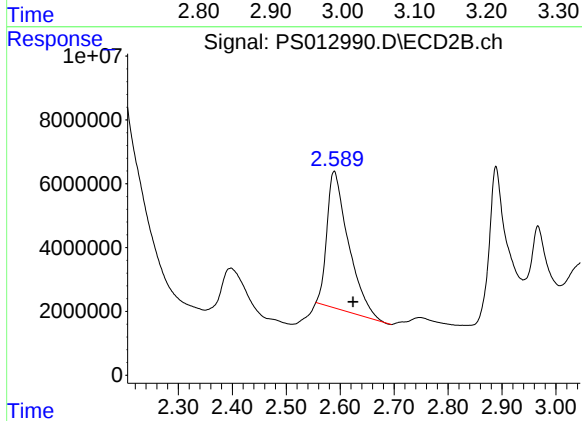


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 118737797
Conc: 225.79 ng/ml

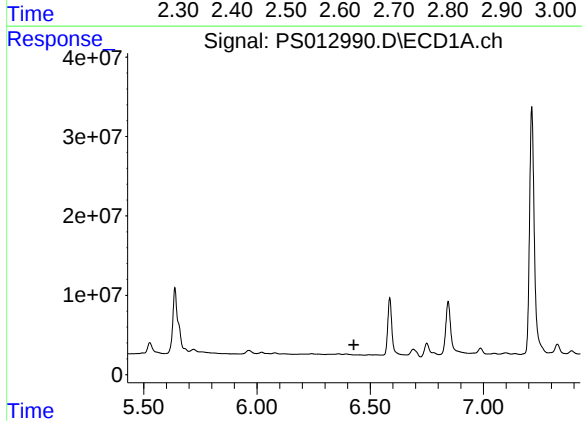


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

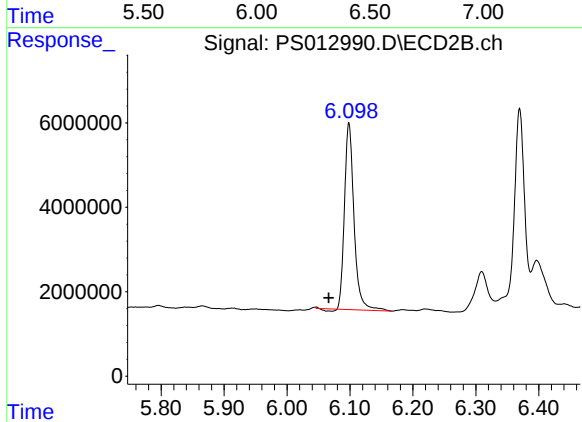

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.099 min
Delta R.T.: 0.032 min
Response: 46364357
Conc: 73.58 ng/ml

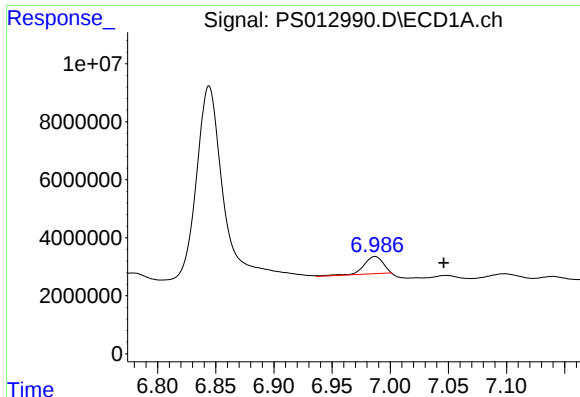

#3 4-Nitrophenol


R.T.: 6.987 min
Delta R.T.: -0.059 min
Response: 6983534
Conc: 16.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

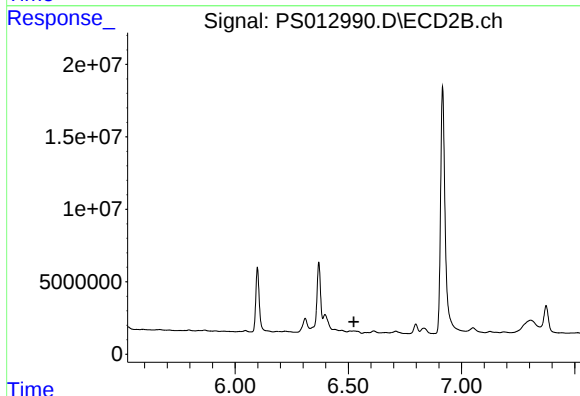


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

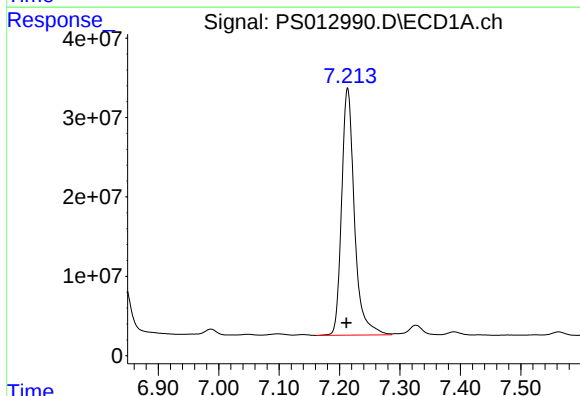


#4 2,4-DCAA

R.T.: 7.213 min
Delta R.T.: 0.002 min
Response: 459231013
Conc: 513.07 ng/ml

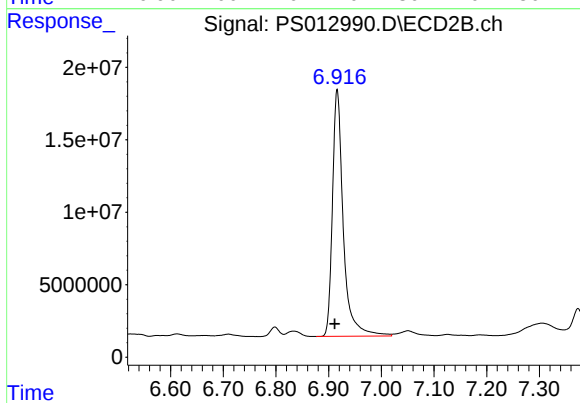

#4 2,4-DCAA


R.T.: 6.916 min
Delta R.T.: 0.005 min
Response: 244009493
Conc: 608.12 ng/ml

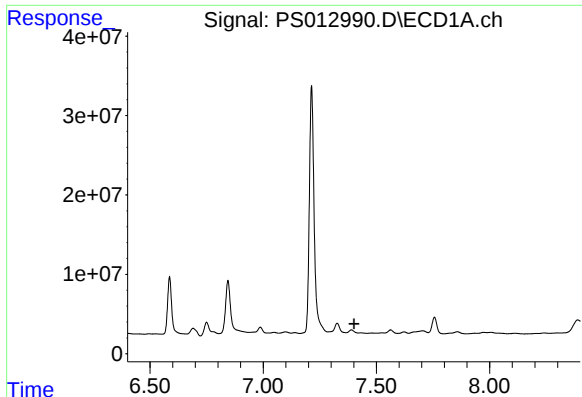

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.401 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

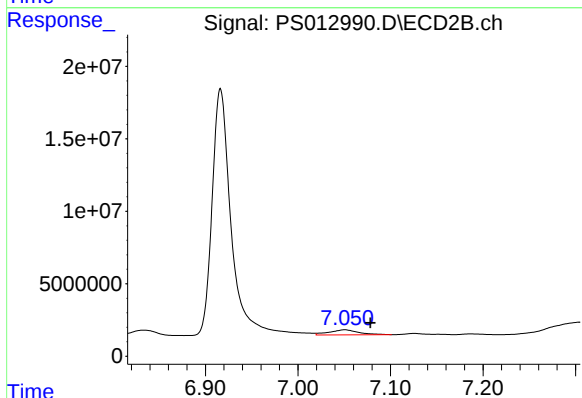


#5 DICAMBA

R.T.: 7.050 min
Delta R.T.: -0.028 min
Response: 7560791
Conc: 4.44 ng/ml

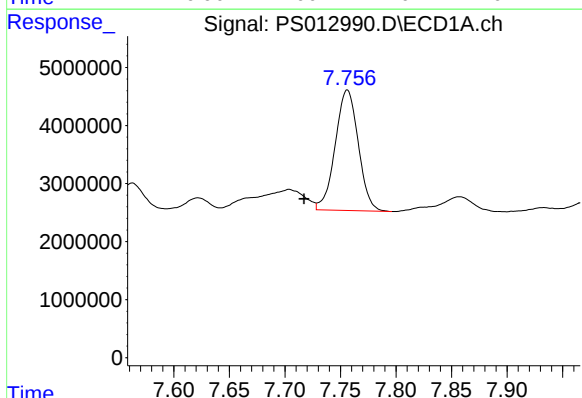


#7 MCPA

R.T.: 7.756 min
Delta R.T.: 0.039 min
Response: 30042548
Conc: 7.85 ug/ml

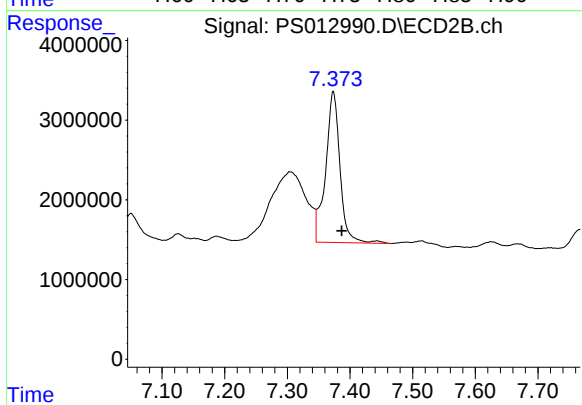

#7 MCPA


R.T.: 7.373 min
Delta R.T.: -0.014 min
Response: 30321029
Conc: 13.84 ug/ml

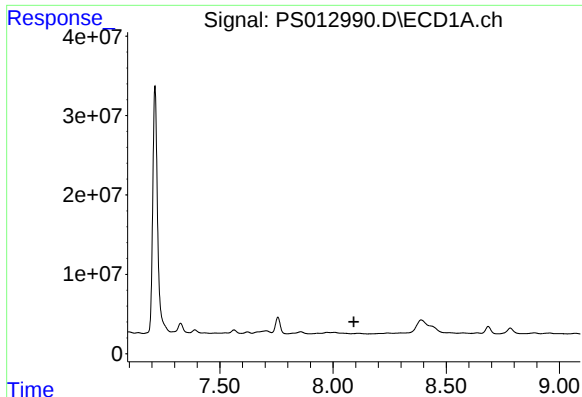

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

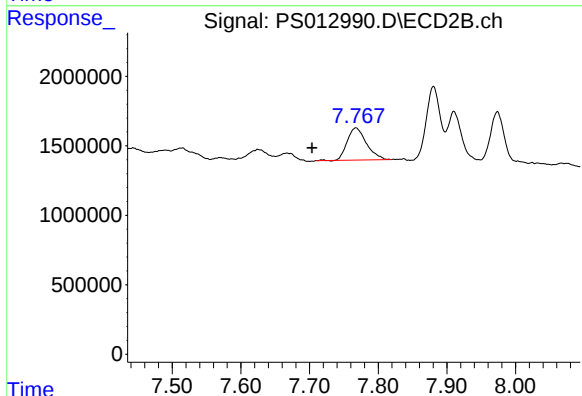


#8 DICHLORPROP

R.T.: 7.768 min
Delta R.T.: 0.064 min
Response: 4484440
Conc: 9.76 ng/ml

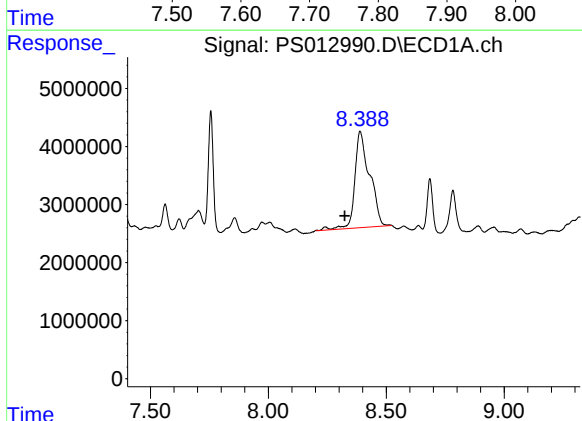


#9 2,4-D

R.T.: 8.389 min
Delta R.T.: 0.065 min
Response: 72271400
Conc: 70.04 ng/ml

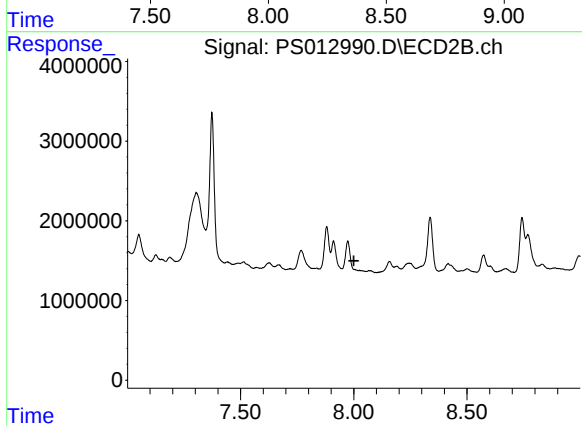

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

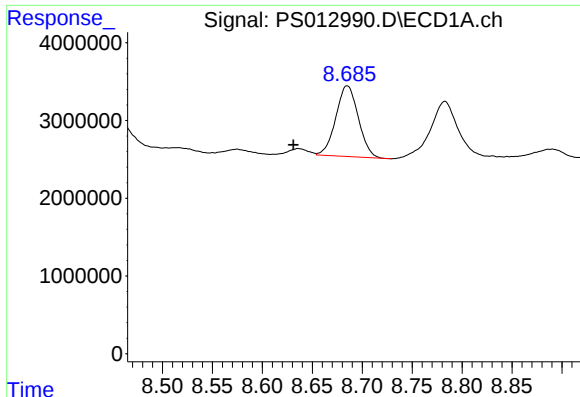

#10 Pentachlorophenol


R.T.: 8.685 min
Delta R.T.: 0.054 min
Response: 14269794
Conc: 1.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

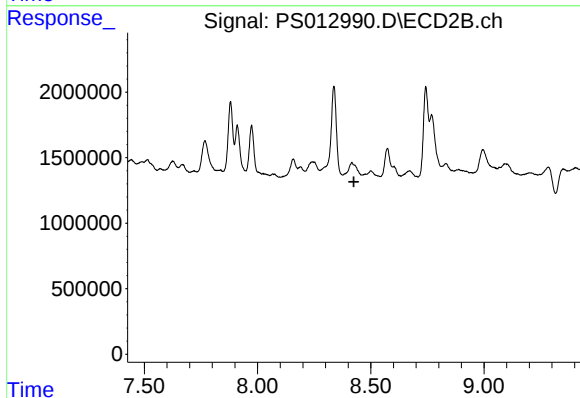


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.425 min
Response: 0
Conc: N.D.

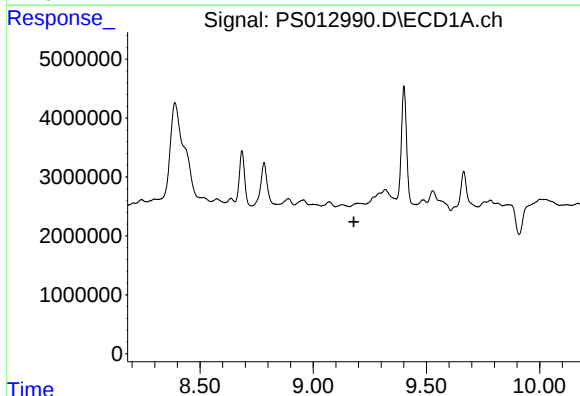


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.180 min
Response: 0
Conc: N.D.

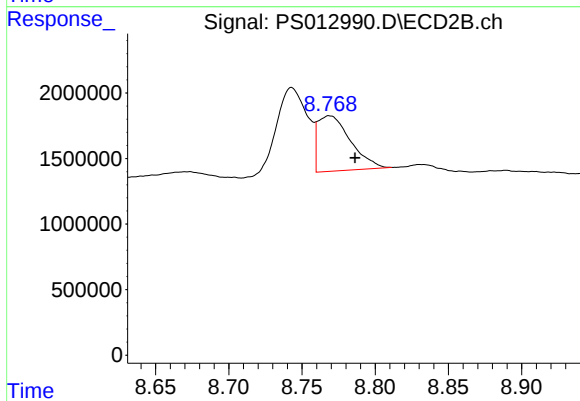

#11 2,4,5-TP (SILVEX)


R.T.: 8.769 min
Delta R.T.: -0.018 min
Response: 6535032
Conc: 2.76 ng/ml

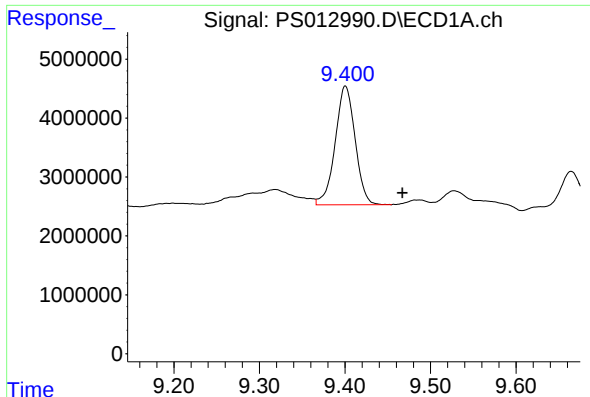

#12 2,4,5-T


R.T.: 9.401 min
Delta R.T.: -0.067 min
Response: 32699449
Conc: 6.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

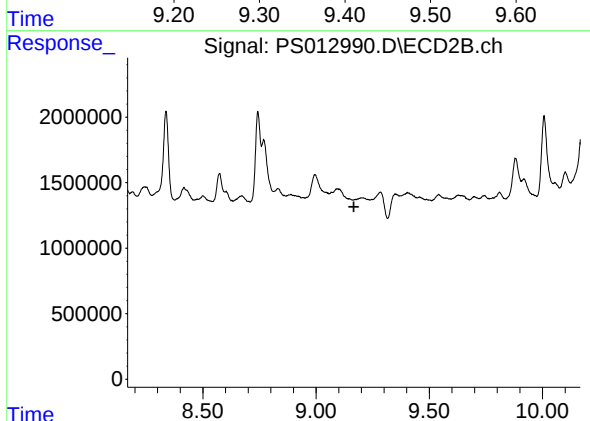


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.167 min
Response: 0
Conc: N.D.

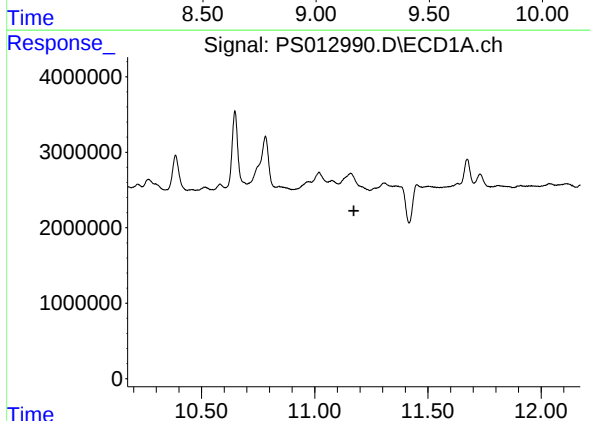


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.173 min
Response: 0
Conc: N.D.

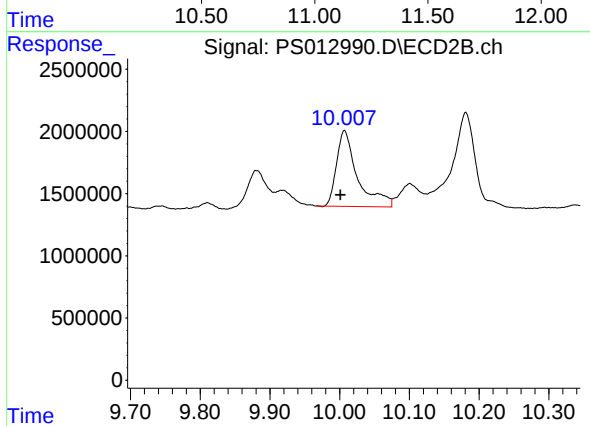

#14 DINOSEB


R.T.: 10.007 min
Delta R.T.: 0.006 min
Response: 12720322
Conc: 7.56 ng/ml

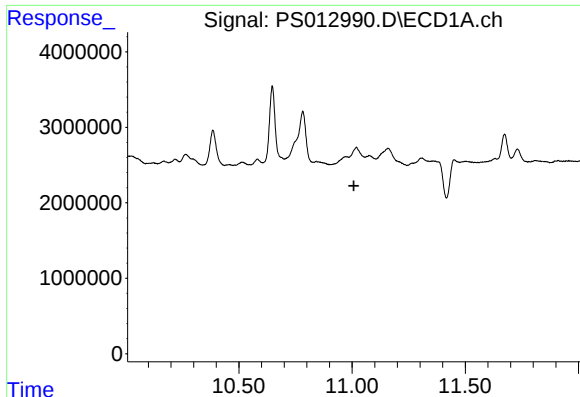

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

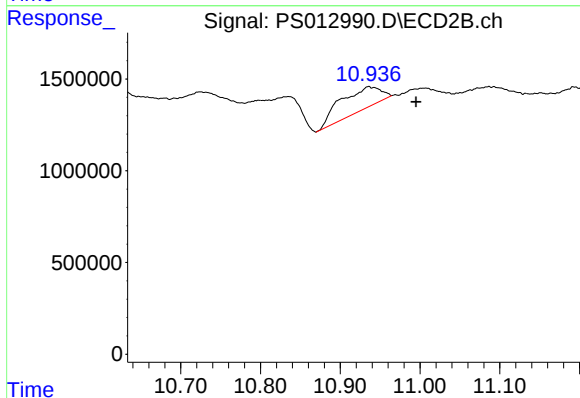


#15 Picloram

R.T.: 10.936 min
Delta R.T.: -0.059 min
Response: 4297238
Conc: 1.19 ng/ml

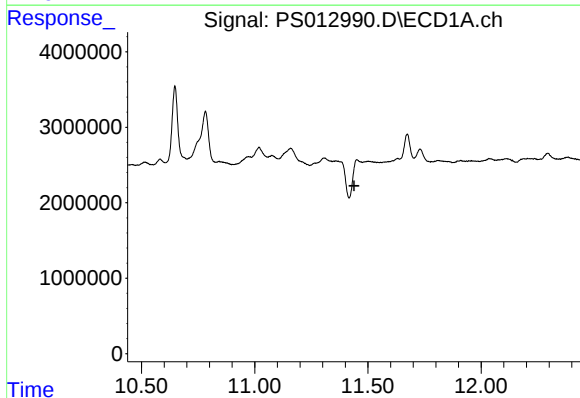

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.438 min
Response: 0
Conc: N.D.

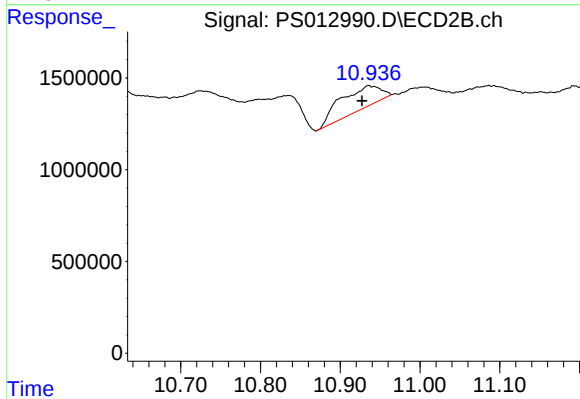

#16 DCPA

R.T.: 10.936 min
Delta R.T.: 0.009 min
Response: 4297238
Conc: 1.41 ng/ml