

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102621\
 Data File : PS017204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2021 08:50
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 14:04:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.158	0.000	19979687	0	13.072	N.D.	#
Target Compounds								
7) T	MCPA	7.604f	0.000	26057298	0	4.224	N.D.	#
8) T	DICHLORPROP	8.077f	0.000	4289448	0	2.861	N.D.	#
13) T	2,4-DB	9.883f	0.000	6069313	0	4.035	N.D.	#
15) T	Picloram	10.941	10.782	35767520	11827935	3.349	3.088	
16) T	DCPA	0.000	10.782f	0	11827935	N.D.	2.772	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102621\
Data File : PS017204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2021 08:50
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 14:04:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

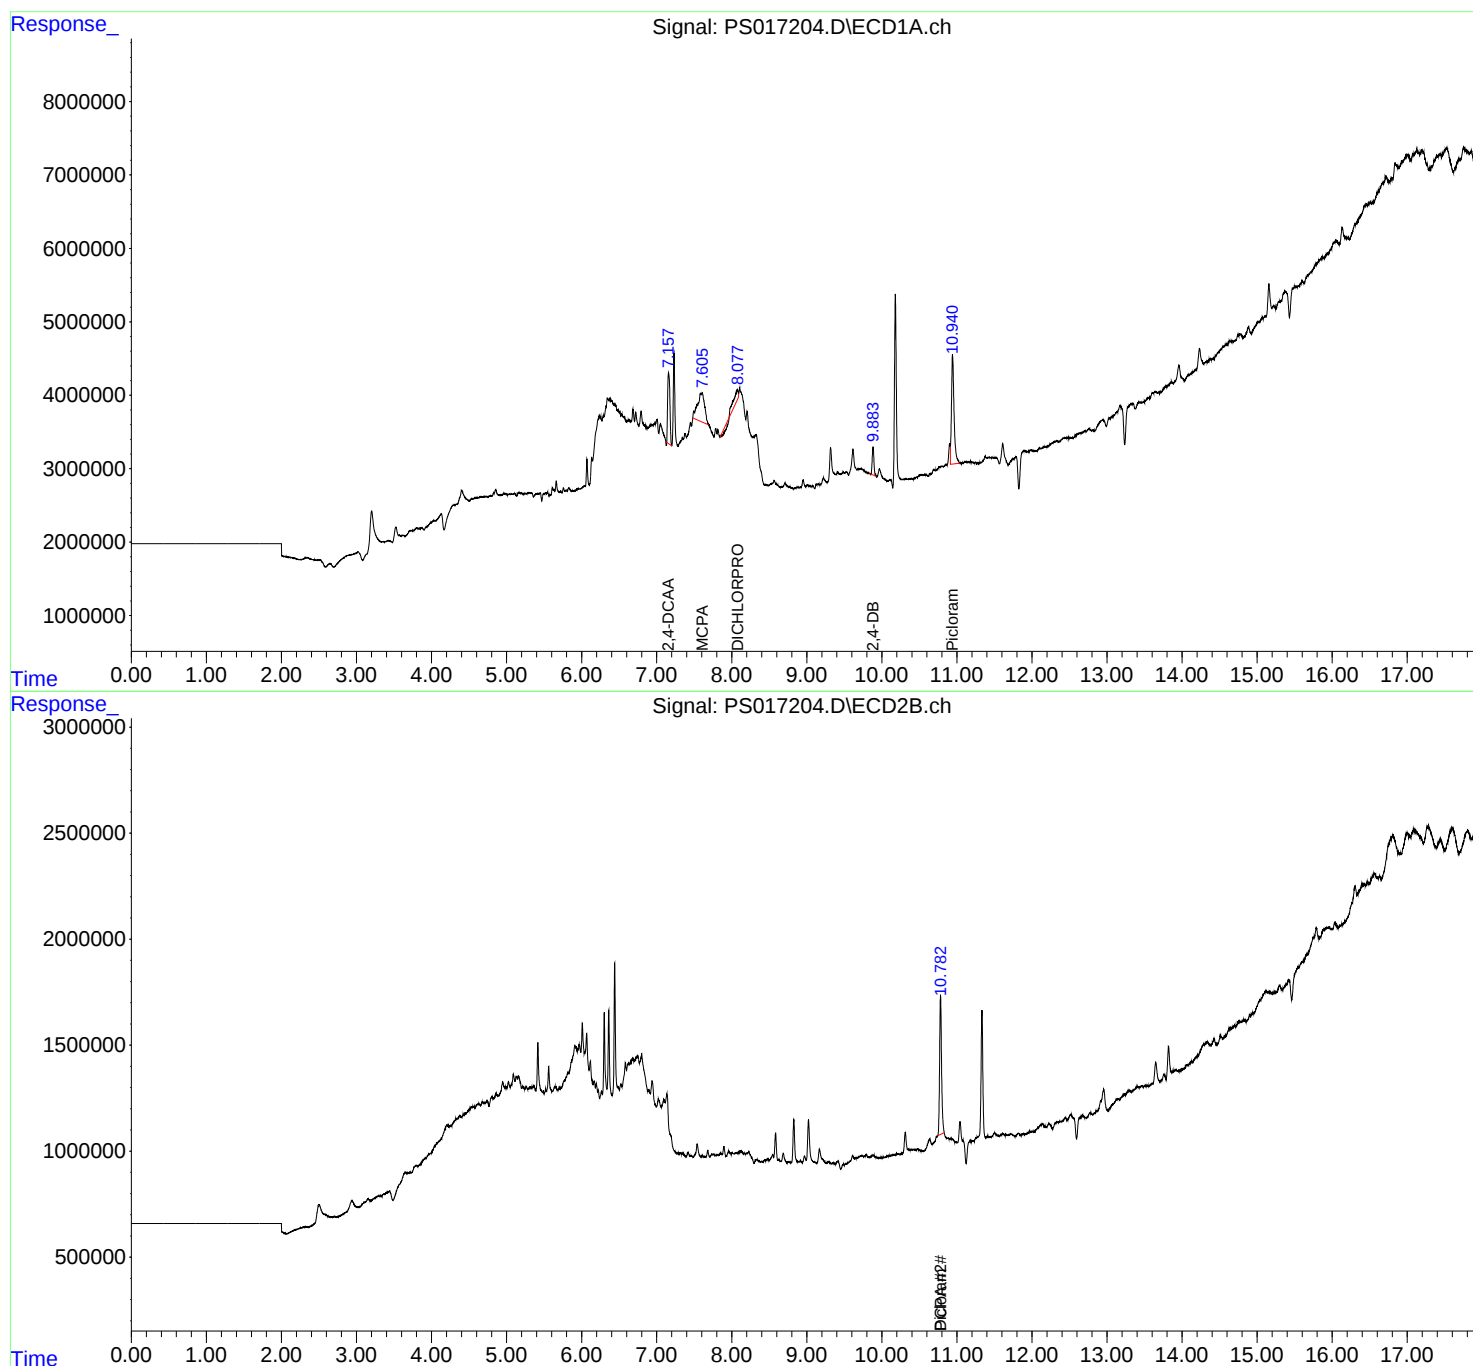


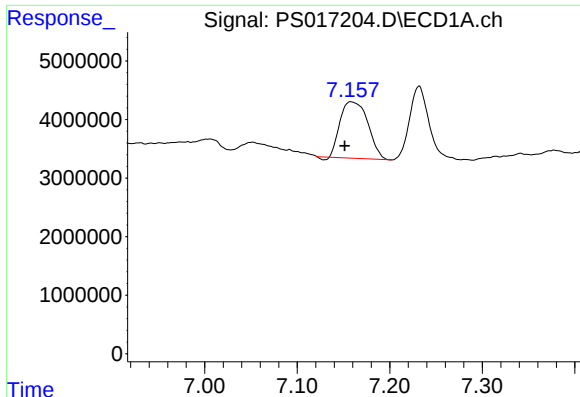

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: 0.007 min
Response: 19979687
Conc: 13.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

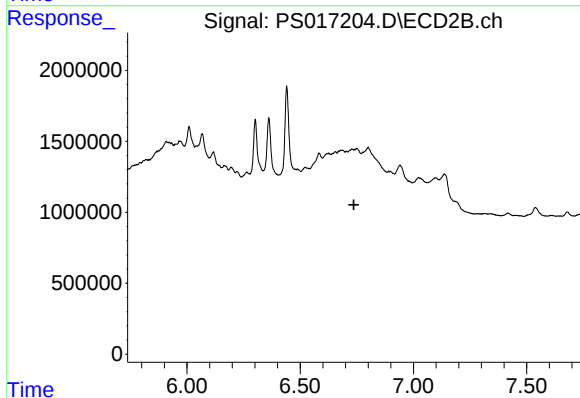


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

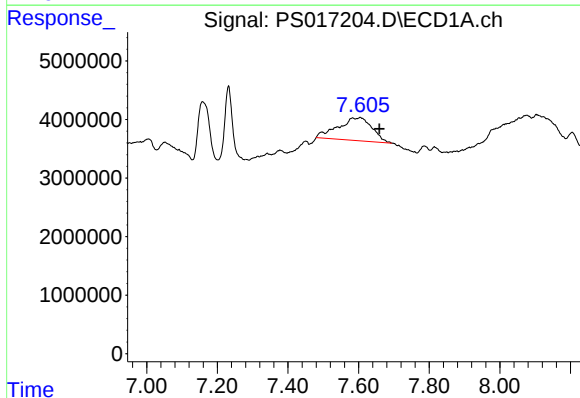


#7 MCPA

R.T.: 7.604 min
Delta R.T.: -0.054 min
Response: 26057298
Conc: 4.22 ug/ml

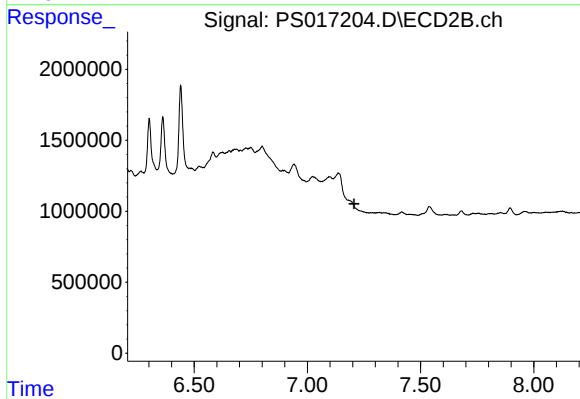

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

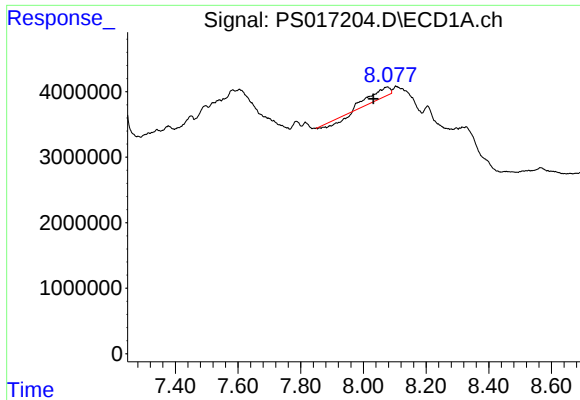

#8 DICHLORPROP


R.T.: 8.077 min
Delta R.T.: 0.045 min
Response: 4289448
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

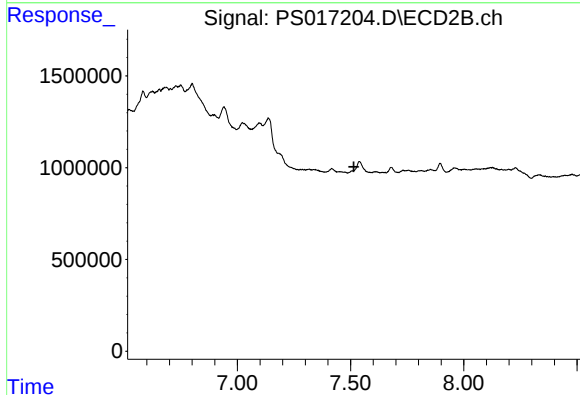


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

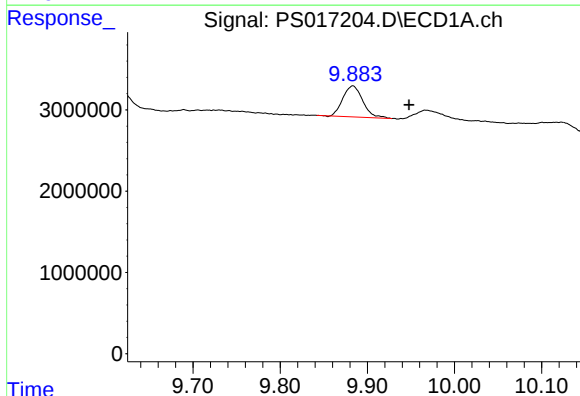


#13 2,4-DB

R.T.: 9.883 min
Delta R.T.: -0.065 min
Response: 6069313
Conc: 4.03 ng/ml

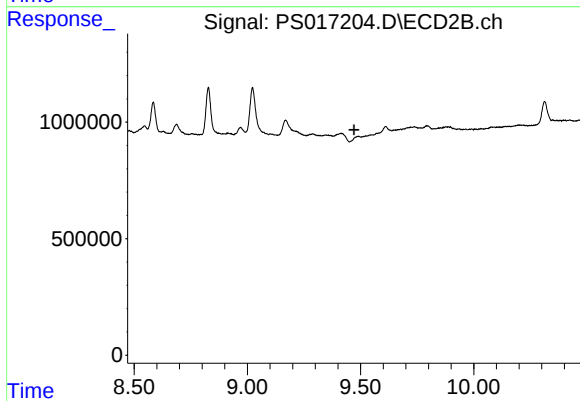

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

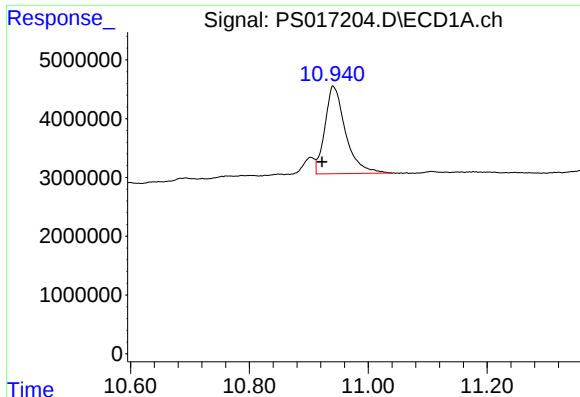

#15 Picloram


R.T.: 10.941 min
Delta R.T.: 0.019 min
Response: 35767520
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

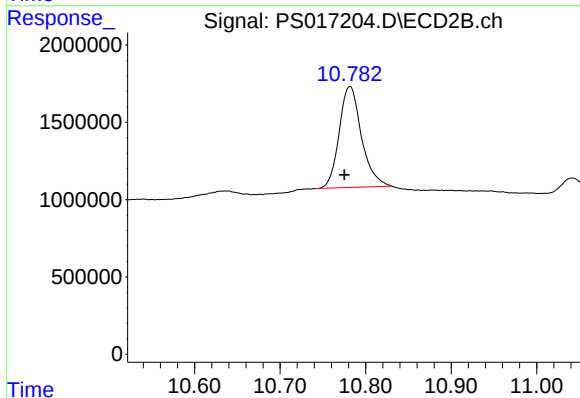


#15 Picloram

R.T.: 10.782 min
Delta R.T.: 0.007 min
Response: 11827935
Conc: 3.09 ng/ml

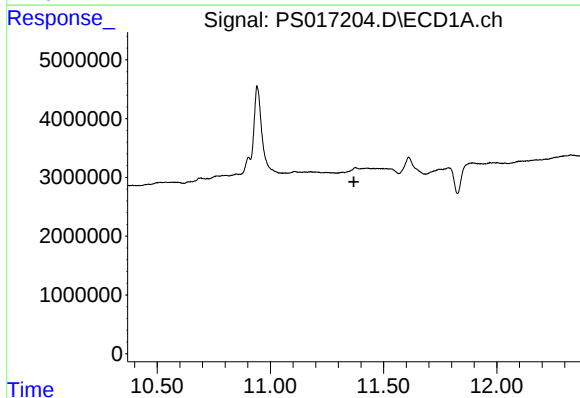

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.369 min
Response: 0
Conc: N.D.

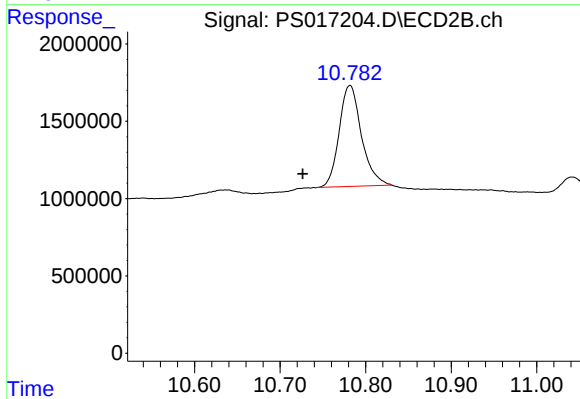

#16 DCPA

R.T.: 10.782 min
Delta R.T.: 0.055 min
Response: 11827935
Conc: 2.77 ng/ml