

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
 Data File : PS002166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 11:57
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:20:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.429	10.903	158.5E6	156.1E6	503.828	434.565
Target Compounds							
6) T	MCP	0.000	11.425	0	890580	N.D.	1.035 #
9) T	2,4-D	13.345	0.000	23446368	0	58.268	N.D. #
12) T	2,4,5-T	0.000	14.525	0	3672676	N.D.	2.453 #
15) T	Picloram	16.954	16.834	5930468	7609886	2.486	3.364 #
16) T	DCPA	0.000	16.834	0	7609886	N.D.	3.214 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
Data File : PS002166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 11:57
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:20:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

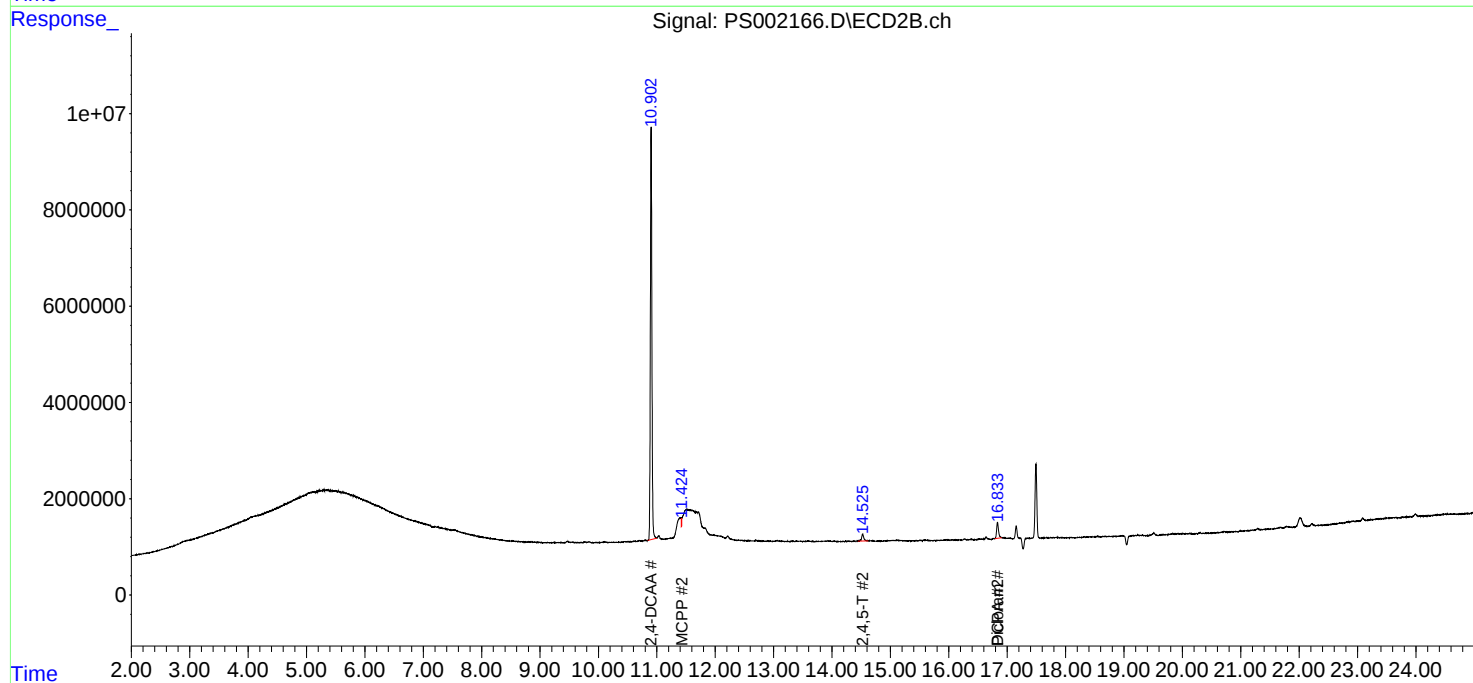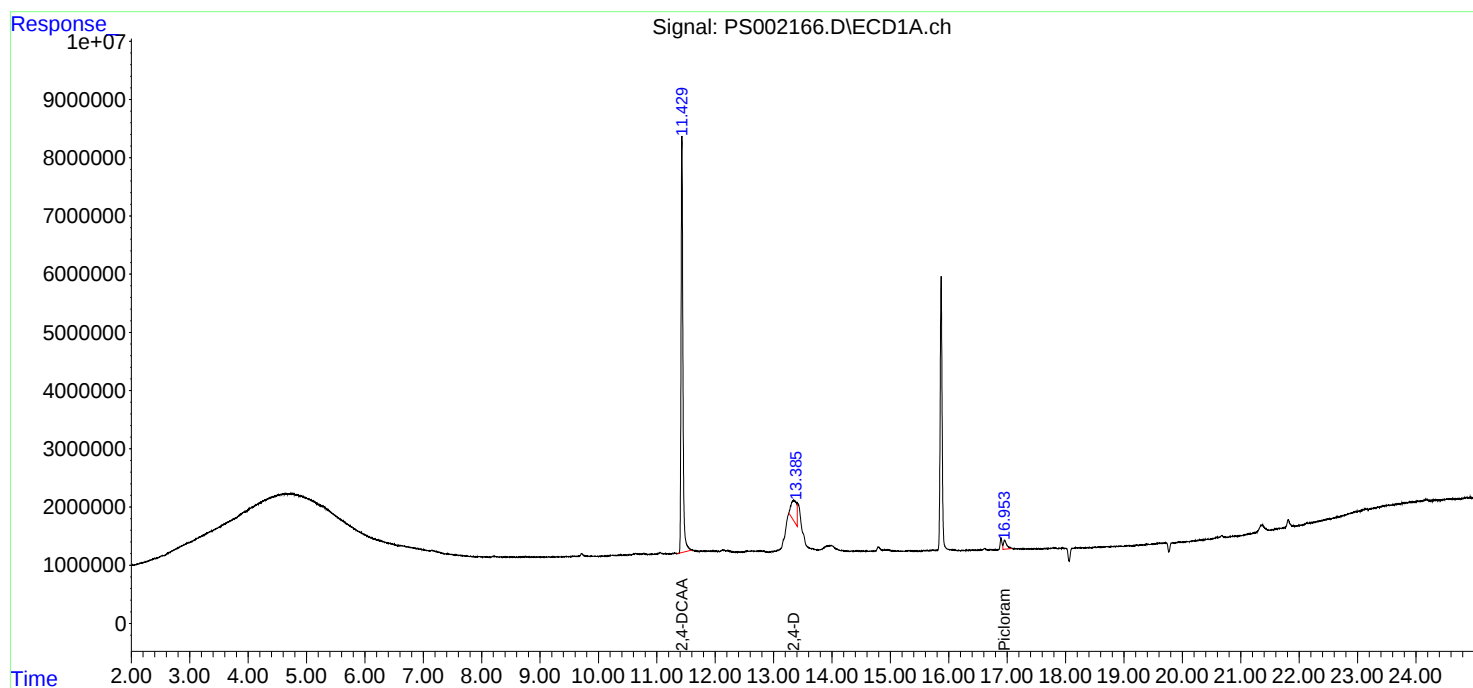


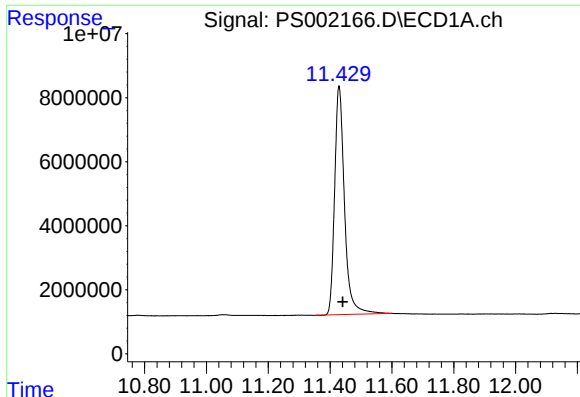

#4 2,4-DCAA


R.T.: 11.429 min
Delta R.T.: -0.012 min
Response: 158547506
Conc: 503.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

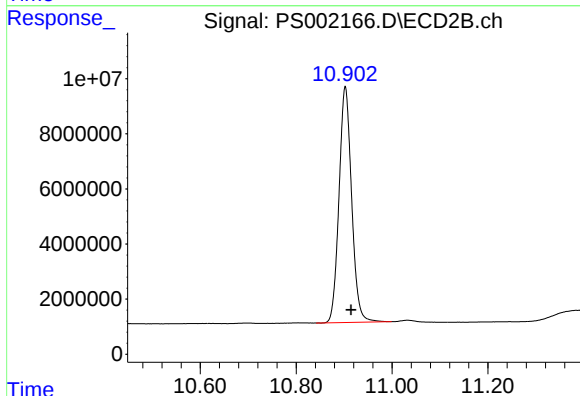


#4 2,4-DCAA

R.T.: 10.903 min
Delta R.T.: -0.012 min
Response: 156051330
Conc: 434.56 ng/ml

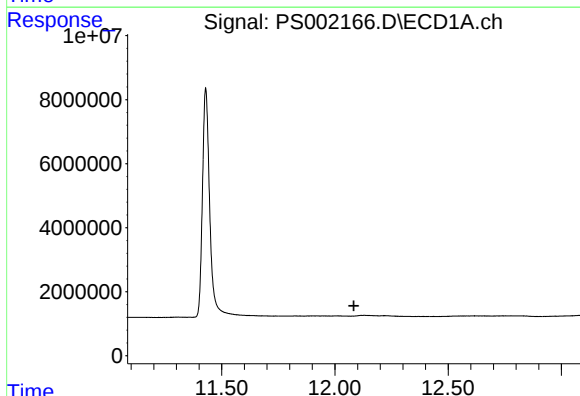


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

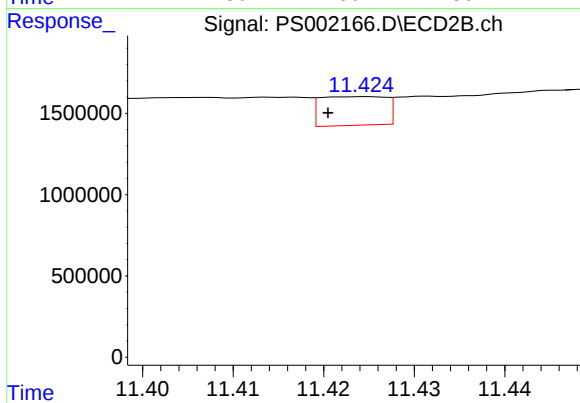

#6 MCP


R.T.: 11.425 min
Delta R.T.: 0.004 min
Response: 890580
Conc: 1.04 ug/ml

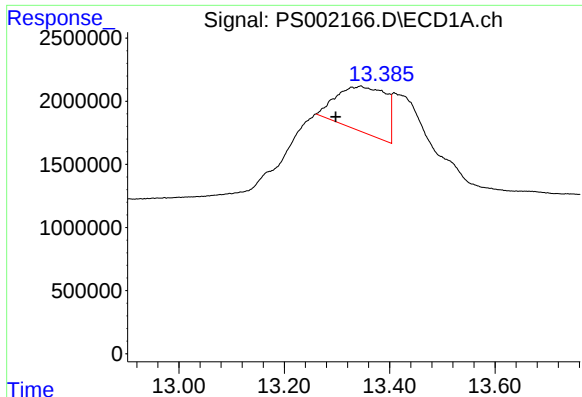

#9 2,4-D


R.T.: 13.345 min
Delta R.T.: 0.047 min
Response: 23446368
Conc: 58.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

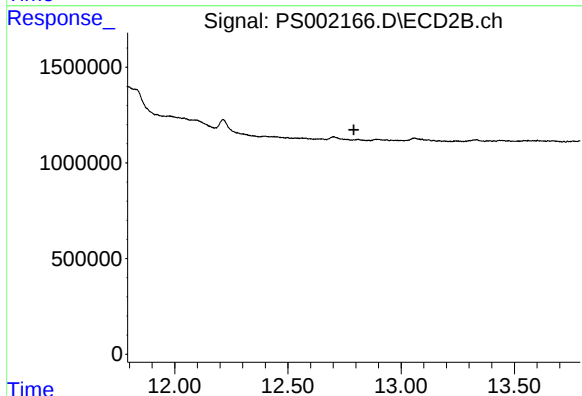


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 12.791 min
Response: 0
Conc: N.D.

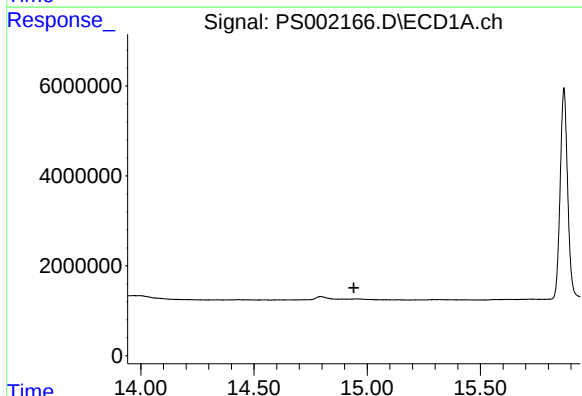


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.941 min
Response: 0
Conc: N.D.

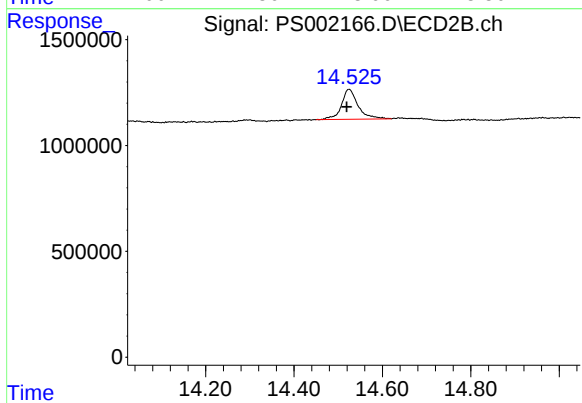

#12 2,4,5-T


R.T.: 14.525 min
Delta R.T.: 0.006 min
Response: 3672676
Conc: 2.45 ng/ml

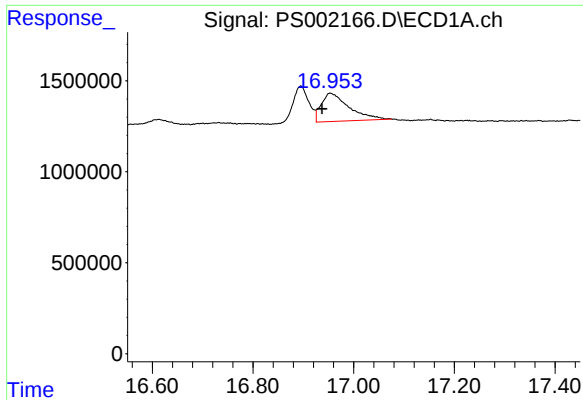

#15 Picloram


R.T.: 16.954 min
Delta R.T.: 0.016 min
Response: 5930468
Conc: 2.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

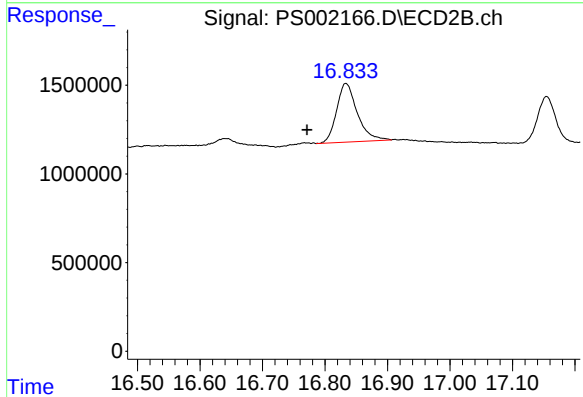


#15 Picloram

R.T.: 16.834 min
Delta R.T.: 0.062 min
Response: 7609886
Conc: 3.36 ng/ml

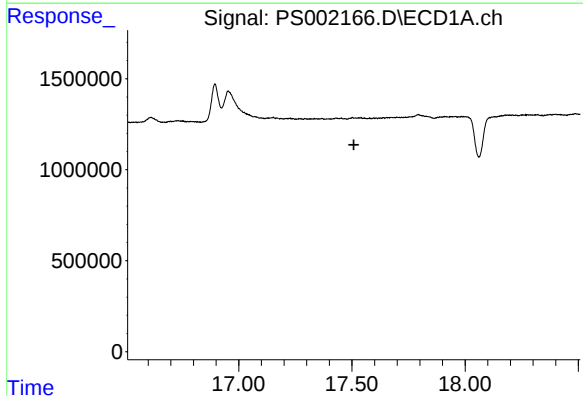

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

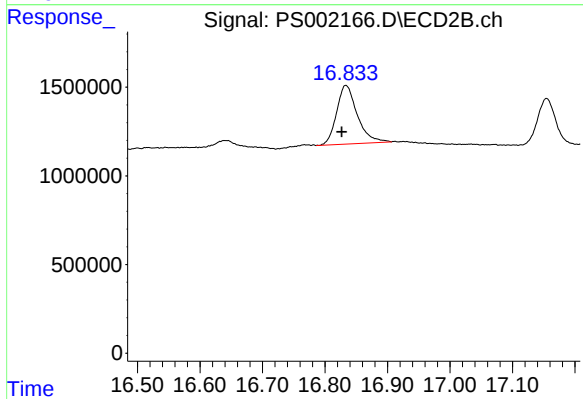

#16 DCPA

R.T.: 16.834 min
Delta R.T.: 0.007 min
Response: 7609886
Conc: 3.21 ng/ml