

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
 Data File : PS002172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 15:07
 Operator : EI\SJ
 Sample : J5654-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:22:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.455	10.937	12932078	9619554	41.095	26.788 #
Target Compounds							
1) T	Dalapon	2.916	2.364	18192796	35441272	39.664	78.496 #
3) T	4-Nitroph...	11.017	10.093	3675195	9418365	22.030	52.820 #
6) T	MCP	12.118	11.402	37405468	48013	37.865	0.056 #
7) T	MCPA	0.000	11.794	0	19293508	N.D.	14.256 #
9) T	2,4-D	0.000	12.799	0	1289600	N.D.	3.028 #
10) T	Pentachlo...	13.688	13.360	5974806	-1365883	1.242	N.D. #
11) T	2,4,5-TP ...	0.000	14.005	0	1797829	N.D.	0.983 #
12) T	2,4,5-T	0.000	14.507	0	1837671	N.D.	1.227 #
13) T	2,4-DB	0.000	15.130	0	361664	N.D.	1.632 #
14) T	DINOSEB	0.000	15.612	0	2412094	N.D.	1.905 #
15) T	Picloram	16.907	16.802	28000398	2597632	11.739	1.148 #
16) T	DCPA	0.000	16.802	0	2597632	N.D.	1.097 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
Data File : PS002172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 15:07
Operator : EI\SJ
Sample : J5654-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:22:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

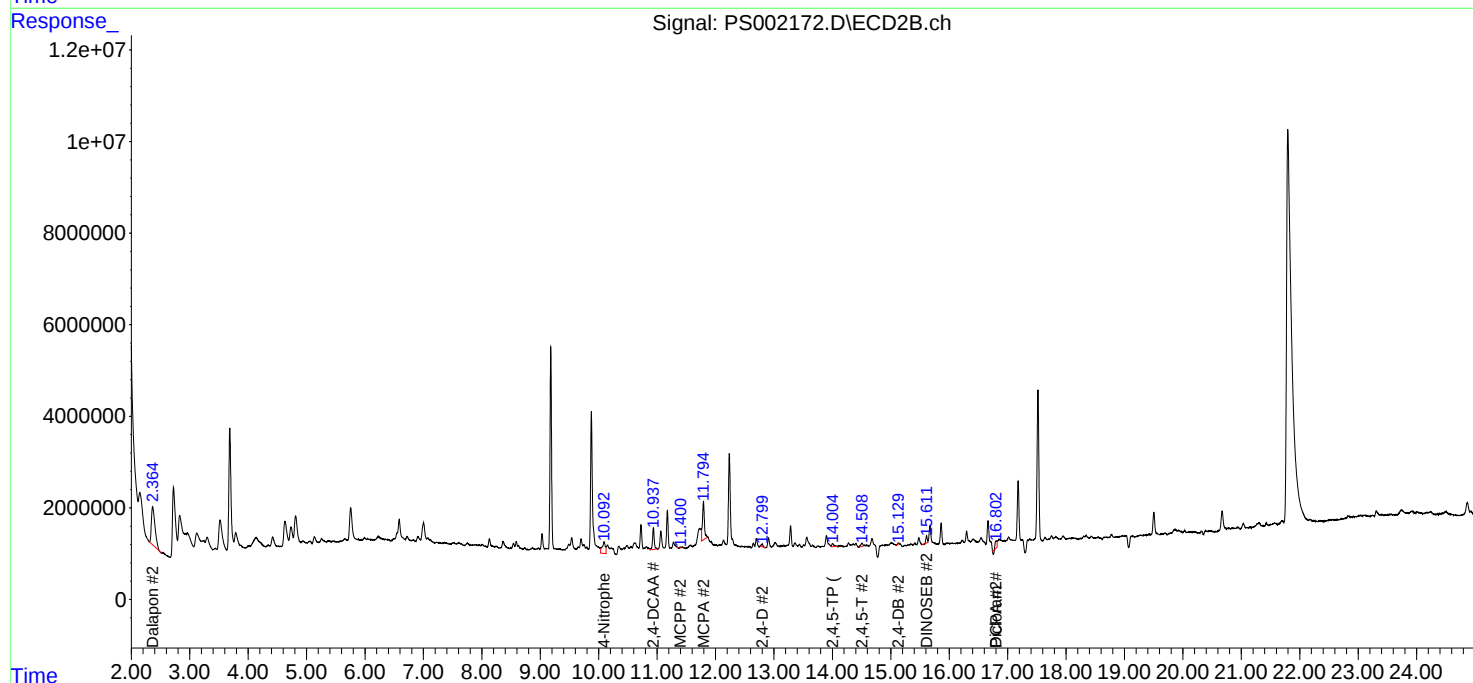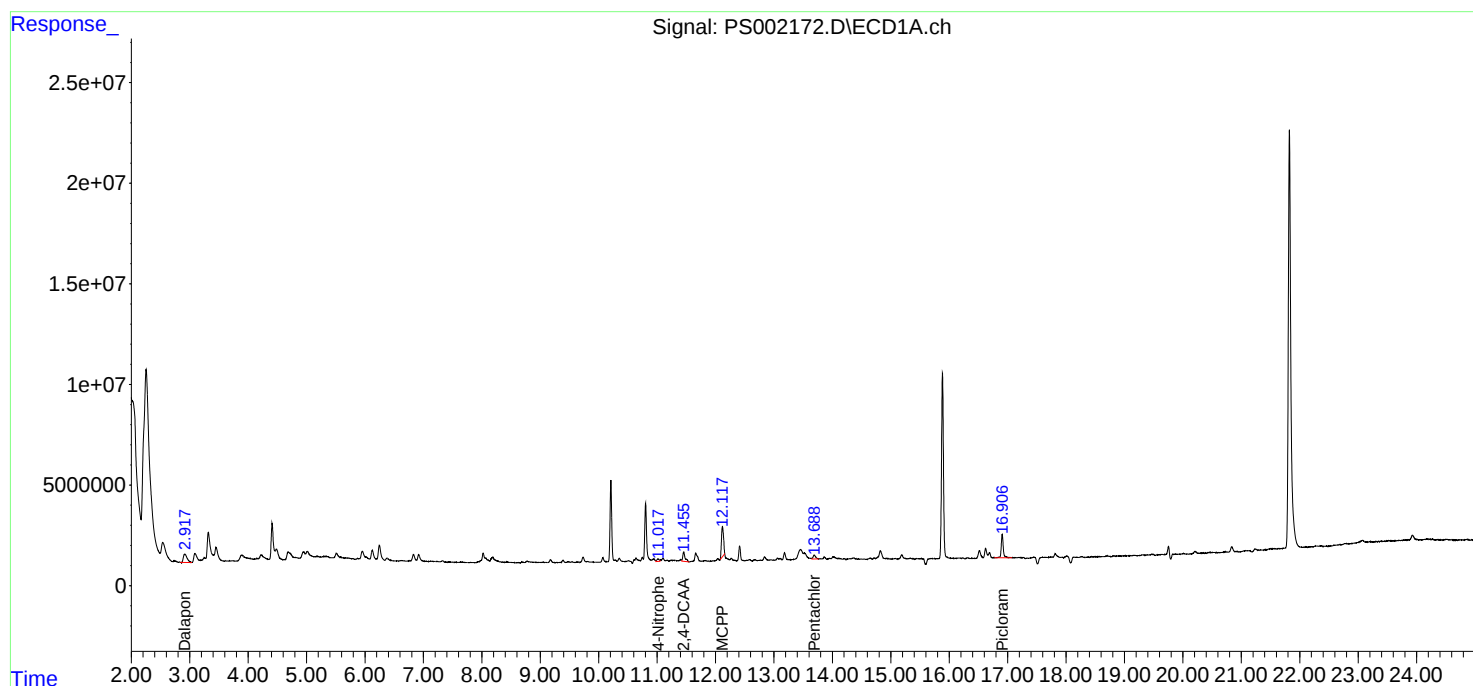


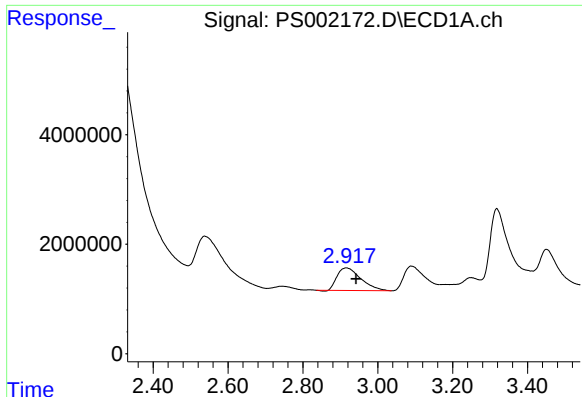

#1 Dalapon


R.T.: 2.916 min
Delta R.T.: -0.026 min
Response: 18192796
Conc: 39.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

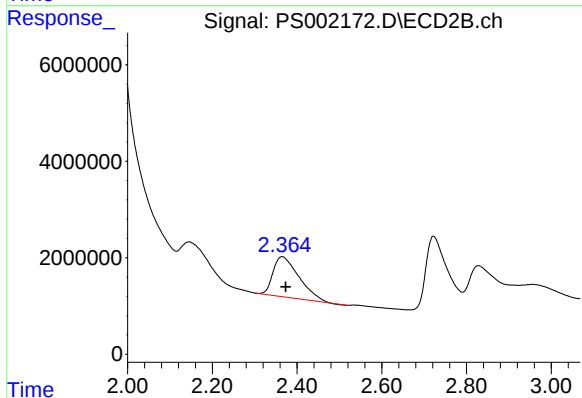


#1 Dalapon

R.T.: 2.364 min
Delta R.T.: -0.009 min
Response: 35441272
Conc: 78.50 ng/ml

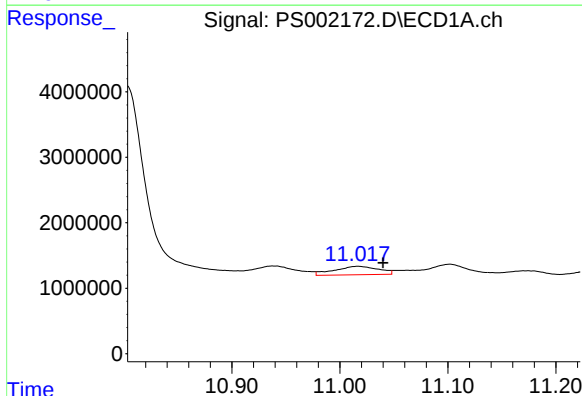


#3 4-Nitrophenol

R.T.: 11.017 min
Delta R.T.: -0.023 min
Response: 3675195
Conc: 22.03 ng/ml

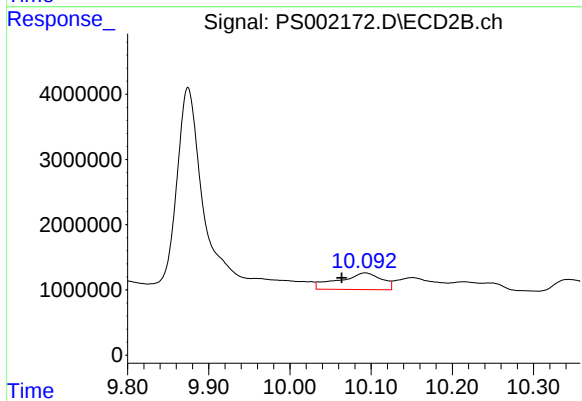

#3 4-Nitrophenol


R.T.: 10.093 min
Delta R.T.: 0.029 min
Response: 9418365
Conc: 52.82 ng/ml

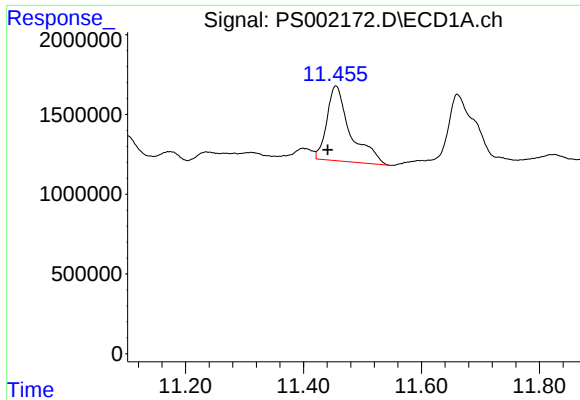

#4 2,4-DCAA


R.T.: 11.455 min
Delta R.T.: 0.014 min
Response: 12932078
Conc: 41.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

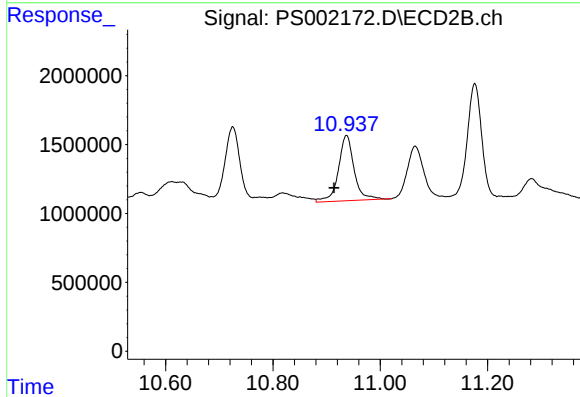


#4 2,4-DCAA

R.T.: 10.937 min
Delta R.T.: 0.023 min
Response: 9619554
Conc: 26.79 ng/ml

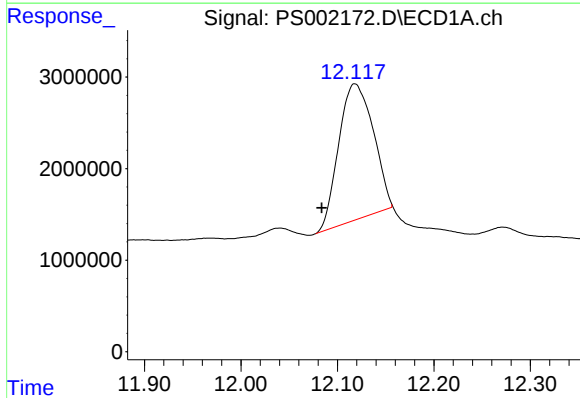


#6 MCP

R.T.: 12.118 min
Delta R.T.: 0.035 min
Response: 37405468
Conc: 37.87 ug/ml

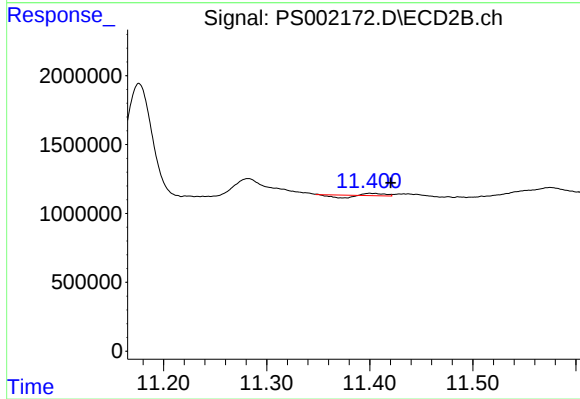

#6 MCP


R.T.: 11.402 min
Delta R.T.: -0.019 min
Response: 48013
Conc: 0.06 ug/ml

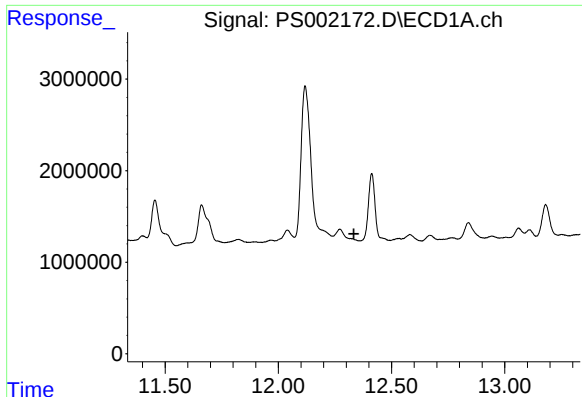

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

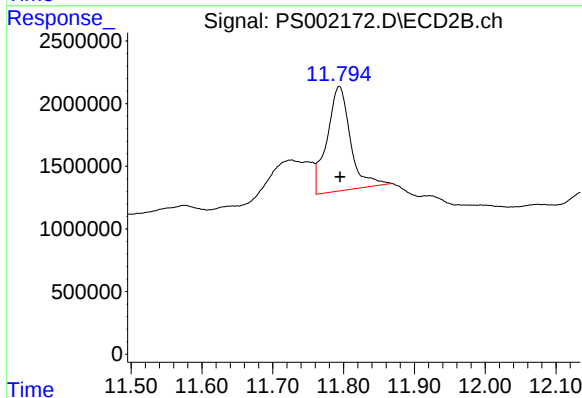


#7 MCPA

R.T.: 11.794 min
Delta R.T.: -0.001 min
Response: 19293508
Conc: 14.26 ug/ml

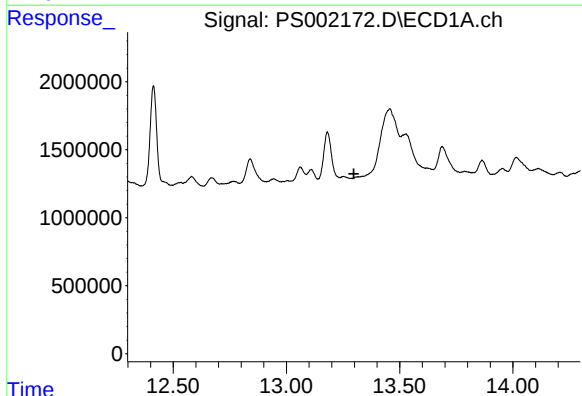


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

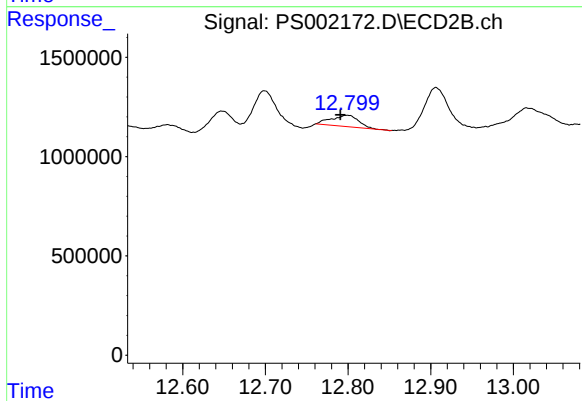

#9 2,4-D


R.T.: 12.799 min
Delta R.T.: 0.008 min
Response: 1289600
Conc: 3.03 ng/ml

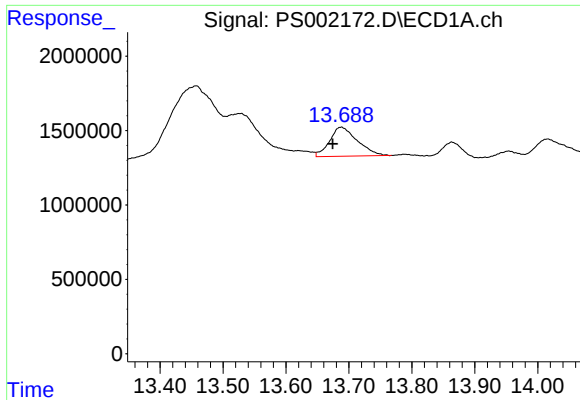

#10 Pentachlorophenol


R.T.: 13.688 min
Delta R.T.: 0.014 min
Response: 5974806
Conc: 1.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

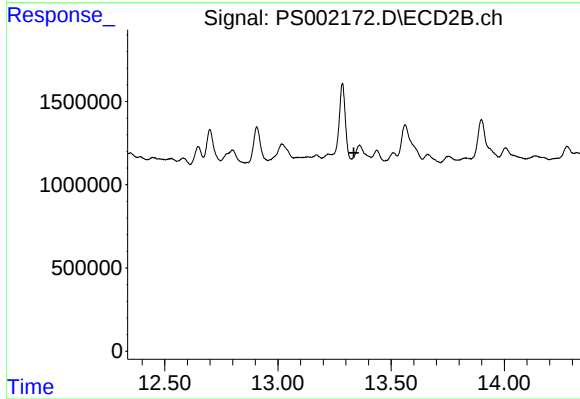


#10 Pentachlorophenol

R.T.: 13.360 min
Delta R.T.: 0.025 min
Response: -1365883
Conc: N.D.

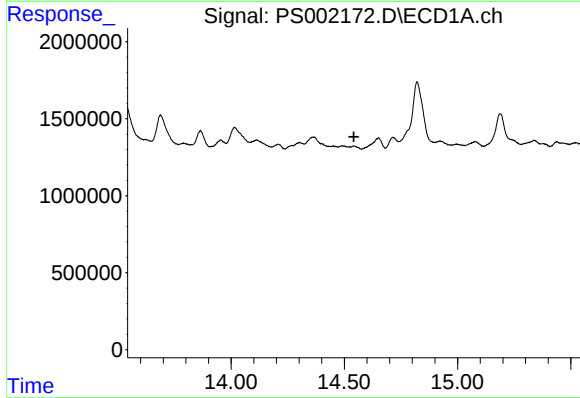


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

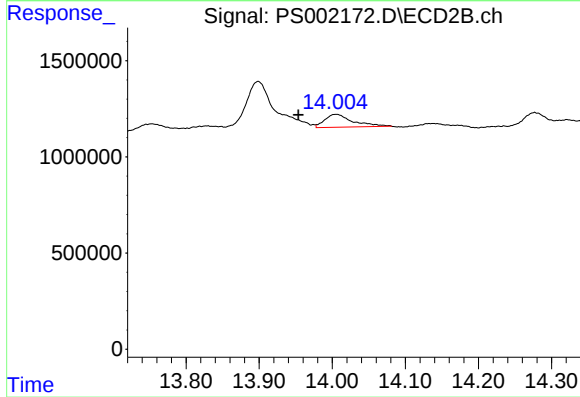

#11 2,4,5-TP (SILVEX)


R.T.: 14.005 min
Delta R.T.: 0.052 min
Response: 1797829
Conc: 0.98 ng/ml

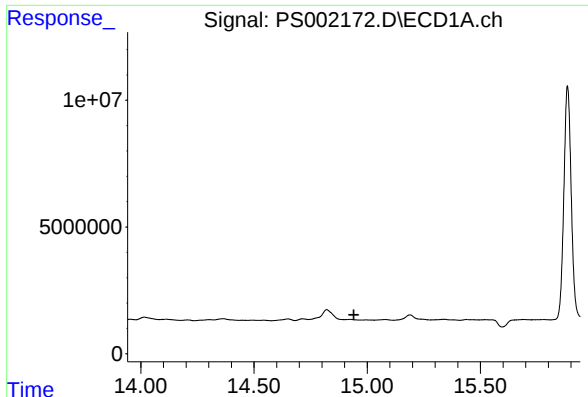

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

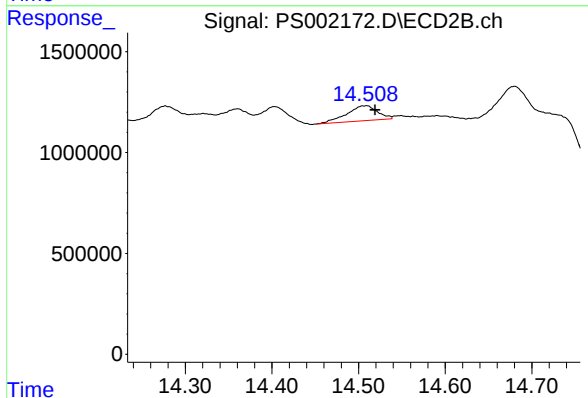


#12 2,4,5-T

R.T.: 14.507 min
Delta R.T.: -0.012 min
Response: 1837671
Conc: 1.23 ng/ml

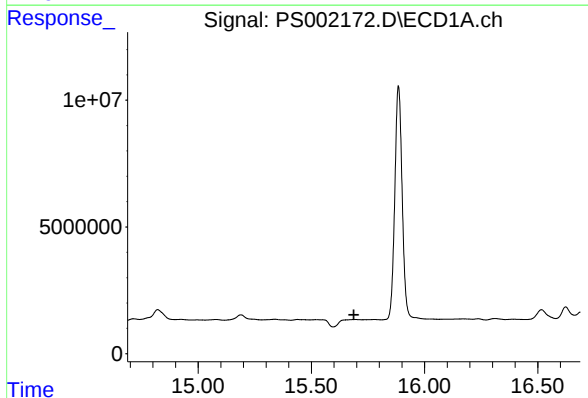


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

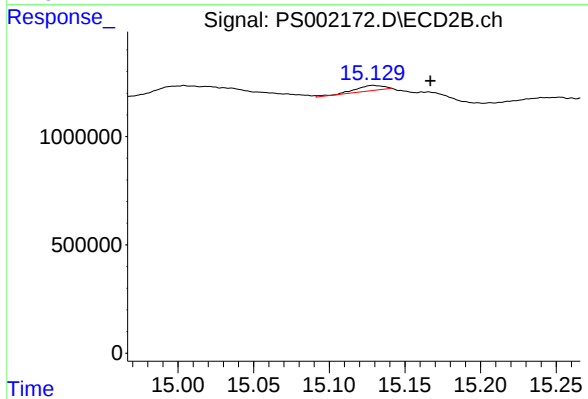

#13 2,4-DB


R.T.: 15.130 min
Delta R.T.: -0.037 min
Response: 361664
Conc: 1.63 ng/ml

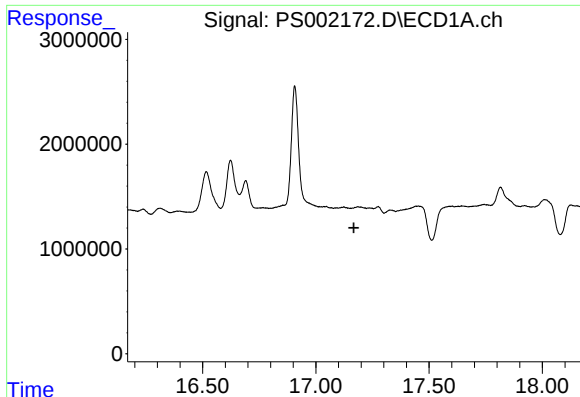

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

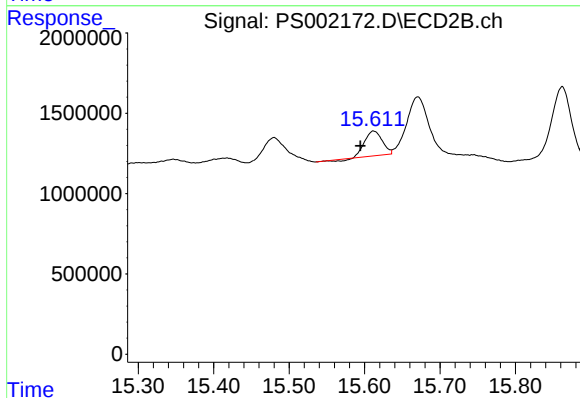


#14 DINOSEB

R.T.: 15.612 min
Delta R.T.: 0.018 min
Response: 2412094
Conc: 1.91 ng/ml

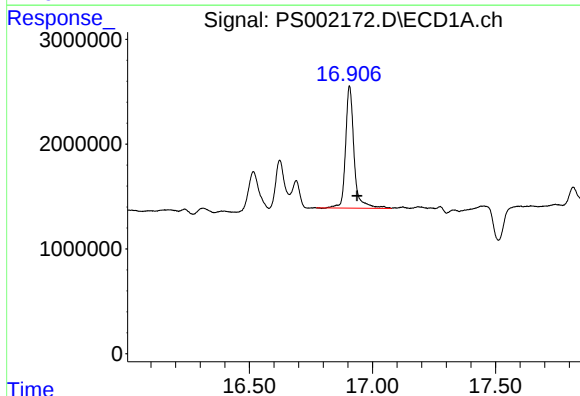


#15 Picloram

R.T.: 16.907 min
Delta R.T.: -0.031 min
Response: 28000398
Conc: 11.74 ng/ml

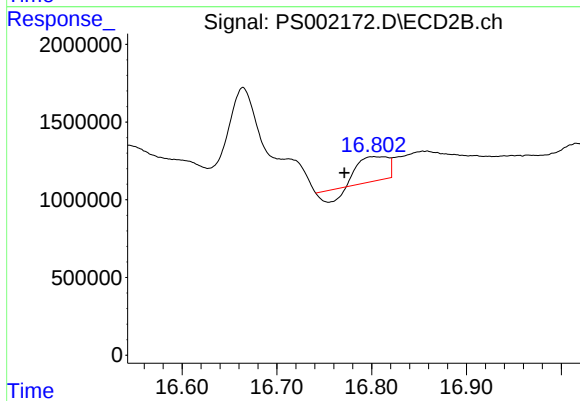

#15 Picloram


R.T.: 16.802 min
Delta R.T.: 0.031 min
Response: 2597632
Conc: 1.15 ng/ml

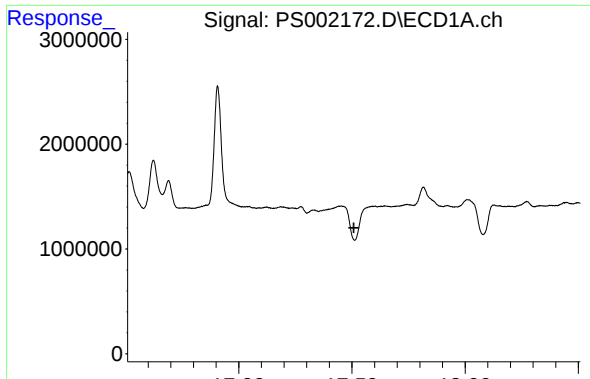

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

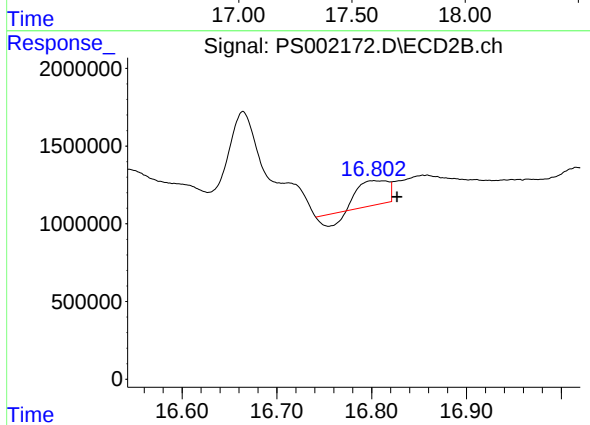

#16 DCPA

R.T.: 16.802 min
Delta R.T.: -0.024 min
Response: 2597632
Conc: 1.10 ng/ml