

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
 Data File : PS002175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 16:40
 Operator : EI\SJ
 Sample : J5626-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:22:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.483	10.903	46562703	3407215	147.966	9.488 #
Target Compounds							
1) T	Dalapon	2.947	2.391	10590392	520567	23.089	1.153 #
2) T	3,5-DICHL...	0.000	9.062	0	43549541	N.D.	98.183 #
3) T	4-Nitroph...	10.970	10.094	3101442	2990768	18.591	16.773
5) T	DICAMBA	11.694	11.209	18126046	76438125	13.649	61.165 #
6) T	MCPD	0.000	11.471	0	3616025	N.D.	4.203 #
7) T	MCPA	12.305	11.826	-713180	17357003	N.D.	12.825
8) T	DICHLORPROP	12.972	12.269	2186740	18370101	6.279	57.204 #
9) T	2,4-D	0.000	12.807	0	2659009	N.D.	6.243 #
10) T	Pentachlo...	13.719	13.318	20948161	8020048	4.355	1.707 #
11) T	2,4,5-TP ...	0.000	13.924	0	2314674	N.D.	1.265 #
12) T	2,4,5-T	0.000	14.531	0	611350	N.D.	0.408 #
13) T	2,4-DB	15.755	15.214	20639329	6852695	87.898	30.930 #
14) T	DINOSEB	17.206	15.583	3808176	1836274	2.780	1.451 #
15) T	Picloram	16.939	16.830	37653061	-3430728	15.786	N.D. #
16) T	DCPA	17.443	16.830	3704258	-3430728	1.578	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
Data File : PS002175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 16:40
Operator : EI\SJ
Sample : J5626-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:22:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

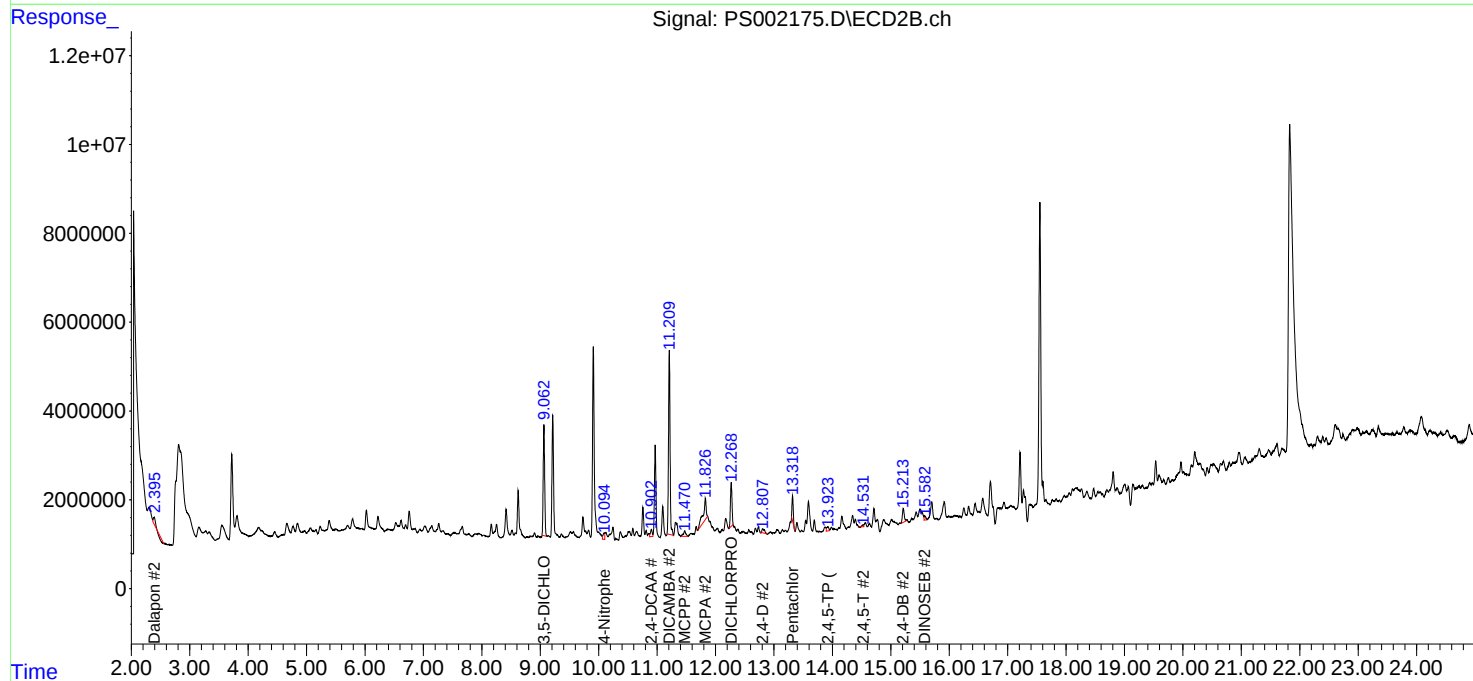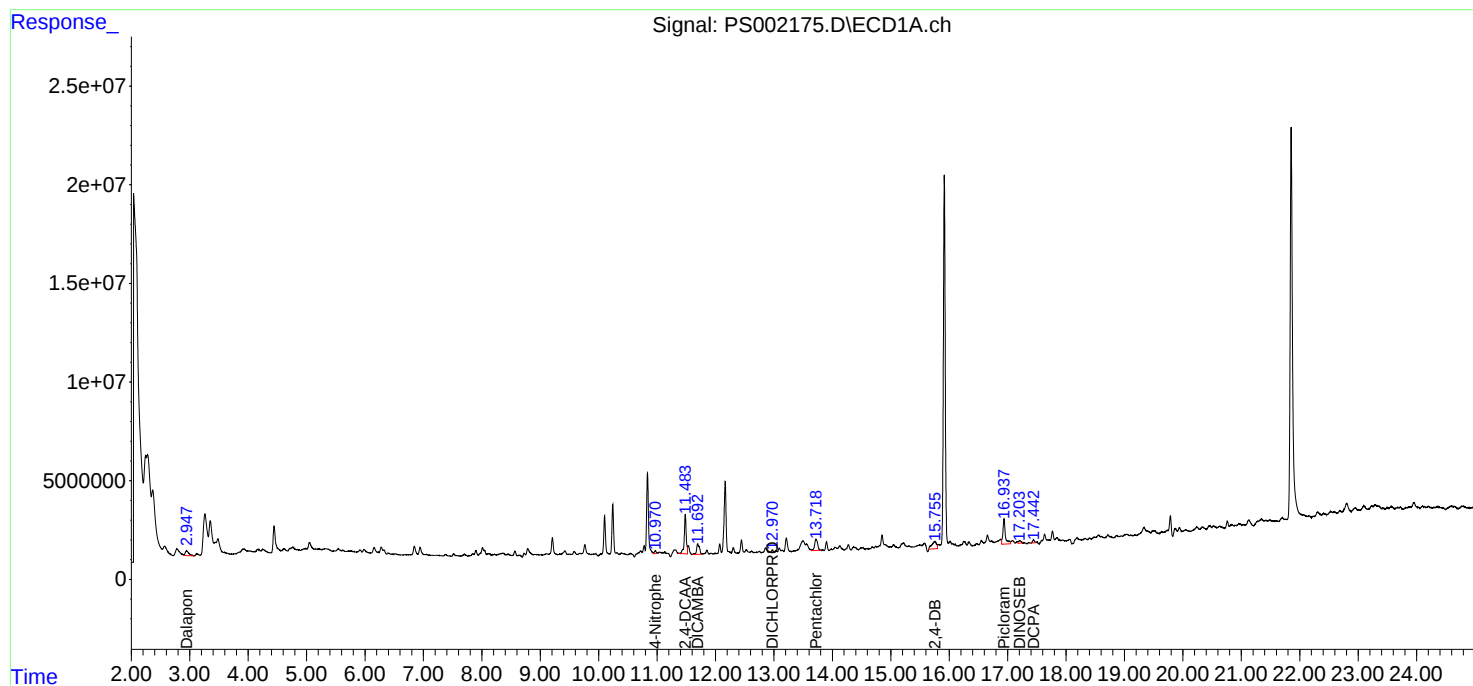


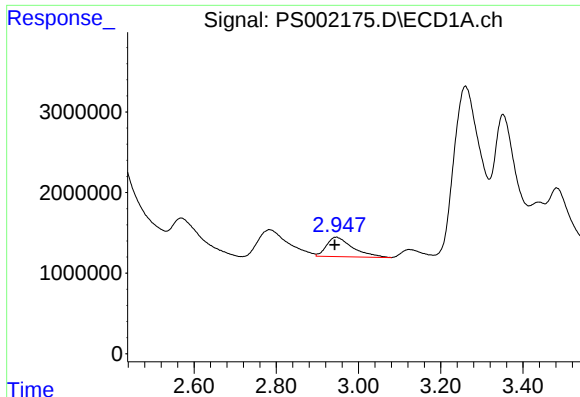

#1 Dalapon


R.T.: 2.947 min
Delta R.T.: 0.005 min
Response: 10590392
Conc: 23.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

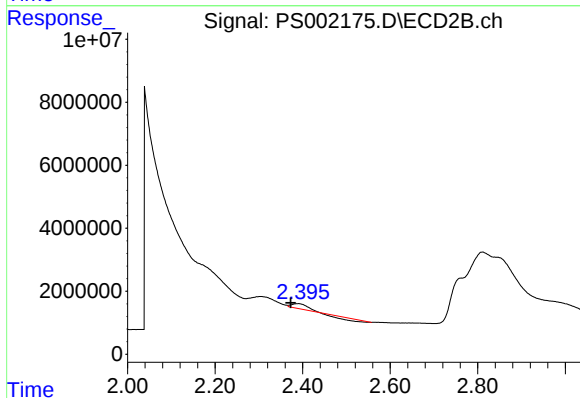


#1 Dalapon

R.T.: 2.391 min
Delta R.T.: 0.018 min
Response: 520567
Conc: 1.15 ng/ml

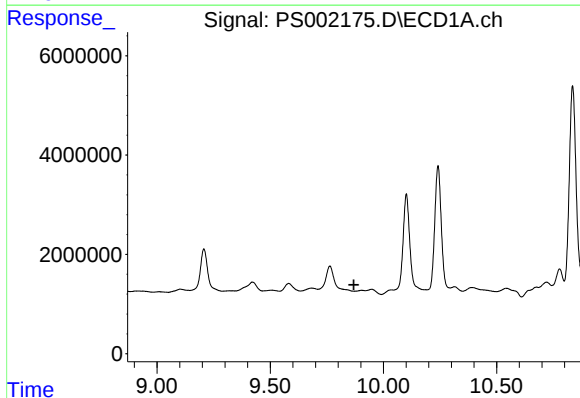


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

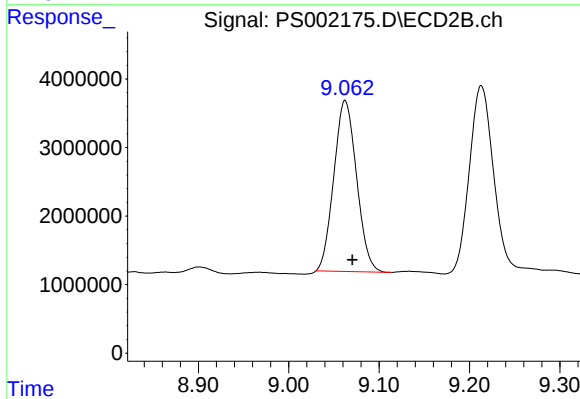

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.062 min
Delta R.T.: -0.008 min
Response: 43549541
Conc: 98.18 ng/ml

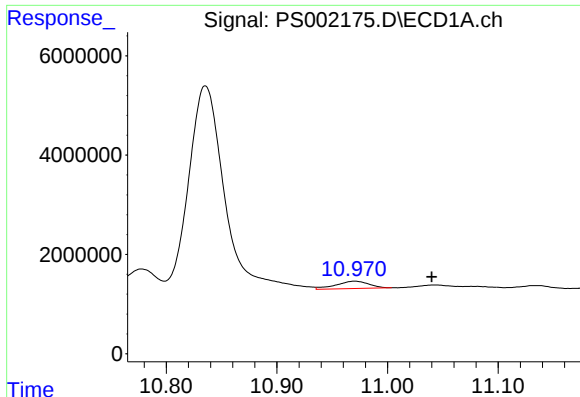

#3 4-Nitrophenol


R.T.: 10.970 min
Delta R.T.: -0.070 min
Response: 3101442
Conc: 18.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

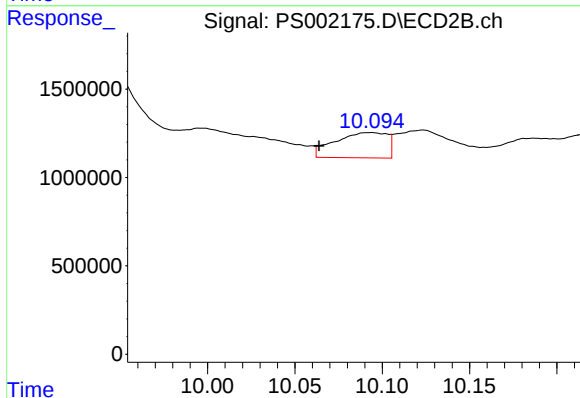


#3 4-Nitrophenol

R.T.: 10.094 min
Delta R.T.: 0.030 min
Response: 2990768
Conc: 16.77 ng/ml

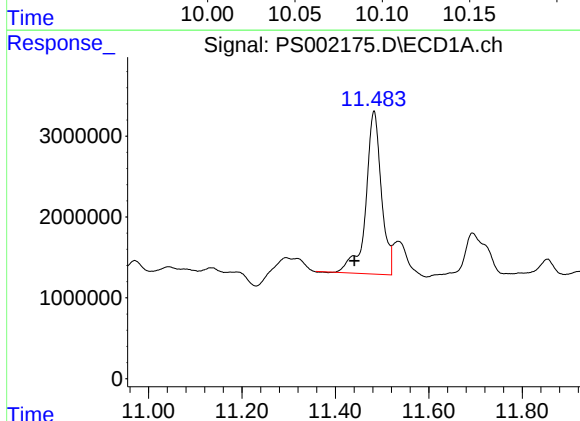


#4 2,4-DCAA

R.T.: 11.483 min
Delta R.T.: 0.042 min
Response: 46562703
Conc: 147.97 ng/ml

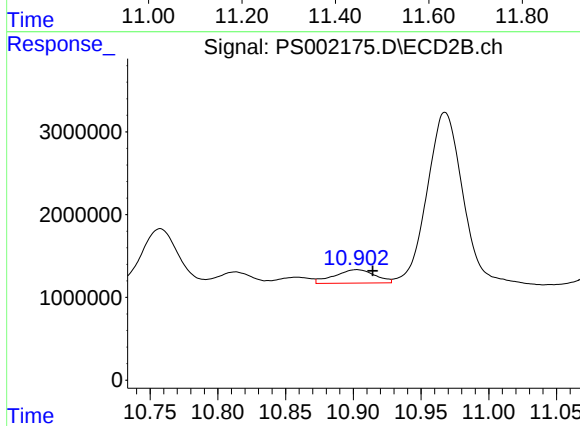

#4 2,4-DCAA


R.T.: 10.903 min
Delta R.T.: -0.012 min
Response: 3407215
Conc: 9.49 ng/ml

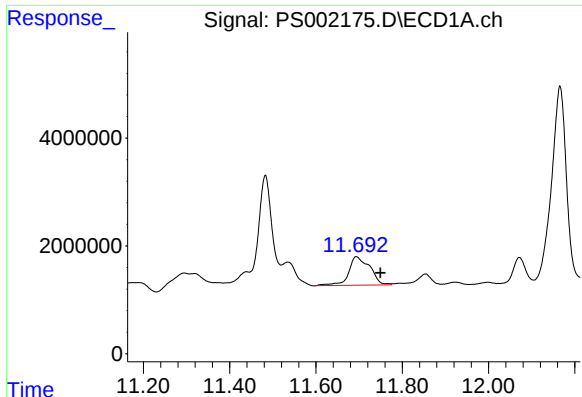

#5 DICAMBA


R.T.: 11.694 min
Delta R.T.: -0.056 min
Response: 18126046
Conc: 13.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

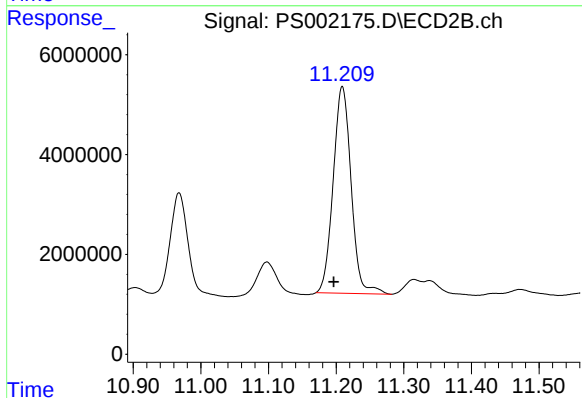


#5 DICAMBA

R.T.: 11.209 min
Delta R.T.: 0.013 min
Response: 76438125
Conc: 61.17 ng/ml

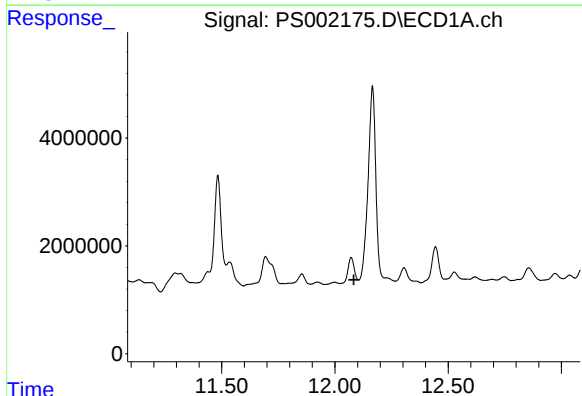


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

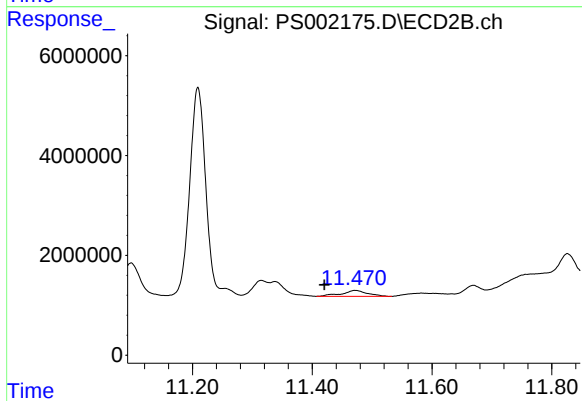

#6 MCP


R.T.: 11.471 min
Delta R.T.: 0.051 min
Response: 3616025
Conc: 4.20 ug/ml

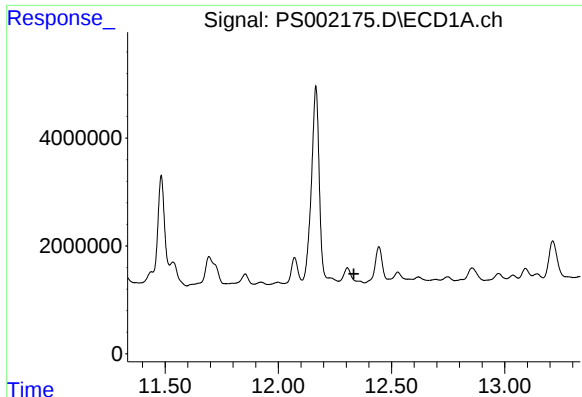

#7 MCPA


R.T.: 12.305 min
Delta R.T.: -0.029 min
Response: -713180
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

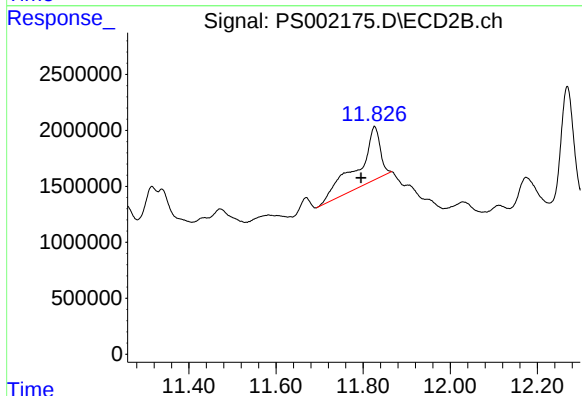


#7 MCPA

R.T.: 11.826 min
Delta R.T.: 0.031 min
Response: 17357003
Conc: 12.82 ug/ml

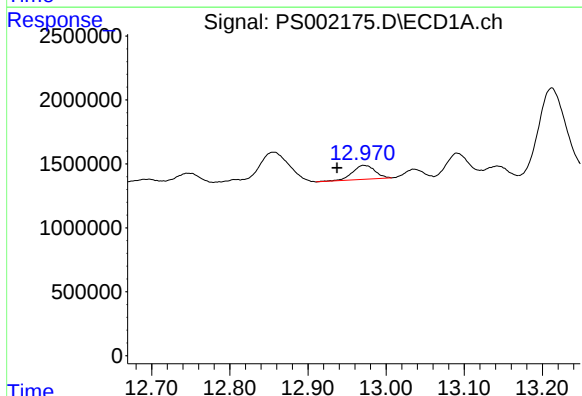


#8 DICHLORPROP

R.T.: 12.972 min
Delta R.T.: 0.035 min
Response: 2186740
Conc: 6.28 ng/ml

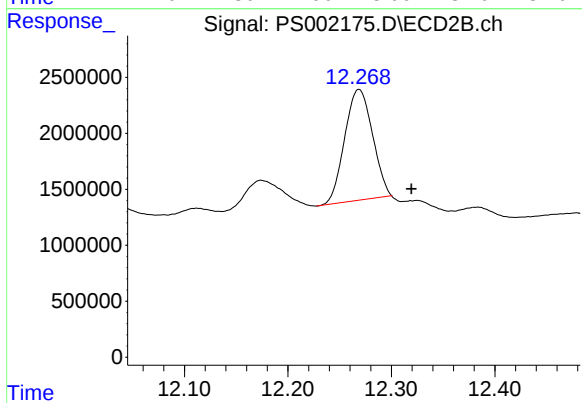

#8 DICHLORPROP


R.T.: 12.269 min
Delta R.T.: -0.051 min
Response: 18370101
Conc: 57.20 ng/ml

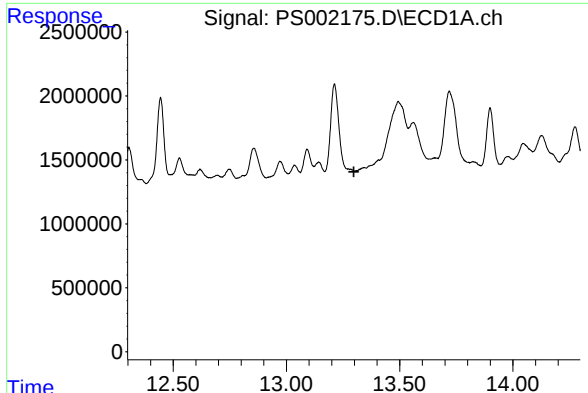

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

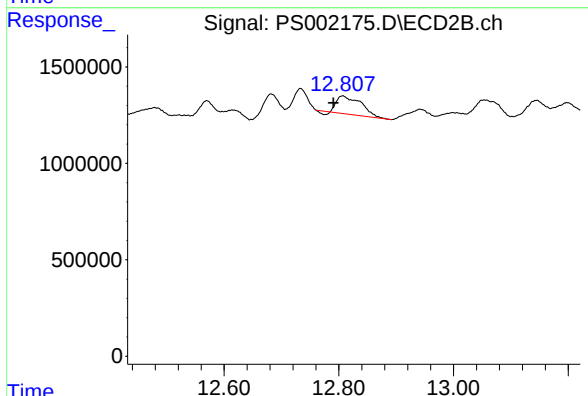


#9 2,4-D

R.T.: 12.807 min
Delta R.T.: 0.016 min
Response: 2659009
Conc: 6.24 ng/ml

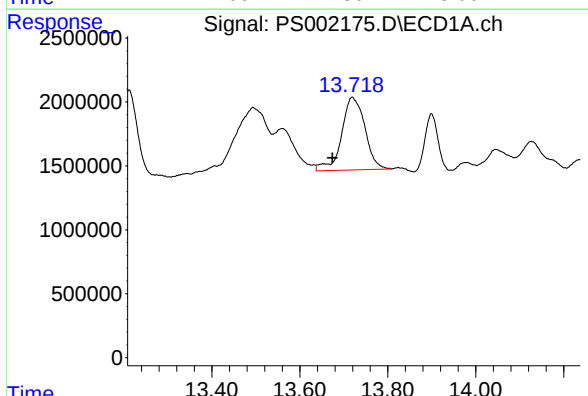


#10 Pentachlorophenol

R.T.: 13.719 min
Delta R.T.: 0.045 min
Response: 20948161
Conc: 4.35 ng/ml

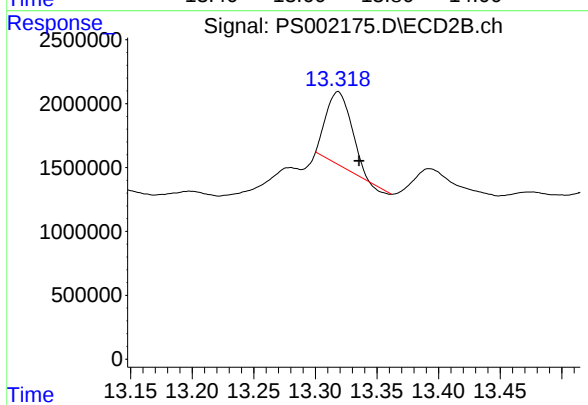

#10 Pentachlorophenol


R.T.: 13.318 min
Delta R.T.: -0.017 min
Response: 8020048
Conc: 1.71 ng/ml

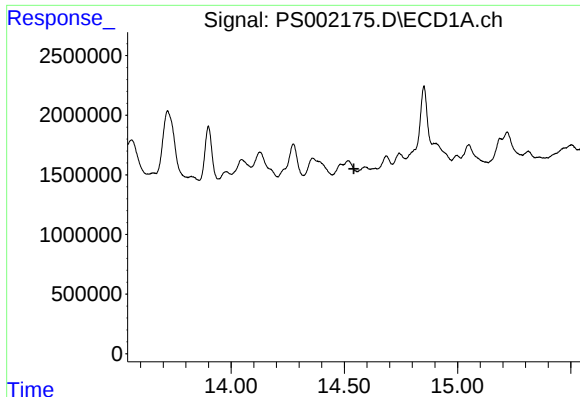

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

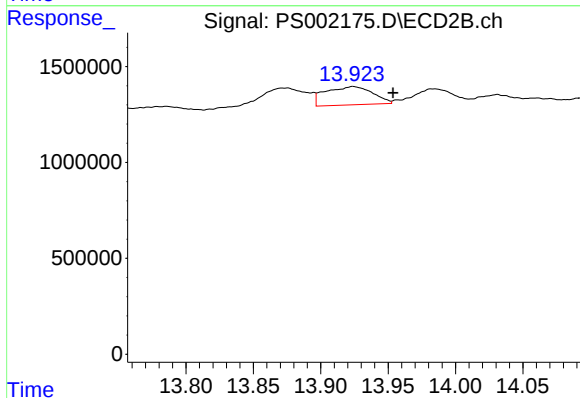


#11 2,4,5-TP (SILVEX)

R.T.: 13.924 min
Delta R.T.: -0.030 min
Response: 2314674
Conc: 1.27 ng/ml

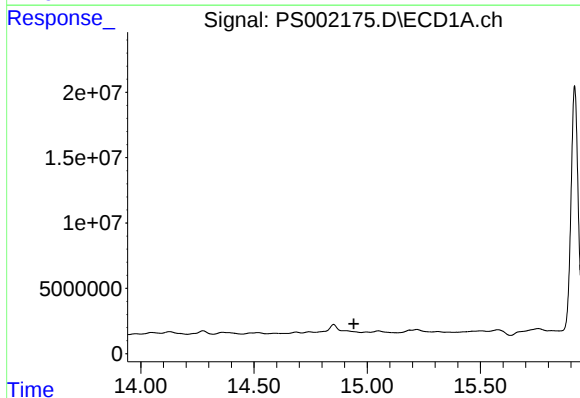


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

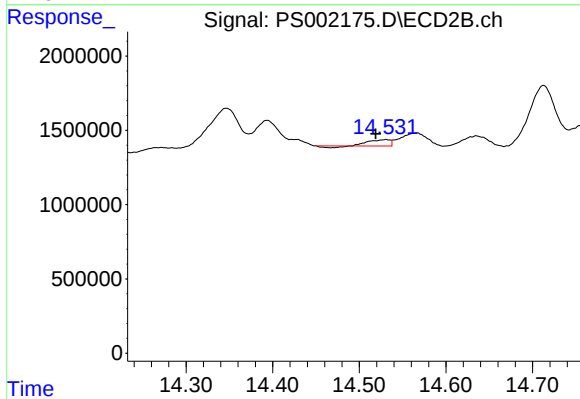

#12 2,4,5-T


R.T.: 14.531 min
Delta R.T.: 0.012 min
Response: 611350
Conc: 0.41 ng/ml

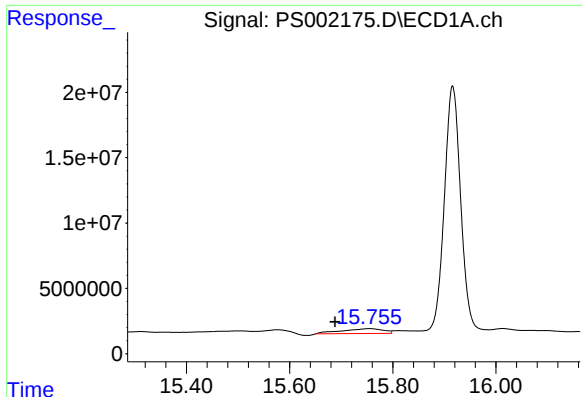

#13 2,4-DB


R.T.: 15.755 min
Delta R.T.: 0.067 min
Response: 20639329
Conc: 87.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

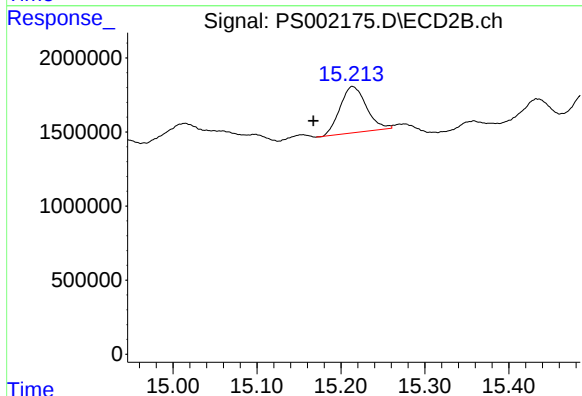


#13 2,4-DB

R.T.: 15.214 min
Delta R.T.: 0.047 min
Response: 6852695
Conc: 30.93 ng/ml

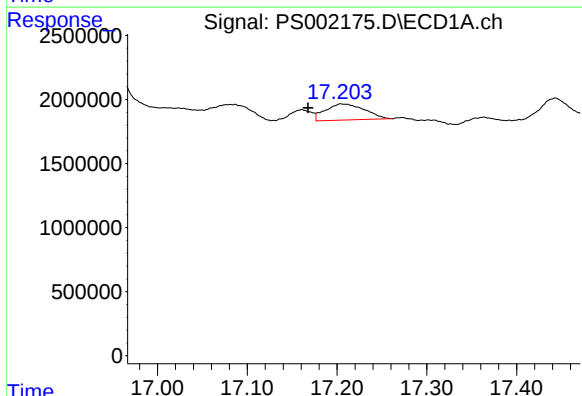


#14 DINOSEB

R.T.: 17.206 min
Delta R.T.: 0.038 min
Response: 3808176
Conc: 2.78 ng/ml

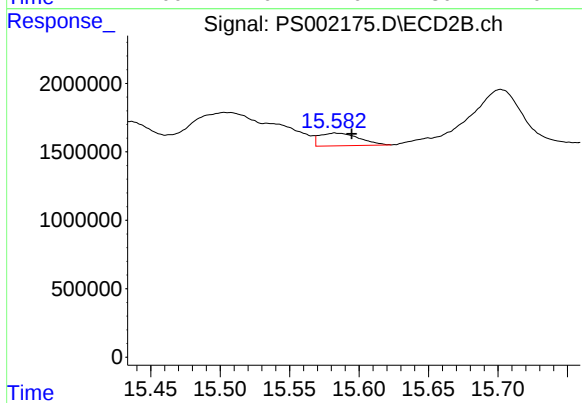

#14 DINOSEB


R.T.: 15.583 min
Delta R.T.: -0.012 min
Response: 1836274
Conc: 1.45 ng/ml

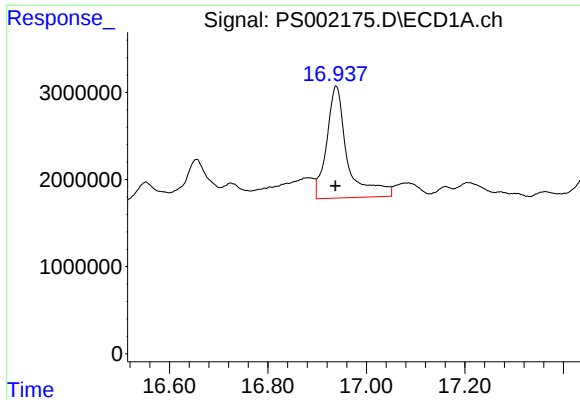

#15 Picloram


R.T.: 16.939 min
Delta R.T.: 0.001 min
Response: 37653061
Conc: 15.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

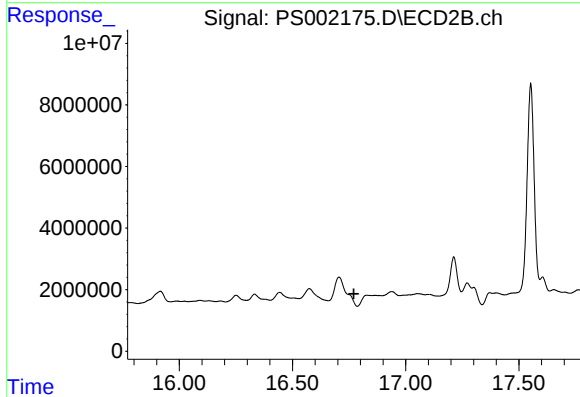


#15 Picloram

R.T.: 16.830 min
Delta R.T.: 0.059 min
Response: -3430728
Conc: N.D.

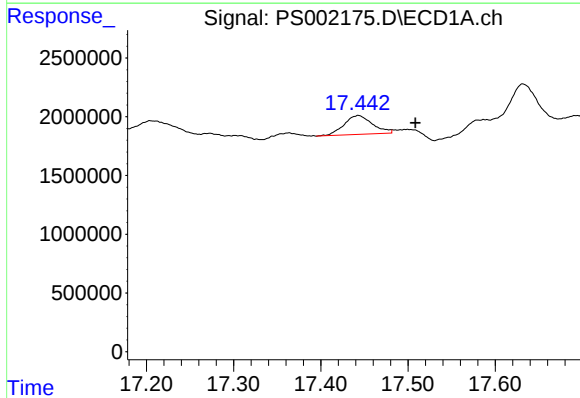

#16 DCPA

R.T.: 17.443 min
Delta R.T.: -0.066 min
Response: 3704258
Conc: 1.58 ng/ml

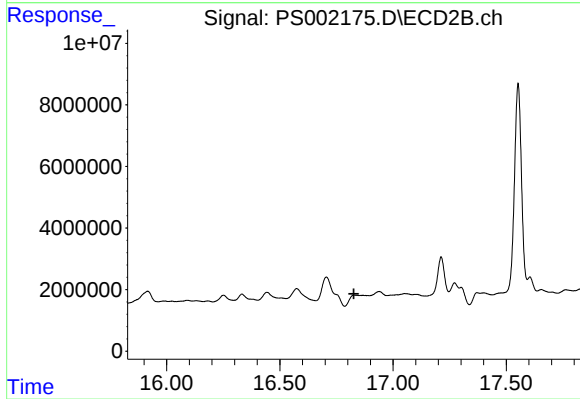

#16 DCPA

R.T.: 16.830 min
Delta R.T.: 0.004 min
Response: -3430728
Conc: N.D.