

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
 Data File : PS002178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 18:13
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 02:23:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.445	10.931	169.0E6	163.9E6	536.921	456.521
Target Compounds							
7) T	MCPA	0.000	11.797	0	283888	N.D.	0.210 #
13) T	2,4-DB	15.631	15.225	-94138	205409	N.D.	0.927
15) T	Picloram	16.900	16.715	8779590	85819	3.681	0.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102718\
Data File : PS002178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 18:13
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 02:23:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

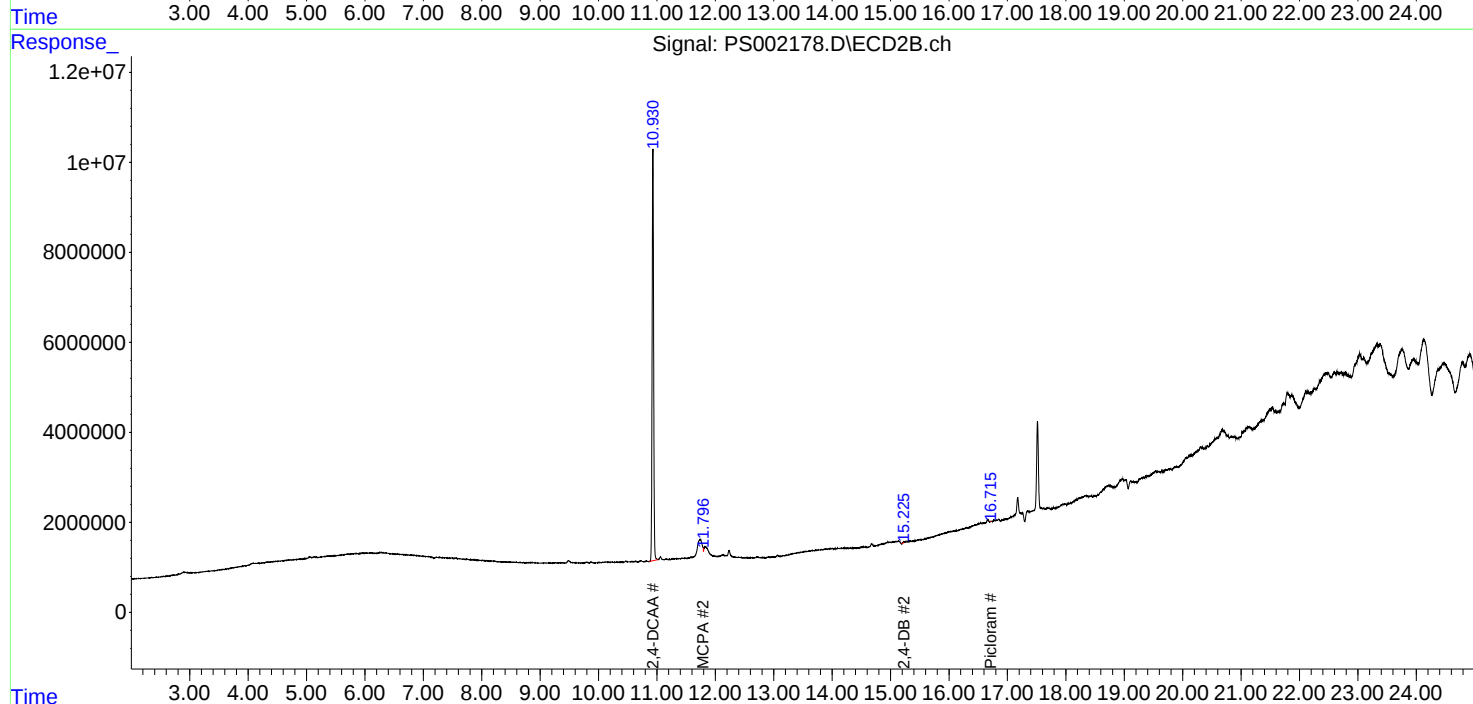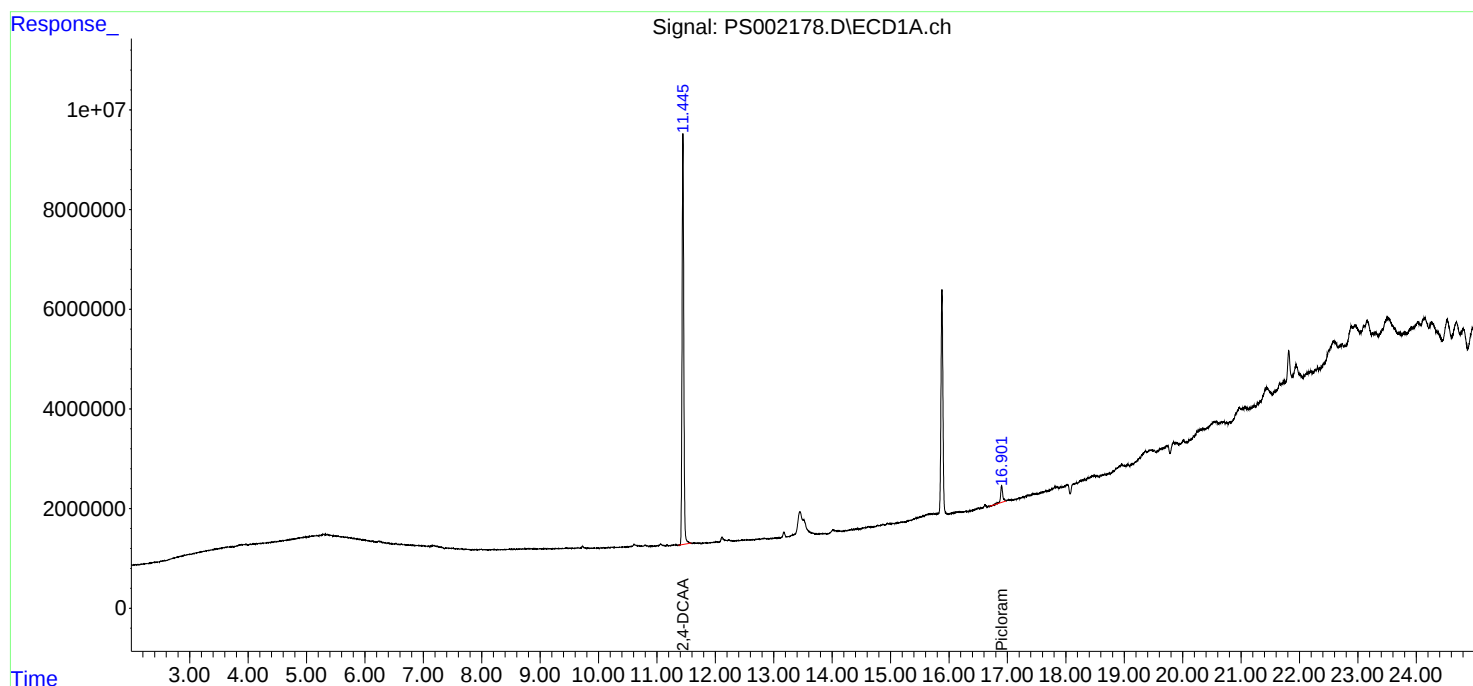


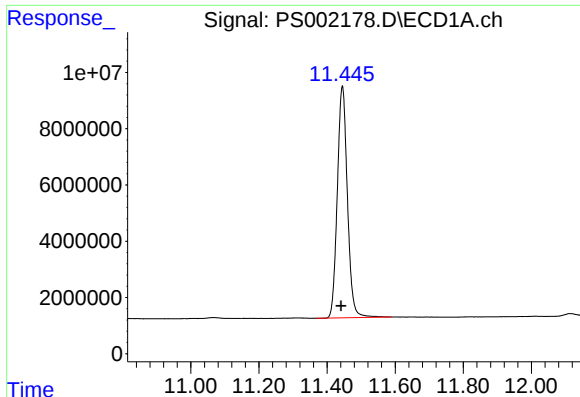

#4 2,4-DCAA


R.T.: 11.445 min
Delta R.T.: 0.004 min
Response: 168961263
Conc: 536.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

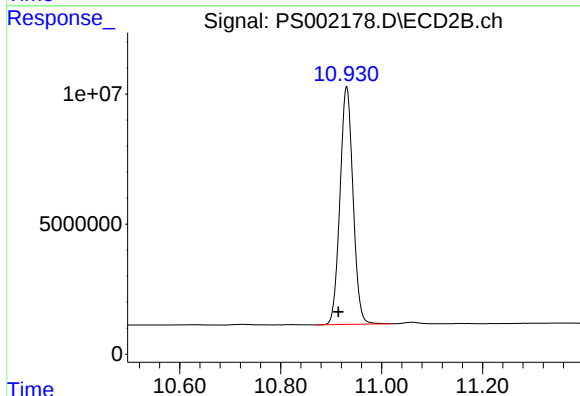


#4 2,4-DCAA

R.T.: 10.931 min
Delta R.T.: 0.016 min
Response: 163935594
Conc: 456.52 ng/ml

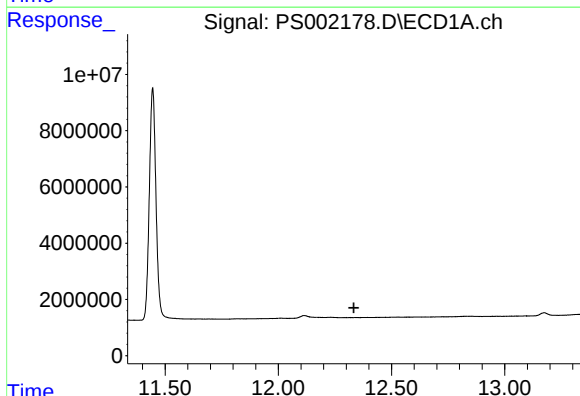


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

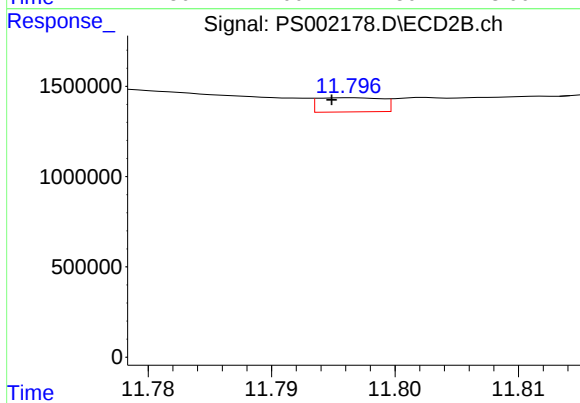

#7 MCPA


R.T.: 11.797 min
Delta R.T.: 0.002 min
Response: 283888
Conc: 0.21 ug/ml

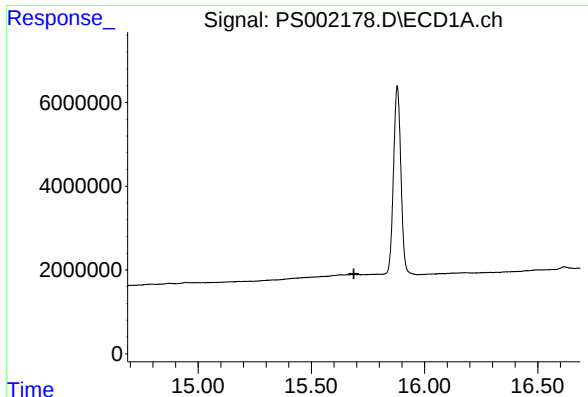

#13 2,4-DB


R.T.: 15.631 min
Delta R.T.: -0.057 min
Response: -94138
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

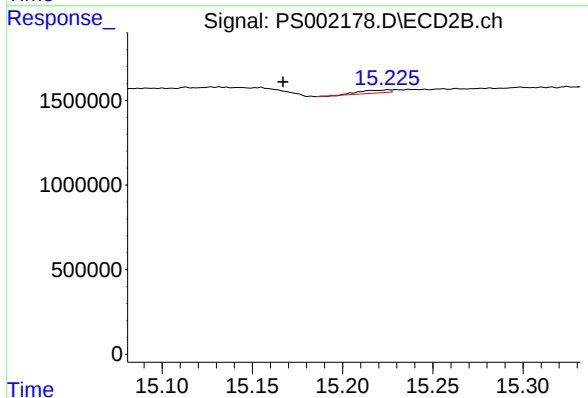


#13 2,4-DB

R.T.: 15.225 min
Delta R.T.: 0.058 min
Response: 205409
Conc: 0.93 ng/ml

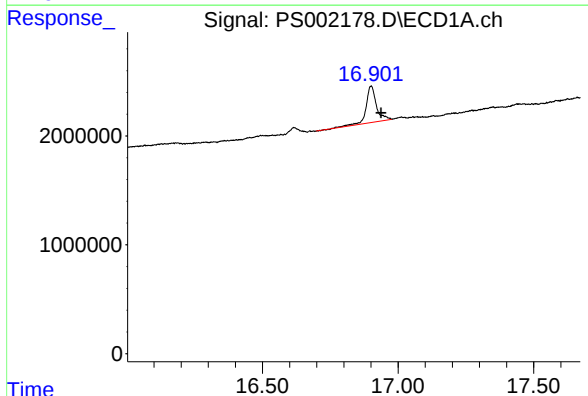

#15 Picloram

R.T.: 16.900 min
Delta R.T.: -0.037 min
Response: 8779590
Conc: 3.68 ng/ml

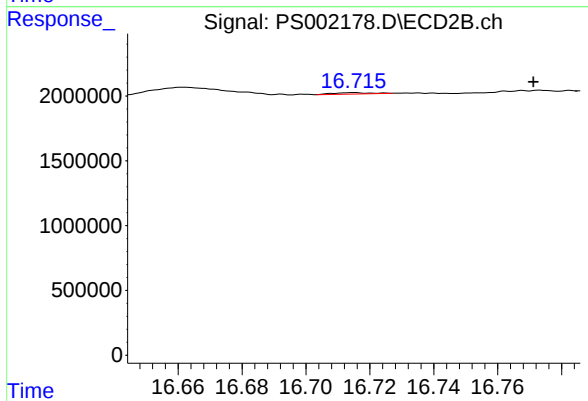

#15 Picloram

R.T.: 16.715 min
Delta R.T.: -0.056 min
Response: 85819
Conc: 0.04 ng/ml