

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102721\
 Data File : PS017235.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2021 09:32
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 01:26:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	0.000	19199337	0	12.561	N.D. #
Target Compounds							
3) T	4-Nitroph...	6.941	6.362	10115570	4566395	11.598	14.166
7) T	MCPA	7.604f	0.000	6633226	0	1.075	N.D. #
8) T	DICHLORPROP	7.979f	0.000	9065389	0	6.046	N.D. #
9) T	2,4-D	8.209f	0.000	7494169	0	4.231	N.D. #
13) T	2,4-DB	9.884f	0.000	6384891	0	4.244	N.D. #
15) T	Picloram	10.940	10.781	32476330	9627611	3.040	2.514
16) T	DCPA	0.000	10.781f	0	9627611	N.D.	2.256



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102721\
Data File : PS017235.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2021 09:32
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 01:26:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

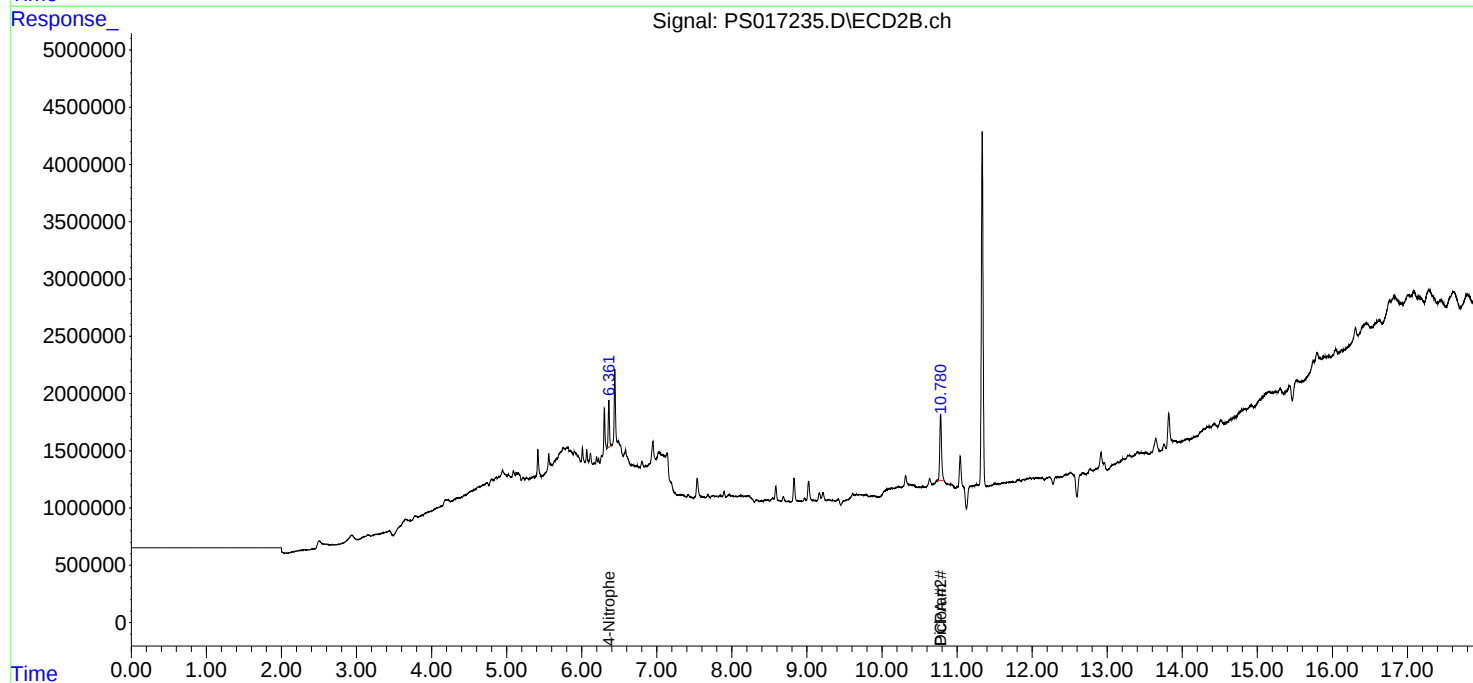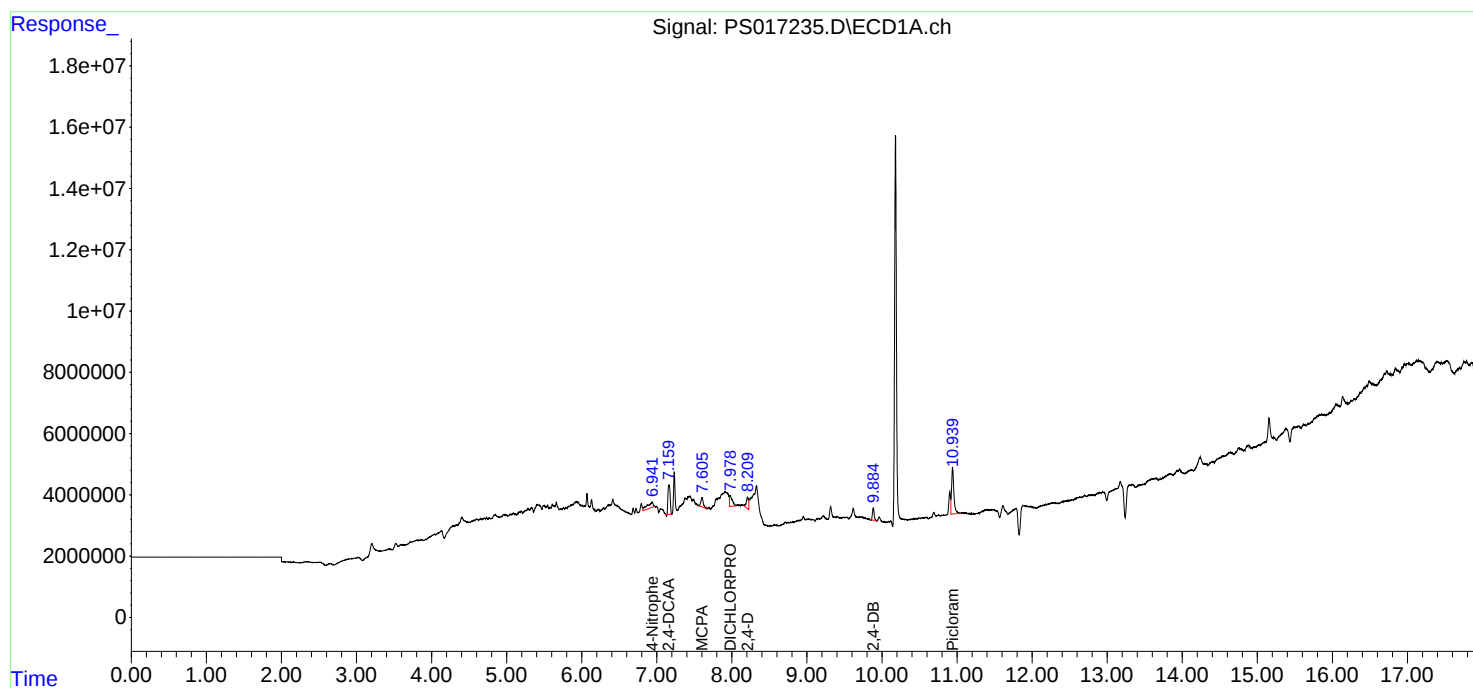


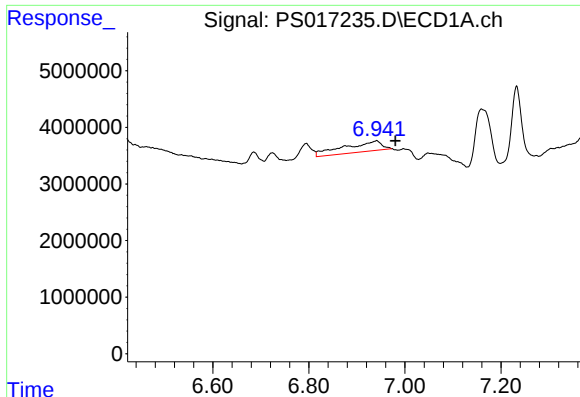

#3 4-Nitrophenol


R.T.: 6.941 min
Delta R.T.: -0.039 min
Response: 10115570
Conc: 11.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

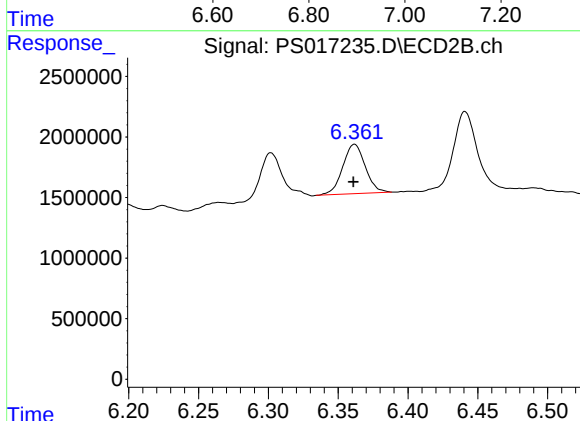


#3 4-Nitrophenol

R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 4566395
Conc: 14.17 ng/ml

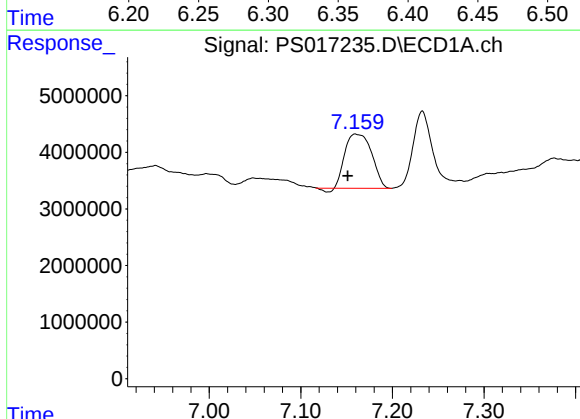


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: 0.008 min
Response: 19199337
Conc: 12.56 ng/ml

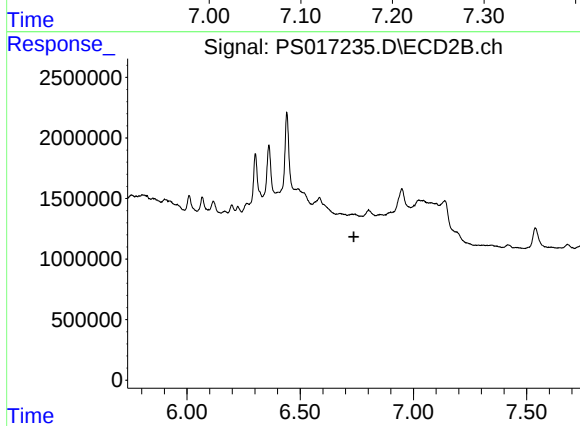

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.737 min
Response: 0
Conc: N.D.

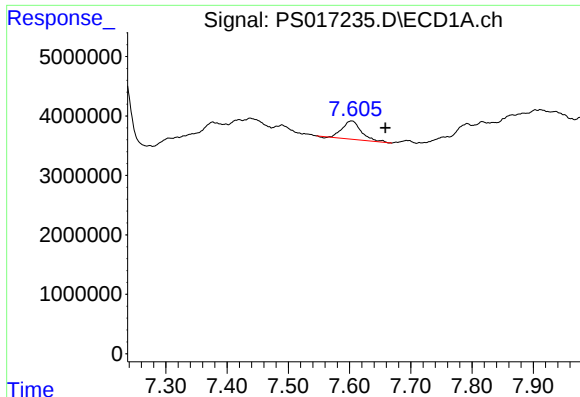

#7 MCPA


R.T.: 7.604 min
Delta R.T.: -0.055 min
Response: 6633226
Conc: 1.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

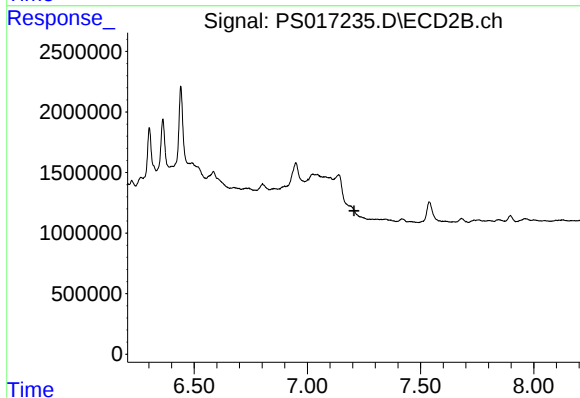


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

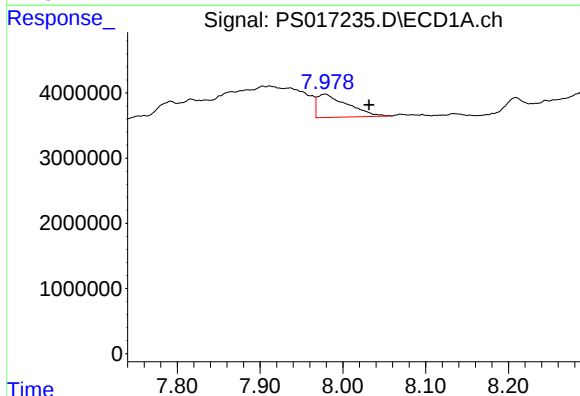


#8 DICHLORPROP

R.T.: 7.979 min
Delta R.T.: -0.053 min
Response: 9065389
Conc: 6.05 ng/ml

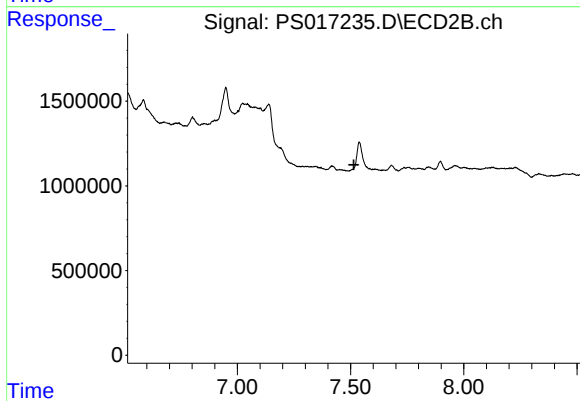

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.514 min
Response: 0
Conc: N.D.

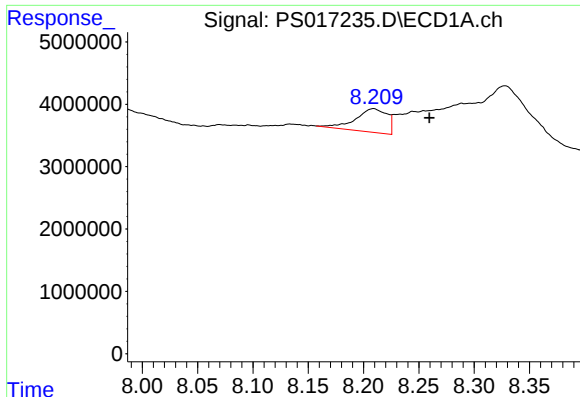

#9 2,4-D


R.T.: 8.209 min
Delta R.T.: -0.051 min
Response: 7494169
Conc: 4.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

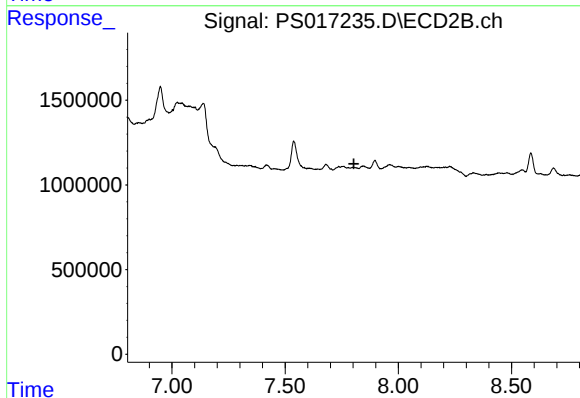


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.804 min
Response: 0
Conc: N.D.

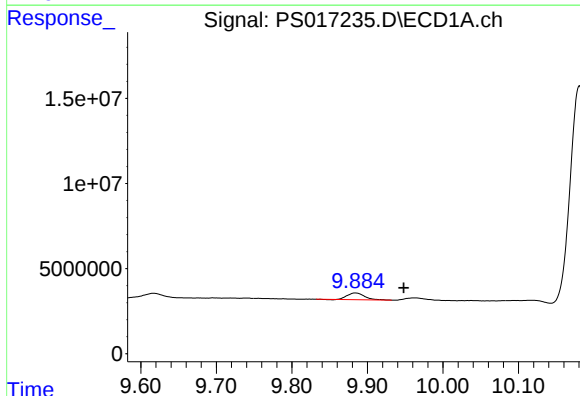


#13 2,4-DB

R.T.: 9.884 min
Delta R.T.: -0.064 min
Response: 6384891
Conc: 4.24 ng/ml

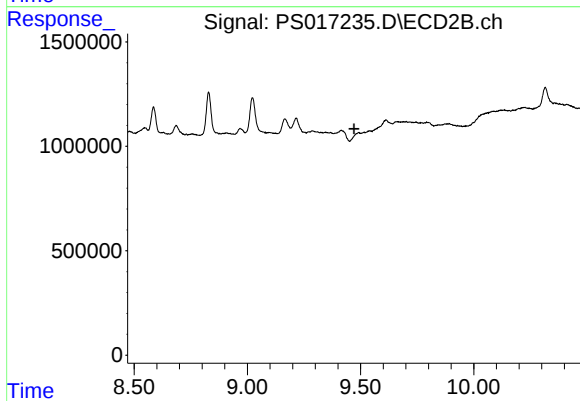

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

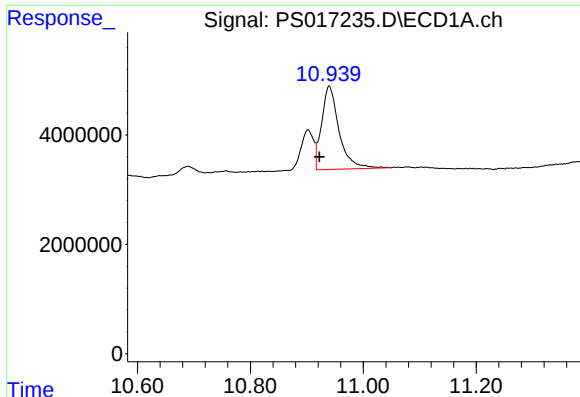

#15 Picloram


R.T.: 10.940 min
Delta R.T.: 0.017 min
Response: 32476330
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

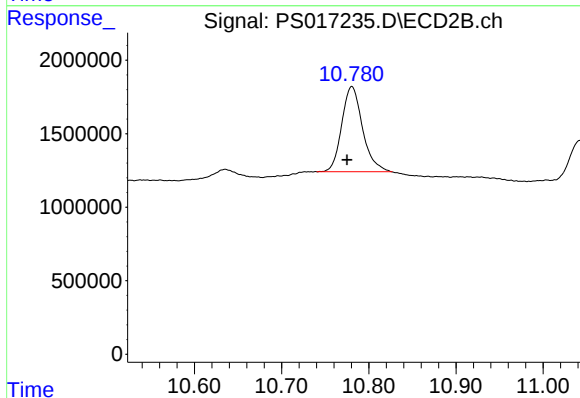


#15 Picloram

R.T.: 10.781 min
Delta R.T.: 0.006 min
Response: 9627611
Conc: 2.51 ng/ml

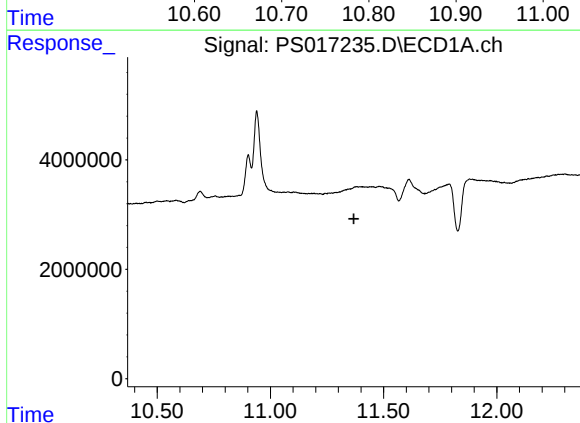

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.369 min
Response: 0
Conc: N.D.

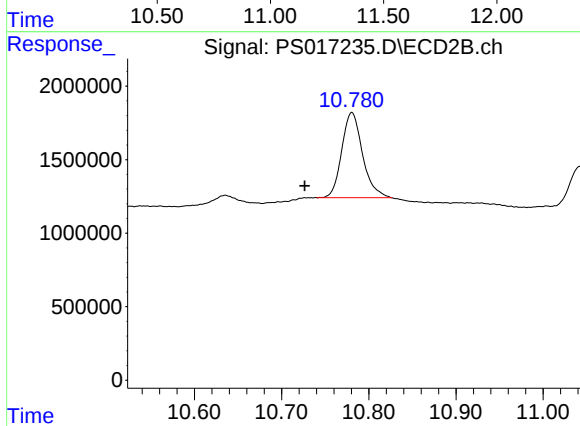

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.054 min
Response: 9627611
Conc: 2.26 ng/ml