

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 17:55
 Operator : AR\AJ
 Sample : Q3449-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CF-620-COMP-41

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:22:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:40:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.272	7.735	2907.3E6	881.3E6	672.424	805.949
Target Compounds							
1) T	Dalapon	2.627f	2.682	1702.8E6	2372.4E6	236.137	645.019 #
2) T	3,5-DICHL...	6.437	6.711	-645266	8317111	N.D.	4.419
6) T	MCPD	0.000	7.986f	0	80366156	N.D.	31.423
7) T	MCPA	0.000	8.235f	0	33696017	N.D.	9.623
8) T	DICHLORPROP	8.176	8.650	21530037	9909994	4.950	5.393
9) T	2,4-D	0.000	9.007	0	10993583	N.D.	5.694
10) T	Pentachlo...	8.692	9.499	4419132	48349727	<MDL	<MDL #
11) T	2,4,5-TP ...	9.320f	9.874	49066679	129.0E6	1.988	6.824 #
12) T	2,4,5-T	9.583	10.282f	55333404	328.2E6	2.656	20.349 #
13) T	2,4-DB	10.151	0.000	183.0E6	0	79.523	N.D. #
15) T	Picloram	11.205f	12.422f	31983713	35079984	1.698	1.207 #
16) T	DCPA	11.616	0.000	24689173	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 17:55
Operator : AR\AJ
Sample : Q3449-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:22:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

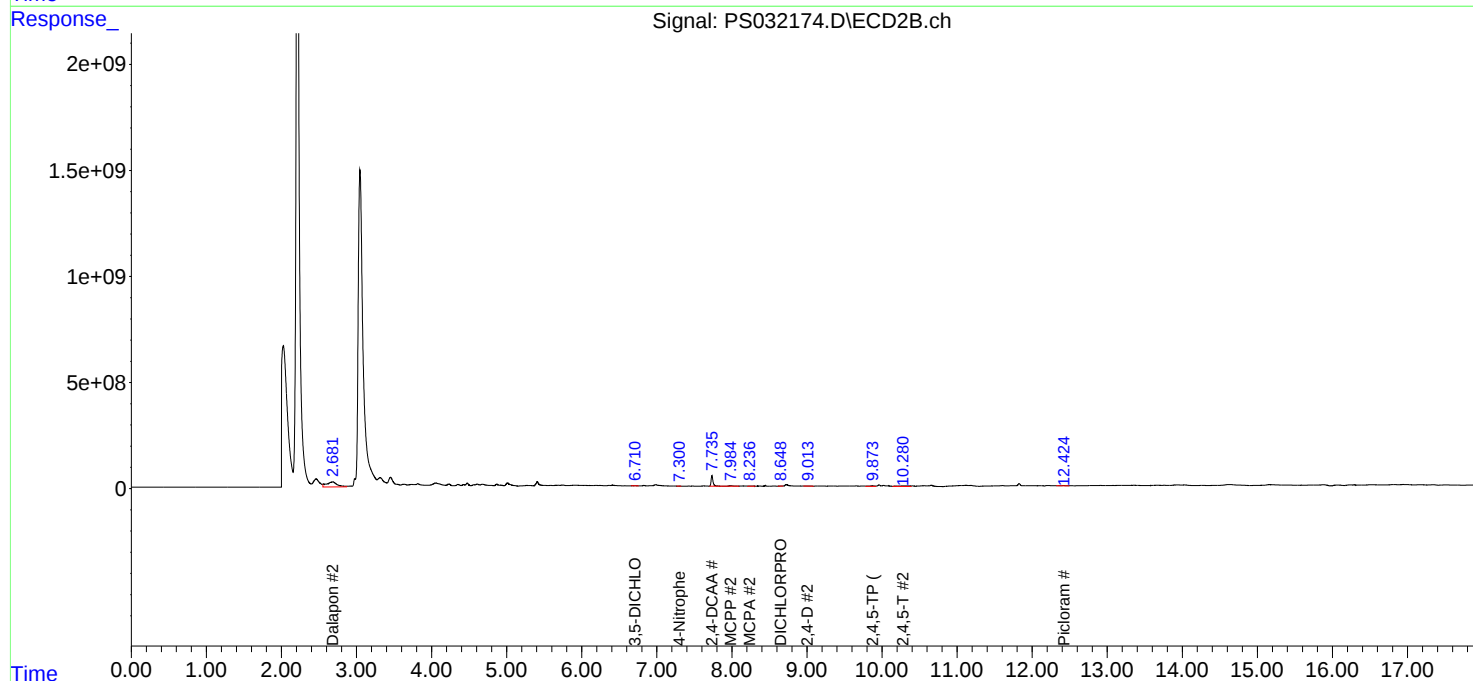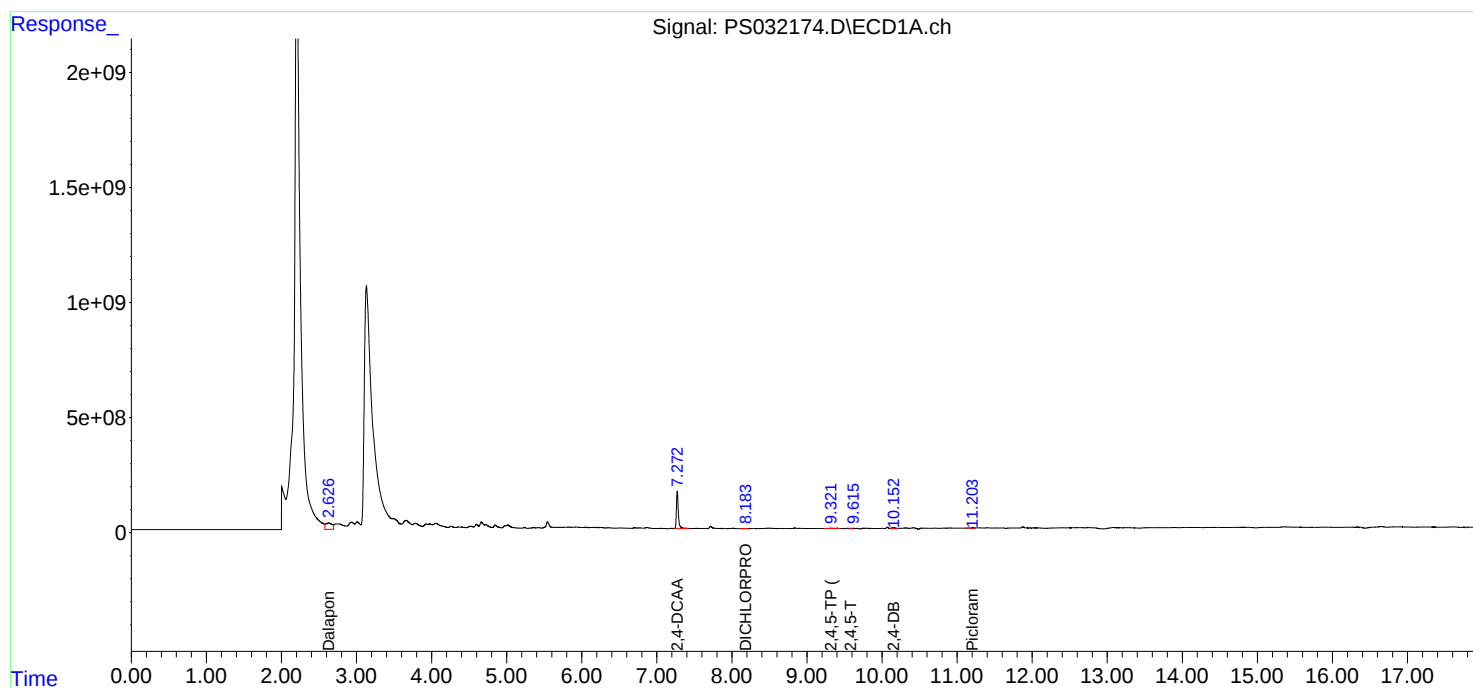


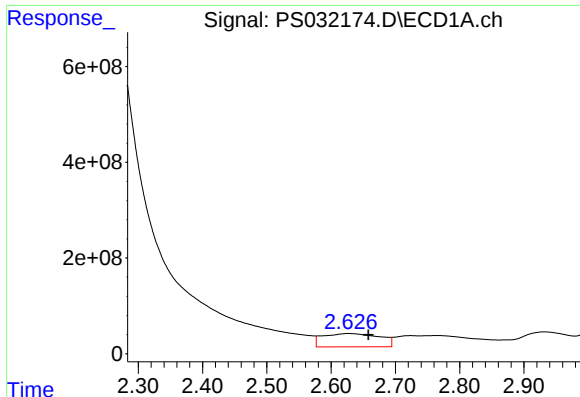

#1 Dalapon


R.T.: 2.627 min
Delta R.T.: -0.031 min
Response: 1702814890
Conc: 236.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

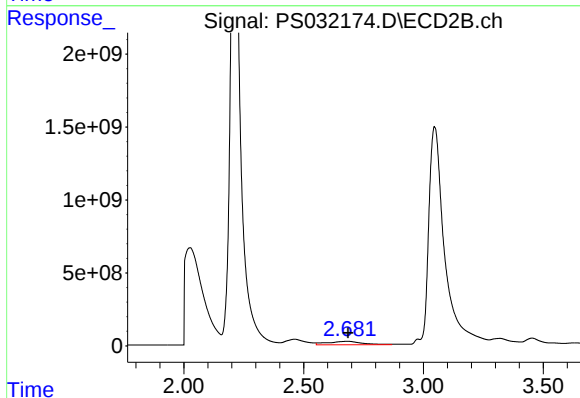


#1 Dalapon

R.T.: 2.682 min
Delta R.T.: -0.003 min
Response: 2372363814
Conc: 645.02 ng/ml

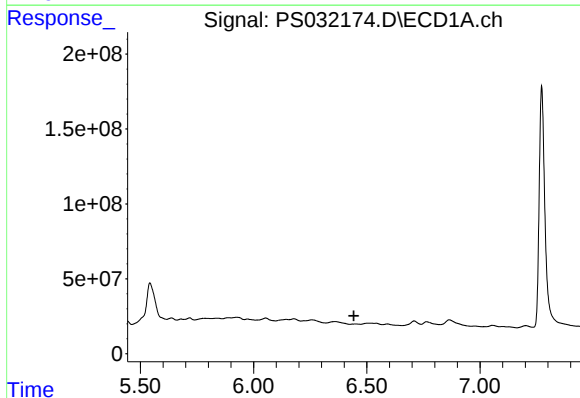


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.437 min
Delta R.T.: -0.006 min
Response: -645266
Conc: N.D.

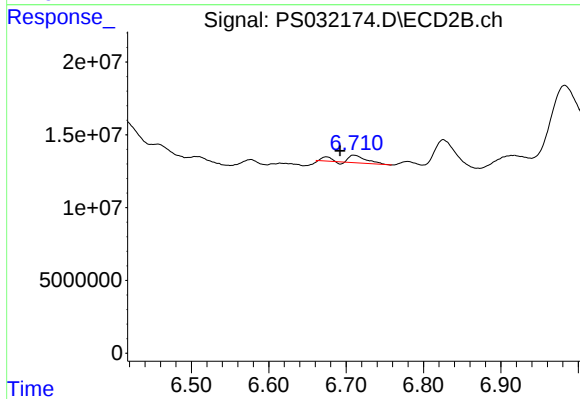

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.711 min
Delta R.T.: 0.019 min
Response: 8317111
Conc: 4.42 ng/ml

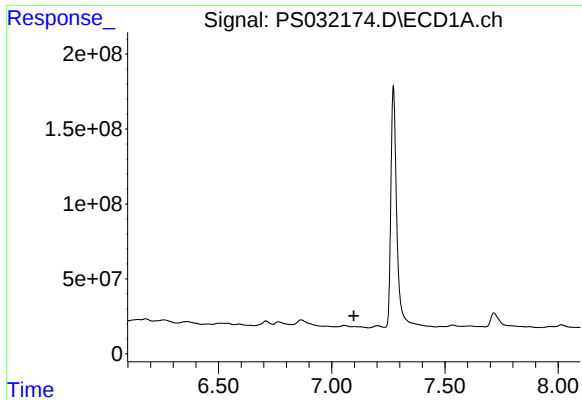

#3 4-Nitrophenol


R.T.: 7.095 min
Delta R.T.: -0.003 min
Response: -2416608
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

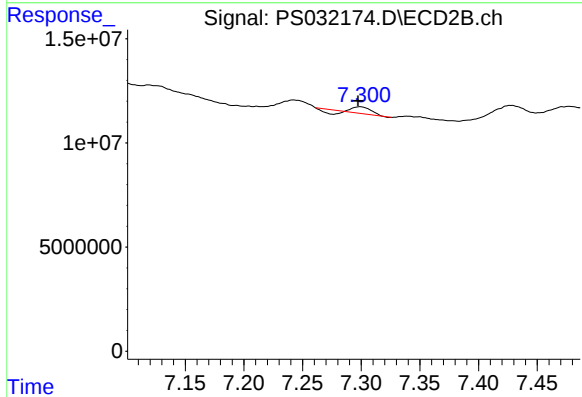


#3 4-Nitrophenol

R.T.: 7.299 min
Delta R.T.: 0.001 min
Response: 1771343
Conc: 1.12 ng/ml

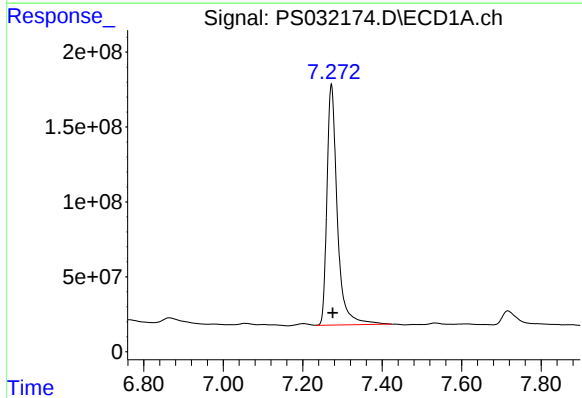


#4 2,4-DCAA

R.T.: 7.272 min
Delta R.T.: -0.003 min
Response: 2907334924
Conc: 672.42 ng/ml

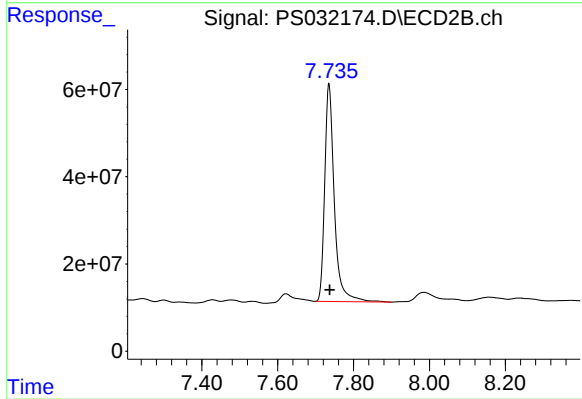

#4 2,4-DCAA


R.T.: 7.735 min
Delta R.T.: -0.002 min
Response: 881333107
Conc: 805.95 ng/ml

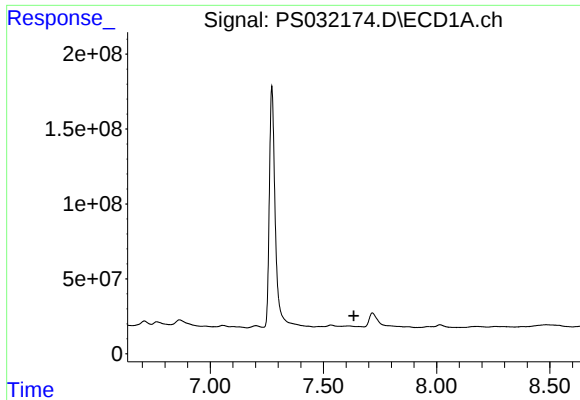

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

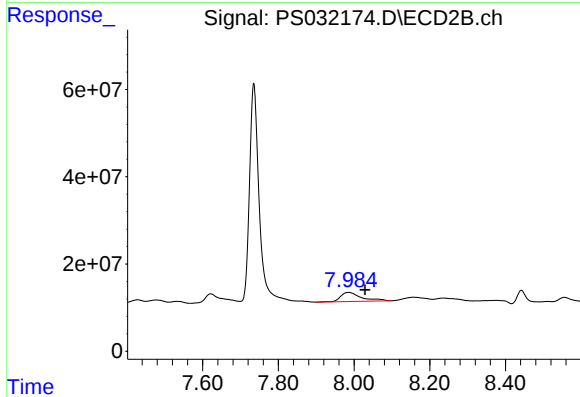


#6 MCPP

R.T.: 7.986 min
Delta R.T.: -0.043 min
Response: 80366156
Conc: 31.42 ug/ml

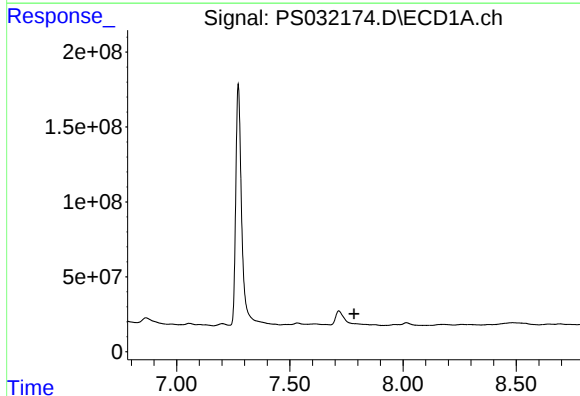


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.783 min
Response: 0
Conc: N.D.

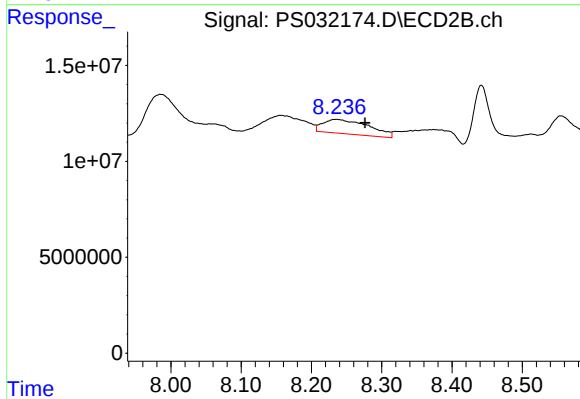

#7 MCPA


R.T.: 8.235 min
Delta R.T.: -0.041 min
Response: 33696017
Conc: 9.62 ug/ml

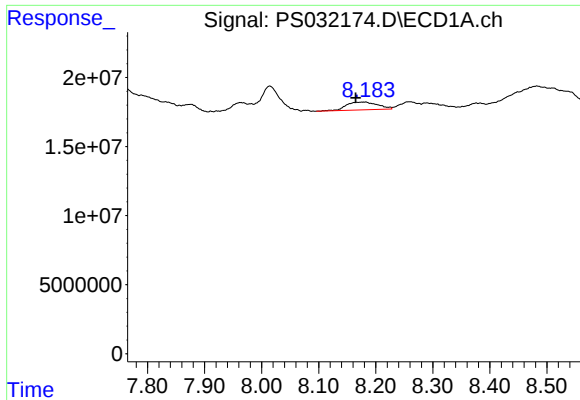

#8 DICHLORPROP


R.T.: 8.176 min
Delta R.T.: 0.011 min
Response: 21530037
Conc: 4.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

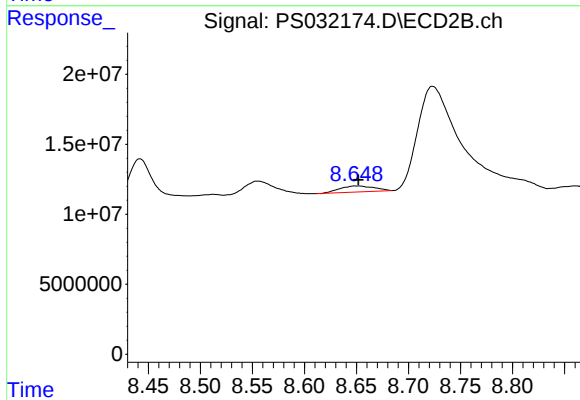


#8 DICHLORPROP

R.T.: 8.650 min
Delta R.T.: -0.001 min
Response: 9909994
Conc: 5.39 ng/ml

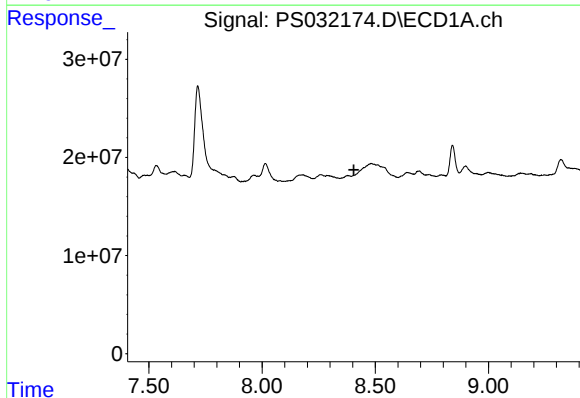


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.406 min
Response: 0
Conc: N.D.

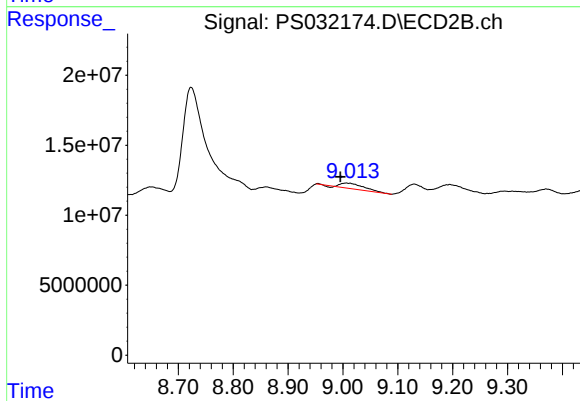

#9 2,4-D


R.T.: 9.007 min
Delta R.T.: 0.011 min
Response: 10993583
Conc: 5.69 ng/ml

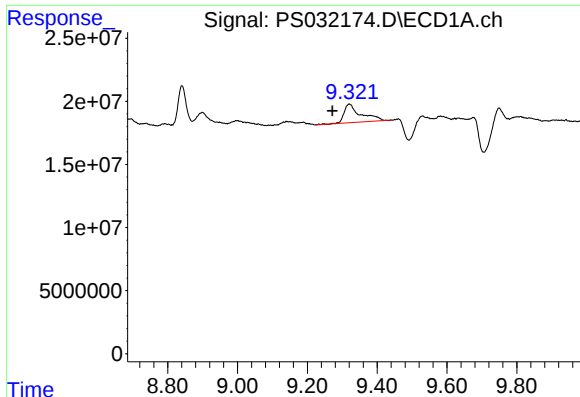

#11 2,4,5-TP (SILVEX)


R.T.: 9.320 min
Delta R.T.: 0.049 min
Response: 49066679
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

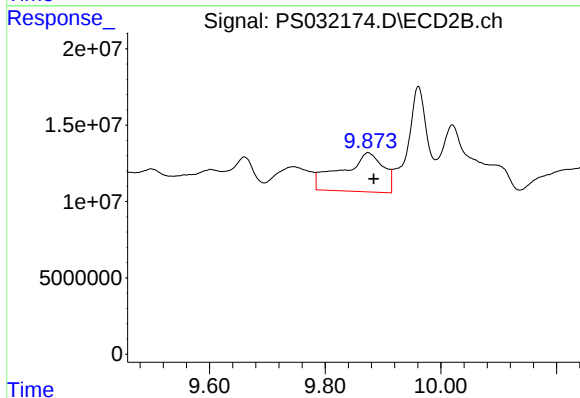


#11 2,4,5-TP (SILVEX)

R.T.: 9.874 min
Delta R.T.: -0.010 min
Response: 128992357
Conc: 6.82 ng/ml

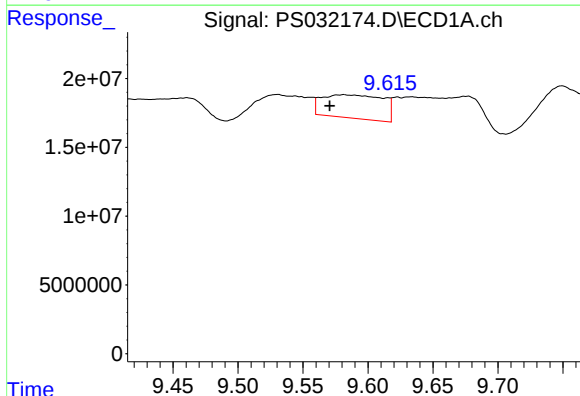


#12 2,4,5-T

R.T.: 9.583 min
Delta R.T.: 0.012 min
Response: 55333404
Conc: 2.66 ng/ml

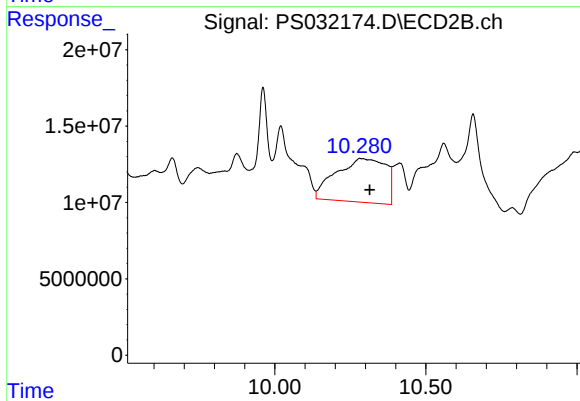

#12 2,4,5-T


R.T.: 10.282 min
Delta R.T.: -0.032 min
Response: 328164043
Conc: 20.35 ng/ml

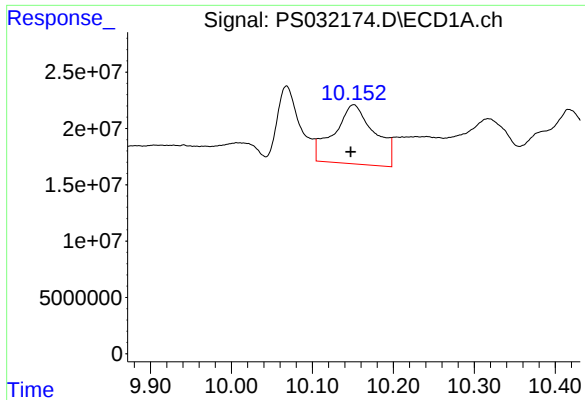

#13 2,4-DB


R.T.: 10.151 min
Delta R.T.: 0.004 min
Response: 183005527
Conc: 79.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

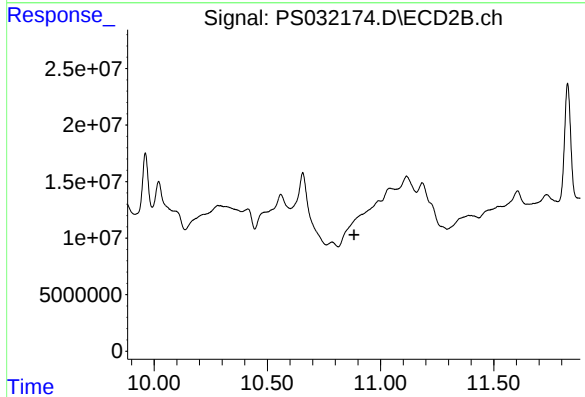


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.882 min
Response: 0
Conc: N.D.

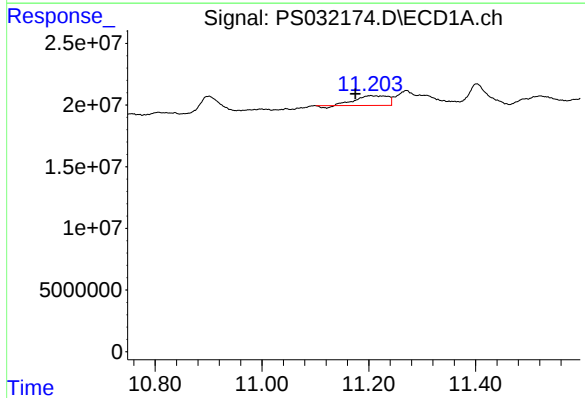

#15 Picloram

R.T.: 11.205 min
Delta R.T.: 0.030 min
Response: 31983713
Conc: 1.70 ng/ml

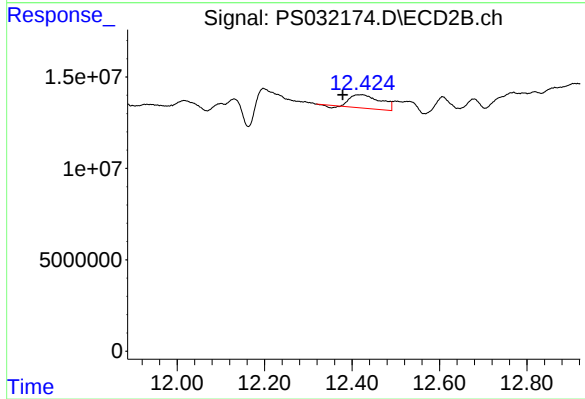

#15 Picloram

R.T.: 12.422 min
Delta R.T.: 0.043 min
Response: 35079984
Conc: 1.21 ng/ml