

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 21:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:23:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:40:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.278	7.748	1775.3E6	574.3E6	410.604	525.134 #
Target Compounds							
2) T	3,5-DICHL...	6.430	0.000	598407	0	<MDL	N.D. #
7) T	MCPA	7.799	8.242f	1551127	22662042	<MDL	6.472 #
8) T	DICHLORPROP	8.182	0.000	3663817	0	<MDL	N.D. #
10) T	Pentachlo...	8.710	9.495	3591367	2020259	<MDL	<MDL #
11) T	2,4,5-TP ...	9.277	9.911f	6959447	7351444	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.298	0	2925581	N.D.	<MDL
13) T	2,4-DB	10.099f	0.000	1647587	0	<MDL	N.D. #
14) T	DINOSEB	11.344	0.000	7946956	0	<MDL	N.D. #
15) T	Picloram	11.153	0.000	1763256	0	<MDL	N.D. #
16) T	DCPA	11.639	12.308	6090918	6023400	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 21:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:23:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

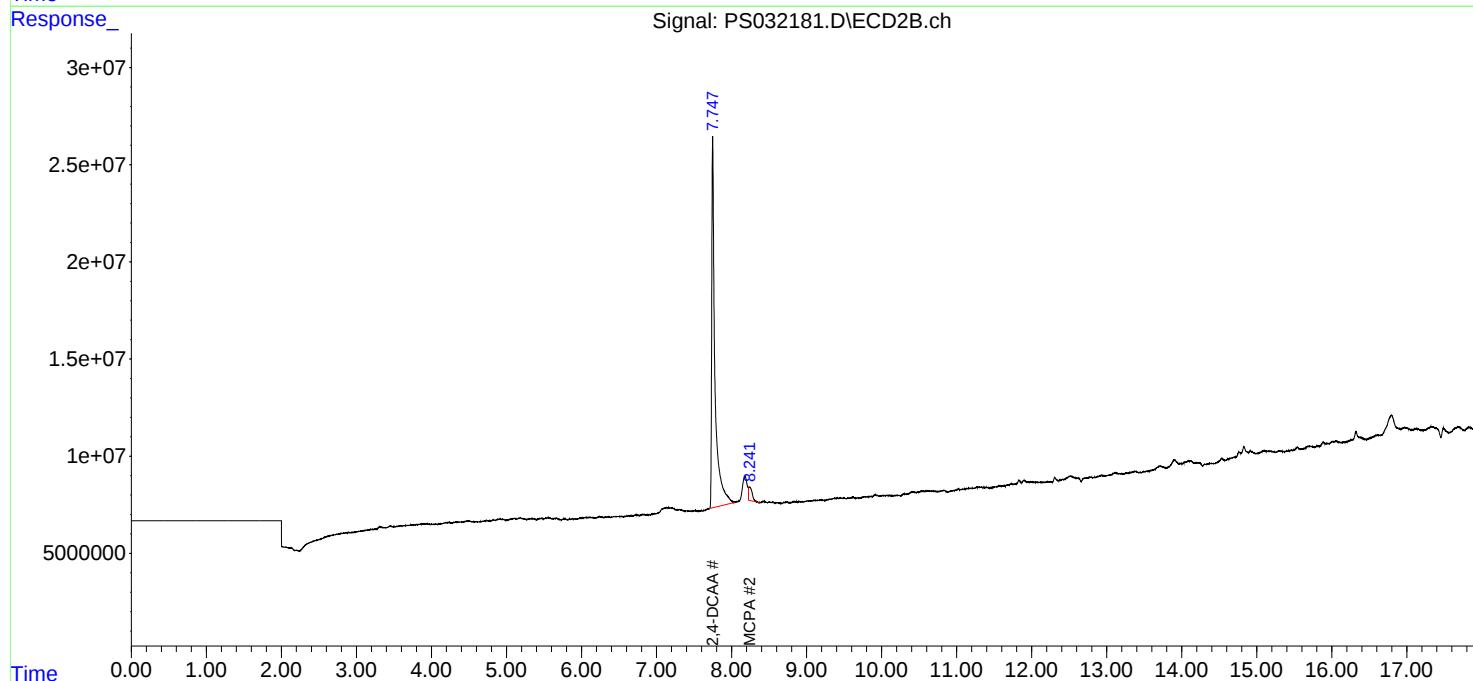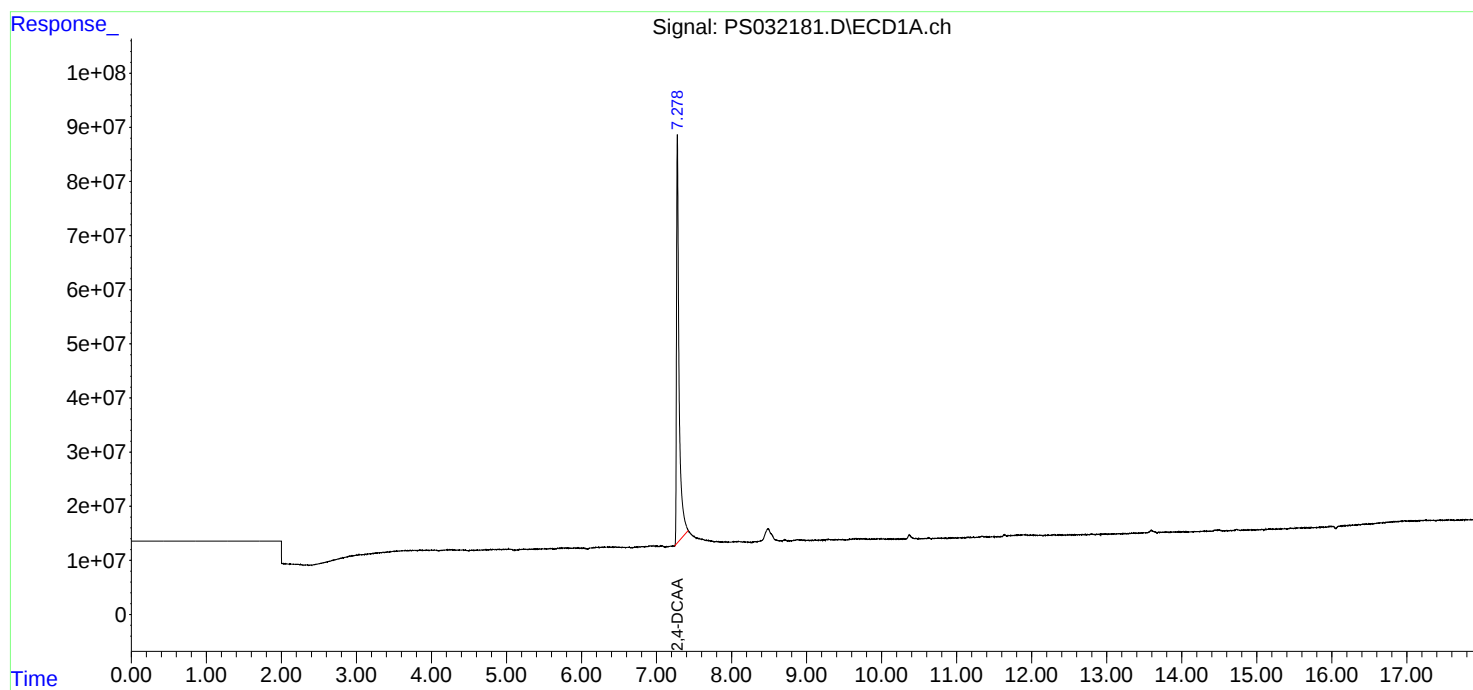


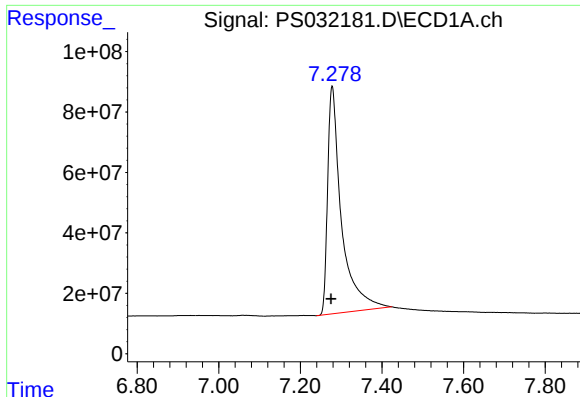

#4 2,4-DCAA


R.T.: 7.278 min
Delta R.T.: 0.003 min
Response: 1775311593
Conc: 410.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

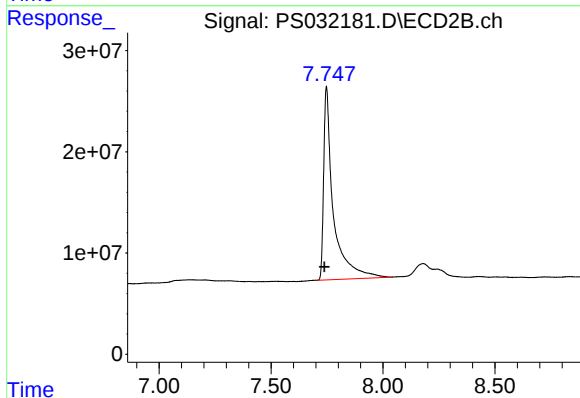


#4 2,4-DCAA

R.T.: 7.748 min
Delta R.T.: 0.010 min
Response: 574252589
Conc: 525.13 ng/ml

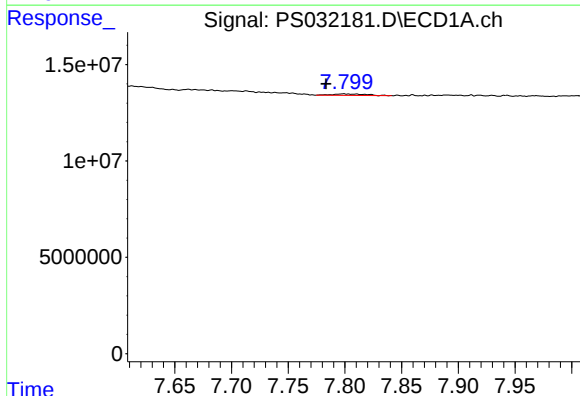

#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.016 min
Response: 1551127
Conc: N.D.

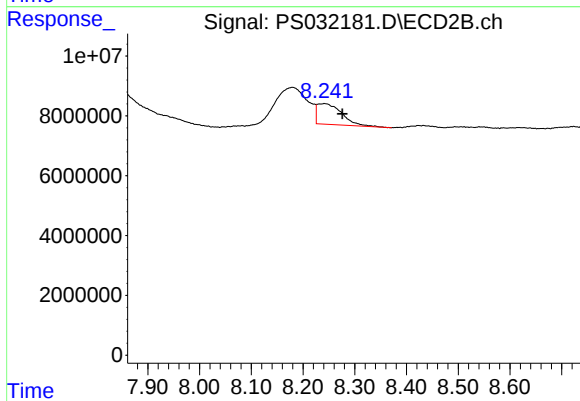

#7 MCPA

R.T.: 8.242 min
Delta R.T.: -0.035 min
Response: 22662042
Conc: 6.47 ug/ml