

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 03:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:25:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:40:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.280	7.754	1809.8E6	575.1E6	418.580	525.914 #
Target Compounds							
2) T	3,5-DICHL...	6.439	0.000	268019	0	<MDL	N.D. #
6) T	MCP	0.000	8.069f	0	1208034	N.D.	<MDL
7) T	MCPA	7.805	0.000	2105229	0	<MDL	N.D. #
8) T	DICHLORPROP	8.150	0.000	2341145	0	<MDL	N.D. #
10) T	Pentachlo...	8.711	0.000	3796478	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.275	0.000	2441333	0	<MDL	N.D. #
12) T	2,4,5-T	9.612f	10.310	4677198	2645292	<MDL	<MDL #
13) T	2,4-DB	10.137	0.000	613690	0	<MDL	N.D. #
14) T	DINOSEB	11.346	0.000	3459076	0	<MDL	N.D. #
15) T	Picloram	11.168	0.000	305105	0	<MDL	N.D. #
16) T	DCPA	11.636	12.328f	2378550	6180574	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 03:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:25:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

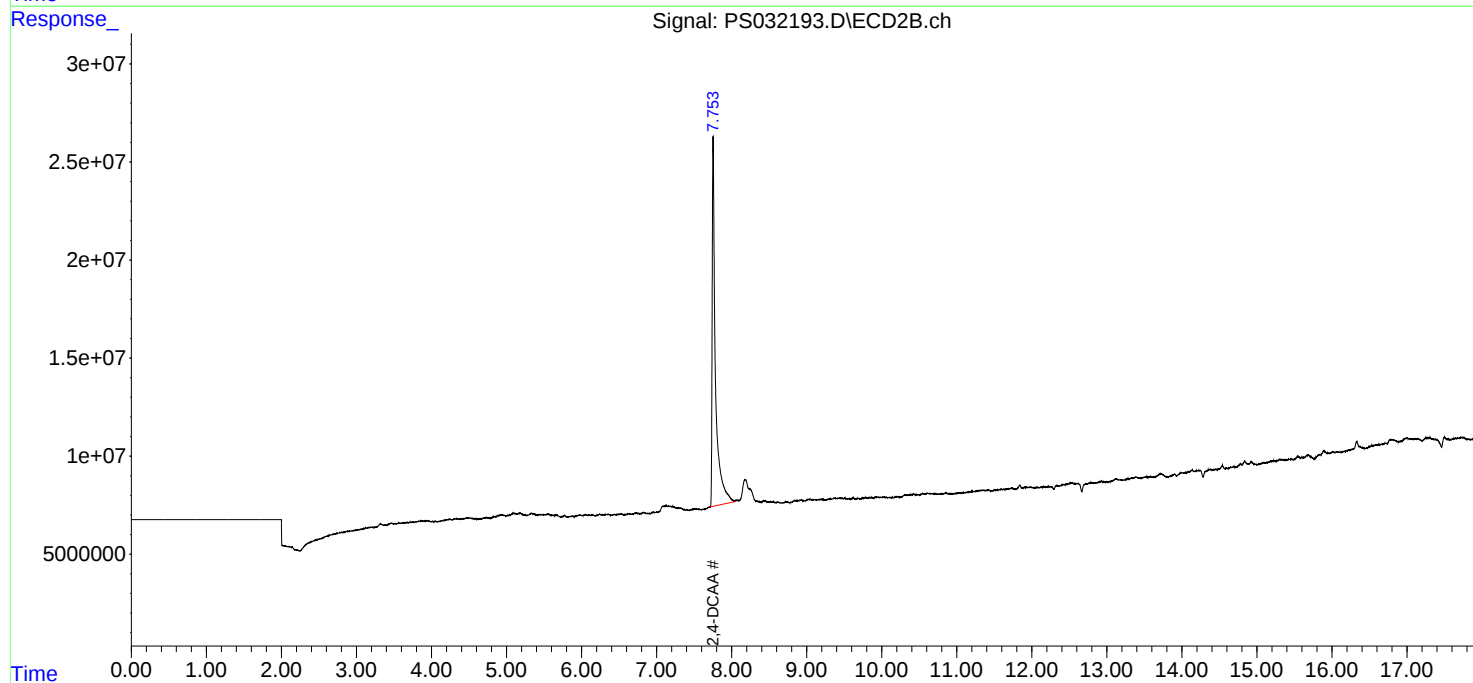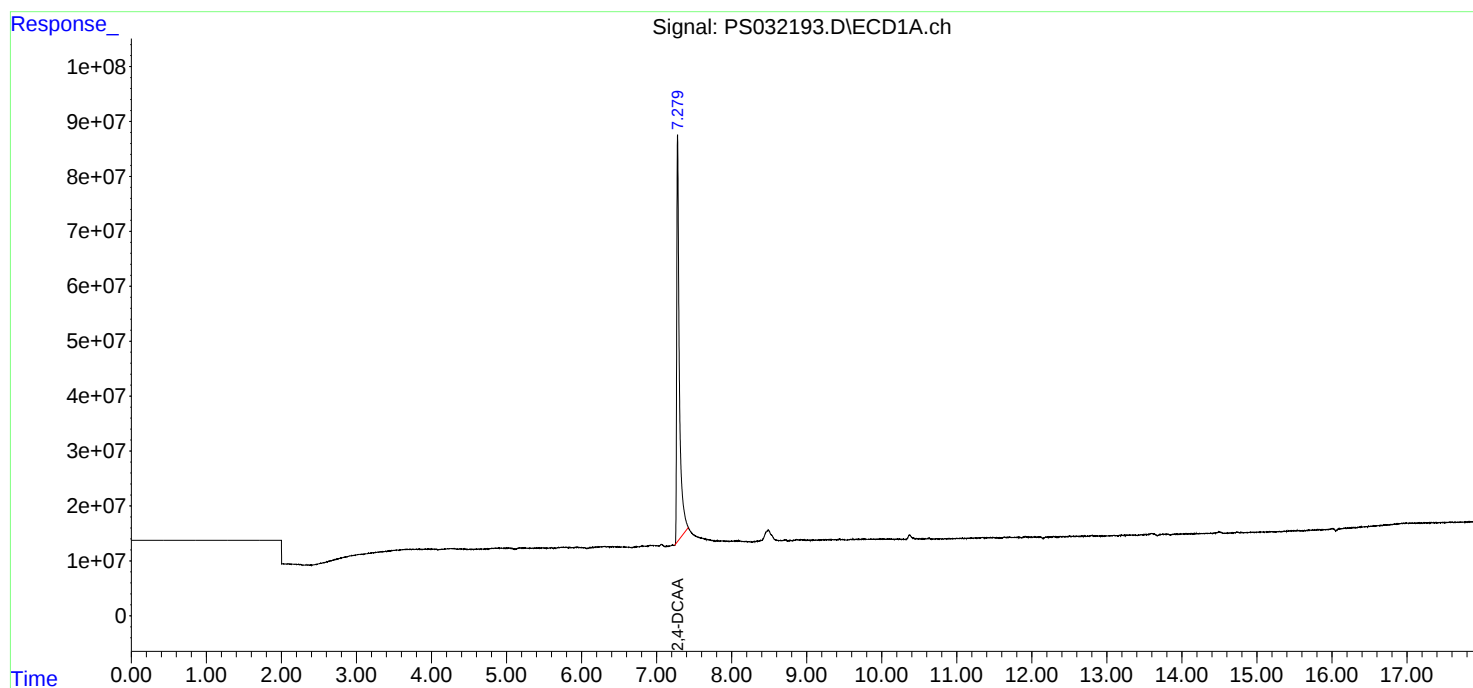


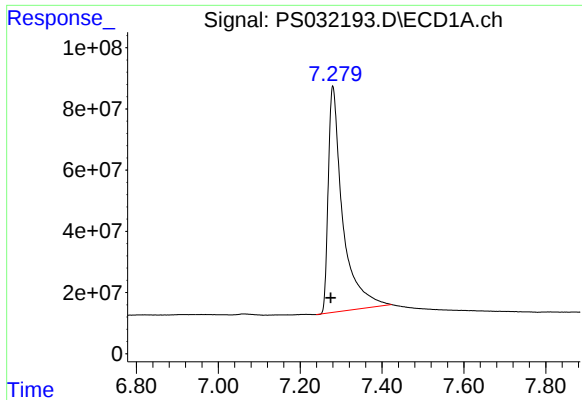

#4 2,4-DCAA

R.T.: 7.280 min
Delta R.T.: 0.005 min
Response: 1809796942
Conc: 418.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

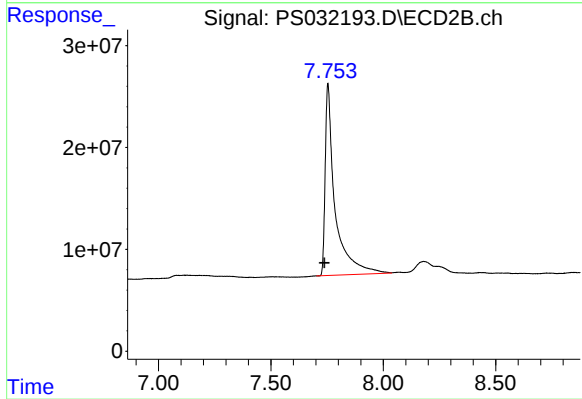

#4 2,4-DCAA

R.T.: 7.754 min
Delta R.T.: 0.016 min
Response: 575105392
Conc: 525.91 ng/ml