

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2025 08:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 09:07:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:40:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.280	7.758	1808.3E6	568.2E6	418.228	519.643
Target Compounds							
2) T	3,5-DICHL...	6.436	0.000	316045	0	<MDL	N.D. #
6) T	MCPD	7.600f	8.066f	76279	1499325	<MDL	<MDL #
7) T	MCPA	7.779	8.244f	125295	17919819	<MDL	5.117 #
8) T	DICHLORPROP	8.158	0.000	1139632	0	<MDL	N.D. #
9) T	2,4-D	8.381f	0.000	140892	0	<MDL	N.D. #
10) T	Pentachlo...	8.709	9.519	4701735	3725824	<MDL	<MDL #
11) T	2,4,5-TP ...	9.280	0.000	2277928	0	<MDL	N.D. #
12) T	2,4,5-T	9.584	10.313	1631066	2220318	<MDL	<MDL #
13) T	2,4-DB	10.134	0.000	1575525	0	<MDL	N.D. #
14) T	DINOSEB	11.343	0.000	4462519	0	<MDL	N.D. #
15) T	Picloram	11.171	0.000	528109	0	<MDL	N.D. #
16) T	DCPA	11.639	12.325f	6774770	11698245	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 08:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 09:07:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

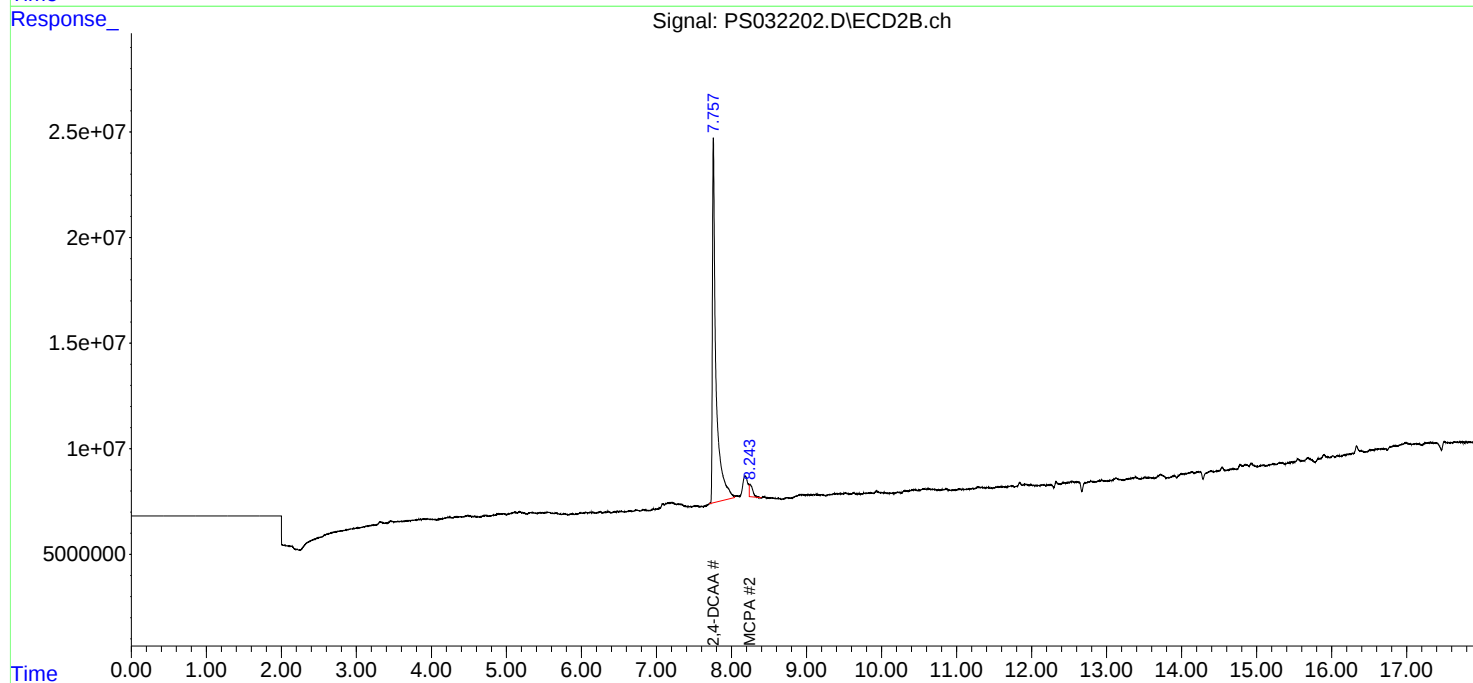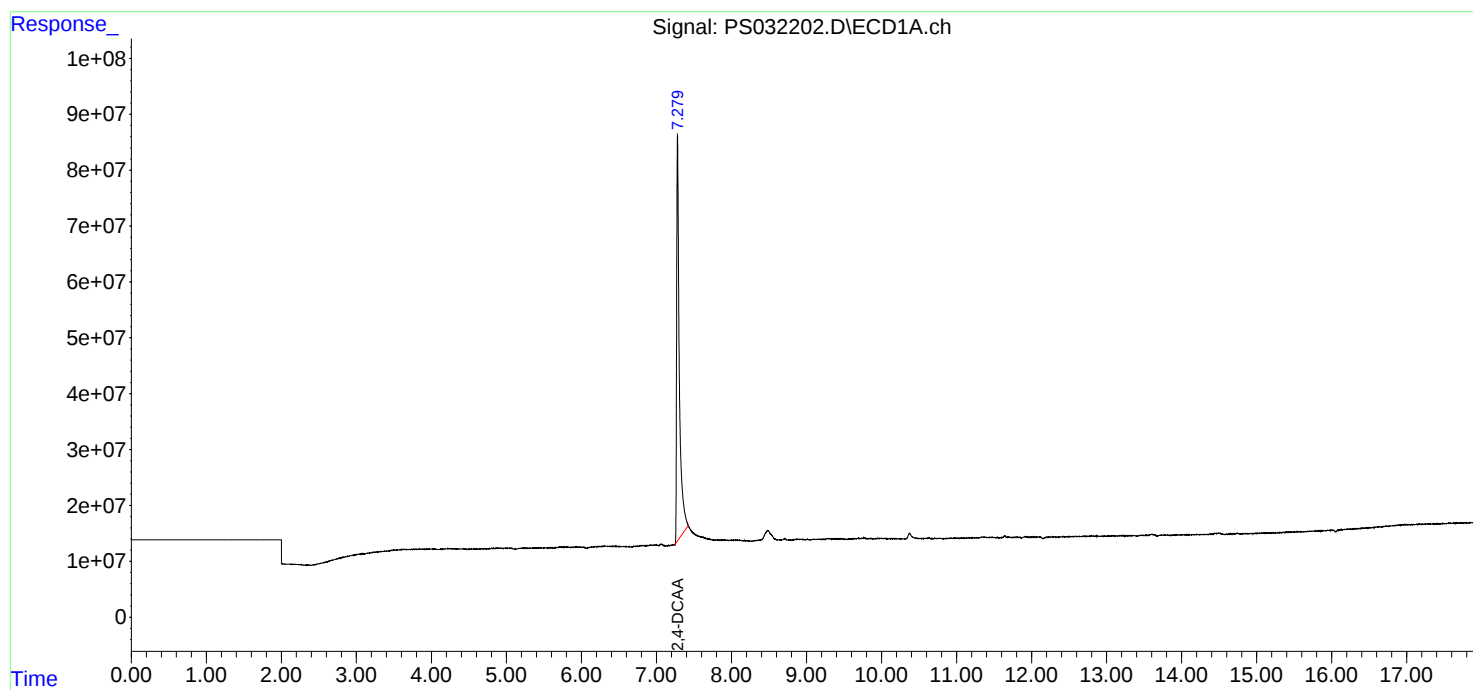


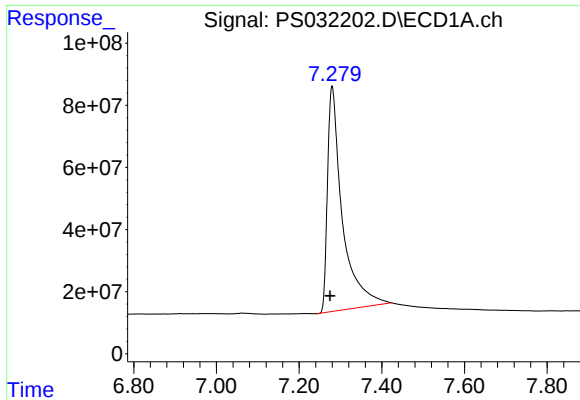

#4 2,4-DCAA


R.T.: 7.280 min
Delta R.T.: 0.005 min
Response: 1808276205
Conc: 418.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

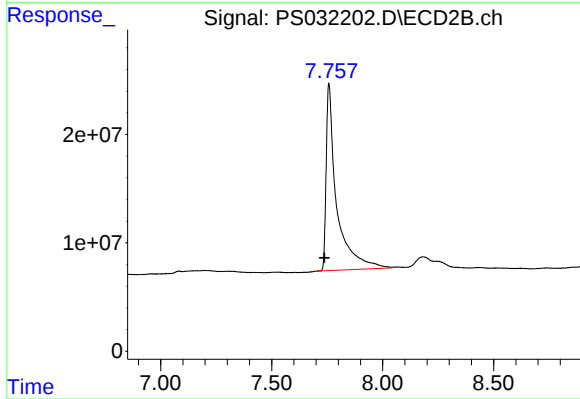


#4 2,4-DCAA

R.T.: 7.758 min
Delta R.T.: 0.020 min
Response: 568247493
Conc: 519.64 ng/ml

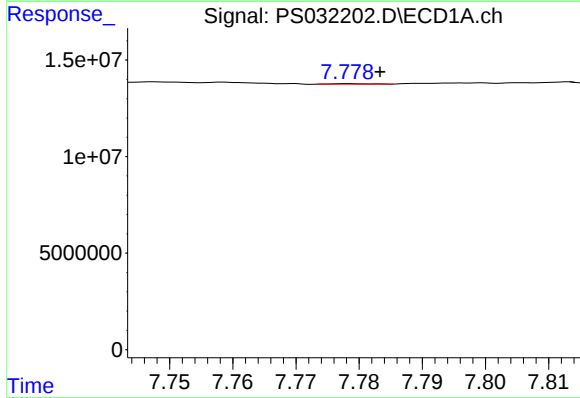

#7 MCPA

R.T.: 7.779 min
Delta R.T.: -0.005 min
Response: 125295
Conc: N.D.

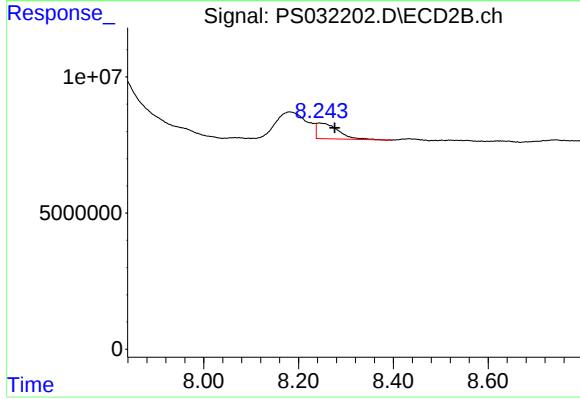

#7 MCPA

R.T.: 8.244 min
Delta R.T.: -0.033 min
Response: 17919819
Conc: 5.12 ug/ml