

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
 Data File : PS032173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2025 17:31
 Operator : AR\AJ
 Sample : Q3449-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CF-620-COMP-41

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/28/2025
 Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 06:22:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 28 04:40:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.274	7.738	1070.9E6	322.6E6	247.681m	295.043m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2025 17:31
Operator : AR\AJ
Sample : Q3449-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/28/2025
Supervised By : mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:22:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

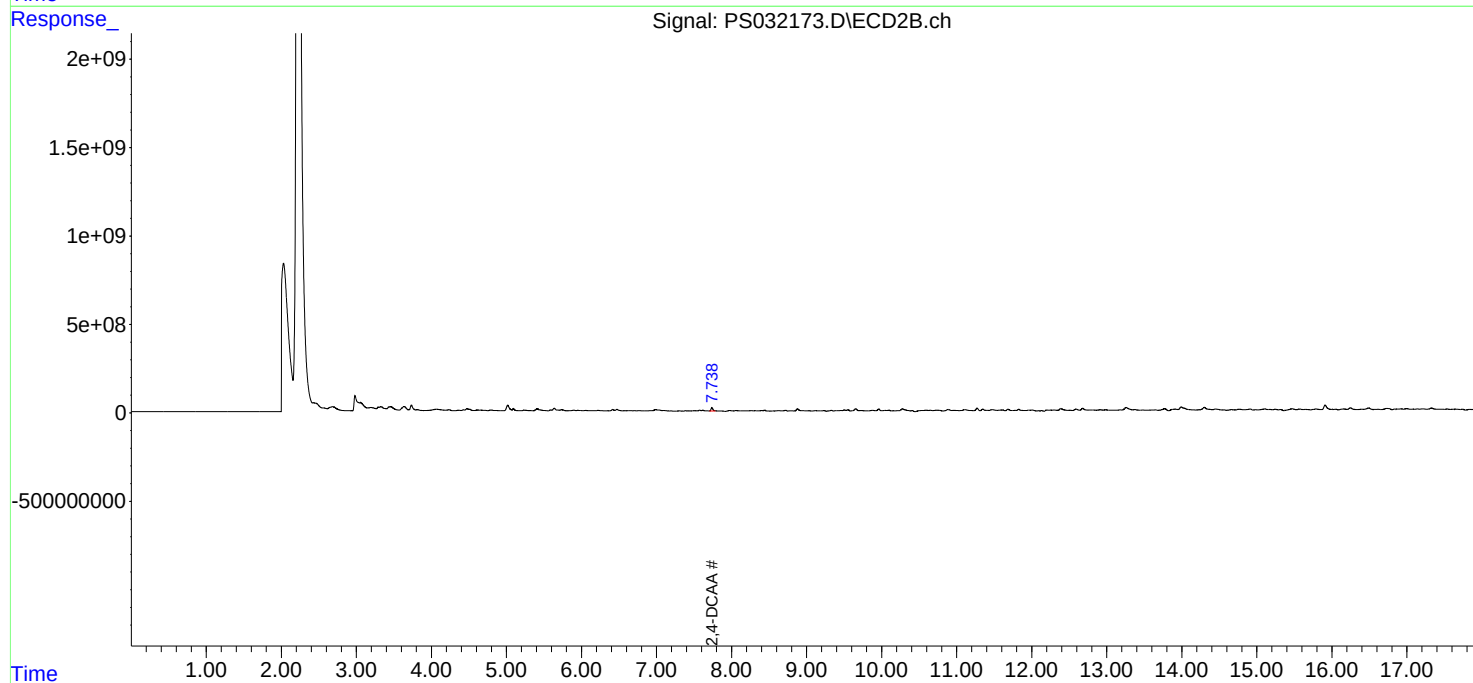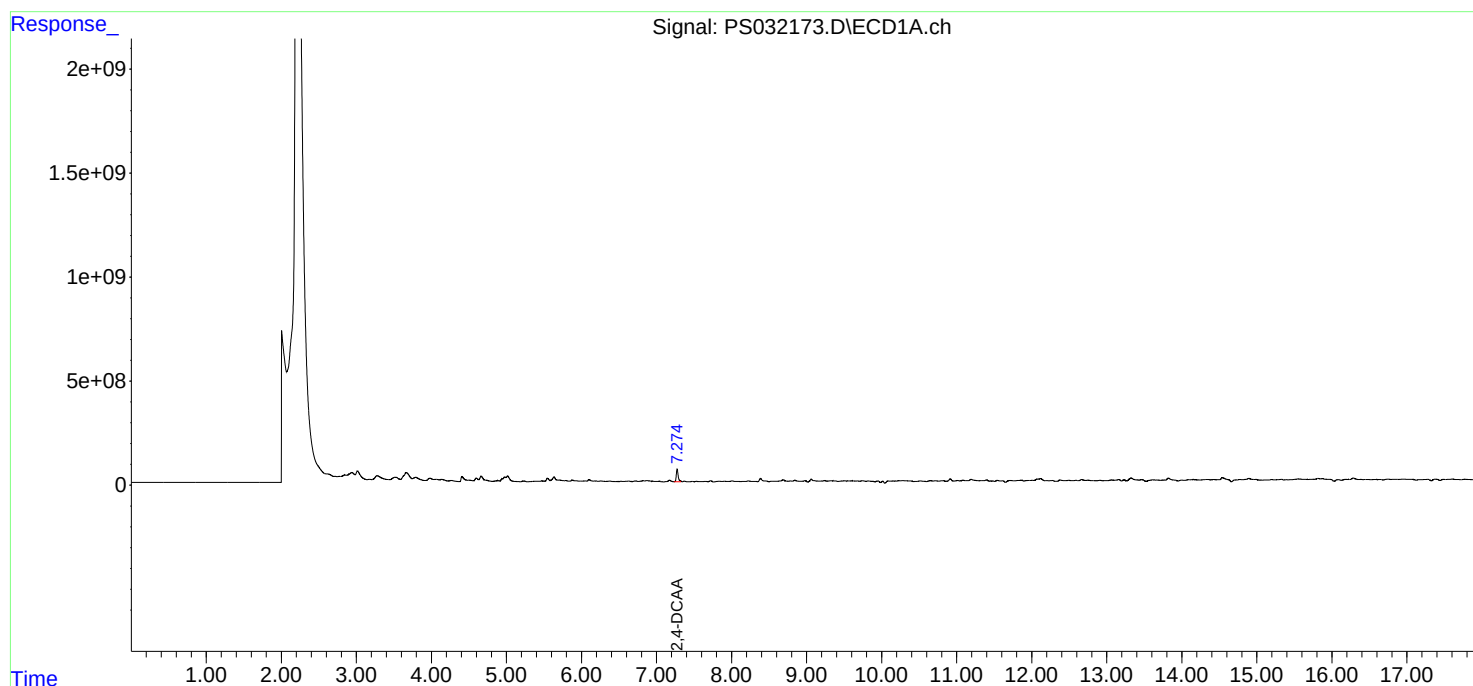

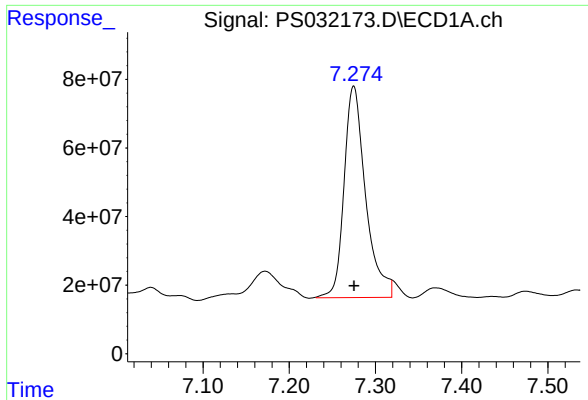


#4 2,4-DCAA

R.T.: 7.274 min
Delta R.T.: 0.000 min
Response: 1070889652
Conc: 247.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
CF-620-COMP-41

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

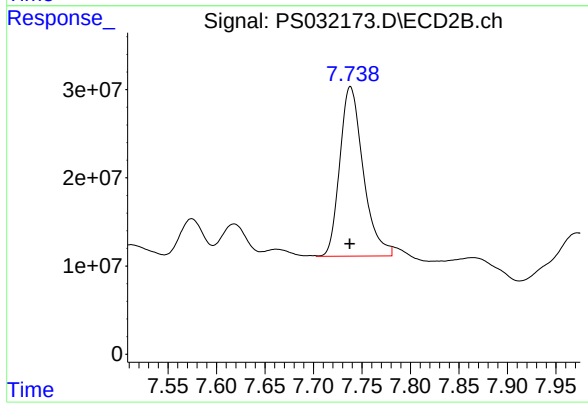

#4 2,4-DCAA

R.T.: 7.738 min
Delta R.T.: 0.000 min
Response: 322640380
Conc: 295.04 ng/ml m