

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 00:28
Operator : AR\AJ
Sample : Q3460-09
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WC-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:24:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.272	7.743	1089.4E6	284.9E6	251.951m	260.566m
------	----------	-------	-------	----------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102725\
Data File : PS032188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2025 00:28
Operator : AR\AJ
Sample : Q3460-09
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
WC-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/28/2025
Supervised By : mohammad ahmed 10/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 06:24:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102725.M
Quant Title : 8080.M
QLast Update : Tue Oct 28 04:40:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

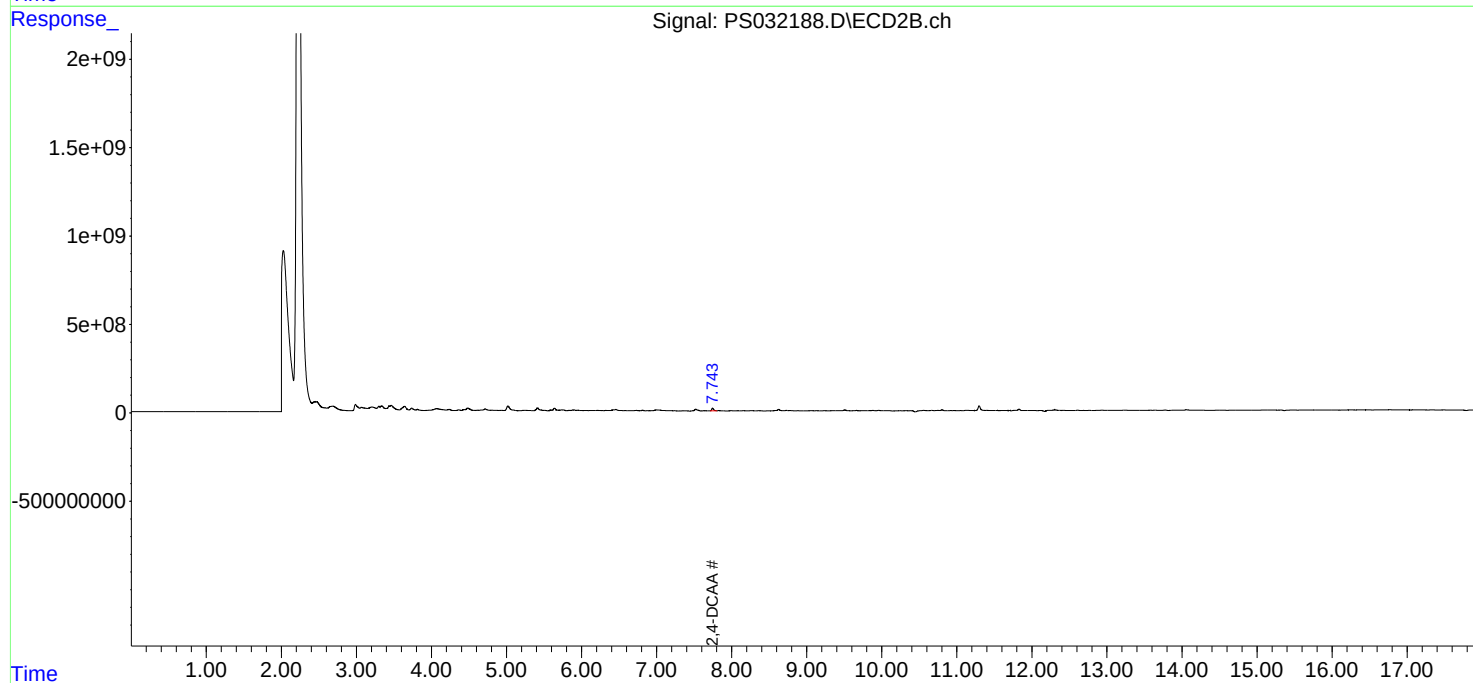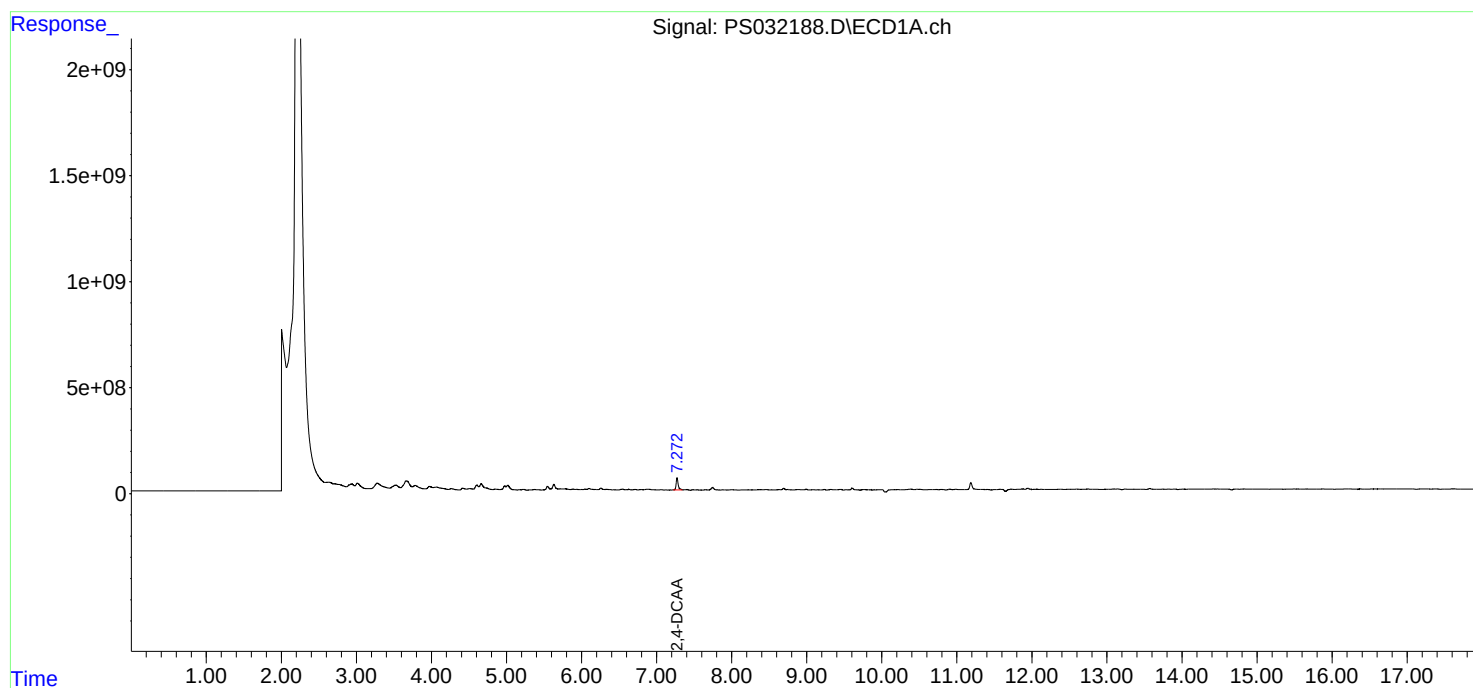

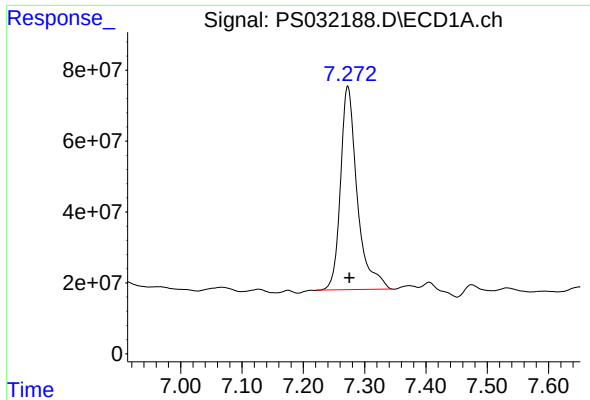


#4 2,4-DCAA

R.T.: 7.272 min
Delta R.T.: -0.003 min
Response: 1089352304
Conc: 251.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
WC-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/28/2025
Supervised By :mohammad ahmed 10/29/2025

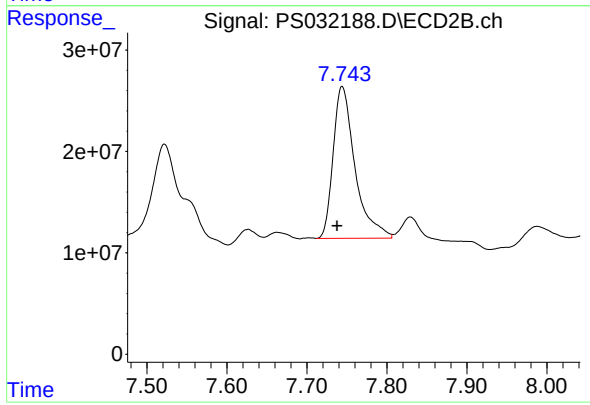

#4 2,4-DCAA

R.T.: 7.743 min
Delta R.T.: 0.006 min
Response: 284938518
Conc: 260.57 ng/ml m