

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
 Data File : PS007389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 10:59
 Operator : SM\AJ
 Sample : PB124307BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 13:01:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.453	5.178	619.6E6	345.1E6	452.700	490.692
Target Compounds							
1) T	Dalapon	0.000	1.719	0 19092599		N.D.	20.981
2) T	3,5-DICHL...	0.000	4.513	0 34630593		N.D.	40.248
5) T	DICAMBA	5.546	0.000	37643259	0	7.661	N.D. #
7) T	MCPA	0.000	5.495	0 51199780		N.D.	17.612
10) T	Pentachlo...	0.000	6.465	0 13961275		N.D.	1.452
11) T	2,4,5-TP ...	0.000	6.777	0 18188617		N.D.	4.782
12) T	2,4,5-T	0.000	7.236	0 43293805		N.D.	12.357
15) T	Picloram	8.973	8.925	94890889	71298654	8.597	11.612 #
16) T	DCPA	0.000	8.925	0 71298654		N.D.	14.218



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
Data File : PS007389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 10:59
Operator : SM\AJ
Sample : PB124307BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 13:01:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

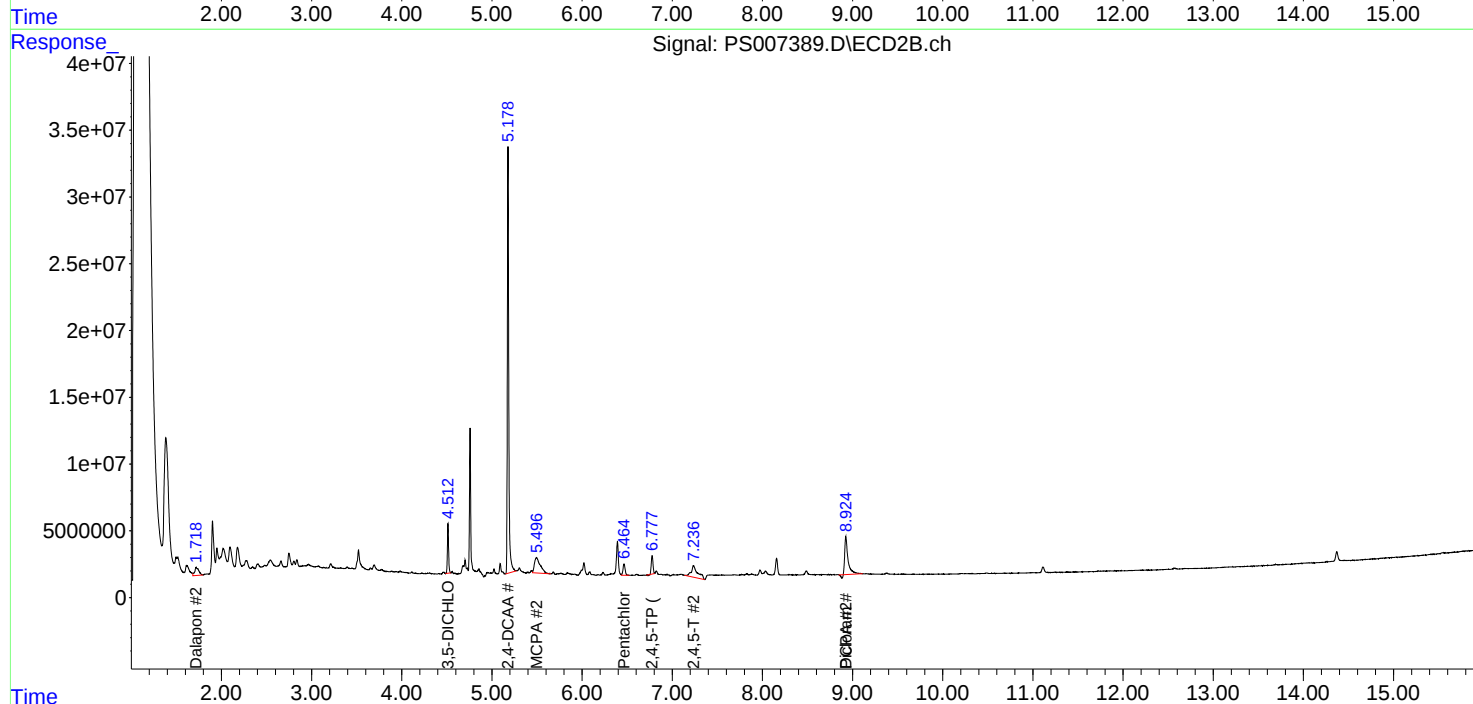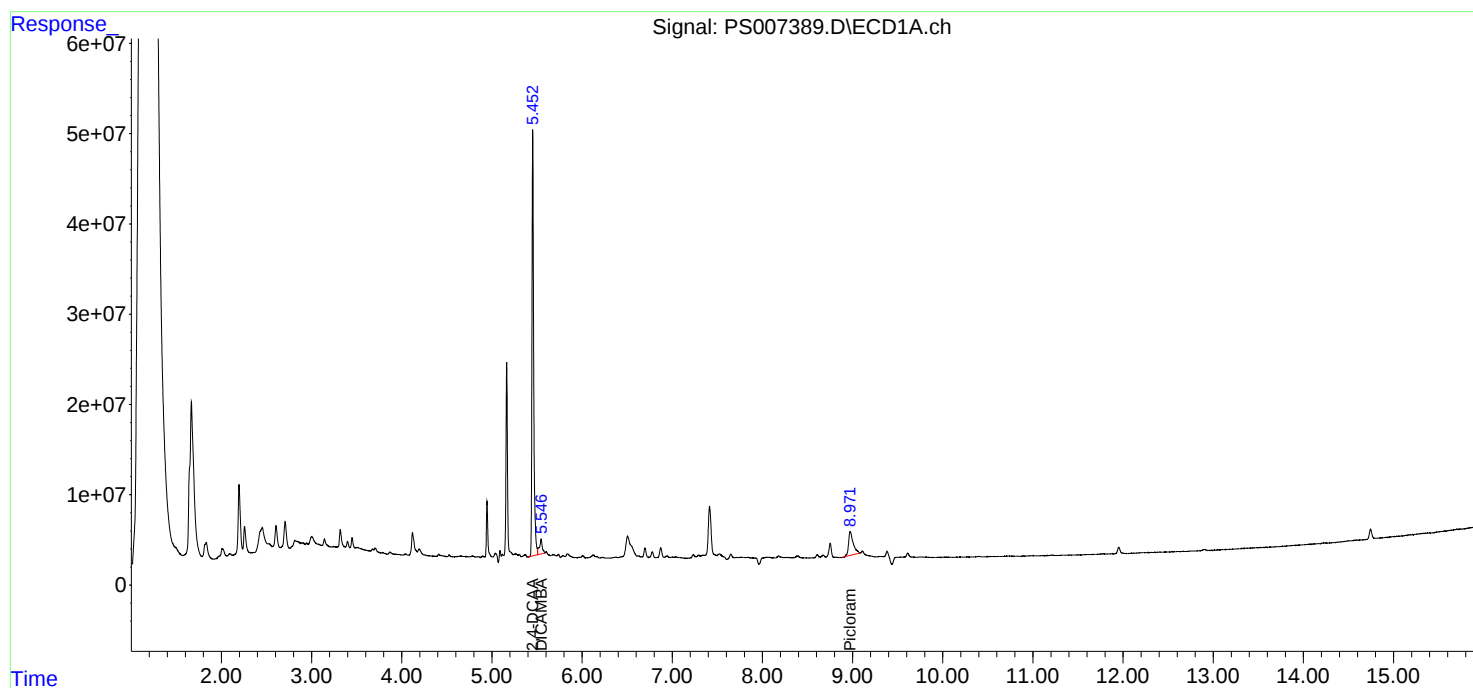


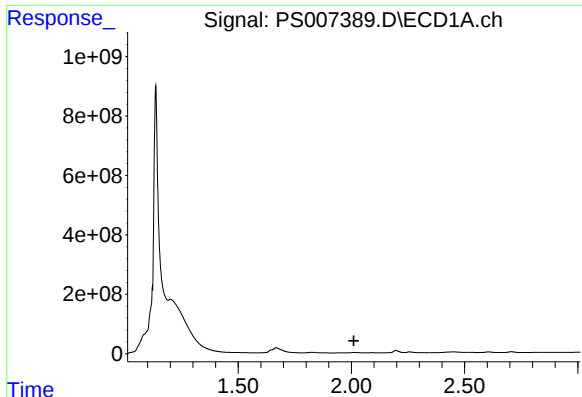

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

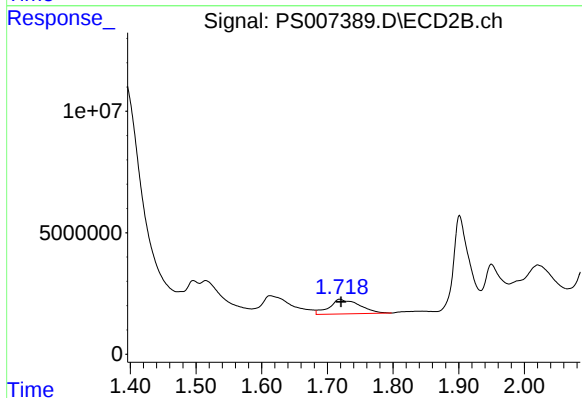


#1 Dalapon

R.T.: 1.719 min
Delta R.T.: -0.001 min
Response: 19092599
Conc: 20.98 ng/ml

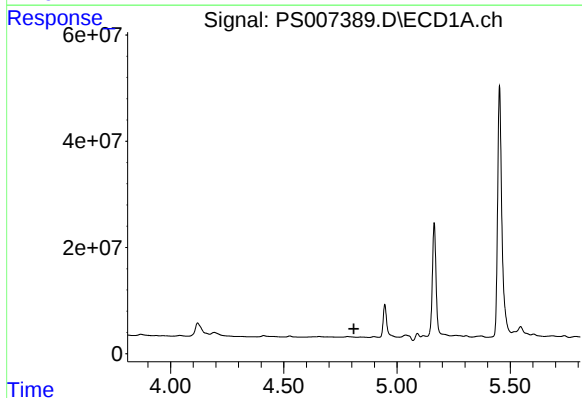


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

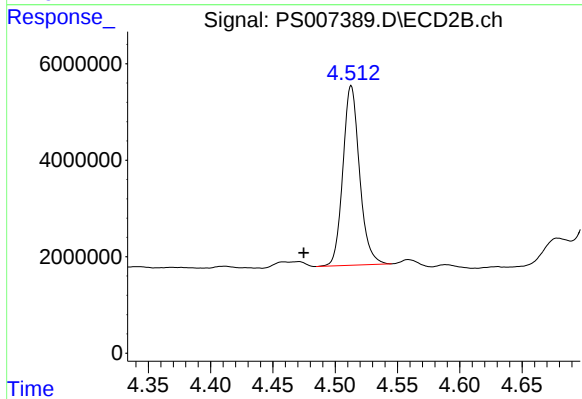

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.513 min
Delta R.T.: 0.038 min
Response: 34630593
Conc: 40.25 ng/ml

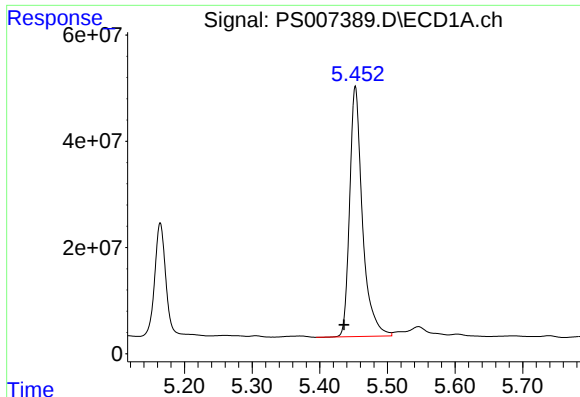

#4 2,4-DCAA


R.T.: 5.453 min
Delta R.T.: 0.017 min
Response: 619596642
Conc: 452.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

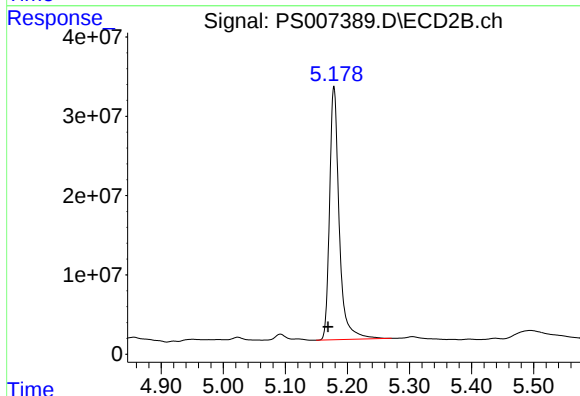


#4 2,4-DCAA

R.T.: 5.178 min
Delta R.T.: 0.010 min
Response: 345106860
Conc: 490.69 ng/ml

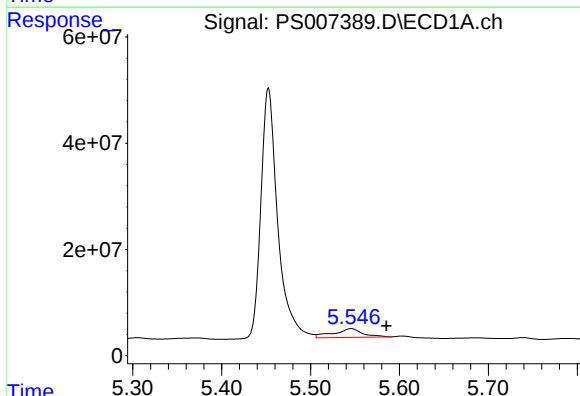


#5 DICAMBA

R.T.: 5.546 min
Delta R.T.: -0.040 min
Response: 37643259
Conc: 7.66 ng/ml

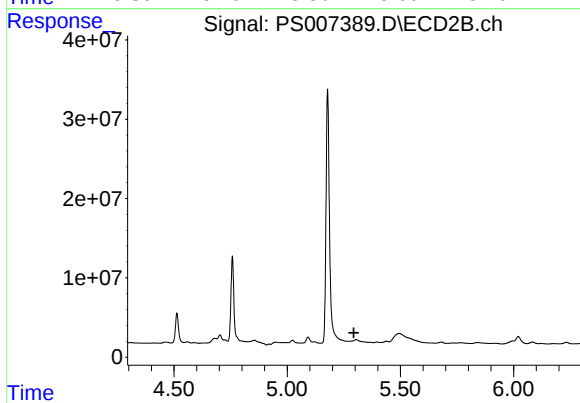

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

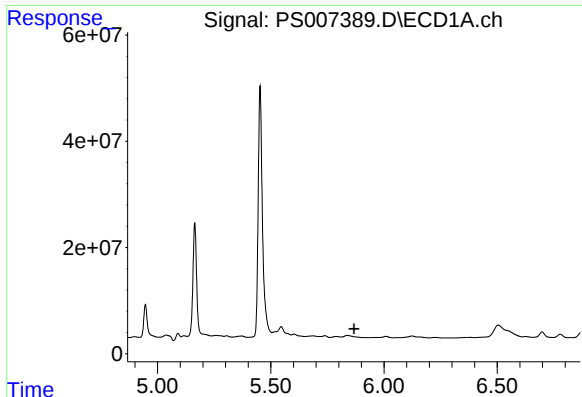

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

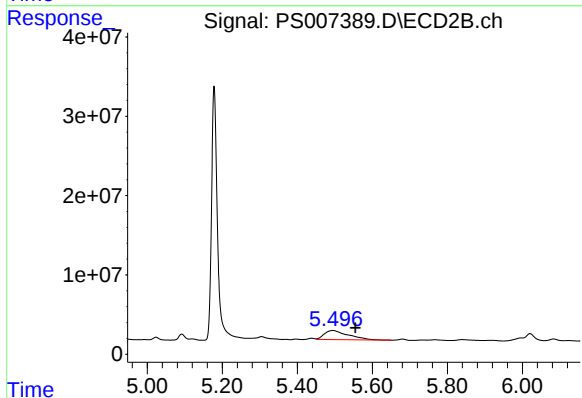


#7 MCPA

R.T.: 5.495 min
Delta R.T.: -0.060 min
Response: 51199780
Conc: 17.61 ug/ml

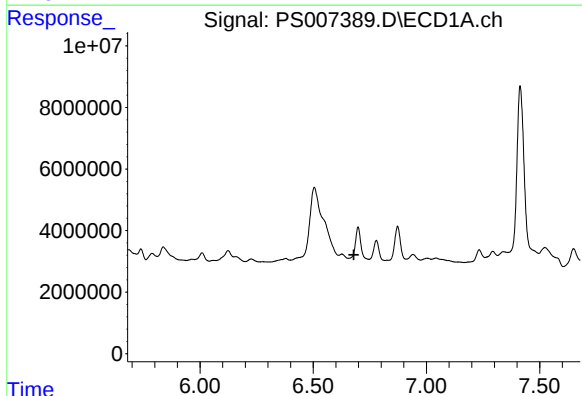


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

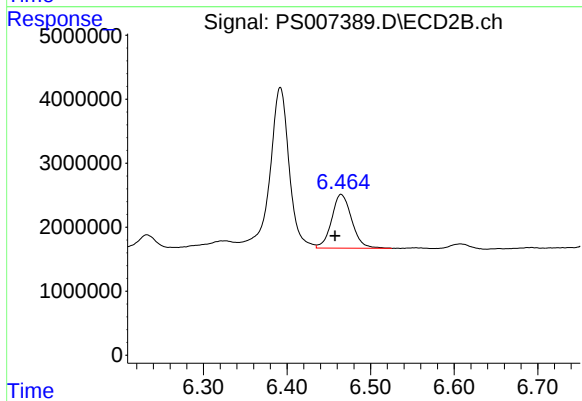

#10 Pentachlorophenol


R.T.: 6.465 min
Delta R.T.: 0.008 min
Response: 13961275
Conc: 1.45 ng/ml

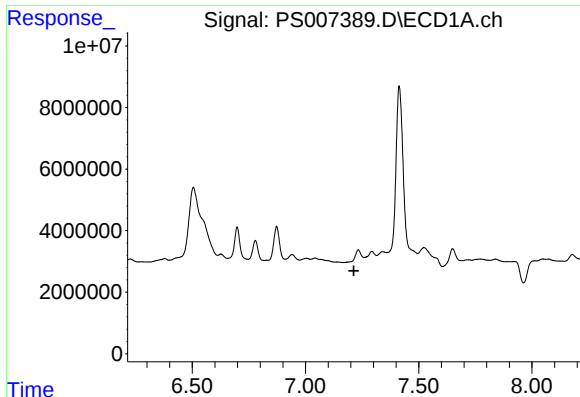

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

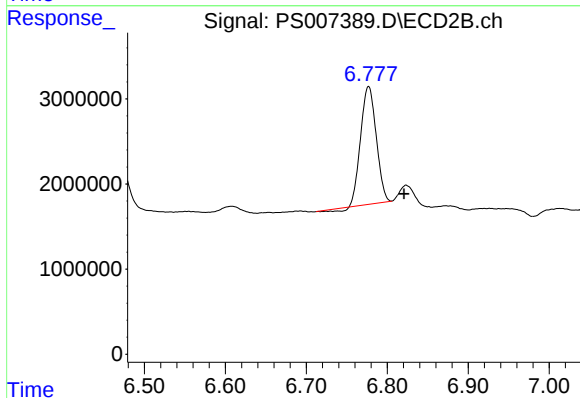


#11 2,4,5-TP (SILVEX)

R.T.: 6.777 min
Delta R.T.: -0.044 min
Response: 18188617
Conc: 4.78 ng/ml

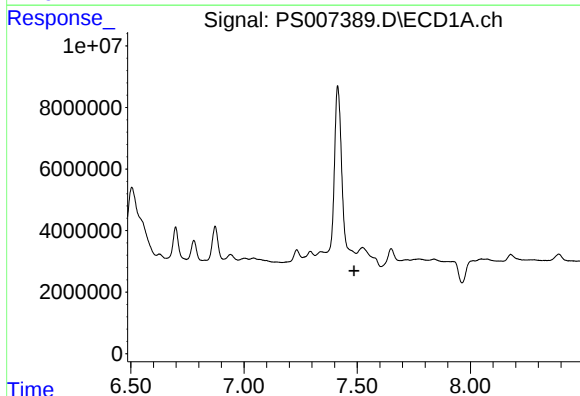


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

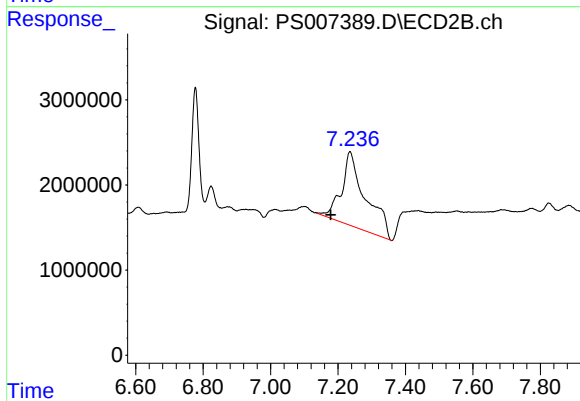

#12 2,4,5-T


R.T.: 7.236 min
Delta R.T.: 0.057 min
Response: 43293805
Conc: 12.36 ng/ml

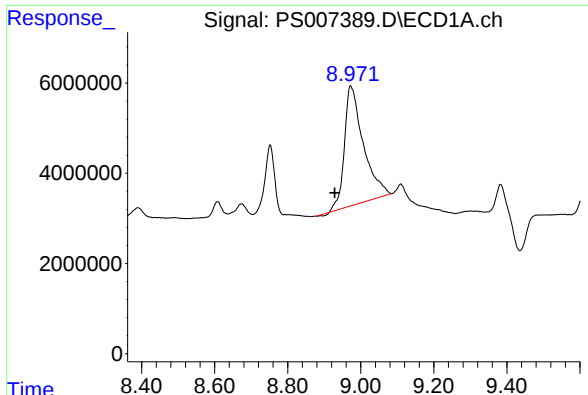

#15 Picloram


R.T.: 8.973 min
Delta R.T.: 0.044 min
Response: 94890889
Conc: 8.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

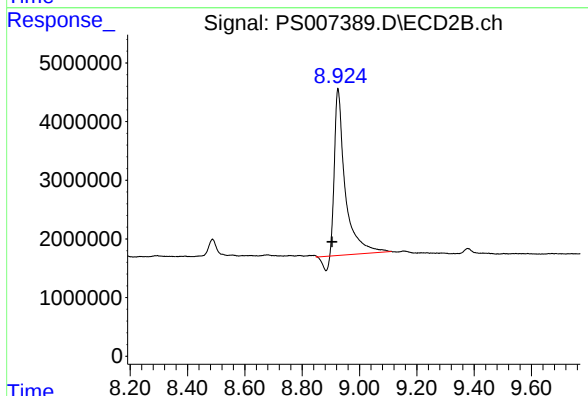


#15 Picloram

R.T.: 8.925 min
Delta R.T.: 0.021 min
Response: 71298654
Conc: 11.61 ng/ml

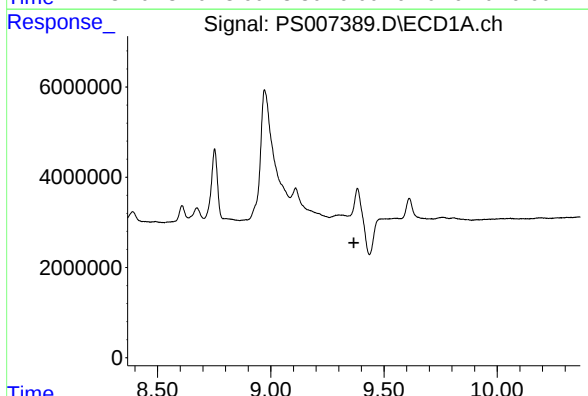

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

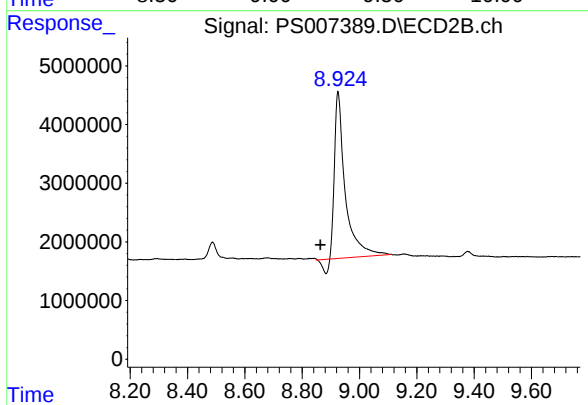

#16 DCPA

R.T.: 8.925 min
Delta R.T.: 0.062 min
Response: 71298654
Conc: 14.22 ng/ml