

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
 Data File : PS007399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 15:23
 Operator : SM\AJ
 Sample : PB124260BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 16:34:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.454	5.180	594.9E6	348.6E6	434.637	495.596
Target Compounds							
1) T	Dalapon	0.000	1.723	0 19394530		N.D.	21.313
2) T	3,5-DICHL...	0.000	4.515	0 35348248		N.D.	41.082
7) T	MCPA	0.000	5.503	0 49492011		N.D.	17.024
10) T	Pentachlo...	0.000	6.393	0 28229867		N.D.	2.936
11) T	2,4,5-TP ...	0.000	6.778	0 23352775		N.D.	6.140
12) T	2,4,5-T	7.418	0.000	81028652	0	10.599	N.D. #
15) T	Picloram	0.000	8.937	0 2415326		N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
Data File : PS007399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 15:23
Operator : SM\AJ
Sample : PB124260BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 16:34:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

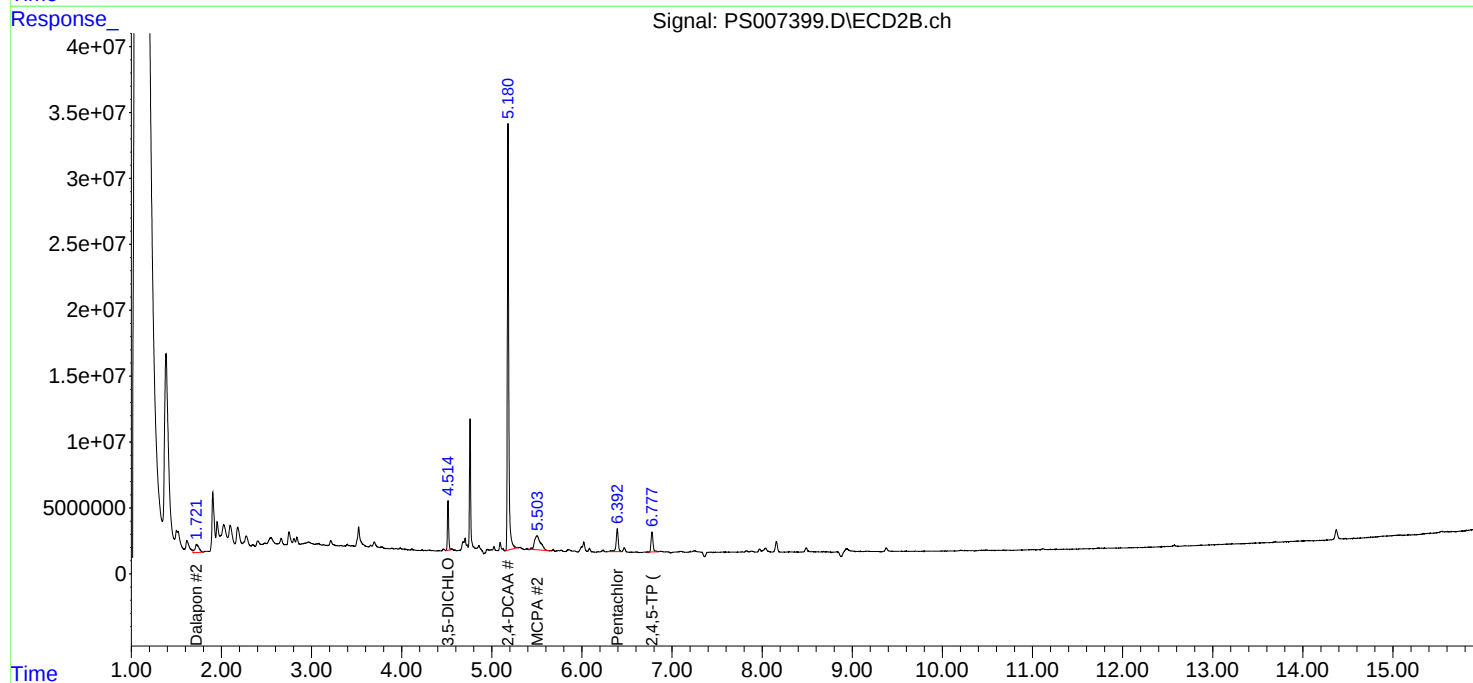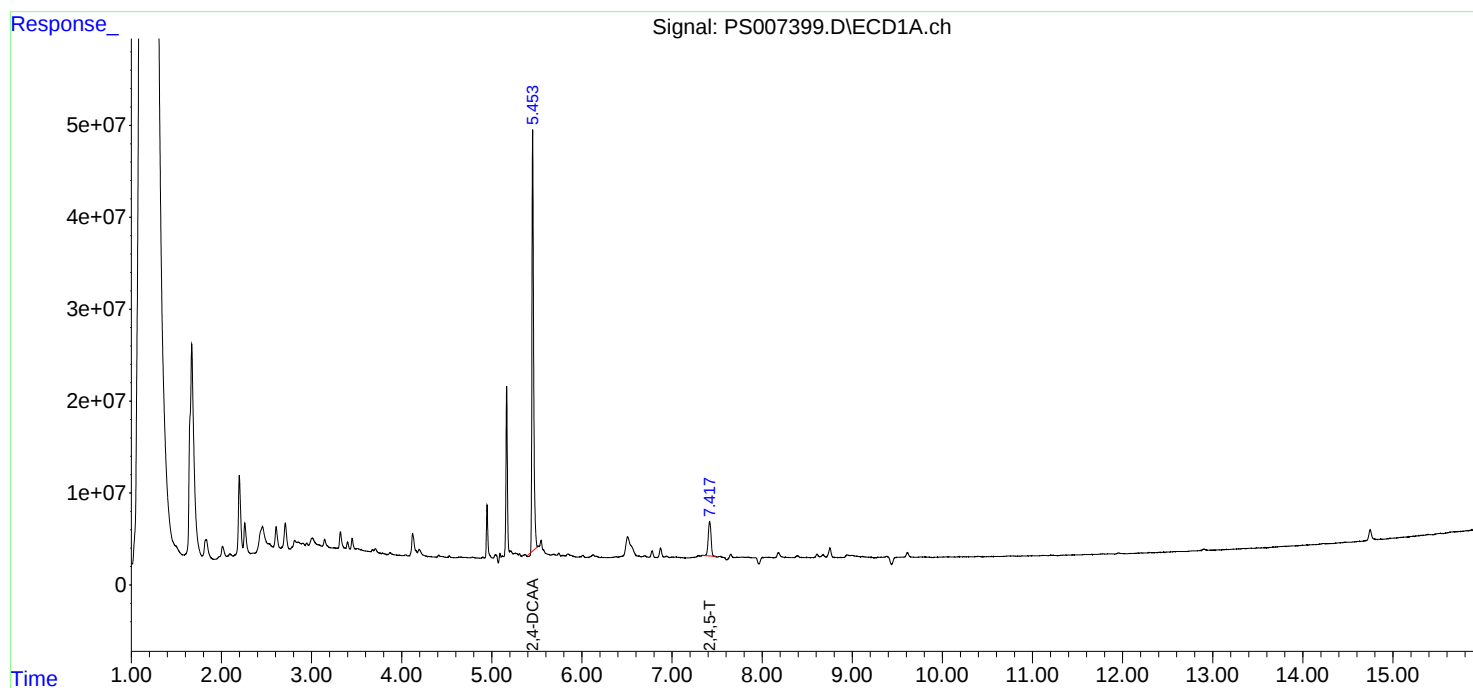


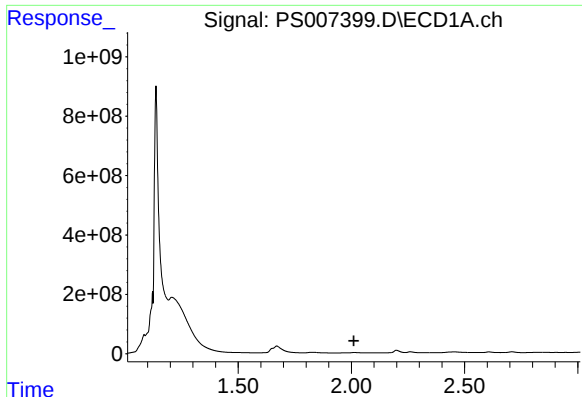

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

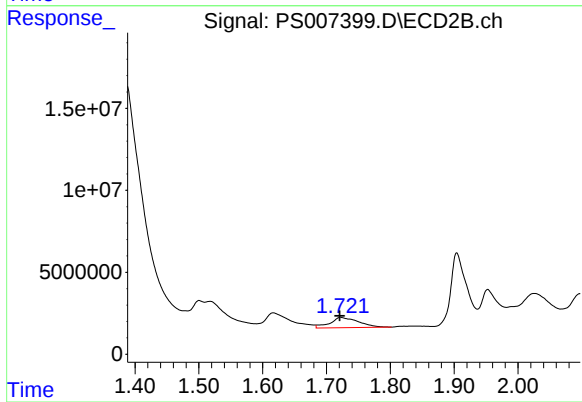


#1 Dalapon

R.T.: 1.723 min
Delta R.T.: 0.002 min
Response: 19394530
Conc: 21.31 ng/ml

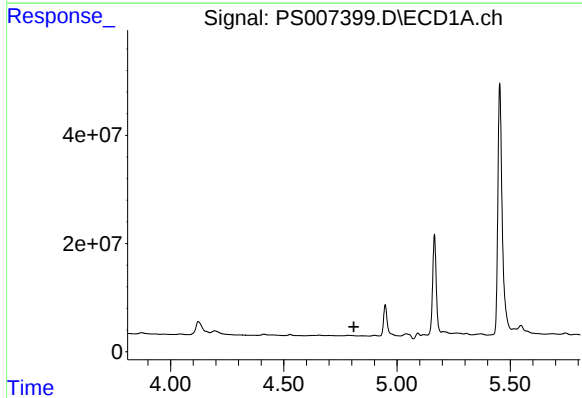


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

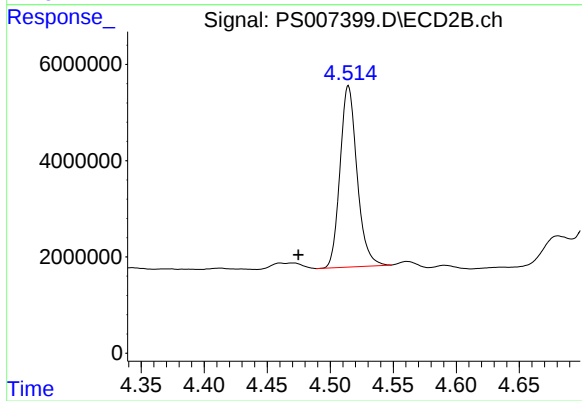

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.515 min
Delta R.T.: 0.040 min
Response: 35348248
Conc: 41.08 ng/ml

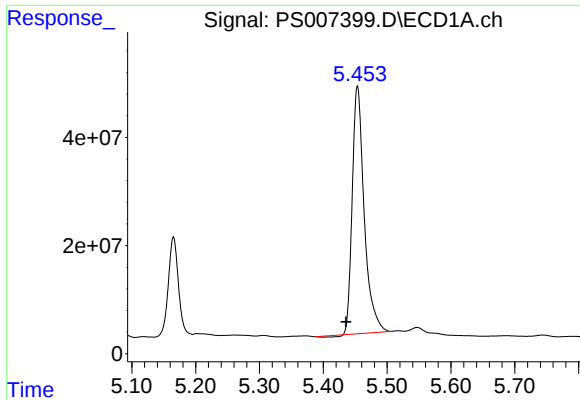

#4 2,4-DCAA


R.T.: 5.454 min
Delta R.T.: 0.018 min
Response: 594873866
Conc: 434.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

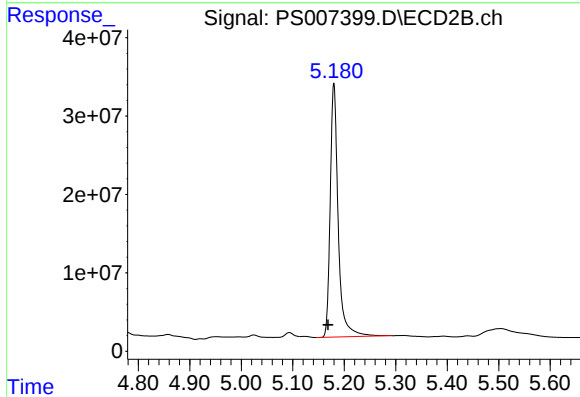


#4 2,4-DCAA

R.T.: 5.180 min
Delta R.T.: 0.011 min
Response: 348556106
Conc: 495.60 ng/ml

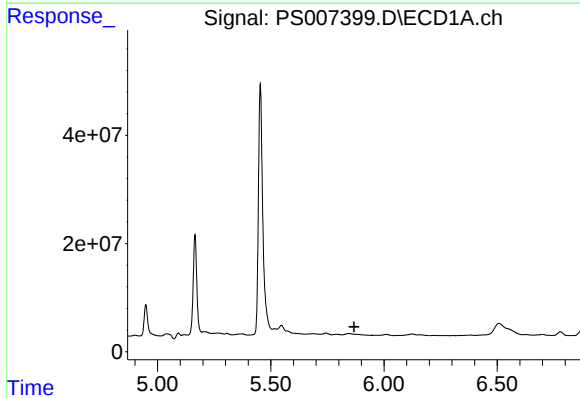


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

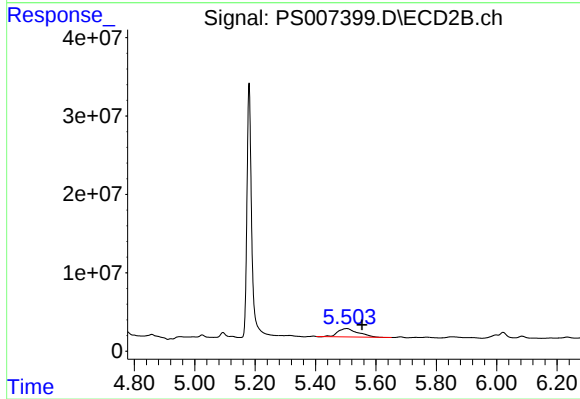

#7 MCPA


R.T.: 5.503 min
Delta R.T.: -0.052 min
Response: 49492011
Conc: 17.02 ug/ml

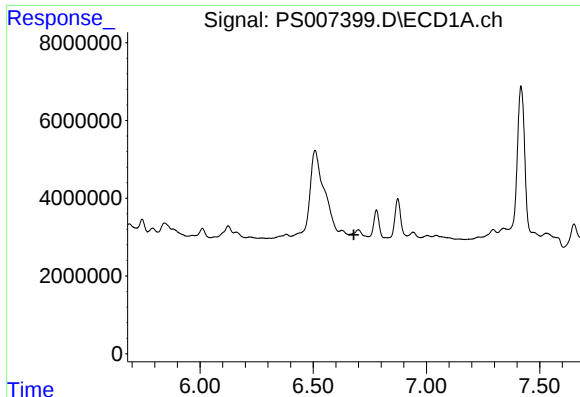

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

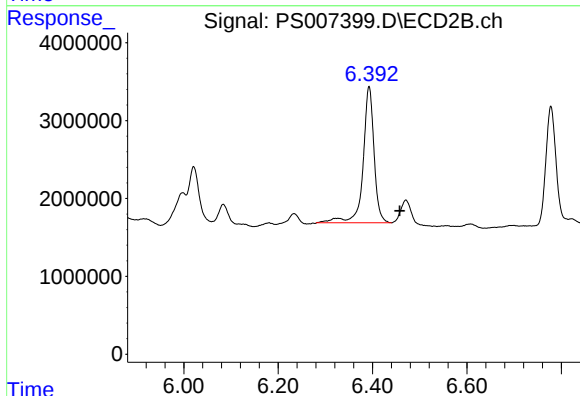


#10 Pentachlorophenol

R.T.: 6.393 min
Delta R.T.: -0.065 min
Response: 28229867
Conc: 2.94 ng/ml

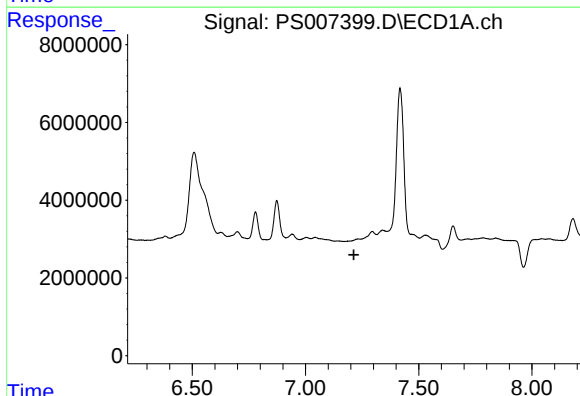


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

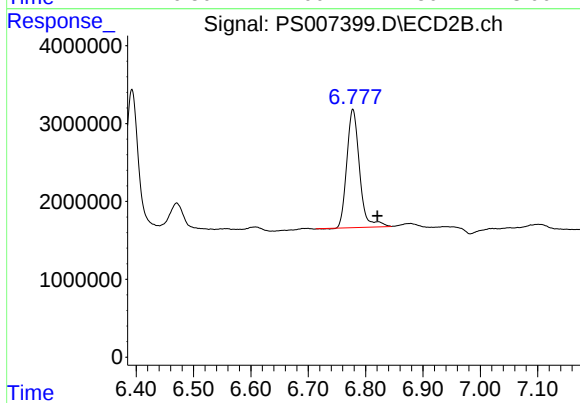

#11 2,4,5-TP (SILVEX)


R.T.: 6.778 min
Delta R.T.: -0.043 min
Response: 23352775
Conc: 6.14 ng/ml

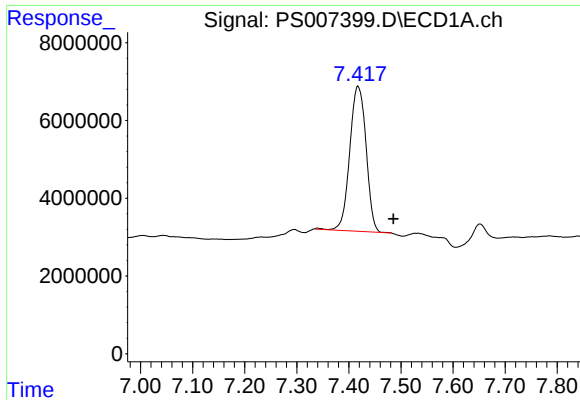

#12 2,4,5-T

R.T.: 7.418 min
Delta R.T.: -0.068 min
Response: 81028652
Conc: 10.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

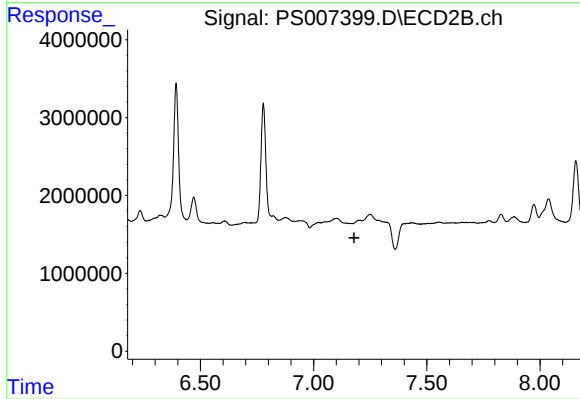

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.