

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
 Data File : PS007422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2019 23:48
 Operator : SM\AJ
 Sample : K5503-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 08:51:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	5.155	0	19419705	N.D.	27.612
Target Compounds							
1) T	Dalapon	0.000	1.690	0	631.1E6	N.D.	693.552
2) T	3,5-DICHL...	0.000	4.525	0	20083702	N.D.	23.341
5) T	DICAMBA	5.559	5.315	58662935	17351817	11.939	6.668 #
6) T	MCP	0.000	5.315	0	17351817	N.D.	9.148
7) T	MCPA	5.933	5.559	10579166	19013384	2.051	6.540 #
9) T	2,4-D	0.000	6.095	0	12596277	N.D.	15.789
10) T	Pentachlo...	0.000	6.474	0	14345089	N.D.	1.492
11) T	2,4,5-TP ...	0.000	6.833	0	15421761	N.D.	4.055
12) T	2,4,5-T	7.418	7.191	122.2E6	16321304	15.991	4.658 #
13) T	2,4-DB	0.000	7.710	0	21224375	N.D.	45.284
14) T	DINOSEB	0.000	7.984	0	2816946	N.D.	1.003
15) T	Picloram	8.962	8.926	244.6E6	137.7E6	22.158	22.432
16) T	DCPA	9.404	8.808	74021103	55617960	8.267	11.091 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102819\
Data File : PS007422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2019 23:48
Operator : SM\AJ
Sample : K5503-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 08:51:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

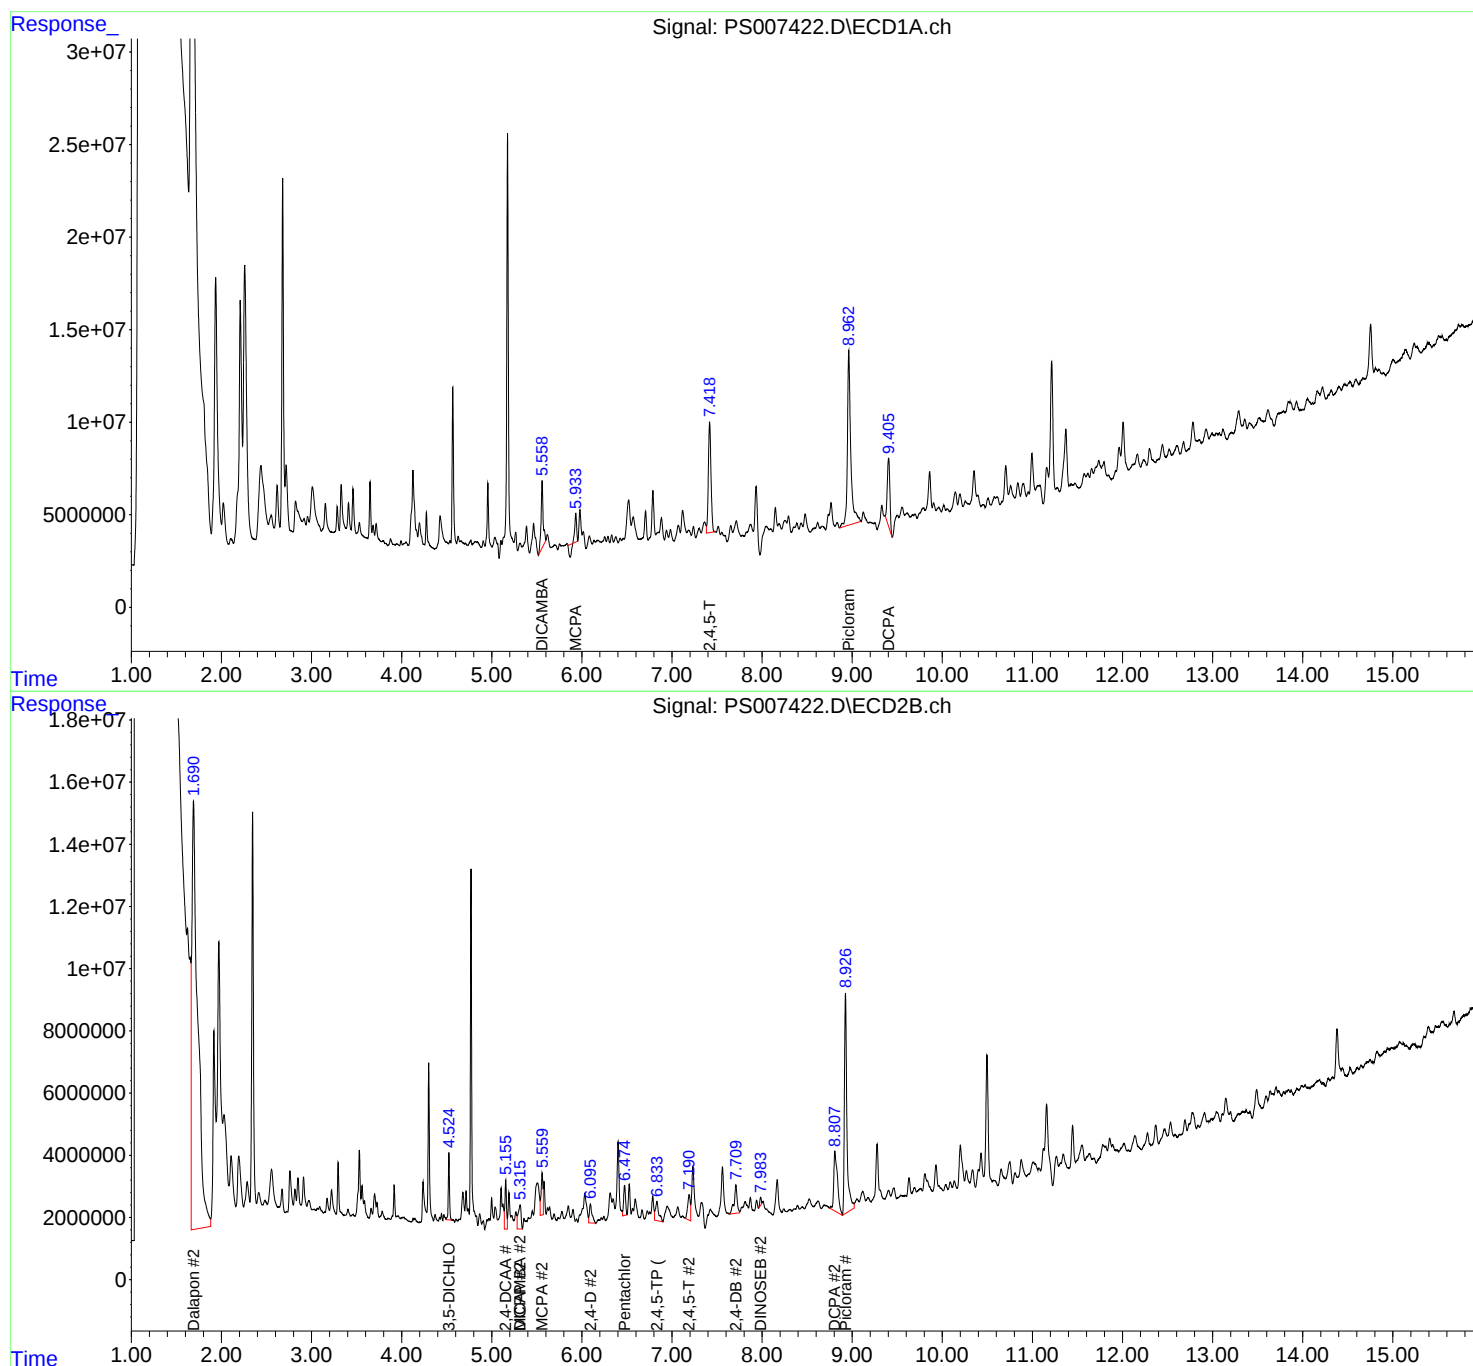


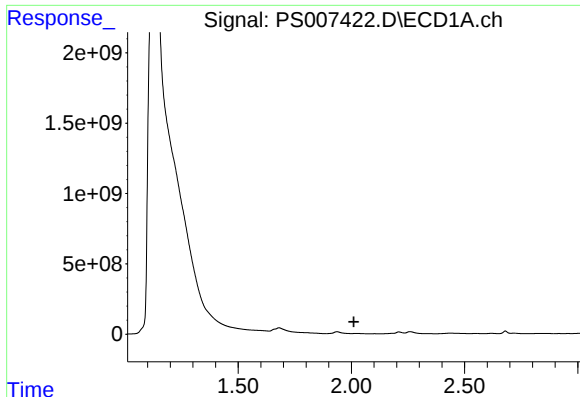

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

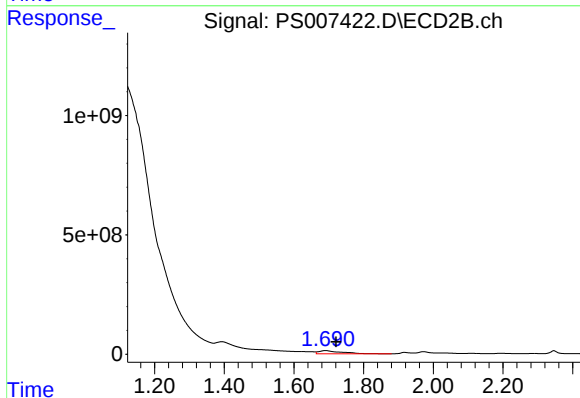


#1 Dalapon

R.T.: 1.690 min
Delta R.T.: -0.030 min
Response: 631134934
Conc: 693.55 ng/ml

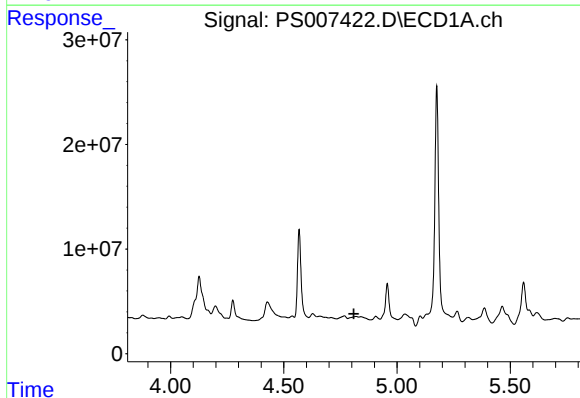


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

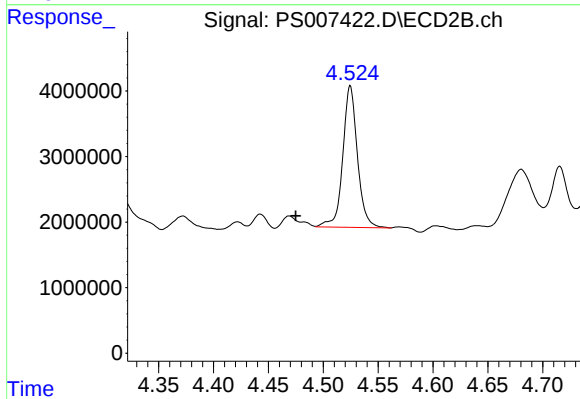

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.525 min
Delta R.T.: 0.050 min
Response: 20083702
Conc: 23.34 ng/ml

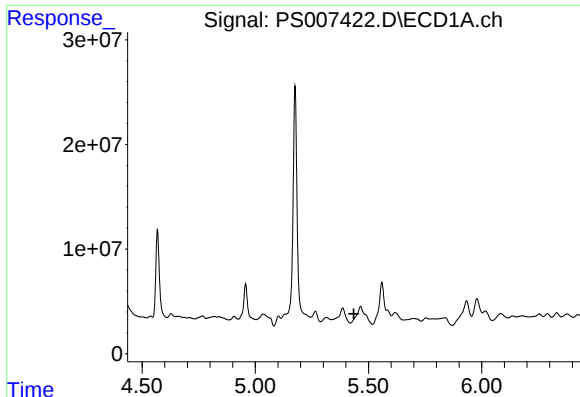

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

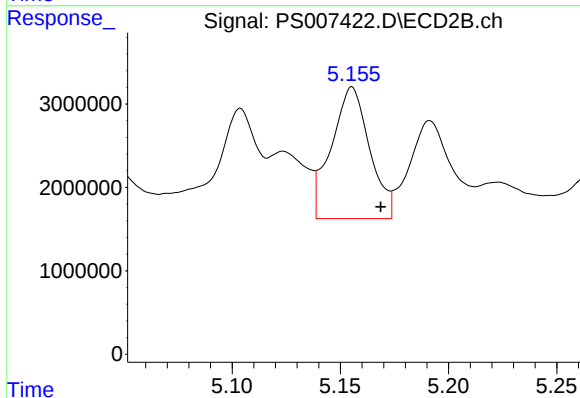


#4 2,4-DCAA

R.T.: 5.155 min
Delta R.T.: -0.013 min
Response: 19419705
Conc: 27.61 ng/ml

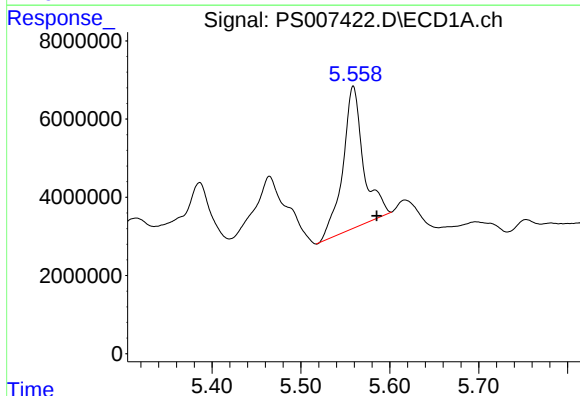


#5 DICAMBA

R.T.: 5.559 min
Delta R.T.: -0.026 min
Response: 58662935
Conc: 11.94 ng/ml

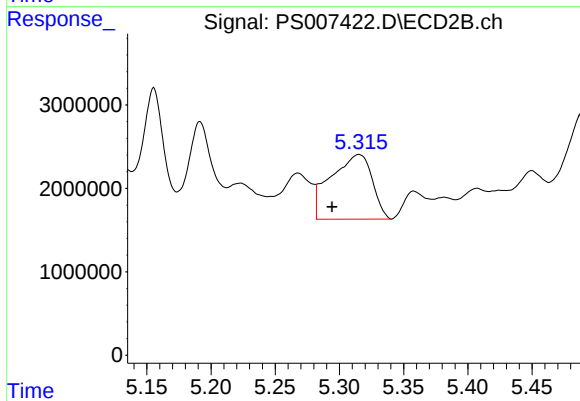

#5 DICAMBA


R.T.: 5.315 min
Delta R.T.: 0.021 min
Response: 17351817
Conc: 6.67 ng/ml

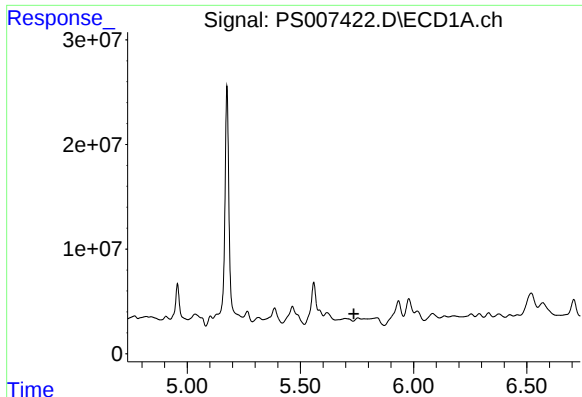

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

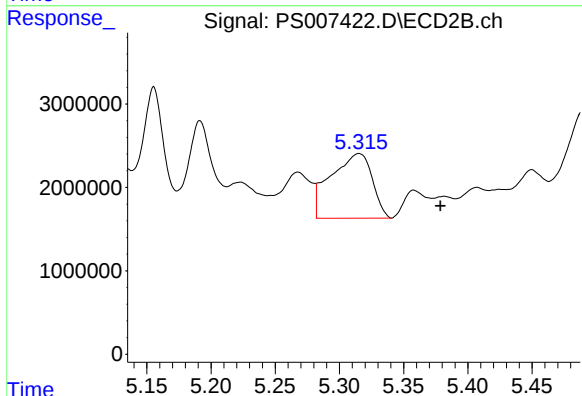


#6 MCPP

R.T.: 5.315 min
Delta R.T.: -0.064 min
Response: 17351817
Conc: 9.15 ug/ml

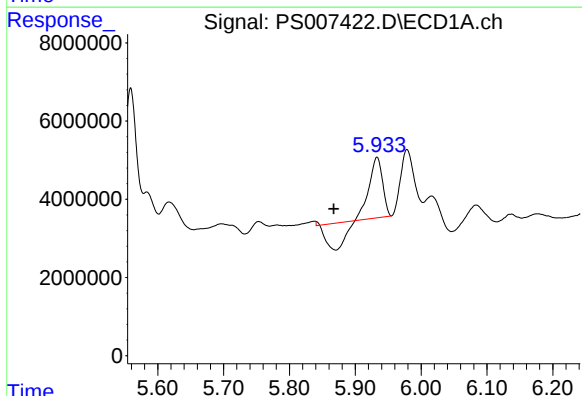


#7 MCPA

R.T.: 5.933 min
Delta R.T.: 0.066 min
Response: 10579166
Conc: 2.05 ug/ml

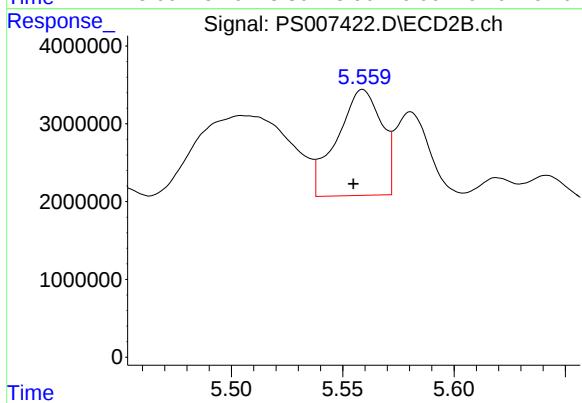

#7 MCPA


R.T.: 5.559 min
Delta R.T.: 0.004 min
Response: 19013384
Conc: 6.54 ug/ml

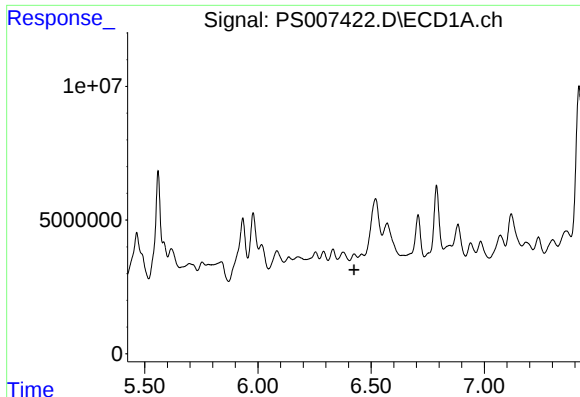

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

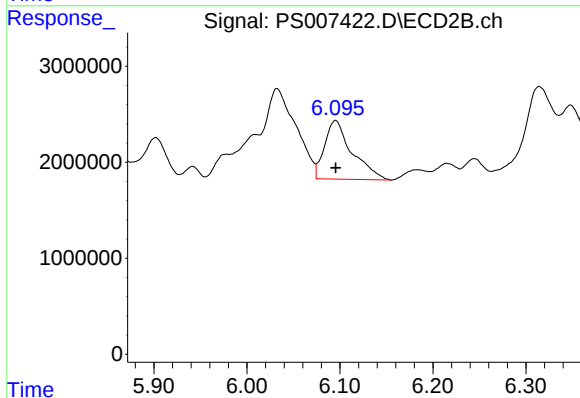


#9 2,4-D

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 12596277
Conc: 15.79 ng/ml

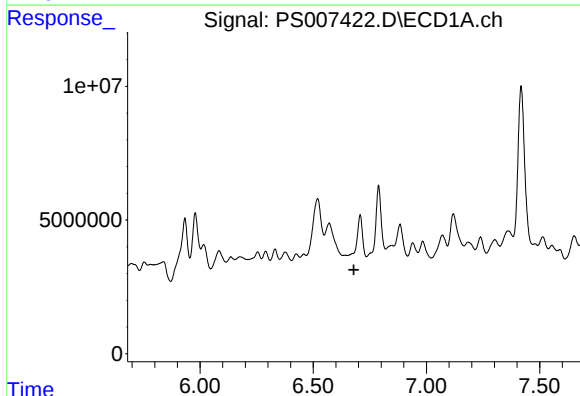


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

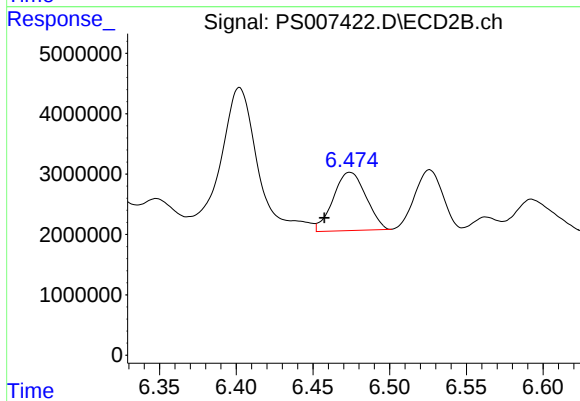

#10 Pentachlorophenol


R.T.: 6.474 min
Delta R.T.: 0.017 min
Response: 14345089
Conc: 1.49 ng/ml

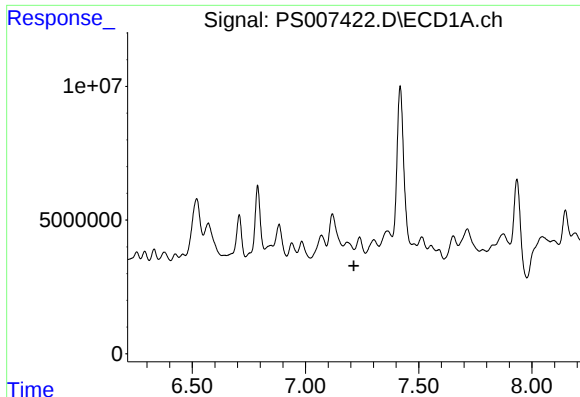

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

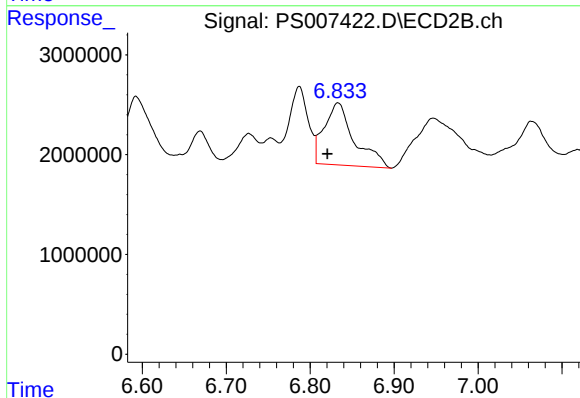


#11 2,4,5-TP (SILVEX)

R.T.: 6.833 min
Delta R.T.: 0.013 min
Response: 15421761
Conc: 4.05 ng/ml

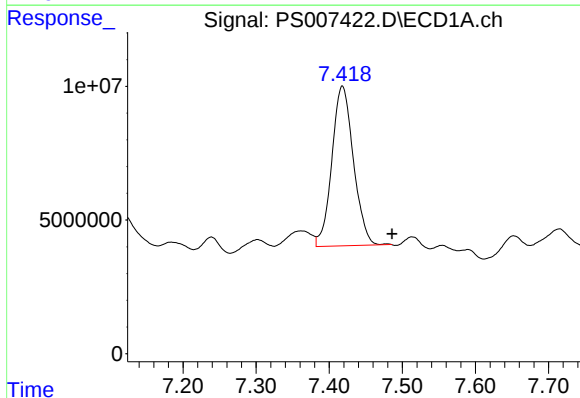


#12 2,4,5-T

R.T.: 7.418 min
Delta R.T.: -0.068 min
Response: 122248649
Conc: 15.99 ng/ml

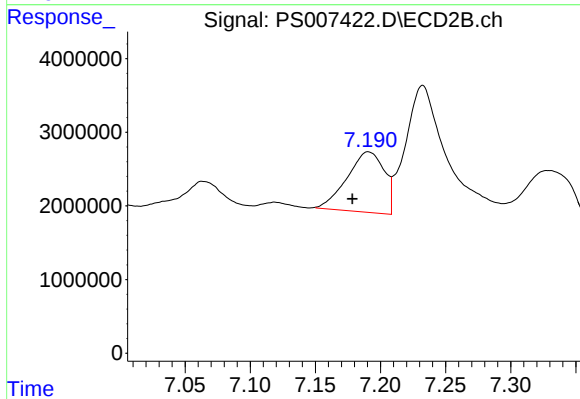

#12 2,4,5-T


R.T.: 7.191 min
Delta R.T.: 0.013 min
Response: 16321304
Conc: 4.66 ng/ml

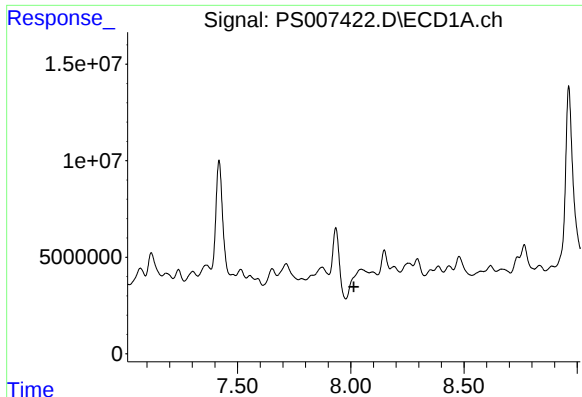

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

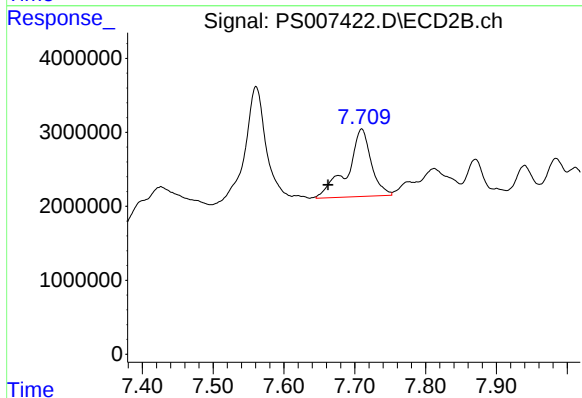


#13 2,4-DB

R.T.: 7.710 min
Delta R.T.: 0.047 min
Response: 21224375
Conc: 45.28 ng/ml

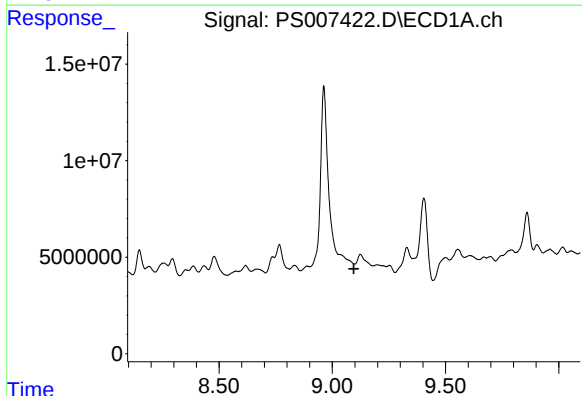


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

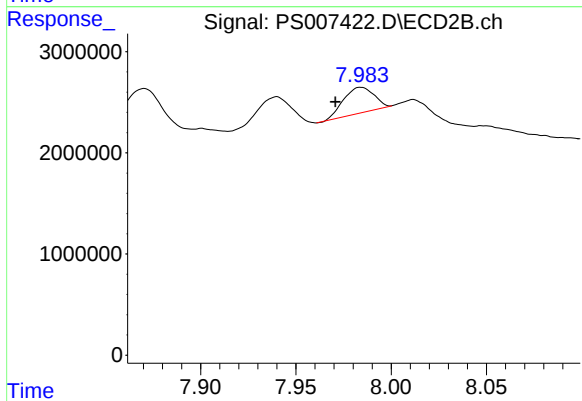

#14 DINOSEB


R.T.: 7.984 min
Delta R.T.: 0.014 min
Response: 2816946
Conc: 1.00 ng/ml

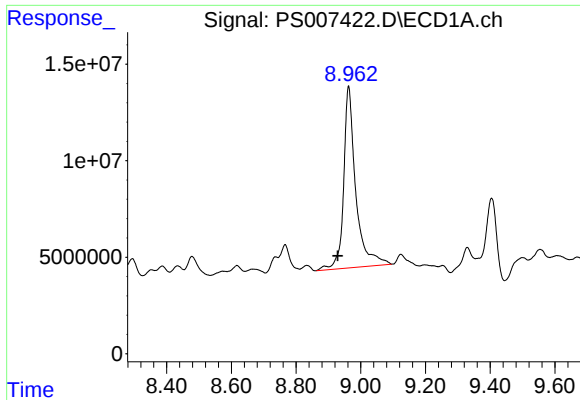

#15 Picloram


R.T.: 8.962 min
Delta R.T.: 0.033 min
Response: 244563050
Conc: 22.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

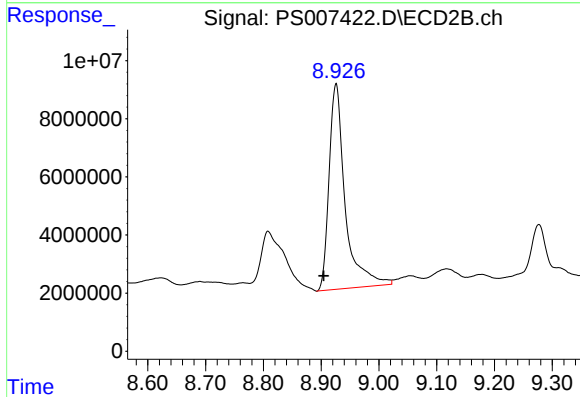


#15 Picloram

R.T.: 8.926 min
Delta R.T.: 0.021 min
Response: 137732908
Conc: 22.43 ng/ml

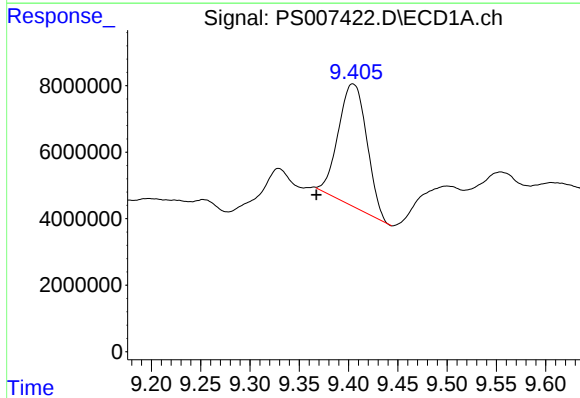

#16 DCPA

R.T.: 9.404 min
Delta R.T.: 0.037 min
Response: 74021103
Conc: 8.27 ng/ml

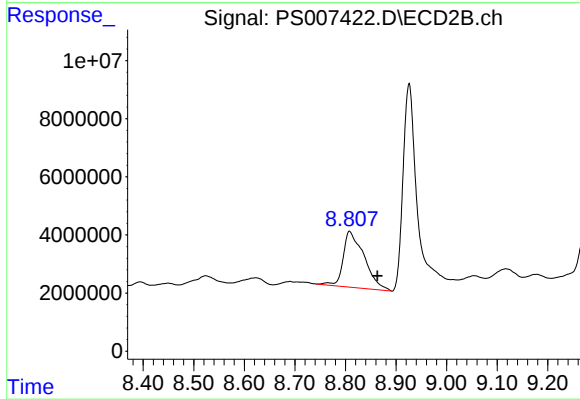

#16 DCPA

R.T.: 8.808 min
Delta R.T.: -0.055 min
Response: 55617960
Conc: 11.09 ng/ml