

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
 Data File : PS013016.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 12:27
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 03:02:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	0.000	6.010	0	308449	N.D. <MDL
6) T	MCCP	7.625	0.000	13026662	0	4.891 N.D. #
15) T	Picloram	0.000	11.056	0	6077837	N.D. 1.688



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
Data File : PS013016.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 12:27
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 03:02:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

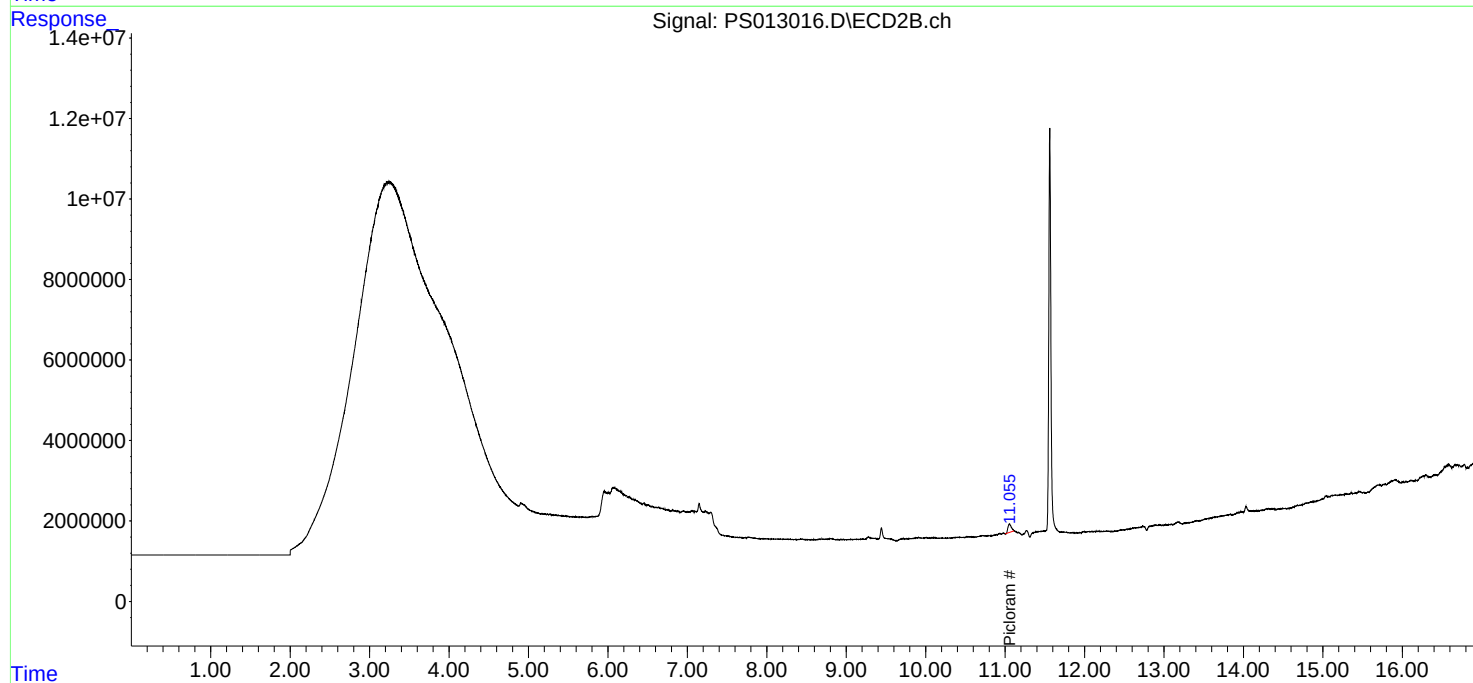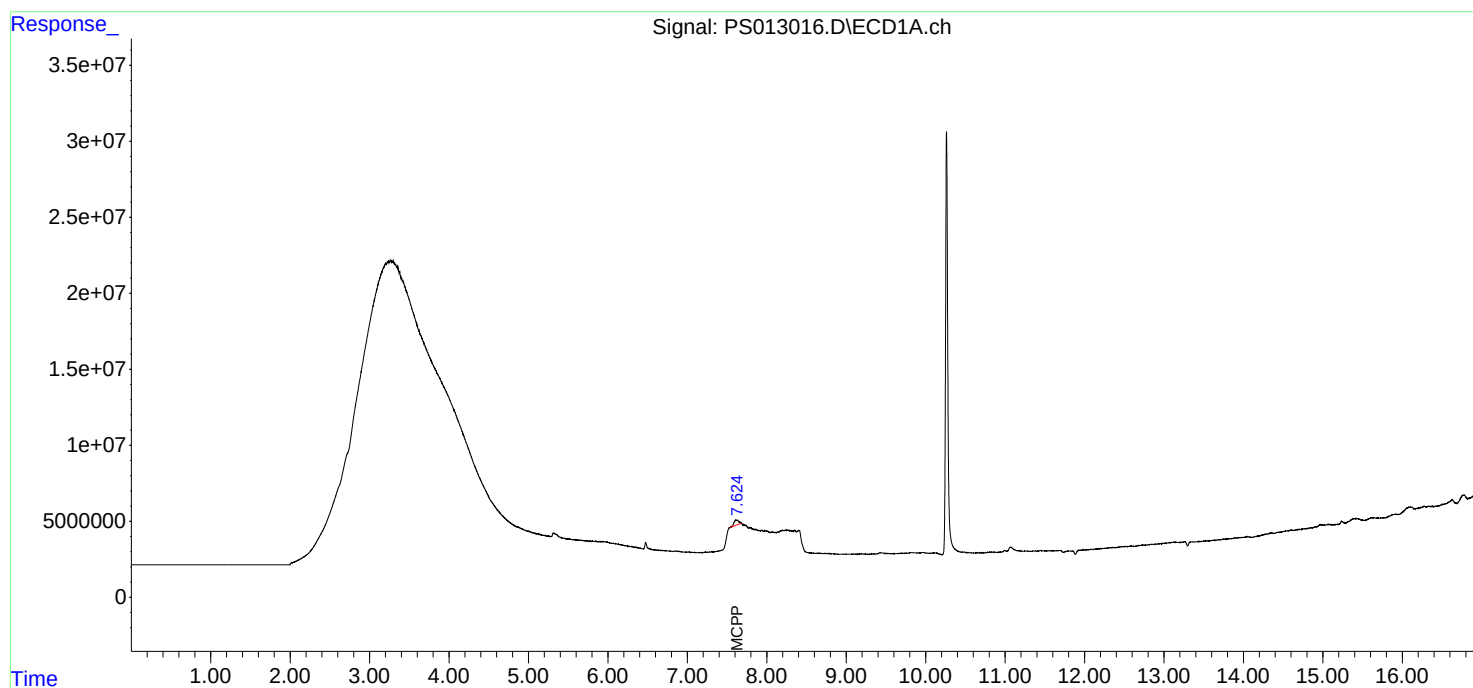


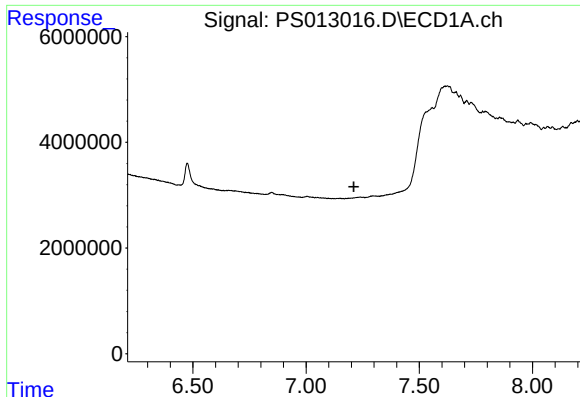

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

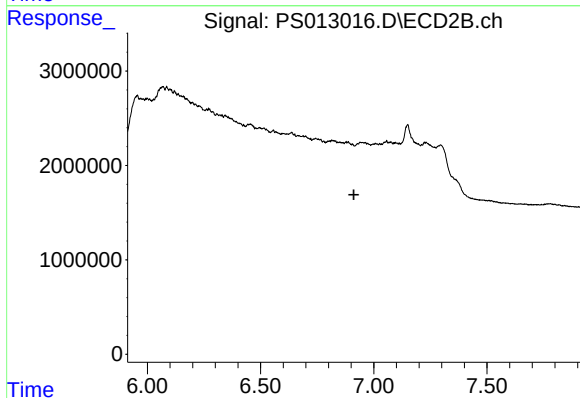


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.912 min
Response: 0
Conc: N.D.

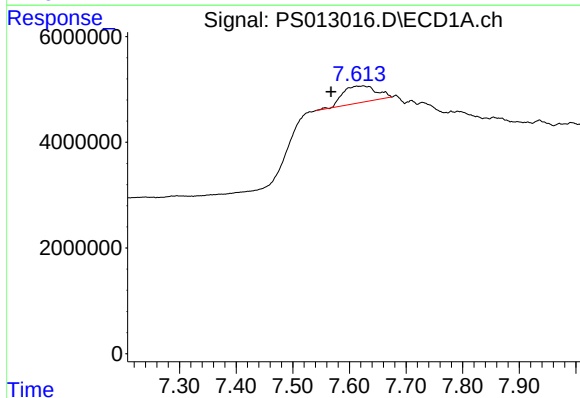


#6 MCPP

R.T.: 7.625 min
Delta R.T.: 0.057 min
Response: 13026662
Conc: 4.89 ug/ml

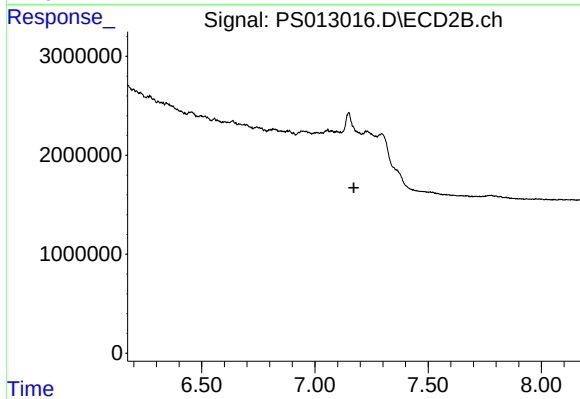

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.172 min
Response: 0
Conc: N.D.

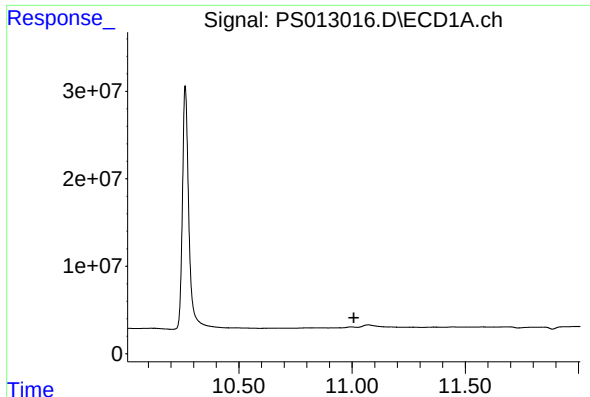

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

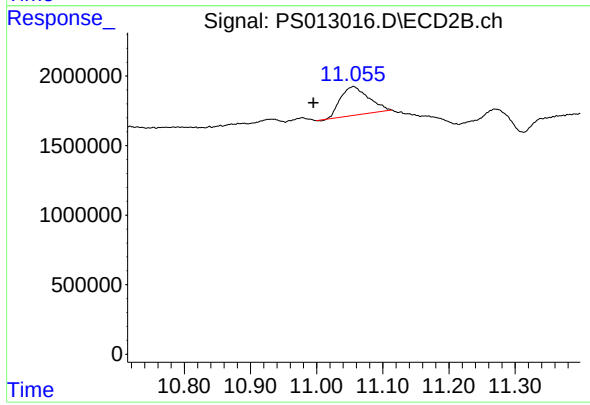

#15 Picloram

R.T.: 11.056 min
Delta R.T.: 0.060 min
Response: 6077837
Conc: 1.69 ng/ml