

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
 Data File : PS013021.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 18:11
 Operator : DD\AJ
 Sample : PB132683TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 03:04:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.916	307.5E6	161.2E6	343.519	401.629
Target Compounds							
1) T	Dalapon	2.992	2.590	67968675	109.4E6	66.860	208.079 #
2) T	3,5-DICHL...	0.000	6.045	0	2783536	N.D.	4.418
3) T	4-Nitroph...	6.982	0.000	2542952	0	6.080	N.D. #
5) T	DICAMBA	7.388	7.048	13013093	3729097	3.655	2.191 #
7) T	MCPA	7.732	0.000	55607864	0	14.523	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	10608769	N.D.	23.094
9) T	2,4-D	8.389	0.000	73912554	0	71.634	N.D. #
10) T	Pentachlo...	8.685	8.428	8492561	4855149	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.742	0	45770335	N.D.	19.307
12) T	2,4,5-T	9.399	0.000	83493098	0	15.944	N.D. #
15) T	Picloram	0.000	11.041	0	5412906	N.D.	1.504
16) T	DCPA	0.000	10.934	0	6227424	N.D.	2.044



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
Data File : PS013021.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 18:11
Operator : DD\AJ
Sample : PB132683TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 03:04:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

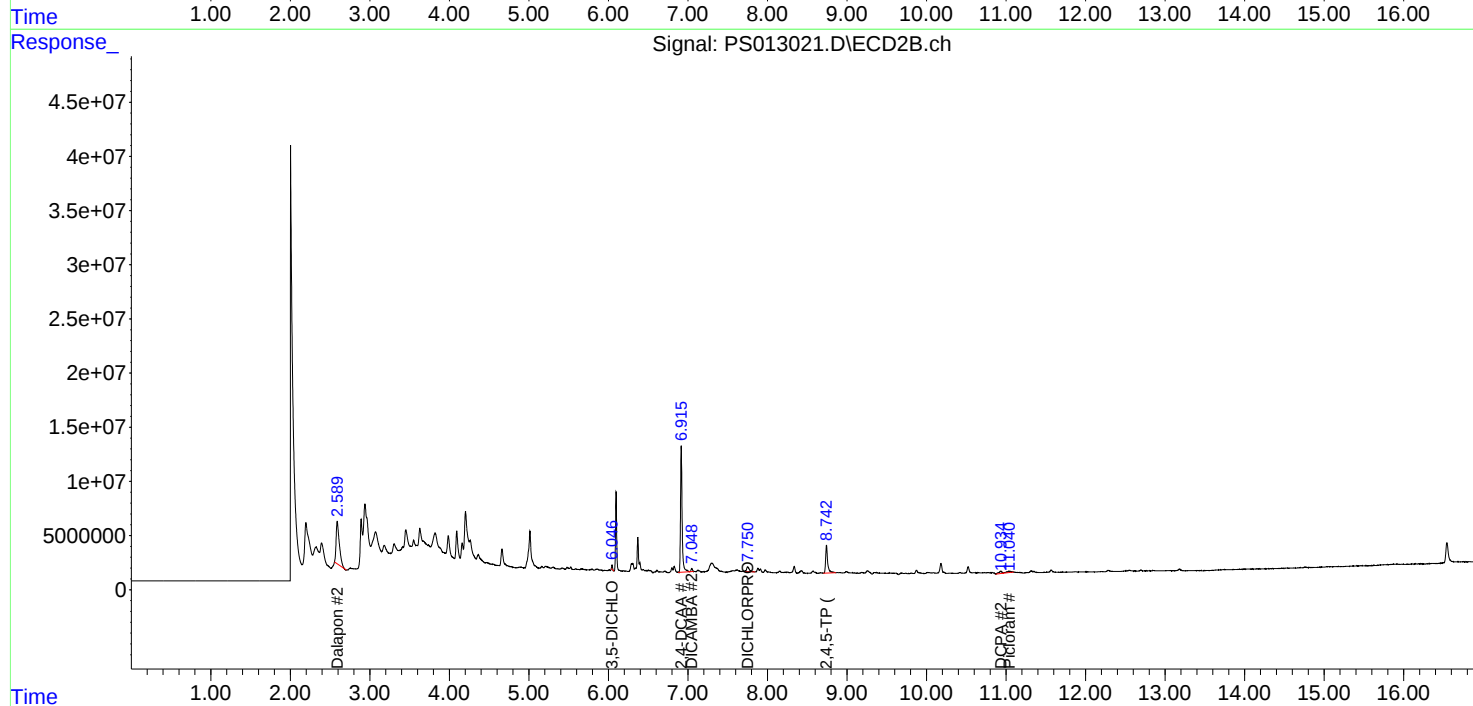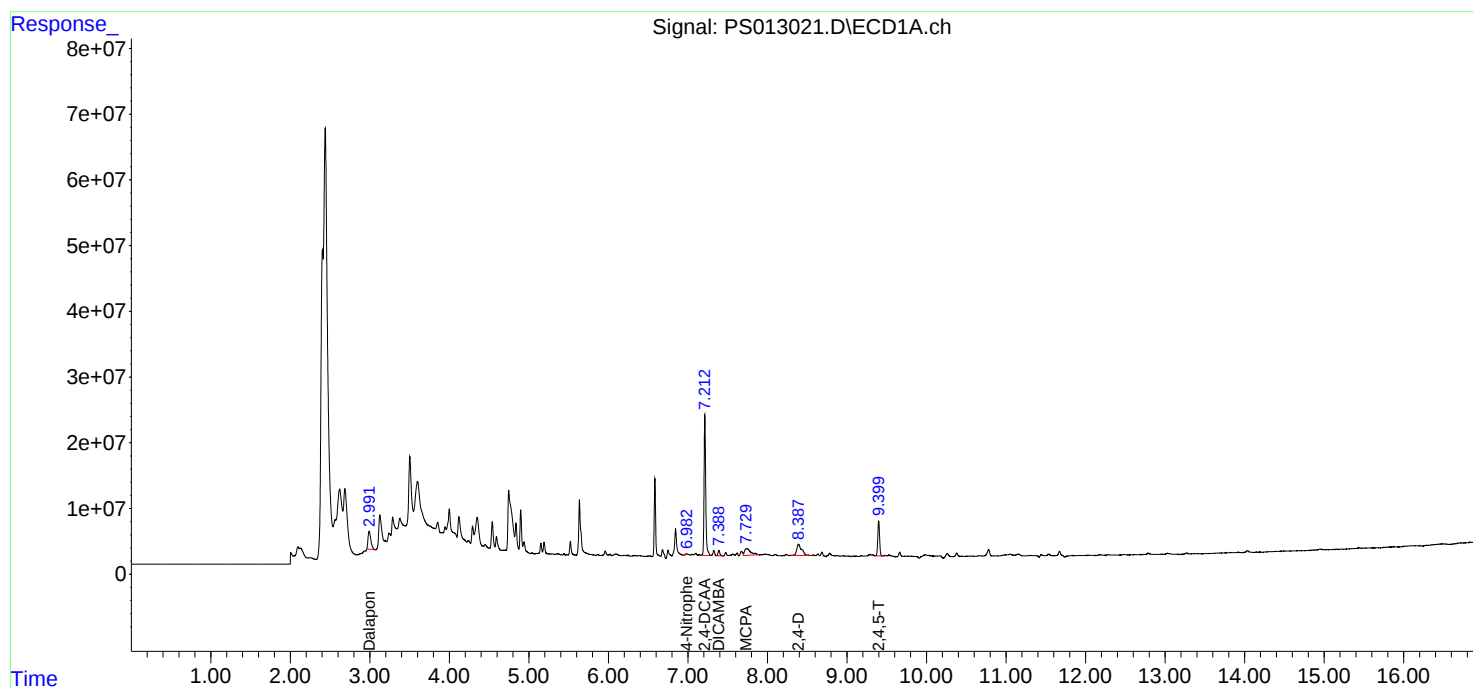


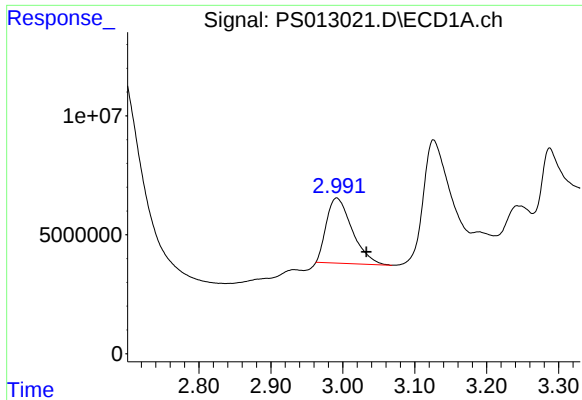

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.041 min
Response: 67968675
Conc: 66.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

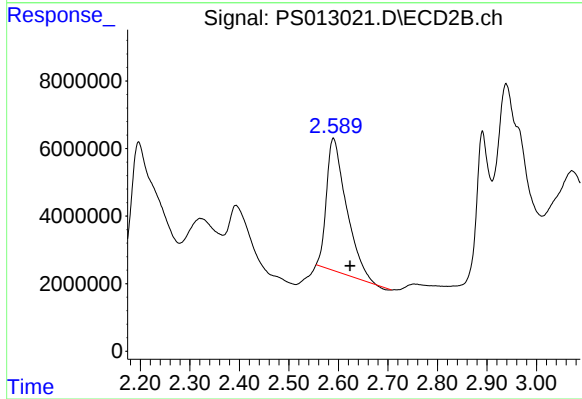


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.034 min
Response: 109423639
Conc: 208.08 ng/ml

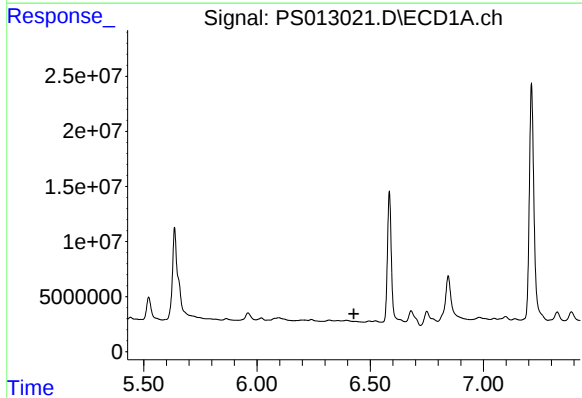


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

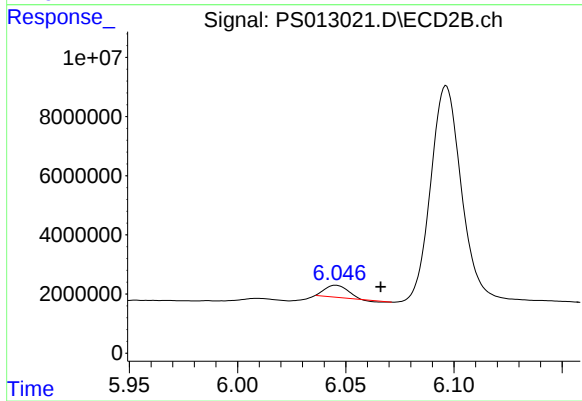

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.045 min
Delta R.T.: -0.021 min
Response: 2783536
Conc: 4.42 ng/ml

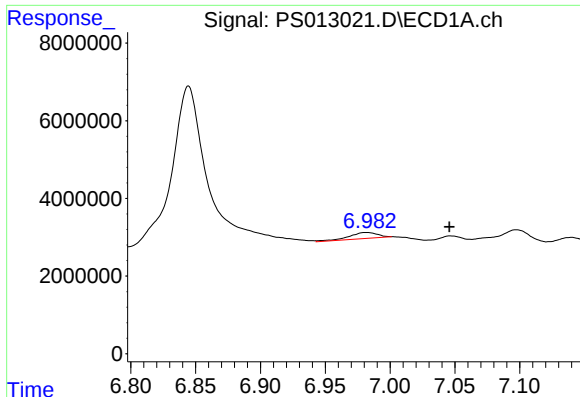

#3 4-Nitrophenol


R.T.: 6.982 min
Delta R.T.: -0.064 min
Response: 2542952
Conc: 6.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

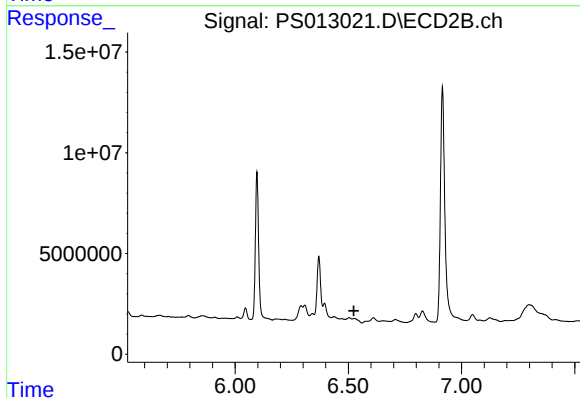


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

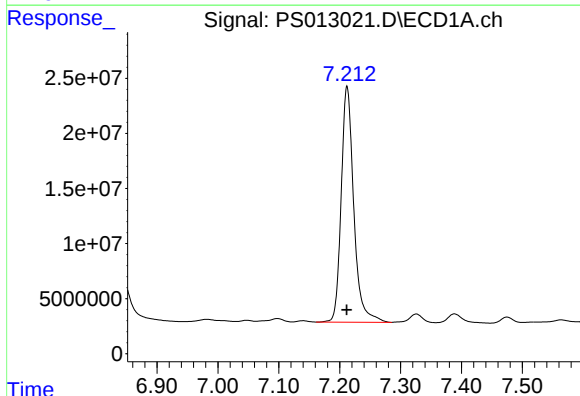


#4 2,4-DCAA

R.T.: 7.212 min
Delta R.T.: 0.000 min
Response: 307473146
Conc: 343.52 ng/ml

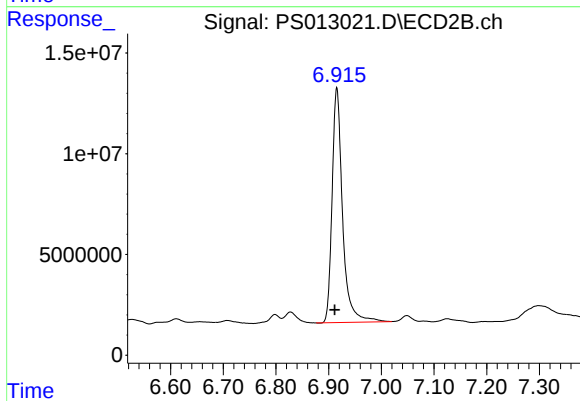

#4 2,4-DCAA


R.T.: 6.916 min
Delta R.T.: 0.004 min
Response: 161154179
Conc: 401.63 ng/ml

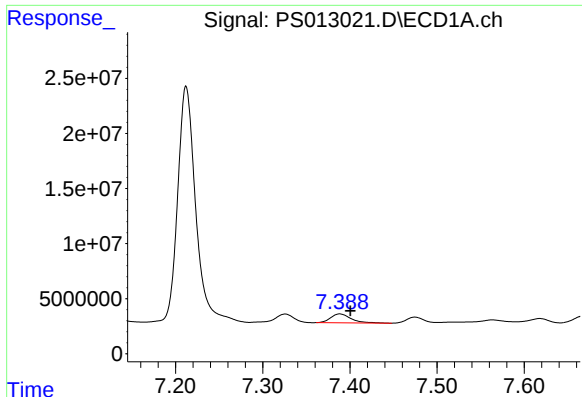

#5 DICAMBA


R.T.: 7.388 min
Delta R.T.: -0.012 min
Response: 13013093
Conc: 3.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

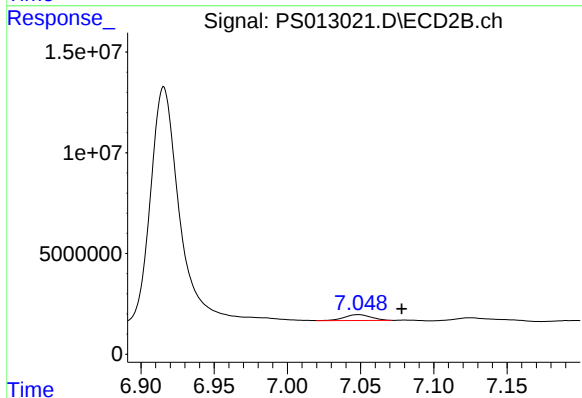


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.030 min
Response: 3729097
Conc: 2.19 ng/ml

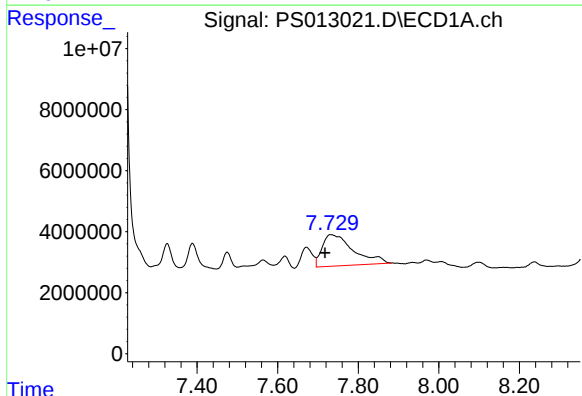


#7 MCPA

R.T.: 7.732 min
Delta R.T.: 0.015 min
Response: 55607864
Conc: 14.52 ug/ml

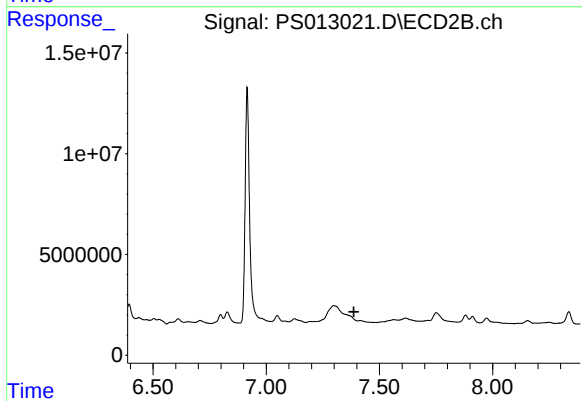

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

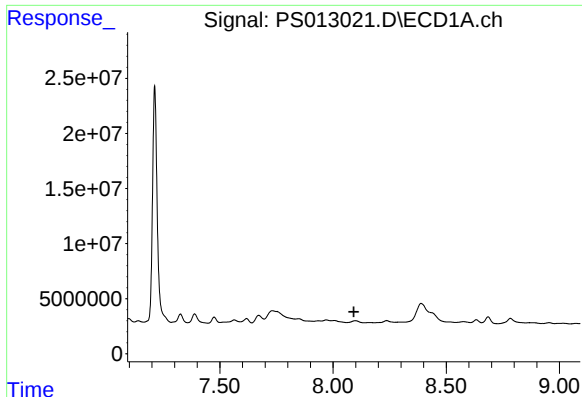

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

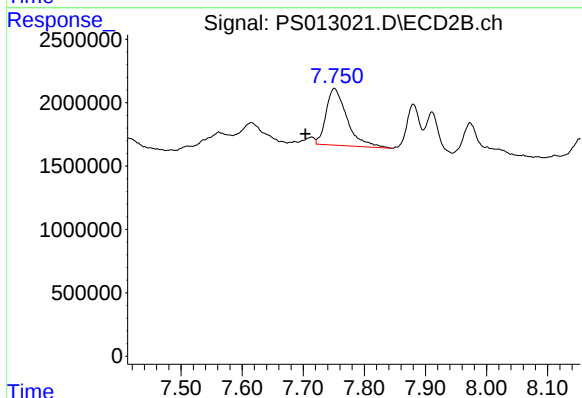


#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.048 min
Response: 10608769
Conc: 23.09 ng/ml

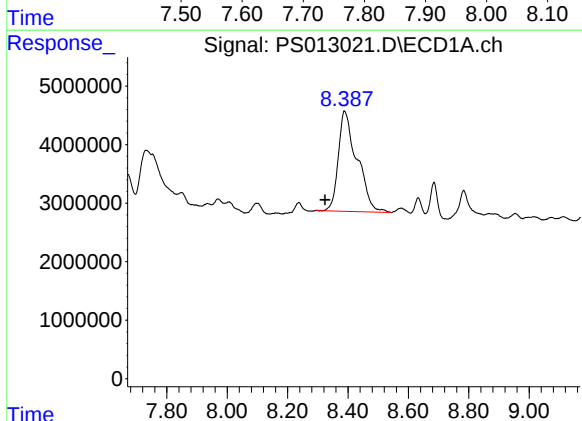


#9 2,4-D

R.T.: 8.389 min
Delta R.T.: 0.064 min
Response: 73912554
Conc: 71.63 ng/ml

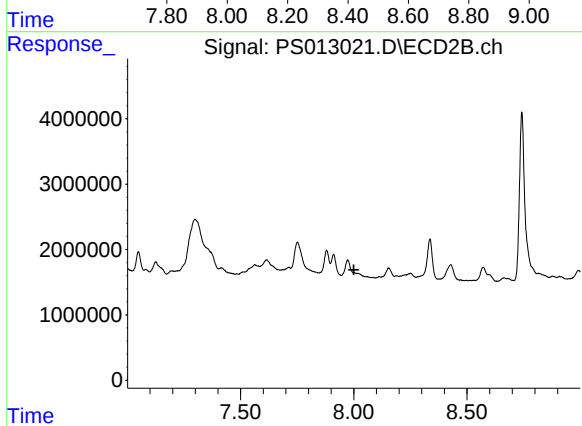

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

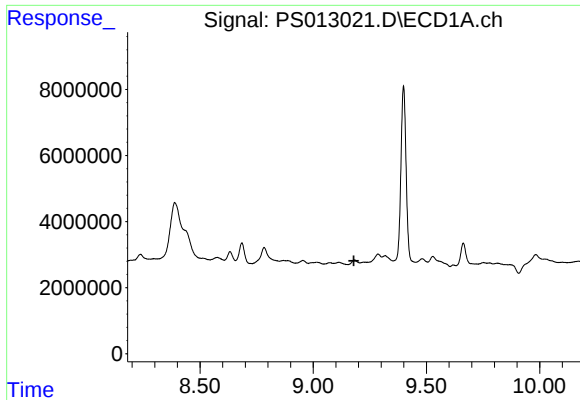

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

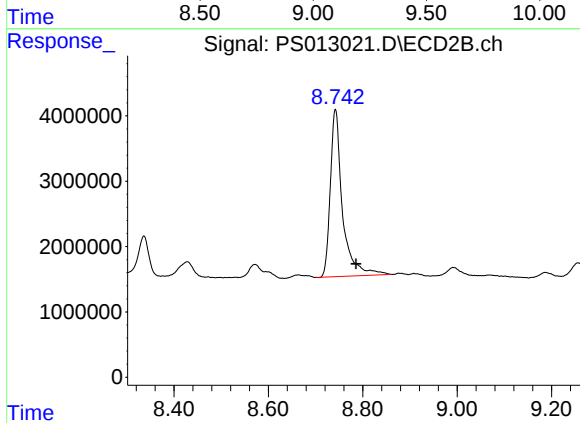


#11 2,4,5-TP (SILVEX)

R.T.: 8.742 min
Delta R.T.: -0.044 min
Response: 45770335
Conc: 19.31 ng/ml

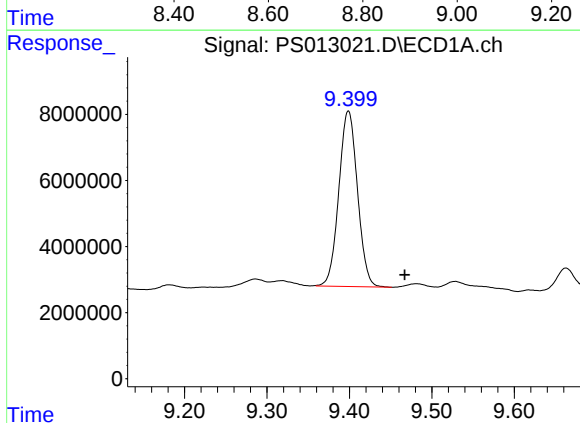


#12 2,4,5-T

R.T.: 9.399 min
Delta R.T.: -0.068 min
Response: 83493098
Conc: 15.94 ng/ml

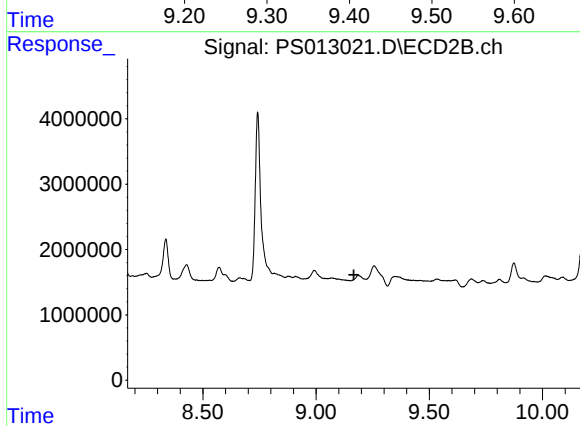

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.167 min
Response: 0
Conc: N.D.

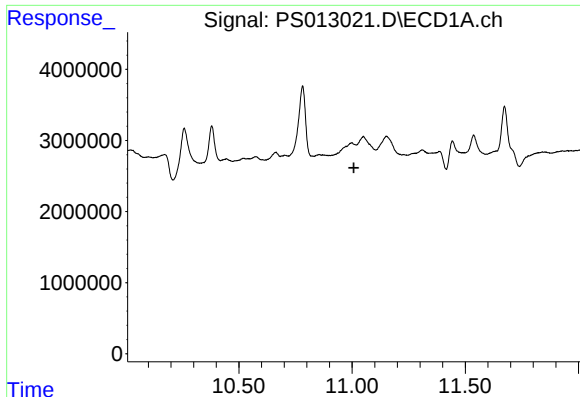

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.008 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

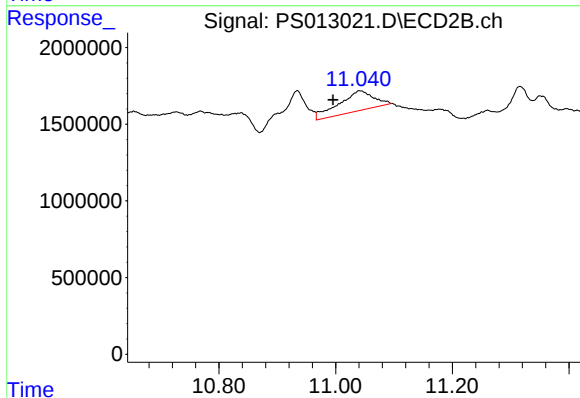


#15 Picloram

R.T.: 11.041 min
Delta R.T.: 0.046 min
Response: 5412906
Conc: 1.50 ng/ml

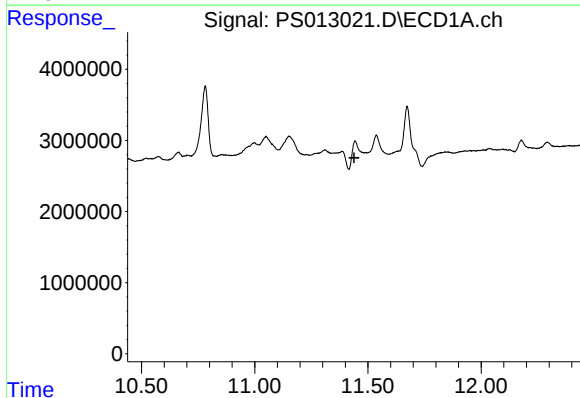

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.438 min
Response: 0
Conc: N.D.

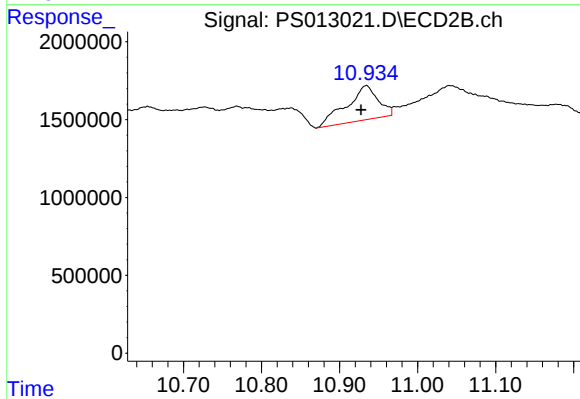

#16 DCPA

R.T.: 10.934 min
Delta R.T.: 0.007 min
Response: 6227424
Conc: 2.04 ng/ml