

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
 Data File : PS013022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2020 18:34
 Operator : DD\AJ
 Sample : L4224-15
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 03:04:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.915	295.0E6	156.0E6	329.538	388.661
Target Compounds							
1) T	Dalapon	2.993	2.591	69620243	122.6E6	68.485	233.191 #
2) T	3,5-DICHL...	0.000	6.046	0	3931660	N.D.	6.240
3) T	4-Nitroph...	6.982	0.000	2959556	0	7.077	N.D. #
5) T	DICAMBA	7.388	7.048	11094233	5517291	3.116	3.242
7) T	MCPA	7.726	0.000	45285117	0	11.827	N.D. #
8) T	DICHLORPROP	0.000	7.750	0	9911965	N.D.	21.577
9) T	2,4-D	8.389	0.000	72273544	0	70.046	N.D. #
10) T	Pentachlo...	8.684	0.000	8236624	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.741	0	41229449	N.D.	17.392
12) T	2,4,5-T	9.398	0.000	85939176	0	16.412	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102820\
Data File : PS013022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2020 18:34
Operator : DD\AJ
Sample : L4224-15
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 03:04:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

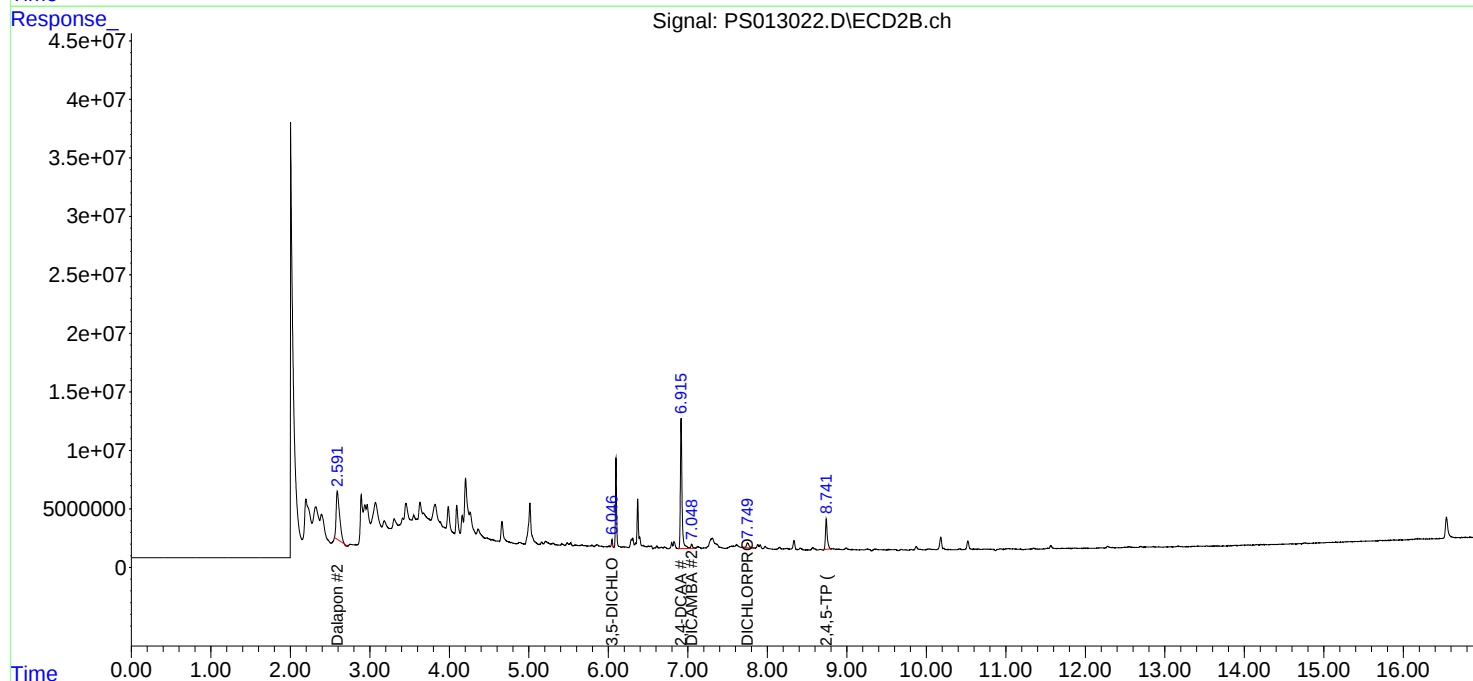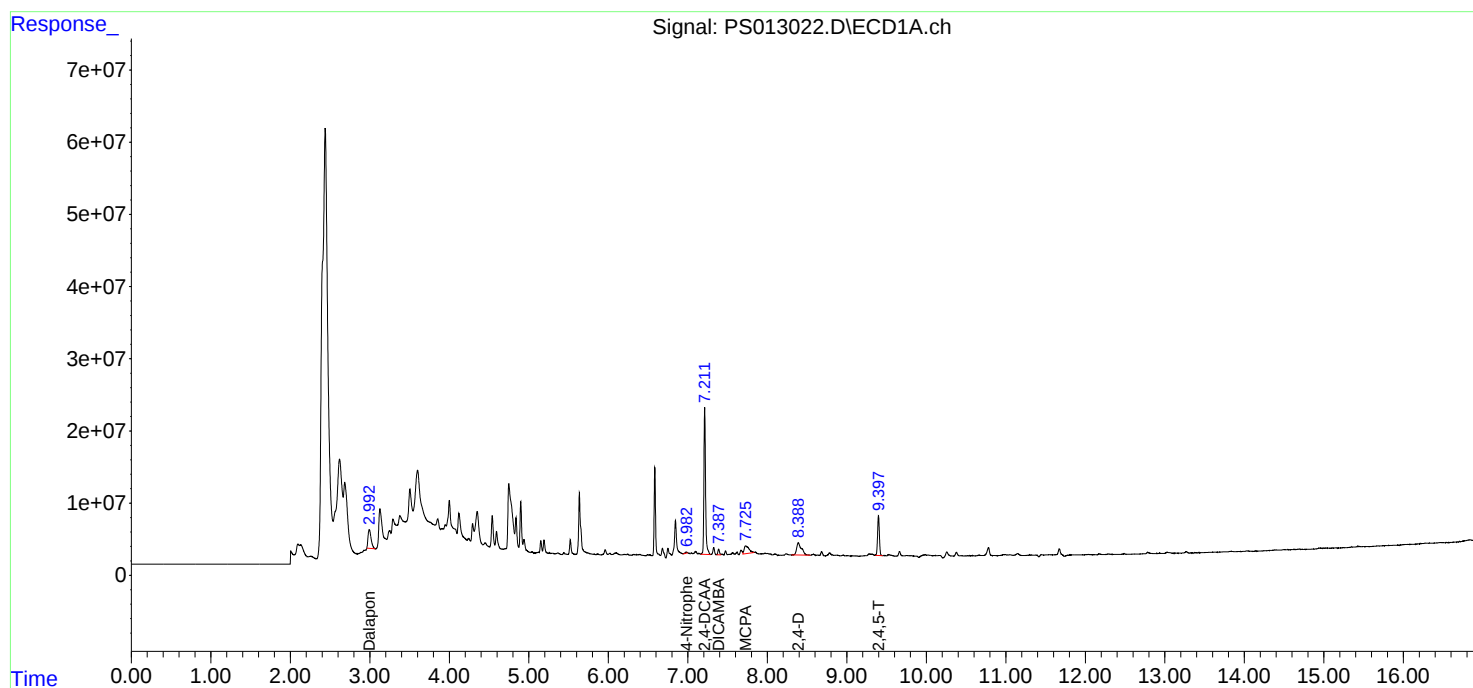


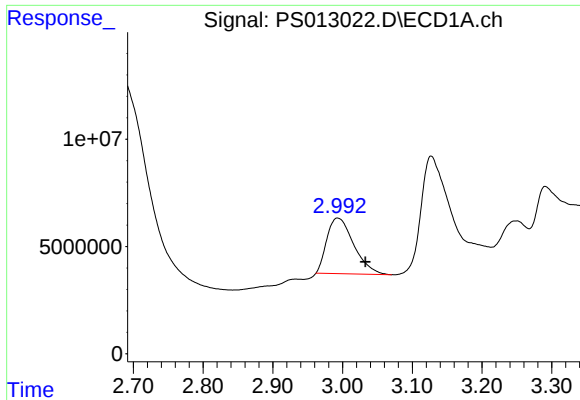

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.040 min
Response: 69620243
Conc: 68.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

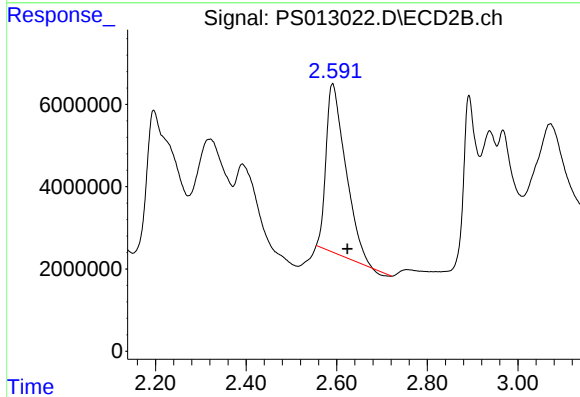


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.033 min
Response: 122629462
Conc: 233.19 ng/ml

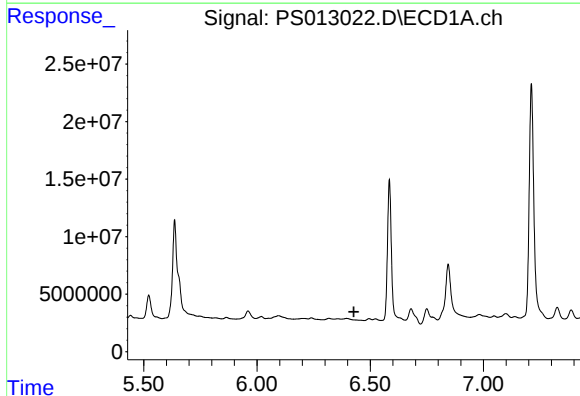


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

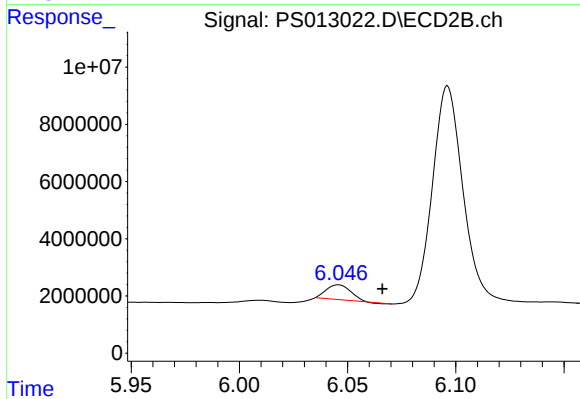

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.046 min
Delta R.T.: -0.020 min
Response: 3931660
Conc: 6.24 ng/ml

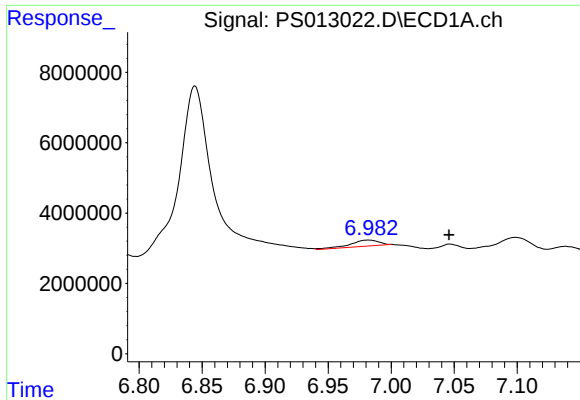

#3 4-Nitrophenol


R.T.: 6.982 min
Delta R.T.: -0.064 min
Response: 2959556
Conc: 7.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

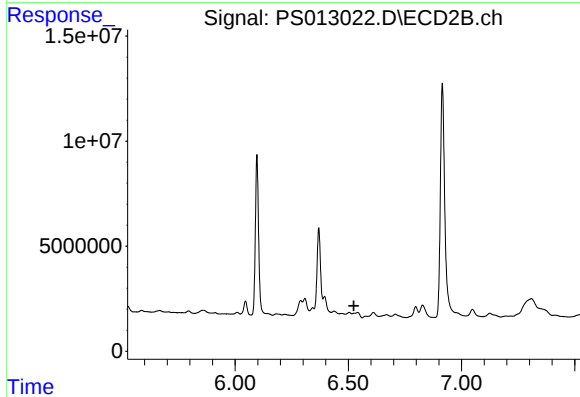


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

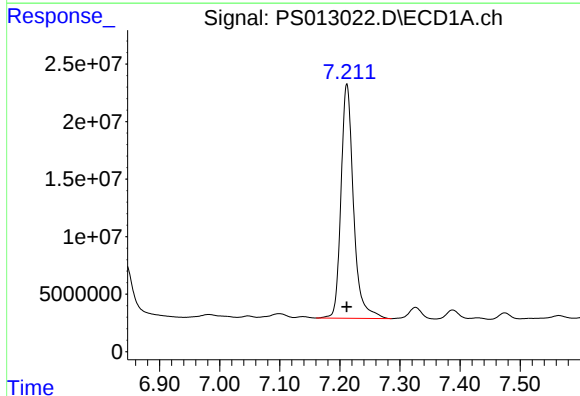


#4 2,4-DCAA

R.T.: 7.212 min
Delta R.T.: 0.000 min
Response: 294959522
Conc: 329.54 ng/ml

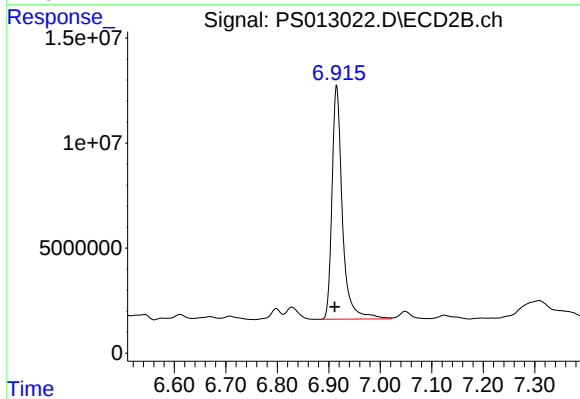

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.003 min
Response: 155950952
Conc: 388.66 ng/ml

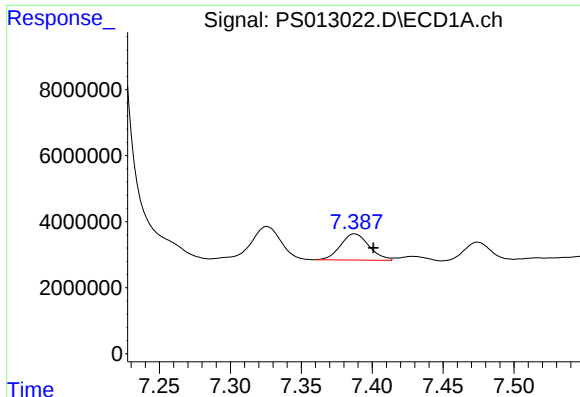

#5 DICAMBA


R.T.: 7.388 min
Delta R.T.: -0.013 min
Response: 11094233
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

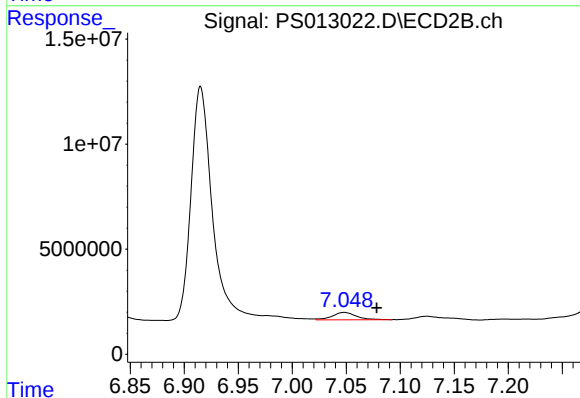


#5 DICAMBA

R.T.: 7.048 min
Delta R.T.: -0.030 min
Response: 5517291
Conc: 3.24 ng/ml

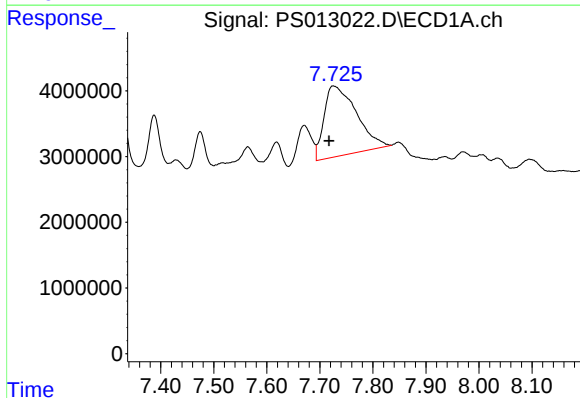


#7 MCPA

R.T.: 7.726 min
Delta R.T.: 0.009 min
Response: 45285117
Conc: 11.83 ug/ml

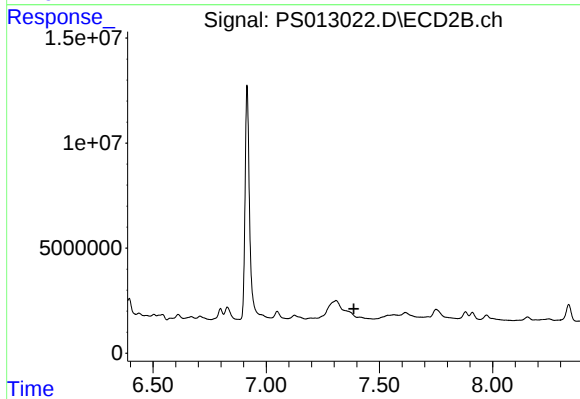

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

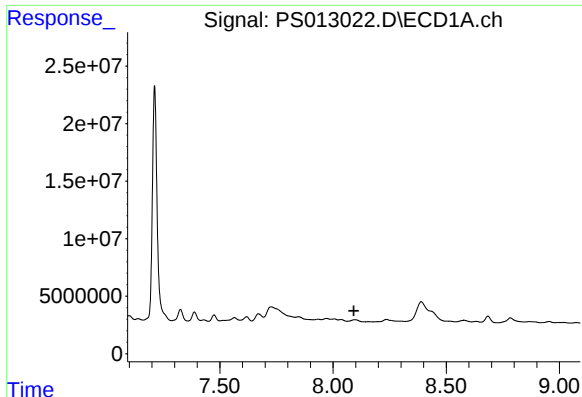

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

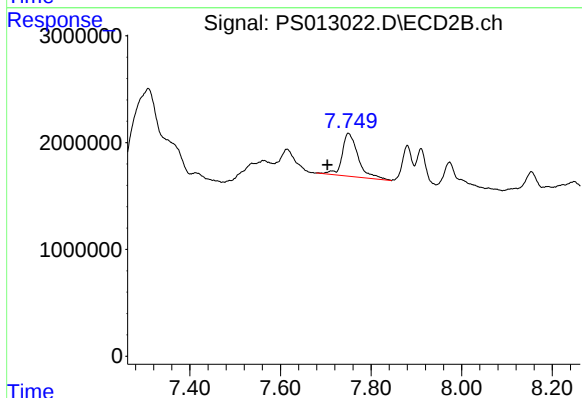


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.046 min
Response: 9911965
Conc: 21.58 ng/ml

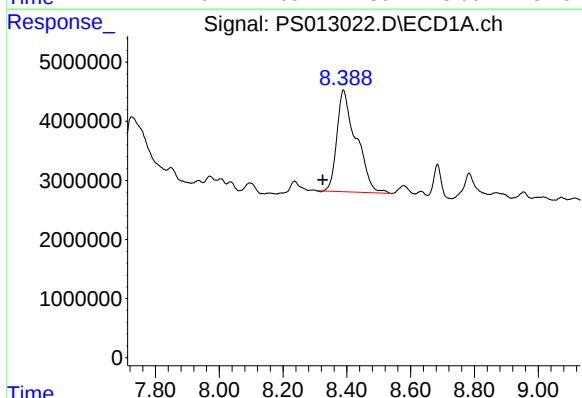


#9 2,4-D

R.T.: 8.389 min
Delta R.T.: 0.065 min
Response: 72273544
Conc: 70.05 ng/ml

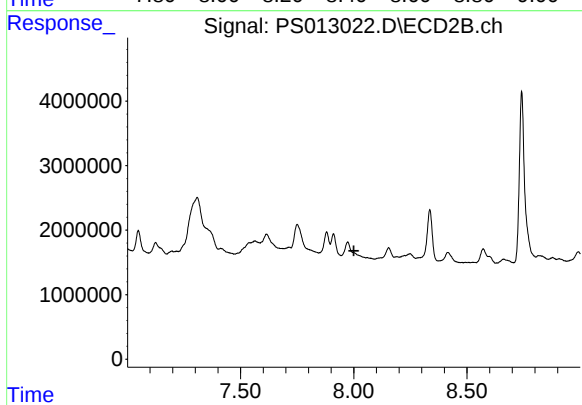

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

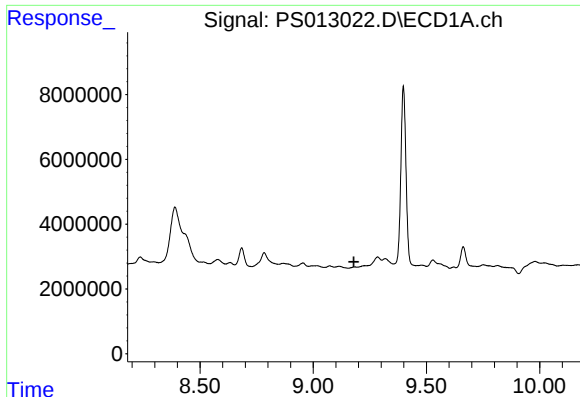

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.180 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

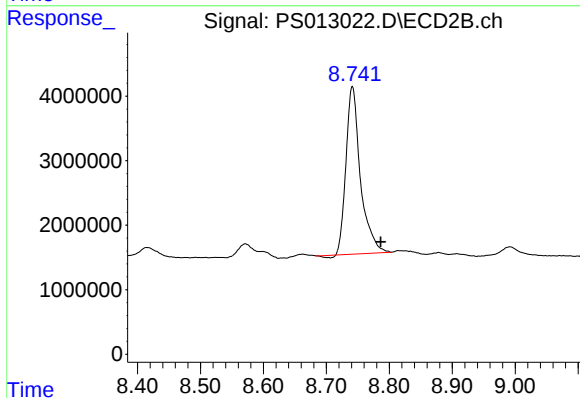


#11 2,4,5-TP (SILVEX)

R.T.: 8.741 min
Delta R.T.: -0.045 min
Response: 41229449
Conc: 17.39 ng/ml

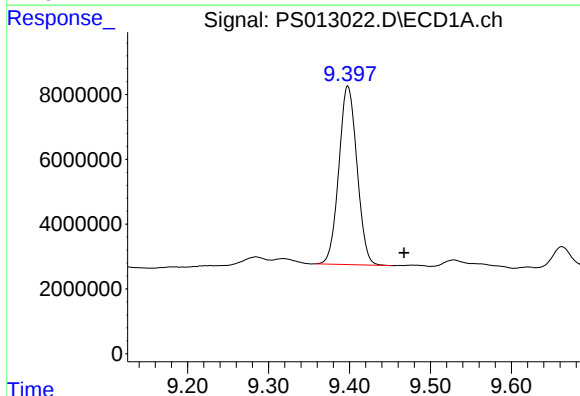

#12 2,4,5-T

R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 85939176
Conc: 16.41 ng/ml

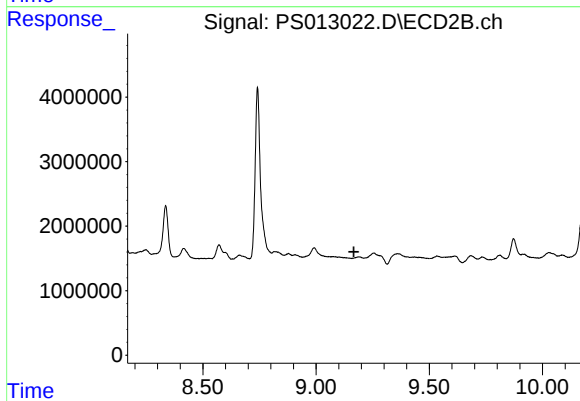

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.167 min
Response: 0
Conc: N.D.