

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102821\
 Data File : PS017248.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2021 10:16
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 28 22:51:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.168	0.000	18168209	0	11.887	N.D.	#
Target Compounds								
7) T	MCPA	7.605f	0.000	5527681	0	<MDL	N.D.	#
9) T	2,4-D	8.205f	0.000	41673319	0	23.528	N.D.	#
13) T	2,4-DB	9.885f	0.000	5628466	0	3.741	N.D.	#
15) T	Picloram	10.905	10.783	8563541	18202964	<MDL	4.753	#
16) T	DCPA	0.000	10.783f	0	18202964	N.D.	4.266	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102821\
Data File : PS017248.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2021 10:16
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 28 22:51:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

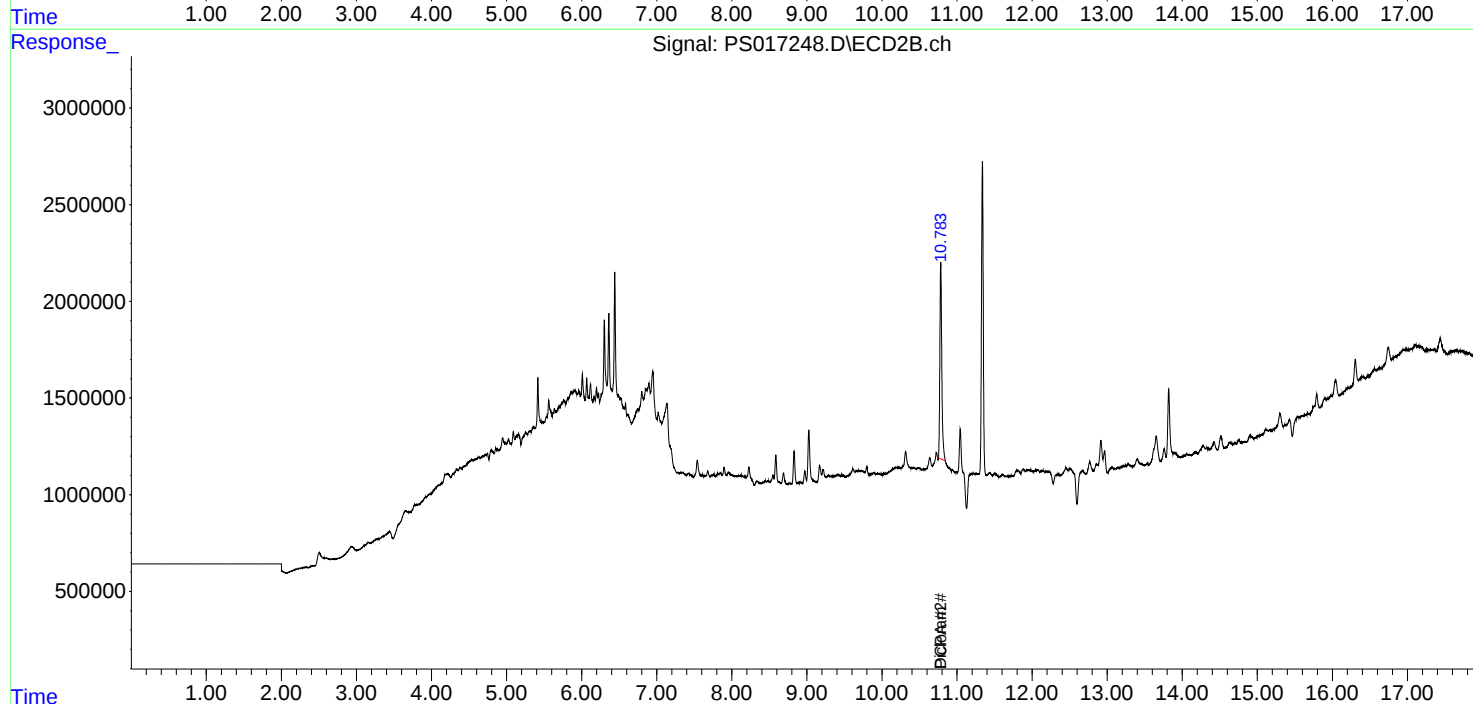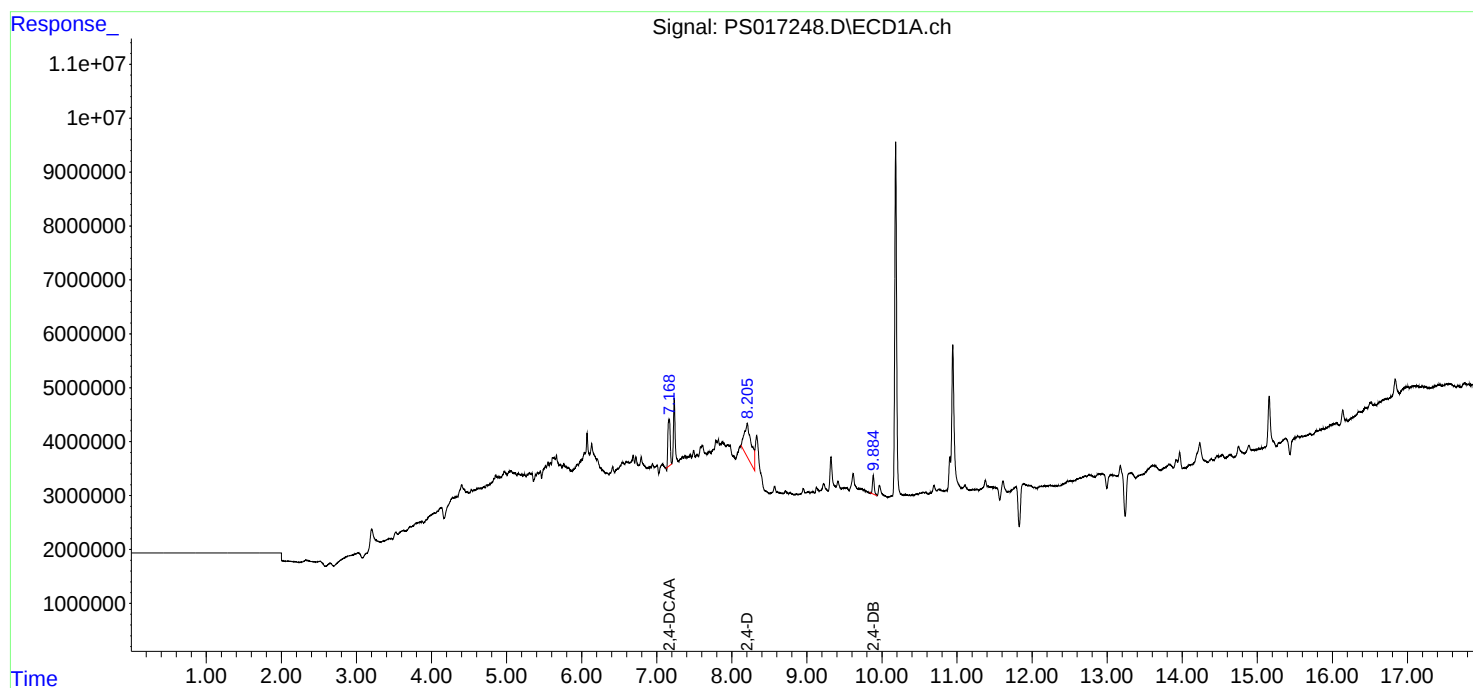


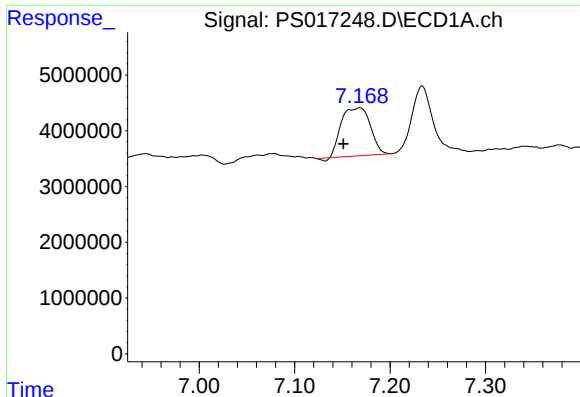

#4 2,4-DCAA


R.T.: 7.168 min
Delta R.T.: 0.017 min
Response: 18168209
Conc: 11.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

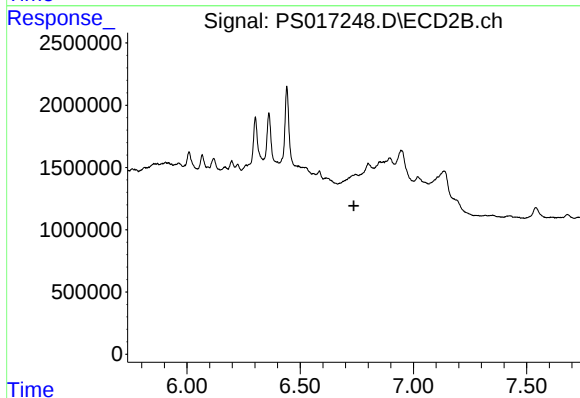


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

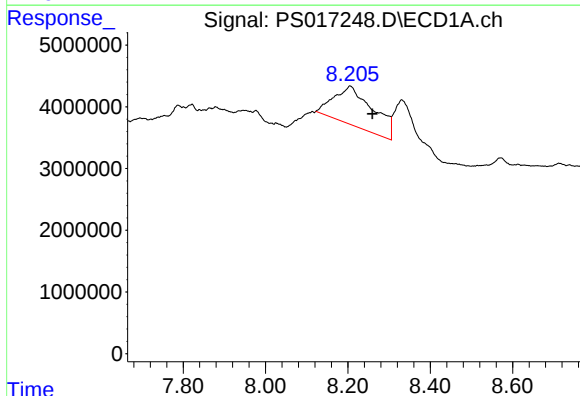


#9 2,4-D

R.T.: 8.205 min
Delta R.T.: -0.055 min
Response: 41673319
Conc: 23.53 ng/ml

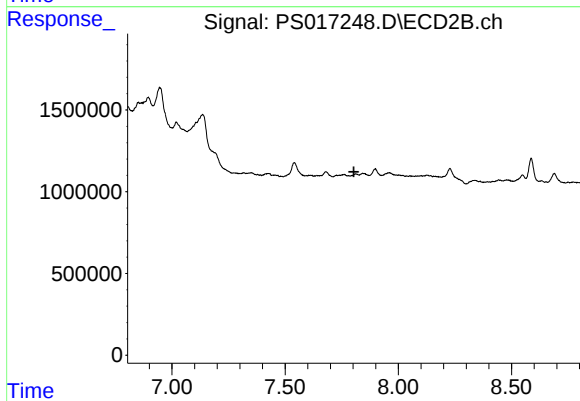

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.804 min
Response: 0
Conc: N.D.

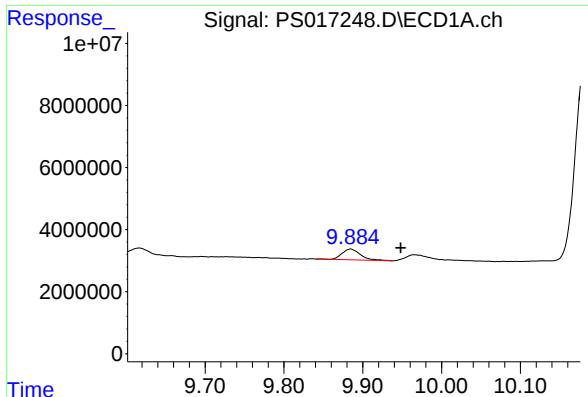

#13 2,4-DB


R.T.: 9.885 min
Delta R.T.: -0.063 min
Response: 5628466
Conc: 3.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

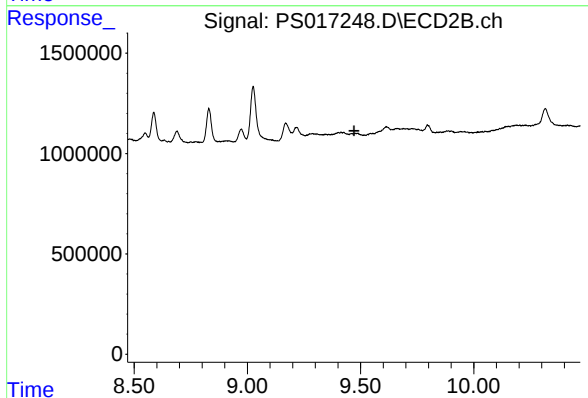


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

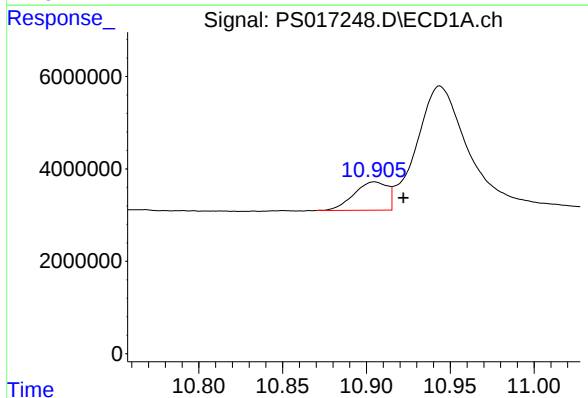


#15 Picloram

R.T.: 10.905 min
Delta R.T.: -0.017 min
Response: 8563541
Conc: N.D.

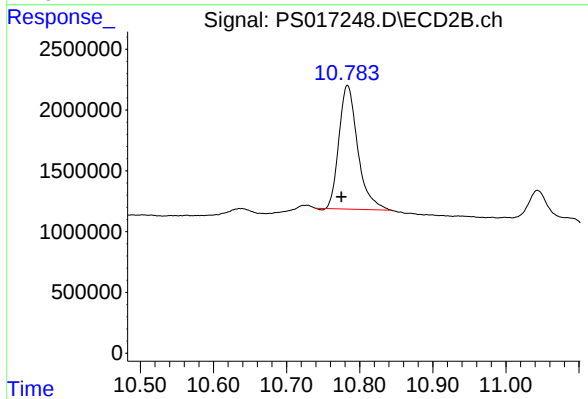

#15 Picloram


R.T.: 10.783 min
Delta R.T.: 0.008 min
Response: 18202964
Conc: 4.75 ng/ml

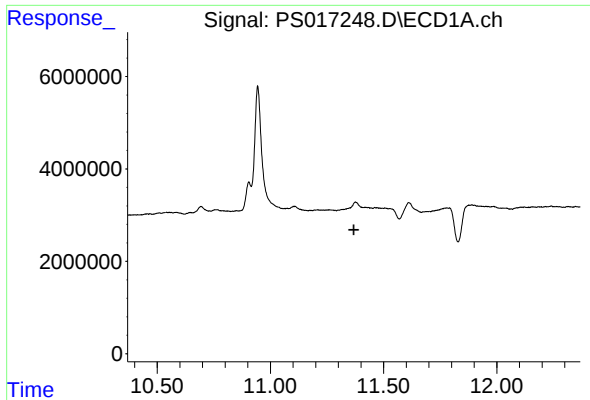

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

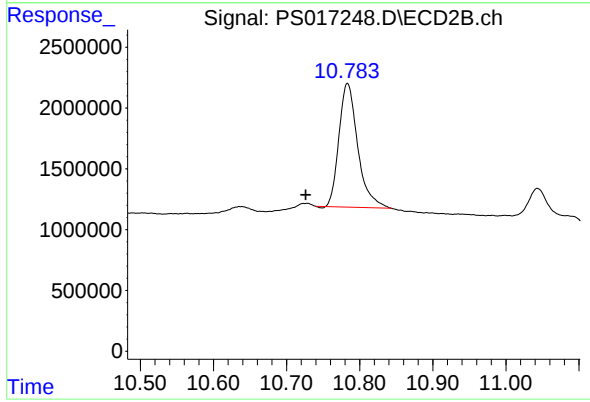

#16 DCPA

R.T.: 10.783 min
Delta R.T.: 0.057 min
Response: 18202964
Conc: 4.27 ng/ml