

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102824\
 Data File : PS028070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Oct 2024 09:44
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 00:21:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 23 13:25:49 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.576f	0.000	52816730	0	11.592	N.D.	#
3) T	4-Nitroph...	6.878	0.000	7004226	0	3.785	N.D.	#
5) T	DICAMBA	0.000	7.788	0	1166835	N.D.	<MDL	
6) T	MCP	7.495f	7.910	8361326	1562210	1.140	<MDL	#
7) T	MCPA	7.613	0.000	1023540	0	<MDL	N.D.	#
8) T	DICHLORPROP	0.000	8.510	0	1164735	N.D.	1.243	
9) T	2,4-D	8.175	8.857	7526539	2472841	2.221	2.480	
10) T	Pentachlo...	8.467	9.387f	3858814	1738036	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.025	9.712	1346864	2304288	<MDL	<MDL	#
12) T	2,4,5-T	9.313	10.116	4966120	3232565	<MDL	<MDL	#
13) T	2,4-DB	9.878	10.702	1663982	2485252	<MDL	4.866	#
14) T	DINOSEB	11.047	0.000	4495635	0	<MDL	N.D.	#
15) T	Picloram	10.868	12.137	46584385	6069241	2.092	1.332	#
16) T	DCPA	11.351	12.074f	5392140	2336508	<MDL	<MDL	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102824\
Data File : PS028070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Oct 2024 09:44
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 00:21:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102324.M
Quant Title : 8080.M
QLast Update : Wed Oct 23 13:25:49 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

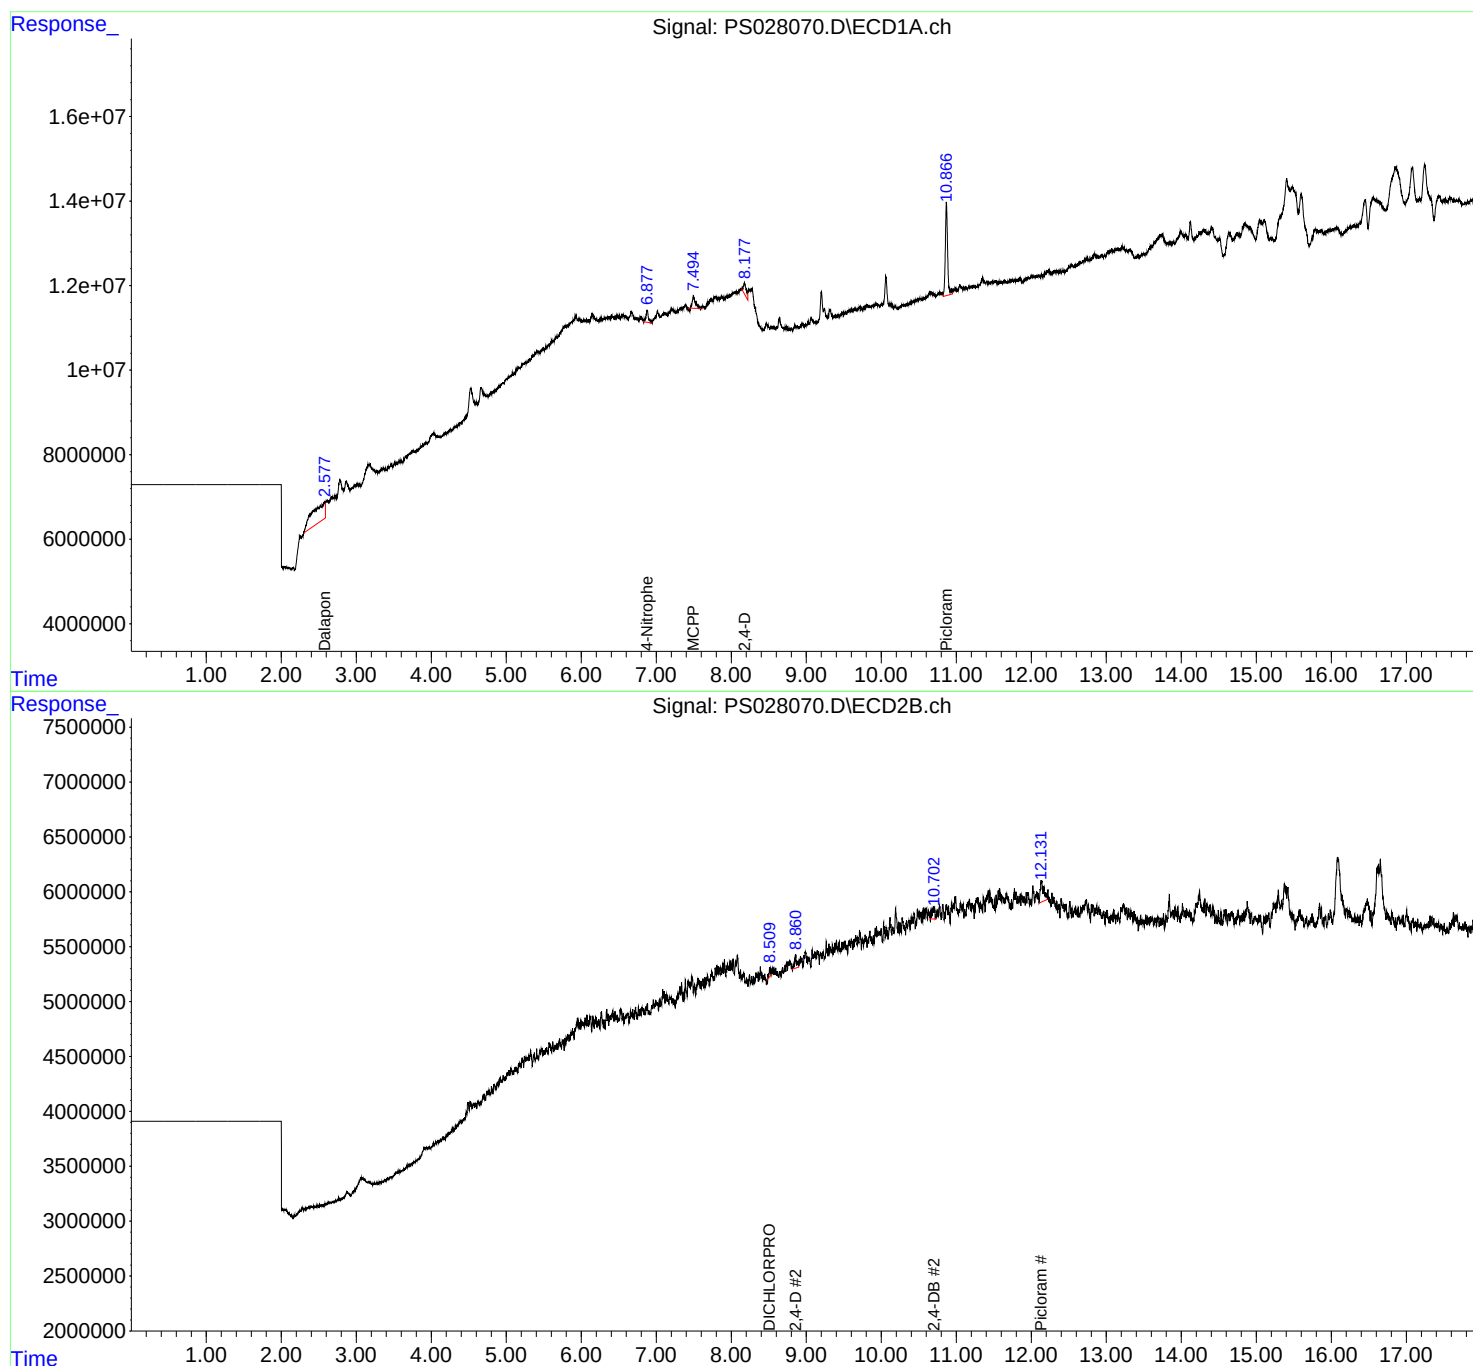


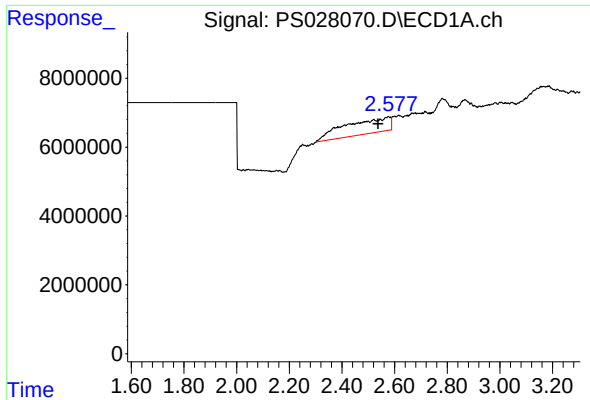

#1 Dalapon


R.T.: 2.576 min
Delta R.T.: 0.038 min
Response: 52816730
Conc: 11.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

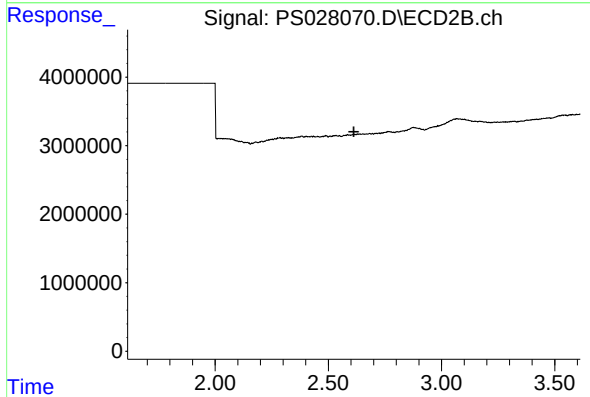


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.613 min
Response: 0
Conc: N.D.

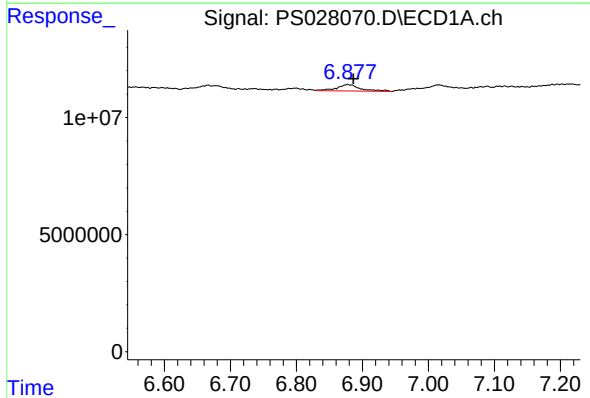


#3 4-Nitrophenol

R.T.: 6.878 min
Delta R.T.: -0.008 min
Response: 7004226
Conc: 3.79 ng/ml

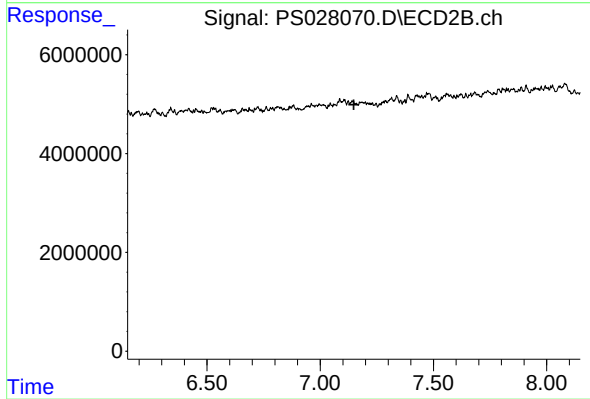

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

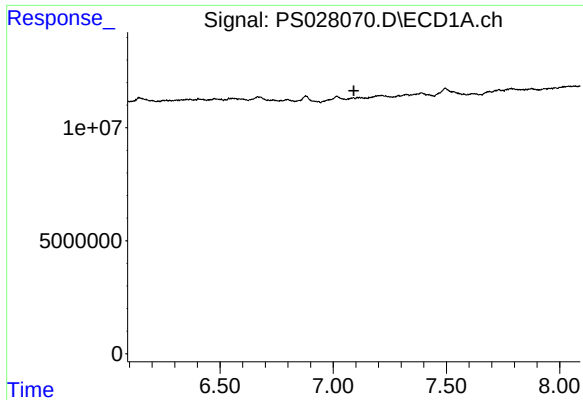

#4 2,4-DCAA


R.T.: 7.115 min
Delta R.T.: 0.024 min
Response: -615666
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

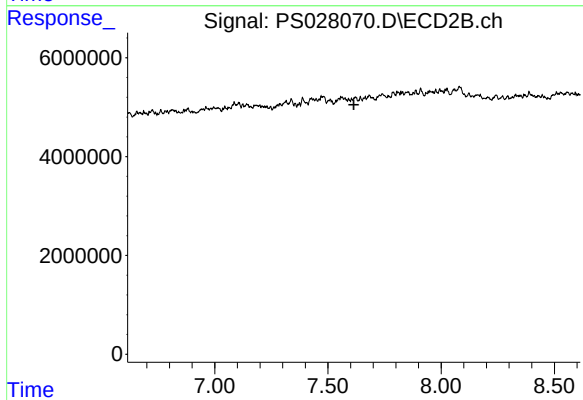


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.614 min
Response: 0
Conc: N.D.

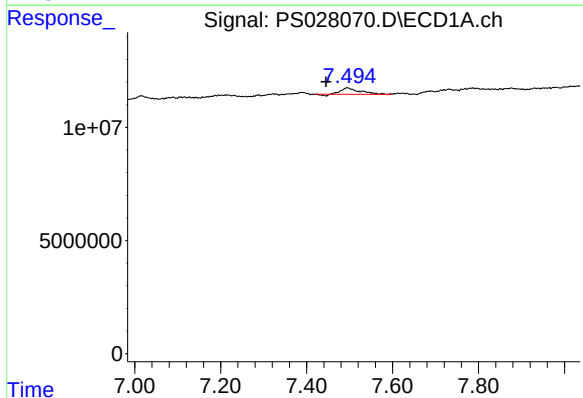


#6 MCP

R.T.: 7.495 min
Delta R.T.: 0.049 min
Response: 8361326
Conc: 1.14 ug/ml

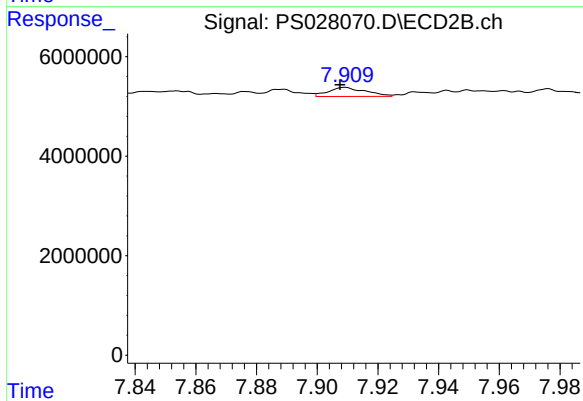

#6 MCP


R.T.: 7.910 min
Delta R.T.: 0.002 min
Response: 1562210
Conc: N.D.

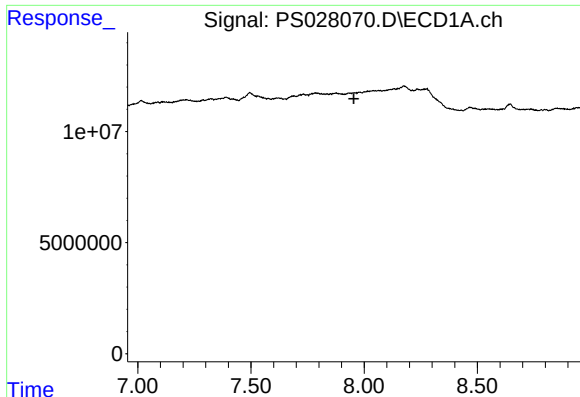

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.955 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

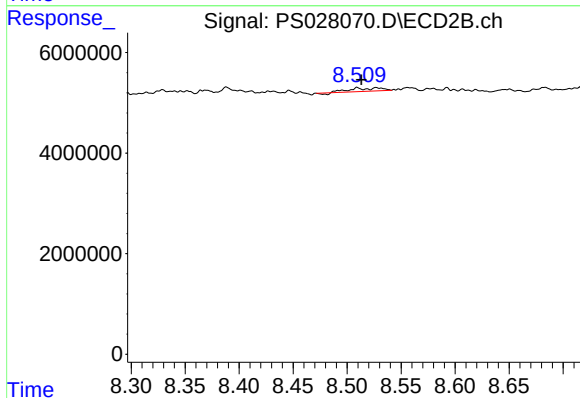


#8 DICHLORPROP

R.T.: 8.510 min
Delta R.T.: -0.004 min
Response: 1164735
Conc: 1.24 ng/ml

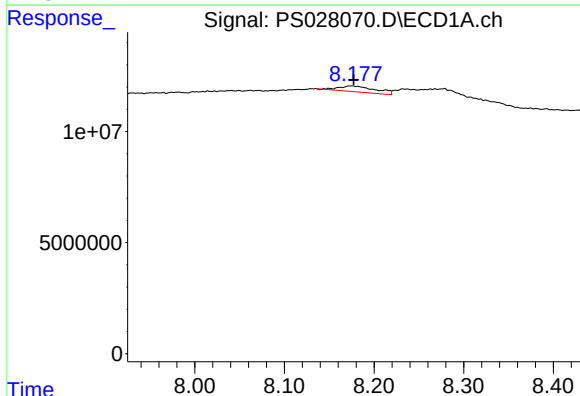


#9 2,4-D

R.T.: 8.175 min
Delta R.T.: -0.002 min
Response: 7526539
Conc: 2.22 ng/ml

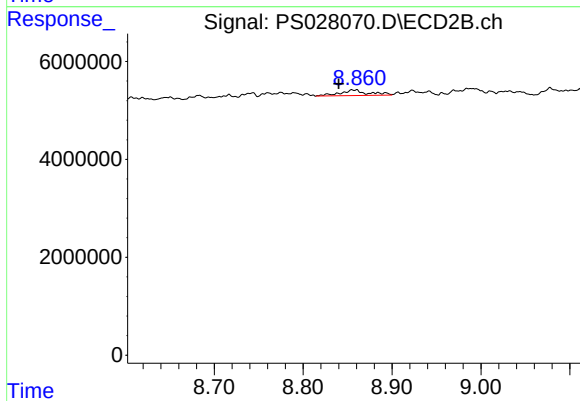

#9 2,4-D


R.T.: 8.857 min
Delta R.T.: 0.017 min
Response: 2472841
Conc: 2.48 ng/ml

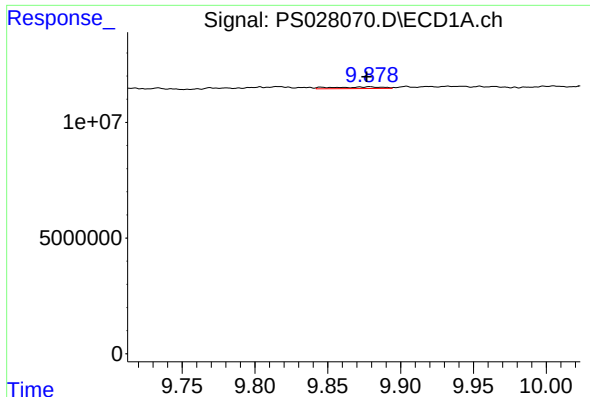

#13 2,4-DB


R.T.: 9.878 min
Delta R.T.: 0.002 min
Response: 1663982
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

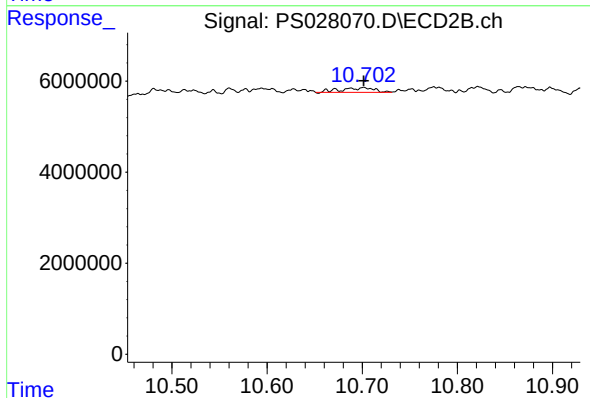


#13 2,4-DB

R.T.: 10.702 min
Delta R.T.: 0.000 min
Response: 2485252
Conc: 4.87 ng/ml

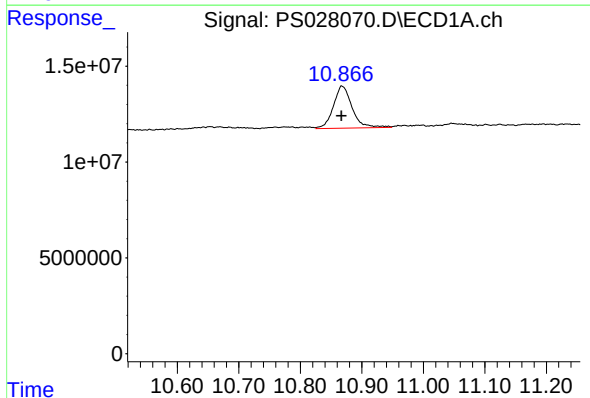

#15 Picloram

R.T.: 10.868 min
Delta R.T.: 0.001 min
Response: 46584385
Conc: 2.09 ng/ml

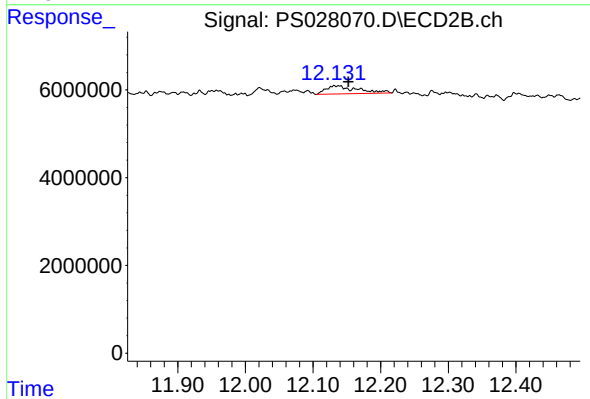

#15 Picloram

R.T.: 12.137 min
Delta R.T.: -0.015 min
Response: 6069241
Conc: 1.33 ng/ml