

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102918\
 Data File : PS002180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 08:27
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 17:16:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.923	0	235442	N.D.	0.656 #
Target Compounds							
1) T	Dalapon	2.904	2.365	16120259	608666	35.146	1.348 #
2) T	3,5-DICHL...	0.000	9.080	0	95235	N.D.	0.215 #
3) T	4-Nitroph...	0.000	10.065	0	172687	N.D.	0.968 #
5) T	DICAMBA	0.000	11.241	0	74580	N.D.	0.060 #
6) T	MCPD	0.000	11.411	0	394787	N.D.	0.459 #
7) T	MCPA	0.000	11.814	0	118350	N.D.	0.087 #
8) T	DICHLORPROP	0.000	12.378	0	109318	N.D.	0.340 #
9) T	2,4-D	0.000	12.801	0	48603	N.D.	0.114 #
10) T	Pentachlo...	0.000	13.290	0	64793	N.D.	0.014 #
11) T	2,4,5-TP ...	0.000	13.981	0	122727	N.D.	0.067 #
12) T	2,4,5-T	0.000	14.526	0	3809421	N.D.	2.544 #
13) T	2,4-DB	0.000	15.192	0	120371	N.D.	0.543 #
14) T	DINOSEB	0.000	15.593	0	111146	N.D.	0.088 #
15) T	Picloram	16.934	16.840	10175480	11327292	4.266	5.007
16) T	DCPA	0.000	16.840	0	11327292	N.D.	4.784 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102918\
Data File : PS002180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 08:27
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 17:16:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

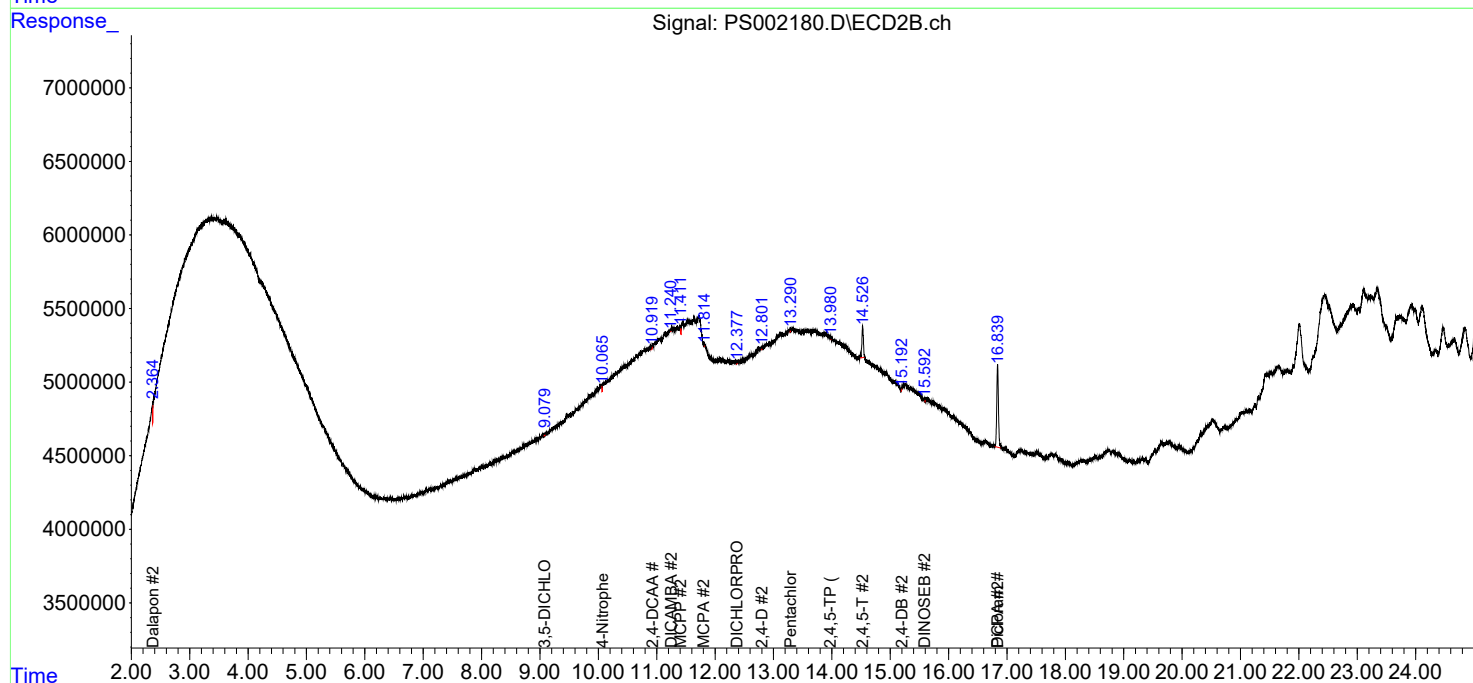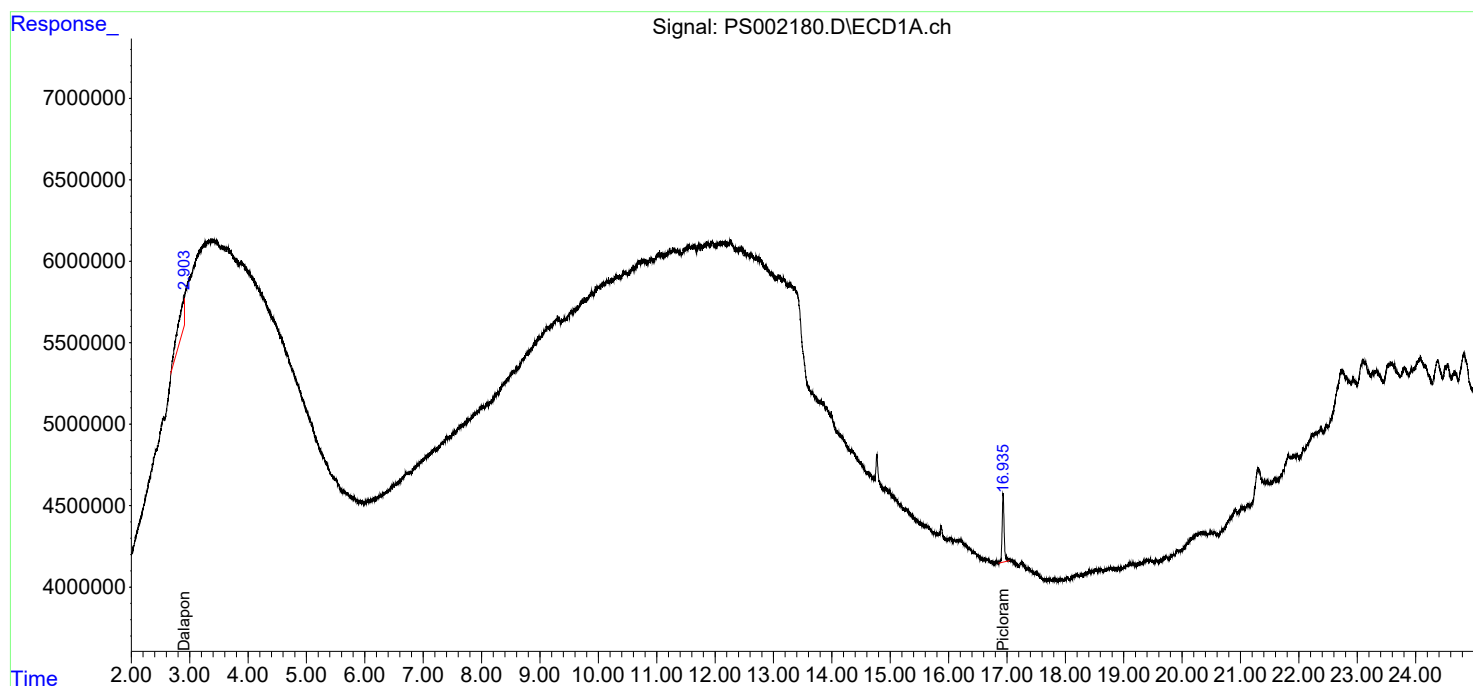


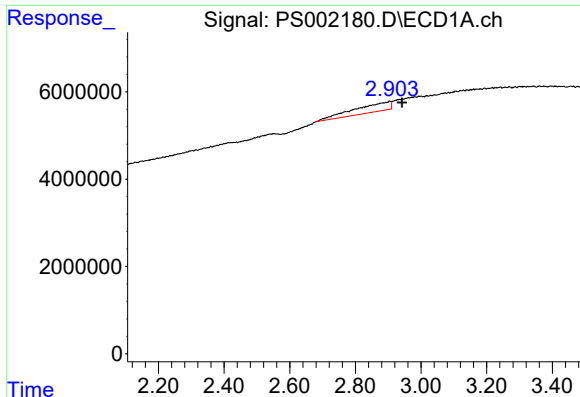

#1 Dalapon


R.T.: 2.904 min
Delta R.T.: -0.038 min
Response: 16120259
Conc: 35.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

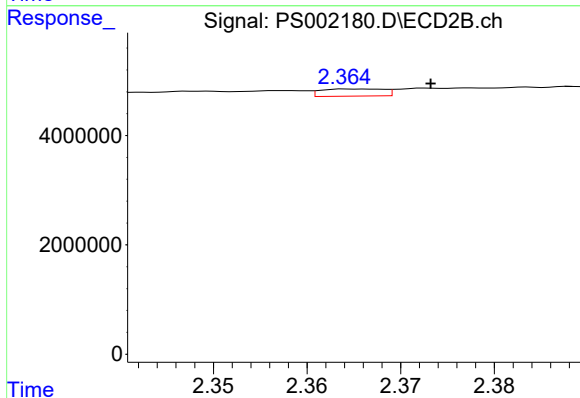


#1 Dalapon

R.T.: 2.365 min
Delta R.T.: -0.009 min
Response: 608666
Conc: 1.35 ng/ml

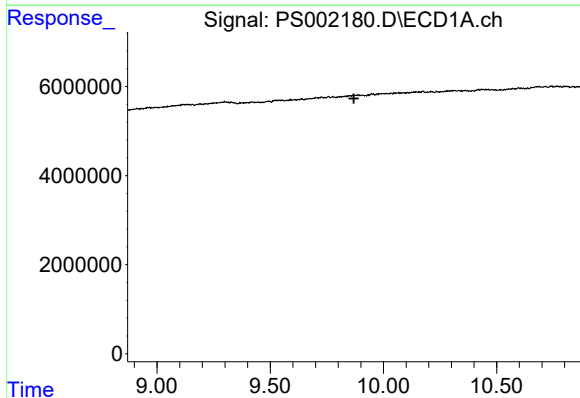


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

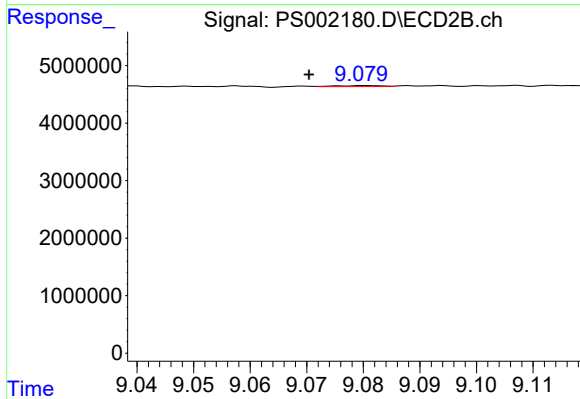

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.080 min
Delta R.T.: 0.010 min
Response: 95235
Conc: 0.21 ng/ml

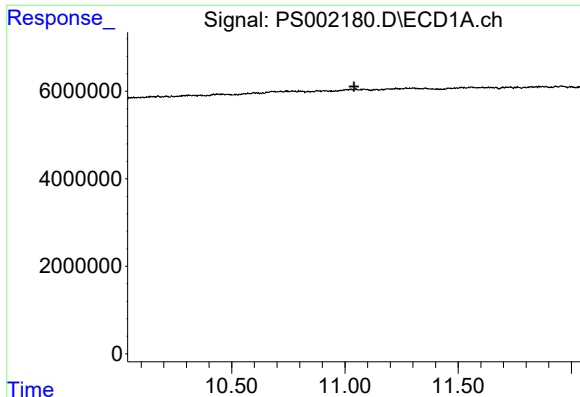

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

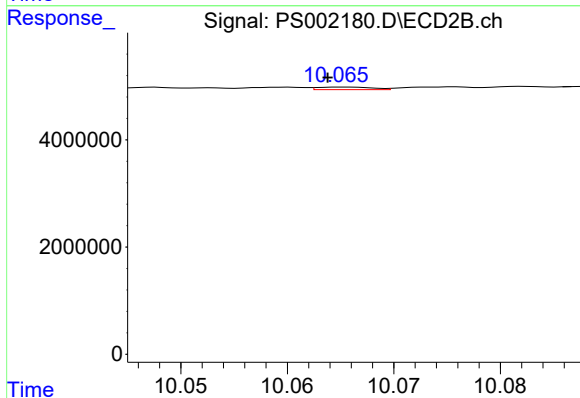


#3 4-Nitrophenol

R.T.: 10.065 min
Delta R.T.: 0.002 min
Response: 172687
Conc: 0.97 ng/ml

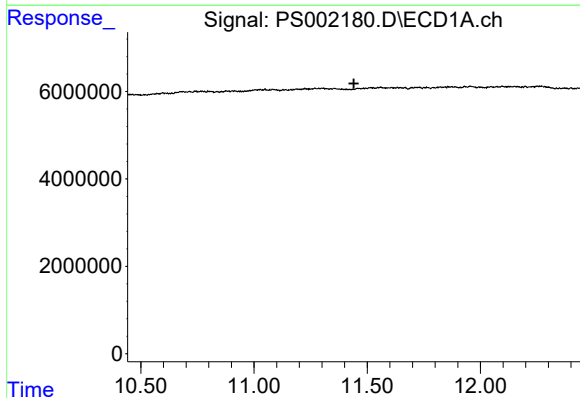


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.441 min
Response: 0
Conc: N.D.

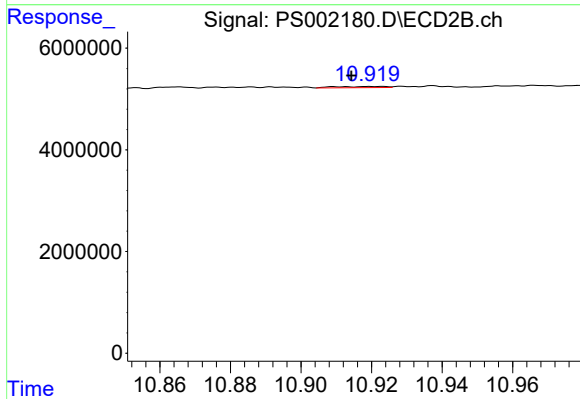

#4 2,4-DCAA


R.T.: 10.923 min
Delta R.T.: 0.009 min
Response: 235442
Conc: 0.66 ng/ml

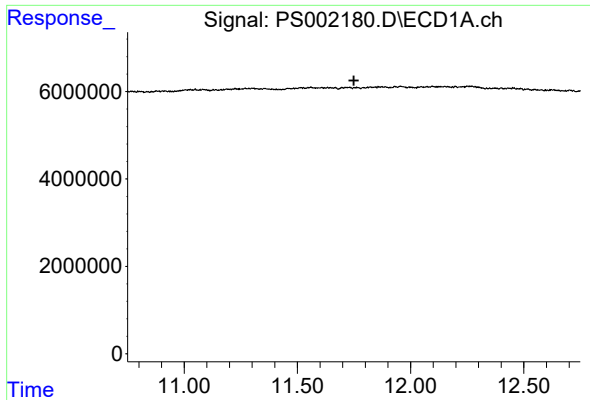

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

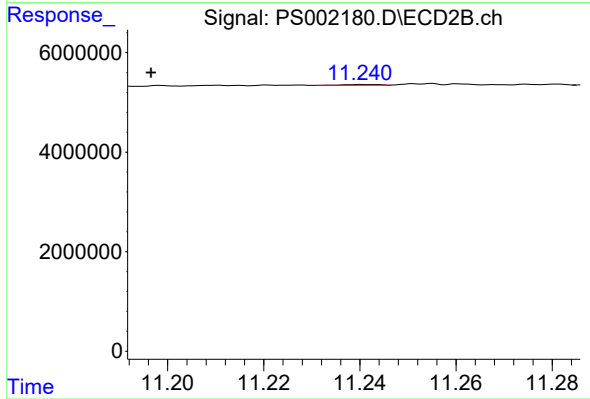


#5 DICAMBA

R.T.: 11.241 min
Delta R.T.: 0.044 min
Response: 74580
Conc: 0.06 ng/ml

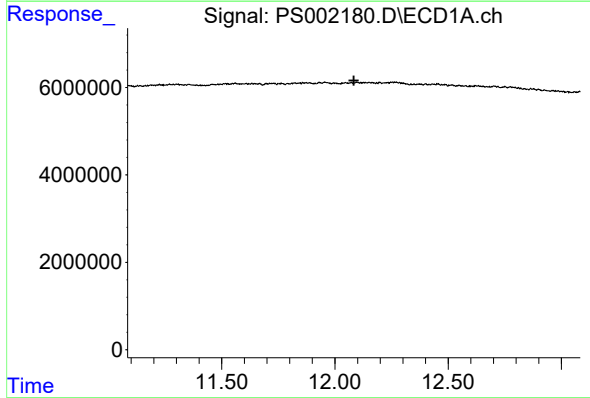


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

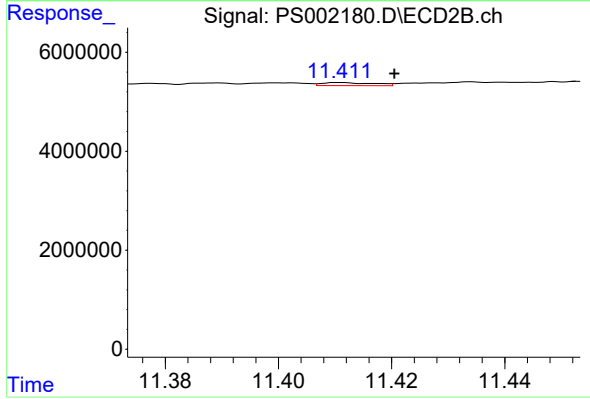

#6 MCP


R.T.: 11.411 min
Delta R.T.: -0.009 min
Response: 394787
Conc: 0.46 ug/ml

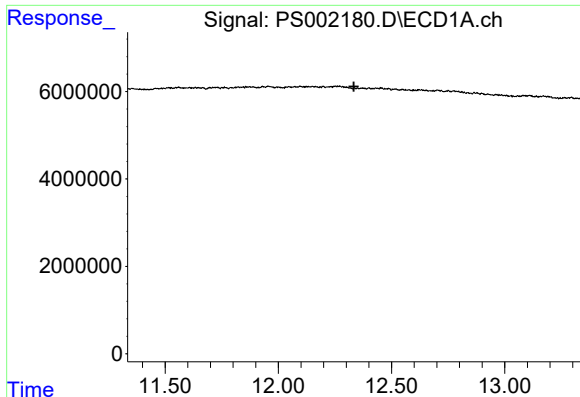

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

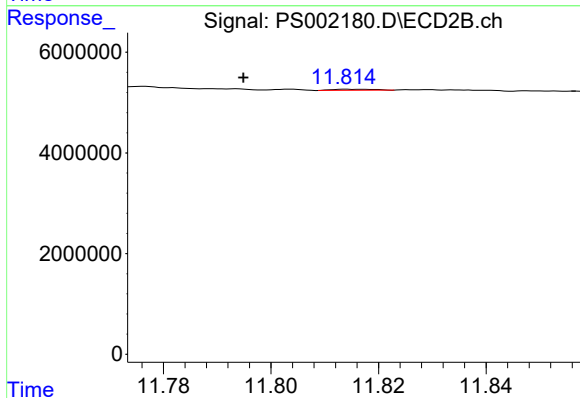


#7 MCPA

R.T.: 11.814 min
Delta R.T.: 0.019 min
Response: 118350
Conc: 0.09 ug/ml

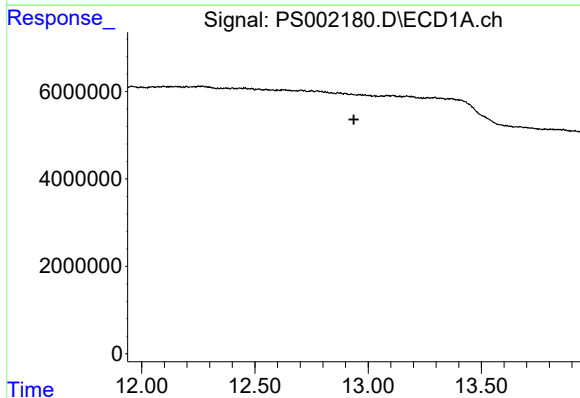


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

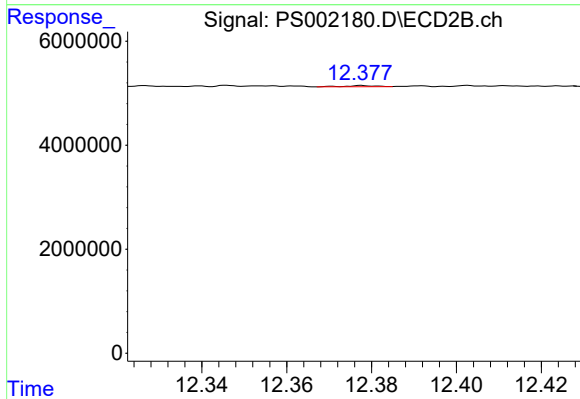

#8 DICHLORPROP


R.T.: 12.378 min
Delta R.T.: 0.058 min
Response: 109318
Conc: 0.34 ng/ml

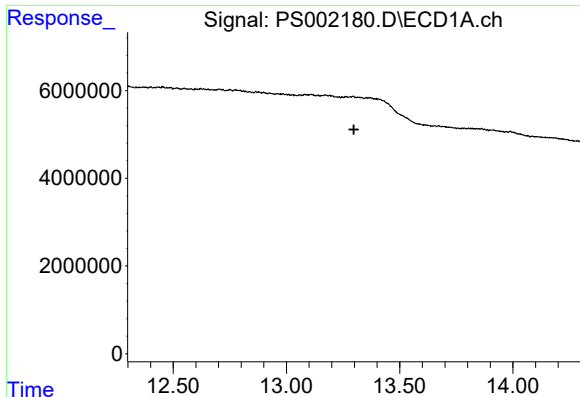

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

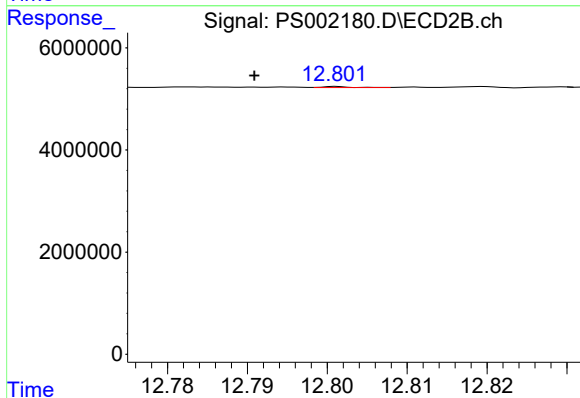


#9 2,4-D

R.T.: 12.801 min
Delta R.T.: 0.010 min
Response: 48603
Conc: 0.11 ng/ml

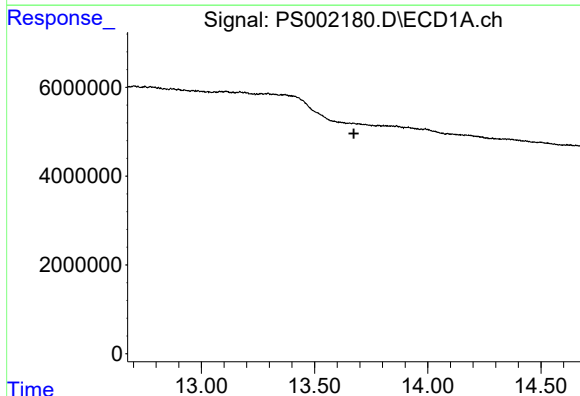


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

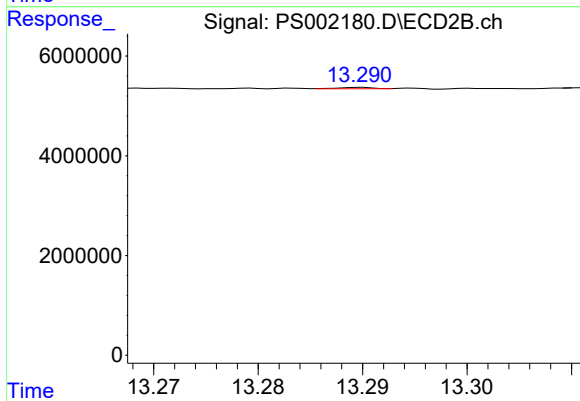

#10 Pentachlorophenol


R.T.: 13.290 min
Delta R.T.: -0.045 min
Response: 64793
Conc: 0.01 ng/ml

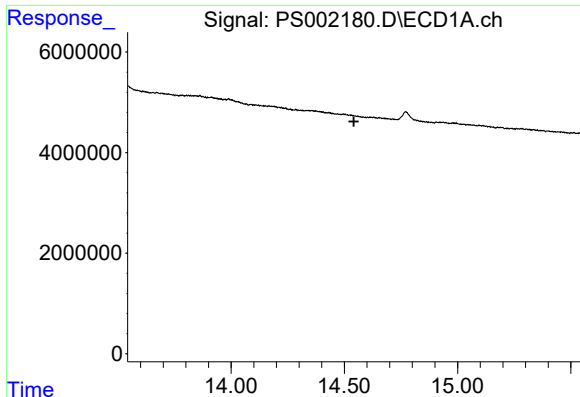

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

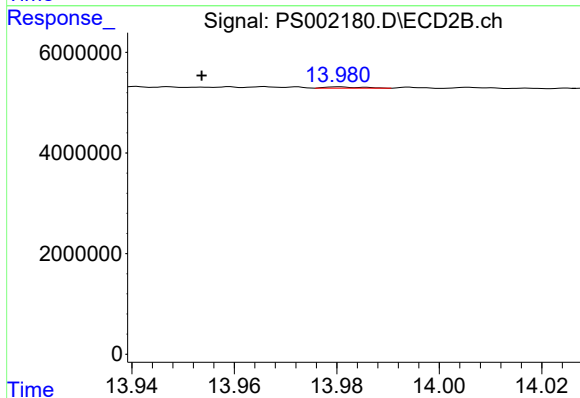


#11 2,4,5-TP (SILVEX)

R.T.: 13.981 min
Delta R.T.: 0.027 min
Response: 122727
Conc: 0.07 ng/ml

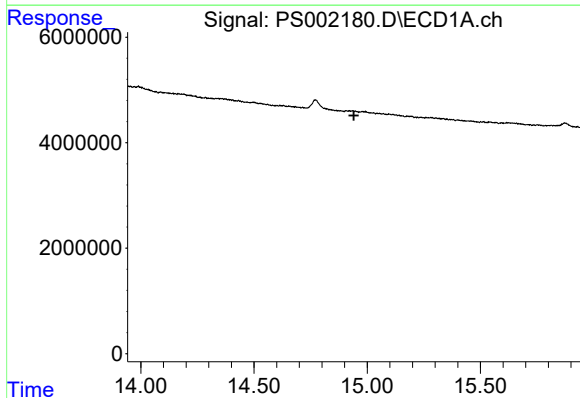


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

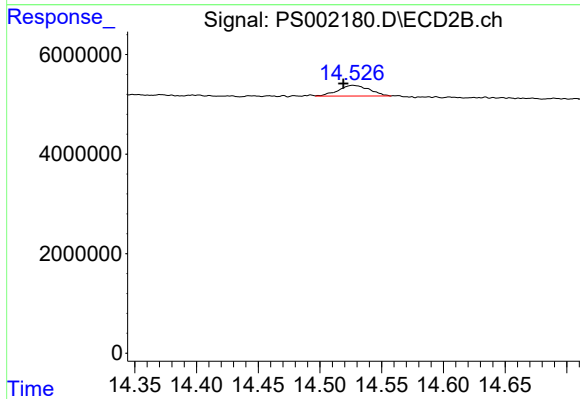

#12 2,4,5-T


R.T.: 14.526 min
Delta R.T.: 0.007 min
Response: 3809421
Conc: 2.54 ng/ml

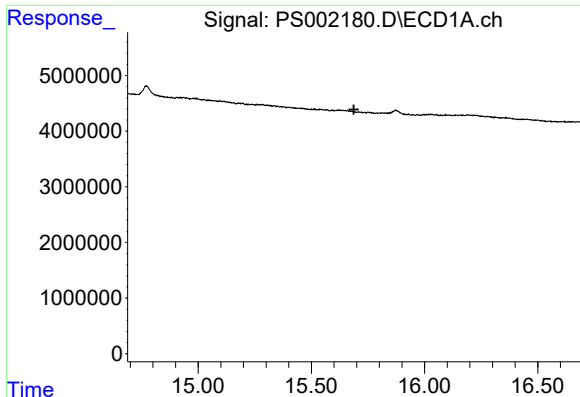

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

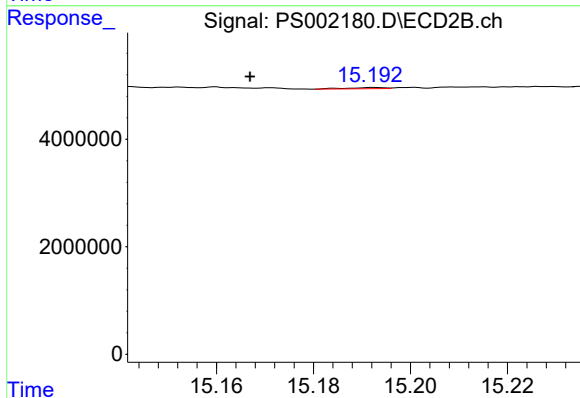


#13 2,4-DB

R.T.: 15.192 min
Delta R.T.: 0.025 min
Response: 120371
Conc: 0.54 ng/ml

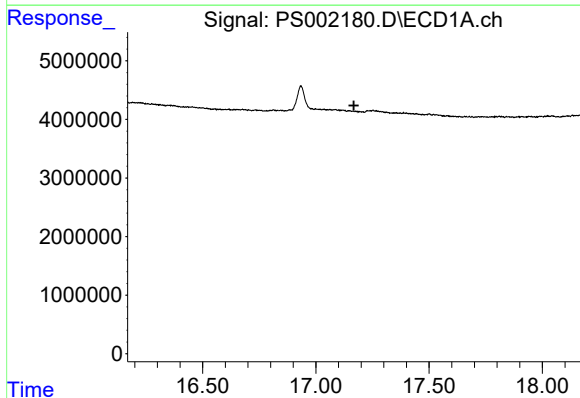


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

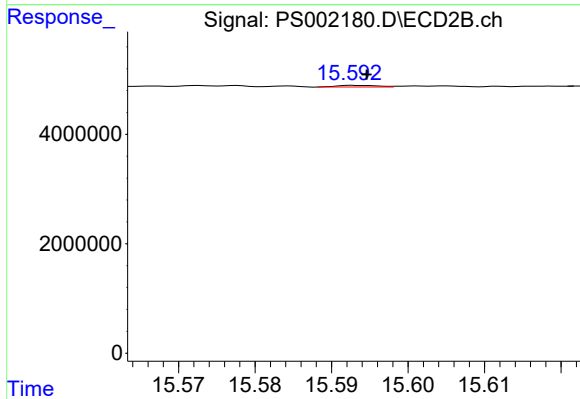

#14 DINOSEB


R.T.: 15.593 min
Delta R.T.: -0.002 min
Response: 111146
Conc: 0.09 ng/ml

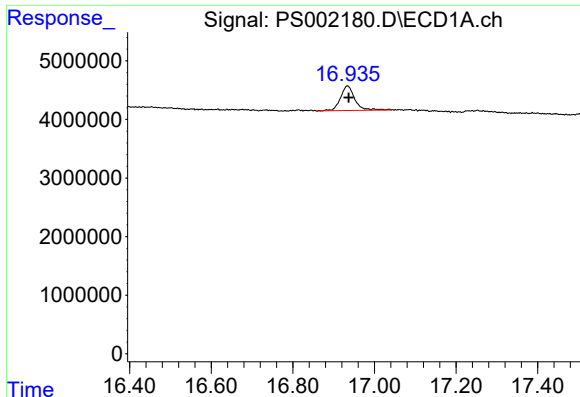

#15 Picloram


R.T.: 16.934 min
Delta R.T.: -0.003 min
Response: 10175480
Conc: 4.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

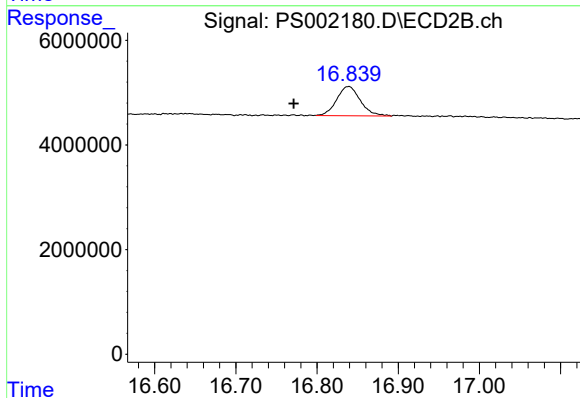


#15 Picloram

R.T.: 16.840 min
Delta R.T.: 0.068 min
Response: 11327292
Conc: 5.01 ng/ml

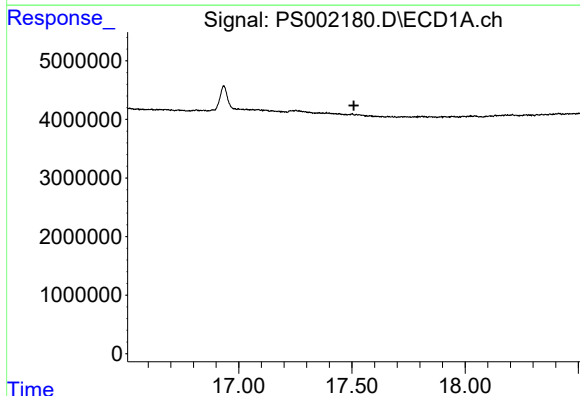

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

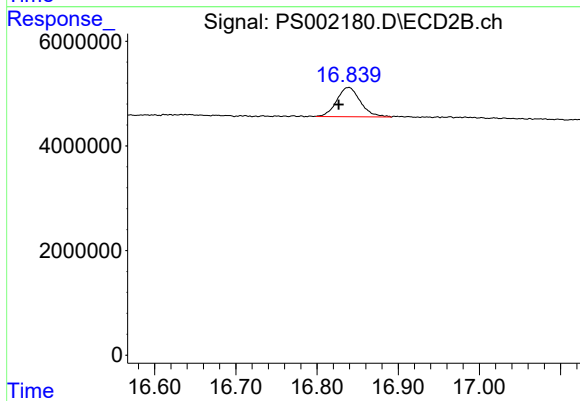

#16 DCPA

R.T.: 16.840 min
Delta R.T.: 0.013 min
Response: 11327292
Conc: 4.78 ng/ml