

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102918\
 Data File : PS002181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2018 08:58
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 17:15:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.411	10.896	151.3E6	143.5E6	480.731	399.684
Target Compounds							
1) T	Dalapon	0.000	2.381	0	310241	N.D.	0.687 #
7) T	MCPA	0.000	11.794	0	855289	N.D.	0.632 #
12) T	2,4,5-T	0.000	14.508	0	1041276	N.D.	0.695 #
13) T	2,4-DB	0.000	15.192	0	78415	N.D.	0.354 #
15) T	Picloram	16.909	16.816	6152428	7627969	2.579	3.372 #
16) T	DCPA	0.000	16.816	0	7627969	N.D.	3.221 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102918\
Data File : PS002181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2018 08:58
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 17:15:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

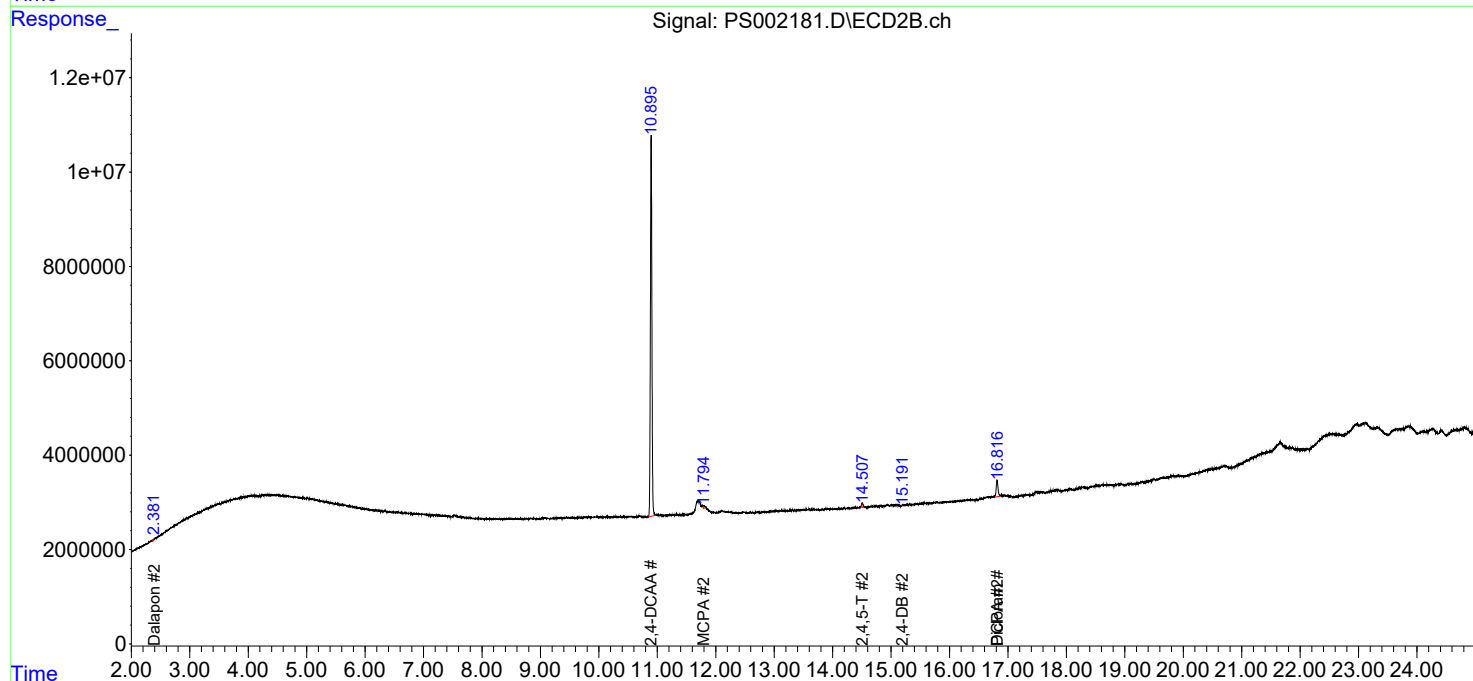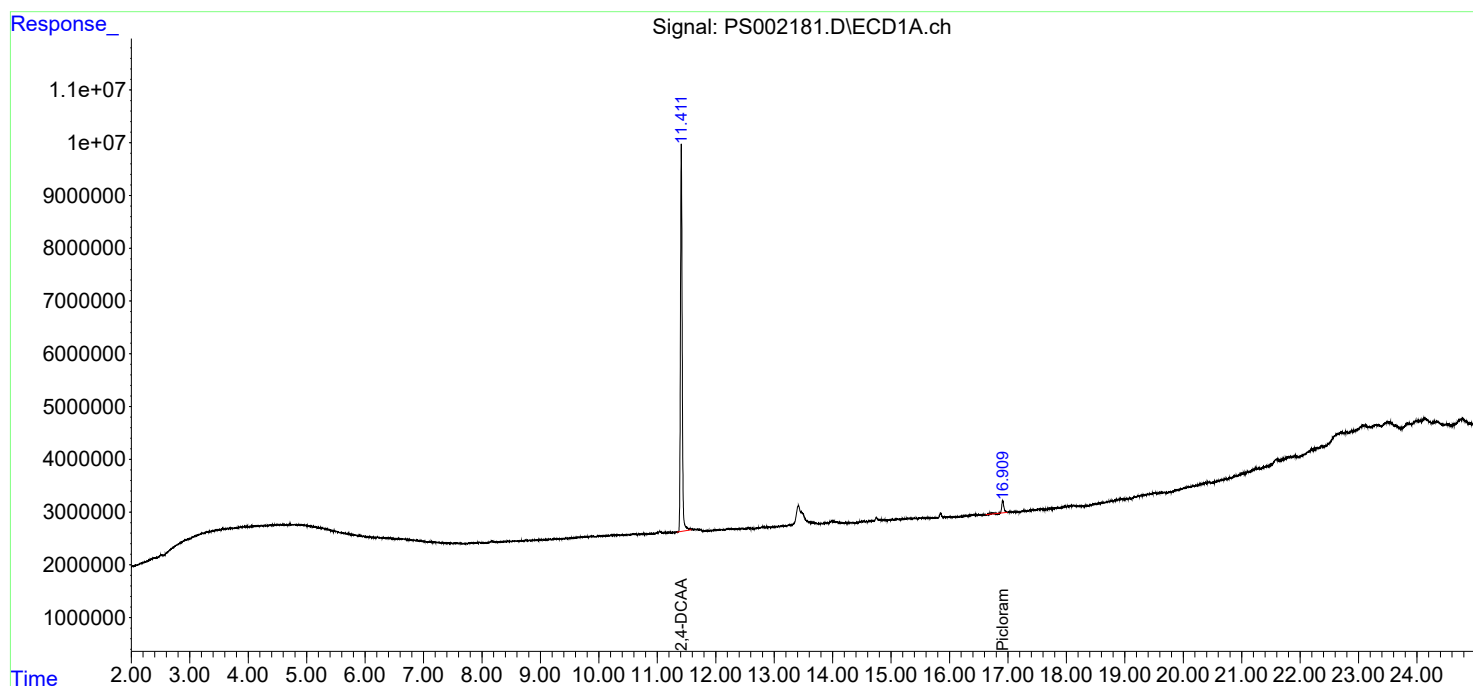


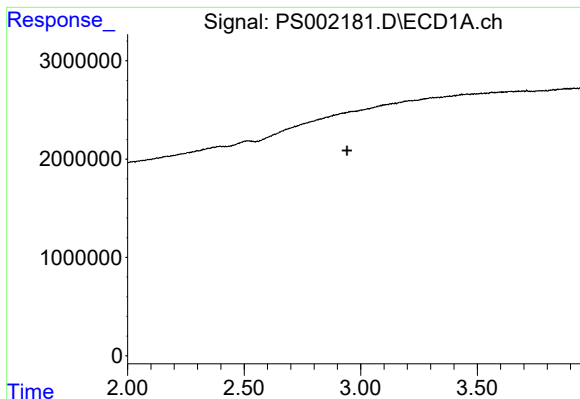

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

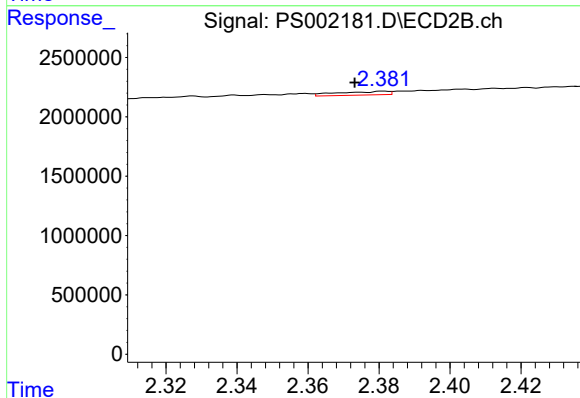


#1 Dalapon

R.T.: 2.381 min
Delta R.T.: 0.008 min
Response: 310241
Conc: 0.69 ng/ml

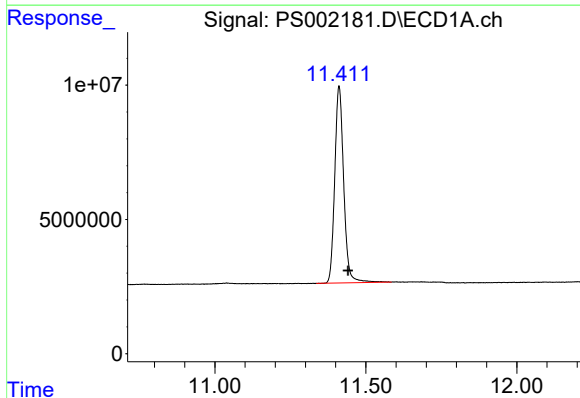


#4 2,4-DCAA

R.T.: 11.411 min
Delta R.T.: -0.030 min
Response: 151279317
Conc: 480.73 ng/ml

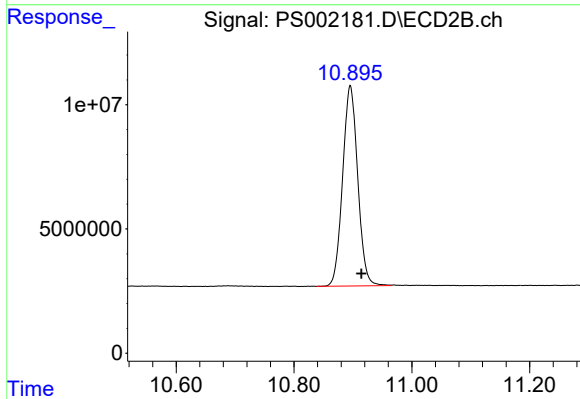

#4 2,4-DCAA


R.T.: 10.896 min
Delta R.T.: -0.019 min
Response: 143525854
Conc: 399.68 ng/ml

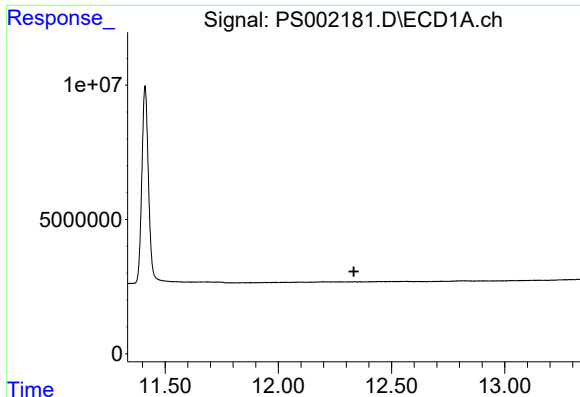

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

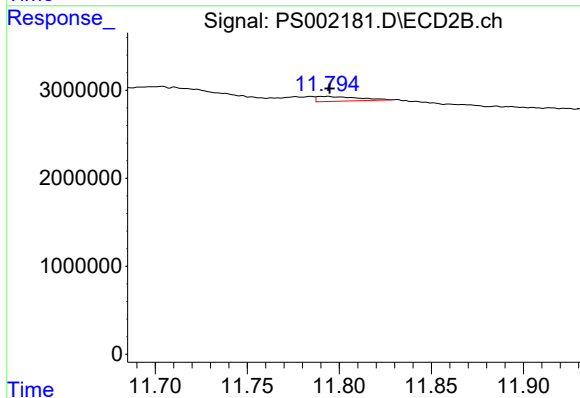


#7 MCPA

R.T.: 11.794 min
Delta R.T.: 0.000 min
Response: 855289
Conc: 0.63 ug/ml

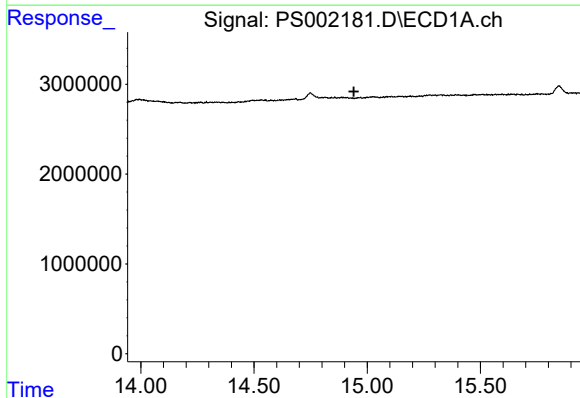


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

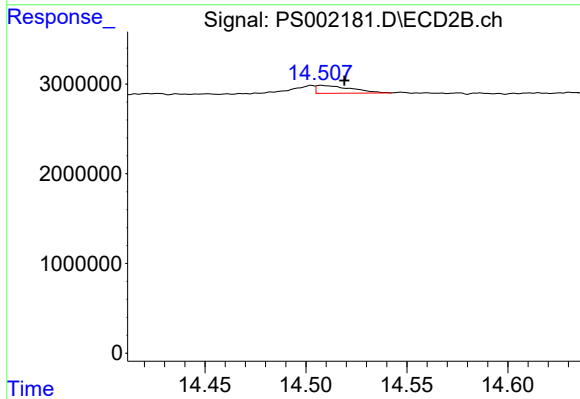

#12 2,4,5-T


R.T.: 14.508 min
Delta R.T.: -0.011 min
Response: 1041276
Conc: 0.70 ng/ml

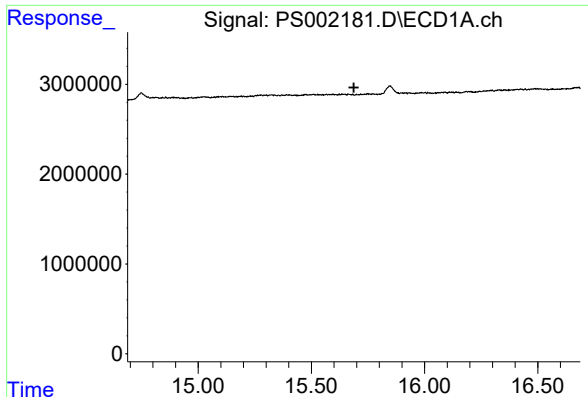

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

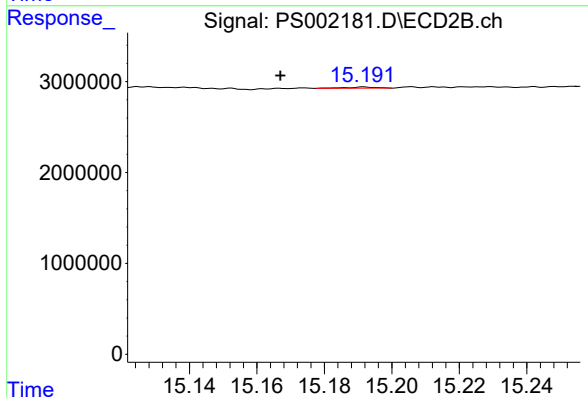


#13 2,4-DB

R.T.: 15.192 min
Delta R.T.: 0.025 min
Response: 78415
Conc: 0.35 ng/ml

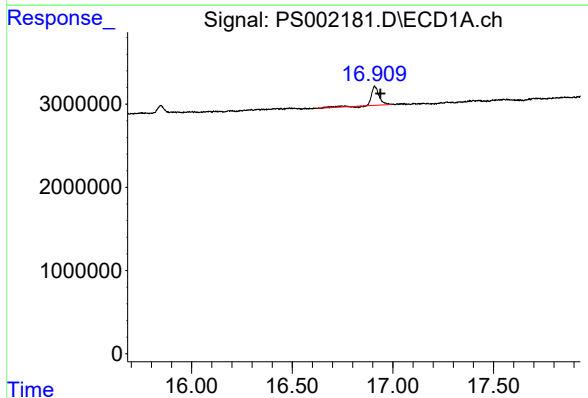


#15 Picloram

R.T.: 16.909 min
Delta R.T.: -0.029 min
Response: 6152428
Conc: 2.58 ng/ml

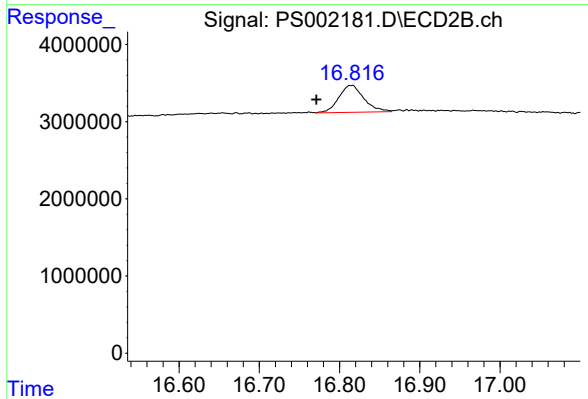

#15 Picloram


R.T.: 16.816 min
Delta R.T.: 0.045 min
Response: 7627969
Conc: 3.37 ng/ml

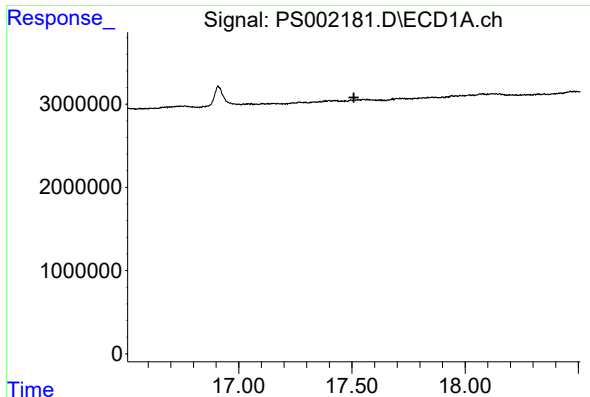

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

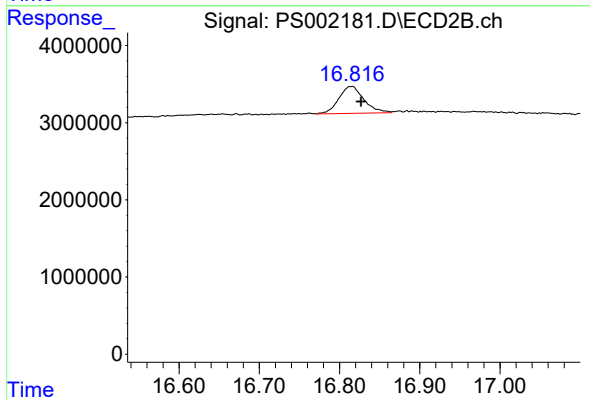

#16 DCPA

R.T.: 16.816 min
Delta R.T.: -0.010 min
Response: 7627969
Conc: 3.22 ng/ml