

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 08:49
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:37:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) T	Pentachlo...	0.000	6.454	0	6649933	N.D. <MDL
12) T	2,4,5-T	0.000	7.215	0	55175900	N.D. 15.748
15) T	Picloram	8.954	8.907	343.8E6	211.5E6	31.149 34.452
16) T	DCPA	0.000	8.861	0	7779739	N.D. 1.551



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 08:49
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:37:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

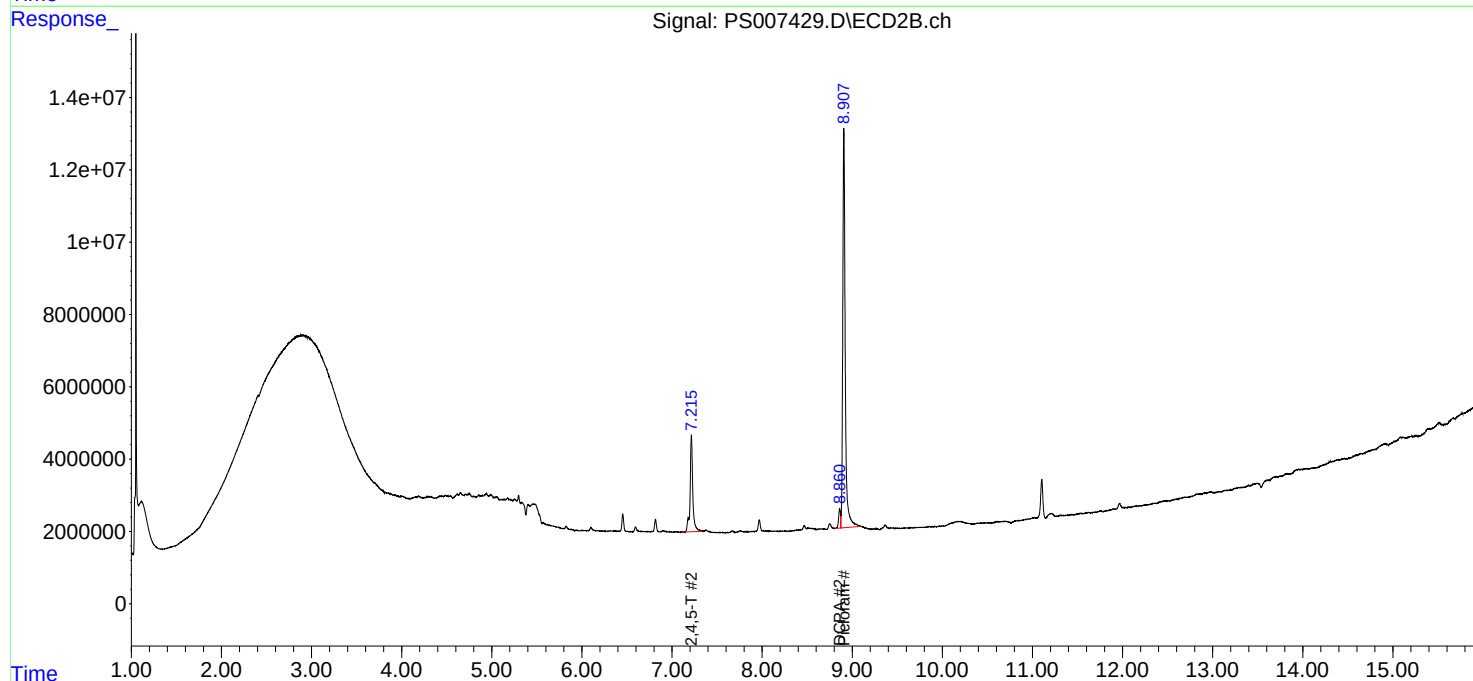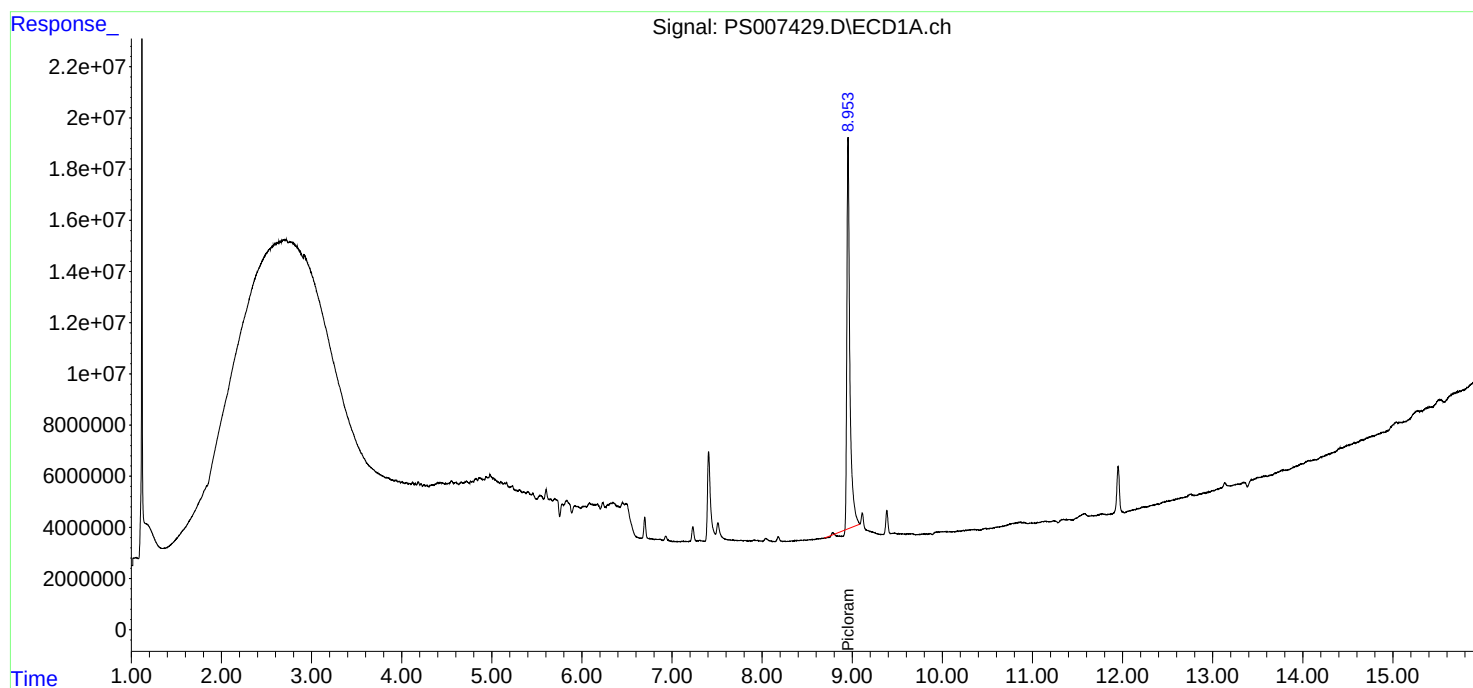


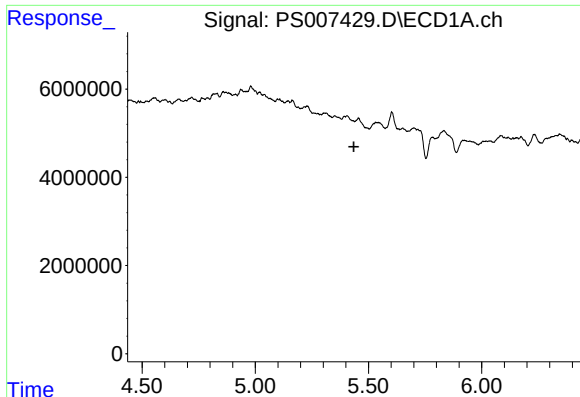

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.436 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

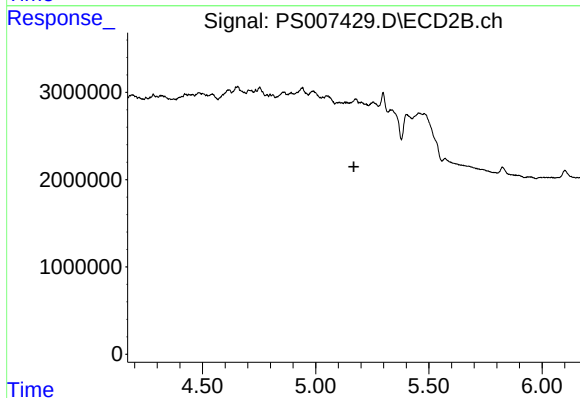


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.169 min
Response: 0
Conc: N.D.

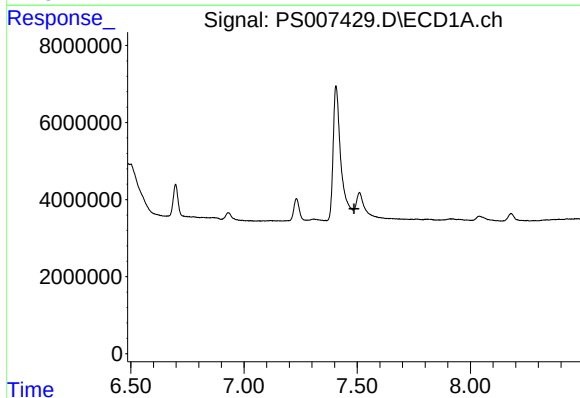


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

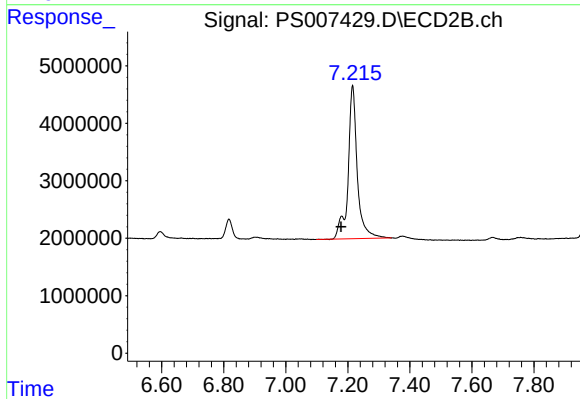

#12 2,4,5-T


R.T.: 7.215 min
Delta R.T.: 0.037 min
Response: 55175900
Conc: 15.75 ng/ml

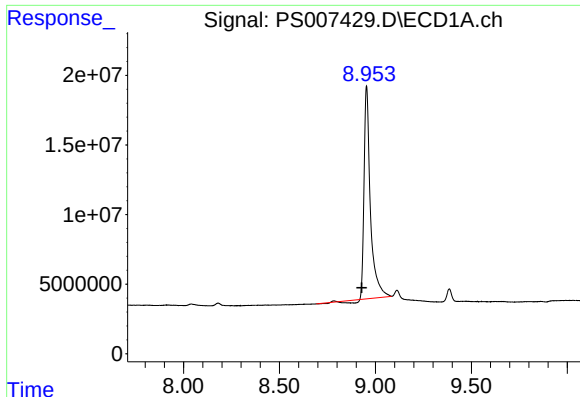

#15 Picloram


R.T.: 8.954 min
Delta R.T.: 0.025 min
Response: 343804832
Conc: 31.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

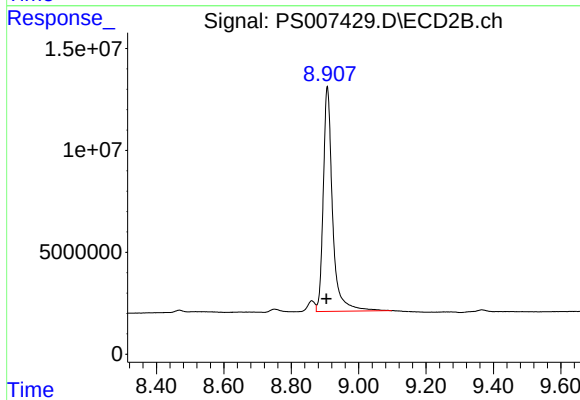


#15 Picloram

R.T.: 8.907 min
Delta R.T.: 0.002 min
Response: 211541776
Conc: 34.45 ng/ml

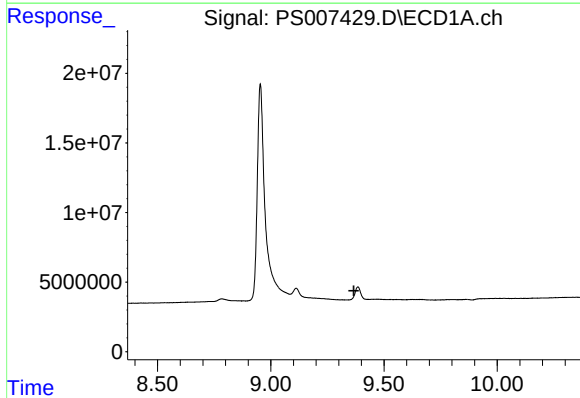

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

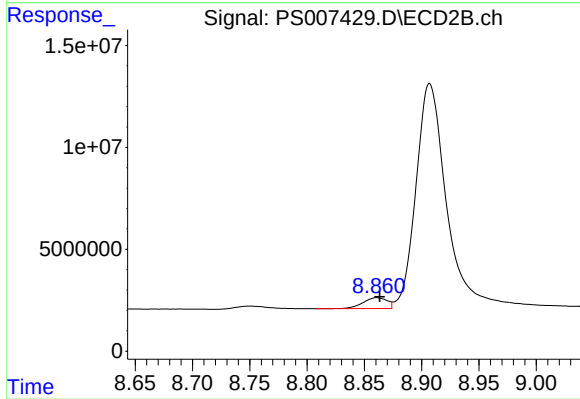

#16 DCPA

R.T.: 8.861 min
Delta R.T.: -0.002 min
Response: 7779739
Conc: 1.55 ng/ml