

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 13:12
 Operator : SM\AJ
 Sample : K5500-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:41:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.161	160.7E6	75721861	117.444	107.666
Target Compounds							
1) T	Dalapon	1.995	1.703	62946894	215.7E6	37.619	237.052 #
2) T	3,5-DICHL...	0.000	4.494	0	68625509	N.D.	79.757
3) T	4-Nitroph...	0.000	4.838	0	6736686	N.D.	17.059
5) T	DICAMBA	5.529	0.000	40166138	0	8.175	N.D. #
7) T	MCPA	0.000	5.530	0	19774819	N.D.	6.802
9) T	2,4-D	6.491	0.000	80935499	0	65.676	N.D. #
10) T	Pentachlo...	0.000	6.453	0	5246894	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.756	0	72991245	N.D.	19.190
14) T	DINOSEB	0.000	7.952	0	6650125	N.D.	2.369
15) T	Picloram	0.000	8.942	0	12436398	N.D.	2.025



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 13:12
Operator : SM\AJ
Sample : K5500-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:41:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

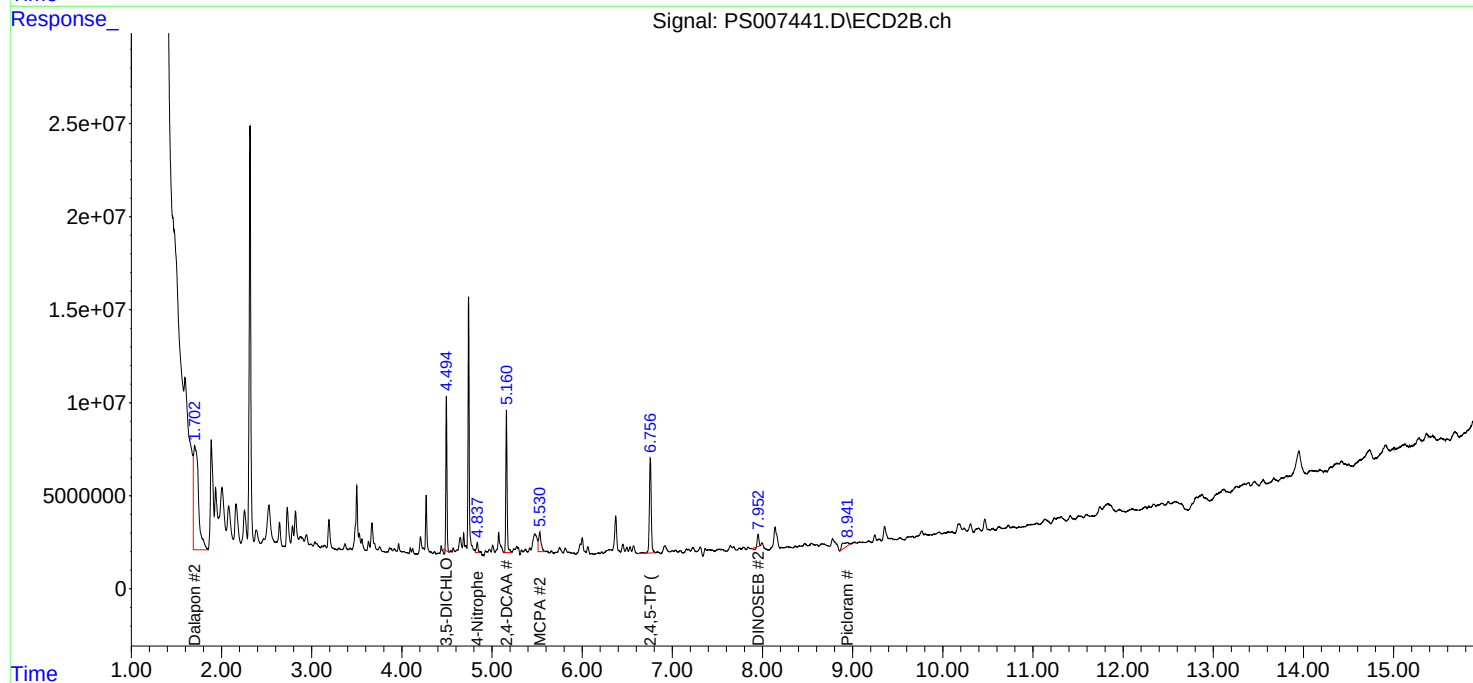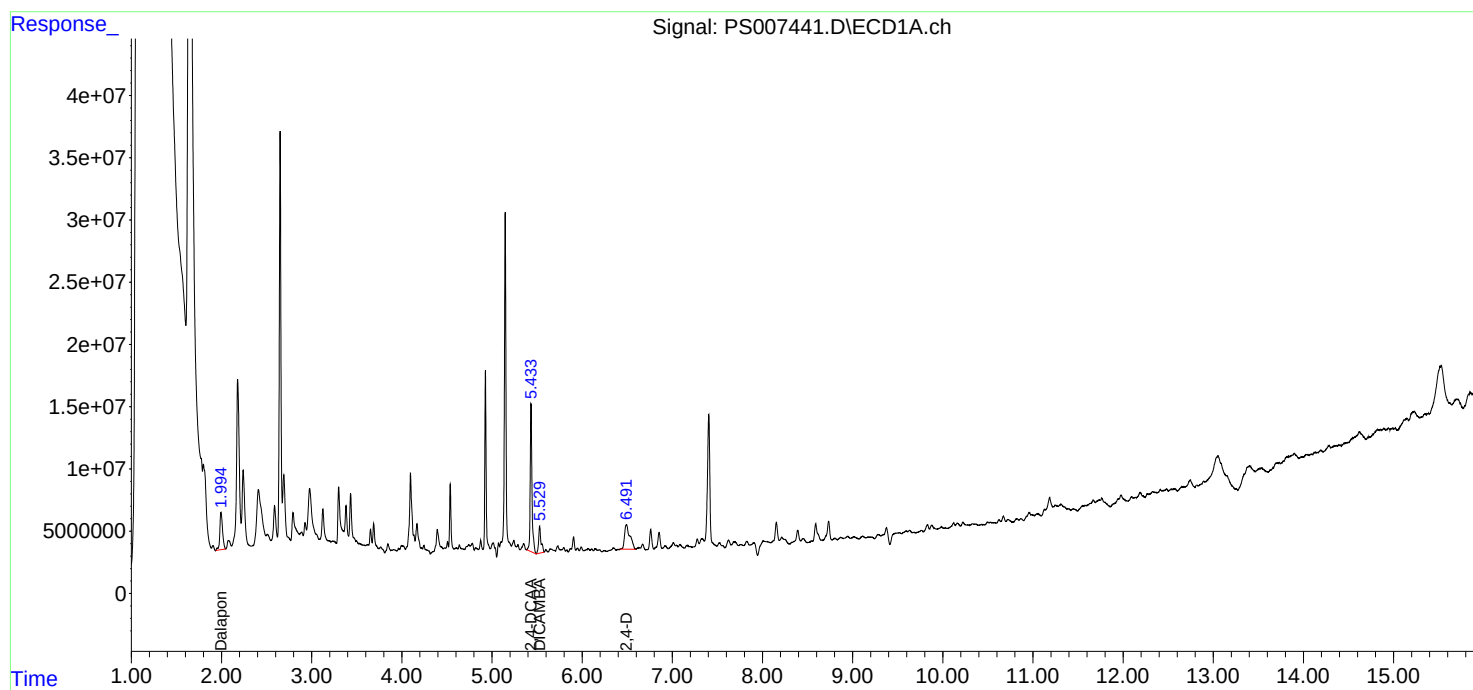


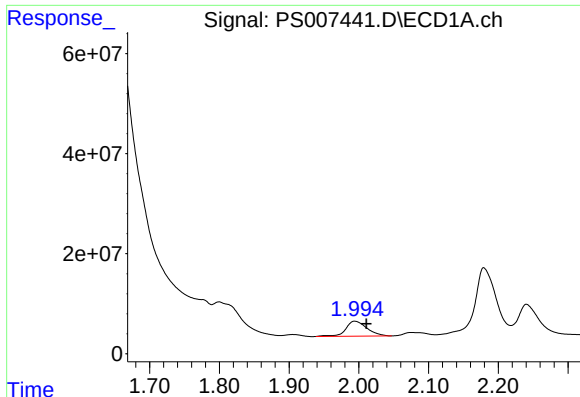

#1 Dalapon


R.T.: 1.995 min
Delta R.T.: -0.016 min
Response: 62946894
Conc: 37.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

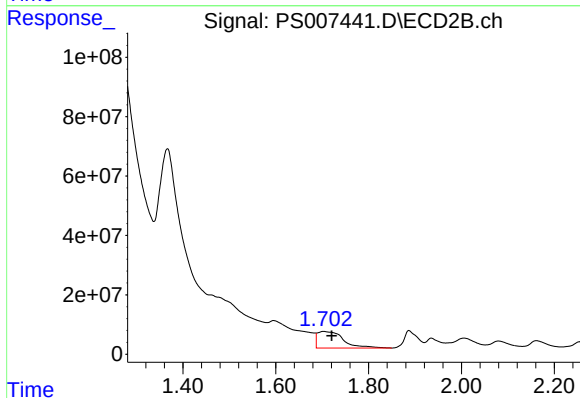


#1 Dalapon

R.T.: 1.703 min
Delta R.T.: -0.017 min
Response: 215718098
Conc: 237.05 ng/ml

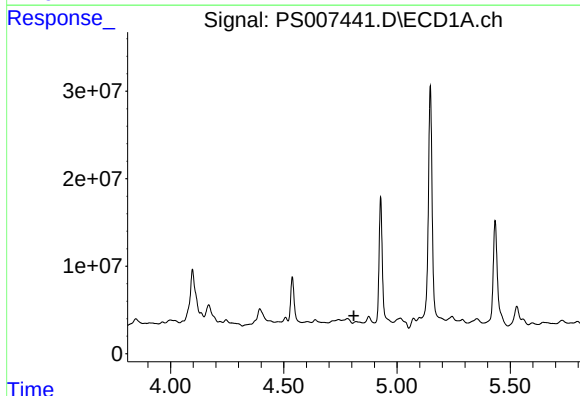


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

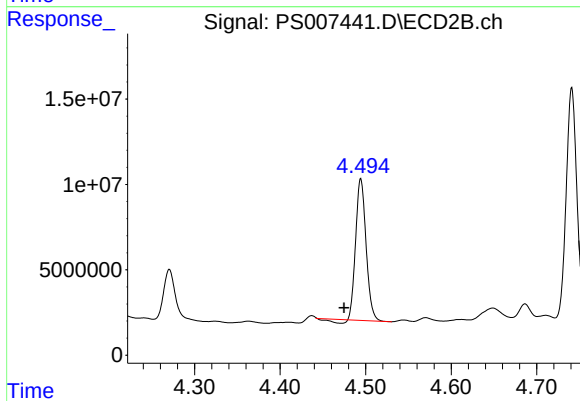

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.494 min
Delta R.T.: 0.020 min
Response: 68625509
Conc: 79.76 ng/ml

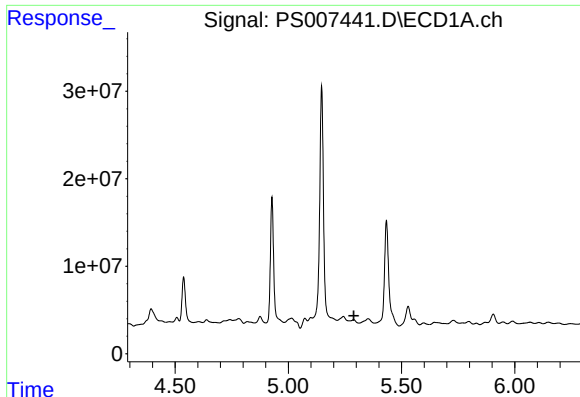

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

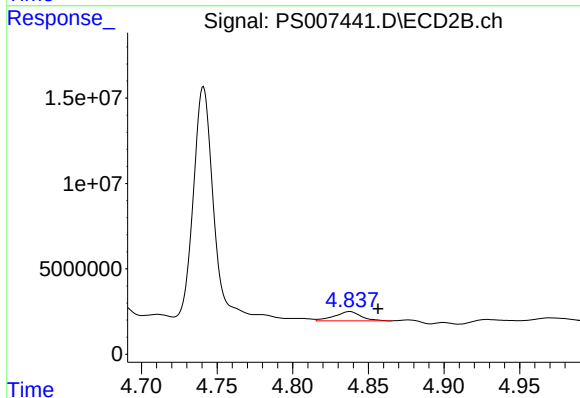


#3 4-Nitrophenol

R.T.: 4.838 min
Delta R.T.: -0.019 min
Response: 6736686
Conc: 17.06 ng/ml

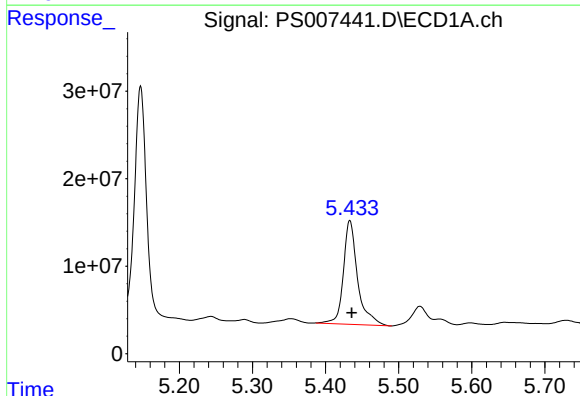


#4 2,4-DCAA

R.T.: 5.433 min
Delta R.T.: -0.002 min
Response: 160741300
Conc: 117.44 ng/ml

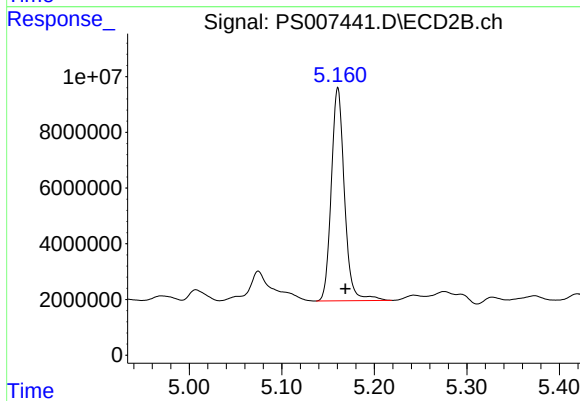

#4 2,4-DCAA


R.T.: 5.161 min
Delta R.T.: -0.008 min
Response: 75721861
Conc: 107.67 ng/ml

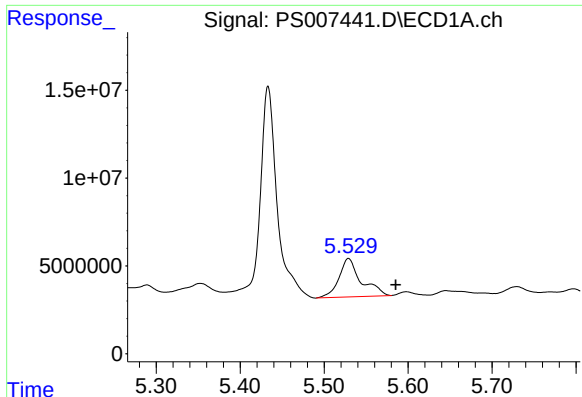

#5 DICAMBA


R.T.: 5.529 min
Delta R.T.: -0.056 min
Response: 40166138
Conc: 8.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

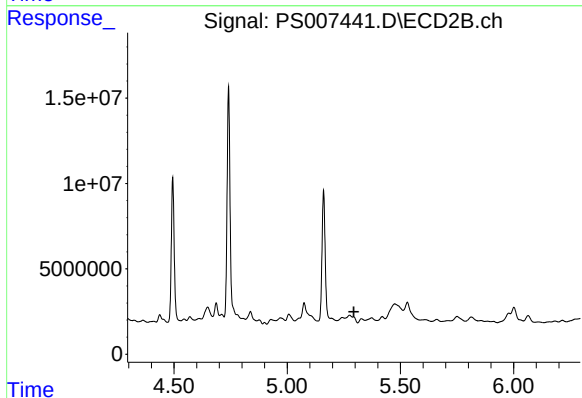


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

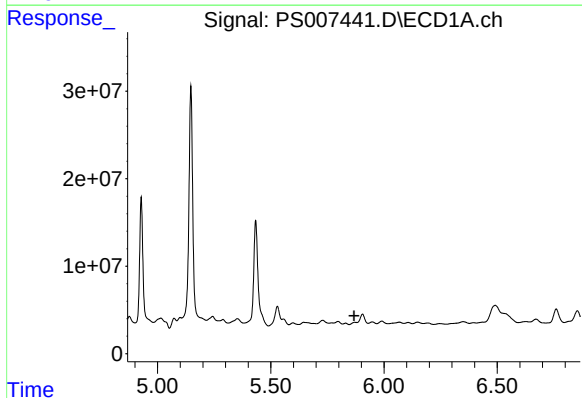


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

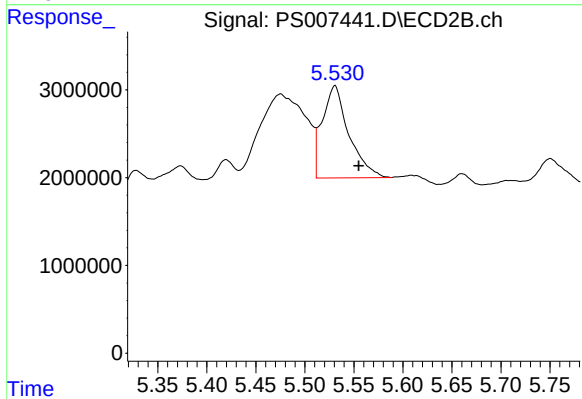

#7 MCPA


R.T.: 5.530 min
Delta R.T.: -0.024 min
Response: 19774819
Conc: 6.80 ug/ml

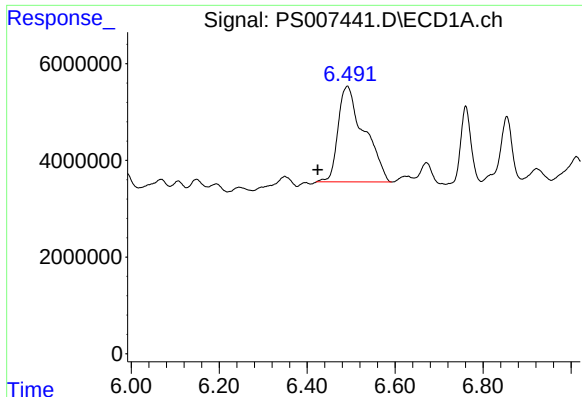

#9 2,4-D


R.T.: 6.491 min
Delta R.T.: 0.067 min
Response: 80935499
Conc: 65.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

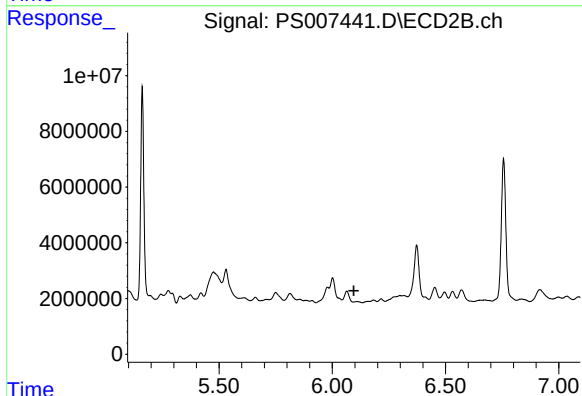


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

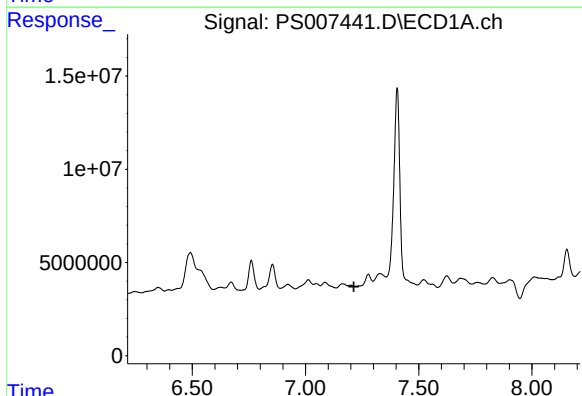


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

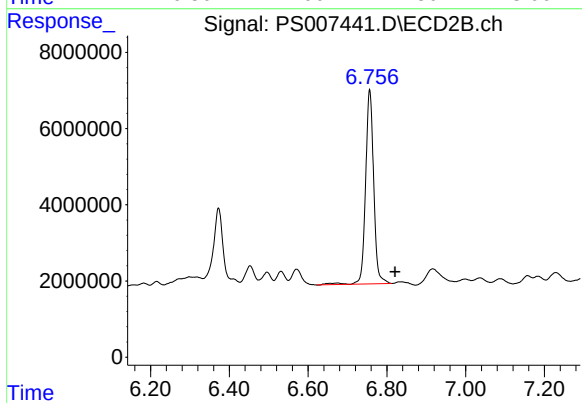

#11 2,4,5-TP (SILVEX)


R.T.: 6.756 min
Delta R.T.: -0.064 min
Response: 72991245
Conc: 19.19 ng/ml

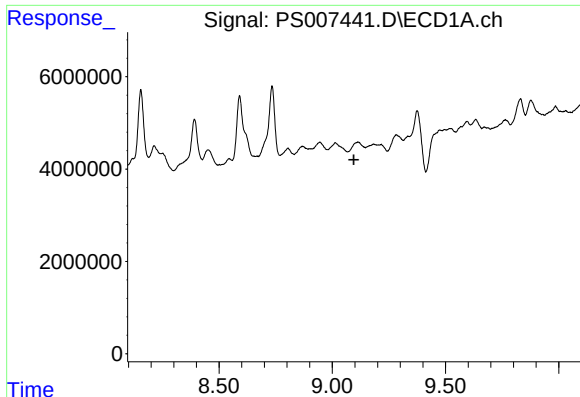

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

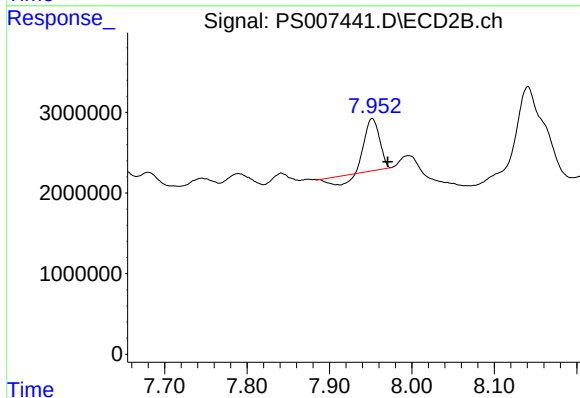


#14 DINOSEB

R.T.: 7.952 min
Delta R.T.: -0.019 min
Response: 6650125
Conc: 2.37 ng/ml

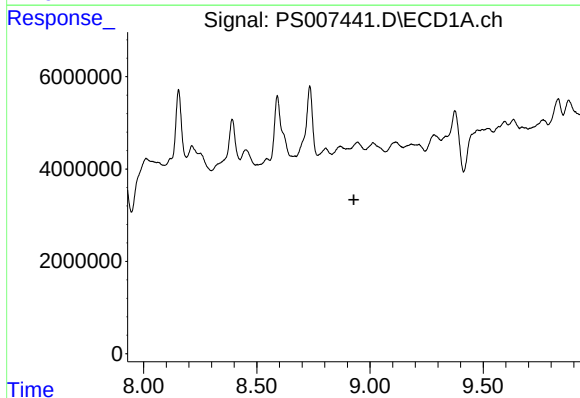

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

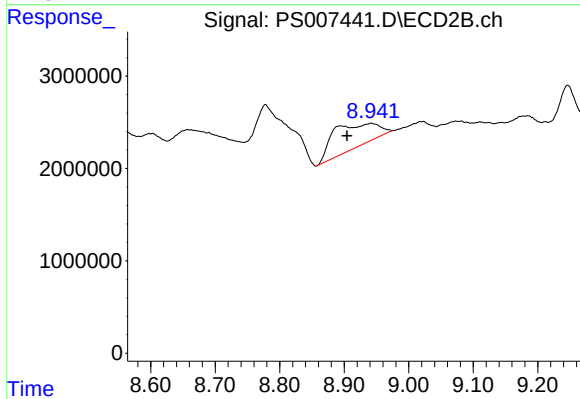

#15 Picloram

R.T.: 8.942 min
Delta R.T.: 0.037 min
Response: 12436398
Conc: 2.03 ng/ml