

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 17:13
 Operator : SM\AJ
 Sample : K5542-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:45:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.160	165.1E6	81766306	120.633	116.260
Target Compounds							
1) T	Dalapon	1.993	1.660	53612244	292.6E6	32.040	321.547 #
2) T	3,5-DICHL...	0.000	4.494	0	63655745	N.D.	73.981
3) T	4-Nitroph...	0.000	4.836	0	9171379	N.D.	23.225
5) T	DICAMBA	5.528	0.000	46464900	0	9.457	N.D. #
7) T	MCPA	0.000	5.529	0	25177608	N.D.	8.661
9) T	2,4-D	6.489	0.000	86557633	0	70.238	N.D. #
10) T	Pentachlo...	6.675	6.444	27378817	17595484	1.534	1.830
11) T	2,4,5-TP ...	0.000	6.756	0	63173266	N.D.	16.609
14) T	DINOSEB	0.000	7.983	0	12741577	N.D.	4.539
15) T	Picloram	0.000	8.936	0	31420824	N.D.	5.117



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 17:13
Operator : SM\AJ
Sample : K5542-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:45:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

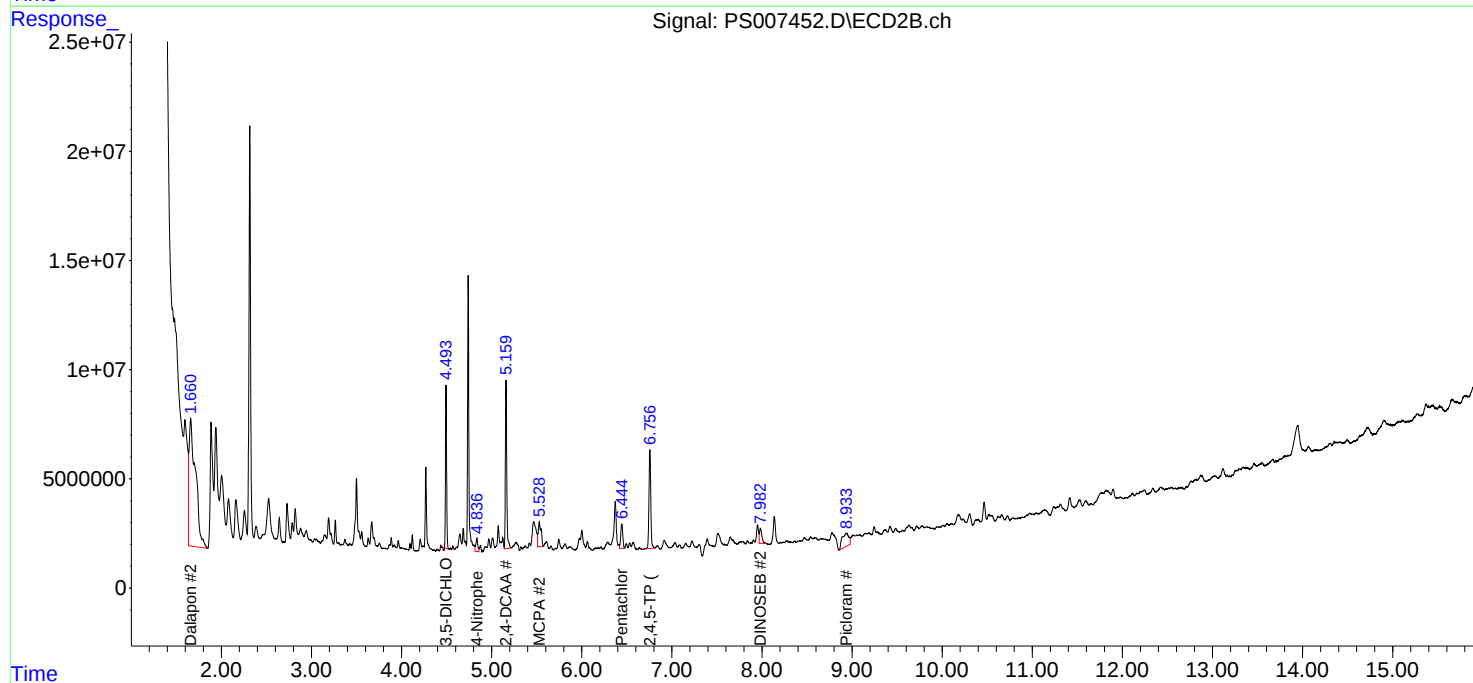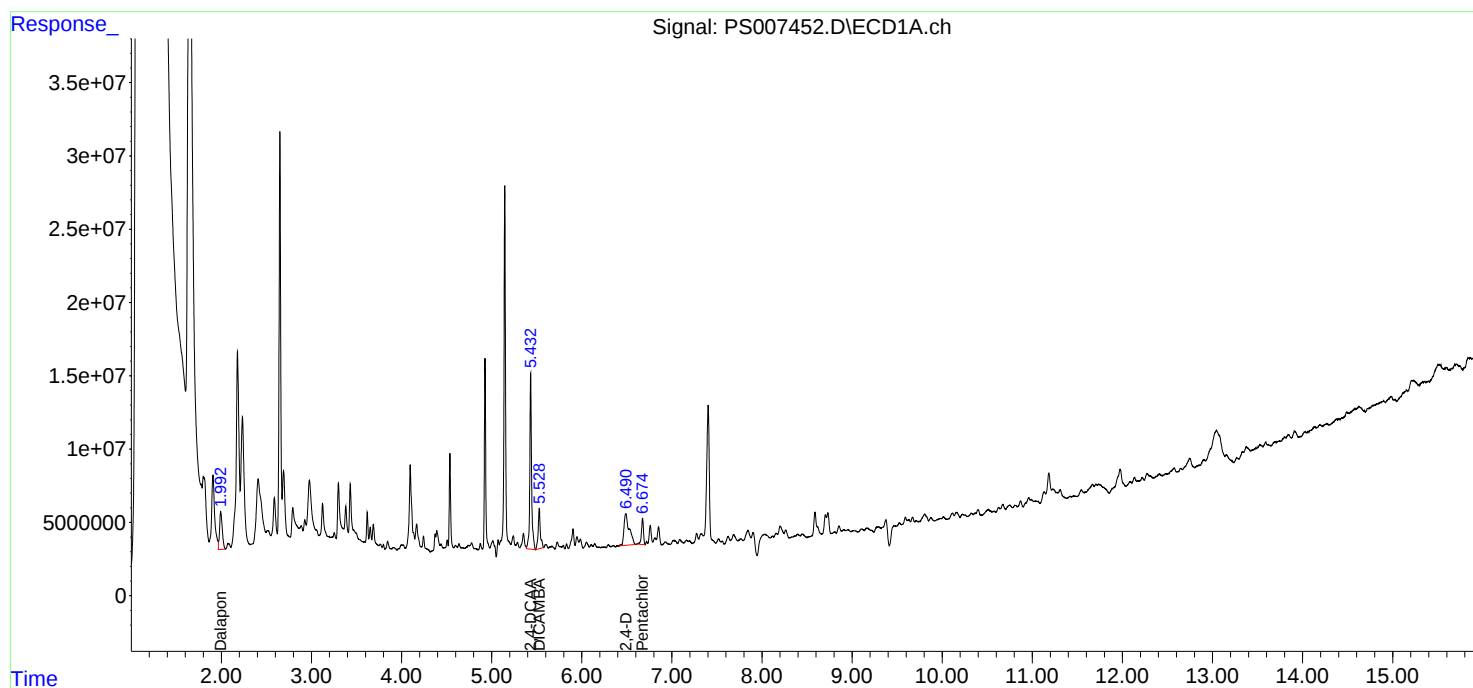


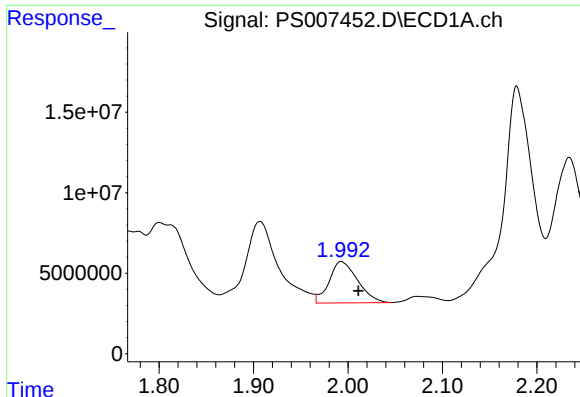

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.018 min
Response: 53612244
Conc: 32.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

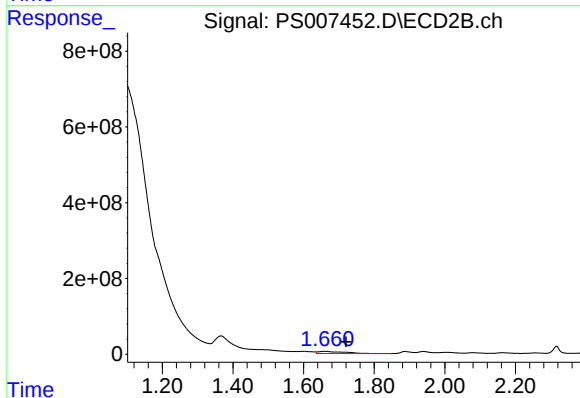


#1 Dalapon

R.T.: 1.660 min
Delta R.T.: -0.061 min
Response: 292608964
Conc: 321.55 ng/ml

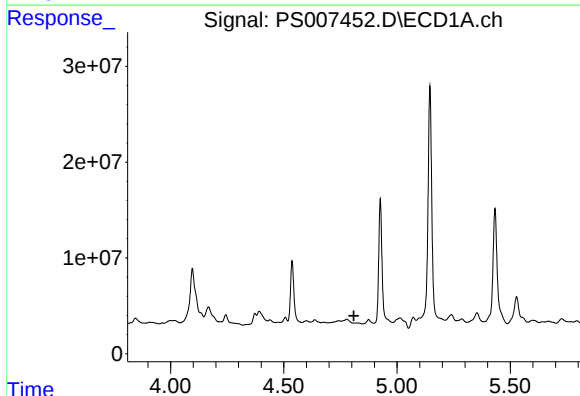


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

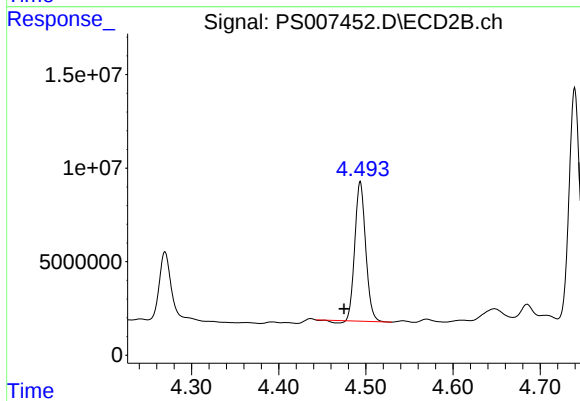

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.494 min
Delta R.T.: 0.019 min
Response: 63655745
Conc: 73.98 ng/ml

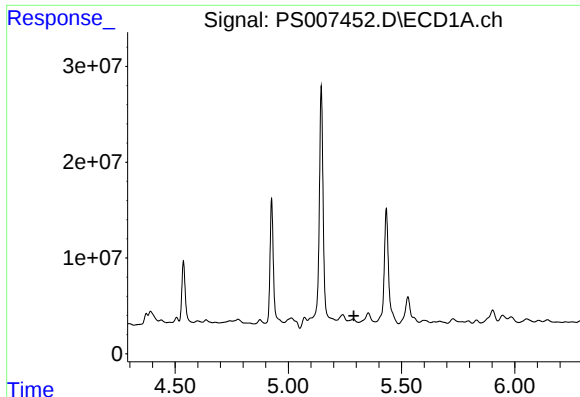

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

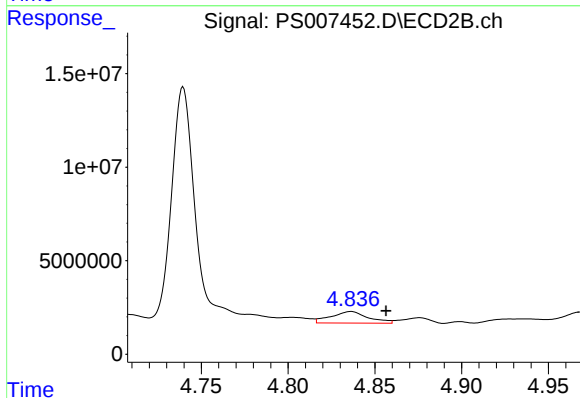


#3 4-Nitrophenol

R.T.: 4.836 min
Delta R.T.: -0.020 min
Response: 9171379
Conc: 23.22 ng/ml

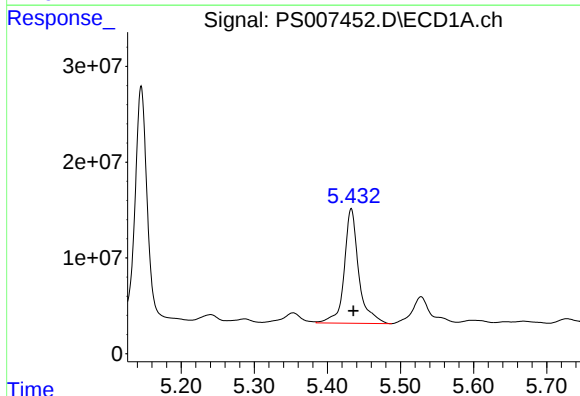


#4 2,4-DCAA

R.T.: 5.433 min
Delta R.T.: -0.003 min
Response: 165106535
Conc: 120.63 ng/ml

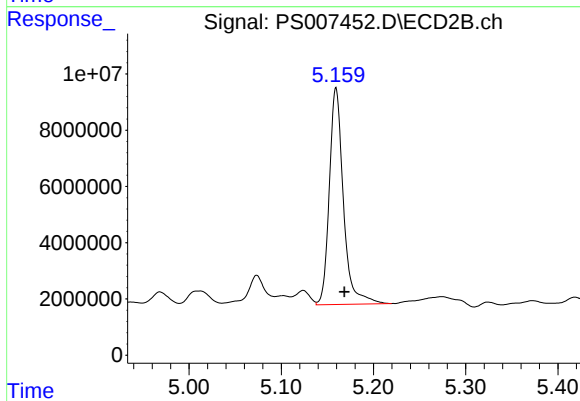

#4 2,4-DCAA


R.T.: 5.160 min
Delta R.T.: -0.009 min
Response: 81766306
Conc: 116.26 ng/ml

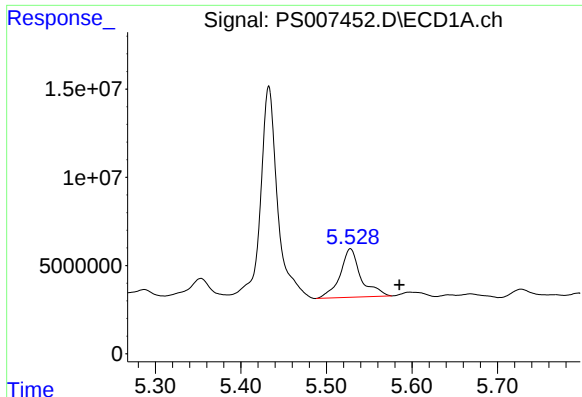

#5 DICAMBA


R.T.: 5.528 min
Delta R.T.: -0.057 min
Response: 46464900
Conc: 9.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

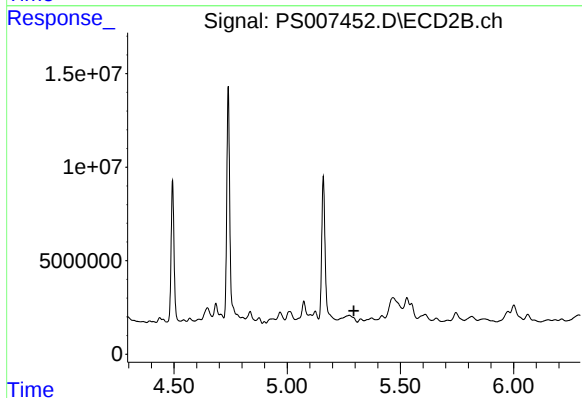


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

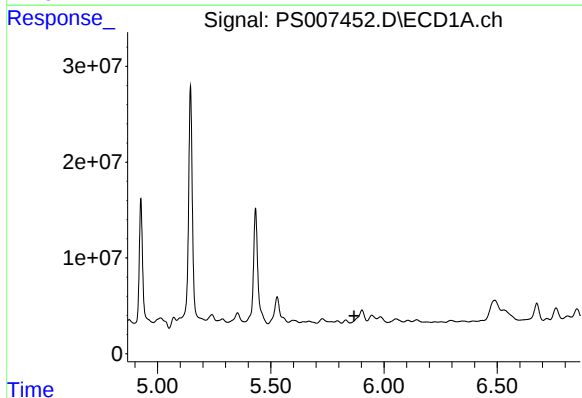


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

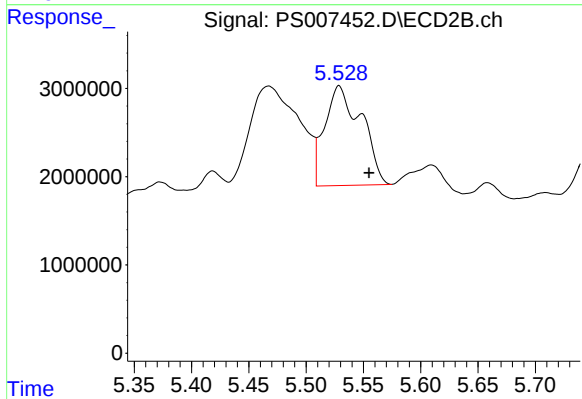

#7 MCPA


R.T.: 5.529 min
Delta R.T.: -0.026 min
Response: 25177608
Conc: 8.66 ug/ml

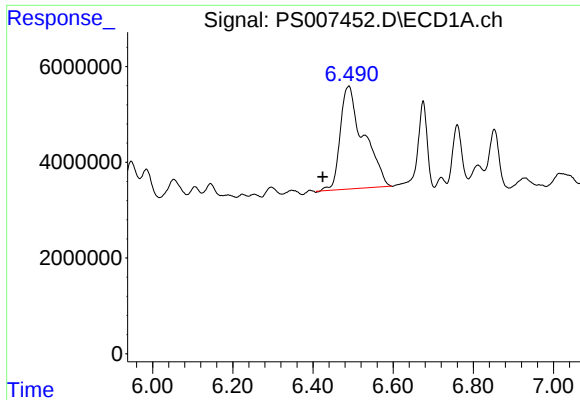

#9 2,4-D


R.T.: 6.489 min
Delta R.T.: 0.065 min
Response: 86557633
Conc: 70.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

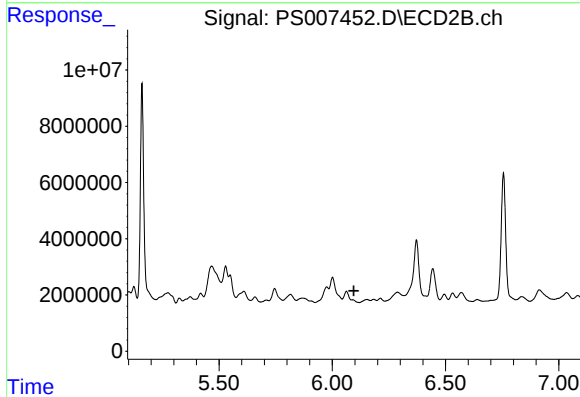


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

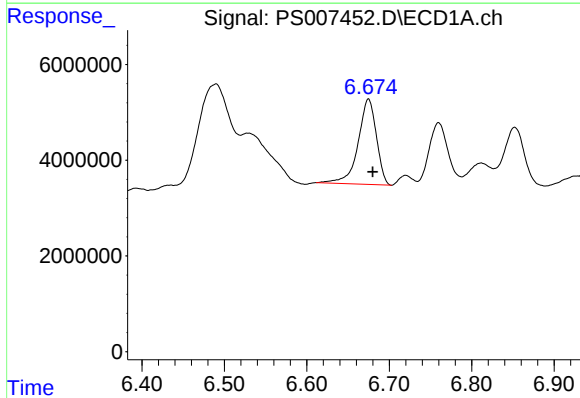


#10 Pentachlorophenol

R.T.: 6.675 min
Delta R.T.: -0.005 min
Response: 27378817
Conc: 1.53 ng/ml

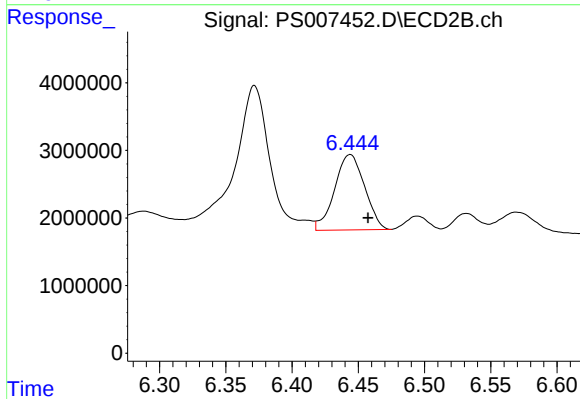

#10 Pentachlorophenol


R.T.: 6.444 min
Delta R.T.: -0.014 min
Response: 17595484
Conc: 1.83 ng/ml

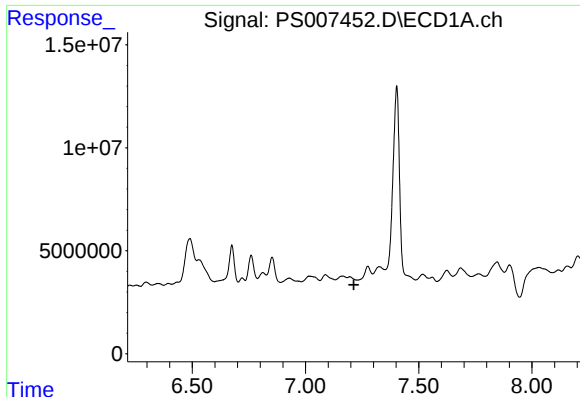

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

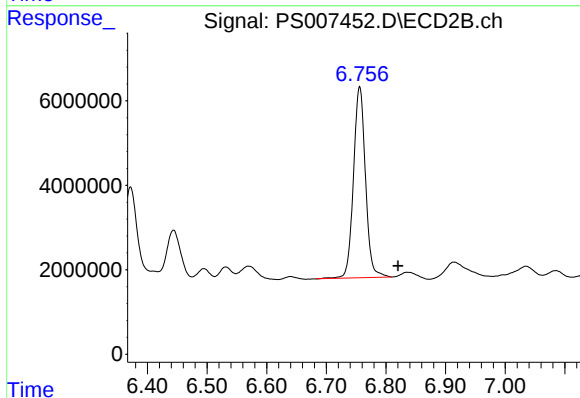


#11 2,4,5-TP (SILVEX)

R.T.: 6.756 min
Delta R.T.: -0.065 min
Response: 63173266
Conc: 16.61 ng/ml

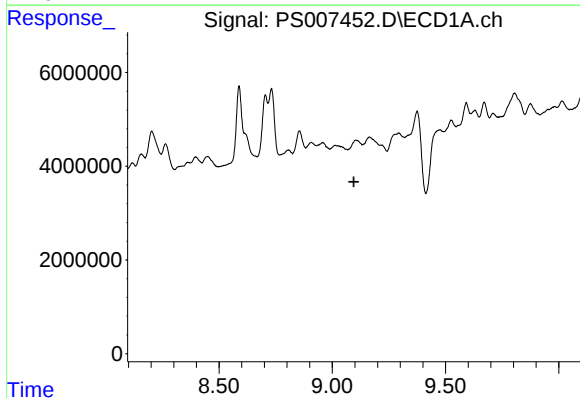


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

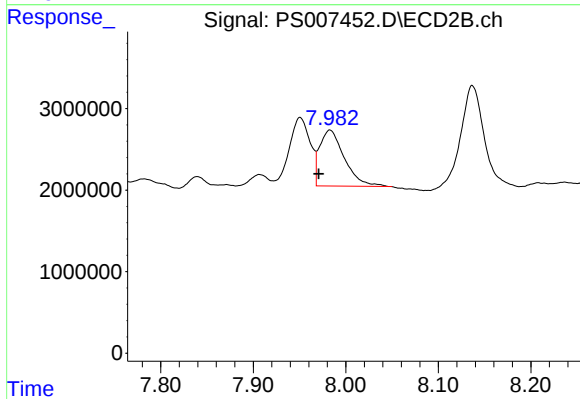

#14 DINOSEB


R.T.: 7.983 min
Delta R.T.: 0.012 min
Response: 12741577
Conc: 4.54 ng/ml

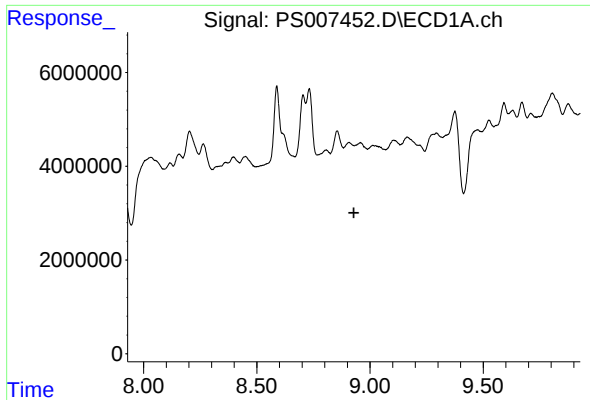

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

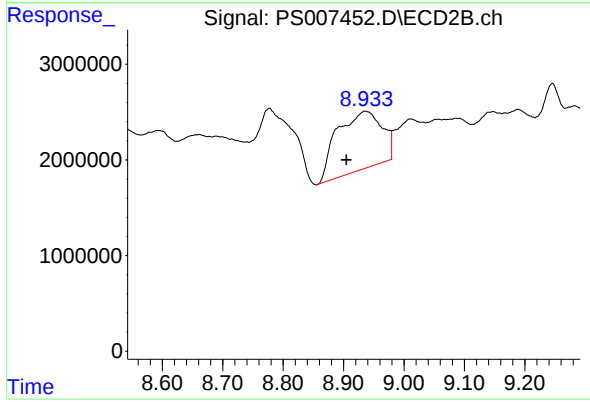

#15 Picloram

R.T.: 8.936 min
Delta R.T.: 0.032 min
Response: 31420824
Conc: 5.12 ng/ml