

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2019 20:09
 Operator : SM\AJ
 Sample : K5149-12
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-01-102819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 03:47:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.447	5.155	436.7E6	226.6E6	319.058	322.252
Target Compounds							
1) T	Dalapon	2.009	1.701	63781376	63349969	38.118	69.615 #
2) T	3,5-DICHL...	0.000	4.489	0	75787638	N.D.	88.081
3) T	4-Nitroph...	0.000	4.833	0	17643979	N.D.	44.680
5) T	DICAMBA	0.000	5.281	0	13202624	N.D.	5.074
9) T	2,4-D	0.000	6.060	0	8063462	N.D.	10.107
10) T	Pentachlo...	0.000	6.439	0	14503435	N.D.	1.508
11) T	2,4,5-TP ...	0.000	6.751	0	76411848	N.D.	20.089
12) T	2,4,5-T	7.418	0.000	211.2E6	0	27.626	N.D. #
15) T	Picloram	0.000	8.895	0	9817396	N.D.	1.599
16) T	DCPA	0.000	8.895	0	9817396	N.D.	1.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2019 20:09
Operator : SM\AJ
Sample : K5149-12
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 03:47:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

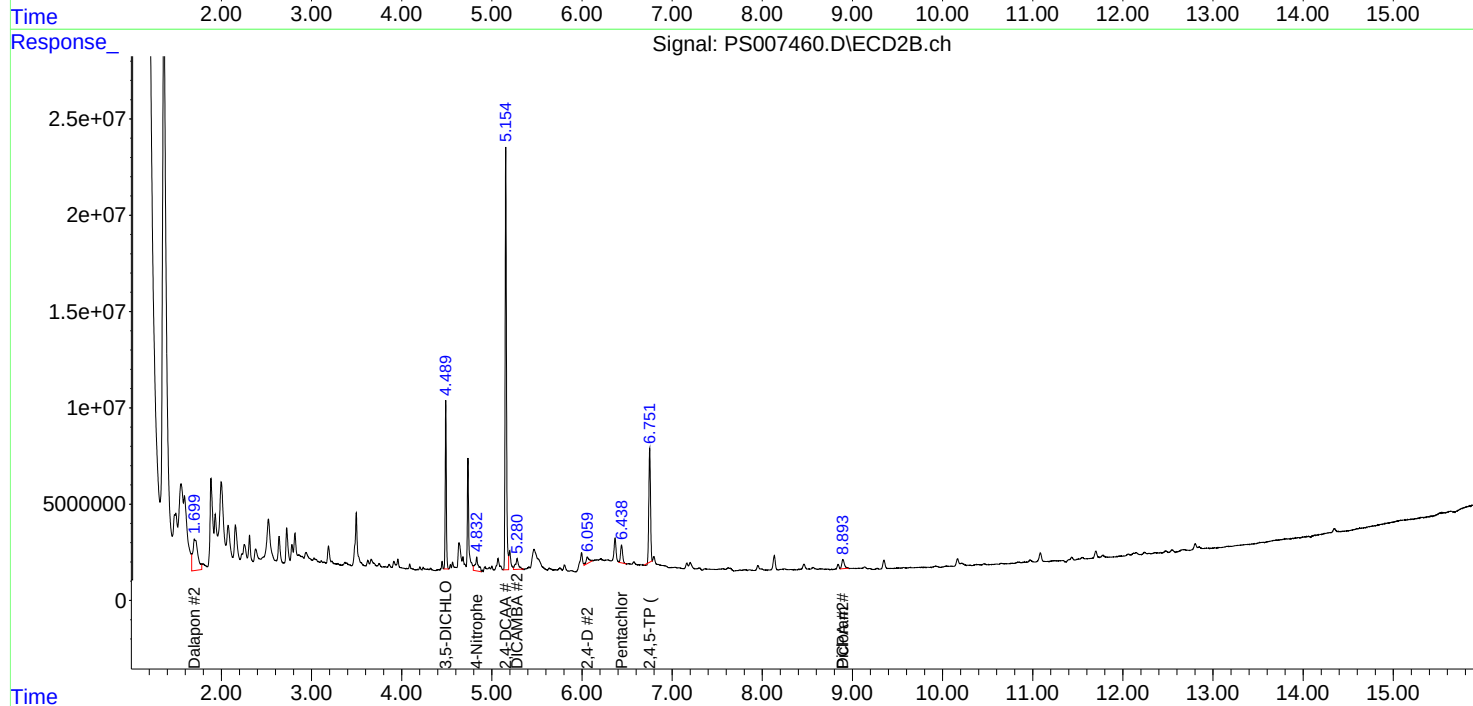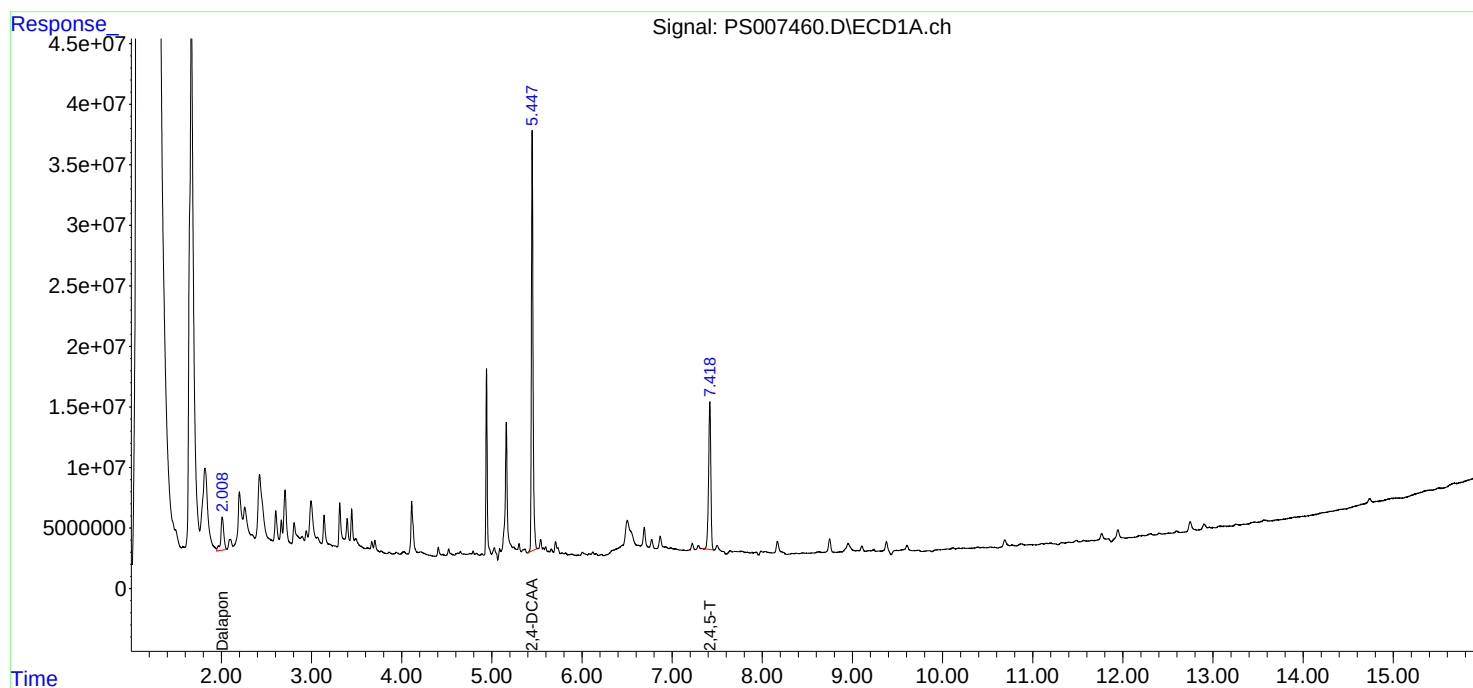


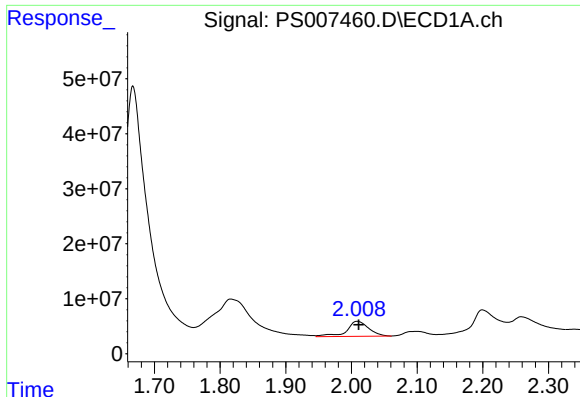

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.002 min
Response: 63781376
Conc: 38.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

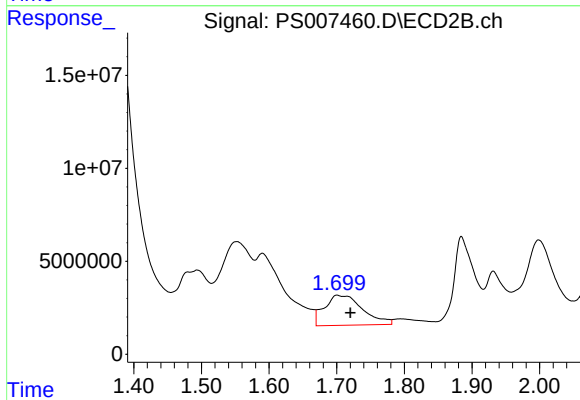


#1 Dalapon

R.T.: 1.701 min
Delta R.T.: -0.019 min
Response: 63349969
Conc: 69.62 ng/ml

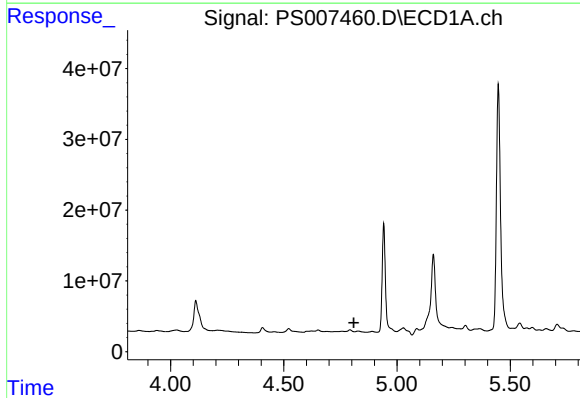


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

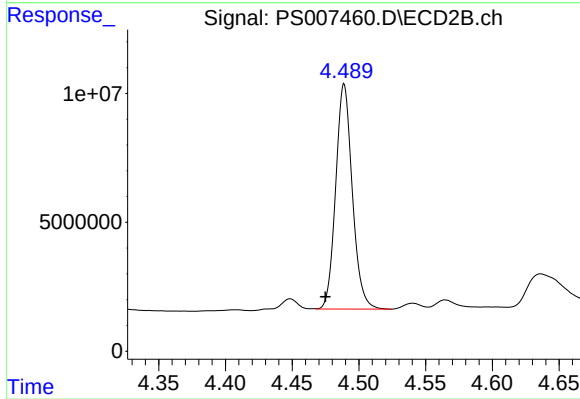

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.014 min
Response: 75787638
Conc: 88.08 ng/ml

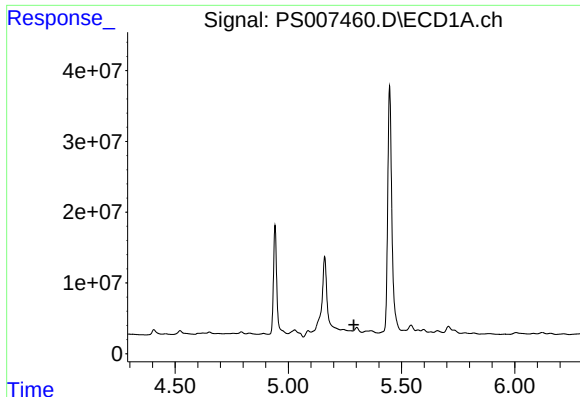

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

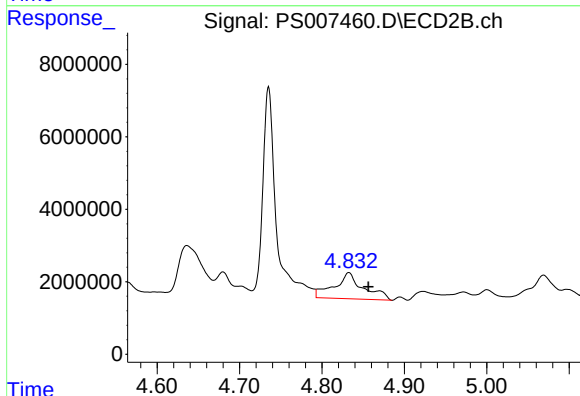


#3 4-Nitrophenol

R.T.: 4.833 min
Delta R.T.: -0.024 min
Response: 17643979
Conc: 44.68 ng/ml

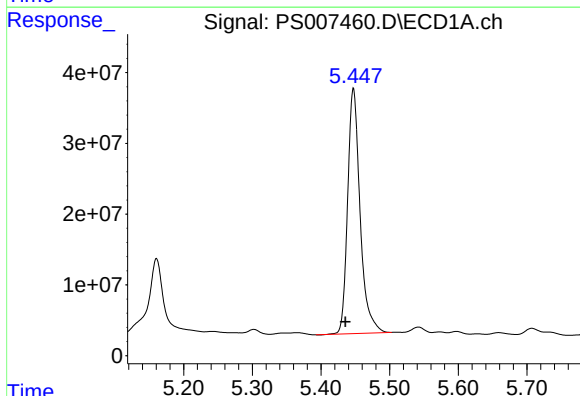


#4 2,4-DCAA

R.T.: 5.447 min
Delta R.T.: 0.012 min
Response: 436685085
Conc: 319.06 ng/ml

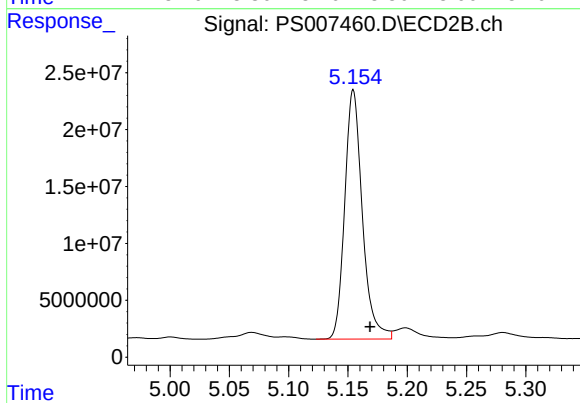

#4 2,4-DCAA


R.T.: 5.155 min
Delta R.T.: -0.014 min
Response: 226642262
Conc: 322.25 ng/ml

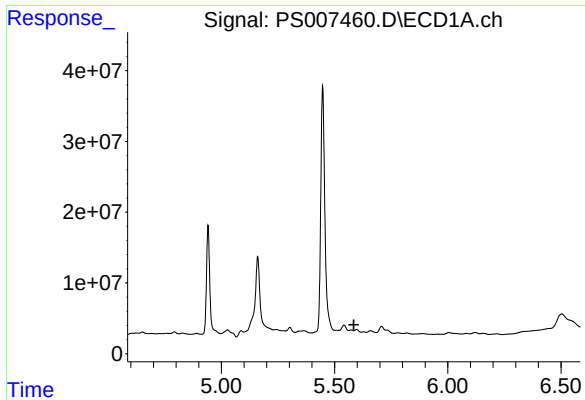

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

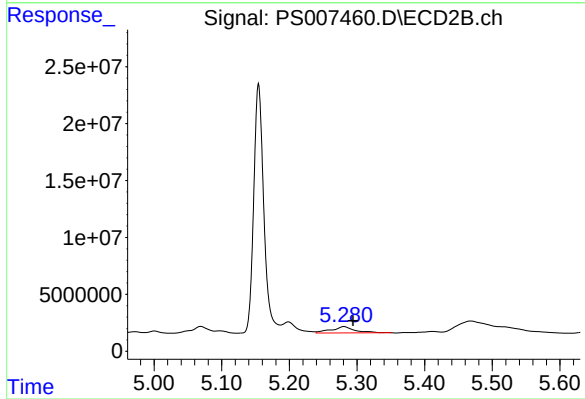


#5 DICAMBA

R.T.: 5.281 min
Delta R.T.: -0.014 min
Response: 13202624
Conc: 5.07 ng/ml

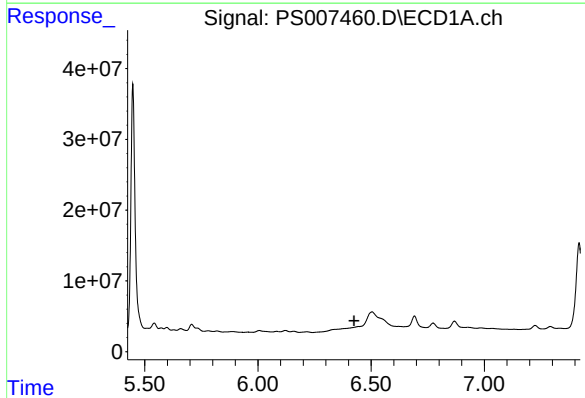


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

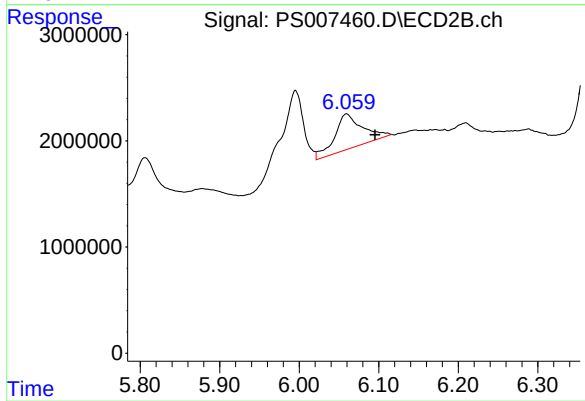

#9 2,4-D


R.T.: 6.060 min
Delta R.T.: -0.036 min
Response: 8063462
Conc: 10.11 ng/ml

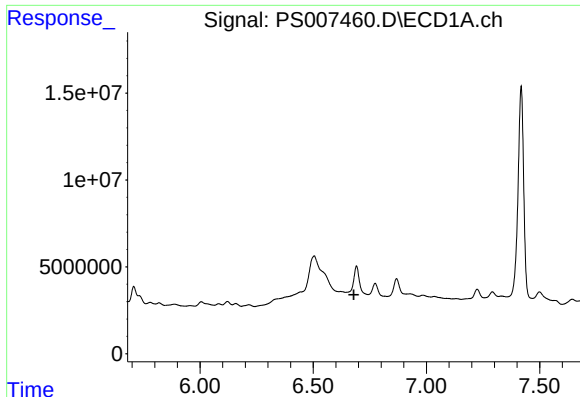

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

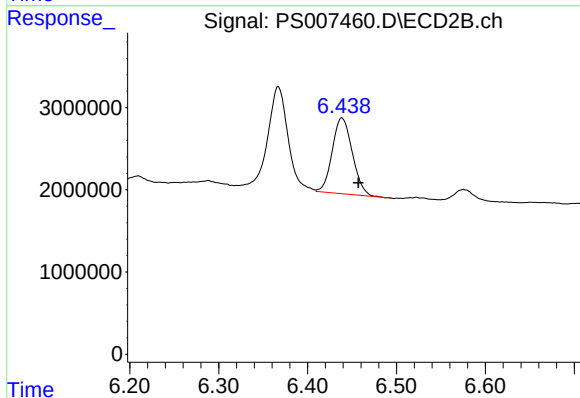


#10 Pentachlorophenol

R.T.: 6.439 min
Delta R.T.: -0.019 min
Response: 14503435
Conc: 1.51 ng/ml

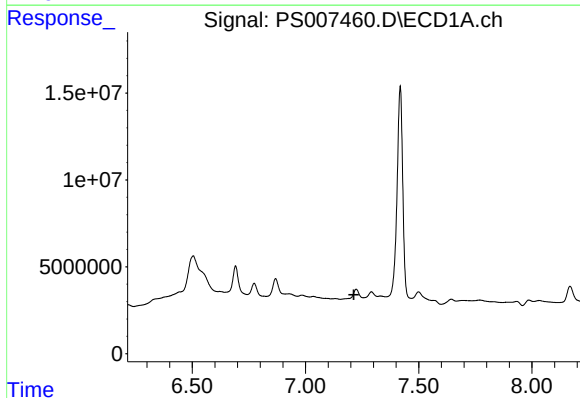


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

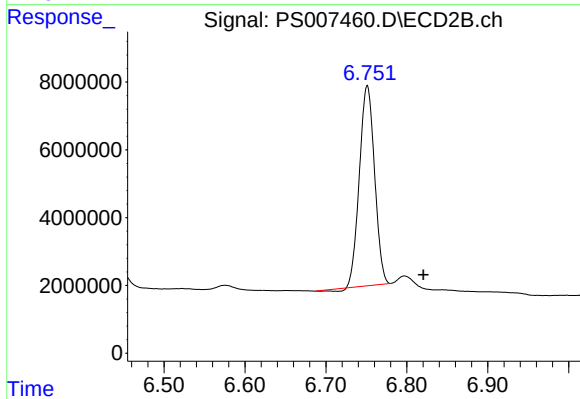

#11 2,4,5-TP (SILVEX)


R.T.: 6.751 min
Delta R.T.: -0.069 min
Response: 76411848
Conc: 20.09 ng/ml

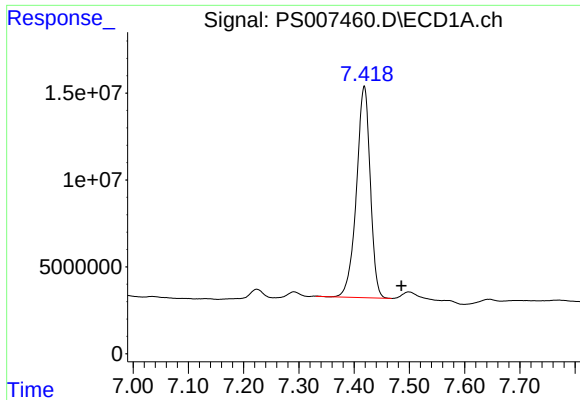

#12 2,4,5-T


R.T.: 7.418 min
Delta R.T.: -0.068 min
Response: 211191703
Conc: 27.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

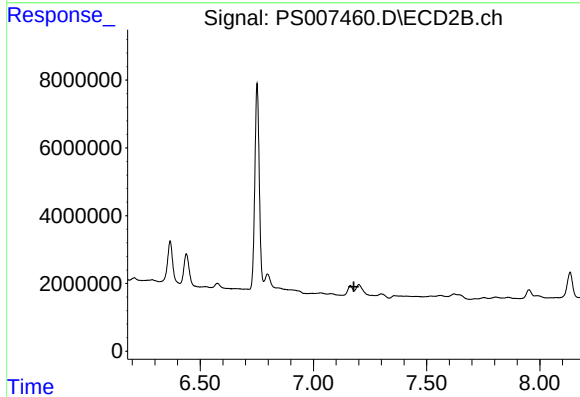


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.

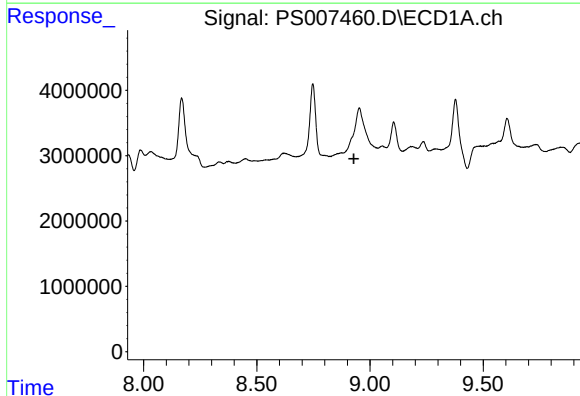


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

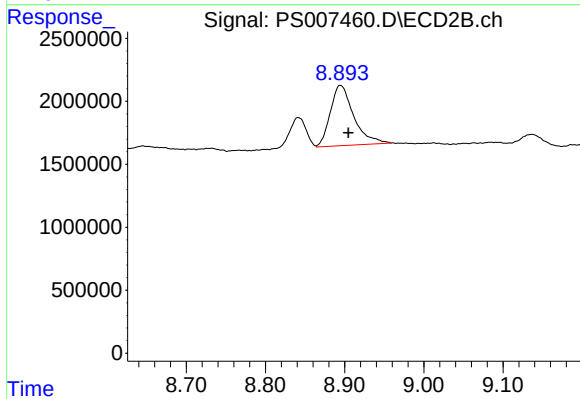

#15 Picloram


R.T.: 8.895 min
Delta R.T.: -0.010 min
Response: 9817396
Conc: 1.60 ng/ml

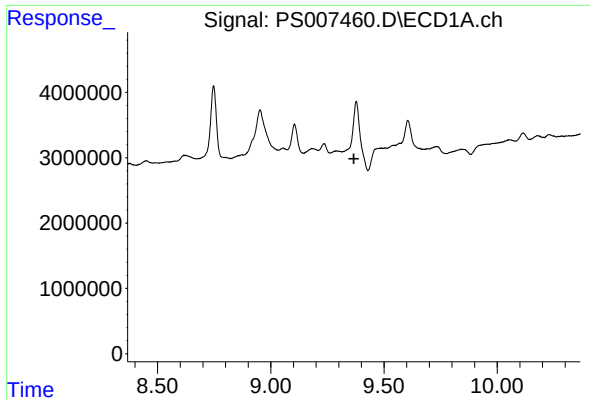

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-102819

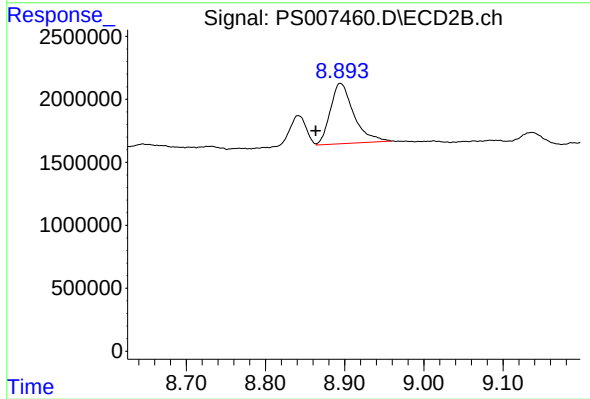

#16 DCPA

R.T.: 8.895 min
Delta R.T.: 0.032 min
Response: 9817396
Conc: 1.96 ng/ml