

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 04:33
 Operator : SM\AJ
 Sample : PB4388BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124388BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 05:00:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	5.157	749.0E6	407.2E6	547.259	579.004
Target Compounds							
2) T	3,5-DICHL...	0.000	4.492	0 40837058		N.D.	47.461
3) T	4-Nitroph...	0.000	4.841	0 26258934		N.D.	66.496
7) T	MCPA	5.808	0.000	59856199	0	11.605	N.D. #
8) T	DICHLORPROP	0.000	5.810	0 43032010		N.D.	66.079
9) T	2,4-D	6.483	0.000	80786670	0	65.555	N.D. #
11) T	2,4,5-TP ...	0.000	6.754	0 26551293		N.D.	6.981
15) T	Picloram	0.000	8.902	0 656474		N.D.	<MDL
16) T	DCPA	0.000	8.902	0 656474		N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 04:33
Operator : SM\AJ
Sample : PB4388BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124388BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 05:00:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

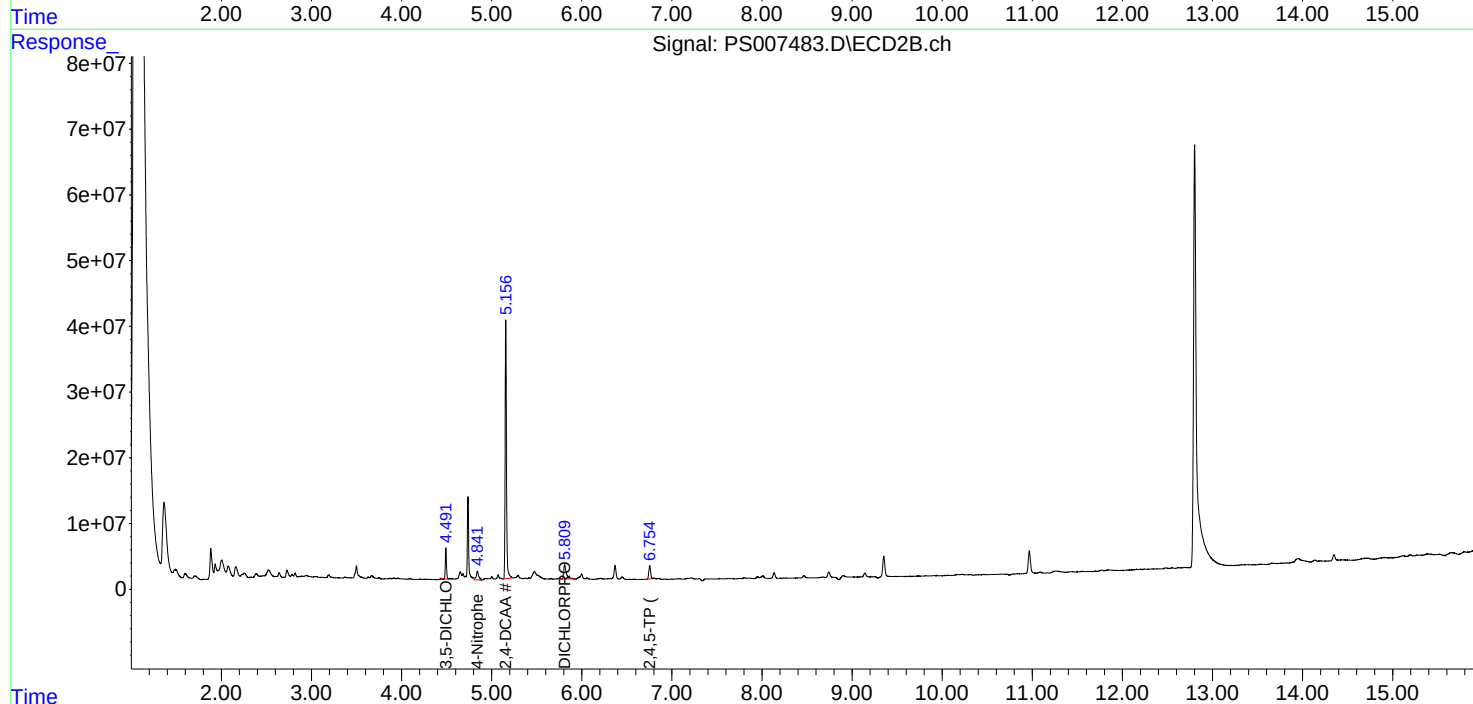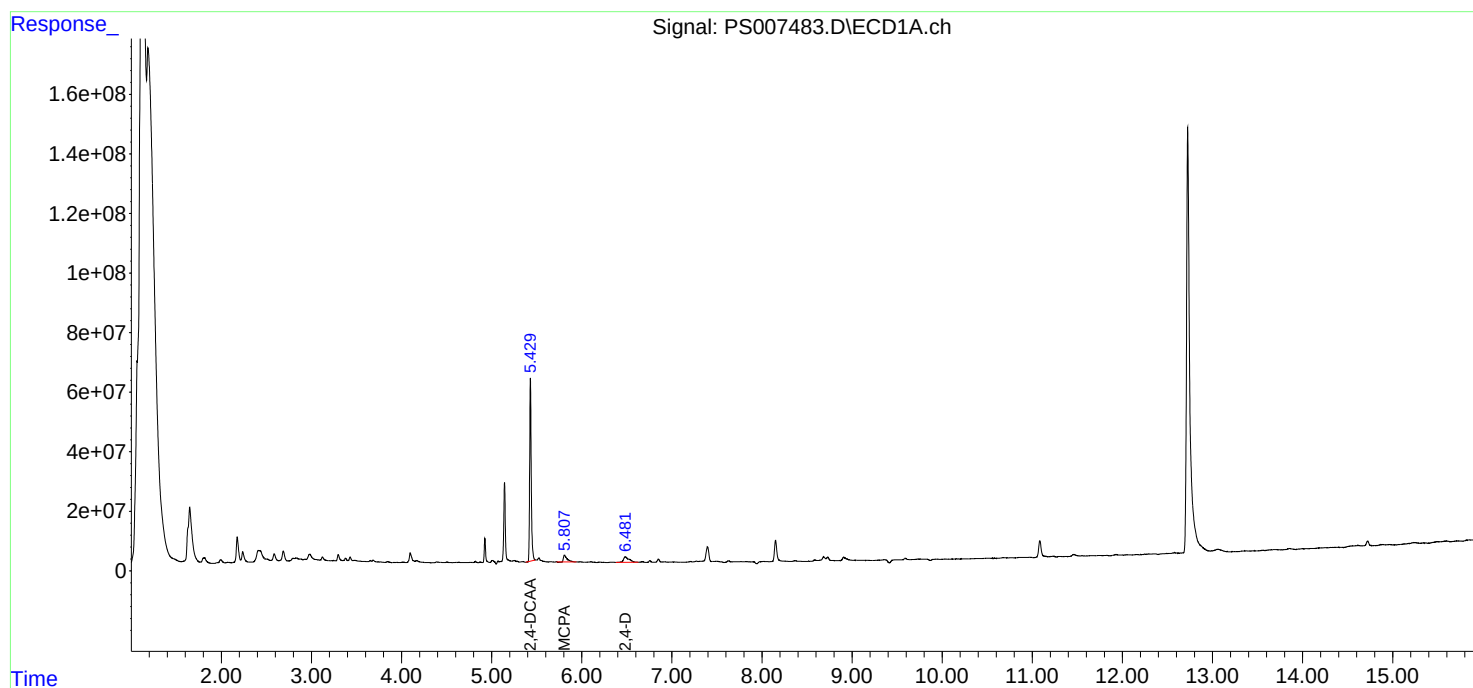


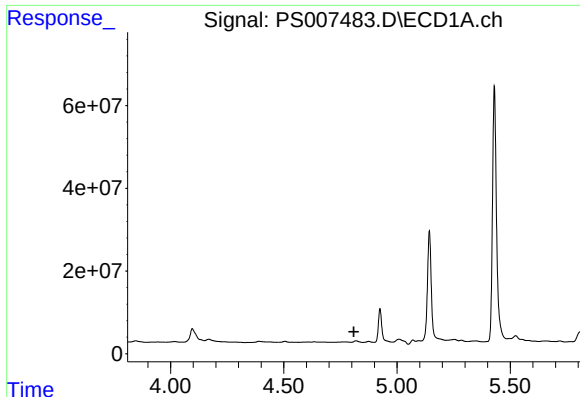

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124388BL

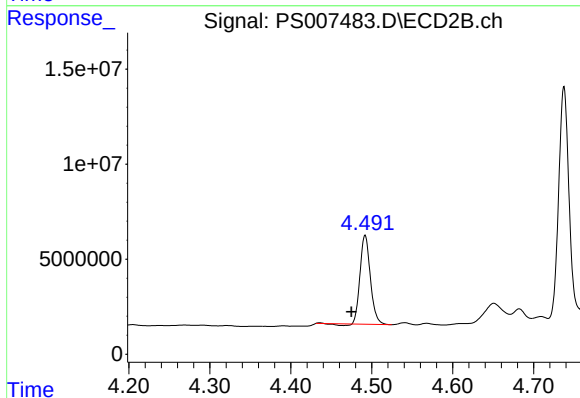


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.492 min
Delta R.T.: 0.017 min
Response: 40837058
Conc: 47.46 ng/ml

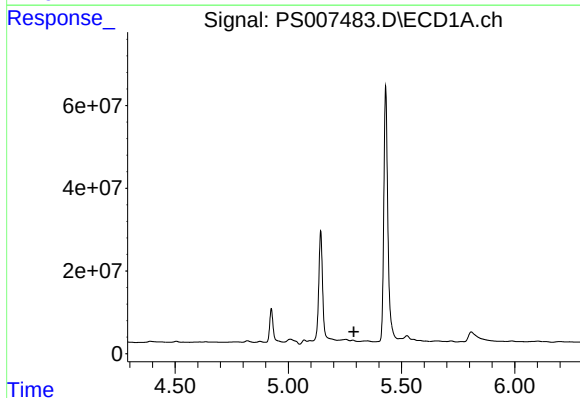


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

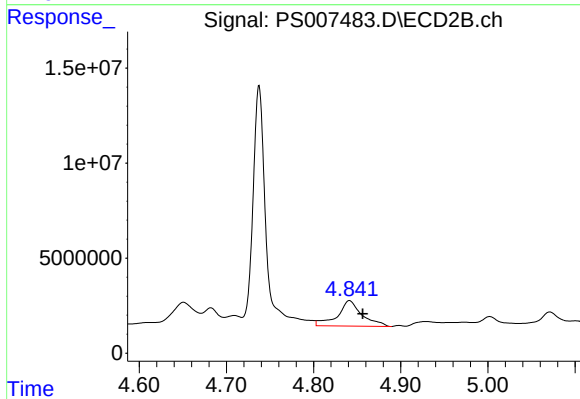

#3 4-Nitrophenol


R.T.: 4.841 min
Delta R.T.: -0.015 min
Response: 26258934
Conc: 66.50 ng/ml

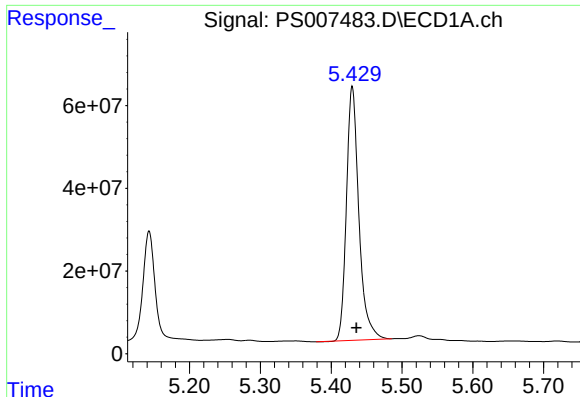

#4 2,4-DCAA


R.T.: 5.430 min
Delta R.T.: -0.006 min
Response: 749015962
Conc: 547.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124388BL

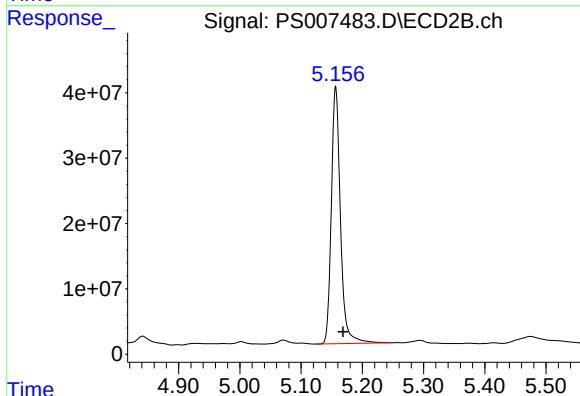


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: -0.012 min
Response: 407217172
Conc: 579.00 ng/ml

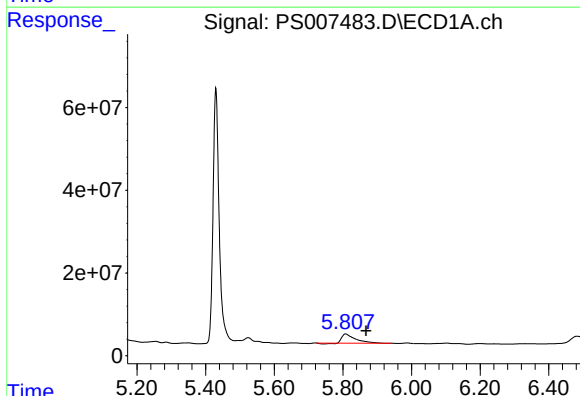


#7 MCPA

R.T.: 5.808 min
Delta R.T.: -0.059 min
Response: 59856199
Conc: 11.60 ug/ml

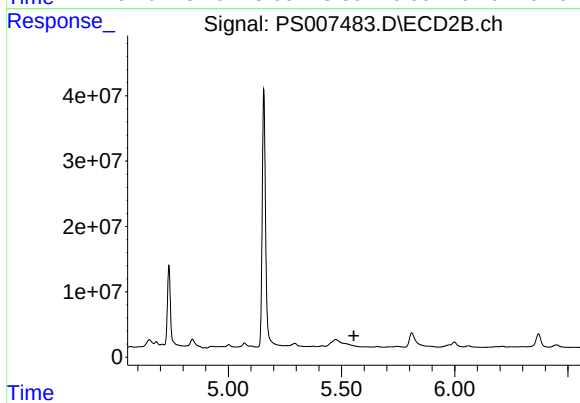

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

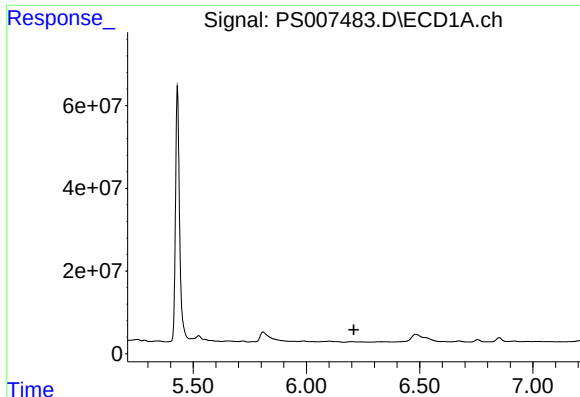

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124388BL

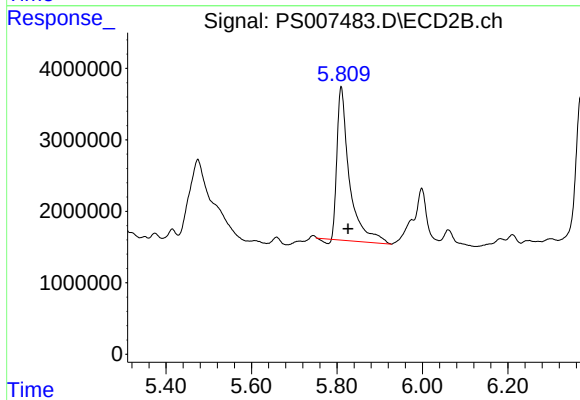


#8 DICHLORPROP

R.T.: 5.810 min
Delta R.T.: -0.016 min
Response: 43032010
Conc: 66.08 ng/ml

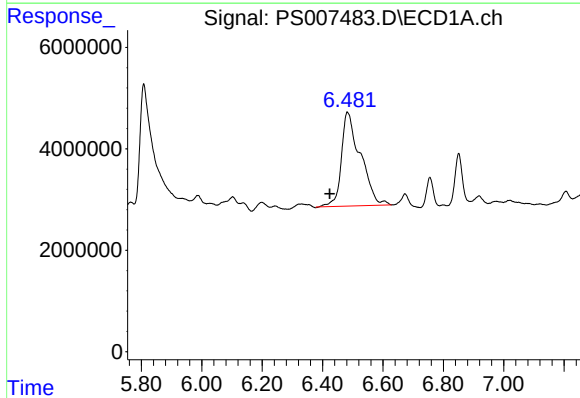


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.059 min
Response: 80786670
Conc: 65.56 ng/ml

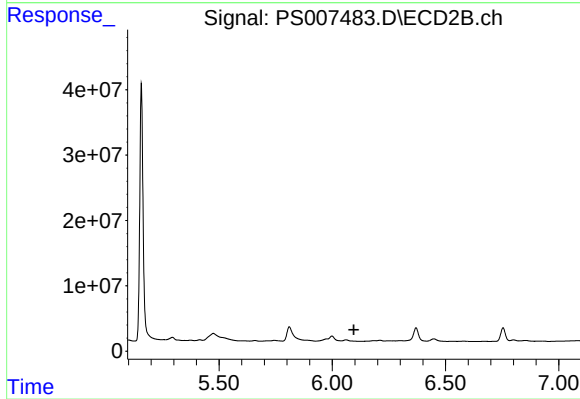

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

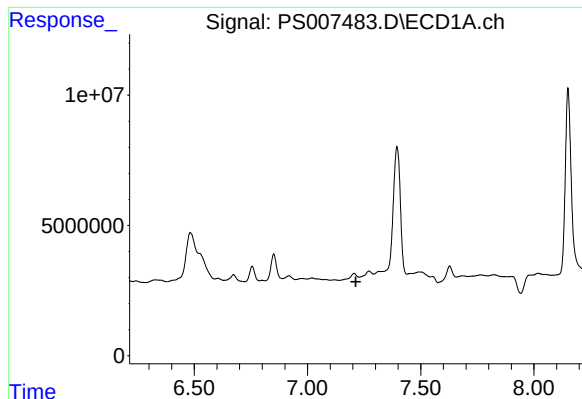

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124388BL

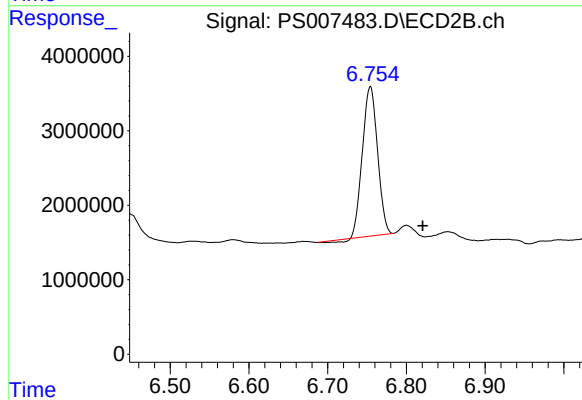

#11 2,4,5-TP (SILVEX)

R.T.: 6.754 min
Delta R.T.: -0.066 min
Response: 26551293
Conc: 6.98 ng/ml