

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 05:39
 Operator : SM\AJ
 Sample : PB124394BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124394BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 07:07:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.473	5.199	594.4E6	329.6E6	434.277	468.658
Target Compounds							
2) T	3,5-DICHL...	0.000	4.534	0	33466412	N.D.	38.895
5) T	DICAMBA	0.000	5.335	0	7647370	N.D.	2.939
6) T	MCP	0.000	5.335	0	7647370	N.D.	4.032
7) T	MCPA	0.000	5.515	0	47560698	N.D.	16.360
8) T	DICHLORPROP	0.000	5.858	0	8437749	N.D.	12.957
9) T	2,4-D	0.000	6.040	0	9290793	N.D.	11.646
10) T	Pentachlo...	0.000	6.483	0	13004637	N.D.	1.352
11) T	2,4,5-TP ...	0.000	6.796	0	19170129	N.D.	5.040
12) T	2,4,5-T	7.435	0.000	113.3E6	0	14.815	N.D. #
15) T	Picloram	8.981	8.940	206.8E6	129.8E6	18.739	21.139



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 05:39
Operator : SM\AJ
Sample : PB124394BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB124394BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 07:07:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

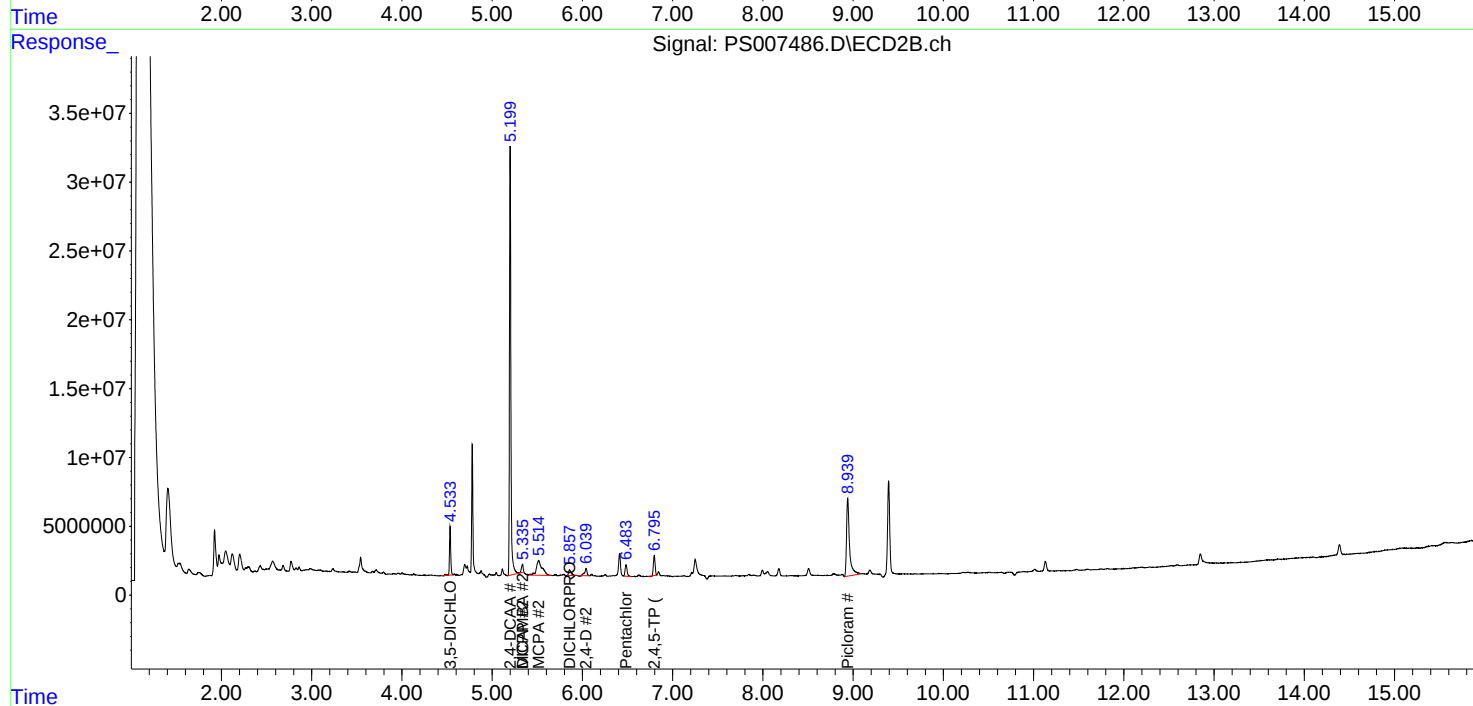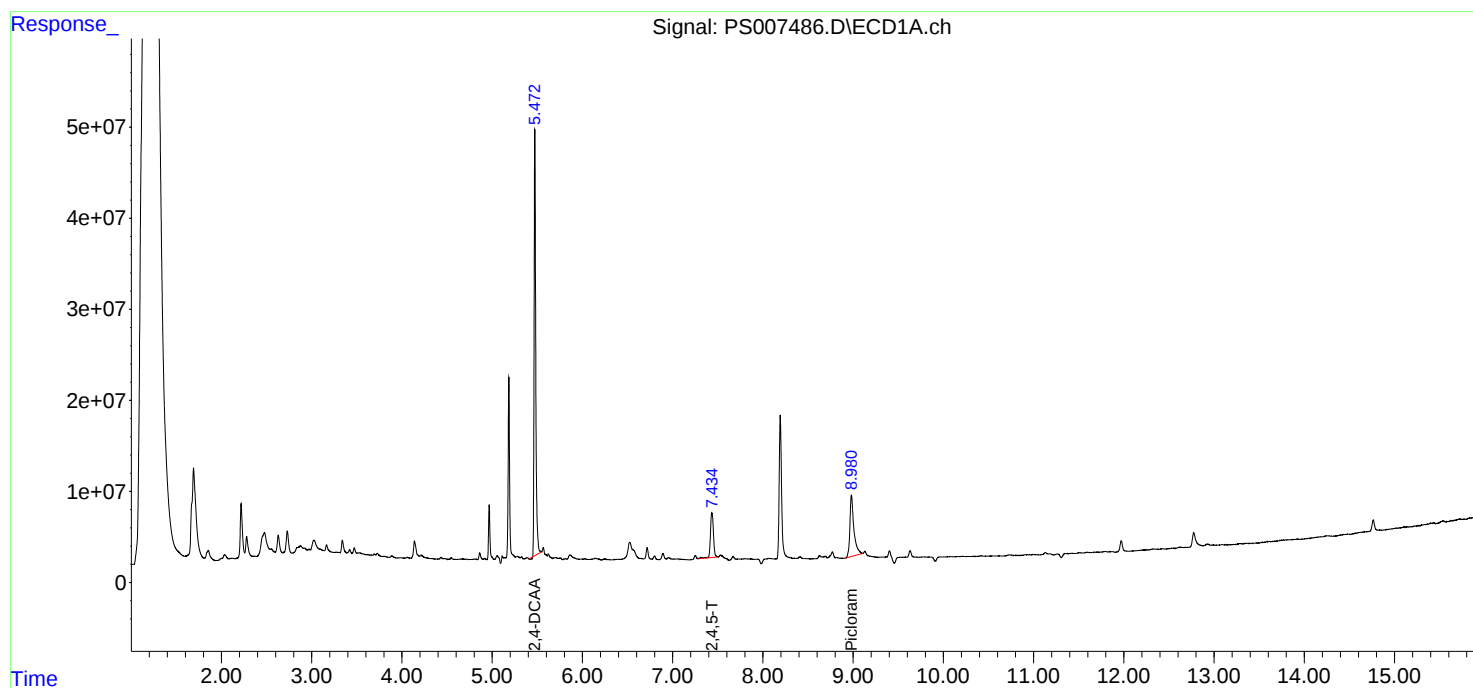


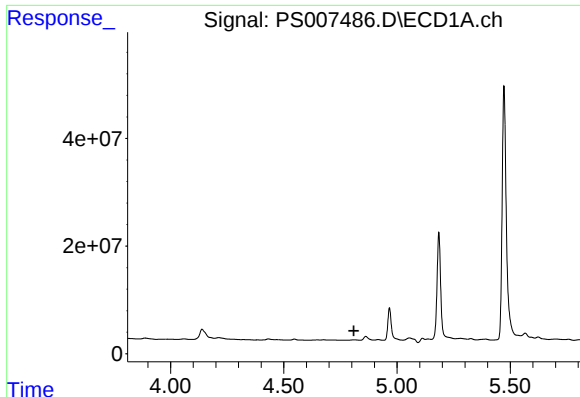

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394BL

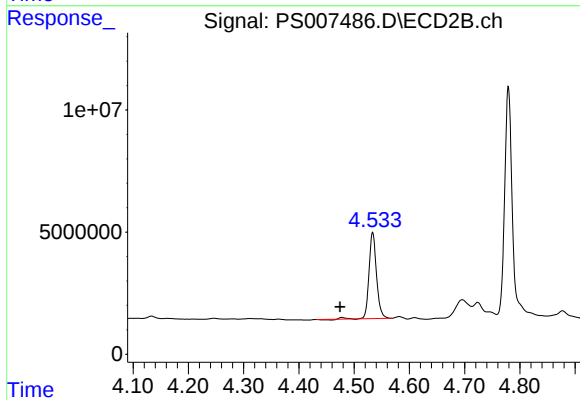


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.534 min
Delta R.T.: 0.059 min
Response: 33466412
Conc: 38.89 ng/ml

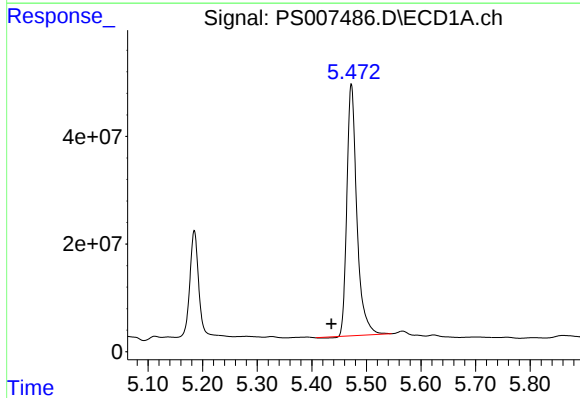


#4 2,4-DCAA

R.T.: 5.473 min
Delta R.T.: 0.037 min
Response: 594381932
Conc: 434.28 ng/ml

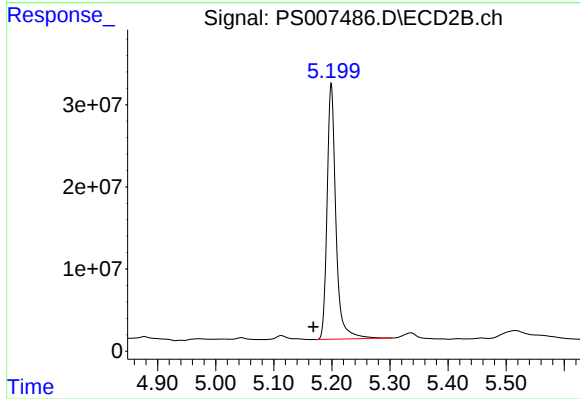

#4 2,4-DCAA


R.T.: 5.199 min
Delta R.T.: 0.030 min
Response: 329610064
Conc: 468.66 ng/ml

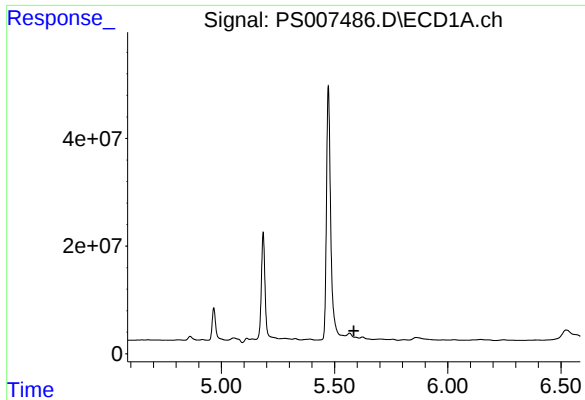

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394BL

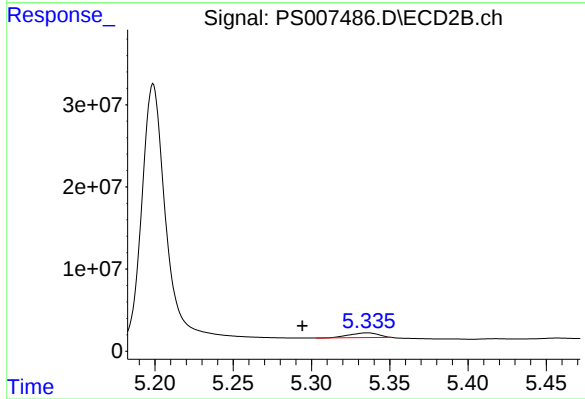


#5 DICAMBA

R.T.: 5.335 min
Delta R.T.: 0.041 min
Response: 7647370
Conc: 2.94 ng/ml

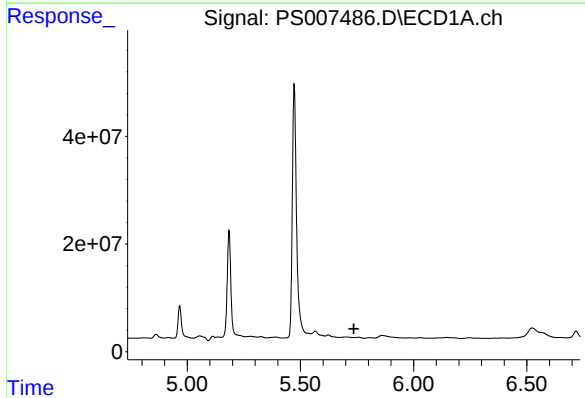


#6 MCP

R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

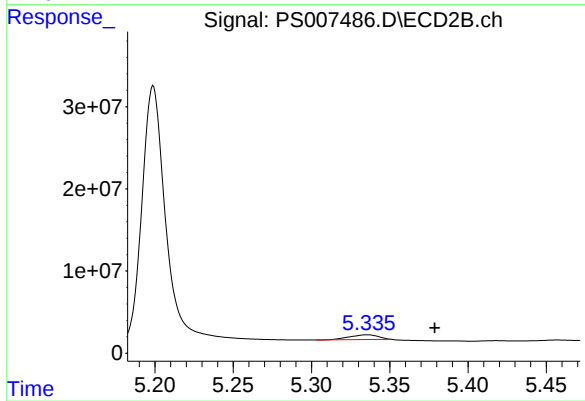

#6 MCP


R.T.: 5.335 min
Delta R.T.: -0.043 min
Response: 7647370
Conc: 4.03 ug/ml

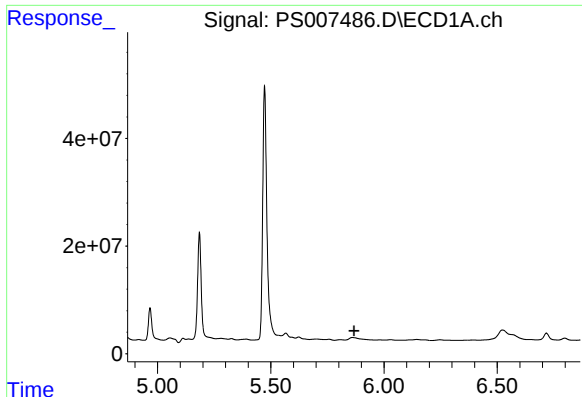

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394BL

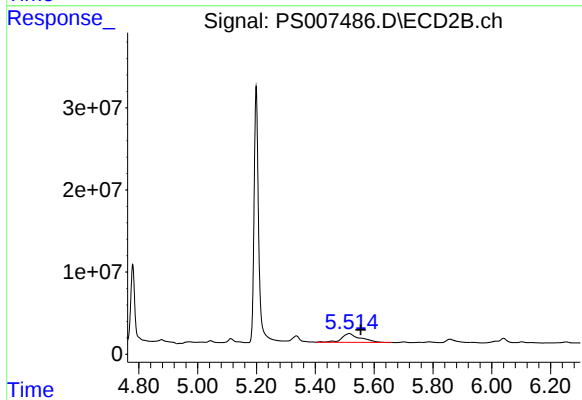


#7 MCPA

R.T.: 5.515 min
Delta R.T.: -0.040 min
Response: 47560698
Conc: 16.36 ug/ml

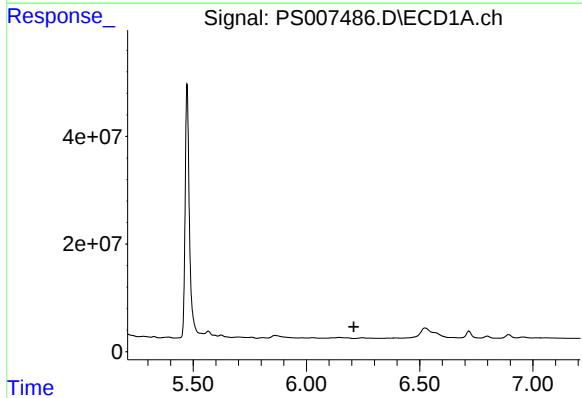


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

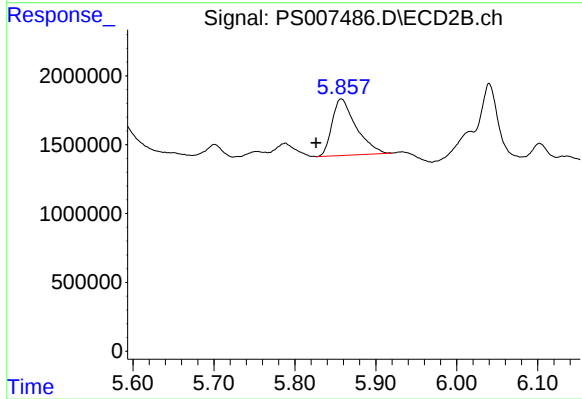

#8 DICHLORPROP


R.T.: 5.858 min
Delta R.T.: 0.031 min
Response: 8437749
Conc: 12.96 ng/ml

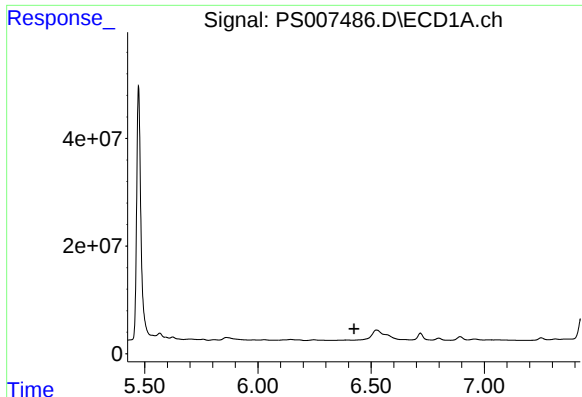

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394BL

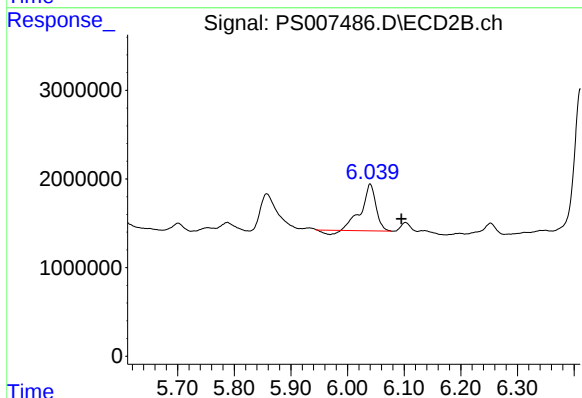


#9 2,4-D

R.T.: 6.040 min
Delta R.T.: -0.055 min
Response: 9290793
Conc: 11.65 ng/ml

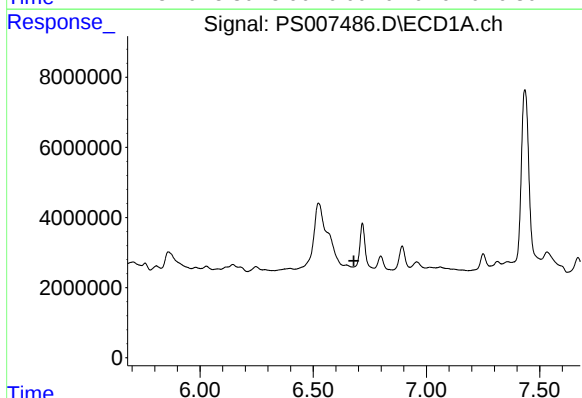


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

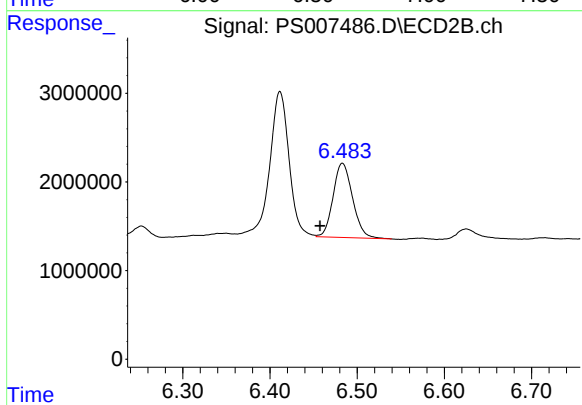

#10 Pentachlorophenol


R.T.: 6.483 min
Delta R.T.: 0.026 min
Response: 13004637
Conc: 1.35 ng/ml

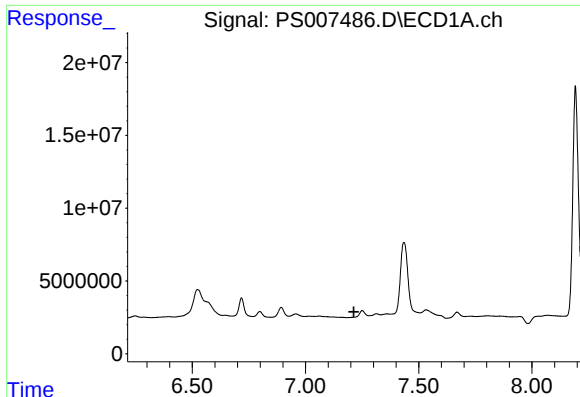

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394BL

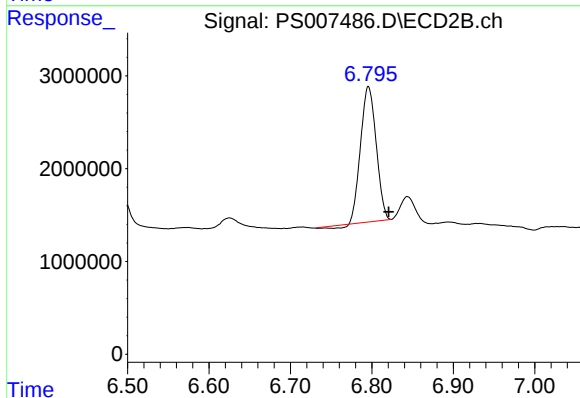


#11 2,4,5-TP (SILVEX)

R.T.: 6.796 min
Delta R.T.: -0.025 min
Response: 19170129
Conc: 5.04 ng/ml

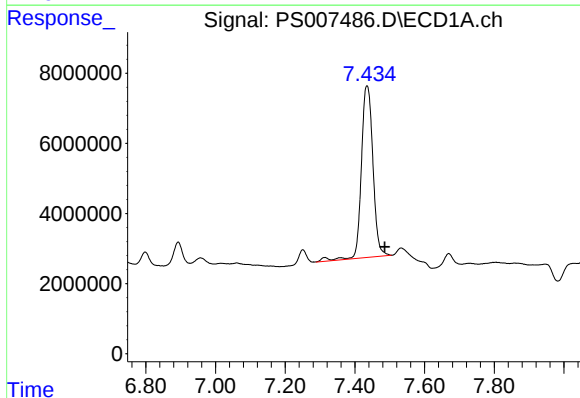


#12 2,4,5-T

R.T.: 7.435 min
Delta R.T.: -0.051 min
Response: 113255999
Conc: 14.81 ng/ml

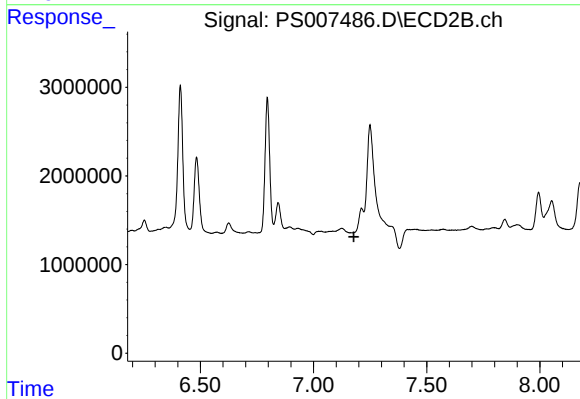

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.

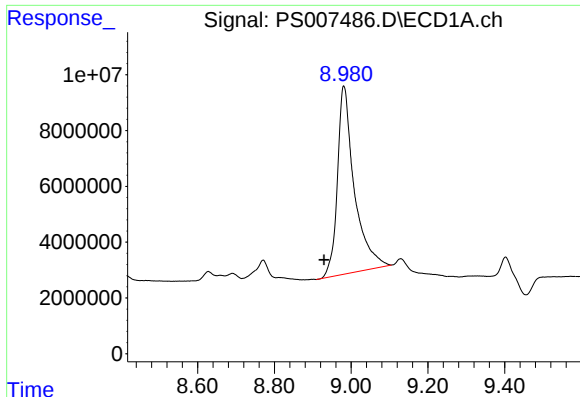

#15 Picloram

R.T.: 8.981 min
Delta R.T.: 0.052 min
Response: 206828648
Conc: 18.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124394BL

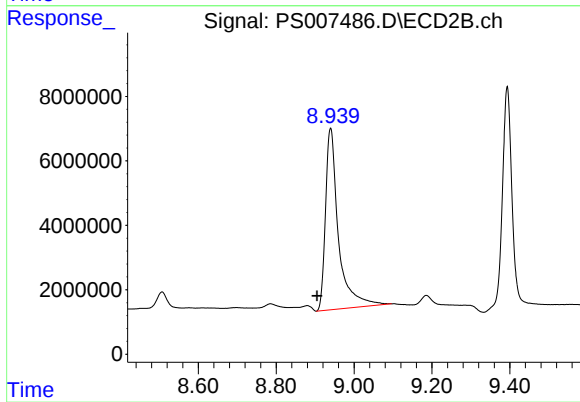

#15 Picloram

R.T.: 8.940 min
Delta R.T.: 0.035 min
Response: 129793895
Conc: 21.14 ng/ml