

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
 Data File : PS007488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 06:23
 Operator : SM\AJ
 Sample : PB124394BS
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124394TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 07:07:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.430	5.157	738.1E6	407.3E6	539.261	579.089
Target Compounds							
2) T	3,5-DICHL...	0.000	4.491	0	40745580	N.D.	47.355
3) T	4-Nitroph...	0.000	4.841	0	19605298	N.D.	49.647
7) T	MCPA	5.814	0.000	68980173	0	13.374	N.D. #
8) T	DICHLORPROP	0.000	5.812	0	47942829	N.D.	73.620
9) T	2,4-D	6.483	0.000	77177697	0	62.627	N.D. #
10) T	Pentachlo...	0.000	6.442	0	14986373	N.D.	1.558
11) T	2,4,5-TP ...	0.000	6.754	0	24428713	N.D.	6.423
12) T	2,4,5-T	0.000	7.208	0	44721304	N.D.	12.764
14) T	DINOSEB	0.000	7.951	0	3615380	N.D.	1.288
15) T	Picloram	8.940	8.897	185.3E6	102.3E6	16.786	16.653
16) T	DCPA	0.000	8.897	0	102.3E6	N.D.	20.390



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102919\
Data File : PS007488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 06:23
Operator : SM\AJ
Sample : PB124394BS
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124394TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 07:07:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

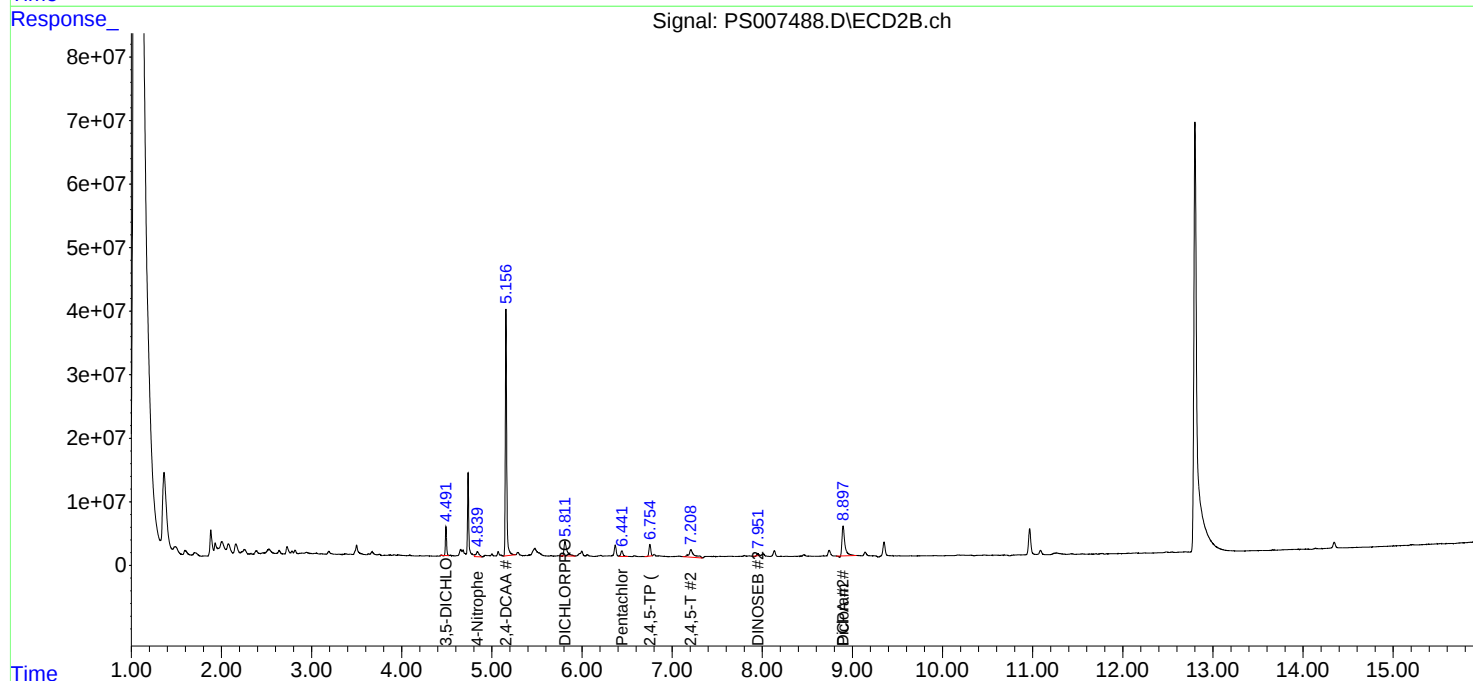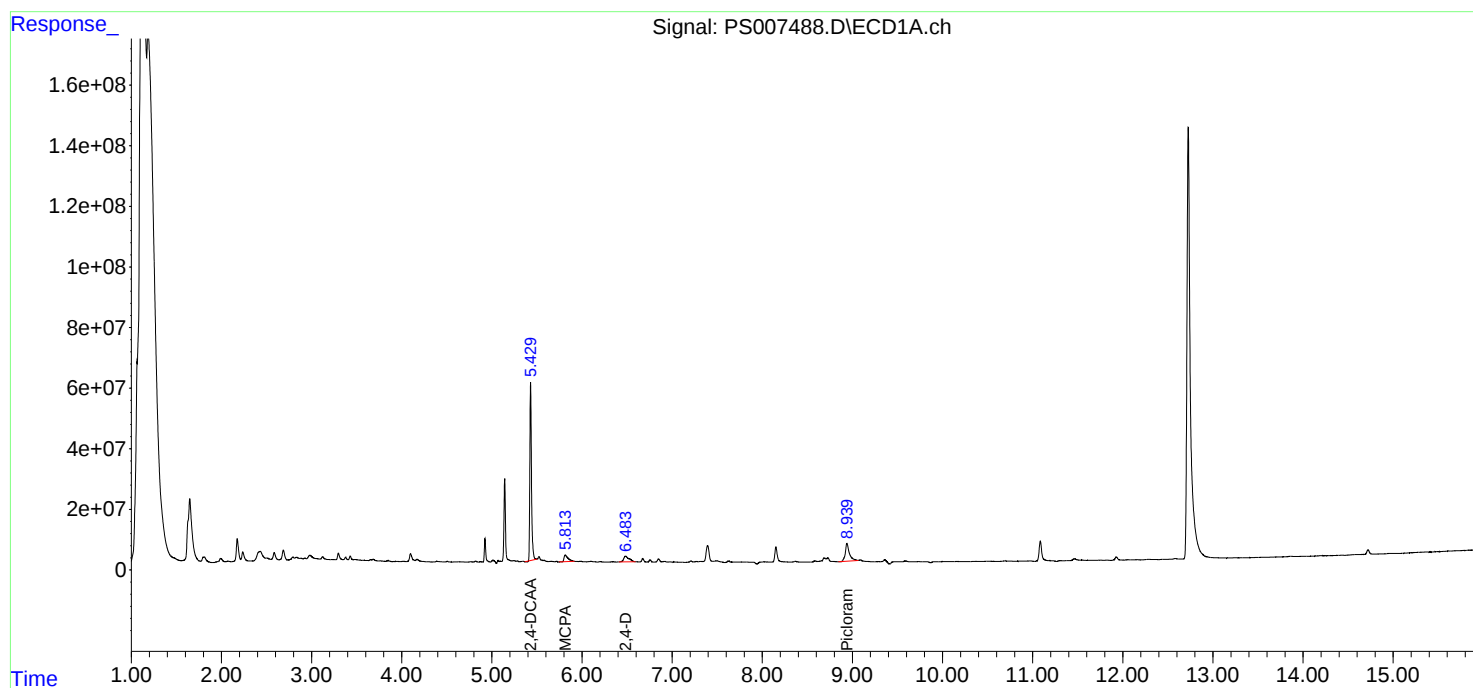


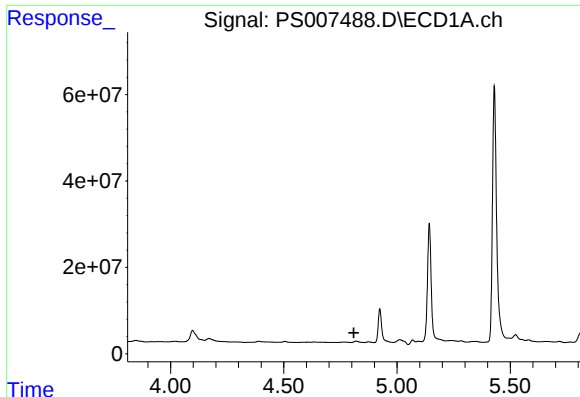

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394TB

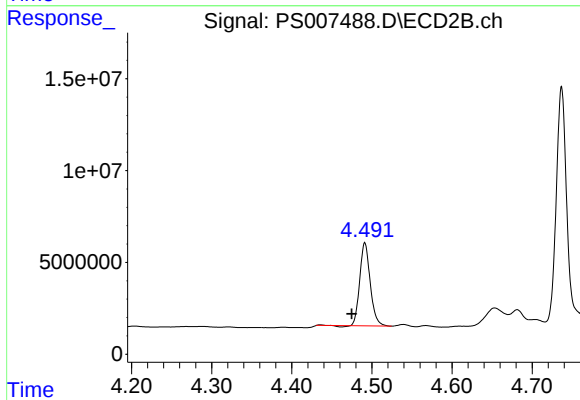


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.491 min
Delta R.T.: 0.017 min
Response: 40745580
Conc: 47.35 ng/ml

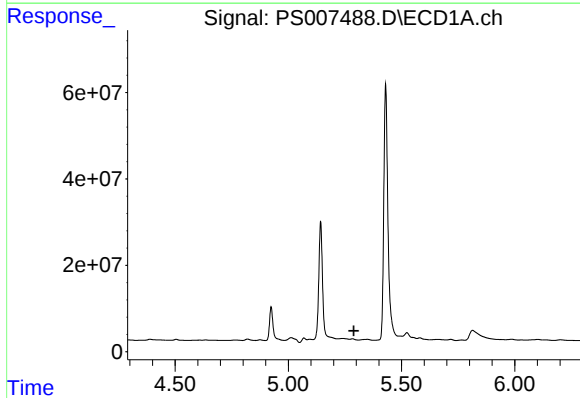


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

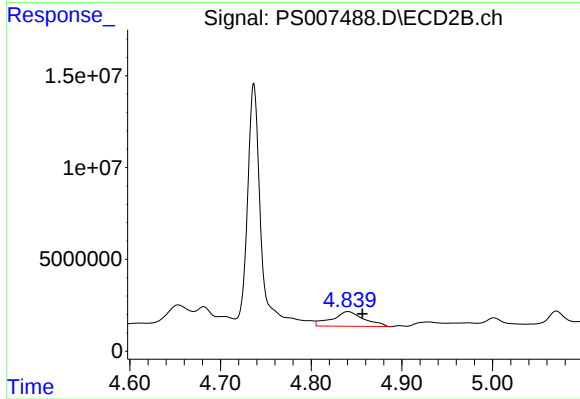

#3 4-Nitrophenol


R.T.: 4.841 min
Delta R.T.: -0.016 min
Response: 19605298
Conc: 49.65 ng/ml

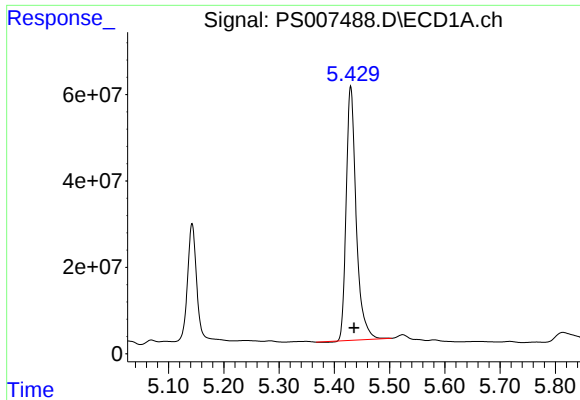

#4 2,4-DCAA


R.T.: 5.430 min
Delta R.T.: -0.006 min
Response: 738069223
Conc: 539.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124394TB

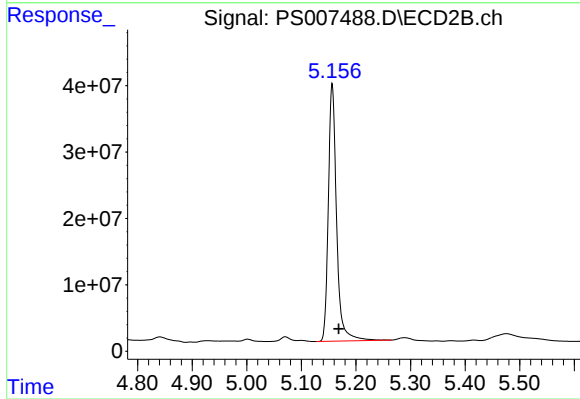


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: -0.012 min
Response: 407277287
Conc: 579.09 ng/ml

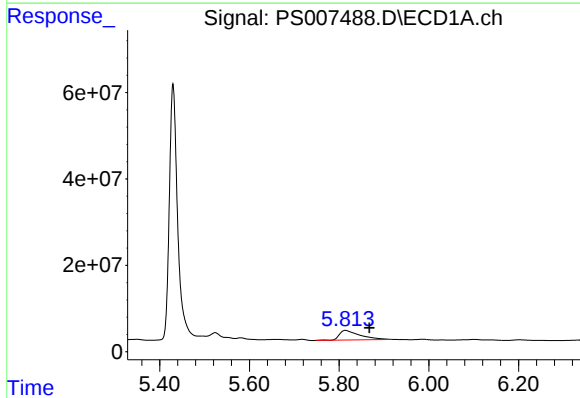


#7 MCPA

R.T.: 5.814 min
Delta R.T.: -0.053 min
Response: 68980173
Conc: 13.37 ug/ml

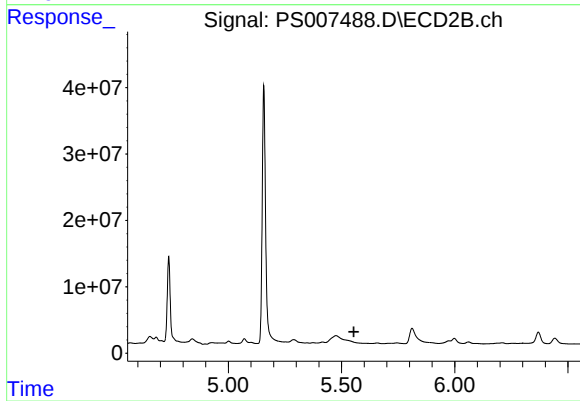

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.555 min
Response: 0
Conc: N.D.

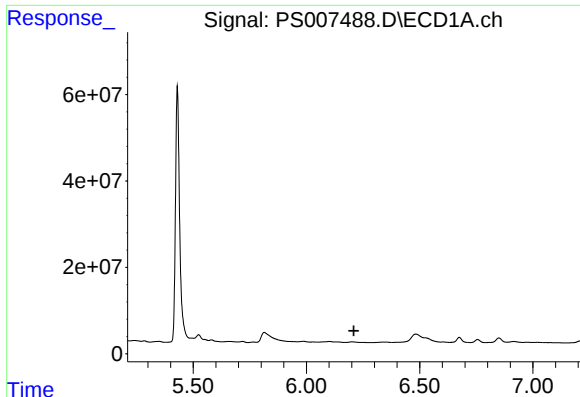

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394TB

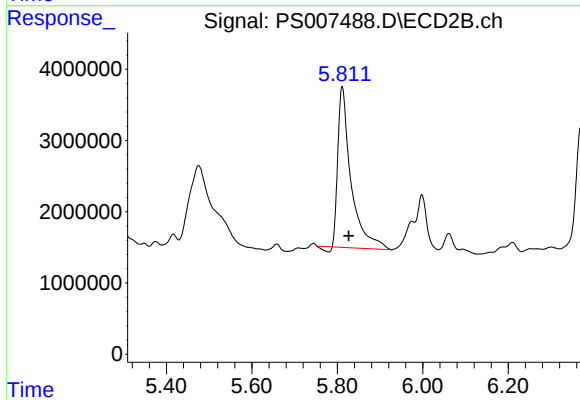


#8 DICHLORPROP

R.T.: 5.812 min
Delta R.T.: -0.015 min
Response: 47942829
Conc: 73.62 ng/ml

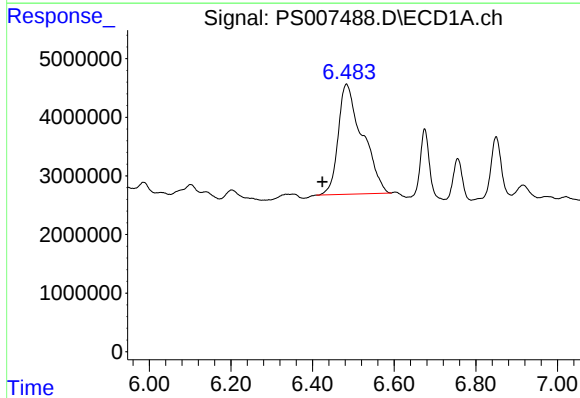


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.059 min
Response: 77177697
Conc: 62.63 ng/ml

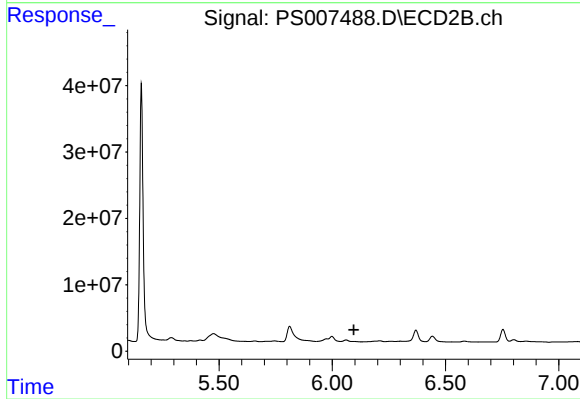

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

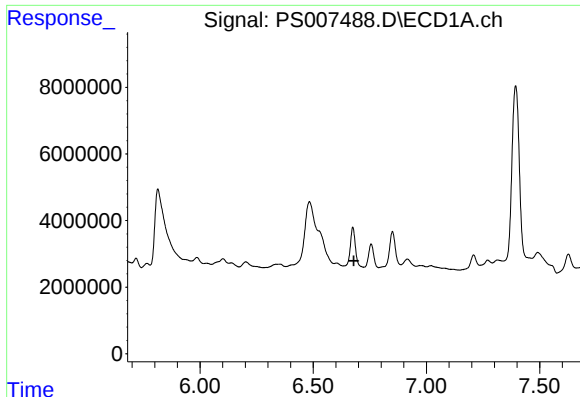

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394TB

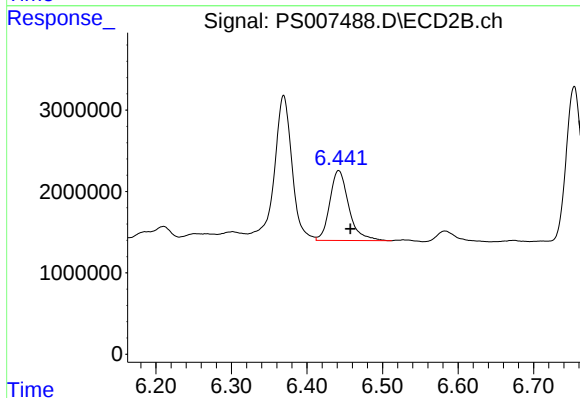


#10 Pentachlorophenol

R.T.: 6.442 min
Delta R.T.: -0.015 min
Response: 14986373
Conc: 1.56 ng/ml

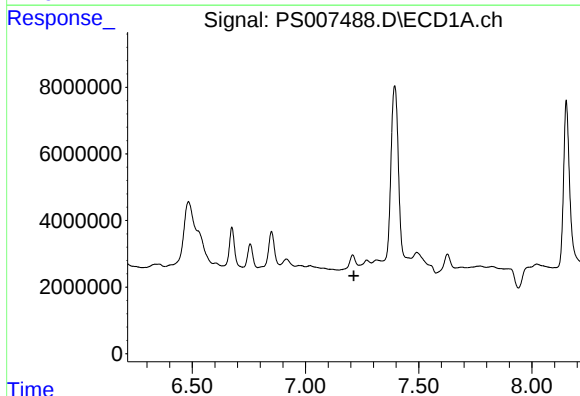


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

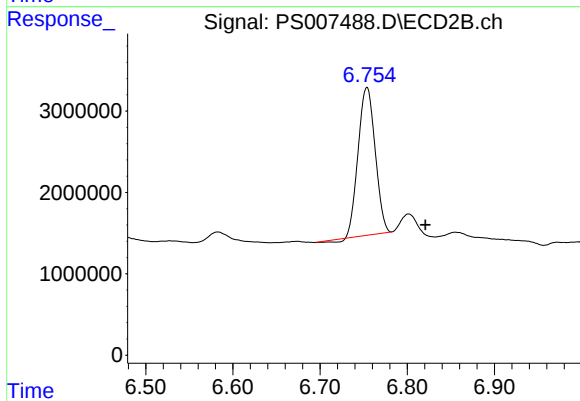

#11 2,4,5-TP (SILVEX)


R.T.: 6.754 min
Delta R.T.: -0.067 min
Response: 24428713
Conc: 6.42 ng/ml

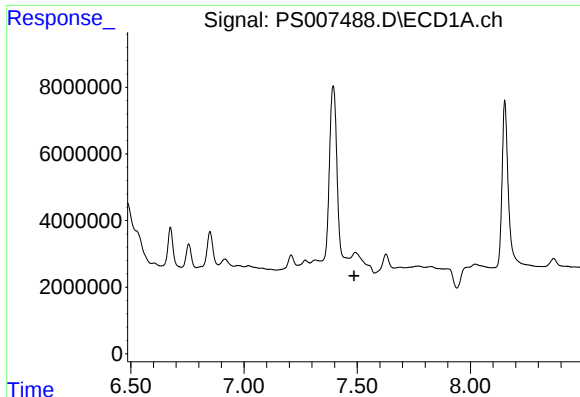

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124394TB

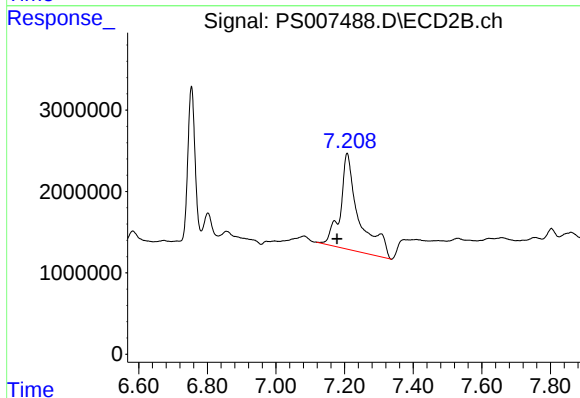


#12 2,4,5-T

R.T.: 7.208 min
Delta R.T.: 0.029 min
Response: 44721304
Conc: 12.76 ng/ml

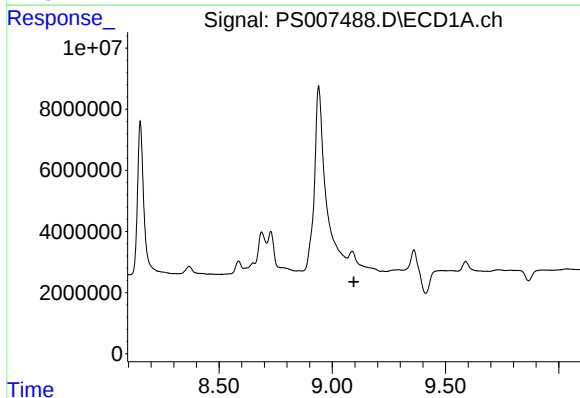


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

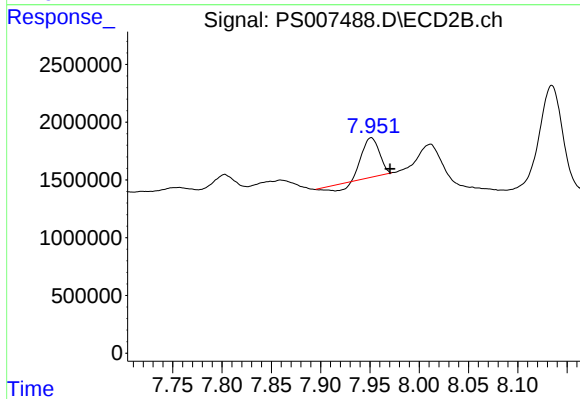

#14 DINOSEB


R.T.: 7.951 min
Delta R.T.: -0.019 min
Response: 3615380
Conc: 1.29 ng/ml

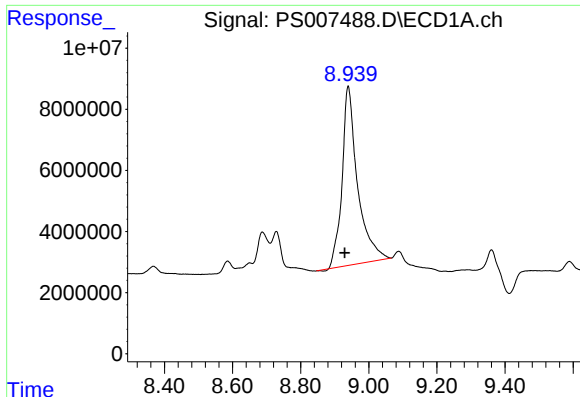

#15 Picloram


R.T.: 8.940 min
Delta R.T.: 0.010 min
Response: 185270046
Conc: 16.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124394TB

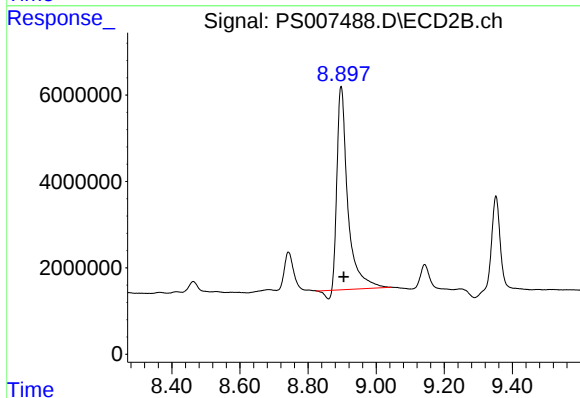


#15 Picloram

R.T.: 8.897 min
Delta R.T.: -0.008 min
Response: 102251185
Conc: 16.65 ng/ml

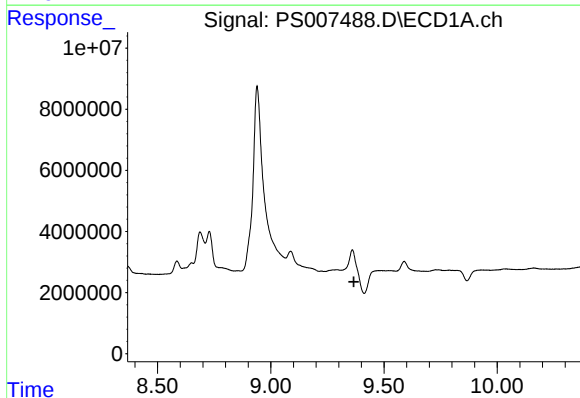

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

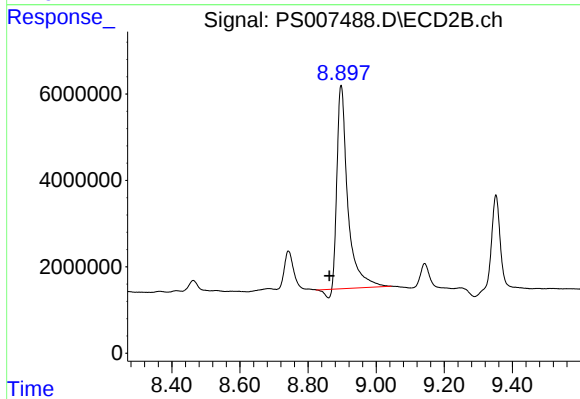

#16 DCPA

R.T.: 8.897 min
Delta R.T.: 0.034 min
Response: 102251185
Conc: 20.39 ng/ml