

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102921\
 Data File : PS017273.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Oct 2021 09:15
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 23:39:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.153	6.737	688.4E6	315.1E6	450.390	539.195
Target Compounds							
2) T	3,5-DICHL...	6.418f	0.000	3331986	0	1.544	N.D. #
12) T	2,4,5-T	9.429	0.000	6698545	0	<MDL	N.D. #
14) T	DINOSEB	11.102	0.000	5578089	0	<MDL	N.D. #
15) T	Picloram	10.955	10.789	156.4E6	50594781	14.640	13.211
16) T	DCPA	0.000	10.789f	0	50594781	N.D.	11.857



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102921\
Data File : PS017273.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Oct 2021 09:15
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 23:39:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

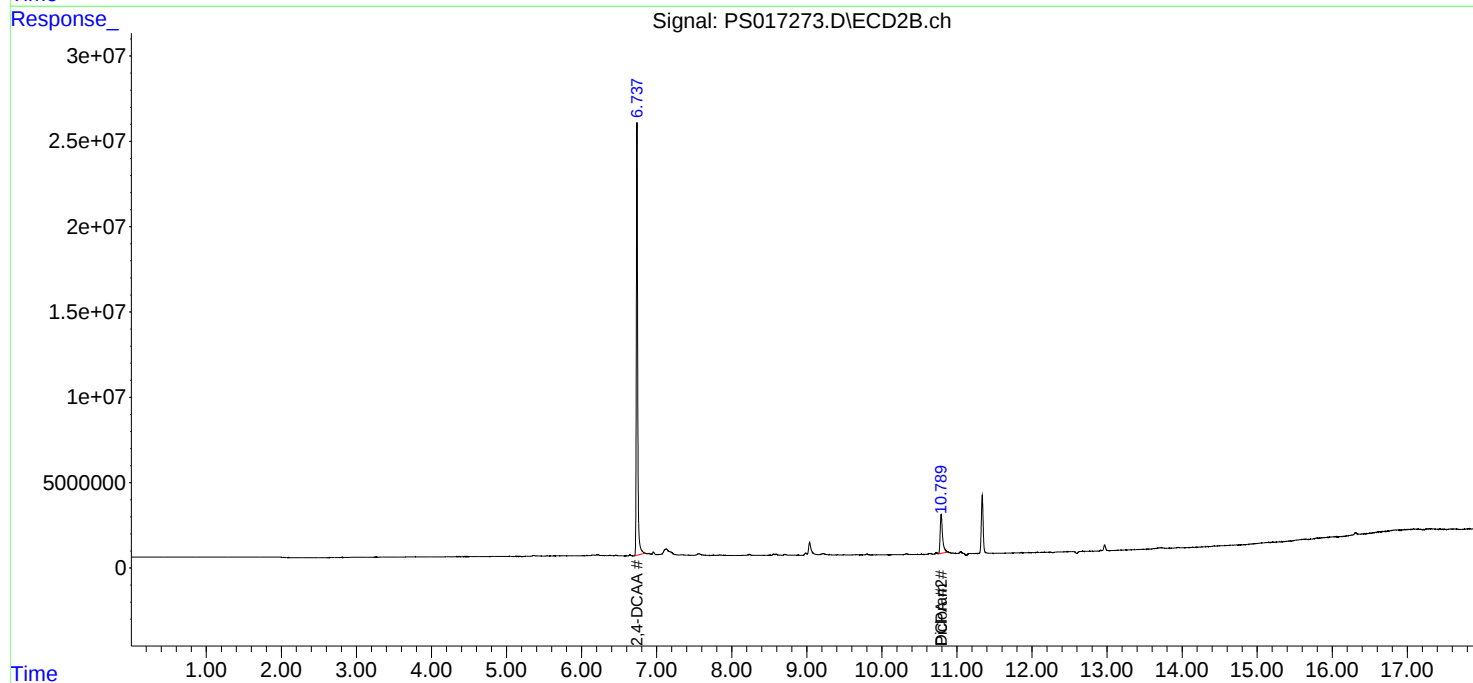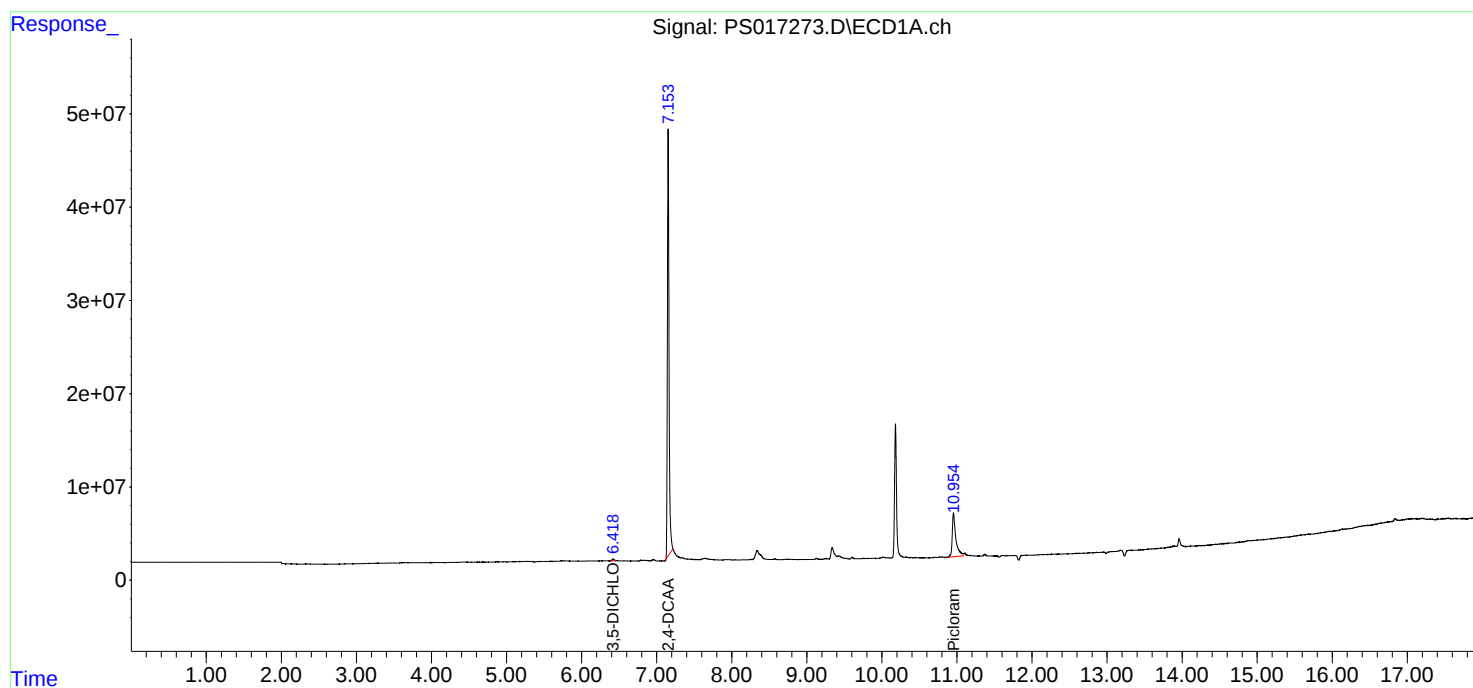


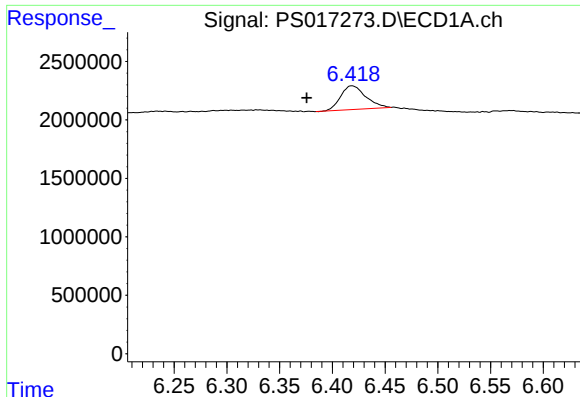

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.418 min
Delta R.T.: 0.043 min
Response: 3331986
Conc: 1.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

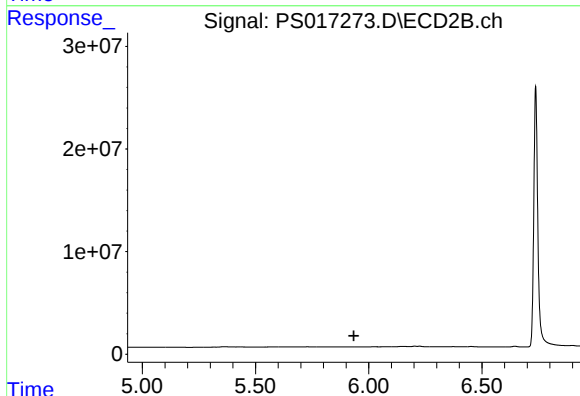


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.934 min
Response: 0
Conc: N.D.

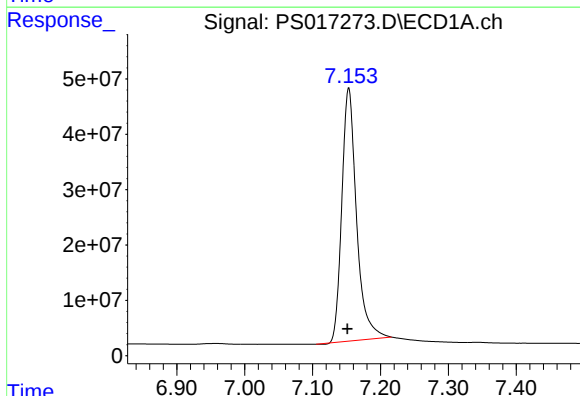


#4 2,4-DCAA

R.T.: 7.153 min
Delta R.T.: 0.002 min
Response: 688402675
Conc: 450.39 ng/ml

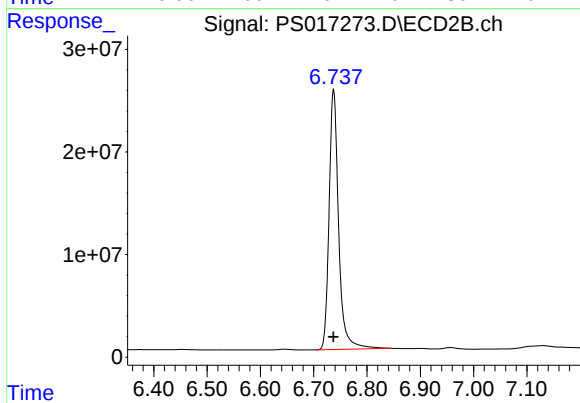

#4 2,4-DCAA


R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 315128168
Conc: 539.20 ng/ml

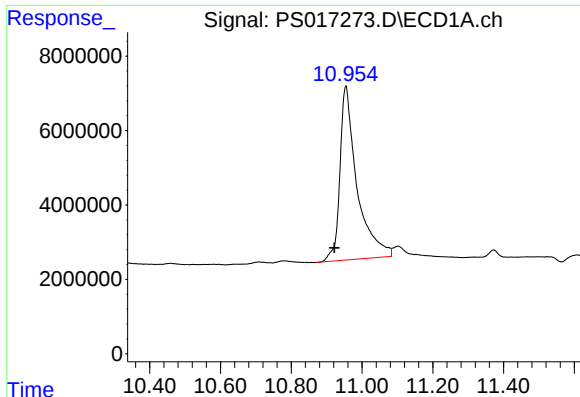

#15 Picloram


R.T.: 10.955 min
Delta R.T.: 0.032 min
Response: 156380502
Conc: 14.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

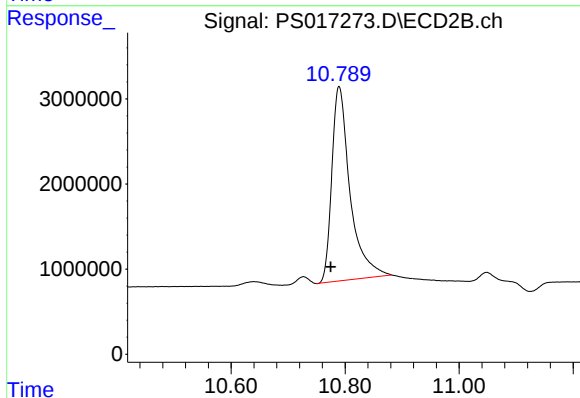


#15 Picloram

R.T.: 10.789 min
Delta R.T.: 0.014 min
Response: 50594781
Conc: 13.21 ng/ml

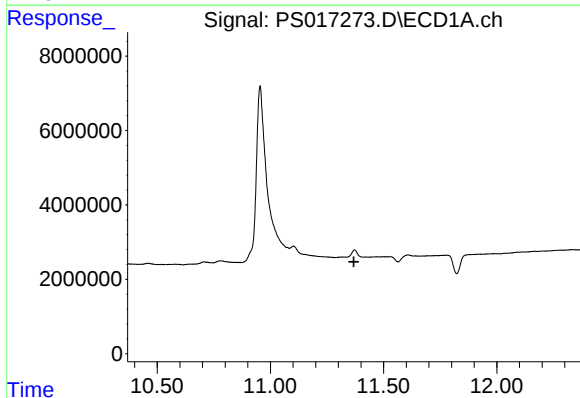

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.369 min
Response: 0
Conc: N.D.

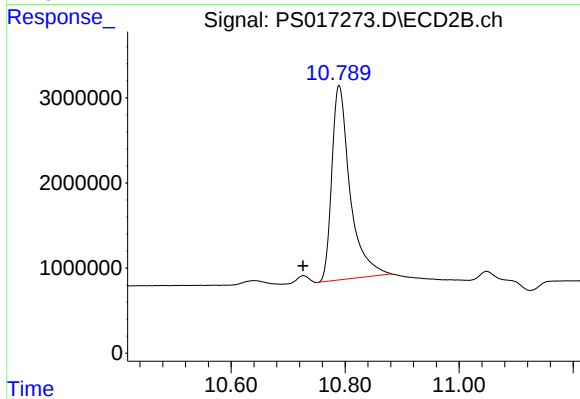

#16 DCPA

R.T.: 10.789 min
Delta R.T.: 0.063 min
Response: 50594781
Conc: 11.86 ng/ml