

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
 Data File : PS002189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 08:22
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 13:48:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.919	0	233048	N.D.	0.649 #
Target Compounds							
1) T	Dalapon	0.000	2.374	0	33874292	N.D.	75.025 #
2) T	3,5-DICHL...	0.000	9.063	0	175930	N.D.	0.397 #
3) T	4-Nitroph...	0.000	10.065	0	486192	N.D.	2.727 #
5) T	DICAMBA	0.000	11.194	0	104737	N.D.	0.084 #
6) T	MCP	0.000	11.406	0	565709	N.D.	0.658 #
7) T	MCPA	0.000	11.827	0	222215	N.D.	0.164 #
8) T	DICHLORPROP	0.000	12.321	0	153418	N.D.	0.478 #
9) T	2,4-D	0.000	12.789	0	153881	N.D.	0.361 #
10) T	Pentachlo...	0.000	13.338	0	36267	N.D.	0.008 #
11) T	2,4,5-TP ...	0.000	13.950	0	260094	N.D.	0.142 #
12) T	2,4,5-T	0.000	14.519	0	583520	N.D.	0.390 #
14) T	DINOSEB	0.000	15.566	0	180217	N.D.	0.142 #
15) T	Picloram	16.920	16.819	7003801	1998958	2.936	0.884 #
16) T	DCPA	0.000	16.824	0	2552419	N.D.	1.078 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
Data File : PS002189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 08:22
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 13:48:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

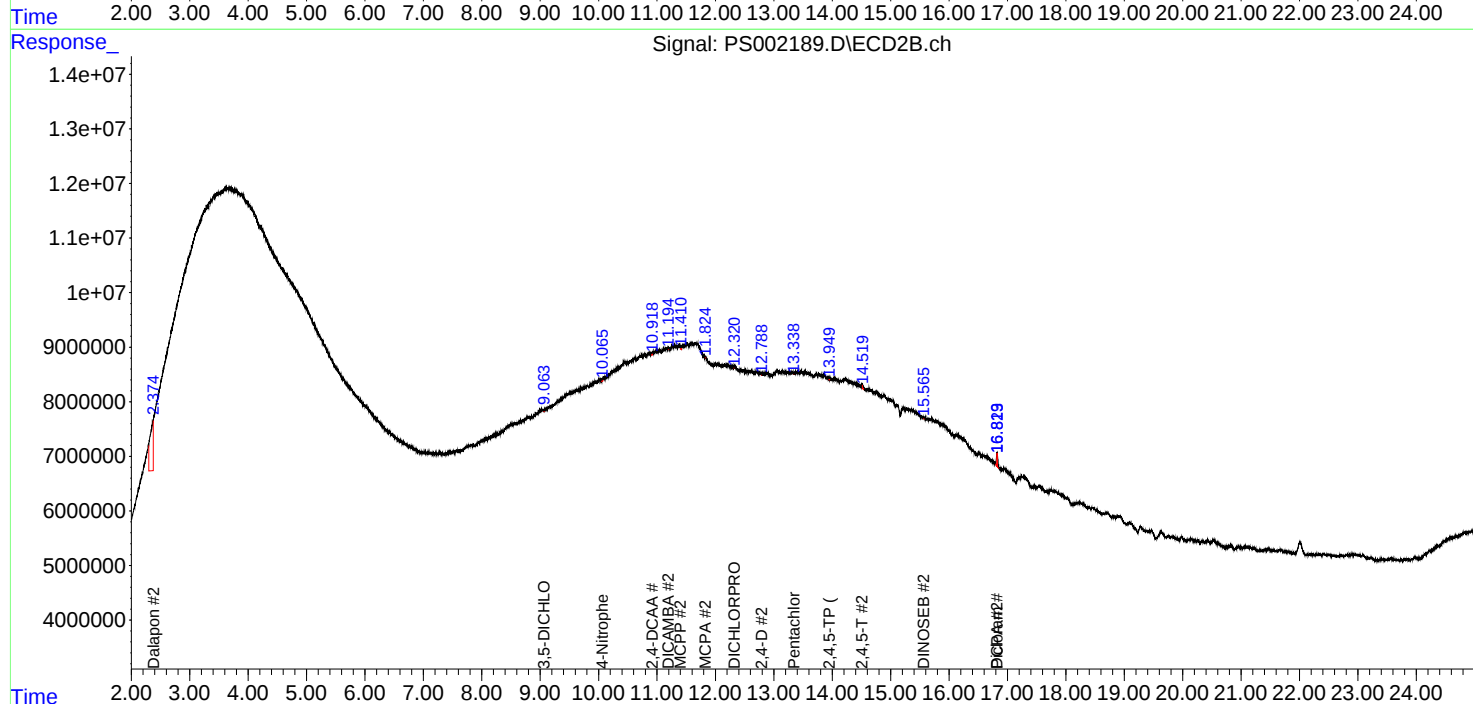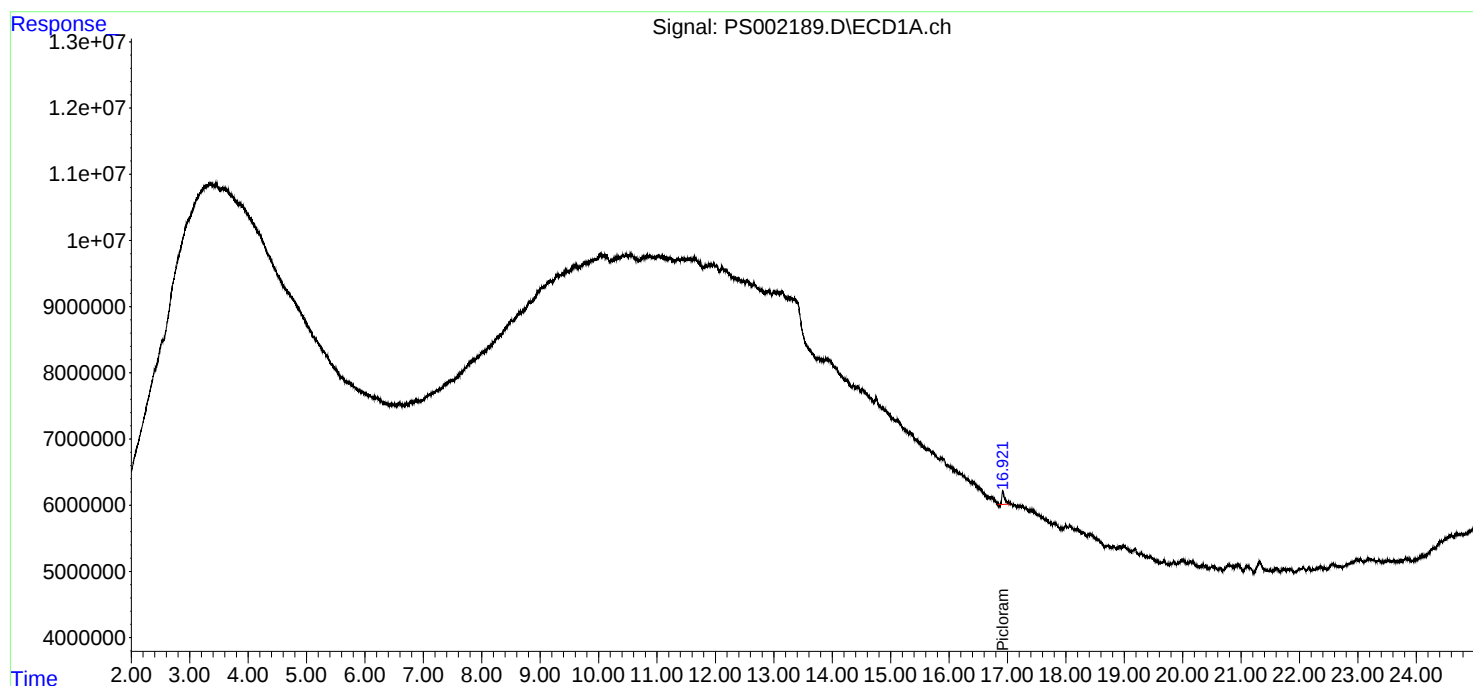


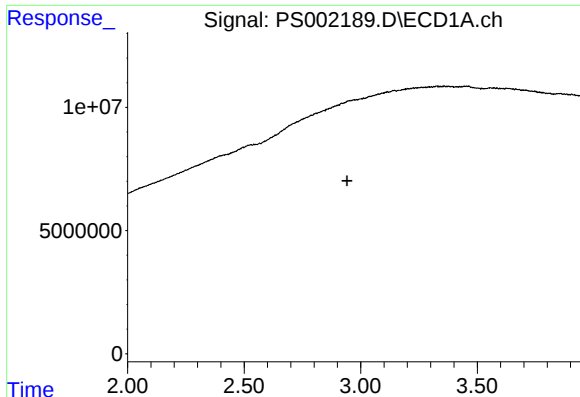

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

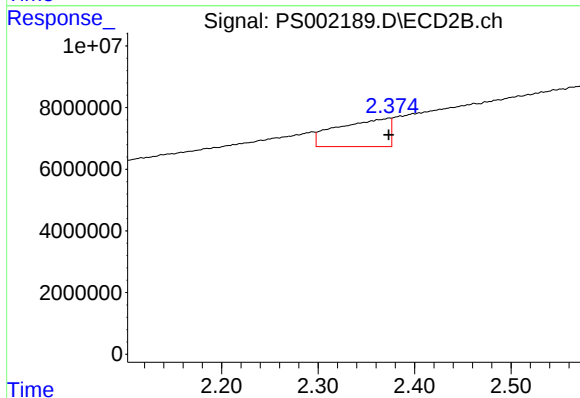


#1 Dalapon

R.T.: 2.374 min
Delta R.T.: 0.000 min
Response: 33874292
Conc: 75.02 ng/ml

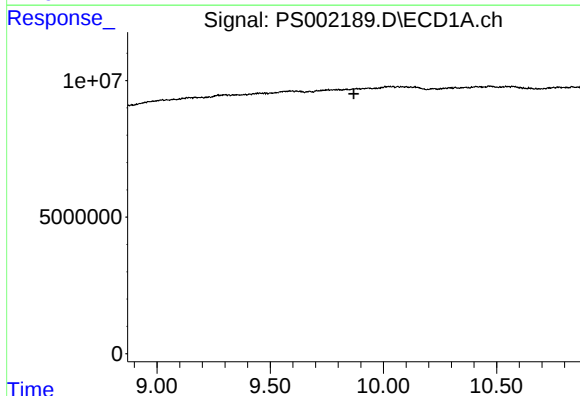


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

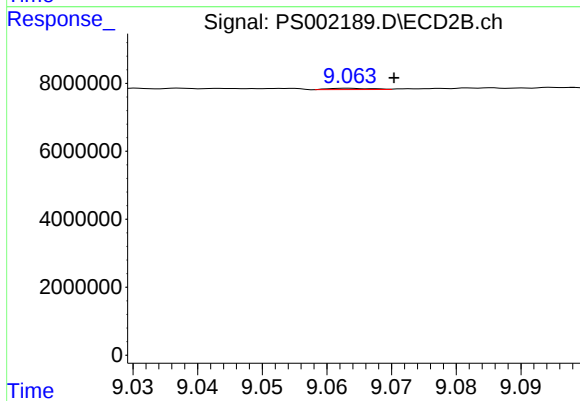

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.063 min
Delta R.T.: -0.007 min
Response: 175930
Conc: 0.40 ng/ml

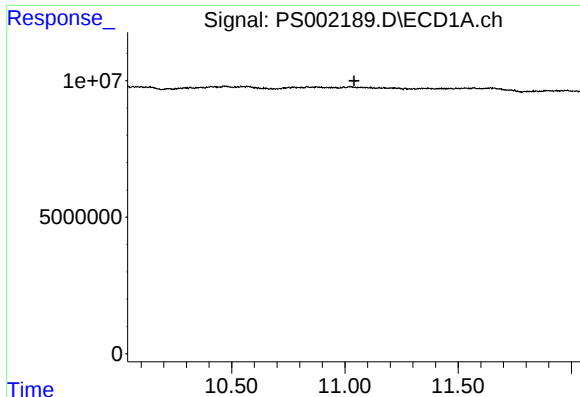

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

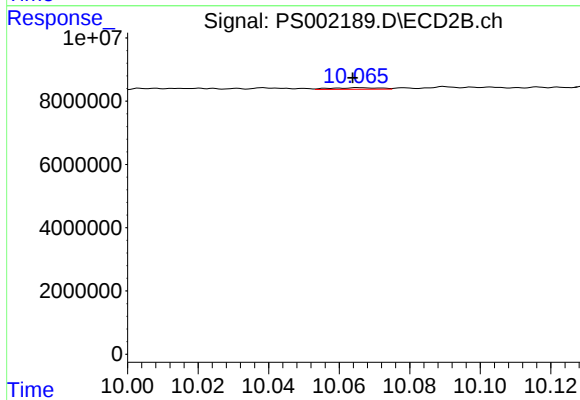


#3 4-Nitrophenol

R.T.: 10.065 min
Delta R.T.: 0.002 min
Response: 486192
Conc: 2.73 ng/ml

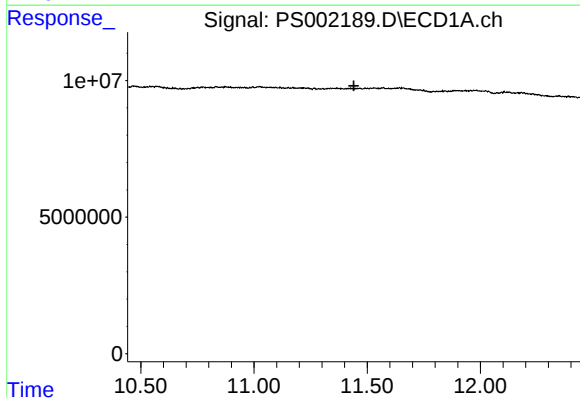


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.441 min
Response: 0
Conc: N.D.

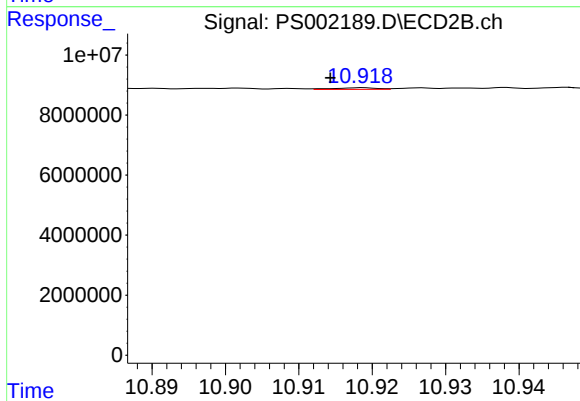

#4 2,4-DCAA


R.T.: 10.919 min
Delta R.T.: 0.004 min
Response: 233048
Conc: 0.65 ng/ml

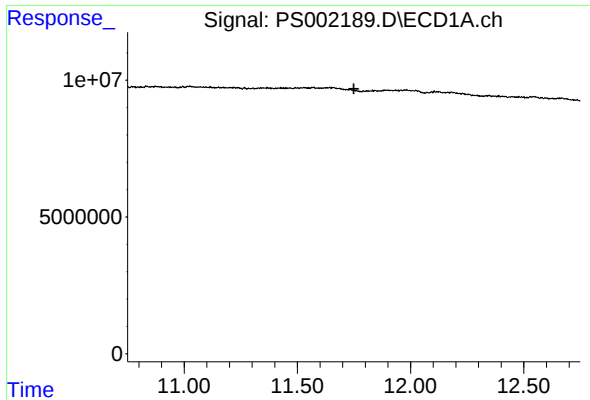

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

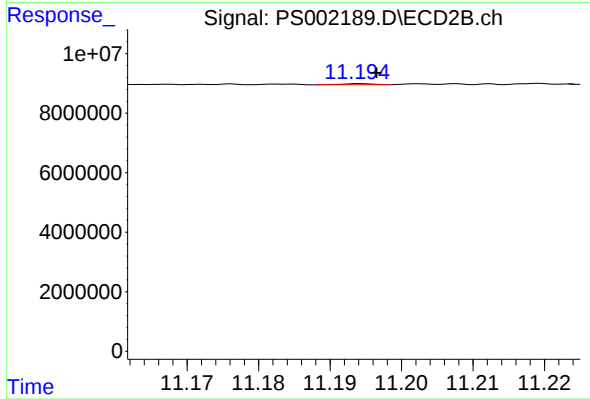


#5 DICAMBA

R.T.: 11.194 min
Delta R.T.: -0.002 min
Response: 104737
Conc: 0.08 ng/ml

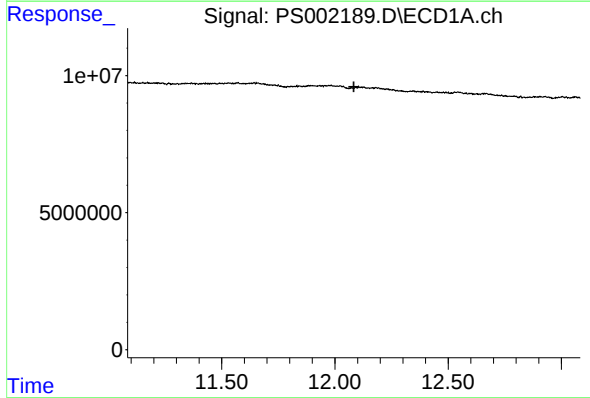


#6 MCP

R.T.: 0.000 min
Exp R.T.: 12.084 min
Response: 0
Conc: N.D.

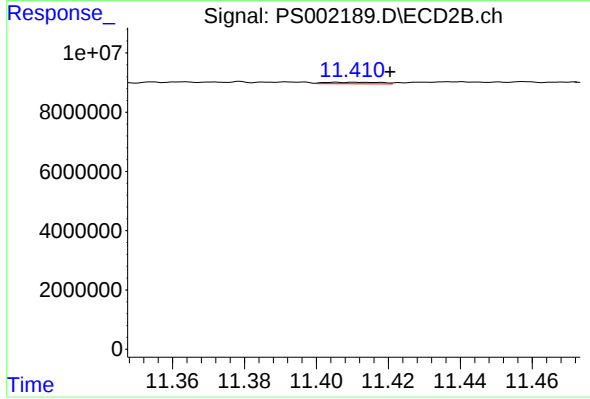

#6 MCP


R.T.: 11.406 min
Delta R.T.: -0.015 min
Response: 565709
Conc: 0.66 ug/ml

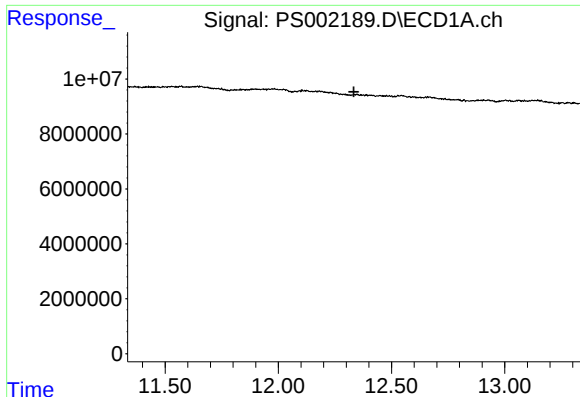

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

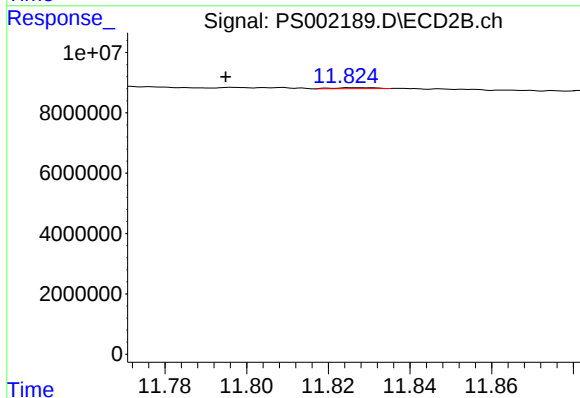


#7 MCPA

R.T.: 11.827 min
Delta R.T.: 0.032 min
Response: 222215
Conc: 0.16 ug/ml

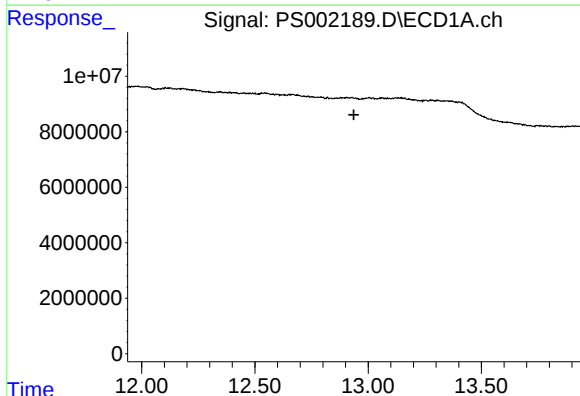


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

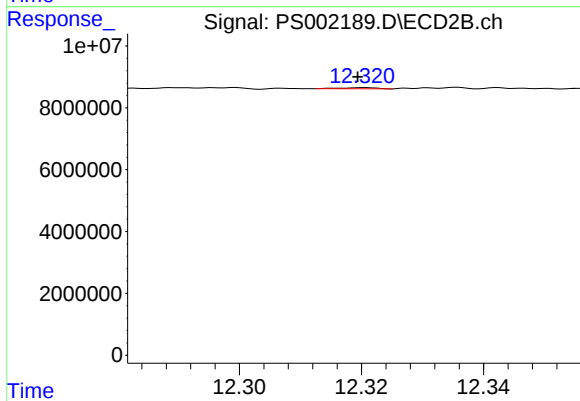

#8 DICHLORPROP


R.T.: 12.321 min
Delta R.T.: 0.001 min
Response: 153418
Conc: 0.48 ng/ml

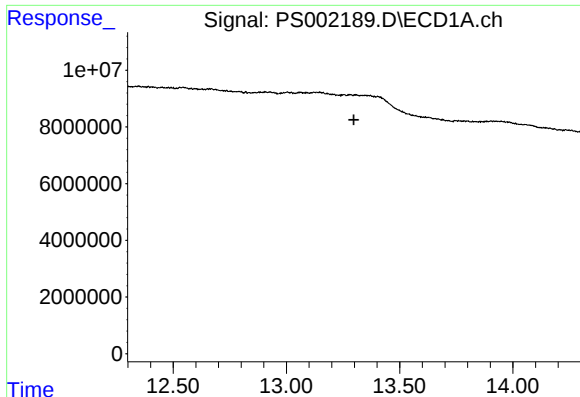

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

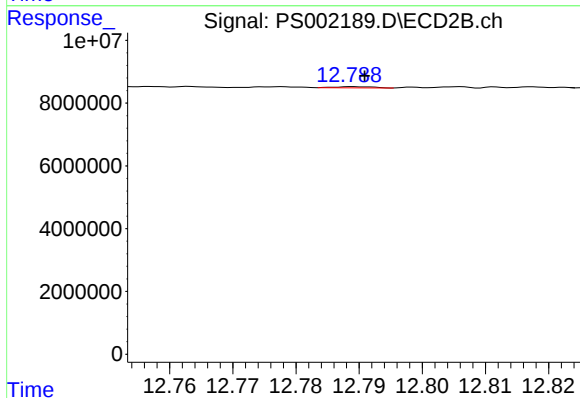


#9 2,4-D

R.T.: 12.789 min
Delta R.T.: -0.002 min
Response: 153881
Conc: 0.36 ng/ml

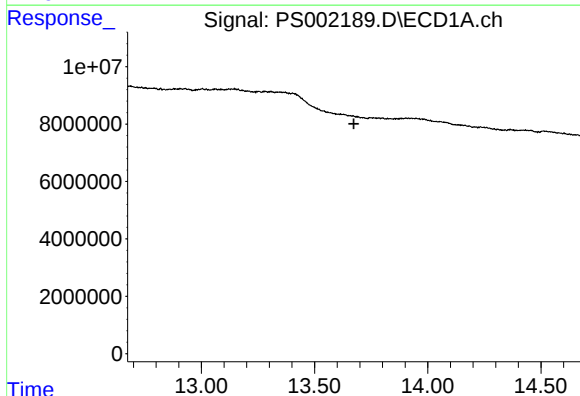


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

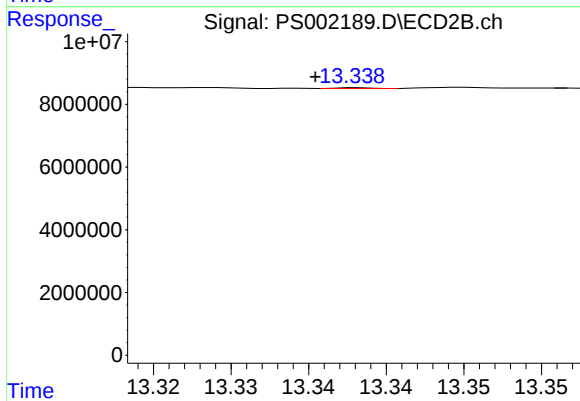

#10 Pentachlorophenol


R.T.: 13.338 min
Delta R.T.: 0.003 min
Response: 36267
Conc: 0.01 ng/ml

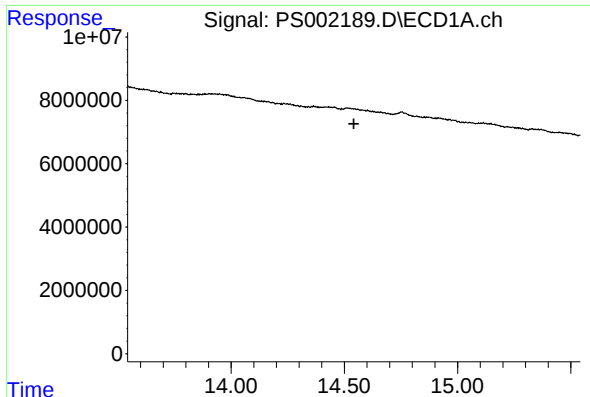

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

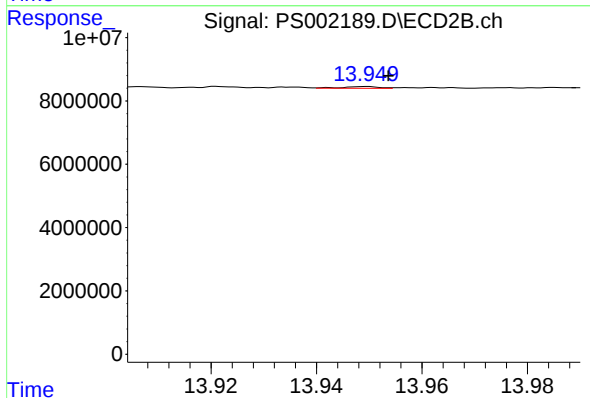


#11 2,4,5-TP (SILVEX)

R.T.: 13.950 min
Delta R.T.: -0.004 min
Response: 260094
Conc: 0.14 ng/ml

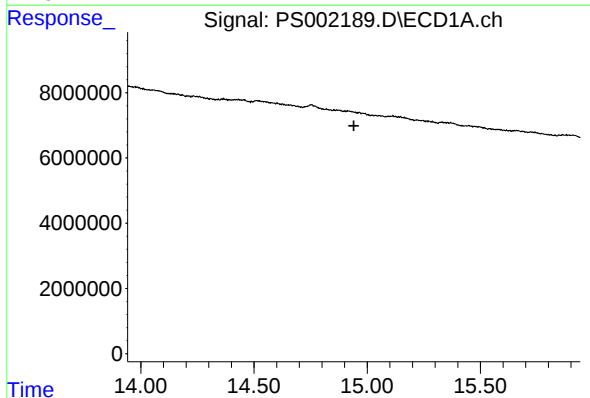


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

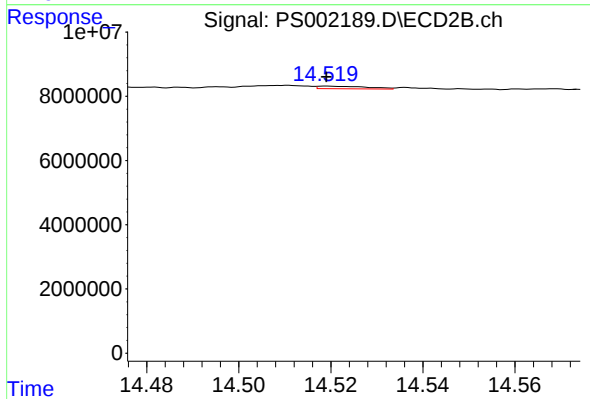

#12 2,4,5-T


R.T.: 14.519 min
Delta R.T.: 0.000 min
Response: 583520
Conc: 0.39 ng/ml

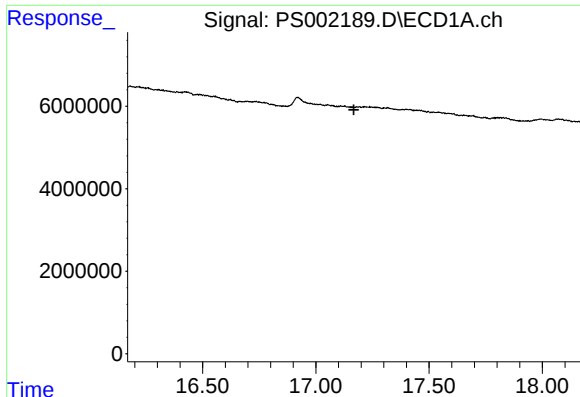

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

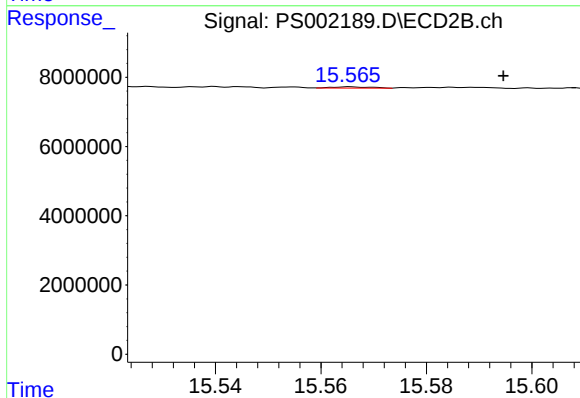


#14 DINOSEB

R.T.: 15.566 min
Delta R.T.: -0.029 min
Response: 180217
Conc: 0.14 ng/ml

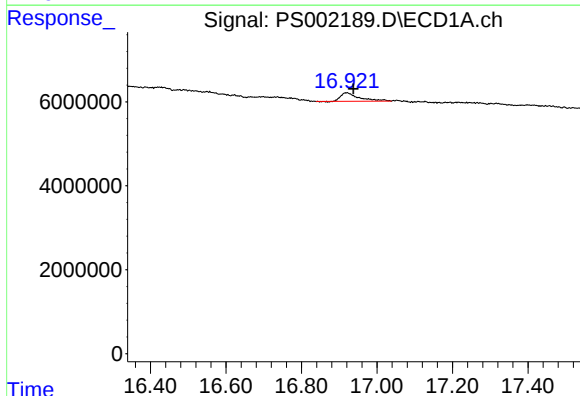


#15 Picloram

R.T.: 16.920 min
Delta R.T.: -0.018 min
Response: 7003801
Conc: 2.94 ng/ml

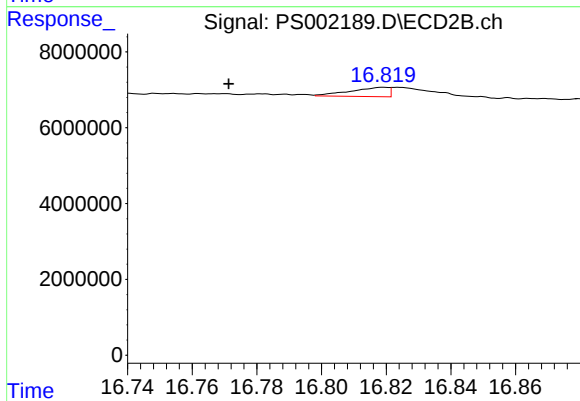

#15 Picloram


R.T.: 16.819 min
Delta R.T.: 0.048 min
Response: 1998958
Conc: 0.88 ng/ml

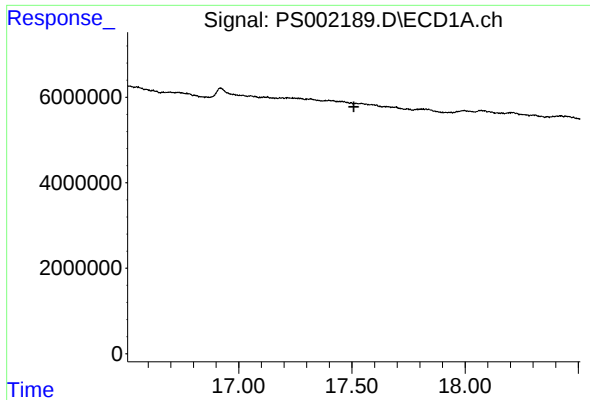

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

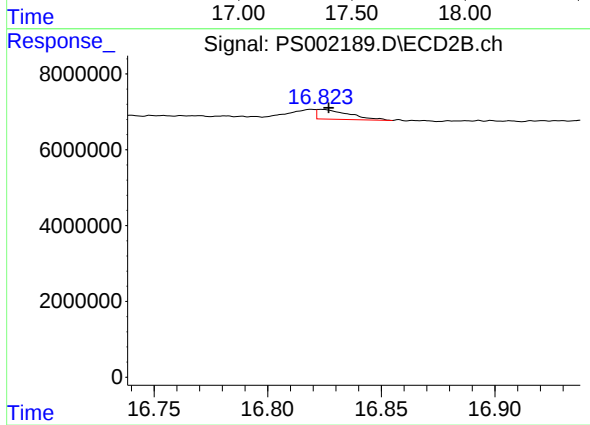

#16 DCPA

R.T.: 16.824 min
Delta R.T.: -0.003 min
Response: 2552419
Conc: 1.08 ng/ml