

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
 Data File : PS002194.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 12:49
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 13:50:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.424	10.908	145.9E6	140.8E6	463.515	391.991
Target Compounds							
1) T	Dalapon	0.000	2.359	0	820232	N.D.	1.817 #
5) T	DICAMBA	0.000	11.152	0	129293	N.D.	0.103 #
15) T	Picloram	0.000	16.769	0	88830	N.D.	0.039 #
16) T	DCPA	0.000	16.831	0	374903	N.D.	0.158 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
Data File : PS002194.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 12:49
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 13:50:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

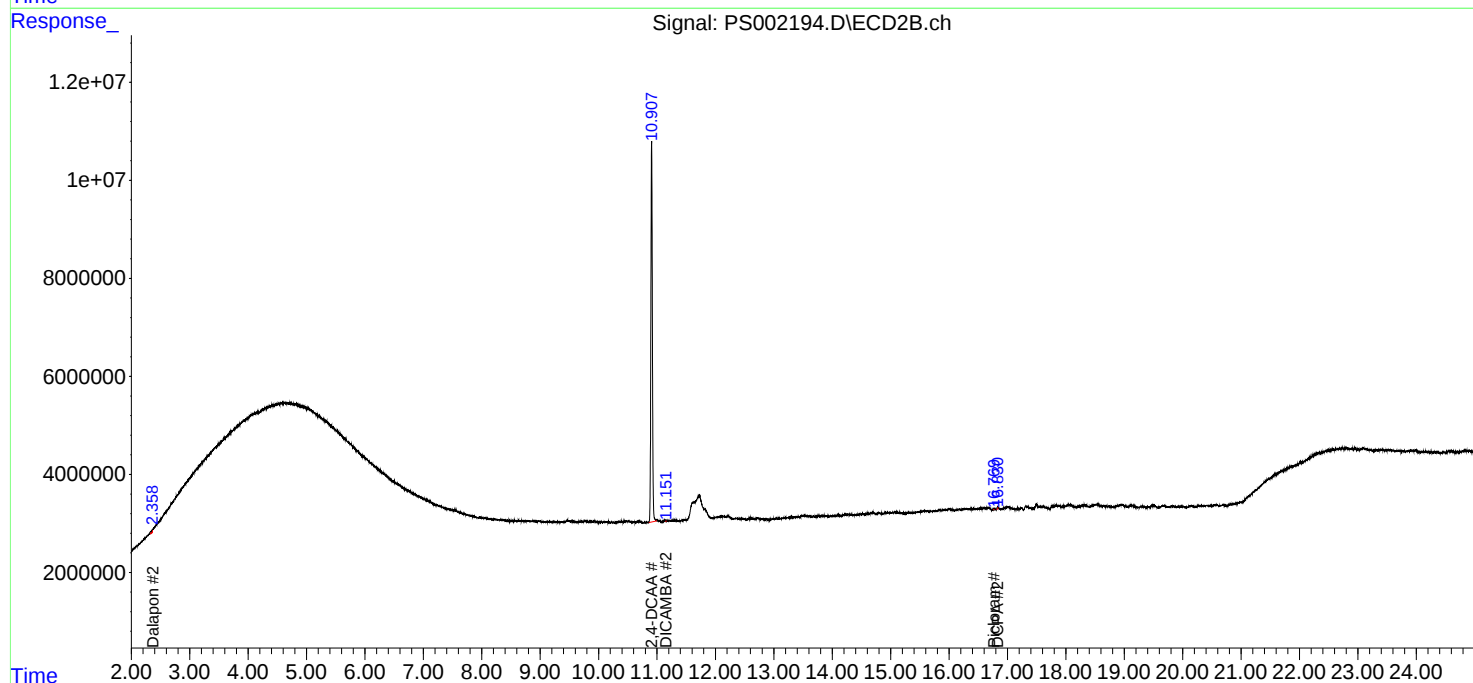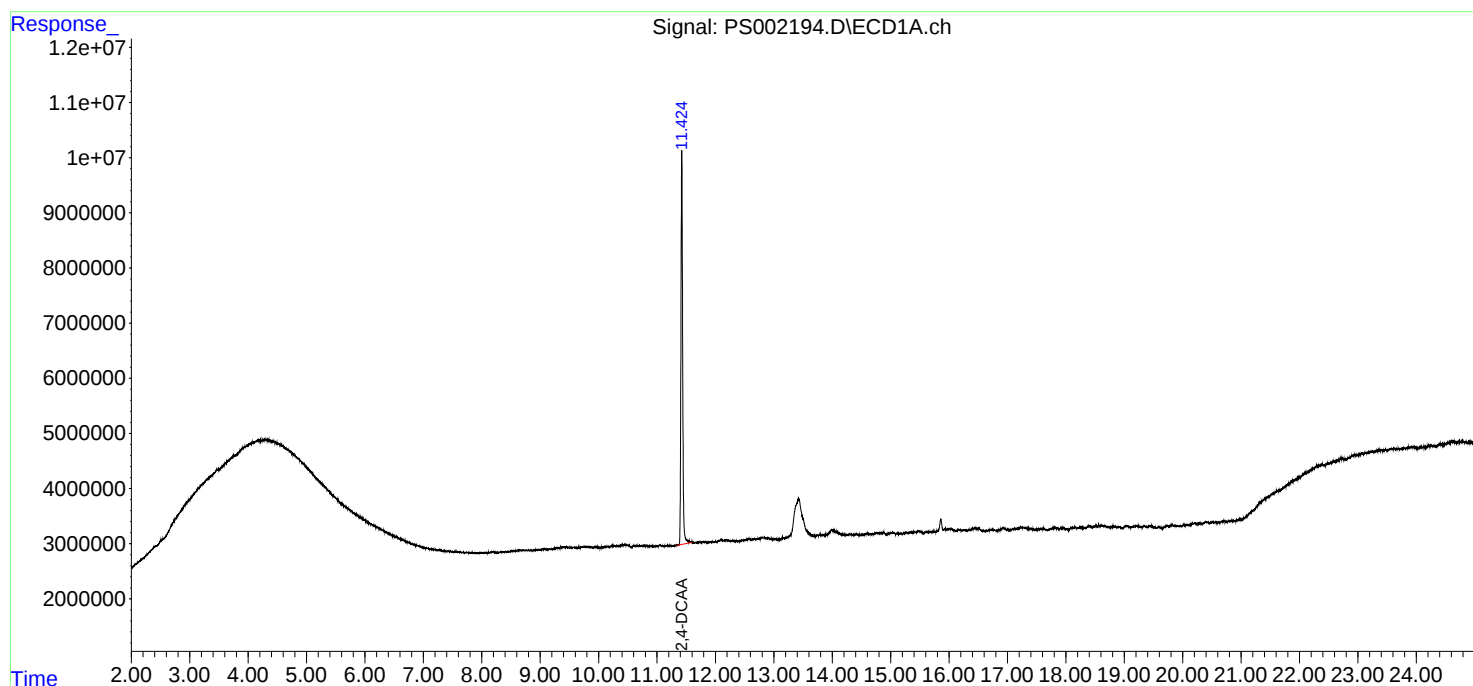


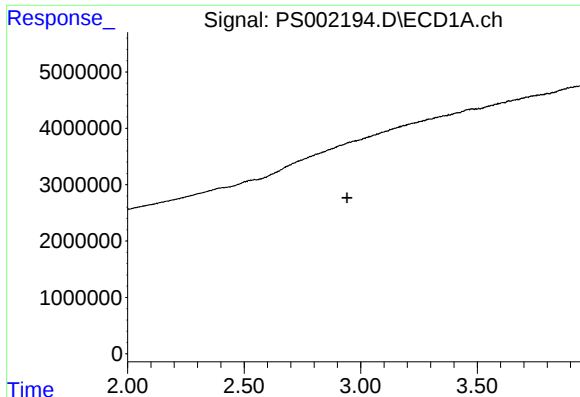

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

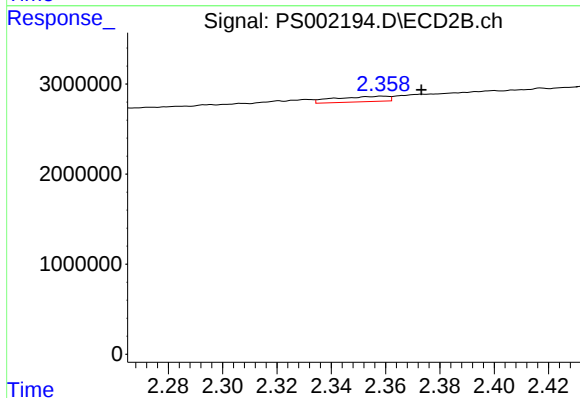


#1 Dalapon

R.T.: 2.359 min
Delta R.T.: -0.014 min
Response: 820232
Conc: 1.82 ng/ml

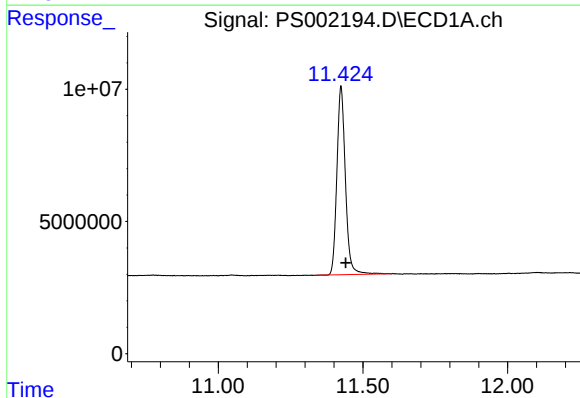


#4 2,4-DCAA

R.T.: 11.424 min
Delta R.T.: -0.017 min
Response: 145861430
Conc: 463.51 ng/ml

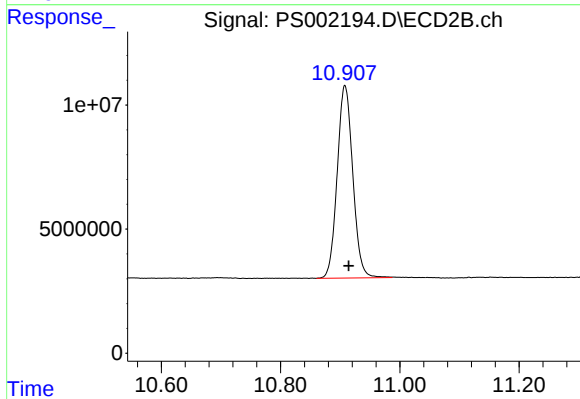

#4 2,4-DCAA


R.T.: 10.908 min
Delta R.T.: -0.007 min
Response: 140763146
Conc: 391.99 ng/ml

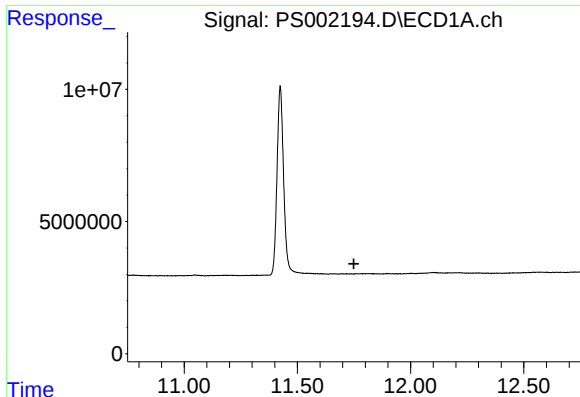

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

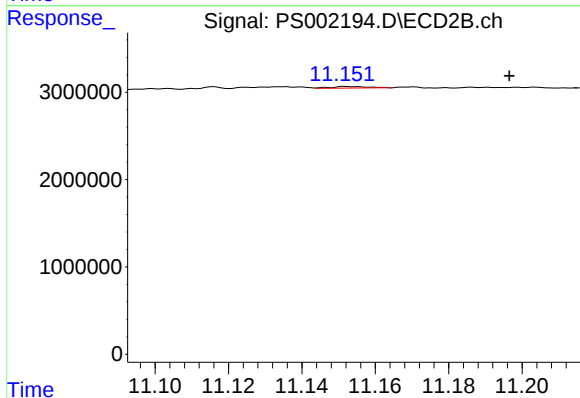


#5 DICAMBA

R.T.: 11.152 min
Delta R.T.: -0.045 min
Response: 129293
Conc: 0.10 ng/ml

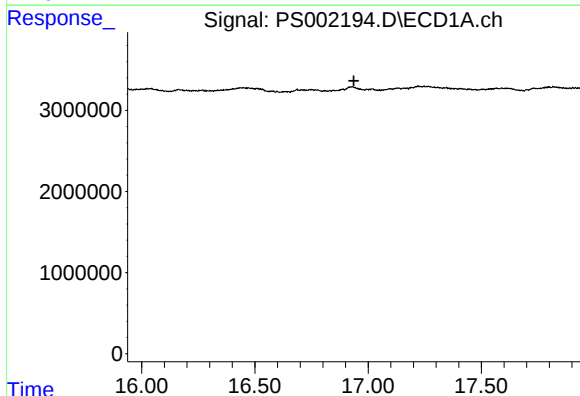


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.937 min
Response: 0
Conc: N.D.

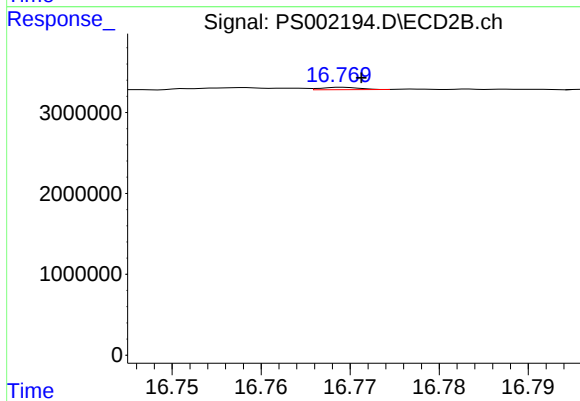

#15 Picloram


R.T.: 16.769 min
Delta R.T.: -0.002 min
Response: 88830
Conc: 0.04 ng/ml

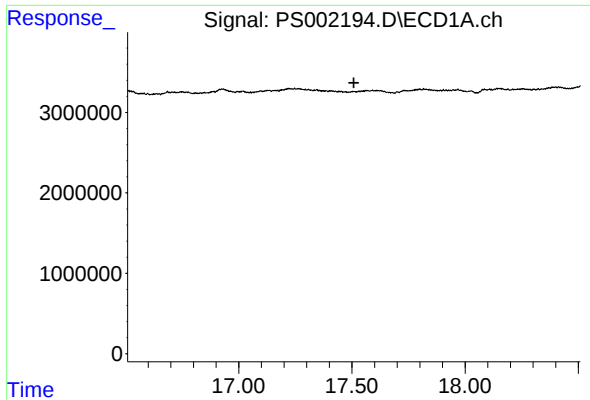

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

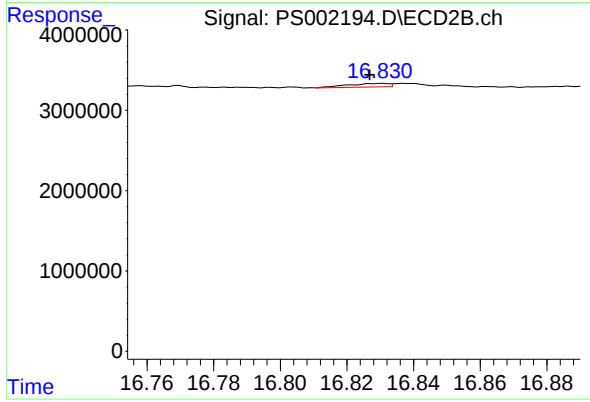

#16 DCPA

R.T.: 16.831 min
Delta R.T.: 0.004 min
Response: 374903
Conc: 0.16 ng/ml