

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
 Data File : PS002205.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2018 20:54
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:33:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.436	10.925	139.9E6	141.4E6	444.639	393.806
Target Compounds							
1) T	Dalapon	0.000	2.401	0	984563	N.D.	2.181 #
3) T	4-Nitroph...	11.069	10.083	45863897	139996	274.916	0.785 #
5) T	DICAMBA	0.000	11.227	0	53042	N.D.	0.042 #
6) T	MCP	0.000	11.429	0	129900	N.D.	0.151 #
7) T	MCPA	0.000	11.796	0	708835	N.D.	0.524 #
8) T	DICHLORPROP	0.000	12.352	0	288758	N.D.	0.899 #
9) T	2,4-D	0.000	12.851	0	338113	N.D.	0.794 #
10) T	Pentachlo...	0.000	13.288	0	107952	N.D.	0.023 #
11) T	2,4,5-TP ...	0.000	13.995	0	129621	N.D.	0.071 #
13) T	2,4-DB	0.000	15.101	0	717789	N.D.	3.240 #
15) T	Picloram	0.000	16.776	0	250929	N.D.	0.111 #
16) T	DCPA	0.000	16.776	0	250929	N.D.	0.106 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
Data File : PS002205.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2018 20:54
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:33:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

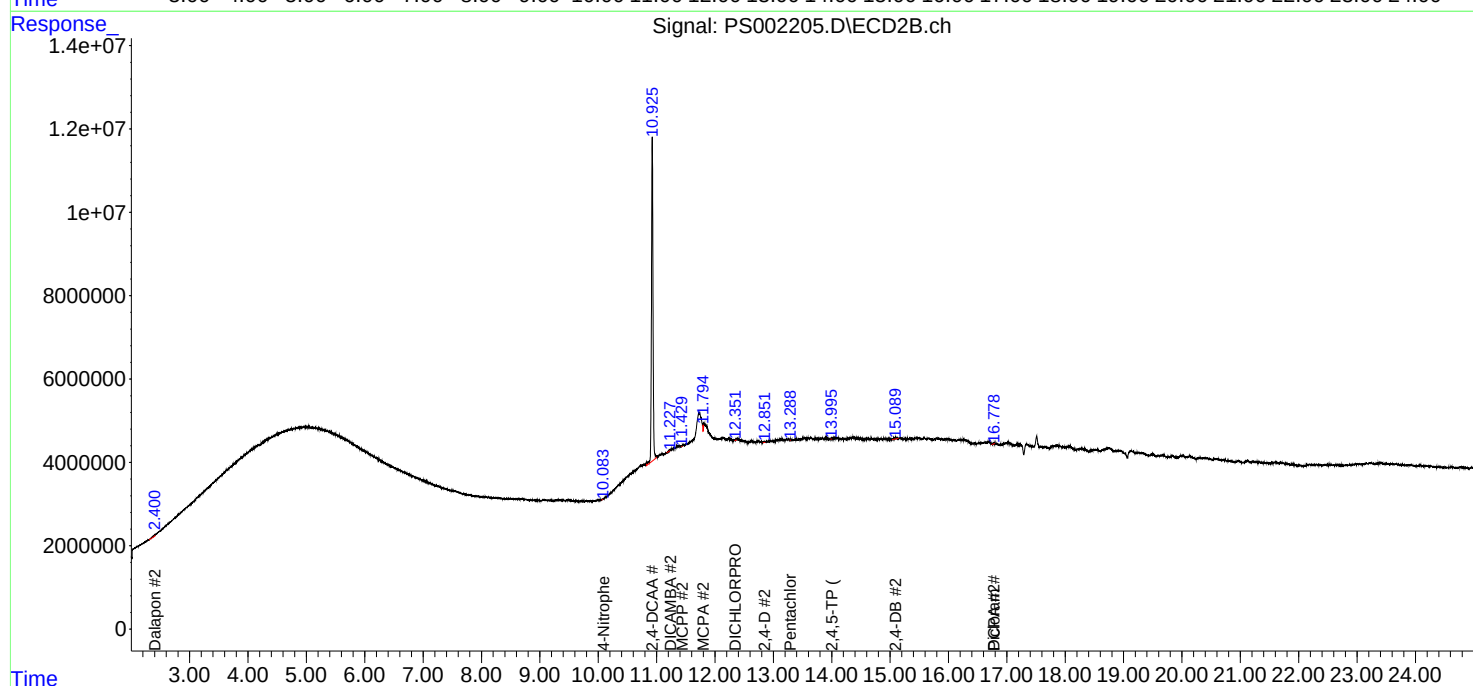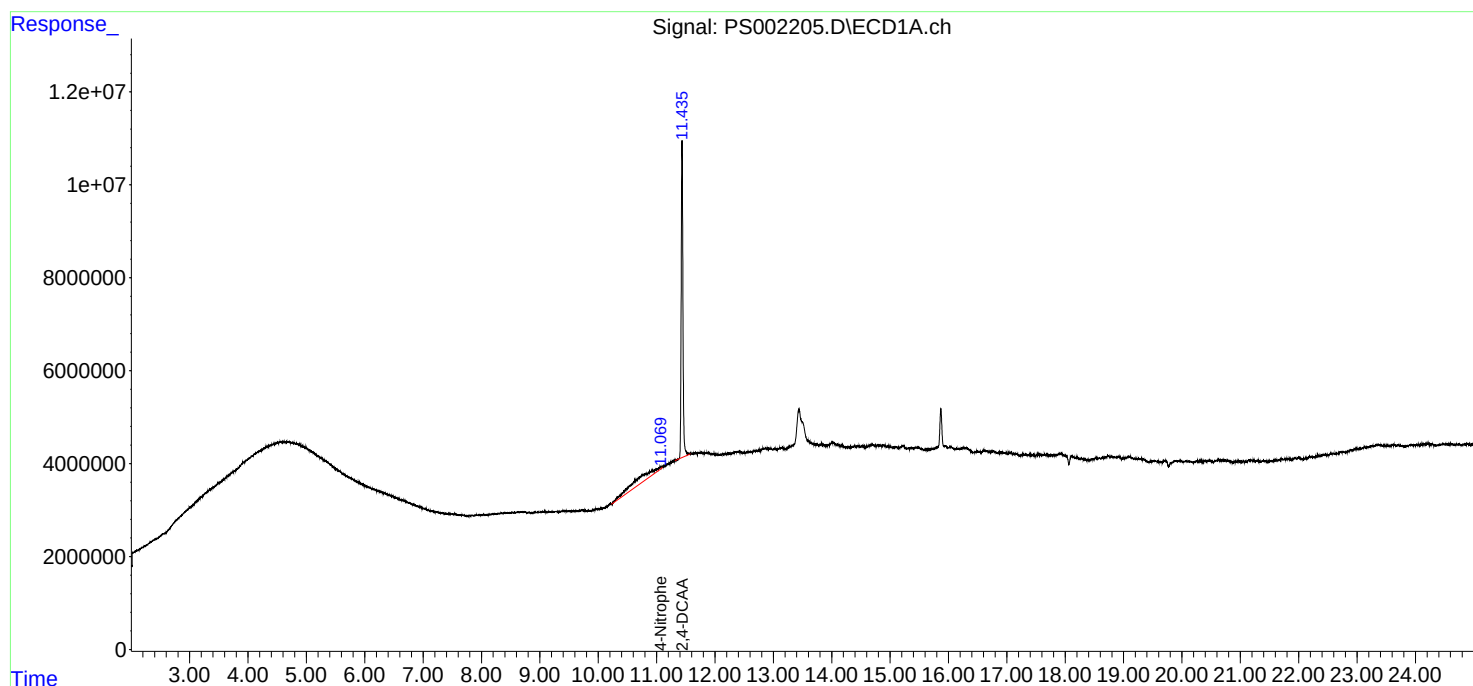


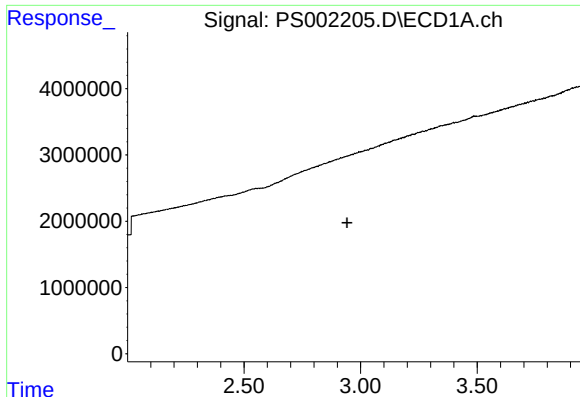

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

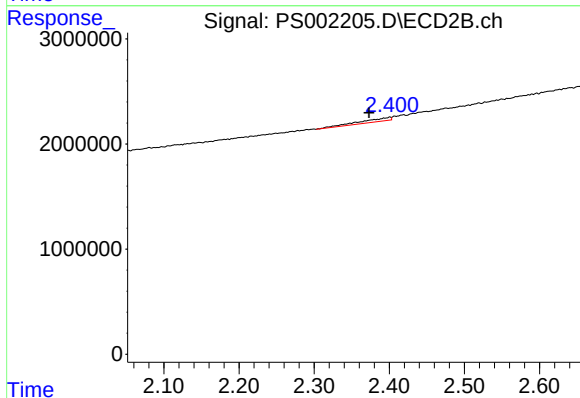


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: 0.028 min
Response: 984563
Conc: 2.18 ng/ml

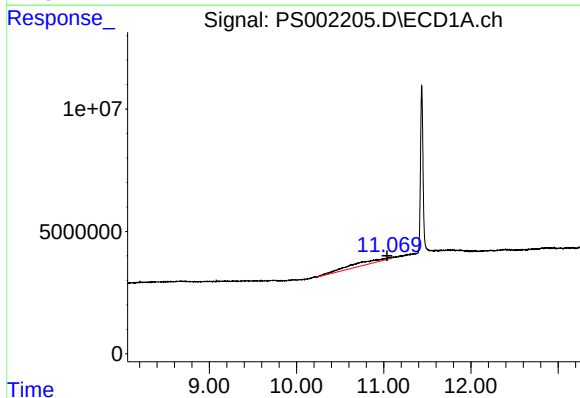


#3 4-Nitrophenol

R.T.: 11.069 min
Delta R.T.: 0.029 min
Response: 45863897
Conc: 274.92 ng/ml

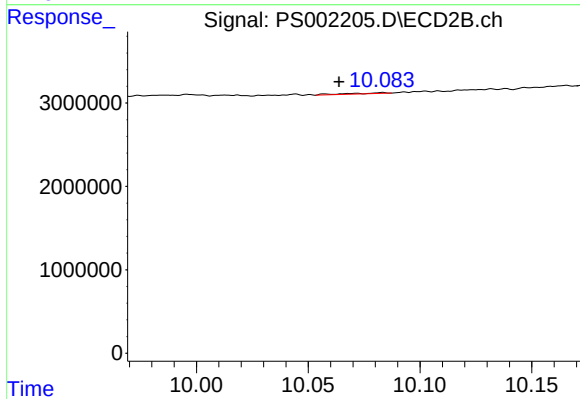

#3 4-Nitrophenol


R.T.: 10.083 min
Delta R.T.: 0.020 min
Response: 139996
Conc: 0.79 ng/ml

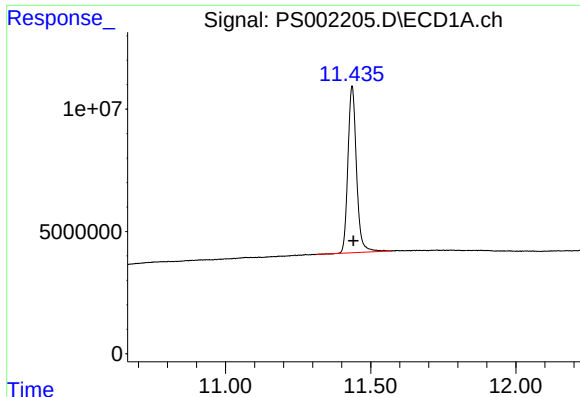

#4 2,4-DCAA


R.T.: 11.436 min
Delta R.T.: -0.005 min
Response: 139921439
Conc: 444.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

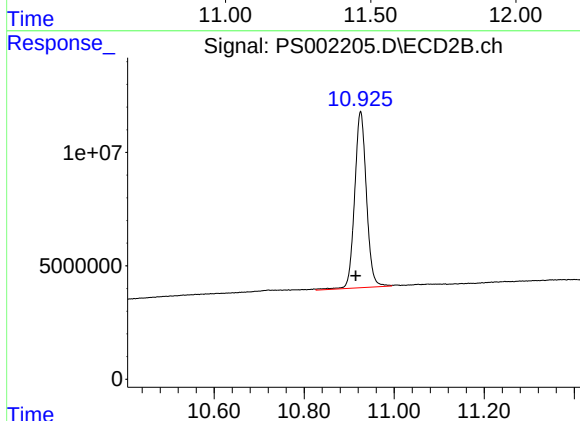


#4 2,4-DCAA

R.T.: 10.925 min
Delta R.T.: 0.011 min
Response: 141414910
Conc: 393.81 ng/ml

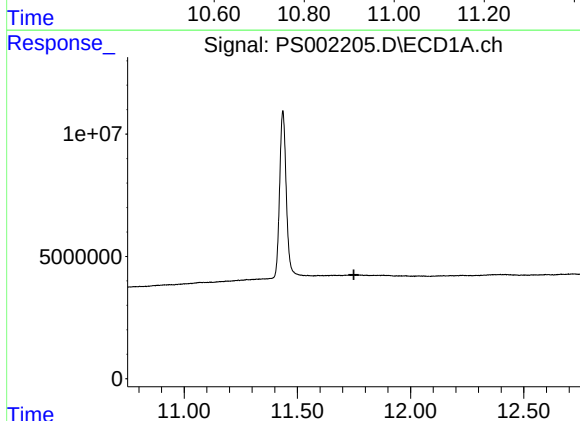


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.750 min
Response: 0
Conc: N.D.

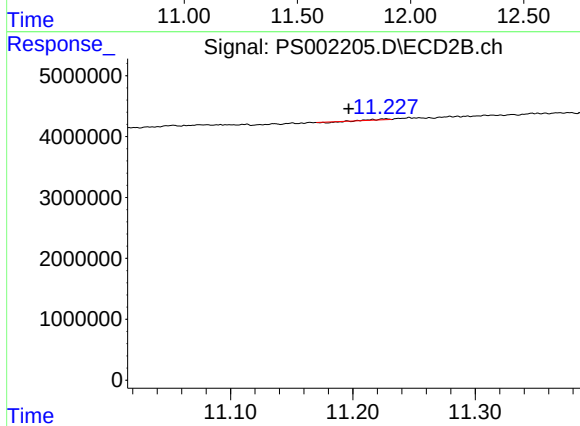

#5 DICAMBA


R.T.: 11.227 min
Delta R.T.: 0.031 min
Response: 53042
Conc: 0.04 ng/ml

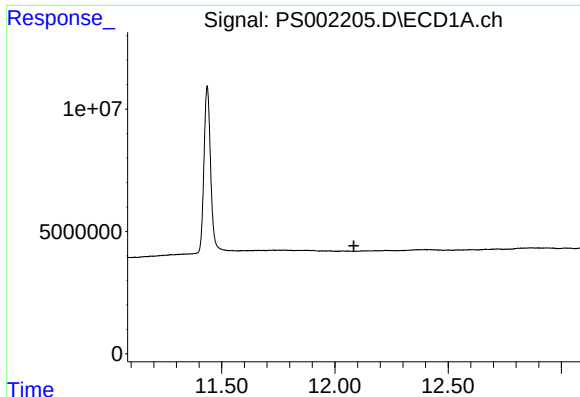

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 12.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

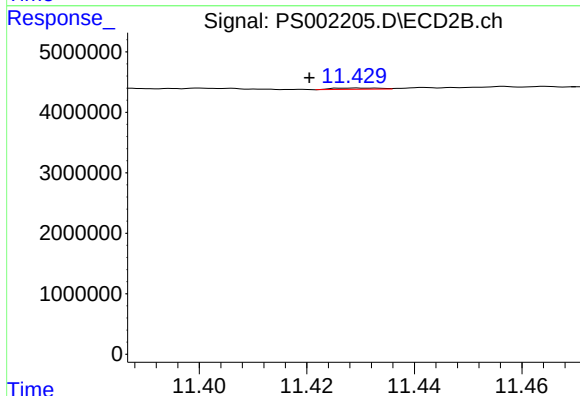


#6 MCPP

R.T.: 11.429 min
Delta R.T.: 0.009 min
Response: 129900
Conc: 0.15 ug/ml

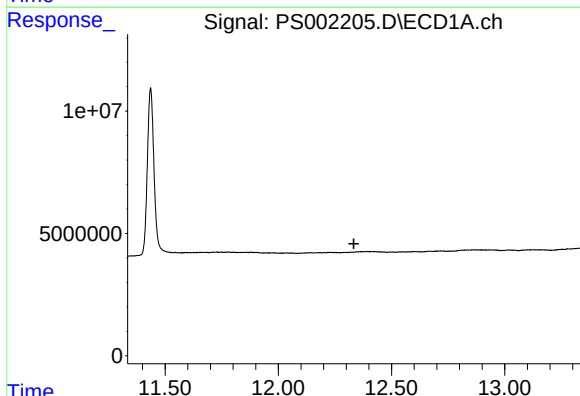


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

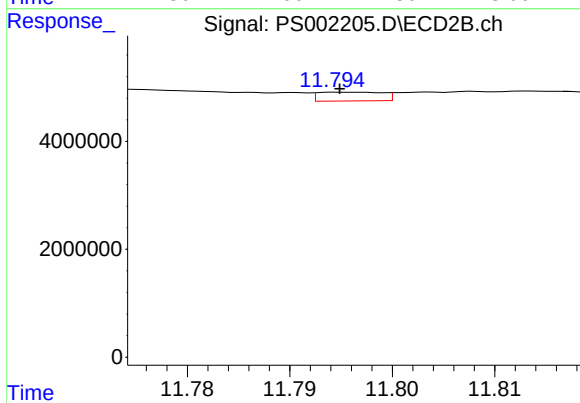

#7 MCPA


R.T.: 11.796 min
Delta R.T.: 0.000 min
Response: 708835
Conc: 0.52 ug/ml

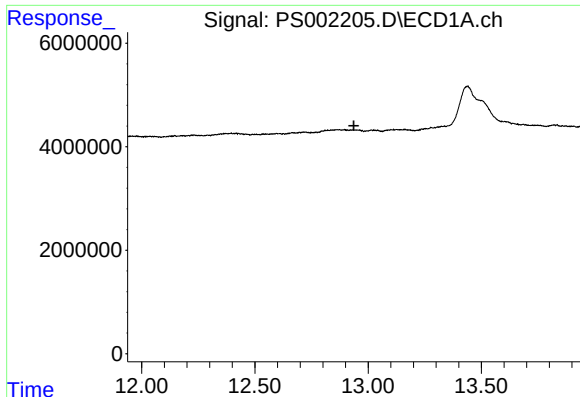

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

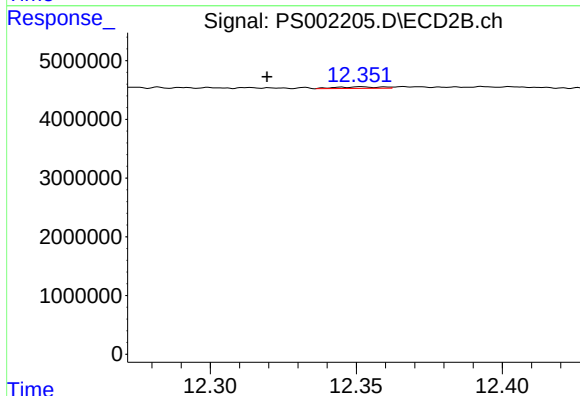


#8 DICHLORPROP

R.T.: 12.352 min
Delta R.T.: 0.032 min
Response: 288758
Conc: 0.90 ng/ml

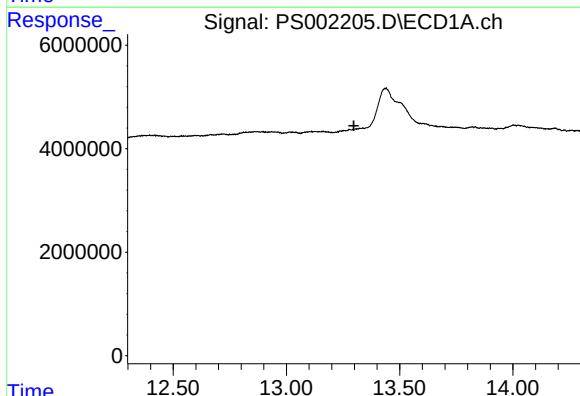


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

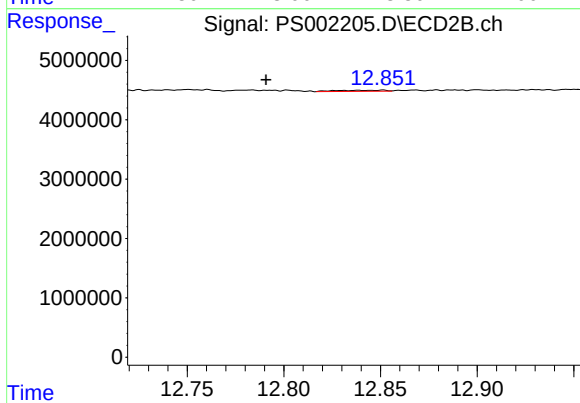

#9 2,4-D


R.T.: 12.851 min
Delta R.T.: 0.061 min
Response: 338113
Conc: 0.79 ng/ml

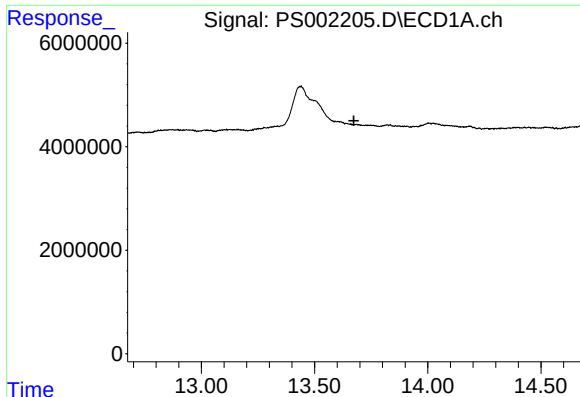

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

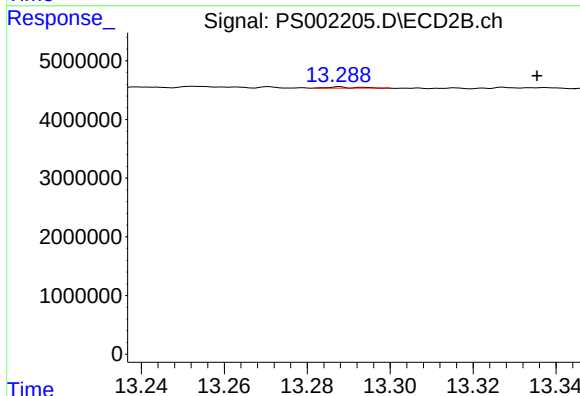


#10 Pentachlorophenol

R.T.: 13.288 min
Delta R.T.: -0.048 min
Response: 107952
Conc: 0.02 ng/ml

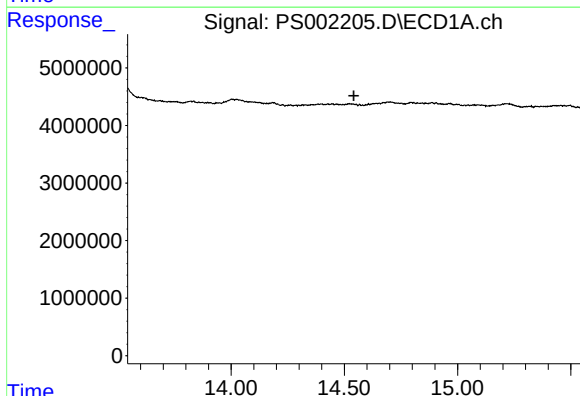


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.542 min
Response: 0
Conc: N.D.

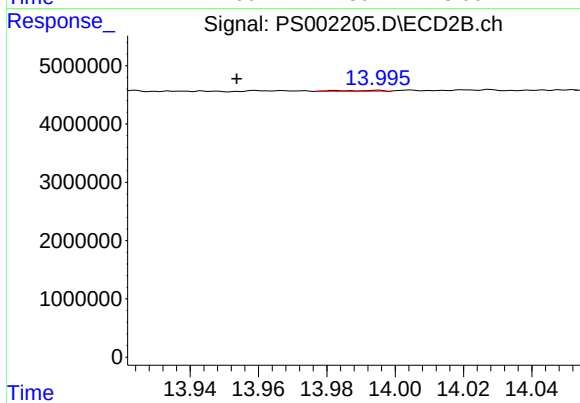

#11 2,4,5-TP (SILVEX)


R.T.: 13.995 min
Delta R.T.: 0.041 min
Response: 129621
Conc: 0.07 ng/ml

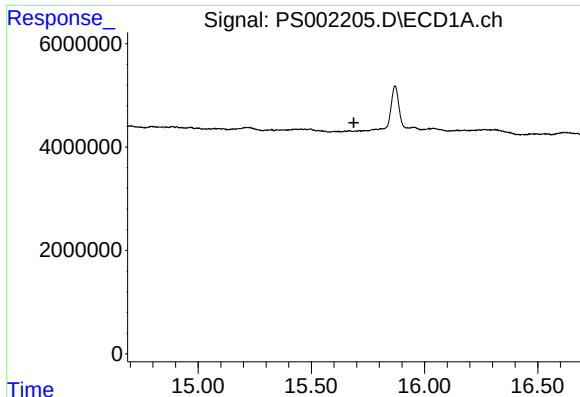

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

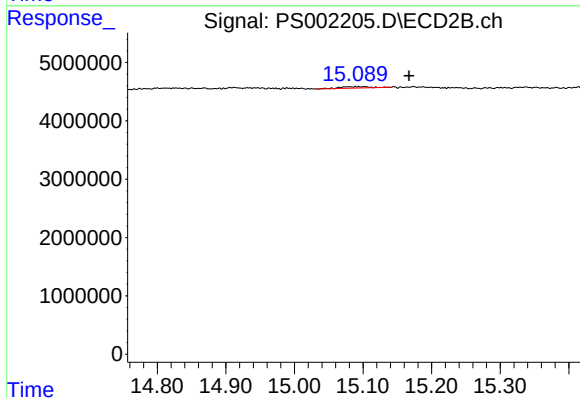


#13 2,4-DB

R.T.: 15.101 min
Delta R.T.: -0.066 min
Response: 717789
Conc: 3.24 ng/ml

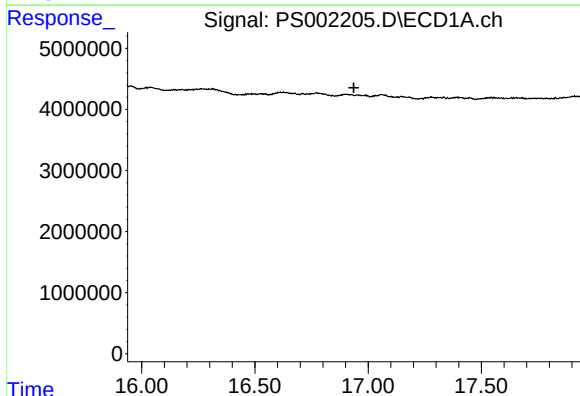


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

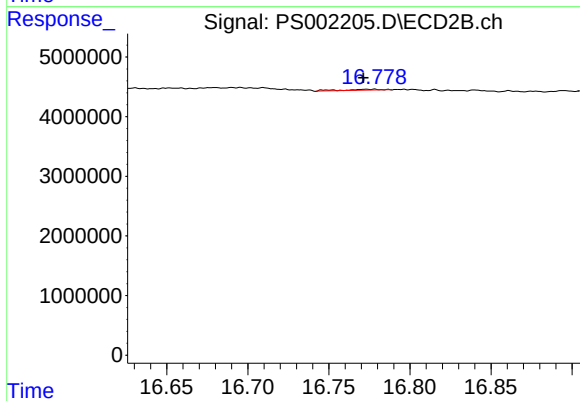

#15 Picloram


R.T.: 16.776 min
Delta R.T.: 0.005 min
Response: 250929
Conc: 0.11 ng/ml

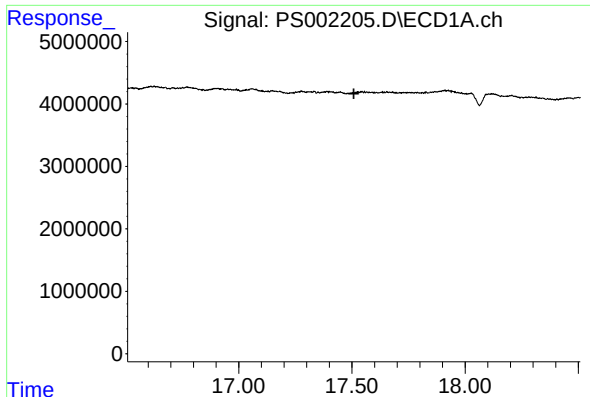

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

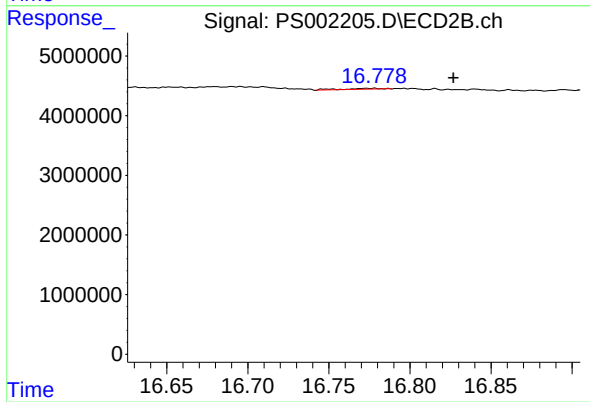

#16 DCPA

R.T.: 16.776 min
Delta R.T.: -0.051 min
Response: 250929
Conc: 0.11 ng/ml