

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
 Data File : PS002214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 01:33
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 02:36:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.456	10.947	144.9E6	140.5E6	460.514	391.380
Target Compounds							
7) T	MCPA	0.000	11.750	0	18377085	N.D.	13.578 #
8) T	DICHLORPROP	0.000	12.255	0	1020738	N.D.	3.179 #
10) T	Pentachlo...	0.000	13.282	0	142892	N.D.	0.030 #
11) T	2,4,5-TP ...	0.000	13.913	0	556384	N.D.	0.304 #
12) T	2,4,5-T	0.000	14.589	0	549828	N.D.	0.367 #
13) T	2,4-DB	0.000	15.213	0	258061	N.D.	1.165 #
14) T	DINOSEB	0.000	15.601	0	294384	N.D.	0.233 #
15) T	Picloram	0.000	16.808	0	74387	N.D.	0.033 #
16) T	DCPA	0.000	16.821	0	87609	N.D.	0.037 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103018\
Data File : PS002214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 01:33
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 02:36:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

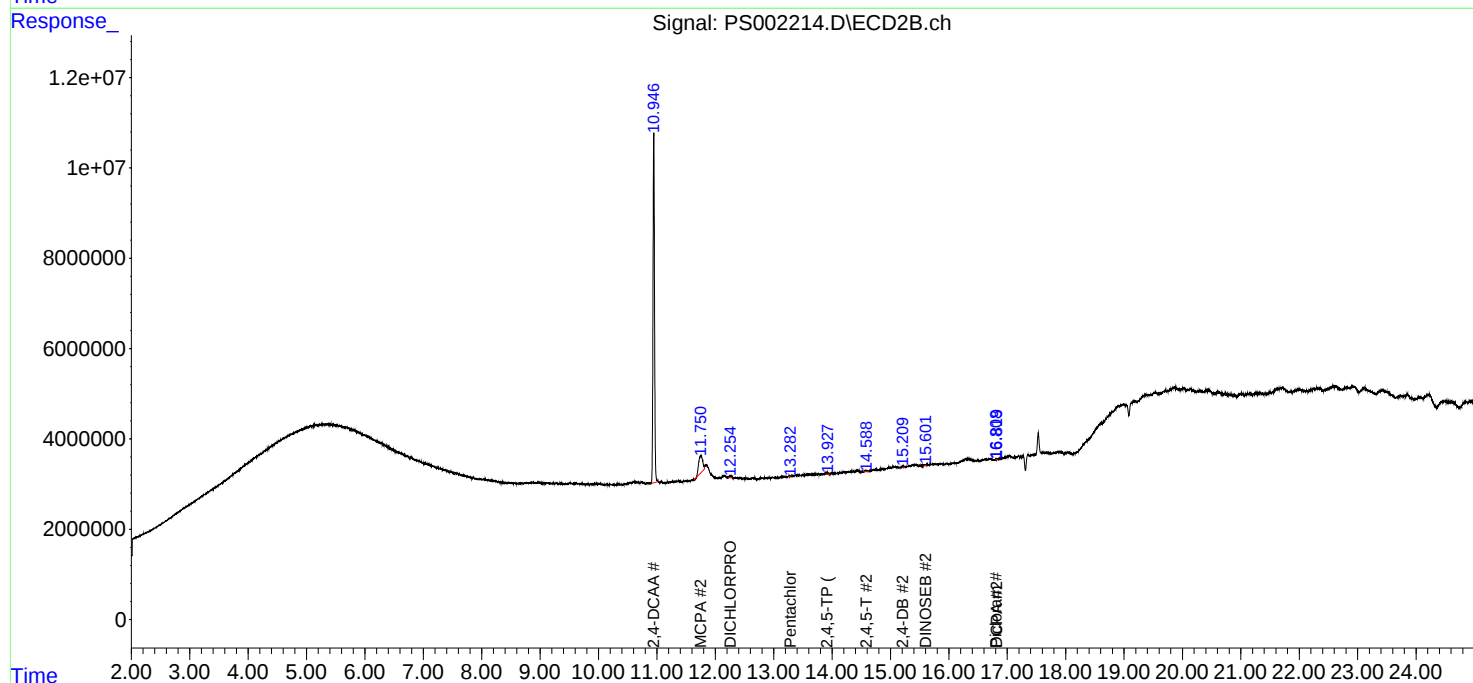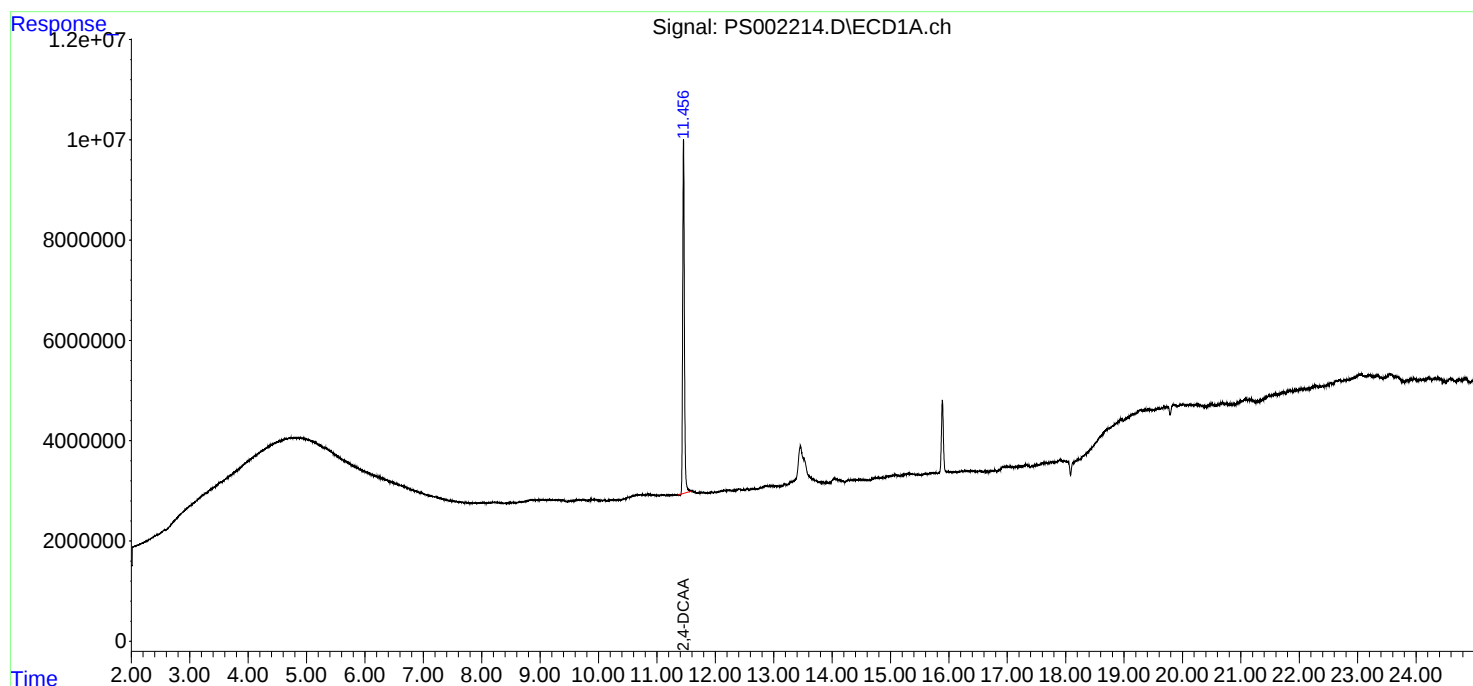


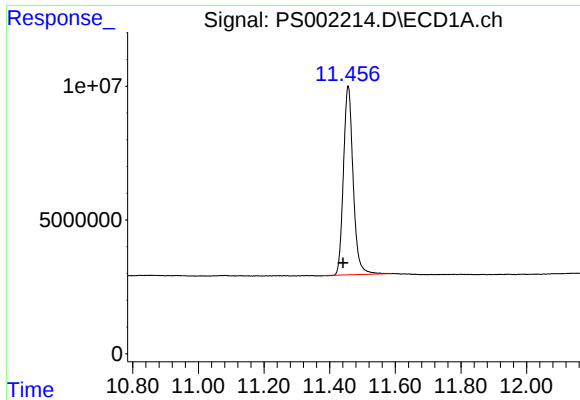

#4 2,4-DCAA


R.T.: 11.456 min
Delta R.T.: 0.015 min
Response: 144917146
Conc: 460.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

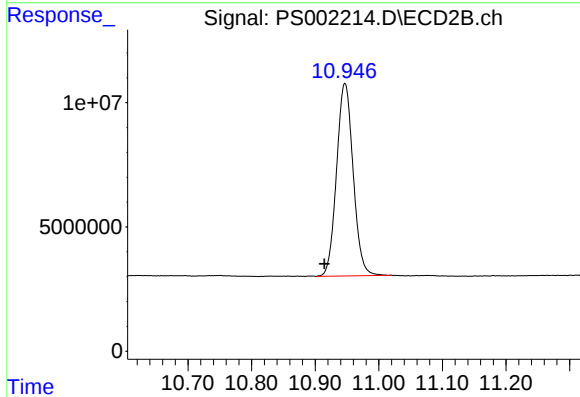


#4 2,4-DCAA

R.T.: 10.947 min
Delta R.T.: 0.032 min
Response: 140543588
Conc: 391.38 ng/ml

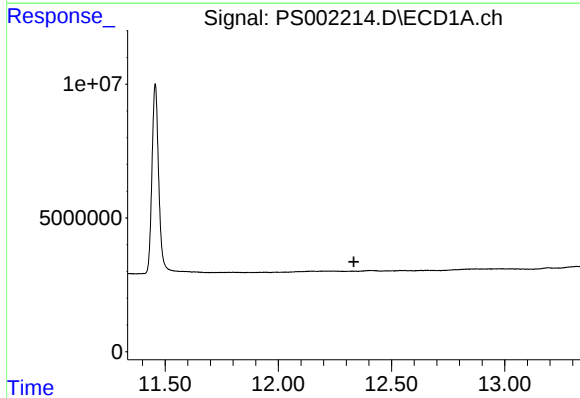


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

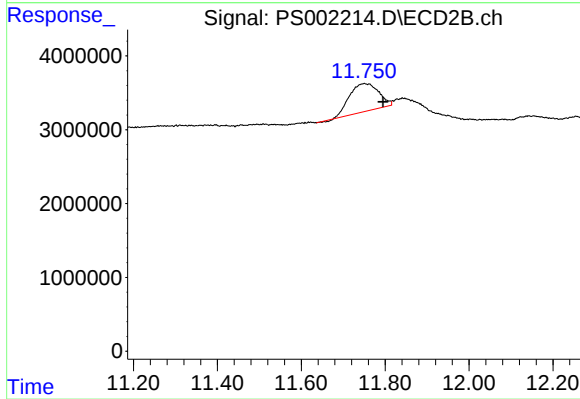

#7 MCPA


R.T.: 11.750 min
Delta R.T.: -0.045 min
Response: 18377085
Conc: 13.58 ug/ml

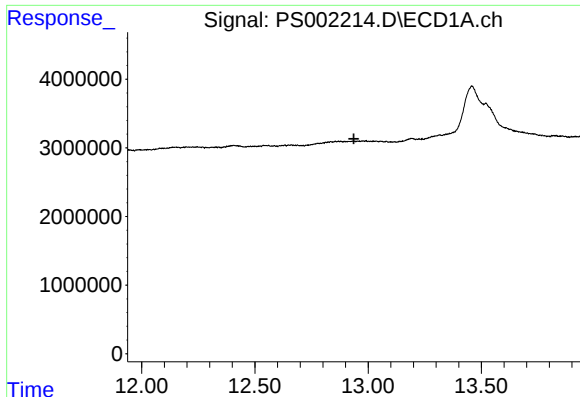

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

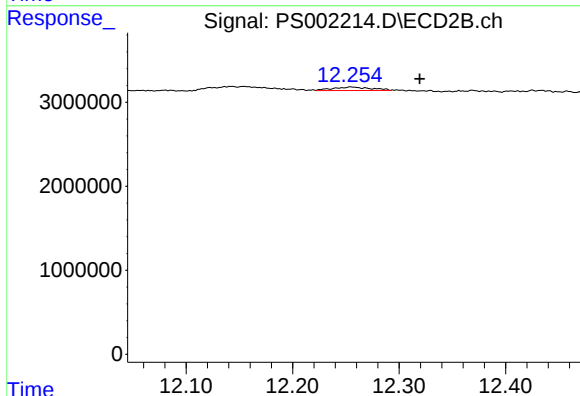


#8 DICHLORPROP

R.T.: 12.255 min
Delta R.T.: -0.065 min
Response: 1020738
Conc: 3.18 ng/ml

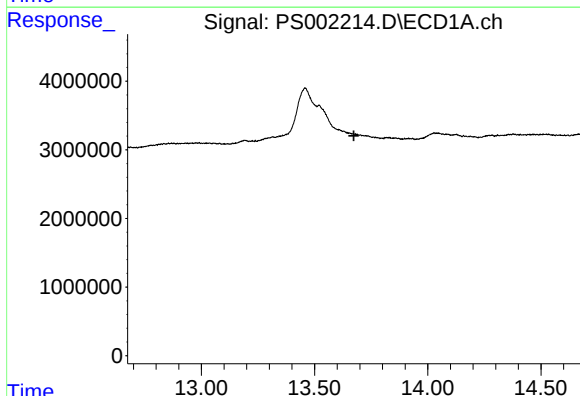


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.674 min
Response: 0
Conc: N.D.

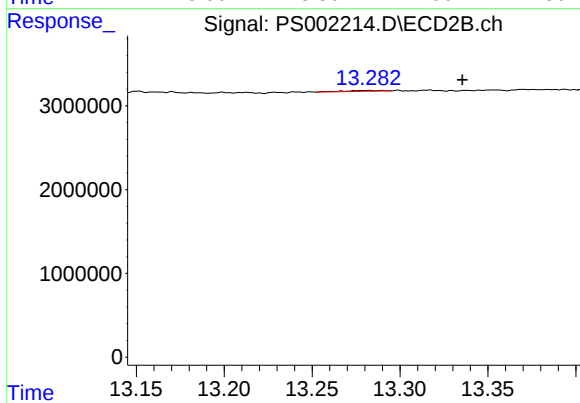

#10 Pentachlorophenol


R.T.: 13.282 min
Delta R.T.: -0.053 min
Response: 142892
Conc: 0.03 ng/ml

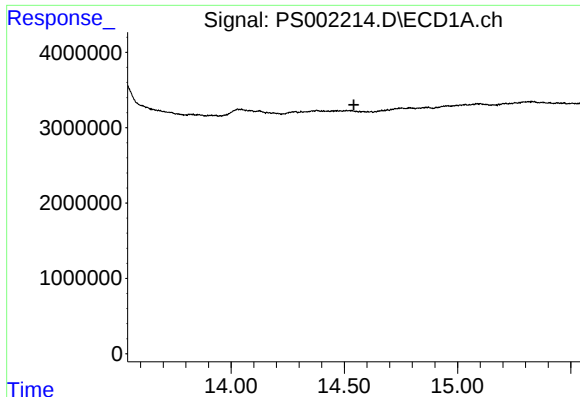

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

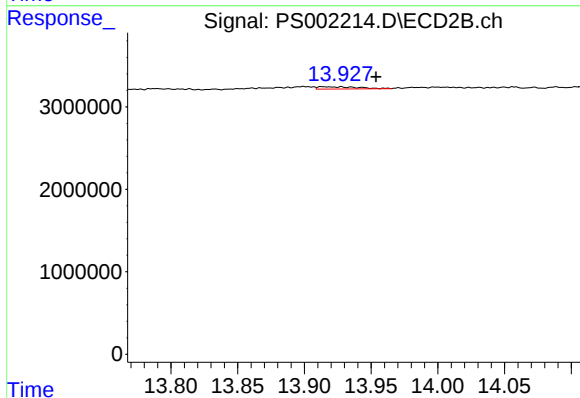


#11 2,4,5-TP (SILVEX)

R.T.: 13.913 min
Delta R.T.: -0.040 min
Response: 556384
Conc: 0.30 ng/ml

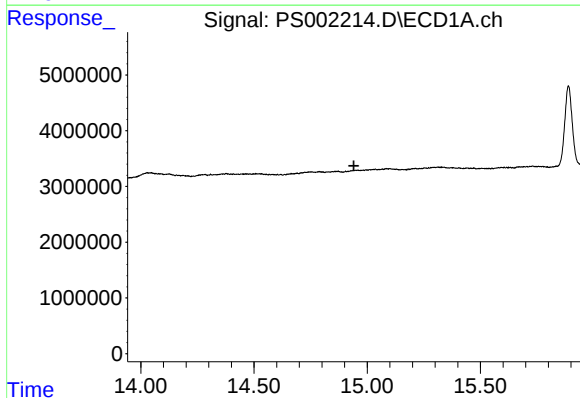


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

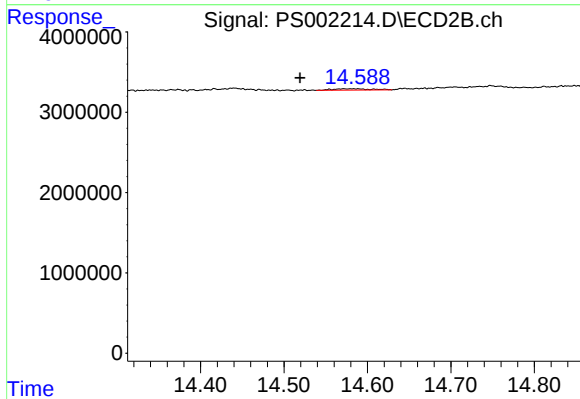

#12 2,4,5-T


R.T.: 14.589 min
Delta R.T.: 0.070 min
Response: 549828
Conc: 0.37 ng/ml

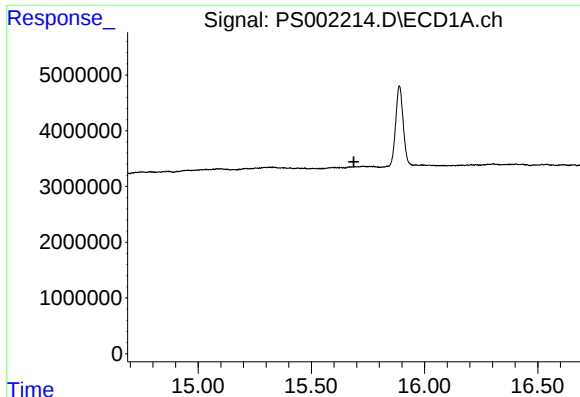

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

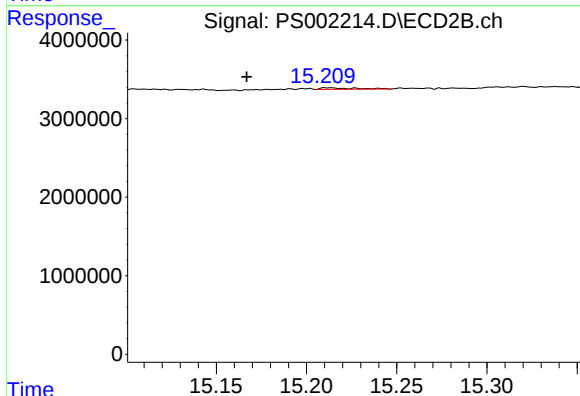


#13 2,4-DB

R.T.: 15.213 min
Delta R.T.: 0.046 min
Response: 258061
Conc: 1.16 ng/ml

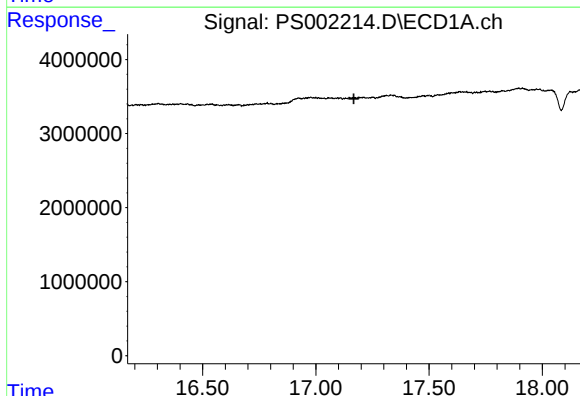


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

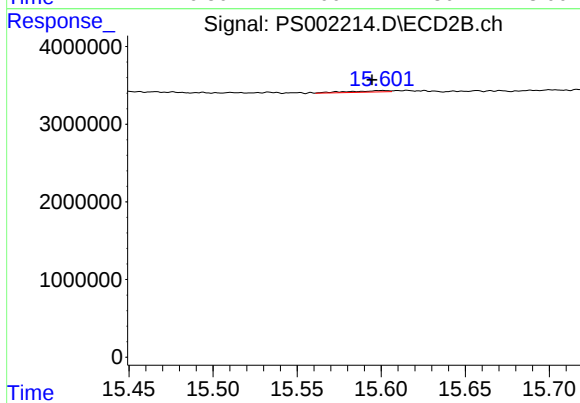

#14 DINOSEB


R.T.: 15.601 min
Delta R.T.: 0.006 min
Response: 294384
Conc: 0.23 ng/ml

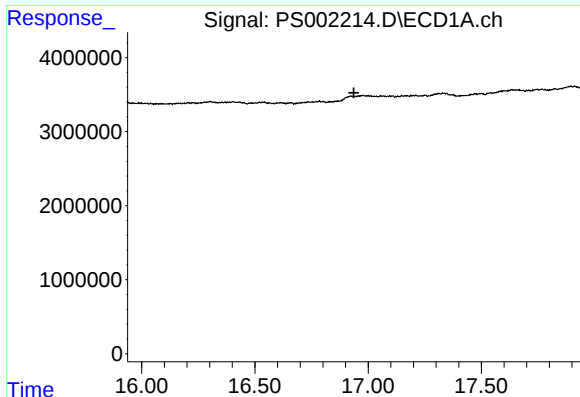

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

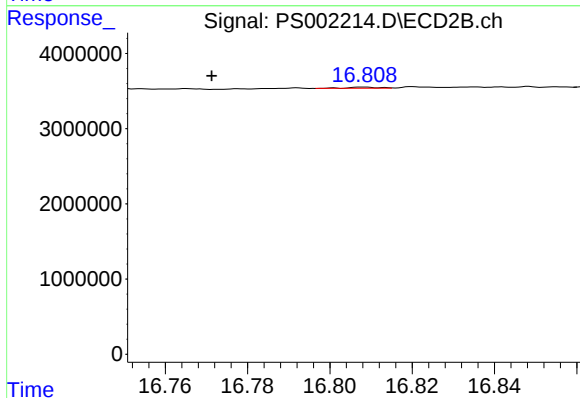


#15 Picloram

R.T.: 16.808 min
Delta R.T.: 0.037 min
Response: 74387
Conc: 0.03 ng/ml

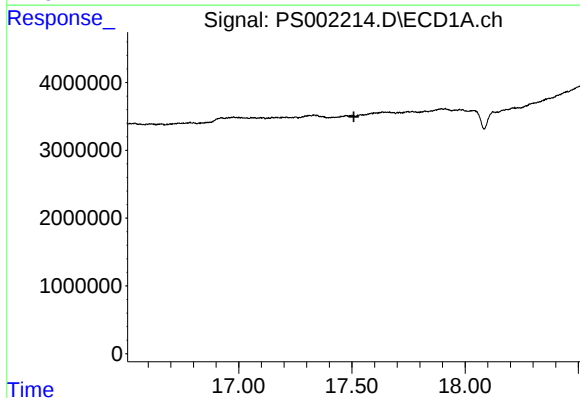

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

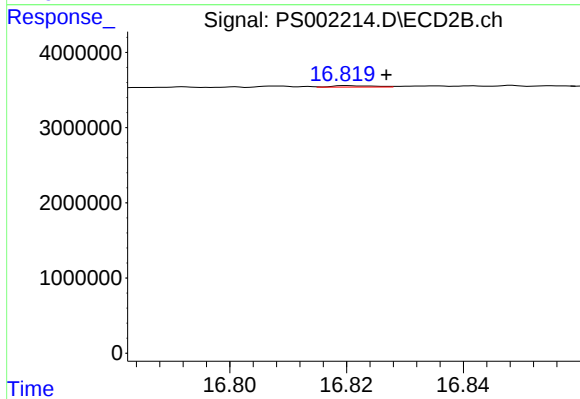

#16 DCPA

R.T.: 16.821 min
Delta R.T.: -0.006 min
Response: 87609
Conc: 0.04 ng/ml