

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
 Data File : PS007495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 10:05
 Operator : SM\AJ
 Sample : PB124343BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 18:12:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.435	5.161	752.6E6	414.7E6	549.841	589.630
Target Compounds							
2) T	3,5-DICHL...	0.000	4.496	0	41420621	N.D.	48.139
3) T	4-Nitroph...	0.000	4.846	0	25613328	N.D.	64.861
7) T	MCPA	5.818	0.000	70092775	0	13.590	N.D. #
8) T	DICHLORPROP	0.000	5.816	0	45217629	N.D.	69.436
9) T	2,4-D	6.489	0.000	76171837	0	61.811	N.D. #
11) T	2,4,5-TP ...	0.000	6.757	0	26850063	N.D.	7.059
15) T	Picloram	0.000	8.906	0	3266744	N.D.	<MDL
16) T	DCPA	0.000	8.906	0	3266744	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
Data File : PS007495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 10:05
Operator : SM\AJ
Sample : PB124343BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 18:12:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

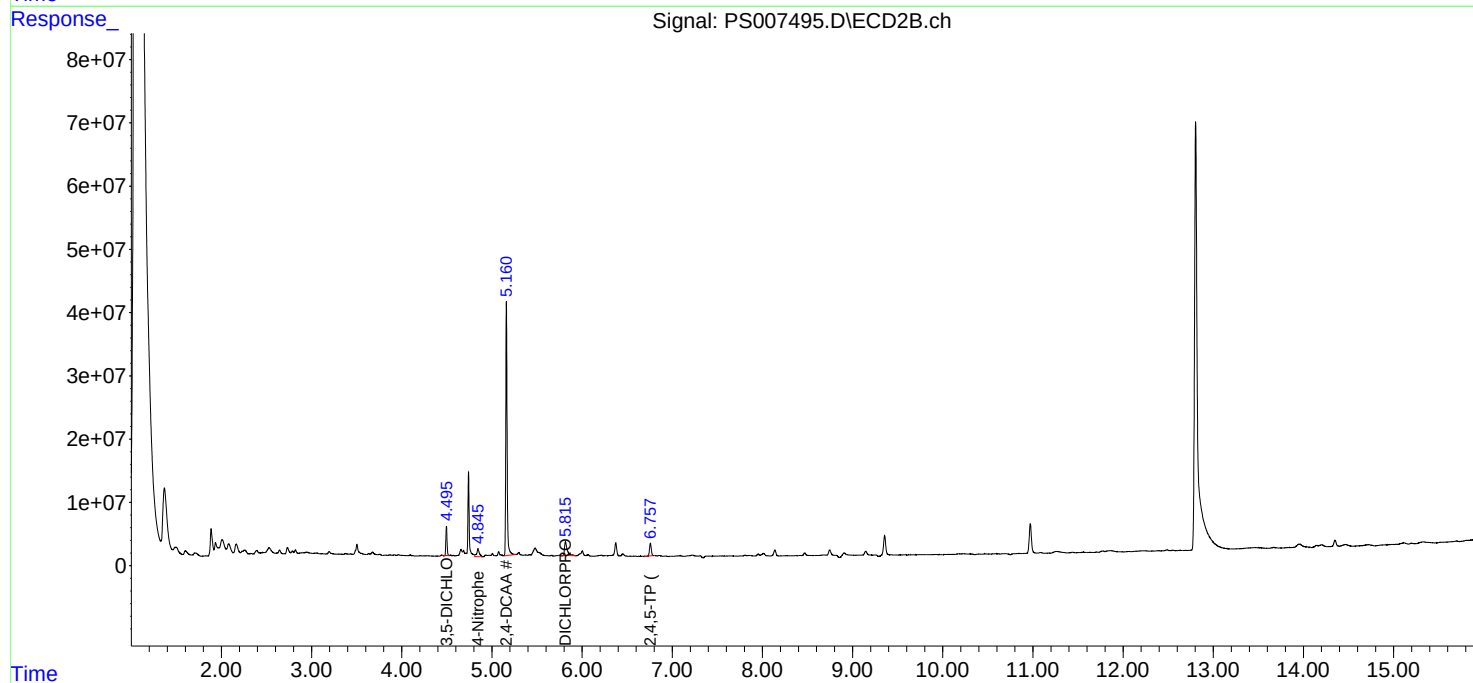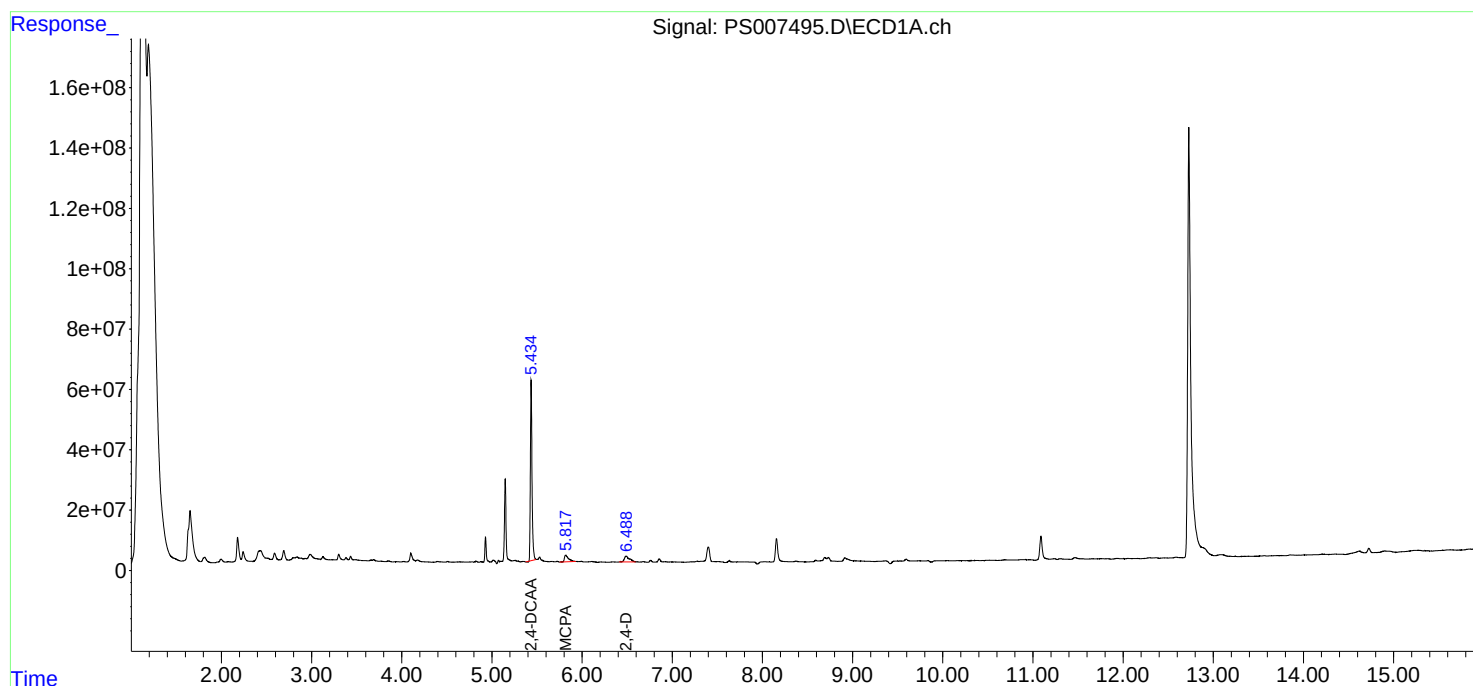


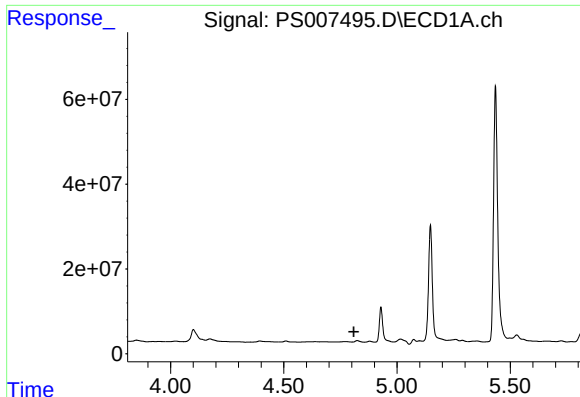

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

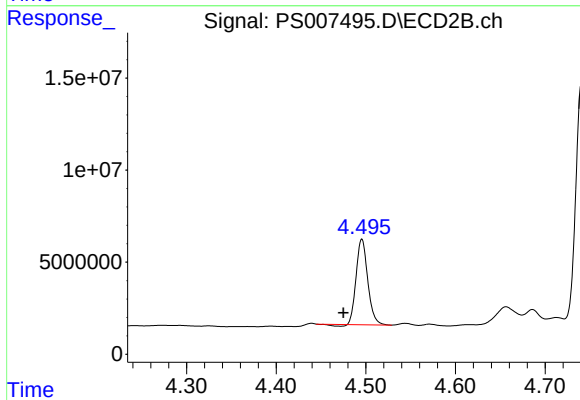


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.496 min
Delta R.T.: 0.021 min
Response: 41420621
Conc: 48.14 ng/ml

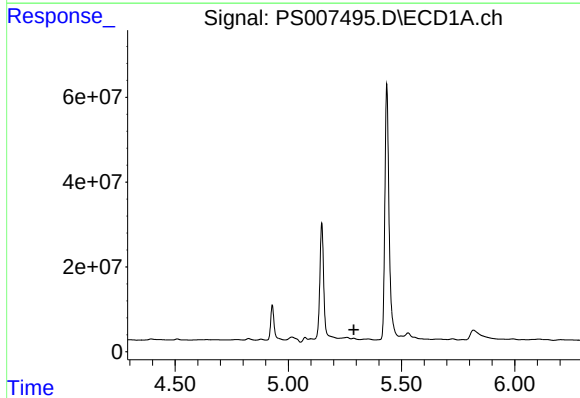


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

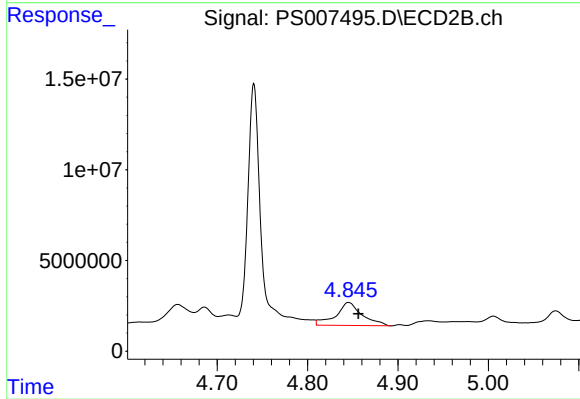

#3 4-Nitrophenol


R.T.: 4.846 min
Delta R.T.: -0.011 min
Response: 25613328
Conc: 64.86 ng/ml

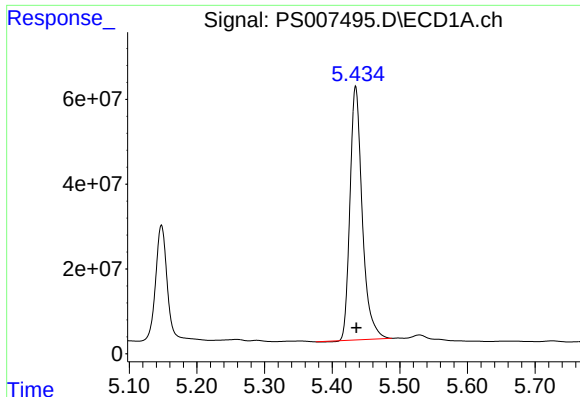

#4 2,4-DCAA


R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 752550554
Conc: 549.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

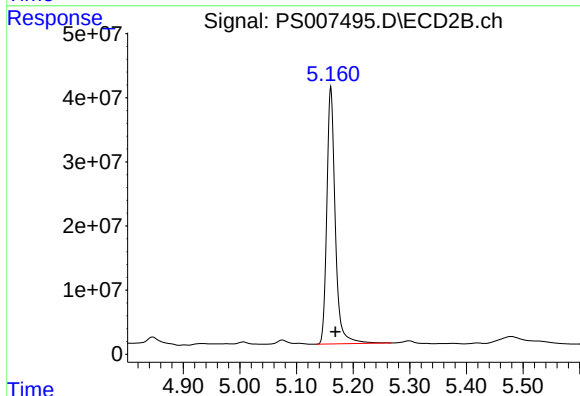


#4 2,4-DCAA

R.T.: 5.161 min
Delta R.T.: -0.008 min
Response: 414690838
Conc: 589.63 ng/ml

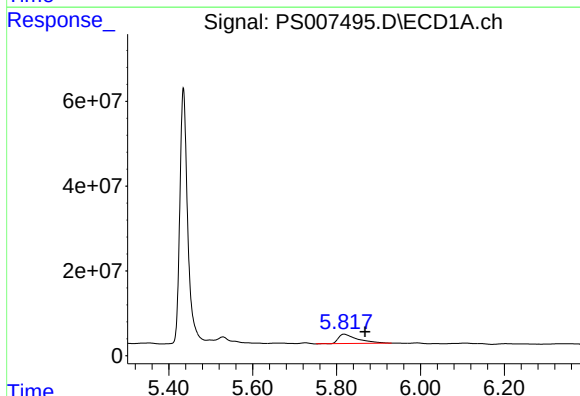


#7 MCPA

R.T.: 5.818 min
Delta R.T.: -0.050 min
Response: 70092775
Conc: 13.59 ug/ml

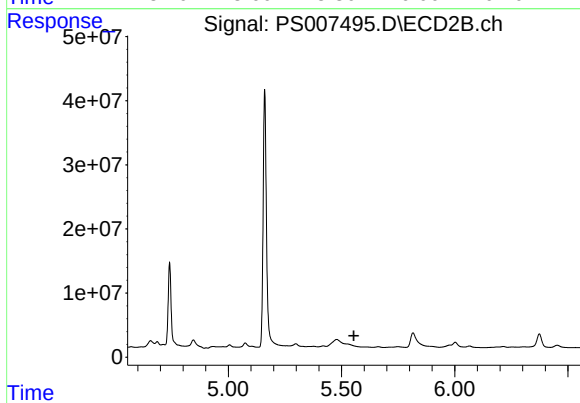

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.555 min
Response: 0
Conc: N.D.

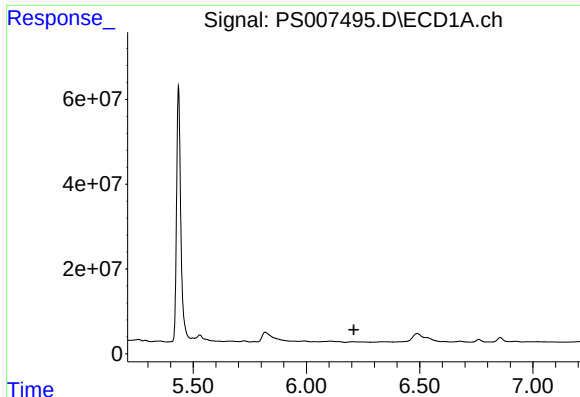

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

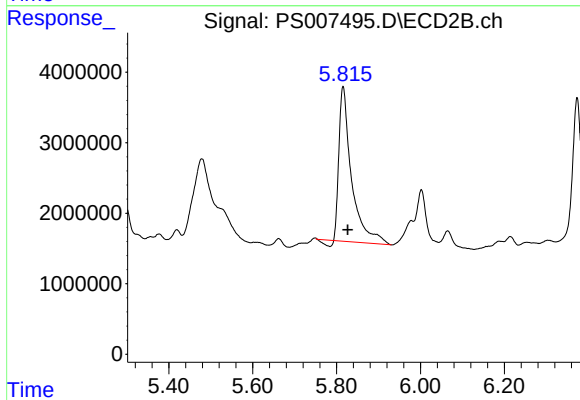


#8 DICHLORPROP

R.T.: 5.816 min
Delta R.T.: -0.011 min
Response: 45217629
Conc: 69.44 ng/ml

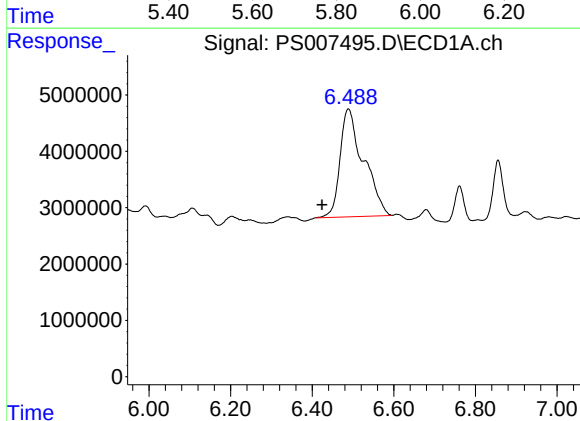


#9 2,4-D

R.T.: 6.489 min
Delta R.T.: 0.064 min
Response: 76171837
Conc: 61.81 ng/ml

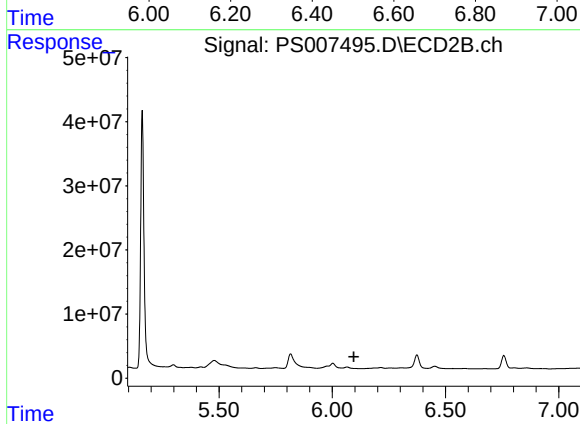

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

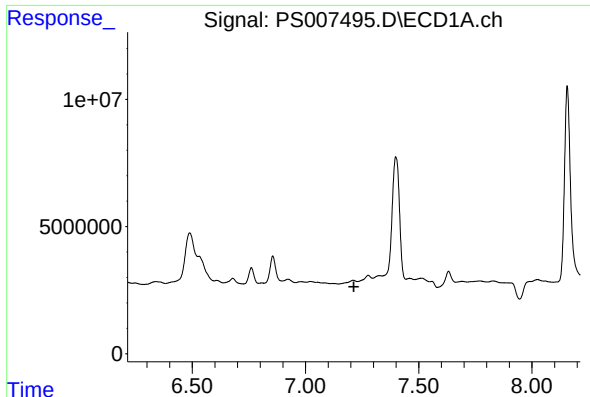

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

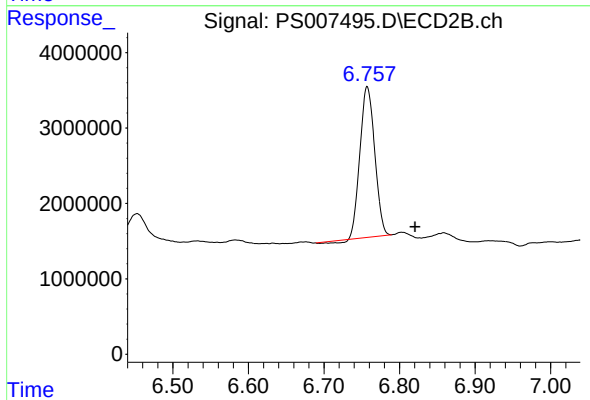

#11 2,4,5-TP (SILVEX)

R.T.: 6.757 min
Delta R.T.: -0.063 min
Response: 26850063
Conc: 7.06 ng/ml