

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
 Data File : PS007500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 11:55
 Operator : SM\AJ
 Sample : K5539-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 18:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.451	5.177	262.5E6	131.5E6	191.757	186.996
Target Compounds							
1) T	Dalapon	2.012	1.720	93614818	276.6E6	55.947	303.956 #
2) T	3,5-DICHL...	0.000	4.512	0	53112579	N.D.	61.728
5) T	DICAMBA	5.545	5.293	54611197	15904356	11.115	6.112 #
7) T	MCPA	5.921	5.547	25759456	23919172	4.994	8.228 #
8) T	DICHLORPROP	0.000	5.765	0	5083832	N.D.	7.807
9) T	2,4-D	0.000	6.081	0	9410790	N.D.	11.796
10) T	Pentachlo...	0.000	6.470	0	4014204	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.773	0	5859127	N.D.	1.540
14) T	DINOSEB	0.000	7.969	0	60535489	N.D.	21.563
15) T	Picloram	0.000	8.917	0	18913300	N.D.	3.080
16) T	DCPA	0.000	8.917	0	18913300	N.D.	3.772



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
Data File : PS007500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 11:55
Operator : SM\AJ
Sample : K5539-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 18:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

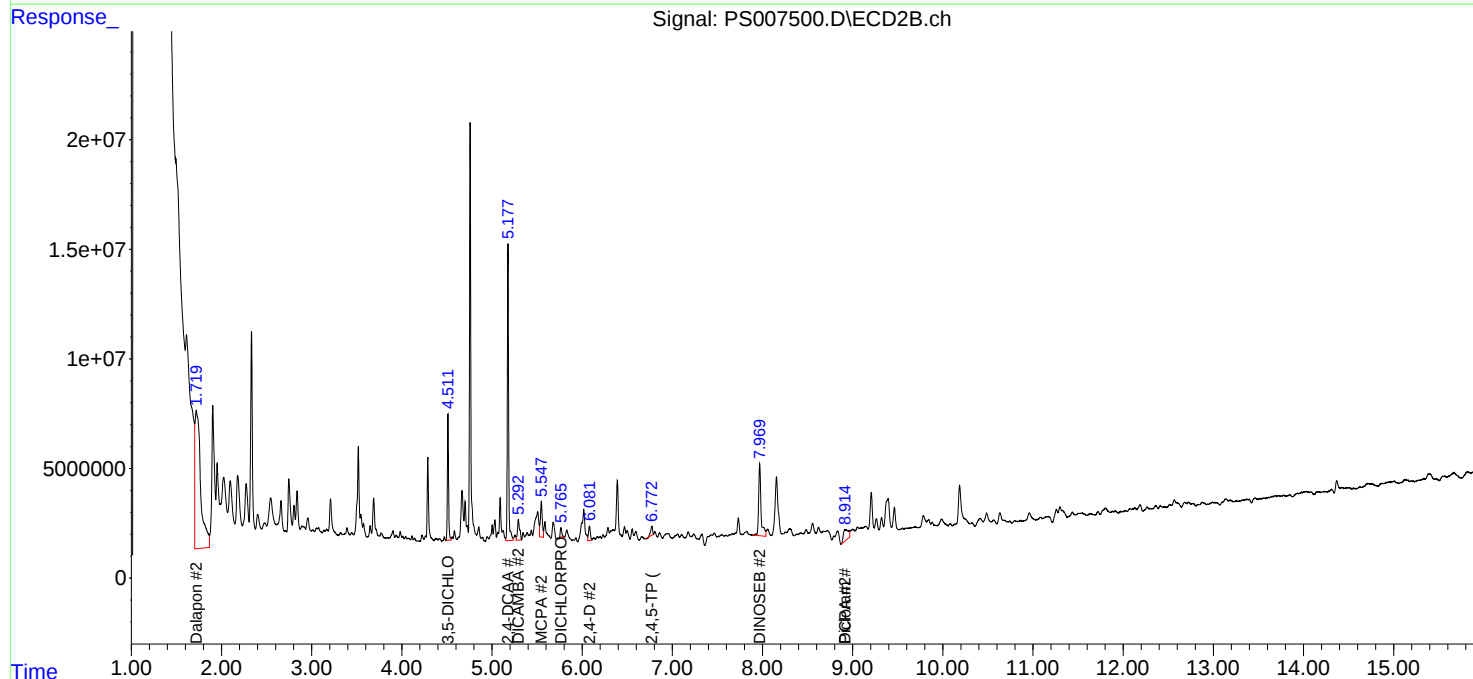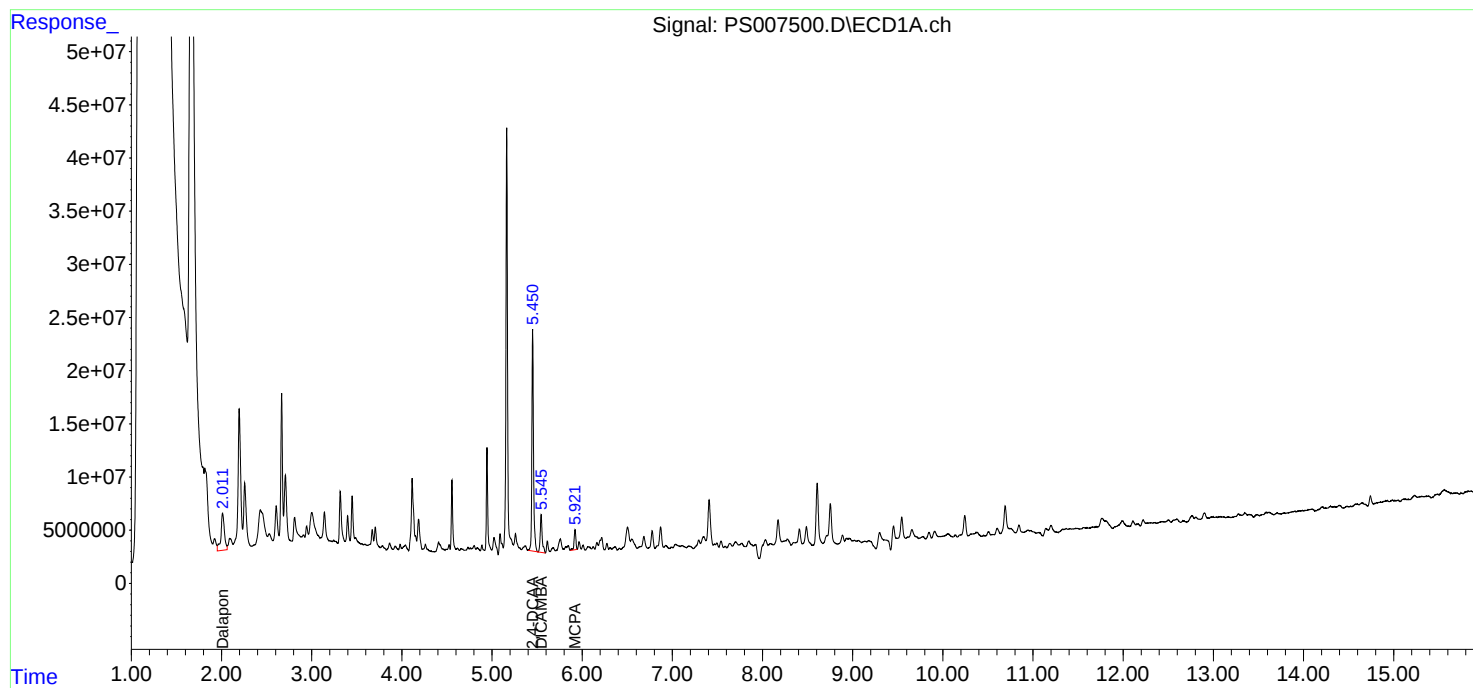


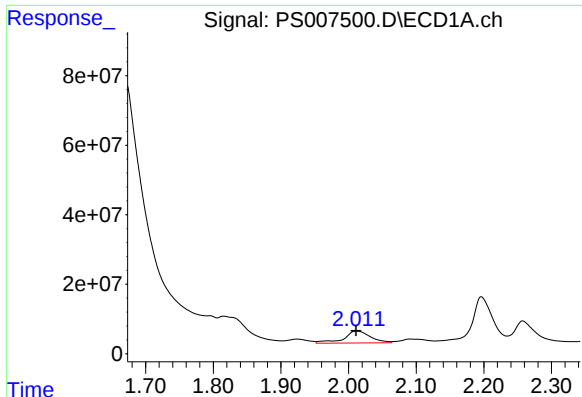

#1 Dalapon


R.T.: 2.012 min
Delta R.T.: 0.001 min
Response: 93614818
Conc: 55.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

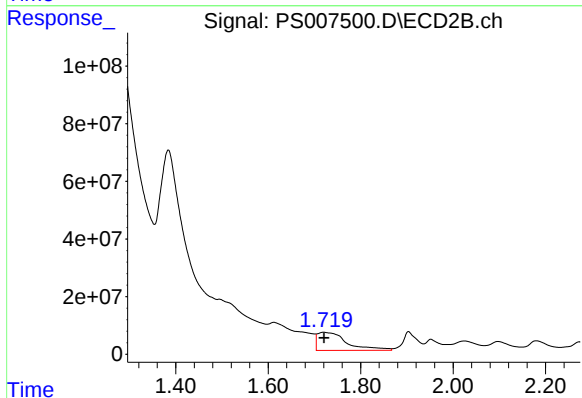


#1 Dalapon

R.T.: 1.720 min
Delta R.T.: 0.000 min
Response: 276600806
Conc: 303.96 ng/ml

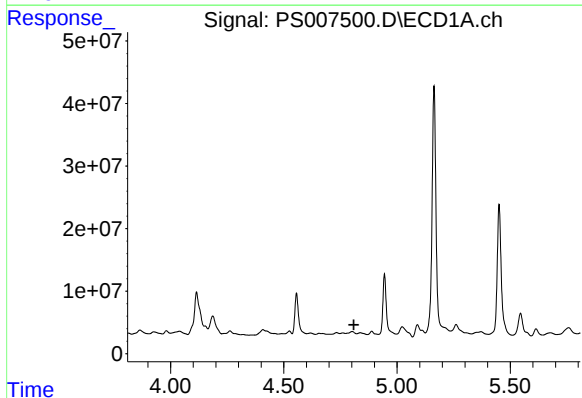


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

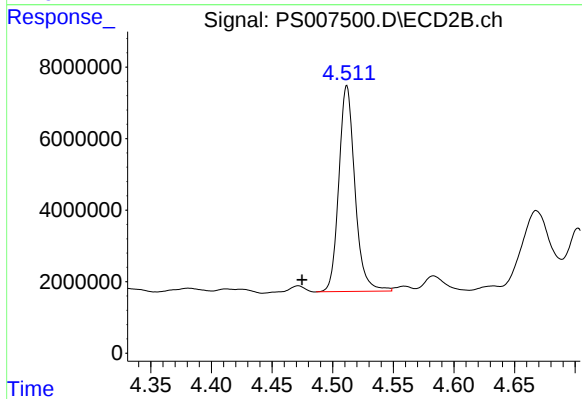

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.512 min
Delta R.T.: 0.037 min
Response: 53112579
Conc: 61.73 ng/ml

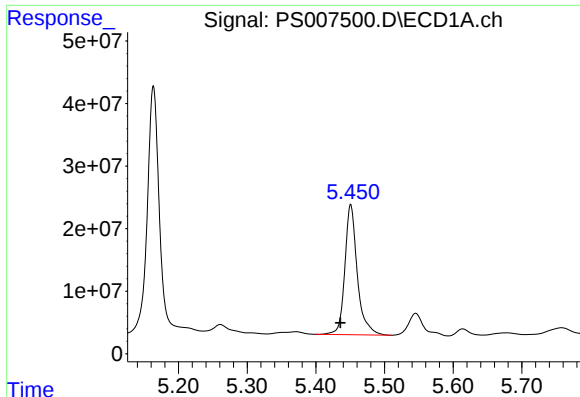

#4 2,4-DCAA


R.T.: 5.451 min
Delta R.T.: 0.015 min
Response: 262451773
Conc: 191.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

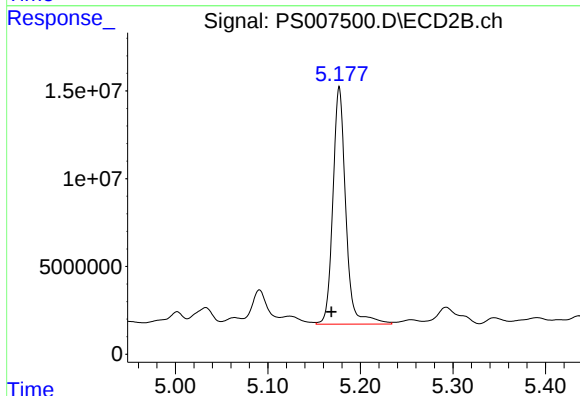


#4 2,4-DCAA

R.T.: 5.177 min
Delta R.T.: 0.009 min
Response: 131515361
Conc: 187.00 ng/ml

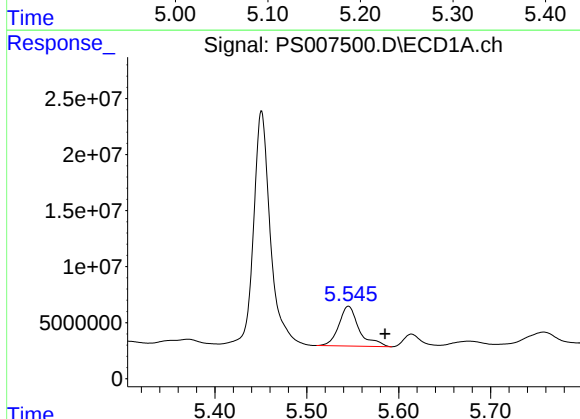


#5 DICAMBA

R.T.: 5.545 min
Delta R.T.: -0.040 min
Response: 54611197
Conc: 11.11 ng/ml

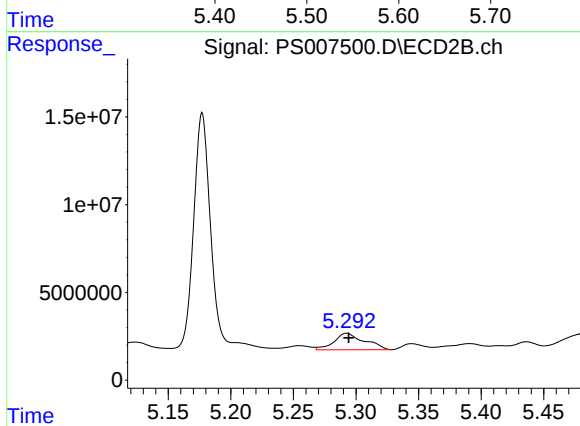

#5 DICAMBA


R.T.: 5.293 min
Delta R.T.: -0.002 min
Response: 15904356
Conc: 6.11 ng/ml

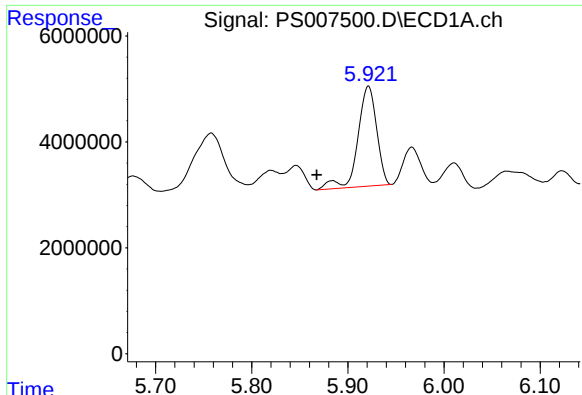

#7 MCPA


R.T.: 5.921 min
Delta R.T.: 0.054 min
Response: 25759456
Conc: 4.99 ug/ml

Instrument :
ECD_S
ClientSampleId :

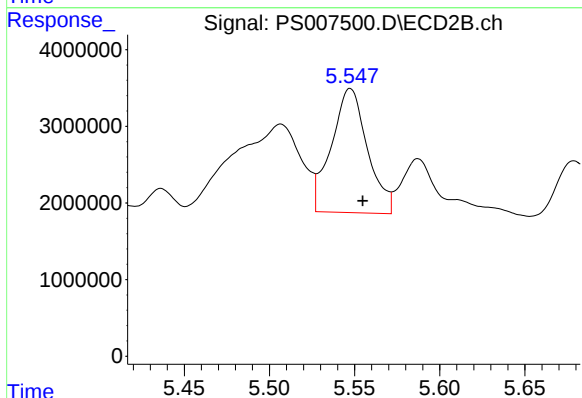


#7 MCPA

R.T.: 5.547 min
Delta R.T.: -0.007 min
Response: 23919172
Conc: 8.23 ug/ml

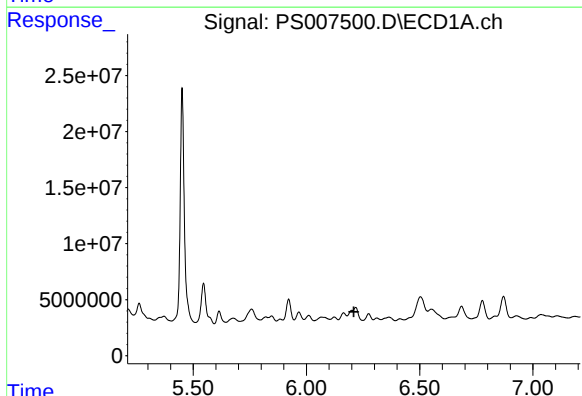


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

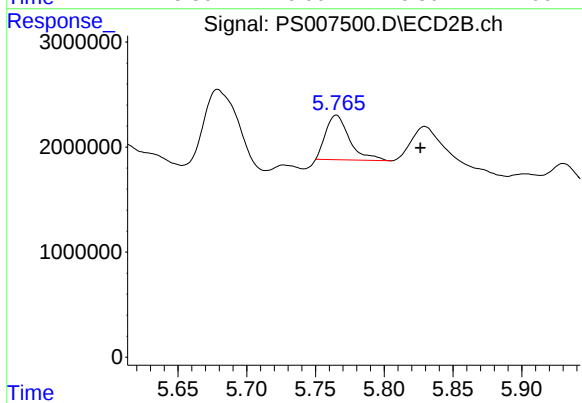

#8 DICHLORPROP


R.T.: 5.765 min
Delta R.T.: -0.061 min
Response: 5083832
Conc: 7.81 ng/ml

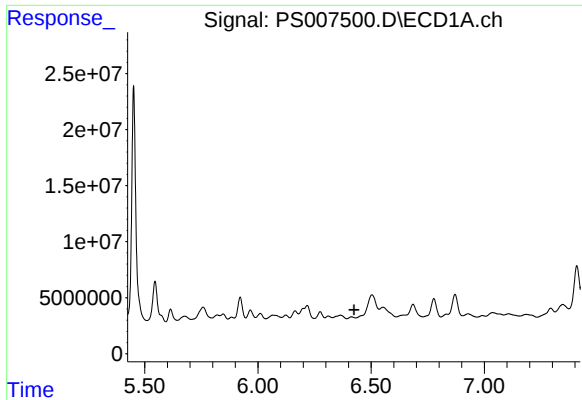

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

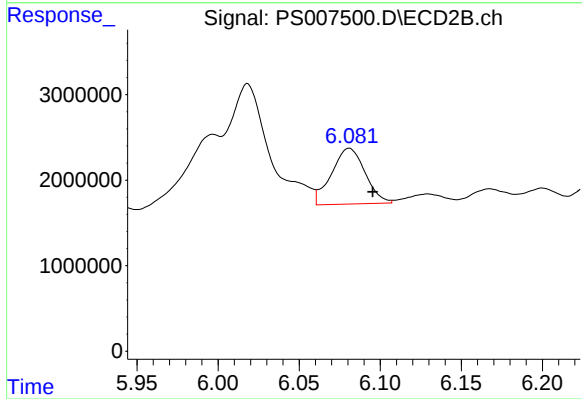


#9 2,4-D

R.T.: 6.081 min
Delta R.T.: -0.014 min
Response: 9410790
Conc: 11.80 ng/ml

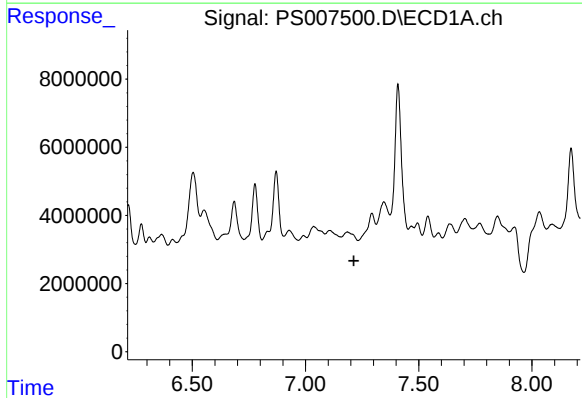


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

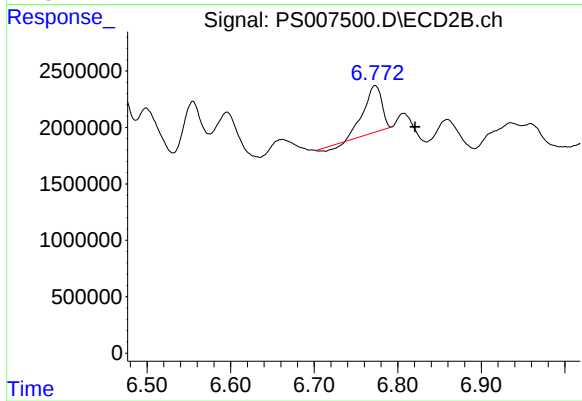

#11 2,4,5-TP (SILVEX)


R.T.: 6.773 min
Delta R.T.: -0.048 min
Response: 5859127
Conc: 1.54 ng/ml

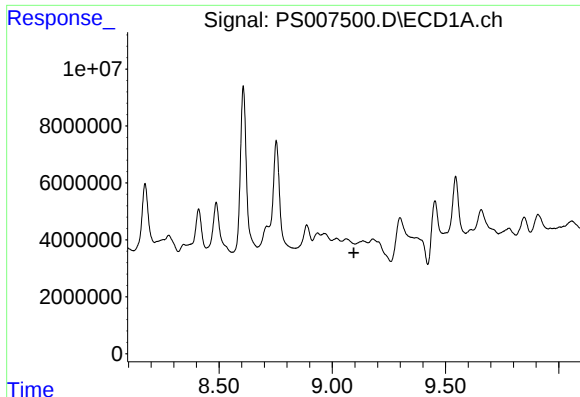

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

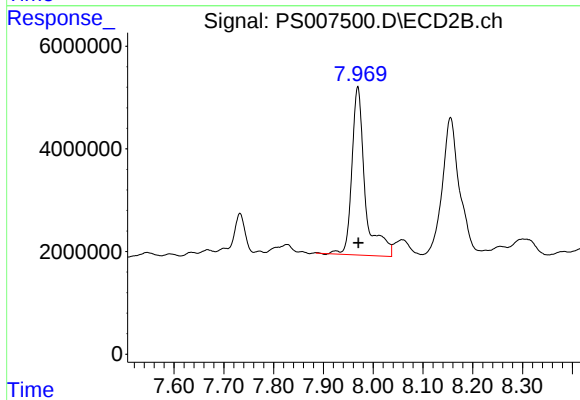


#14 DINOSEB

R.T.: 7.969 min
Delta R.T.: -0.002 min
Response: 60535489
Conc: 21.56 ng/ml

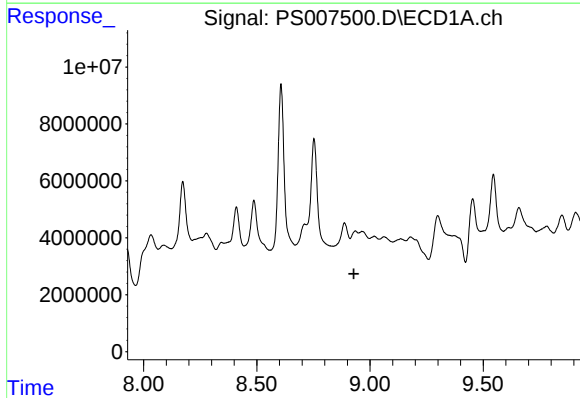


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

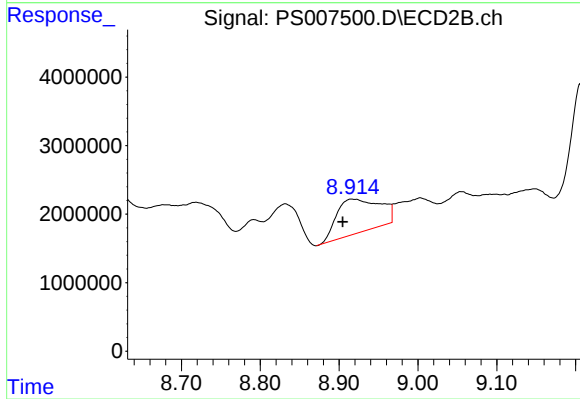

#15 Picloram


R.T.: 8.917 min
Delta R.T.: 0.013 min
Response: 18913300
Conc: 3.08 ng/ml

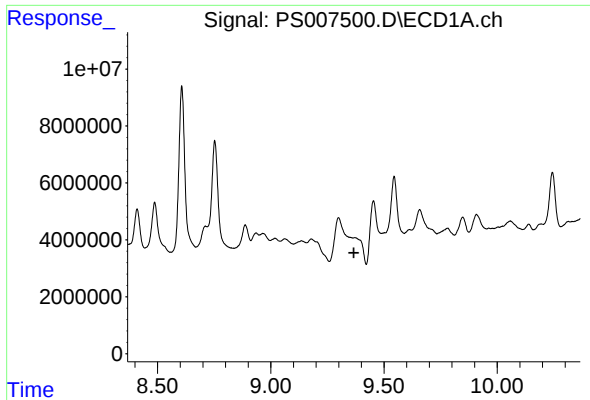

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

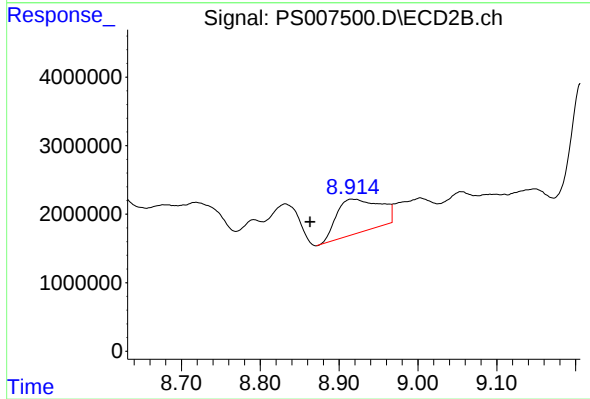

#16 DCPA

R.T.: 8.917 min
Delta R.T.: 0.054 min
Response: 18913300
Conc: 3.77 ng/ml