

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
 Data File : PS007501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 12:17
 Operator : SM\AJ
 Sample : K5539-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 30 18:13:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.157	149.9E6	67897075	109.506	96.540
Target Compounds							
1) T	Dalapon	1.990	0.000	47889313	0	28.620	N.D. #
2) T	3,5-DICHL...	0.000	4.490	0	57672738	N.D.	67.028
5) T	DICAMBA	5.525	5.291	58685360	15211468	11.944	5.846 #
7) T	MCPA	5.900	5.526	24537934	24011261	4.757	8.259 #
9) T	2,4-D	6.483	6.060	86733698	5807039	70.381	7.279 #
10) T	Pentachlo...	0.000	6.443	0	9425213	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.752	0	4242608	N.D.	1.115
14) T	DINOSEB	0.000	7.947	0	47182901	N.D.	16.807
15) T	Picloram	0.000	8.935	0	30920733	N.D.	5.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
Data File : PS007501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 12:17
Operator : SM\AJ
Sample : K5539-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 30 18:13:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

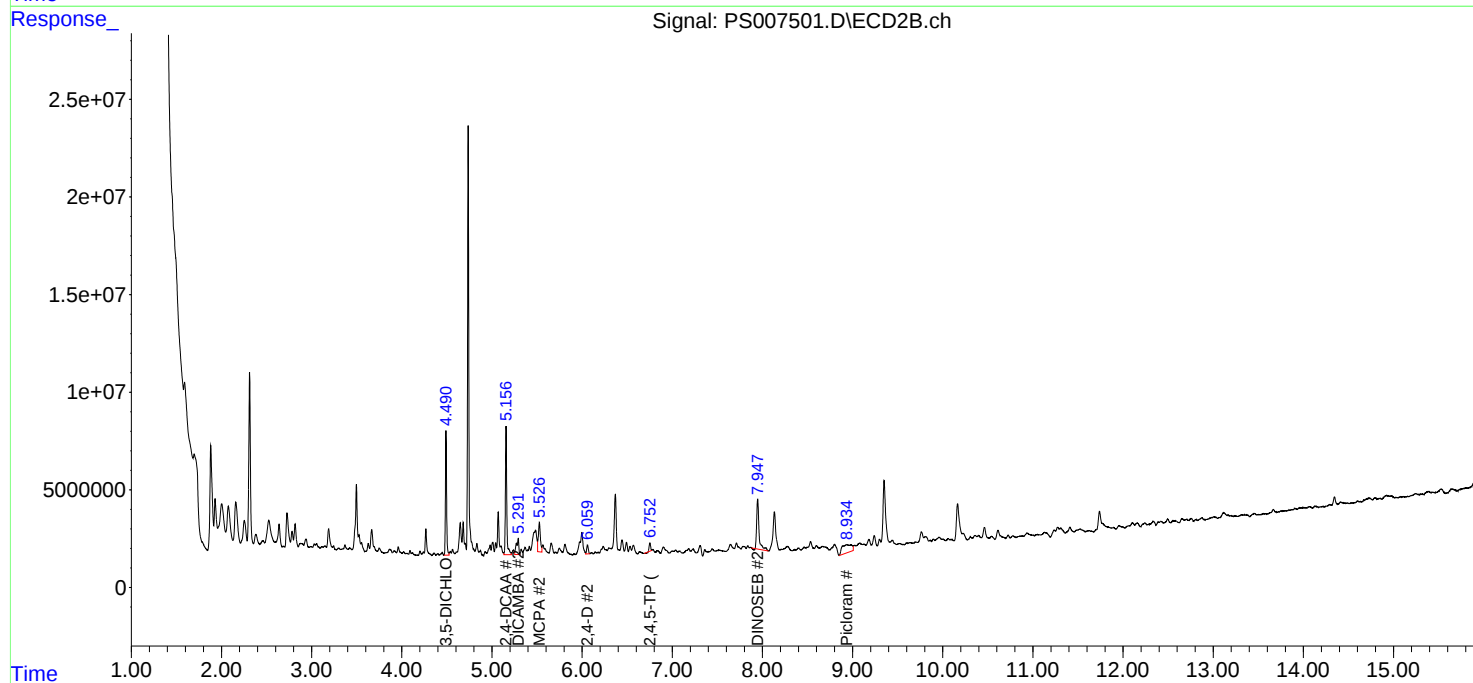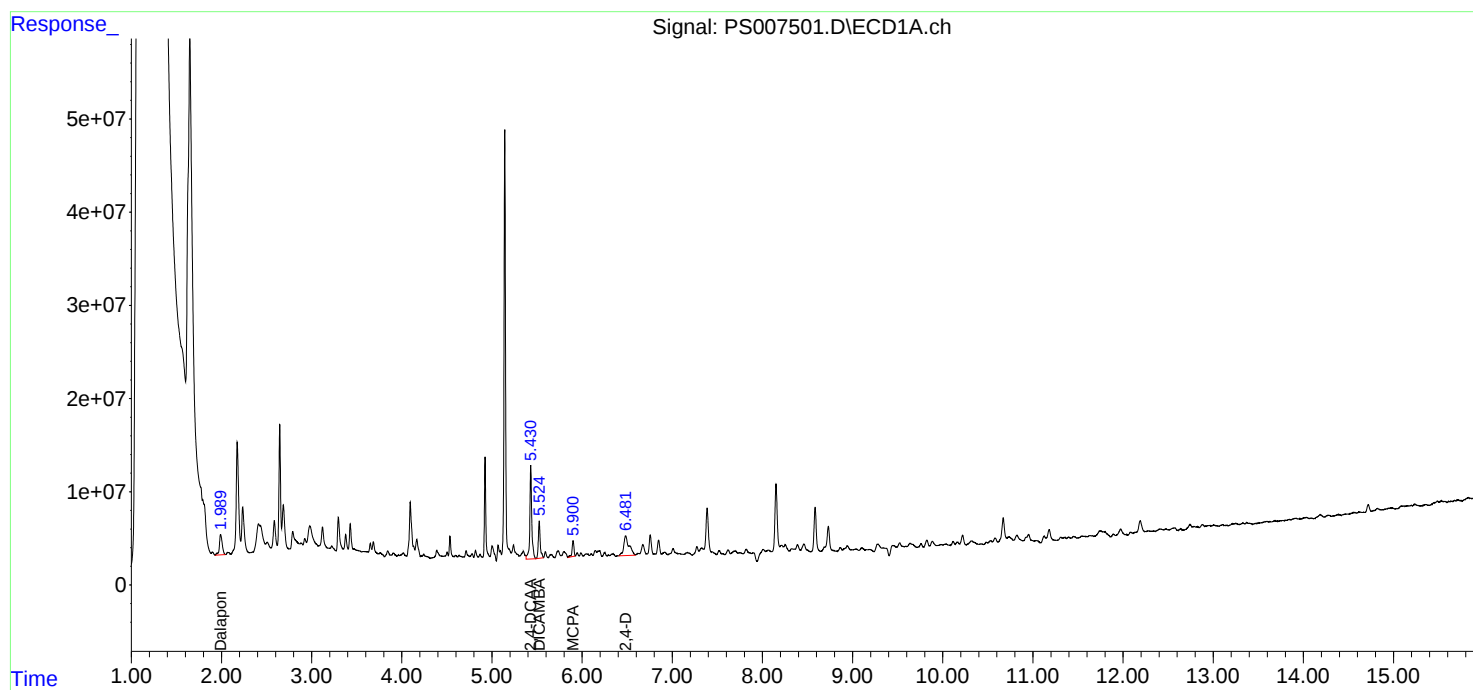


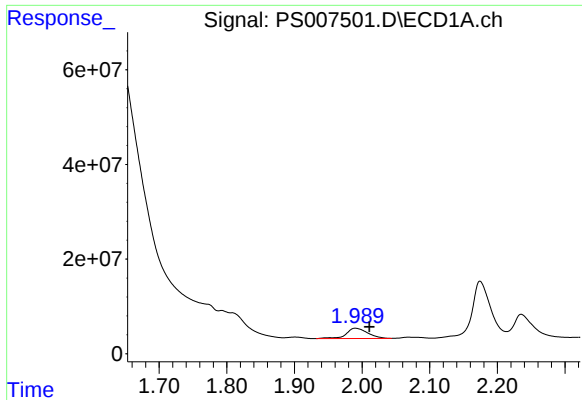

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.021 min
Response: 47889313
Conc: 28.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

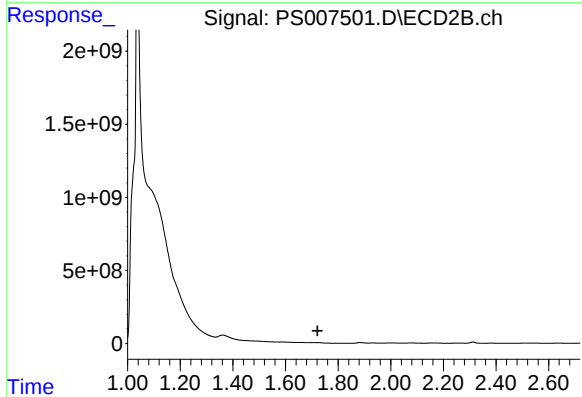


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

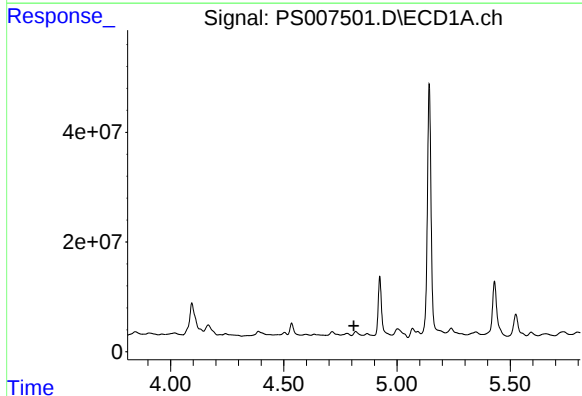


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

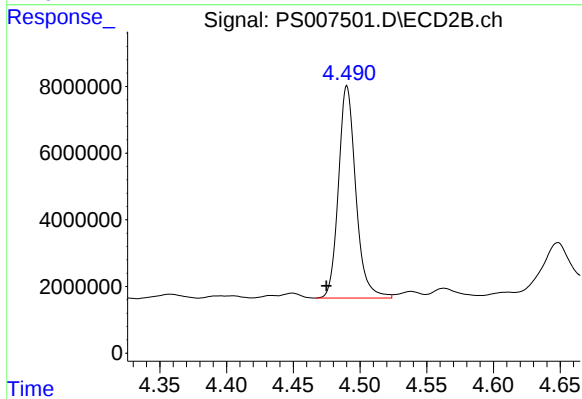

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.490 min
Delta R.T.: 0.016 min
Response: 57672738
Conc: 67.03 ng/ml

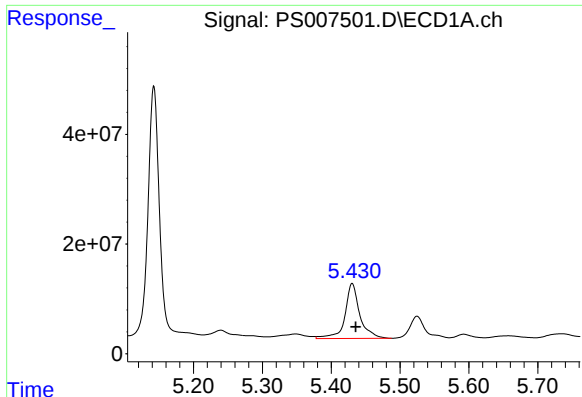

#4 2,4-DCAA


R.T.: 5.431 min
Delta R.T.: -0.005 min
Response: 149876777
Conc: 109.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

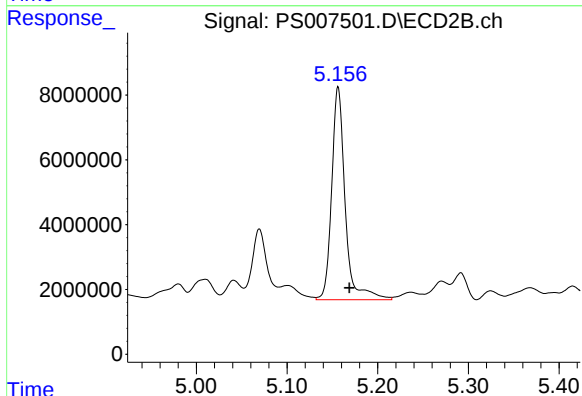


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: -0.012 min
Response: 67897075
Conc: 96.54 ng/ml

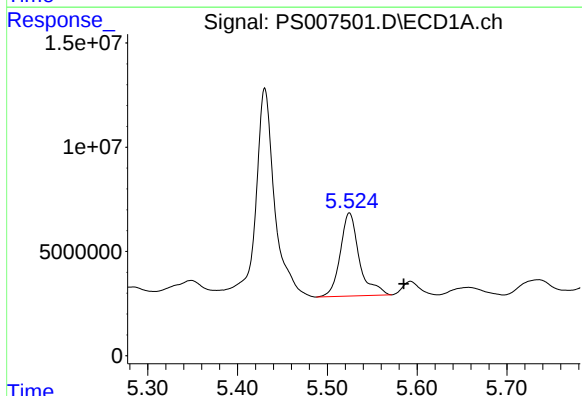


#5 DICAMBA

R.T.: 5.525 min
Delta R.T.: -0.061 min
Response: 58685360
Conc: 11.94 ng/ml

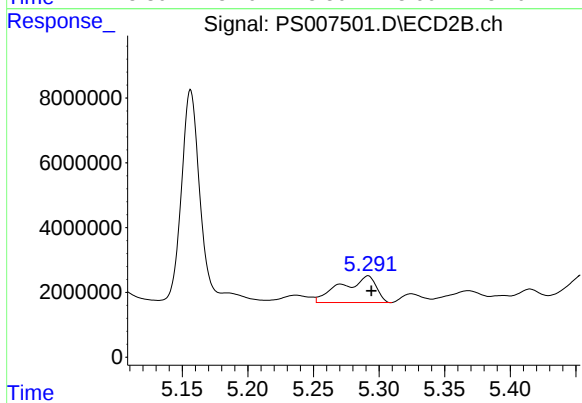

#5 DICAMBA


R.T.: 5.291 min
Delta R.T.: -0.003 min
Response: 15211468
Conc: 5.85 ng/ml

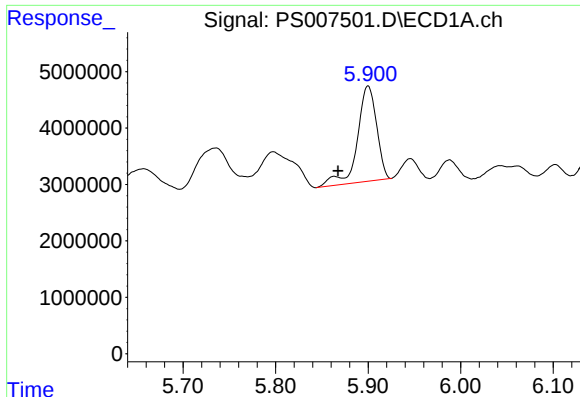

#7 MCPA


R.T.: 5.900 min
Delta R.T.: 0.033 min
Response: 24537934
Conc: 4.76 ug/ml

Instrument :
ECD_S
ClientSampleId :

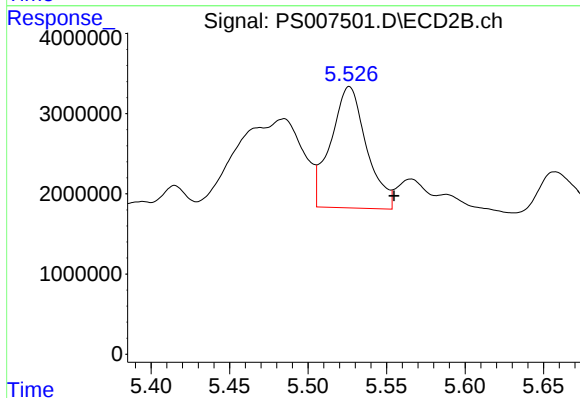


#7 MCPA

R.T.: 5.526 min
Delta R.T.: -0.029 min
Response: 24011261
Conc: 8.26 ug/ml

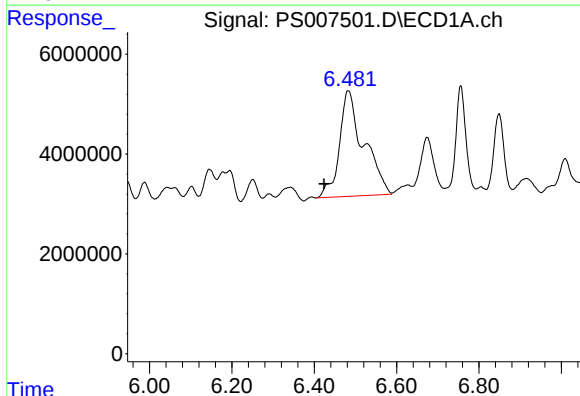


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.059 min
Response: 86733698
Conc: 70.38 ng/ml

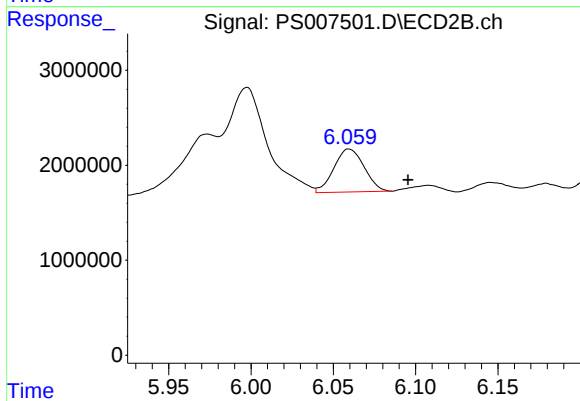

#9 2,4-D


R.T.: 6.060 min
Delta R.T.: -0.036 min
Response: 5807039
Conc: 7.28 ng/ml

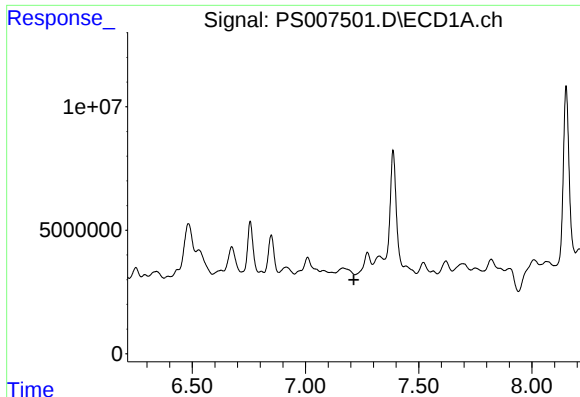

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

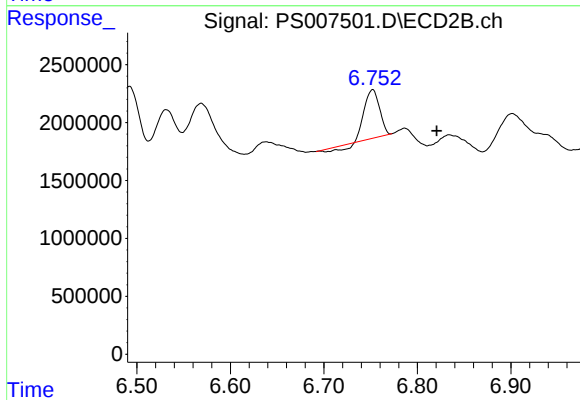


#11 2,4,5-TP (SILVEX)

R.T.: 6.752 min
Delta R.T.: -0.069 min
Response: 4242608
Conc: 1.12 ng/ml

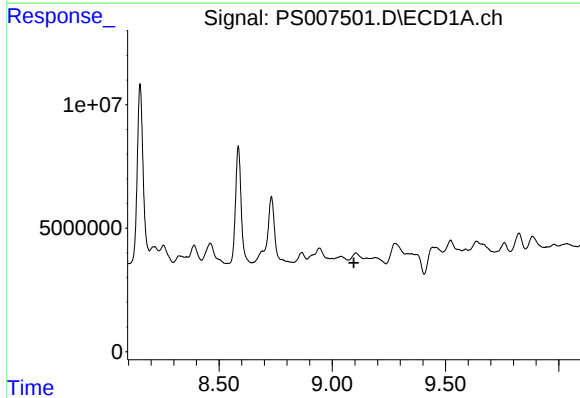


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

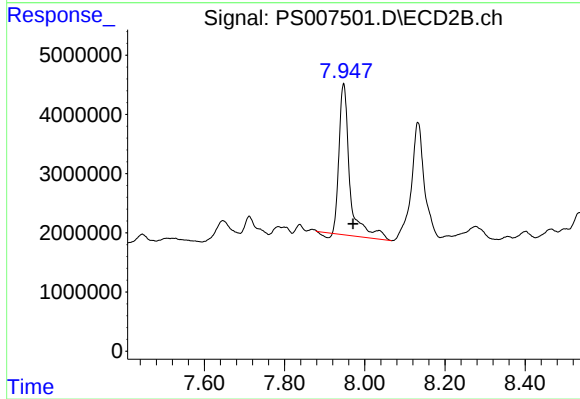

#14 DINOSEB


R.T.: 7.947 min
Delta R.T.: -0.023 min
Response: 47182901
Conc: 16.81 ng/ml

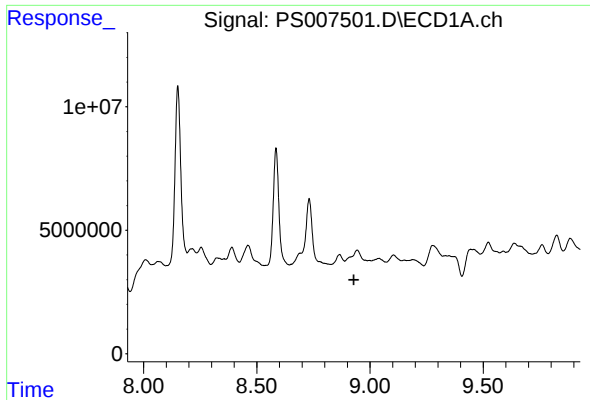

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

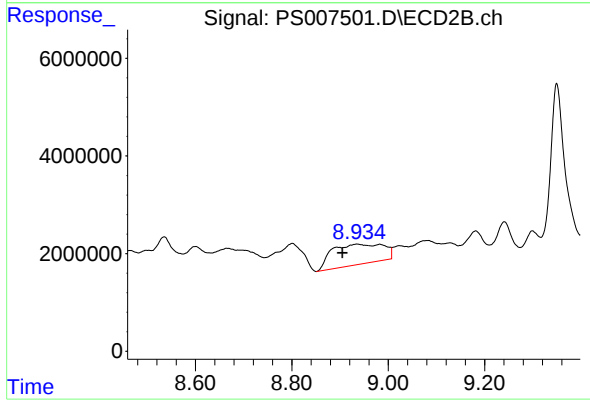

#15 Picloram

R.T.: 8.935 min
Delta R.T.: 0.031 min
Response: 30920733
Conc: 5.04 ng/ml